


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130143</u> ✓
Name	<u>Bob Butler</u>	ID#	<u>3694</u> Date <u>2/20/08</u> ✓
A Agency	<u>Fort Wainwright Police</u> ✓	Phone #	<u>353-7564</u>
Instrument Location	<u>Bldg # 3028, Fort Wainwright, AK 99703</u>		
B Alco S/N	<u>57345</u> ✓	Target Value	<u>0.081</u> ✓ High Pressure <u>250</u>
Alco Test Values	<u>0.082</u> ✓ 1 <sup>st</sup> Alco	<u>0.082</u> ✓ 2 <sup>nd</sup> Alco	
Signature			<u>003</u> <u>4/21/08</u>
(OVER)			

Under the Alaska Rules of Evidence, I certify that (I am the operator in the area below)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Robert A Butler, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,





Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

4/27/08  
Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N


130143

(CONTINUED FROM FRONT PAGE)


C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.


## NONDRINKING SUBJECT TEST

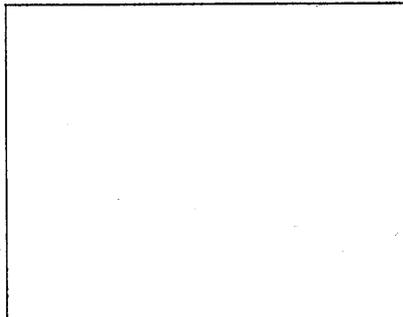

<b>Breath Test Record</b>			
Serial Number	130143	Model	DataMaster
Location	FAI4	Fl. Wainwright Provost Marshal	
<b>Subject Information</b>			
Last Name	Verification Of Cal	O.L. #	1234
First Name	V OI C		
<b>Operator Information</b>			
Operator Name	Butler	Case	1234
Operator #	3694	Department	FAI4
<b>Test Results</b>			
Alco Target	0.081	Alco Serial	57345
Nominal	0.078	Barometer	29.12
Dry Gas 1	0.082	Time	14:45:05
Subject Alcohol	0.000	Time	14:46:31
Dry Gas 2	0.082	Time	14:47:50
		Report	Y

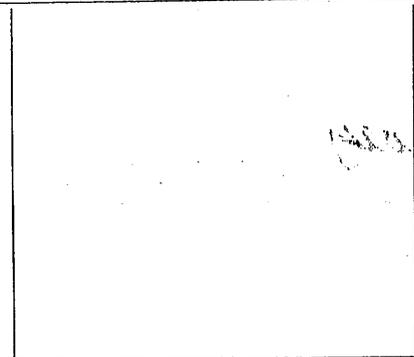

## DIAGNOSTIC CHECK

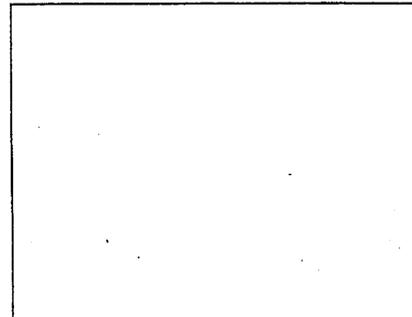

<b>Diagnostic Test Record</b>	
Serial Number	130143
Model	DataMaster
Location	FAI4
Fl. Wainwright Provost Marshal	
<b>Diagnostic Test Results</b>	
Test Date	02/20/2008
Test Time	14:39:41
Computer	Okay
Program	Okay
Software Date	02/20/2001
Sample Chamber (C)	49
Breath Tube (C)	41
Barometer (in)	29.12
Flow Detector	Okay
High Speed Pump	Okay
Detector	Okay
Filter	Okay
Quartz	Okay
Calibration	Okay

