

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130171 ✓
Name	CHRISTOPHER M. CHAPMAN	AWC ID#	6390 613
Date	2 Apr 08 ✓		
A Agency	EIL4 ✓	Phone #	377-1408
Instrument Location	451 DIVISION STREET EIELSON AFB, AK 99702		
B Alco S/N	x301596 ✓	Target Value	.080 ✓
		High Pressure	690
Alco Test Values	.079 ✓	.079 ✓	
	1 st Alco	2 nd Alco	
Signature			
	(OVER)		


Under the Alaska Rules of Evidence, I certify that:
(Do Not write in the area below)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Christopher M Chapman, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

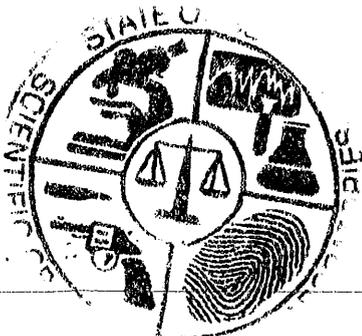



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

4/14/08

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130171

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130171

APRIL 02, 2008

OPERATOR'S NAME: *CPB 4/14/08*
CHAPMAN CHRISTOPHER M
OPERATOR'S NUMBER: 6390
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
UOC

O.L. #: 1
DEPT/AGENCY: ETL4
CASE/REPORT:
TEST TYPE: U
ALCO TARGET VALUE: 0.00
ALCO S/N: X301596

--- BREATH ANALYSIS ---

20/03/10

.000 ADJUSTED FOR 29.55 in		
ALCO TARGET	.079	06:39
BLANK TEST	.000	06:41
INTERNAL STANDARD	VERIFIED	06:41
ALCO TU 29.55 in	.079	06:41
BLANK TEST	.000	06:42
SUBJECT SAMPLE	.000 <i>CPB</i>	06:42
BLANK TEST	.000 <i>4/14/08</i>	06:43
ALCO TU 29.55 in	.079	06:43
BLANK TEST	.000	06:44

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130171

APRIL 02, 2008
TIME 06:45

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 43c

BAROMETER: 29.55 in

FLOW DETECTOR: OKAY

PUMP
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJKL
MNPQRSTUVWXYZ[\]^_`abcdefghijklmnopqrstuvwxyz{|}~