


FEB 14 2008

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130179</u>
Name	<u>John T. Ostoj</u>	ID#	<u>4823</u> Date <u>2-12-08</u>
A Agency	<u>Soldotna AST</u>	Phone #	<u>262-4453</u>
Instrument Location	<u>Soldotna AST Post</u>		
B Alco S/N	<u>X124658</u> ✓	Target Value	<u>.081</u> ✓ High Pressure <u>950</u>
Alco Test Value Average	<u>1.078</u> 1 <sup>st</sup> Alco	<u>1.077</u> 2 <sup>nd</sup> Alco	
Signature			<u>CSB</u> <u>2/28/08</u>

(OVER)


(Do Not write in the area below)

Under the Alaska Rules of Evidence, I certify that;


(a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, John Ostoj, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

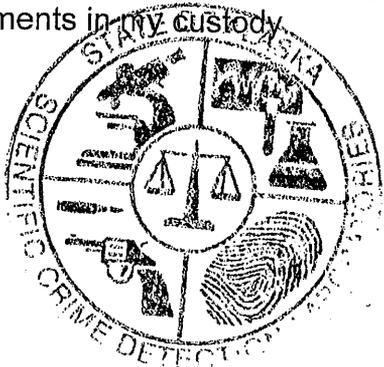

Signed and sealed



Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

3/1/08

Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130179<sup>N</sup>

(CONTINUED FROM FRONT PAGE)

C. TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130179

FEBRUARY 12, 2000 *CB 2/23/00*

OPERATOR'S NAME:  
OSTOJ, JOHN/T  
OPERATOR'S NUMBER: 4023  
SUBJECT'S LAST NAME:  
UOC  
SUBJECT'S FIRST NAME/MI :  
TEST  
O.L. #: UOC TEST  
DEPT/AGENCY: SLD0  
CASE/REPORT: TEST  
TEST TYPE: U  
ALCO TARGET VALUE: .001  
ALCO S/N: K124658

--- BREATH ANALYSIS ---

.001 ADJUSTED FOR 29.59 in		
ALCO TARGET	.000	07:24
BLANK TEST	.000	07:25
INTERNAL STANDARD	VERIFIED	07:25
ALCO TU 29.59 in	.078	07:26
BLANK TEST	.000	07:26
SUBJECT SAMPLE	.000	07:27
BLANK TEST	.000	07:28
ALCO TU 29.59 in	.077	07:28
BLANK TEST	.000	07:29

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130179

FEBRUARY 12, 2000  
TIME 07:31

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHECKED: 49c  
BREATH TUBE: 41c  
BAROMETER: 29.59 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

114462 12/11/00 10:07:59.1(K=)296005FG  
ALCO INSTRUMENT MODEL 130179  
SERIAL # 130179