

**JUL 01 2008 VERIFICATION OF CALIBRATION REPORT**

*of DataMaster cdm Breath Test Instrument*

*State of Alaska*

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130181</u>
Name	<u>Colleen</u>	ID#	<u>6237</u> Date <u>6/26/08</u>
A Agency	<u>SCD</u>	Phone #	<u>269-5783</u>
Instrument Location	<u>AST/Merana</u>		
Alco S/N		Target Value	High Pressure
<u>X301532</u>		<u>0.079</u>	<u>1175</u>
Alco Test Values		<u>0.078</u>	<u>0.076</u>
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
Signature	<u>C. O'Bryant</u>		<u>COB</u> <u>7/10/08</u>

(OVER)


Under the Alaska Rules of Evidence, I certify that (copy and paste in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Colleen S O'Bryant, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed

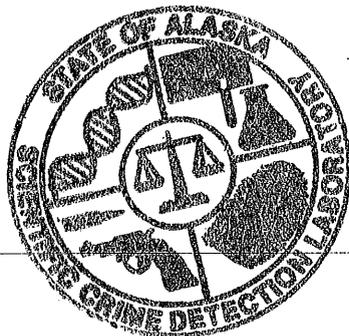

Jeanne Swartz

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

7/13/08  
Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130181

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130181

JUNE 26, 2008 *COB 7/10/08*

OPERATOR'S NAME:  
OBRYANT/COLLEEN/S  
OPERATOR'S NUMBER: 6237  
SUBJECT'S LAST NAME:  
VOC  
SUBJECT'S FIRST NAME/NI :  
VOC  
O.L. #: 0123456  
DEPT/AGENCY: AAA1  
CASE/REPORT: 08-1234  
TEST TYPE: V  
ALCO TARGET VALUE: .079  
ALCO S/N: X301532

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 29.55 in		
ALCO TARGET	.078	12:42
BLANK TEST	.000	12:43
INTERNAL STANDARD	VERIFIED	12:43
ALCO TV 29.55 in	.078	12:44
BLANK TEST	.000	12:45
SUBJECT SAMPLE	.000 <i>COB 7/10/08</i>	12:45
BLANK TEST	.000	12:46
ALCO TV 29.54 in	.076	12:46
BLANK TEST	.000	12:47

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130181

JUNE 26, 2008  
TIME 12:40

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01

HEATERS:  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c

BAROMETER: 29.55 in

FLOW DETECTOR: OKAY

PUMP  
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST  
!"#\$%&'()\*+,-./0123456789:;<=>@ABCDEFGHI  
HIJKLMNOPQRSTUVWXYZ[\]^\_`abcde{ghi,jklmno  
pqrstuvwxyz{|}~