

# VERIFICATION OF CALIBRATION REPORT

of DataMaster edm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

OCT 15 2009


|  |  |                                  |                                       |
|--|--|----------------------------------|---------------------------------------|
| Supervisor/Operator Performing the Verification Procedure: |  | DataMaster edm S/N <u>130181</u> |                                       |
| Name   | <u>Malik Jones</u>   | ID#                              | <u>5830</u> Date <u>10/10/09</u>      |
| A Agency   | <u>AST</u>   | Phone #                          | <u>451-5100</u>                       |
| Instrument Location  | <u>Nenana</u>  |                                  |                                       |
| B Alco S/N   | <u>75602</u>   | Target Value                     | <u>.083</u> High Pressure <u>1200</u> |
| Alco Test Value Average                                    | <u>.083</u>  | <u>.083</u>                      |                                       |
|  | 1 <sup>st</sup> Alco   | 2 <sup>nd</sup> Alco             |                                       |
| Signature  |  |                                  |                                       |
|  |  |                                  | <u>MS</u><br><u>10/7/09</u>           |


(OVER)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows (DataMaster follows in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

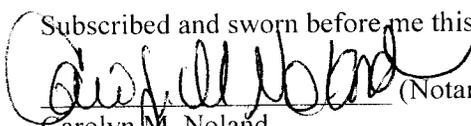Subscribed and sworn before me this 10th day of Nov., 2009.  
  
(Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

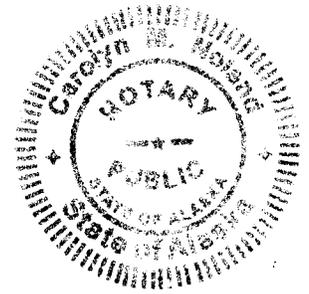

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130181

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130181

OCTOBER 10, 2009

OPERATOR'S NAME:

JONES/HALIK/JAMAL

OPERATOR'S NUMBER: 5830

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

V

O.L. #: 1

DEPT/AGENCY: NEN1

CASE/REPORT:

TEST TYPE: V

ALCO TARGET VALUE: .003

ALCO S/N: 75602

### --- BREATH ANALYSIS ---

|                            |          |       |
|----------------------------|----------|-------|
| .003 ADJUSTED FOR 29.64 in |          |       |
| ALCO TARGET                | .002     | 11:23 |
| BLANK TEST                 | .000     | 11:24 |
| INTERNAL STANDARD          | VERIFIED | 11:24 |
| ALCO TV 29.64 in           | .003     | 11:24 |
| BLANK TEST                 | .000     | 11:25 |
| SUBJECT SAMPLE             | .000     | 11:26 |
| BLANK TEST                 | .000     | 11:26 |
| ALCO TV 29.64 in           | .003     | 11:27 |
| BLANK TEST                 | .000     | 11:28 |

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130181

OCTOBER 10, 2009

TIME 11:31

### --- DIAGNOSTIC CHECK ---

|                  |          |
|------------------|----------|
| COMPUTER:        | OKAY     |
| PROGRAM:         | OKAY     |
| SOFTWARE DATE:   | 02/20/01 |
| HEATERS          |          |
| SAMPLE CHAMBER:  | 49c      |
| BREATH TUBE:     | 41c      |
| BAROMETER:       | 29.64 in |
| FLOW DETECTOR:   | OKAY     |
| PUMP             |          |
| HIGH SPEED:      | OKAY     |
| DETECTOR:        | OKAY     |
| FILTERS:         | OKAY     |
| QUARTZ STANDARD: | OKAY     |
| CALIBRATION:     | OKAY     |

### PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@ABCDEF  
HIJKLMNOPQRSTUVWXYZ\]^\_`abcdefghijklmnop  
qrstuvwxyz{|}~