

DEC 09 2010

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130182</u> ✓
Name	<u>STEVE DUNN</u>	ID#	<u>4106</u> ✓
		Date	<u>12-9-10</u> ✓
A	Agency	<u>APD</u>	Phone # <u>786-8900</u>
	Instrument Location	<u>ANCHORAGE JAIL</u>	
B	Alco S/N	<u>1 D</u>	Target Value <u>.080</u> ✓
			High Pressure <u>1000</u>
	Alco Test Values	<u>.080</u> ✓	<u>.081</u> ✓
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
	Signature		


(OVER)

AMB  
12/14/10

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

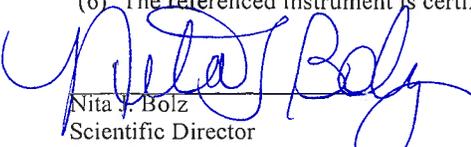
  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 18<sup>th</sup> day of JAN, 2011 DUN



 (Notary Seal Stamp)

Daniel L. Nicholas  
 Notary Public, State of Alaska  
 Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130182 <sup>BMB</sup> 12/16/10

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130182

DECEMBER 09, 2010

OPERATOR'S NAME:  
DUNN/S  
OPERATOR'S NUMBER: 4106  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :  
V  
O.L. #: V  
DEPT/AGENCY: ANCI  
CASE/REPORT: V  
TEST TYPE: V  
ALCO TARGET VALUE: .080  
ALCO S/N: 1D

### --- BREATH ANALYSIS ---

.080 ADJUSTED FOR 29.88 in  
ALCO TARGET .079 11:00  
BLANK TEST .000 11:01  
INTERNAL STANDARD VERIFIED 11:01  
ALCO TV 29.88 in .080 11:01  
BLANK TEST .000 11:02  
SUBJECT SAMPLE .000 11:02  
BLANK TEST .000 11:03  
ALCO TV 29.88 in .081 11:03  
BLANK TEST .000 11:04

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130182

DECEMBER 09, 2010  
TIME 10:58

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 29.88 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGH  
IJKLMNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopq  
rstuvwxyz{|}~Δ