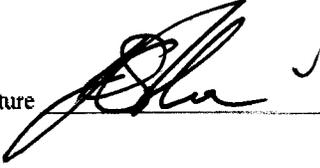


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument  
State of Alaska

SEP 28 2009

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130184</u> ✓
Name	<u>SERGEANT JOHN HAMILTON</u>	ID#	<u>3192</u> Date <u>9/21/09</u> ✓
A Agency	<u>PETERSBURG POLICE DEPARTMENT</u>	Phone #	<u>772-3838</u>
Instrument Location	<u>PETERSBURG</u> ✓		
B Alco S/N	<u>78268</u> ✓	Target Value	<u>.081</u>
		High Pressure	<u>700/51</u> ✓
Alco Test Values	<u>.081</u> ✓	<u>.080</u> ✓	
	1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco	
Signature			

(OVER)


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 9<sup>th</sup> day of Oct., 2009.

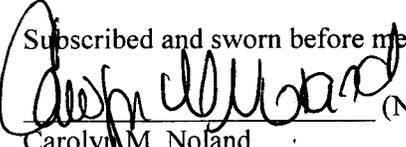  
(Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



