

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130192 ✓
Name		J Swartz	ID# 4294 Date 1/7/08 ✓
A	Agency	SCDL	Phone # 269-5592
Instrument Location		SCDL ✓	
Alco S/N		SC0107 ✓	Target Value .080 ✓ High Pressure 600 psi
Alco Test Values		.078 ✓ 1 st Alco	.078 ✓ 2 nd Alco
Signature			CSB 7/8/08

(OVER)


Under the Alaska Rules of Evidence, I certify that: (Do Not write in the area below)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Jeanne M Swartz, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

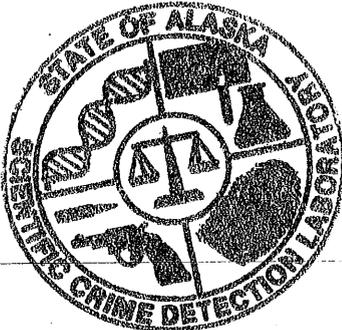



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

7/09/08
Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130192 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130192

JANUARY 07, 2008

OPERATOR'S NAME:

SWARTZ/J

OPERATOR'S NUMBER: 4314

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

L

O.L. #: L

DEPT/AGENCY: AAAA

CASE/REPORT:

TEST TYPE: U

ALCO TARGET VALUE: .060

ALCO S/N: SCOTT97

--- BREATH ANALYSIS ---

.060 ADJUSTED FOR 29.18 in

ALCO TARGET	.078	14:38
BLANK TEST	.000	14:39
INTERNAL STANDARD	VERIFIED	14:39
ALCO TV 29.18 in	.078	14:39
BLANK TEST	.000	14:40
SUBJECT SAMPLE	.060	14:40
BLANK TEST	.000	14:41
ALCO TV 29.18 in	.078	14:42
BLANK TEST	.000	14:42

1171088

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130192

JANUARY 07, 2008 ✓

TIME 14:36

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 29.18 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHI
HIJKLMNPOQRSTUVWXYZ[\]^_`abcdefghijklmnopqrstuvwxyz{|}~#