

VERIFICATION OF CALIBRATION REPORT

of DataMaster edm Breath Test Instrument

State of Alaska


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster edm S/N <u>1300192</u>
Name <u>BRANDON LAWRENSEN</u>	ID# <u>06609</u>	Date <u>06/04/08</u>
Agency <u>JUNEAU POLICE DEPT</u>	Phone # <u>580-0600</u>	
Instrument Location <u>JUNEAU POLICE DEPT</u>		
Alco S/N <u>70108</u>		Target Value <u>.080</u> High Pressure <u>500</u>
Alco Test Values		
<u>.081</u> 1 st Alco	<u>.081</u> 2 nd Alco	
Signature 	CAB 6/13/08	
(OVER)		

Under the Alaska Rules of Evidence, I certify that, (Do not write in the area below)

- (a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.
- (b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Brandon Lawrenson, whose name appears in my records, is qualified to verify the calibration of the above instrument.
- (c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

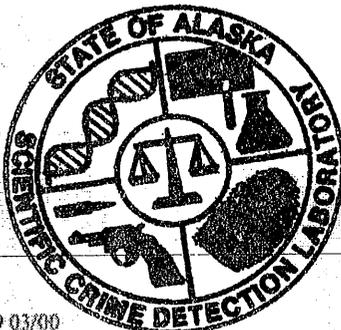



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

6/16/08
Date

VERIFICATION OF CALIBRATION REPORT
of DataMaster cdm breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130192

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
 DATAMASTER cdm 130192

JUNE 04, 2008 ✓ *COB 6/12/08*

OPERATOR'S NAME:
 LAWRENSEN/BRANDON/J
 OPERATOR'S NUMBER: 6609
 SUBJECT'S LAST NAME:
 VOC

SUBJECT'S FIRST NAME/INIT:
 VOC

O.L. #: 0000000

DEPT/AGENCY: JNU1

CASE/REPORT: 000000

TEST TYPE: U

ALCO TARGET VALUE: .000 ✓

ALCO S/N: 70100

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 30.14 in		
ALCO TARGET	.000	00:34
BLANK TEST	.000	00:35
INTERNAL STANDARD	VERIFIED	00:35
ALCO TV 30.14 in	.001 ✓	00:35
BLANK TEST	.000	00:36
SUBJECT SAMPLE	.000 <i>COB 6/12/08</i>	00:37
BLANK TEST	.000	00:38
ALCO TV 30.14 in	.001	00:38
BLANK TEST	.000	00:39

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
 DATAMASTER cdm 130192

JUNE 04, 2008 ✓
 TIME 00:32

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	41c
BAROMETER:	30.14 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

! " # % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
 H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
 p q r s t u v w x y z { } ~ |