

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130194</u>
Name	<u>Jaime L. Smith</u>	ID# <u>6762</u> Date <u>1/12/12</u> <sup>JLS.</sup>
A Agency	<u>Denali National Park</u>	Phone # <u>907-683-9525</u>
Instrument Location	<u>Ranger Station- Headquarters</u>	
B Alco S/N	<u>X301591</u>	Target Value <u>0.080</u> High Pressure <u>50 psi</u>
Alco Test Values	<u>0.077</u> 1 <sup>st</sup> Alco	<u>0.076</u> 2 <sup>nd</sup> Alco
Signature	<u>Jaime L. Smith</u>	

(OVER)

BMB  
1/18/12

(Do Not write in the area below)



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 2nd day of Feb 2012 <sup>AK</sup> ~~2010.~~

Nikki Roth (Notary Seal Stamp)  
~~Carolyn M. Noland~~ Nikki Roth  
Notary Public, State of Alaska  
Commission Expires with Office

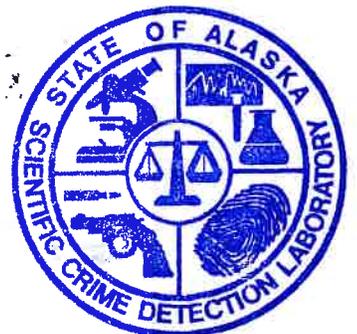

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130194

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

██████████  
ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130194

JANUARY 12, 2012 *BMB 11/18/12*

OPERATOR'S NAME:  
SMITH/JL

OPERATOR'S NUMBER: 6752

SUBJECT'S LAST NAME:  
X

SUBJECT'S FIRST NAME/ni :  
X

O.L. #: X

DEPT/AGENCY: DNLB

CASE/REPORT:

TEST TYPE: V

ALCO TARGET VALUE: .030

ALCO S/N: K301531

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 27.85 in		
ALCO TARGET	.074	10:15
BLANK TEST	.000	10:16
INTERNAL STANDARD	VERIFIED	12:16
ALCO @ 27.85 in	.077	10:17
BLANK TEST	.000	10:17
SUBJECT SAMPLE <i>BMB 11/18/12</i>	.000	10:18
BLANK TEST	.000	10:18
ALCO @ 27.85 in	.076	10:19
BLANK TEST	.000	10:19

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130194

JANUARY 12, 2012  
TIME 10:21

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	01/08/09
HEATERS	
SAMPLE CHAMBER:	50c
BREATH TUBE:	41c
BAROMETER:	27.85 in
FLOW DETECTOR:	OKAY
BLUP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@ABCDEF  
HIJKL"#\$%&'()\*+,-./:;?@\_`abcde fghijklmno  
pqrstuvwxy z{|}~>

