

# VERIFICATION OF CALIBRATION REPORT

FEB 25 2009

of DataMaster cdm Breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:  
Name JAMIES MICHELS ID# 6502 Date 2-21-09  
A Agency USIBPD Phone # 852-6111  
Instrument Location SQUAD ROOM - BARROW  
B Alco S/N X172971 Target Value .081 High Pressure 750 PSR  
Alco Test Values .084 .084  
1<sup>st</sup> Alco 2<sup>nd</sup> Alco  
Signature SCA Nick Michels MS  
3/2/09  
(OVER)


Under the Alaska Rules of Evidence, I certify that (if not true, write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, James Michels, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

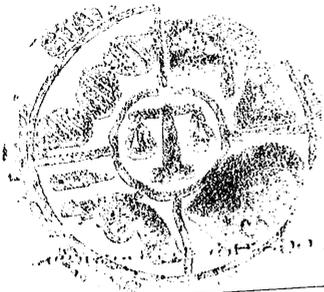

Jeanne Swartz

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

3/2/09  
Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130194

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130194

FEBRUARY 21, 2009

OPERATOR'S NAME:

NICHOLS, JAMES/D

OPERATOR'S NUMBER: 6502

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI :

VOC

O.L. #: VOC

DEPT/AGENCY: DMH

CASE/REPORT: VOC

TEST TYPE: V

ALCO TARGET VALUE: .051

ALCO S/N: K172971

--- BREATH ANALYSIS ---

.301 ADJUSTED FOR 31.00 in  
ALCO TARGET .053 07:38  
BLANK TEST .000 07:39  
INTERVAL STANDARD VERIFIED 07:39  
ALCO TV 31.00 in .004 ✓ 07:39  
BLANK TEST .000 07:40  
SUBJECT SAMPLE .000 07:41  
BLANK TEST .000 07:42  
ALCO TV 31.00 in .004 ✓ 07:42  
BLANK TEST .000 07:43

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130194

FEBRUARY 21, 2009

TIME 07:55

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 31.00 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@ABCDEF  
HIJKLMNOPQRSTUVWXYZ[ ]^\_`abcedefghijklmno  
pqrstuvwxyz{|}~