

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N <u>130195</u>	
Supervisor/Operator Performing the Verification Procedure:	
A Name <u>Robert J. Ely</u>	ID# <u>2681</u> Date <u>09-05-2008</u> ✓
Agency <u>Craig Police Department</u>	Phone # <u>(907) 826-3330</u>
Instrument Location <u>506 2nd Street, Craig Alaska 99921</u>	✓
Alco S/N <u>77286</u> ✓	Target Value <u>.079</u> ✓ High Pressure <u>600</u> PSI
Alco Test Value Average <u>.084</u> ✓	<u>.084</u> ✓
1 st Alco	2 nd Alco
Signature <u><i>Robert J. Ely</i></u>	<i>CS</i> <i>9/2/08</i>
(OVER)	

(Do Not write in the area below)


Under the Alaska Rules of Evidence, I certify that:

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Robert J Ely, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

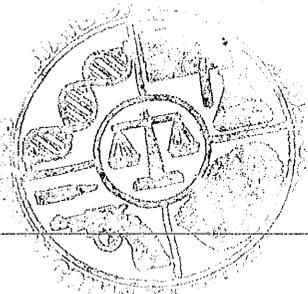

J Swartz 10/5/08
Jeanne Swartz Date
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130195

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130195

SEPTEMBER 05, 2008 *CS 9/2/08*

OPERATOR'S NAME:

ELY, RJ

OPERATOR'S NUMBER: 2691

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

VER OF CAL

O.I.L. #: 123456789

DEPT/AGENCY: CRG1

CASE/REPORT: 2008-XXXX

TEST TYPE: U

ALCO TARGET VALUE: .079 ✓

ALCO S/N: 77286 ✓

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 30.45 in		
ALCO TARGET	.080	14:06
BLANK TEST	.000	14:07
INTERNAL STANDARD	VERIFIED	14:07
ALCO TV 30.45 in	.084 ✓	14:07
BLANK TEST	.000	14:08
SUBJECT SAMPLE	.080 <i>CS</i>	14:08
BLANK TEST	.000 <i>CS</i>	14:09
ALCO TV 30.45 in	.084 ✓	14:09
BLANK TEST	.000	14:10

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130195

SEPTEMBER 05, 2008 ✓
TIME 14:03

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	41c
BAROMETER:	30.45 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@BCDEFG
HIJKL/MNOPQRSTUVWXYZ\|_`abcedefghijklmnop
qrs tuvwxyz{|}~