

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAY 31 2011

DataMaster cdm S/N 130195

Supervisor/Operator Performing the Verification Procedure:

**A**  
Name Robert J. Ely ID# 2681 Date 05-24-2011  
Agency Craig Police Department Phone # (907) 826-3330  
Instrument Location 506 2<sup>nd</sup> Street, Craig Alaska 99921

**B**  
Alco S/N 75509 Target Value .079 High Pressure 900 PSI  
Alco Test Value Average .081 .081  
1<sup>st</sup> Alco 2<sup>nd</sup> Alco

Signature Robert J. Ely

(OVER)

(Do Not write in the area below)

*amb*  
*5/31/11*

I, Nita J. Bolz, after being first duly sworn, depose and state as follows;


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons Responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska

Nita J. Bolz  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 15 day of JUNE, 2011 *NJB*



Kyle Klopfer (Notary Seal Stamp)  
Daniel L. Nicholas *Kyle Klopfer*  
Notary Public, State of Alaska  
Commission Expires with Office

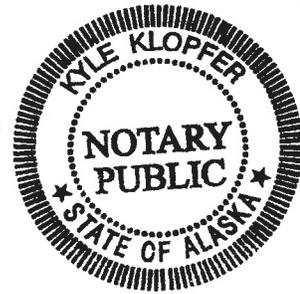

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130195

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130195

MAY 24, 2011

OPERATOR'S NAME:

ELV, RJ

OPERATOR'S NUMBER: 2681

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

VER OF CAL

CAL #1: 123456789

DEST AGENCY: DRG1

CASE/REPORT: 11-XXXXX

TEST TYPE: U

ALCO TARGET VALUE: .079

ALCO G/M: 75589

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 30.24 in  
ALCO TARGET .079 14:45  
BLANK TEST .000 14:45  
INTERNAL STANDARD VERIFIED 14:45  
CALIBRATED 30.24 in .081 14:46  
BLANK TEST .000 14:47  
SUBJECT SAMPLE .000 14:47  
BLANK TEST .000 14:48  
CALIBRATED 30.24 in .081 14:49  
BLANK TEST .000 14:49

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130195

MAY 24, 2011

TIME 14:43

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 42c

BAROMETER: 30.24 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

\*\*\*\*\*  
ALCO#0123456789: (X=)??ABCDEF6  
HOLD#OPQRSTUWXYZ\^\_`'abcde fghijklmno  
pqrstu vwxyz{|}~@

