

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

| | |
|---|---|
| Supervisor/Operator Performing the Verification Procedure: <u>DataMaster cdm S/N 130196</u> | |
| Name <u>JEAN ACHEE</u> | ID# <u>1470</u> Date <u>6/13/08</u> |
| A Agency <u>WASILLA POLICE DEPT.</u> Phone # <u>352-5401</u> | |
| Instrument Location <u>WASILLA POLICE DEPT.</u> | |
| B Alco S/N <u>31085</u> ✓ Target Value <u>.080</u> ✓ High Pressure <u>900 lbs.</u> | |
| Alco Test Value Average <u>.081</u> ✓ 1 st Alco | <u>.082</u> ✓ 2 nd Alco |
| Signature <u>Jean Achee</u> | <u>CSB</u> <u>8 CSB</u> <u>7/3/08</u> |


(OVER)

Under the Alaska Rules of Evidence, I certify that:
(Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Jean P Achee, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

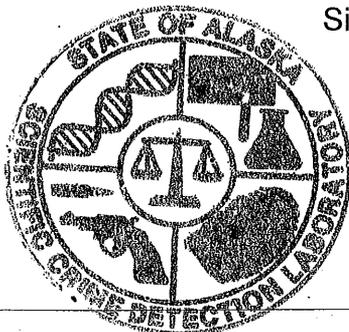

Signed and sealed,

Jeanne Swartz

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

7/7/08
Date

JUN 20 2008

BT9 03/00

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130196

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130196

JUNE 13, 2008

OPERATOR'S NAME:

ACHEE, JEAN P

OPERATOR'S NUMBER: 1470

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI :

VOC

O.L. #: 1234567890

DEPT/AGENCY: WASH

CASE/REPORT: 00-0613

TEST TYPE: V

ALCO TARGET VALUE: .000

ALCO S/N: 31065

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 29.93 in
ALCO TARGET .000 17:58
BLANK TEST .000 17:59
INTERNAL STANDARD VERIFIED 17:59
ALCO TV 29.93 in .001 17:59
BLANK TEST .000 18:00
SUBJECT SAMPLE .000 18:01
BLANK TEST .000 18:01
ALCO TV 29.93 in .002 18:02
BLANK TEST .000 18:03

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130196

JUNE 13, 2008

TIME 17:56

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 40c

BREATH TUBE: 41c

BAROMETER: 29.93 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>@ABCDEFGHIJK
LMNOPQRSTUVWXYZ[\]^_`abcdefgijklmnop
qrstuvwxyz{|}~