

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N <u>130289</u> ✓	
Name <u>Byron D. Redburn</u>	ID# <u>2087</u> Date <u>9-13-2008</u>
Agency <u>Nome Police Dept</u>	Phone # <u>443-5262</u>
Instrument Location <u>Nome Police Dept</u> ✓	
Alco S/N <u>X301548</u> ✓ Target Value <u>.079</u> ✓ High Pressure <u>1100</u>	
Alco Test Values	
1 st Alco <u>.077</u> ✓	2 nd Alco <u>.077</u> ✓
Signature <u>B. D. Redburn</u>	<u>CSB</u> <u>9/15/08</u>

(OVER)

(Do Not write in the area below)


Under the Alaska Rules of Evidence, I certify that;

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Byron D Redburn, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

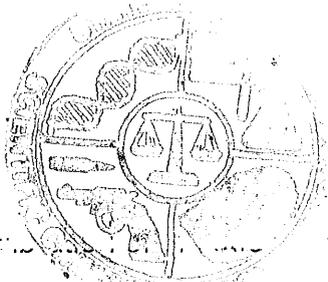

Juanes

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

10/5/08
Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130289

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130289

SEPTEMBER 13, 2000 *cds 9/21/00*

OPERATOR'S NAME:

REDBURN BYRON D

OPERATOR'S NUMBER: 2087

SUBJECT'S LAST NAME:

NON DRINKING

SUBJECT'S FIRST NAME/MI :

VERIFICATION OF CAL

O.L. #: A

DEPT/AGENCY: OMEI

CASE/REPORT: A

TEST TYPE: V

ALCO TARGET VALUE: .079 ✓

ALCO S/N: X301540 ✓

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 29.98 in		
ALCO TARGET	.079	07:55
BLANK TEST	.000	07:56
INTERNAL STANDARD	VERIFIED	07:56
ALCO TV 29.98 in	.077 ✓	07:56
BLANK TEST	.000	07:57
SUBJECT SAMPLE	.000 <i>cds 9/21/00</i>	07:58
BLANK TEST	.000	07:58
ALCO TV 29.98 in	.077 ✓	07:59
BLANK TEST	.000	08:00

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130289

SEPTEMBER 13, 2000 ✓
TIME 07:52

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	48c
BREATH TUBE:	42c
BAROMETER:	29.98 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~