

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program JUN 16 2010

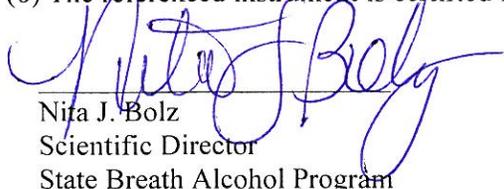
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130292 ✓		
Name	C. RITALA	ID#	3791	Date	6/15/10 ✓
Agency	APD	Phone #	786 2640		
Instrument Location	EAGLE RIVER WILLAM SUB ✓				
Alco S/N	75260 ✓	Target Value	.081 ✓	High Pressure	1200
Alco Test Values	080 ✓	080 ✓			
	1 st Alco	2 nd Alco			
Signature		RITALA/1349			088 6/21/10

(OVER)

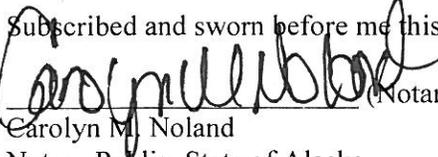
(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 21st day of July, 2010.


(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT
of DataMaster cdm breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130292 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST



ALASKA DEPARTMENT OF PUBLIC SAFETY
 DATAMASTER cdm 130292

JUNE 15, 2010 ✓

OPERATOR'S NAME:

RITALA

OPERATOR'S NUMBER: 3791

SUBJECT'S LAST NAME:

VERIFICATION OF CALIBRATION

SUBJECT'S FIRST NAME/MI :

INSTALL NEW INSTUMENT

O.L. #: EAGLE RIVER SUB

DEPT/AGENCY: ANCI

CASE/REPORT: A

TEST TYPE: V

ALCO TARGET VALUE: .081 ✓

ALCO S/N: 75260

COB 6/21/10

CR/12/09 6/15/10

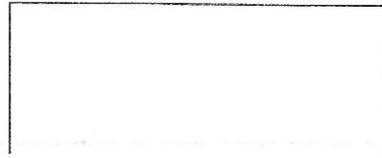
--- BREATH ANALYSIS ---

.081 ADJUSTED FOR 29.94 in		
ALCO TARGET	.081	16:57
BLANK TEST	.000	16:58
INTERNAL STANDARD	VERIFIED	16:58
ALCO TV 29.94 in	.080	16:58
BLANK TEST	.000	16:59
SUBJECT SAMPLE	.000	17:00
BLANK TEST	.000	17:00
ALCO TV 29.94 in	.080	17:01
BLANK TEST	.000	17:01

COB 6/21/10



DIAGNOSTIC CHECK



ALASKA DEPARTMENT OF PUBLIC SAFETY
 DATAMASTER cdm 130292

JUNE 15, 2010 ✓
 TIME 16:55

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	01/08/09
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	43c
BAROMETER:	29.94 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

CR/12/09 6/15/10

PRINTER TEST
 !"#%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
 KLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmnopqrstuvwxyz{|}~Δ

