

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130296</u>
Name		<u>JENNIFER L. SHOCKLEY</u>	ID# <u>4552</u> Date <u>11 FEB 2008</u>
A	Agency	<u>UNALASKA DEPT. OF PUBLIC SAFETY (UDPS)</u>	Phone # <u>907-581-1233</u>
Instrument Location		<u>UDPS</u>	
Alco S/N		<u>X301573</u>	Target Value <u>.075</u> High Pressure <u>550</u>
B	Alco Test Values	<u>.076</u> 1 st Alco	<u>.076</u> 2 nd Alco
Signature			<u>COB</u> <u>2/11/08</u>
(OVER)			

Under the Alaska Rules of Evidence, I certify that, ^(Do Not write in the area below)


(a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Jennifer L Shockley, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

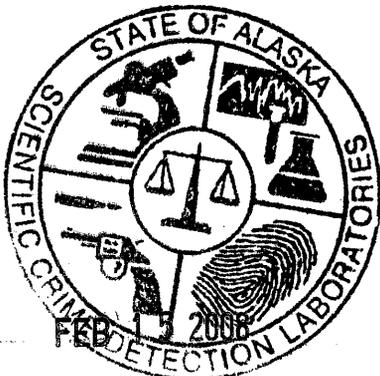

Signed and sealed



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

02/22/08
Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130296

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130296

FEBRUARY 11, 2008

OPERATOR'S NAME:
SHOCKLEY/JENNIFER/L
OPERATOR'S NUMBER: 4552
SUBJECT'S LAST NAME:
VOC

SUBJECT'S FIRST NAME/MI :
VOC

O.L. #: VOC
DEPT/AGENCY: UNK1
CASE/REPORT: VOC
TEST TYPE: V

ALCO TARGET VALUE: .075
ALCO S/N: X301573

--- BREATH ANALYSIS ---

.075 ADJUSTED FOR 29.62 in
ALCO TARGET .074 20:36
BLANK TEST .000 20:37
INTERNAL STANDARD VERIFIED 20:37
ALCO TV 29.62 in .076 20:37
BLANK TEST .000 20:38
SUBJECT SAMPLE .000 20:38
BLANK TEST .000 20:39
ALCO TV 29.62 in .076 20:39
BLANK TEST .000 20:40

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130296

FEBRUARY 11, 2008
TIME 20:33

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 29.62 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!""#%&'()*+,-./0123456789:;<=>?@ABCDEF
GHIJKLMNOPQRSTUVWXYZ\]^_`abcde fghijklmno
pqrstuvwxy z{|}~