


VERIFICATION OF CALIBRATION REPORT
Of Data-Master cdm Breath Test Instrument
 State of Alaska
 Scientific Crime Detection Laboratory -- Statewide Breath Alcohol Program

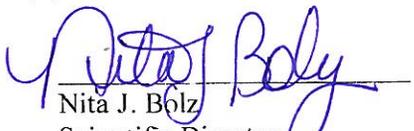
JUN 10 2010

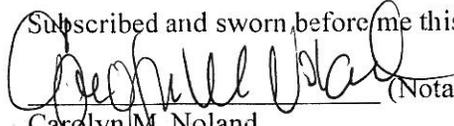
Data-Master cdm S/N: <u>130296</u>		
Supervisor/Operator Performing the Verification Procedure:		
Name <u>John J. Waldron</u> ID: # <u>3392</u> Date: <u>06/05/10</u>		
A. Agency <u>Unalaska Department of Public Safety</u> Phone <u>907-581-1233</u>		
Instrument Location <u>Unalaska Department of Public Safety, PO Box 370, 29 Safety Way, Unalaska, AK 99685</u>		
Alco S/N: <u>78966</u> Target Value: <u>.082</u> High Pressure: <u>700</u>		
B. Alco Test Values		
	<u>.084</u> 1 st Test Value	<u>.084</u> 2 nd Test Value
Signature <u></u>		<u>CB</u> <u>6/11/10</u>
(OVER)		

(Do not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 24th day of June, 2010.
 (Notary Seal Stamp)
 Carolyn M. Noland
 Notary Public, State of Alaska
 Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

**Of Data-Master cdm Breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory -- Statewide Breath Alcohol Program**

Data-Master cdm S/N: 130296 ✓

**Supervisor/Operator & Number Performing the Verification Procedure: John J. Waldron, #3392
Department and Date: Unalaska DPS,**

(CONTINUED FROM FRONT PAGE)

**C. TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE
DIAGNOSTIC CHECK IN THE MARKED BOXES.**

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130296 ✓

JUNE 05, 2010 ✓

OPERATOR'S NAME: *ccs 6/11/10*
WALDRON/JOHN/J
OPERATOR'S NUMBER: 3392
SUBJECT'S LAST NAME:
UOC
SUBJECT'S FIRST NAME/MI :
UOC
O.L. #: 0123456789
DEPT/AGENCY: UNK1
CASE/REPORT: 10-00000
TEST TYPE: U ✓
ALCO TARGET VALUE: .002 ✓
ALCO S/N: 78966 ✓

--- BREATH ANALYSIS ---

.002 ADJUSTED FOR 29.93 in	✓	
ALCO TARGET	.002	04:31
BLANK TEST	.000	04:33
INTERNAL STANDARD	VERIFIED	04:33
ALCO TV 29.91 in	.004 ✓	04:33
BLANK TEST	.000	04:34
SUBJECT SAMPLE	.000	04:34
BLANK TEST	.000	04:35
ALCO TV 29.93 in	.004 ✓	04:36
BLANK TEST	.000	04:36

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130296 ✓

JUNE 05, 2010 ✓
TIME 04:38 ✓

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 00/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 43c
BAROMETER: 29.93 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!##%&'()*+,-./:0123456789:;<=>?@ABCDEFG
HIJKL*NOPQRSTUUVWXYZ[]^_`abcde!ghijklmno
pqrstuvwxyz{|}~||