

# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument*

*State of Alaska*

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

|   |  |
|---|--|
| DataMaster cdm S/N <u>130296</u> ✓  |  |
| Supervisor/Operator Performing the Verification Procedure:                    |  |
| Name <u>John J Waldron</u>  | ID# <u>3392</u> ✓ Date <u>08/03/2010</u> ✓ |
| A Agency <u>Unalaska DPS</u> Phone # <u>907-581-1233</u>                      |  |
| Instrument Location <u>Unalaska DPS, PO Box 370, 29 Safety Way, Unalaska</u>  |  |
| B Alco S/N <u>78966</u> ✓ Target Value <u>.082</u> ✓ High Pressure <u>550</u> |  |
| Alco Test Values  | <u>.085</u> ✓<br>1st Alco                  |
|   | <u>.084</u> ✓<br>2nd Alco                  |
| Signature <u>[Handwritten Signature]</u>                                      | <u>[Handwritten Initials]</u><br>8/12/10   |

(OVER)

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) **The referenced instrument is certified for evidentiary use in the State of Alaska.**

[Handwritten Signature]  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 23<sup>rd</sup> day of SEPT, 2010.

[Handwritten Signature] (Notary Seal Stamp)  
 Daniel L. Nicholas  
 Notary Public, State of Alaska  
 Commission Expires with Office

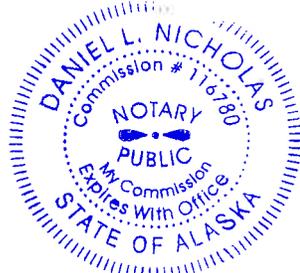

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130296  
COB 8/12/10

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130296

AUGUST 03, 2010

COB  
8/12/10

OPERATOR'S NAME:  
WALDRON, JOHN J  
OPERATOR'S NUMBER: 3352  
SUBJECT'S LAST NAME:  
UOC  
SUBJECT'S FIRST NAME/MI :  
UOC  
U.L. #: 0123456789  
DEPT/AGENCY: UNK1  
CASE/REPORT: 10-00000  
TEST TYPE: U  
ALCO TARGET VALUE: .002  
ALCO S/N: 78966

--- BREATH ANALYSIS ---

|                            |          |       |
|----------------------------|----------|-------|
| .002 ADJUSTED FOR 30.09 in |          |       |
| ALCO TARGET                | .002     | 23:38 |
| BLANK TEST                 | .000     | 23:39 |
| INTERNAL STANDARD          | VERIFIED | 23:39 |
| ALCO TV 30.09 in           | .035     | 23:40 |
| BLANK TEST                 | .000     | 23:40 |
| SUBJECT SAMPLE             | .000     | 23:41 |
| BLANK TEST                 | .000     | 23:42 |
| ALCO TV 30.09 in           | .004     | 23:42 |
| BLANK TEST                 | .000     | 23:43 |

COB  
8/12/10

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130296

AUGUST 03, 2010  
TIME 23:44

--- DIAGNOSTIC CHECK ---

|                  |          |
|------------------|----------|
| COMPUTER:        | OKAY     |
| PROGRAM:         | OKAY     |
| SOFTWARE DATE:   | 02/20/01 |
| HEATERS          |          |
| SAMPLE CHAMBER:  | 40c      |
| BREATH TUBE:     | 40c      |
| PAPOMETER:       | 30.09 in |
| FLOW DETECTOR:   | OKAY     |
| PUMP             |          |
| HIGH SPEED:      | OKAY     |
| DETECTOR:        | OKAY     |
| FILTERS:         | OKAY     |
| QUARTZ STANDARD: | OKAY     |
| CALIBRATION:     | OKAY     |

PRINTER TEST

!@#%?'( )+ , - . : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~ ¡ ¢ £ ¤ ¥ ¦ § ¨ © ª « ¬ ® ¯ ° ± ² ³ ´ µ ¶ · ¸ ¹ º » ¼ ½ ¾