

MAR 9 9 2011

# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument  
State of Alaska*

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

DataMaster cdm S/N <u>130300</u>	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>JEREMY FERNANDES</u>	ID# <u>6345</u> Date <u>11-20-10</u>
A Agency <u>FORT YUKON POLICE</u> Phone # <u>662-2311</u>	
Instrument Location <u>FORT YUKON</u>	
B Alco S/N <u>K124617</u> Target Value <u>.084</u> High Pressure <u>450</u>	
Alco Test Values	<u>.090</u> <u>.085</u>
1st Alco	2nd Alco
Signature <u>[Handwritten Signature]</u>	<u>ZF</u> <u>3/8/11</u>

(OVER)

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Handwritten Signature]  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 9<sup>th</sup> day of MAR, 2011.

[Handwritten Signature] (Notary Seal Stamp)  
 Daniel L. Nicholas  
 Notary Public, State of Alaska  
 Commission Expires with Office

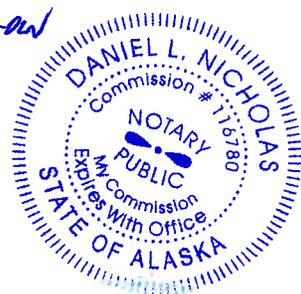

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130300

NOVEMBER 20, 2010

OPERATOR'S NAME:  
FERNANDES/JEREMY/GILMORE  
OPERATOR'S NUMBER: 6345  
SUBJECT'S LAST NAME:  
VERIFICATION  
SUBJECT'S FIRST NAME/NI :  
OF/CAL

O.L. #: 0000000  
DEPT/AGENCY: FVUI  
CASE/REPORT: 10-00  
TEST TYPE: U  
ALCO TARGET VALUE: .004  
ALCO S/N: X124617

### — BREATH ANALYSIS —

.004 ADJUSTED FOR 29.99 in  
ALCO TARGET .004 22:18  
BLANK TEST .000 22:19  
INTERNAL STANDARD VERIFIED 22:19  
ALCO TV 29.98 in .090 22:20  
BLANK TEST .000 22:20  
SUBJECT SAMPLE .000 22:21  
BLANK TEST .000 22:22  
ALCO TV 29.99 in .008 22:22  
BLANK TEST .000 22:23

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130300

NOVEMBER 20, 2010  
TIME 22:15

### — DIAGNOSTIC CHECK —

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 29.99 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
BLANKET STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@ABCDEF  
HIJKLMNOPQRSTUVWXYZ[\]^\_`abcde fghijklmnop  
qrstuvwxy z{|}~