

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument


State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130301</u>
Name		<u>STEVE DUNN</u>	ID# <u>4106</u> Date <u>3-18-08</u>
A	Agency	<u>APD</u>	Phone # <u>786-8900</u>
Instrument Location		<u>ANCHORAGE JAIL</u>	
Alco S/N		<u>78890</u>	Target Value <u>.082</u> High Pressure <u>850</u>
B	Alco Test Value Average		<u>.078</u> <u>.078</u>
		1 st Alco	2 nd Alco
Signature		<u>[Signature]</u> <u>03/24/08</u>	
(OVER)			

Under the Alaska Rules of Evidence, I certify that:
(Do Not write in the area below)

- (a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.
- (b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Steve P Dunn, whose name appears in my records, is qualified to verify the calibration of the above instrument.
- (c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

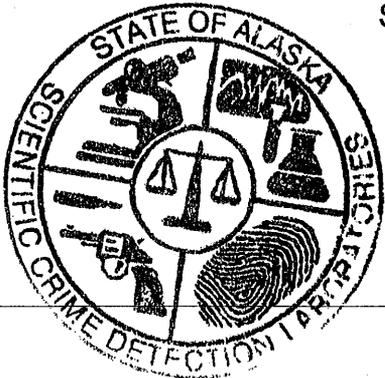

Signed and sealed,

[Signature]

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

3/24/08
Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130301

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

S. DUNN #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130301

MARCH 18, 2008 *COB 3/21/08*

OPERATOR'S NAME: *DUNN/S*
OPERATOR'S NUMBER: 4106
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
U
O.L. #: U
DEPT/AGENCY: ANCI
CASE/REPORT: U
TEST TYPE: U
ALCO TARGET VALUE: .082
ALCO S/N: 78890

--- BREATH ANALYSIS ---

.082 ADJUSTED FOR 29.60 in		
ALCO TARGET	.081	10:39
BLANK TEST	.000	10:40
INTERNAL STANDARD	VERIFIED	10:40
ALCO TU 29.59 in	.078	10:41
BLANK TEST	.000	10:41
SUBJECT SAMPLE	.000 <i>COB 3/21/08</i>	10:42
BLANK TEST	.000	10:43
ALCO TU 29.60 in	.078	10:43
BLANK TEST	.000	10:44

80/1/08

DIAGNOSTIC CHECK

S. DUNN #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130301

MARCH 18, 2008
TIME 10:36

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01

HEATERS
SAMPLE CHAMBER: 40c
BREATH TUBE: 41c

BAROMETER: 29.59 in

FLOW DETECTOR: OKAY

PUMP
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST
!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~||