

DEC 24 2008

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130302 ✓

Name Sgt. Kevin Nelson ID# 5349 Date 12/20/08 ✓ CAMS ✓  
12-29

A Agency North Pole Police Department Phone # (907)488-0612

Instrument Location 125 Snowman Lane, North Pole, AK 99705 ✓

---

B Alco S/N X17298E ✓ Target Value .080 ✓ High Pressure 900 psi

Alco Test Values .080 ✓ .082 ✓  
1<sup>st</sup> Alco 2<sup>nd</sup> Alco

Signature [Signature] ✓ CDB  
12/30/08


(OVER)

Under the Alaska Rules of Evidence, I certify that, (Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Kevin Nelson, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

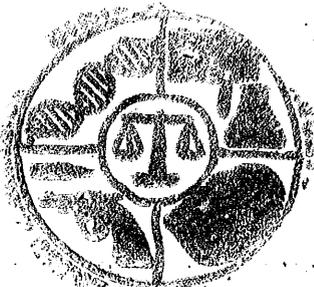

Signed and sealed

[Signature]

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

12/31/08

Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130302 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130302

DECEMBER 29, 2008

OPERATOR'S NAME:  
NELSON, KEVIN HOON  
OPERATOR'S NUMBER: 5349  
SUBJECT'S LAST NAME:

VOC  
SUBJECT'S FIRST NAME/MI :  
VOC

D.L. #: 0000000  
DEPT/AGENCY: MPL  
CASE/REPORT: 08-000  
TEST TYPE: V  
ALCO TARGET VALUE: .000 ✓  
ALCO S/N: X172988

### --- BREATH ANALYSIS ---

.000 ADJUSTED FOR 29.99 in  
ALCO TARGET .000 12:49  
BLANK TEST .000 12:50  
INTERNAL STANDARD VERIFIED 12:50  
ALCO TV 29.99 in .000 ✓ 12:51  
BLANK TEST .000 12:52  
SUBJECT SAMPLE .000 12:53  
BLANK TEST .000 12:54  
ALCO TV 29.99 in .002 ✓ 12:54  
BLANK TEST .000 12:55

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130302

DECEMBER 29, 2008 ✓  
TIME 11:56

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c  
BAROMETER: 29.99 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF  
HIJKL MNOPQRSTUVWXYZ[\]^\_`abcde fghi jklmno  
pqrstuvwxyz{|}~`