

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N <u>130305</u> ✓		
Name <u>ANDRE ACHEE</u>	ID# <u>2385</u> Date <u>8-15-2008</u> ✓	
A Agency <u>BETHEL POLICE DEPARTMENT</u> Phone # <u>543-3781</u>		
Instrument Location <u>BPD SQUAD ROOM</u> ✓		
B Alco S/N <u>X172939</u> ✓ Target Value <u>.081</u> ✓ High Pressure <u>400 PSI</u>		
Alco Test Values	<u>.081</u> ✓ 1 <sup>st</sup> Alco	<u>.081</u> ✓ 2 <sup>nd</sup> Alco
Signature	 ✓ <u>ACHEE / BPD</u>	<u>MS</u> <u>8/29/08</u>
(OVER)		

Under the Alaska Rules of Evidence, I certify that, (Do Not write in the area below)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Andre Achee, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

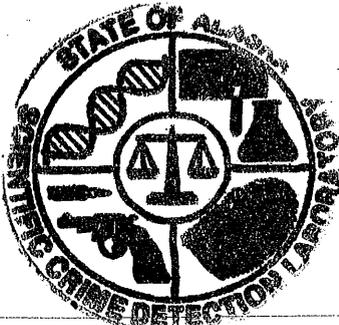

Signed and sealed,



Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

9/2/08

Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130305 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130305

AUGUST 15, 2008

OPERATOR'S NAME: ACHEE/ANDRE/A  
OPERATOR'S NUMBER: 2385  
SUBJECT'S LAST NAME: TEST  
SUBJECT'S FIRST NAME/MI: VCR  
O.L. #: 1234567  
DEPT/AGENCY: BET1  
CASE/REPORT: XX-XXXX  
TEST TYPE: T  
ALCO TARGET VALUE: .081  
ALCO S/N: X172939

### --- BREATH ANALYSIS ---

.081 ADJUSTED FOR 30.14 in  
ALCO TARGET .081 06:31  
BLANK TEST .000 06:33  
INTERNAL STANDARD VERIFIED 06:33  
ALCO TV 30.14 in .081 06:33  
BLANK TEST .000 06:34  
SUBJECT SAMPLE .000 06:34  
BLANK TEST .000 06:35  
ALCO TV 30.16 in .081 06:36  
BLANK TEST .000 06:36

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130305

AUGUST 15, 2008 ✓  
TIME 06:38

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 48c  
BREATH TUBE: 42c  
BAROMETER: 30.16 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJK  
LMNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnop  
qrstuvwxyz{|}~