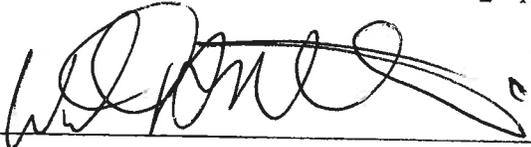


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130305</u>
Name	<u>William Mills</u>	ID# <u>2688</u> Date <u>8/5/11</u>
A Agency	<u>Hoonah Police Dept</u>	Phone # <u>9079453655</u>
Instrument Location	<u>379 Raven Drive, Hoonah Ak</u>	
B Alco S/N	<u>X301532</u>	Target Value <u>.082</u> High Pressure <u>400</u>
Alco Test Value Average	<u>.088</u> 1 <sup>st</sup> Alco	<u>.088</u> 2 <sup>nd</sup> Alco
Signature		


(OVER)

BMB  
8/15/11

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

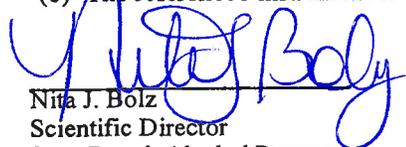  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 18 day of Aug, 2011 <sup>NJB</sup>

  
(Notary Seal Stamp)  
Daniel L. Nicholas Nikki Roth  
Notary Public, State of Alaska  
Commission Expires with Office

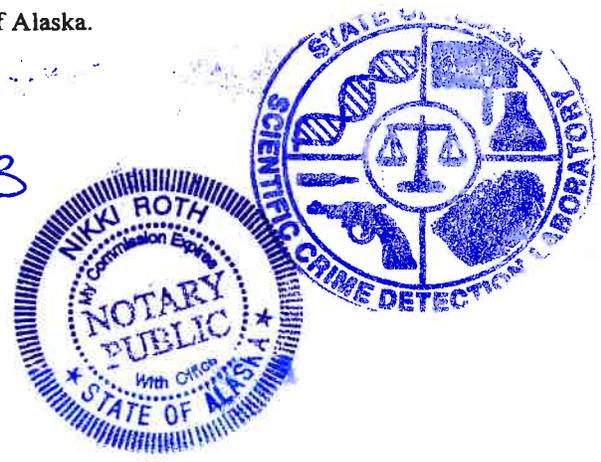

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130305

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130305

AUGUST 06, 2011 *Bmb 8/15/11*

OPERATOR'S NAME:  
MILLS WILLIAM A  
OPERATOR'S NUMBER: 2688  
SUBJECT'S LAST NAME:  
VERIFICATION OF  
SUBJECT'S FIRST NAME/MI :  
CALIBRATION  
O.L. #: 1234567890  
DEPT/AGENCY: HNH1  
CASE/REPORT: 1234567890  
TEST TYPE: U  
ALCO TARGET VALUE: .002  
ALCO S/N: X301532

— BREATH ANALYSIS —

.002 ADJUSTED FOR 30.32 in		
ALCO TARGET	.003	17:49
BLANK TEST	.000	17:50
INTERNAL STANDARD	VERIFIED	17:50
ALCO TU 30.32 in	.000	17:51
BLANK TEST	.000	17:51
SUBJECT SAMPLE <i>Bmb 8/15/11</i>	.000	17:52
BLANK TEST	.000	17:53
ALCO TU 30.33 in	.000	17:53
BLANK TEST	.000	17:54

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130305

AUGUST 06, 2011 *Bmb 8/15/11*  
TIME 17:56

— DIAGNOSTIC CHECK —

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 40c  
BREATH TUBE: 43c  
BAROMETER: 30.32 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST  
!@#%&'()\*+,-./0123456789:;<=?@BCDEF6  
HIJKL NOPQRSTU VWXYZ[\]^\_`abcdefg h i j k l m n o  
p q r s t u v w x y z { | } ~