

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

MAR 11 2010

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

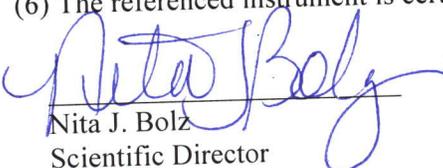
Supervisor/Operator Performing the Verification Procedure:	
DataMaster cdm S/N <u>130306</u>	
Name <u>STEVE DUNN</u> ID# <u>4106</u> Date <u>3-11-10</u>	
A	Agency <u>APD</u> Phone # <u>764-1361</u>
Instrument Location <u>4th AVE SUB</u>	
Alco S/N <u>58428</u> Target Value <u>.084</u> High Pressure <u>1000 Psi</u>	
B	Alco Test Value Average <u>.078</u> <u>.079</u>
	1 <sup>st</sup> Alco 2 <sup>nd</sup> Alco
Signature 	
(OVER)	

BMB  
3/18/2010

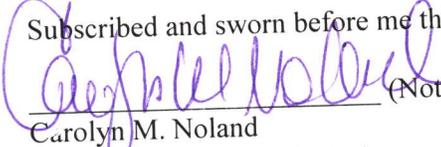
(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 2nd day of April, 2010.

  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130306 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

S. DUNN #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130306 ✓

MARCH 11, 2010 ✓ *BMS 3/18/2010*

OPERATOR'S NAME:  
DUNN/S

OPERATOR'S NUMBER: 4106

SUBJECT'S LAST NAME:  
VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :  
U

O.L. #: U

DEPT/AGENCY: ANCI

CASE/REPORT: U

TEST TYPE: U

ALCO TARGET VALUE: .084 ✓

ALCO S/N: 58428 ✓

### — BREATH ANALYSIS —

.084 ADJUSTED FOR 29.25 in ✓

ALCO TARGET	.082	08:55
BLANK TEST	.000	08:56
INTERNAL STANDARD	VERIFIED	08:56
ALCO TV 29.25 in	.078	08:57
BLANK TEST	.000	08:57
SUBJECT SAMPLE	.000	08:58
BLANK TEST	.000	08:59
ALCO TV 29.25 in	.079	08:59
BLANK TEST	.000	09:00

*BMS 3/18/2010*

## DIAGNOSTIC CHECK

S. DUNN #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130306 ✓

MARCH 11, 2010 ✓

TIME 08:51

### — DIAGNOSTIC CHECK —

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/28/01
HEATERS	
SAMPLE CHAMBER:	42c
BREATH TUBE:	42c
BAROMETER:	29.25 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

### PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@ABCDEFG  
HIJKL NOPQRSTU VWXYZ[\]^\_`'abc defghijklmno  
pqrstuvwxyz{|}~@