

MAR 03 2008

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

		DataMaster cdm S/N <u>130404</u> ✓	
Supervisor/Operator Performing the Verification Procedure:			
Name <u>ERIC C. WALLA</u>		ID# <u>5505</u>	Date <u>2008/02/19</u>
A	Agency <u>FORT GREELY POLICE DEPARTMENT</u>		Phone # <u>907-873-9135</u>
Instrument Location <u>663 FIRST STREET FORT GREELY, ALASKA 99731</u>			
Alco S/N <u>X301581</u> ✓		Target Value <u>.080</u> ✓	High Pressure <u>500 PSI</u>
B	Alco Test Values		
	<u>.075</u>	<u>.075</u>	
	1 st Alco	2 nd Alco	
Signature <u><i>Eric C Walla</i></u>		<u>CSB</u> <u>3/6/08</u>	
(OVER)			


(Do Not write in the area below)

Under the Alaska Rules of Evidence, I certify that;

(a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Eric C Walla, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

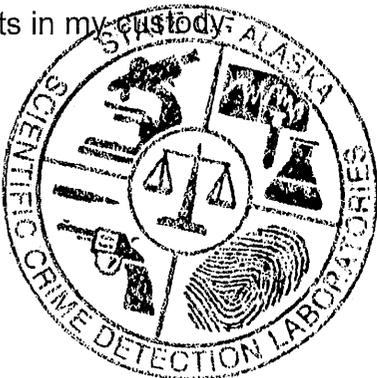

Signed and sealed,

J Swartz

3/6/08

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

Date

✓

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130404 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130404

FEBRUARY 19, 2008

OPERATOR'S NAME: *CSB 2/16/08*
WALLA ERIC C
OPERATOR'S NUMBER: 5505
SUBJECT'S LAST NAME:

VOC
SUBJECT'S FIRST NAME/MI :
X

O.L. #: 19FEB2007
DEPT/AGENCY: B164
CASE/REPORT: VOC19FEB08
TEST TYPE: V
ALCO TARGET VALUE: .000
ALCO S/N: X301581

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 27.96 in
ALCO TARGET .074 16:47
BLANK TEST .000 16:48
INTERNAL STANDARD VERIFIED 16:48
ALCO TV 27.96 in .075 16:49
BLANK TEST .000 16:49
SUBJECT SAMPLE .000 *CSB 2/16/08* 16:51
BLANK TEST .000 16:52
ALCO TV 27.95 in .075 16:52
BLANK TEST .000 16:53

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130404

FEBRUARY 19, 2008
TIME 16:44

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 27.96 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! "# % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~