

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

AUG 18 2009

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130567 ✓
A	Name	Tyron Walker	ID# 4555 Date 8/14/09
	Agency	Ketchikan Police Dept.	Phone # 225-6631
	Instrument Location	3601 Main St.	✓
B	Alco S/N	X124662 ✓	Target Value .080 High Pressure 900
	Alco Test Values	.085 ✓ 1 <sup>st</sup> Alco	.086 ✓ 2 <sup>nd</sup> Alco
	Signature	Tyron Walker	COB 8/27/09

(OVER)

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

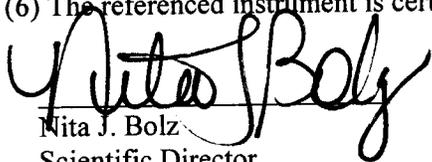


Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 29<sup>th</sup> day of Sept, 2009.

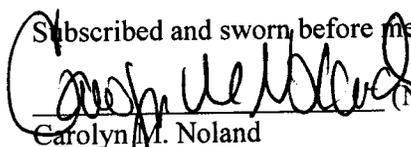  
(Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

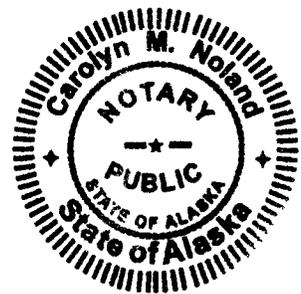

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130567

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130567

AUGUST 14, 2009

OPERATOR'S NAME:

WALKER TY

OPERATOR'S NUMBER: 4555

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

T

O.L. #: 12345

DEPT/AGENCY: KET1

CASE/REPORT: 09-1234

TEST TYPE: V

ALCO TARGET VALUE: .000

ALCO S/N: X124662

### --- BREATH ANALYSIS ---

.000 ADJUSTED FOR 30.27 in ✓  
ALCO TARGET .000 06:41  
BLANK TEST .000 06:41  
INTERNAL STANDARD VERIFIED 06:41  
ALCO TV 30.27 in .005 ✓ 06:42  
BLANK TEST .000 06:43  
SUBJECT SAMPLE .000 06:43  
BLANK TEST .000 06:44  
ALCO TV 30.27 in .006 ✓ 06:45  
BLANK TEST .000 06:46

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130567

AUGUST 14, 2009

TIME 06:38

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 50c  
BREATH TUBE: 42c  
BAROMETER: 30.27 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJ  
KLMNOPQRSTUVWXYZ[\]^\_`abcde fghijklmno  
pqrstuvwxyz{|}~>