


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

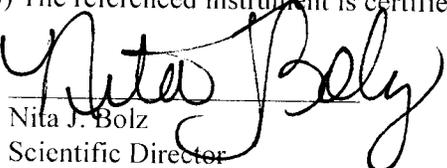
OCT 15 2009

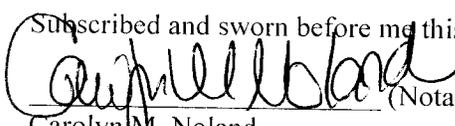
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130578
Name	Malik Jones	ID#	5830
Date	10/10/09	Phone #	451-5100
Agency	AST	Instrument Location	Cantwell
Alco S/N	X172969	Target Value	.085
High Pressure	1300 PSI	Alco Test Value Average	.077
1 <sup>st</sup> Alco		2 <sup>nd</sup> Alco	.078
Signature			


CMB  
10/21/09

(OVER)

- I, Nita J. Bolz, after being first duly sworn, depose and state as follows (to be read in the area below)
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
  - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
  - (3) I am the Scientific Director of the State Breath Alcohol Program.
  - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
  - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
  - (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 10th day of Nov., 2009.  
  
(Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130578

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130578

OCTOBER 10, 2009

OPERATOR'S NAME:

JONES/MALIK/JAMAL

OPERATOR'S NUMBER: 5830

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

Y

D.L. #: 1

DEPT/AGENCY: ONT

CASE/REPORT:

TEST TYPE: V

ALCO TARGET VALUE: .065

ALCO S/N: K172953

--- BREATH ANALYSIS ---

.065 ADJUSTED FOR 27.93 in

ALCO TARGET	.079	14:19
BLANK TEST	.000	14:20
INTERNAL STANDARD	VERIFIED	14:20
ALCO @ 27.93 in	.077	14:20
BLANK TEST	.000	14:21
SUBJECT SAMPLE	.060	14:22
BLANK TEST	.000	14:23
ALCO @ 27.95 in	.078	14:23
BLANK TEST	.000	14:24

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130578

OCTOBER 10, 2009  
TIME 14:27

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	58c
BREATH TUBE:	42c
BAROMETER:	27.95 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

#####(0)#####(0130456789)#####>8BDCDEF6  
#####(0)#####(0130456789)#####>8BDCDEF6  
#####(0)#####(0130456789)#####>8BDCDEF6