

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N <u>130579</u> ✓	
A	Name <u>STEVE DUNN</u> ID# <u>4106</u> Date <u>1-5-09</u> ✓
	Agency <u>APD</u> Phone # <u>786-8900</u>
	Instrument Location <u>ANCHORAGE JAIL</u>
B	Alco S/N <u>70729</u> ✓ Target Value <u>.076</u> ✓ High Pressure <u>650</u>
	Alco Test Value Average <u>.079</u> ✓ <u>.079</u> ✓
	1 st Alco 2 nd Alco
	Signature <u>[Signature]</u> <u>CS</u>
	<u>1/9/09</u>
(OVER)	


Under the Alaska Rules of Evidence, I certify that:
(Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Steve P Dunn, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

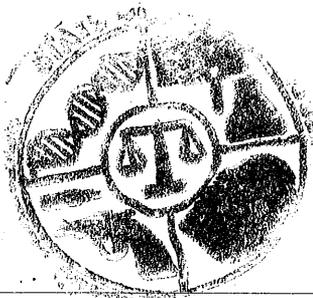

[Signature]

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

1/10/09
Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130579 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

S. Dunn #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130579

JANUARY 05, 2009 ✓ *COB 1/9/09*

OPERATOR'S NAME:
DUNN/S

OPERATOR'S NUMBER: 4106

SUBJECT'S LAST NAME:
VERIFICATION OF CAL

SUBJECT'S FIRST NAME/NI:
V

O.L. #: V

DEPT/AGENCY: ANCI

CASE/REPORT: V

TEST TYPE: V

ALCO TARGET VALUE: .076 ✓

ALCO S/N: 70729

--- BREATH ANALYSIS ---

.076 ADJUSTED FOR 29.67 in		
ALCO TARGET	.075	11:07
BLANK TEST	.000	11:08
INTERNAL STANDARD	VERIFIED	11:08
ALCO TV 29.67 in	.079 ✓	11:08
BLANK TEST	.000	11:09
SUBJECT SAMPLE <i>COB 1/9/09</i>	.000	11:09
BLANK TEST	.000 ✓	11:10
ALCO TV 29.67 in	.079	11:10
BLANK TEST	.000	11:11

DIAGNOSTIC CHECK

S. Dunn #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130579

JANUARY 05, 2009 ✓

TIME 11:05

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	12/11/08
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	42c
BAROMETER:	29.67 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

"#%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmnop
qrstuvwxy{|}~"