

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAR 02 2009

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130579 ✓
Name	C. RITALA	ID#	3791 Date 2/28/09 ✓
A Agency	APD	Phone #	786-2640
Instrument Location	ANCHORAGE JAIL ✓		
B Alco S/N	X124630 ✓	Target Value	.084 ✓ High Pressure 1200
Alco Test Values	.084 ✓ 1 st Alco	.085 ✓ 2 nd Alco	
Signature	Chris Ritala / 1349 ✓		CS 3/24/09

(OVER)


Under the Alaska Rules of Evidence, I certify that:
(Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Chris Ritala, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

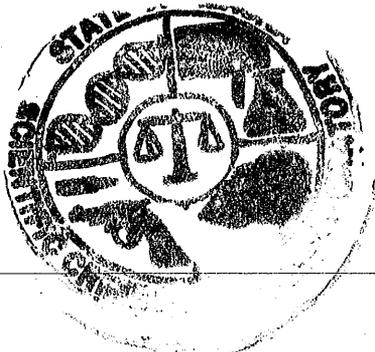

Jeanne Swartz

Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

3/24/09

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAR 02 2009

DataMaster cdm S/N 130579 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130579

FEBRUARY 28, 2009

OPERATOR'S NAME: *OS 3/24/09*
RITALA

OPERATOR'S NUMBER: 3791

SUBJECT'S LAST NAME:
VERIFICATION OF CALIBRATION

SUBJECT'S FIRST NAME/MI:
NEWALCO

O.L. #: X

DEPT/AGENCY: ANCI

CASE/REPORT: X

TEST TYPE: V

ALCO TARGET VALUE: .084 ✓

ALCO S/N: X124630 ✓

--- BREATH ANALYSIS ---

.084 ADJUSTED FOR 30.46 in		
ALCO TARGET	.085	00:11
BLANK TEST	.000	00:12
INTERNAL STANDARD	VERIFIED	00:12
ALCO TV 30.46 in	.084 ✓	00:12
BLANK TEST	.000	00:13
SUBJECT SAMPLE <i>OS 3/24/09</i>	.000	00:14
BLANK TEST	.000	00:15
ALCO TV 30.46 in	.085 ✓	00:15
BLANK TEST	.000	00:16

OS 3/24/09

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130579

FEBRUARY 28, 2009 ✓
TIME 00:07

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	12/11/08
HEATERS:	
SAMPLE CHAMBER:	49c
BREATH TUBE:	48c
BAROMETER:	30.45 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST
!@#%&'()*+,-./0123456789:;<=>?@ABCDEF
HIJKLMNOPQRSTUVWXYZ[\]^_`abcde fghi jklmno
pqrstuvwxyz{|}~

OS 3/24/09