

DEC 17 2007

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130666

Supervisor/Operator Performing the Verification Procedure:
 Name Matthew L. Soden ID# 3378 Date 12-13-2007

A
 Agency Fairbanks Police Department Phone # (907) 459-6500
 Instrument Location 911 Cushman St. Fairbanks, AK 99701

B
 Alco S/N 78890 Target Value .078 High Pressure 800 psi

Alco Test Values	0.078008 0.07777 1 st Alco	0.080008 0.078 2 nd Alco
------------------	---	---

Signature [Handwritten Signature] [Handwritten Signature]
12/17/07


(OVER)

(Do Not write in the area below)

Under the Alaska Rules of Evidence, I certify that;

- (a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.
- (b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Matthew Soden, whose name appears in my records, is qualified to verify the calibration of the above instrument.
- (c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

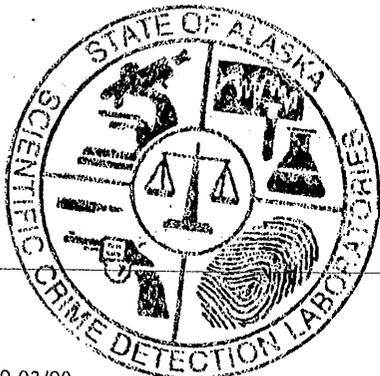

[Handwritten Signature]

Jeanne Swartz
 Scientific Director Designee
 State of Alaska
 State Breath Alcohol Testing Program

12/19/07
 Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130666

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130666

DECEMBER 13, 2007

OPERATOR'S NAME:

SOBEN, MATTHEW L.

OPERATOR'S NUMBER: 3378

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/NI :

X

O.L. #: X

DEPT/AGENCY: FBK1

CASE/REPORT: X

TEST TYPE: V

ALCO TARGET VALUE: .078

ALCO S/N: 73090

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 29.88 in

ALCO TARGET	.077	04:13
BLANK TEST	.000	04:13
INTERNAL STANDARD	VERIFIED	04:14
ALCO TV 29.88 in	.078	04:14
BLANK TEST	.000	04:15
SUBJECT SAMPLE	.000	04:16
BLANK TEST	.000	04:16
ALCO TV 29.88 in	.030	04:17
BLANK TEST	.000	04:18

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130666

DECEMBER 13, 2007

TIME 04:08

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 29.88 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!#\$%&'()*+,-./0123456789:;<=>@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmnop
qrstuvwxyz{|}~