

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

JUL 13 2010

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

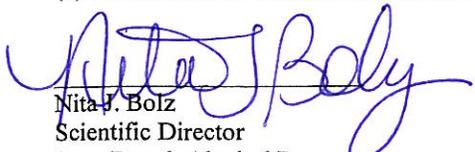
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130666 ✓
Name	Burlyn C Rigdon Jr.	ID#	4154 ✓
		Date	07/08/2010 ✓
A	Agency	Fairbanks Police Dept	Phone # (907) 450-6500
	Instrument Location	911 Cushman Street Fairbanks, AK 99701	
B	Alco S/N	X301599 ✓	Target Value .081 ✓
			High Pressure 200 psi
	Alco Test Values	.082 ✓	.082 ✓
		1 st Alco	2 nd Alco
	Signature		 7/15/10

(OVER)

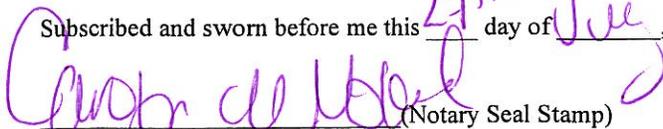
(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 27th day of July, 2010.


(Notary Seal Stamp)

Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

BT9 06/03



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130666

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130666

JULY 08, 2010

OPERATOR'S NAME:

RIGDON BURLYN C

OPERATOR'S NUMBER: 4154

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI :

VOC

O.L. #: 00000

DEPT/AGENCY: FBK1

CASE/REPORT: 0000

TEST TYPE: V

ALCO TARGET VALUE: .001

ALCO S/N: X301599

--- BREATH ANALYSIS ---

.001 ADJUSTED FOR 29.88 in
ALCO TARGET .000 02:25
BLANK TEST .000 02:26
INTERNAL STANDARD VERIFIED 02:26
ALCO TV 29.88 in .002 02:27
BLANK TEST .000 02:27
SUBJECT SAMPLE .000 02:28
BLANK TEST .000 02:29
ALCO TV 29.88 in .002 02:29
BLANK TEST .000 02:30

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130666

JULY 08, 2010

TIME 02:31

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 03/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 29.88 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < (=) ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } + ~