



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories

Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100671

Report Issue Date: 07/19/2023
Date Received: 2023-01-25
Condition of Item: Good

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

Start Date 01/25/2023 - As Found - End Date 01/25/2023 As Found - Evaluation Analyst: Colleen O'Bryant
 As Found Conditions - Barometric Pressure (inHg): 29.39 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.3
 Relative Humidity (%): 21

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.019	0.020	0.020	0.020	0.019	0.020	
0.080	0.079	AG113402	0.077	0.078	0.078	0.078	0.078	0.078	
0.300	0.295	AG217903	0.295	0.296	0.296	0.295	0.295	0.295	

Start Date 06/27/2023 - As Left - End Date 06/27/2023
 As Left Conditions - Barometric Pressure (inHg): 29.61 Barometer Used: Fisher S/N 221250180 Temperature (C): 23.2 Relative
 Humidity (%): 40

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.020	0.020	0.020	0.019	0.020	0.020	+/- 0.002
0.040	0.040	AG217904	0.040	0.040	0.039	0.039	0.039	0.039	+/- 0.003
0.080	0.079	09523080A1	0.079	0.079	0.079	0.079	0.079	0.079	+/- 0.004
0.100	0.099	AG211003	0.099	0.099	0.099	0.098	0.098	0.099	+/- 0.004
0.150	0.148	AG134205	0.148	0.148	0.148	0.148	0.148	0.148	+/- 0.005
0.300	0.297	AG217903	0.297	0.297	0.298	0.297	0.298	0.297	+/- 0.011

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Colleen O'Bryant on 07/06/2023

colleen.obryant@alaska.gov

Technically and administratively reviewed by Brandi Barnett on 07/19/2023

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100671

Analyst: Tatiana Malnoche

Start Date: 06/27/2023

- Diagnostic Test (attached)
- Adjust voltages, if needed
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
- Internal Standard value \leq 3.00%
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)

- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.6 L (1.3L to 1.7L)

Data Interpretation

06/27/2023

2023.07.06

TLM

COB

As Left Conditions:

Barometric Pressure (in Hg): 29.63 Temperature (C): 23.2 Relative Humidity (%): 40%

Linearity Test (attached)

0.020g/210L Mnf:	<u>Airgas</u>	Lot: <u>AG217902</u>	Exp: <u>06/28/2024</u>
0.040g/210L Mnf:	<u>Airgas</u>	Lot: <u>AG217904</u>	Exp: <u>06/28/2024</u>
0.080g/210L Mnf:	<u>ILMD</u>	Lot: <u>09523080A1</u>	Exp: <u>05/05/2025</u>
0.100g/210L Mnf:	<u>Airgas</u>	Lot: <u>AG211003</u>	Exp: <u>04/20/2024</u>
0.150g/210L Mnf:	<u>Airgas</u>	Lot: <u>AG134205</u>	Exp: <u>12/08/2023</u>
0.300g/210L Mnf:	<u>Airgas</u>	Lot: <u>AG217903</u>	Exp: <u>06/28/2024</u>

Functional Tests (attached)

- Incomplete
 - Maximum Attempts Exceeded
 - Interference (Volatiles)
 - Invalid
 - Radio Frequency Interference (RFI)
- Acetone Mnf: Lifeloc Lot: 22HP41201 Level: 0.100 Exp: 08/24/2024
Simulator S/N: DR4176 Verification Performed?
- Isopropanol Mnf: Lifeloc Lot: 22HP41201 Level: 0.100 Exp: 08/24/2024
Simulator S/N: DR4177 Verification Performed?
- Neg. Control Mnf: Lifeloc Lot: 21KP41172 Level: 0.100 Exp: 11/09/2023
Simulator S/N: DR6267 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 210958384 Calibration Due Date: 11/09/2023

- Verify stylus is calibrated
 - Reset Options
 - Clear Memory
 - Verification of Calibration (VOC)
 - Non-Drinking Subject Test
 - Upload
 - Remove Tank Prior to Shutdown
- Calibration End Date: 06/27/2023

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100671

Date: 06/27/2023
Time: 08:01:47

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 47.3°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.67 V PASSED
(1.01 V - 2.37 V)
Cooler Voltage = 1.78 V PASSED
(1.00 V - 2.32 V)
Bias Voltage = 78 V PASSED
(47 V - 111 V)
Chopper Freq = 518 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.6 in

PUMP INFO

Flow Rate = 4.615 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.001 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED
Xq = 0.100 1.69% (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100671

Date: 06/27/2023
Time: 8:08 AM

Temperatures (°C)

Sample Cell: 48.7°C
Breath Tube: 48.0°C

Current Barometer 29.6 in
Volume (Ltr) 1.50

Settings

Lamp: 1.72 V
Bias: 78 V
Cooler: 1.73 V
Chopper: 517 Hz

Voltages (V)

Flow: 1.06 V
Detector: -0.023 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100671

Date: 04/09/2012
Time: 10:19:13

OPERATOR NAME:
CHARLES FOSTER
CERTIFICATE #: 7734

Ca = 0.1000
CAL = 0.981393 0.800 <= CAL < 1.200
b1 = 0.0003 0.0000 <= b1 < 0.0040
b2 = 0.0063 0.0010 <= b2 < 0.0100
b3 = 0.0001 0.0000 <= b3 < 0.0040
Xq = 0.0987 0.0500 <= Xq < 0.2000
a21 = 1.187324 1.050 <= a21 < 1.300
a31 = 0.451266 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100671

Date: 06/27/2023
Time: 08:19:20

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.62: 0.079
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	08:20
BLANK TEST	0.000	08:20
INTERNAL STANDARD	VERIFIED	08:20
EXTERNAL STANDARD	0.079	08:20
BLANK TEST	0.000	08:21
SUBJECT SAMPLE (Vol=1.54L)	0.000	08:22
BLANK TEST	0.000	08:23
EXTERNAL STANDARD	0.079	08:23
BLANK TEST	0.000	08:24

Time

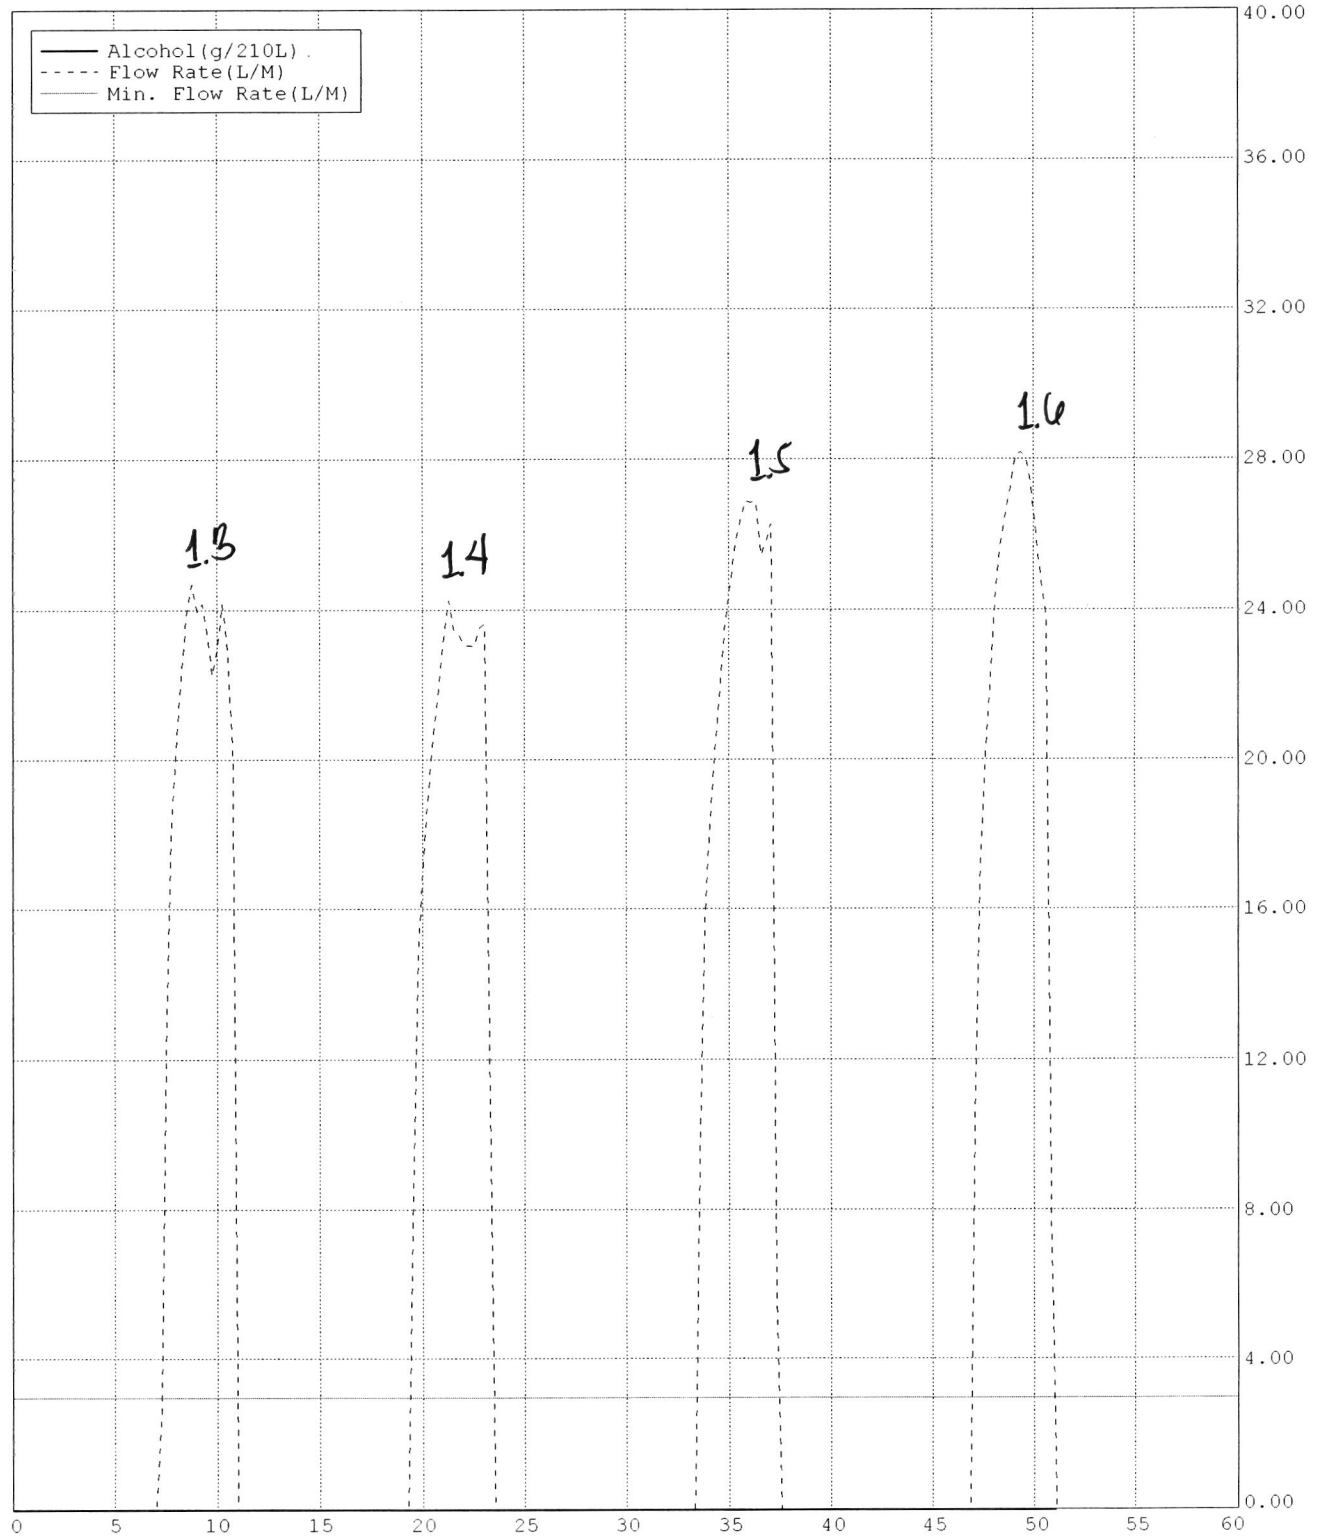

LINEARITY CHECK

Alaska Department of Public Safety
DATAMASTER dmt: 100671


Date: 06/27/2023
Time: 08:29:15

SUPERVISOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

TARGET	AVERAGE	STD. DEV.
0.020	0.0198	0.0004
0.040	0.0394	0.0005
0.079	0.0790	0.0000
0.099	0.0986	0.0005
0.148	0.1480	0.0000
0.297	0.2974	0.0005

SLOPE = 1.002822
R² = 0.999996

TAM

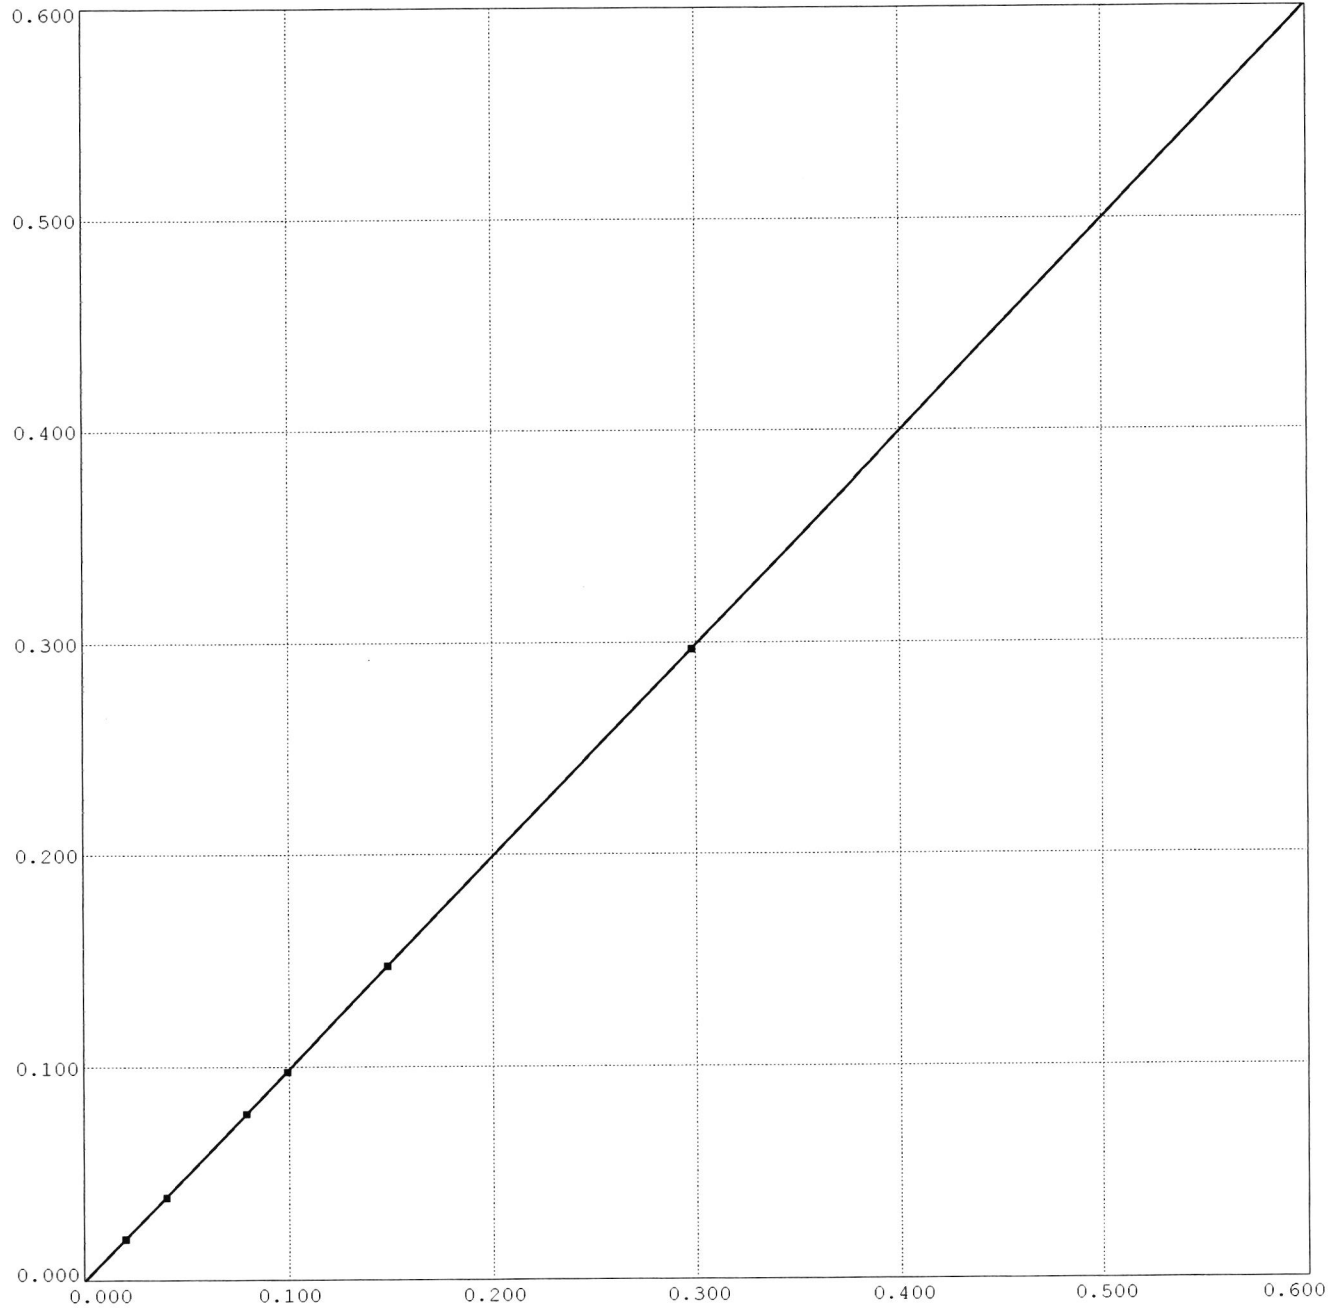

LINEARITY CHECK: Control Test 1

 Alaska Department of Public Safety
 DATAMASTER dmt: 100671






Date: 06/27/2023
 Time: 08:29:17

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 29.62: 0.020
 LOT #: AG217902
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 952 psi

BLANK TEST	0.000	08:30
INTERNAL STANDARD	VERIFIED	08:30
EXTERNAL STANDARD	0.020	08:30
BLANK TEST	0.000	08:31
EXTERNAL STANDARD	0.020	08:32
BLANK TEST	0.000	08:32
EXTERNAL STANDARD	0.020	08:33
BLANK TEST	0.000	08:34
EXTERNAL STANDARD	0.019	08:34
BLANK TEST	0.000	08:35
EXTERNAL STANDARD	0.020	08:35
BLANK TEST	0.000	08:36

Average = 0.0198
 Std Dev = 0.0004

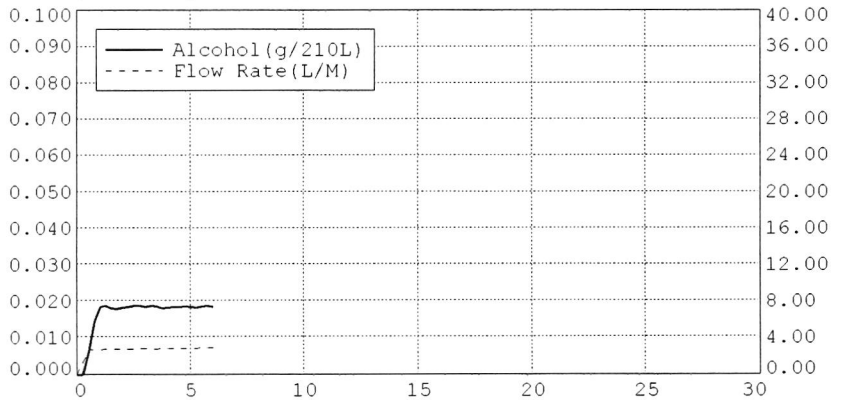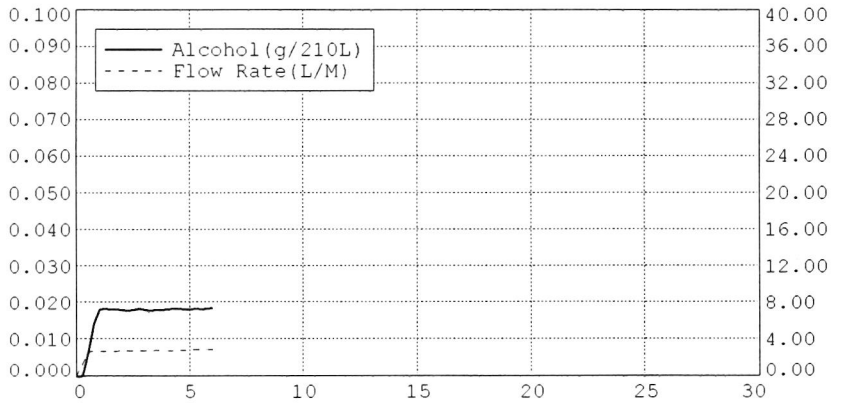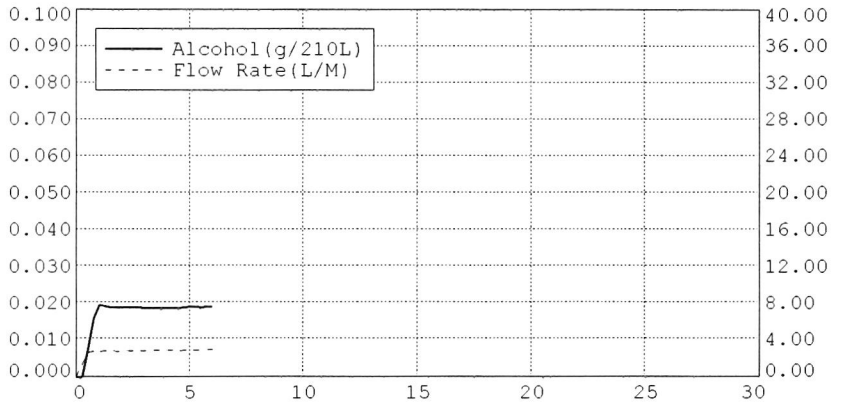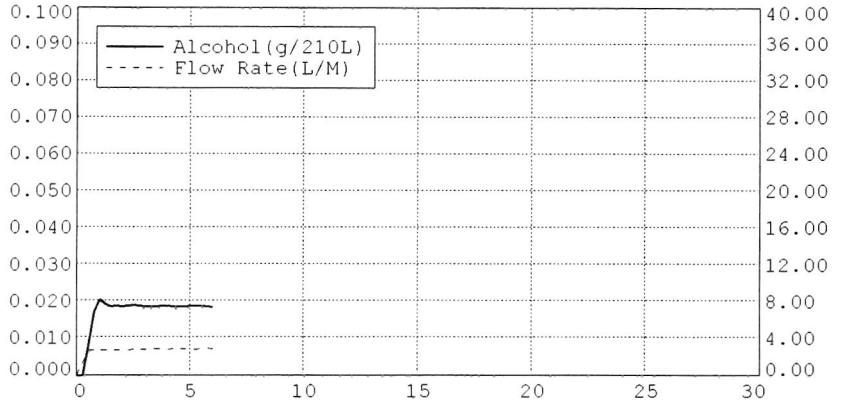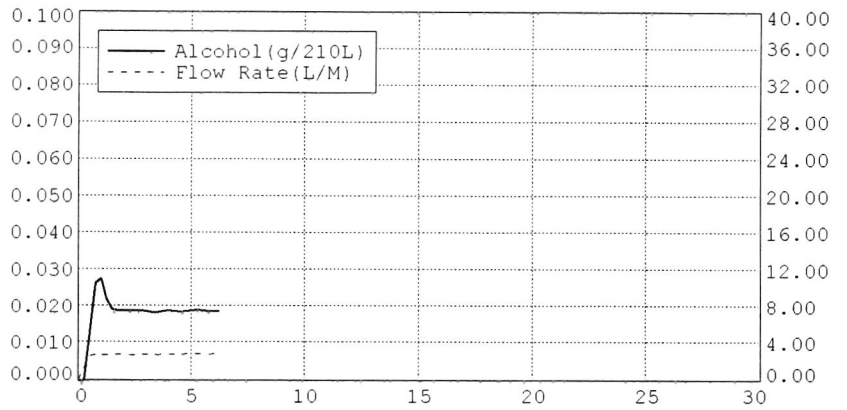

LINEARITY CHECK: Control Test 2

 Alaska Department of Public Safety
 DATAMASTER dmt: 100671






Date: 06/27/2023
 Time: 08:37:20

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 29.62: 0.040
 LOT #: AG217904
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 950 psi

BLANK TEST	0.000	08:38
INTERNAL STANDARD	VERIFIED	08:38
EXTERNAL STANDARD	0.040	08:39
BLANK TEST	0.000	08:39
EXTERNAL STANDARD	0.040	08:40
BLANK TEST	0.000	08:41
EXTERNAL STANDARD	0.039	08:41
BLANK TEST	0.000	08:42
EXTERNAL STANDARD	0.039	08:42
BLANK TEST	0.000	08:43
EXTERNAL STANDARD	0.039	08:43
BLANK TEST	0.000	08:44

Average = 0.0394
 Std Dev = 0.0005

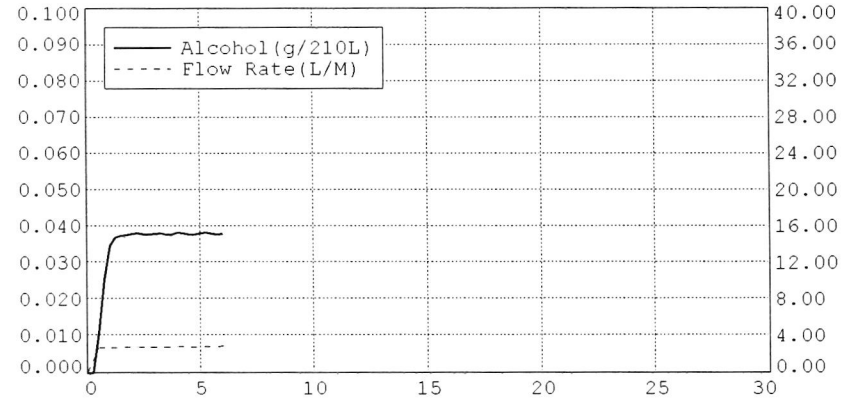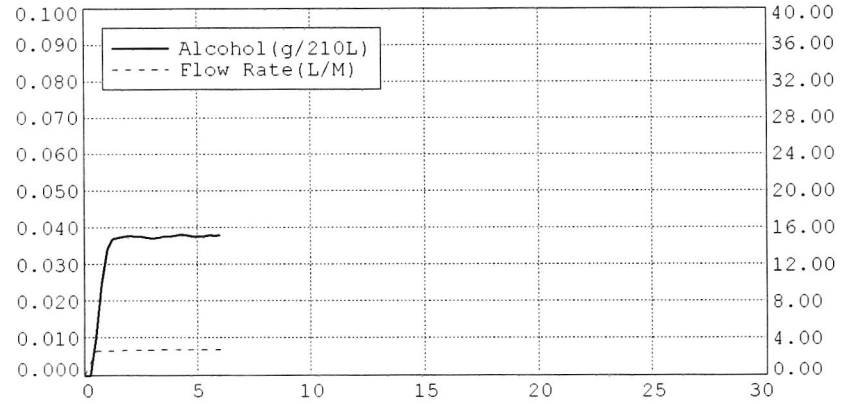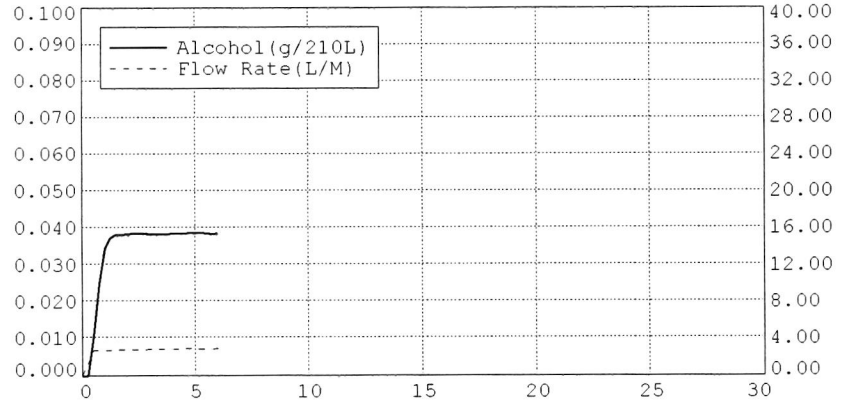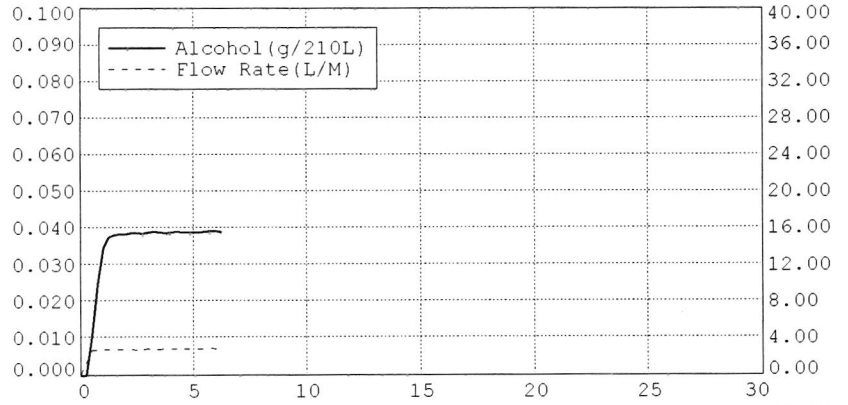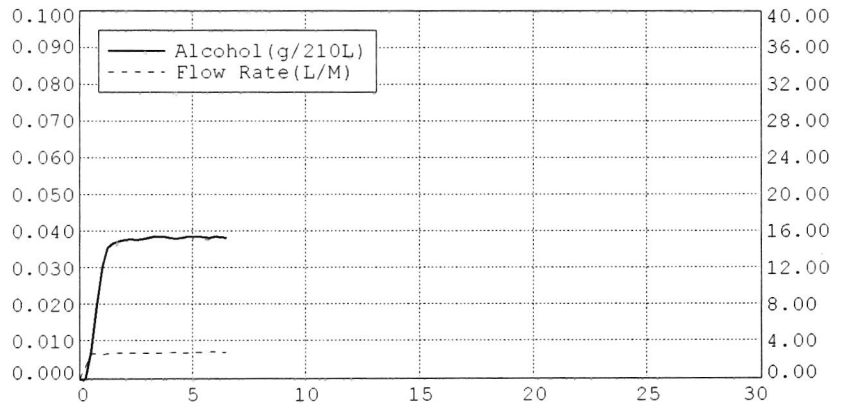

LINEARITY CHECK: Control Test 3

 Alaska Department of Public Safety
 DATAMASTER dmt: 100671






Date: 06/27/2023
 Time: 08:47:40

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.61: 0.079
 LOT #: 09523080A1
 EXPIRATION: 05/05/2025
 TANK PRESSURE: 703 psi

BLANK TEST	0.000	08:48
INTERNAL STANDARD	VERIFIED	08:49
EXTERNAL STANDARD	0.079	08:49
BLANK TEST	0.000	08:50
EXTERNAL STANDARD	0.079	08:50
BLANK TEST	0.000	08:51
EXTERNAL STANDARD	0.079	08:51
BLANK TEST	0.000	08:52
EXTERNAL STANDARD	0.079	08:52
BLANK TEST	0.000	08:53
EXTERNAL STANDARD	0.079	08:53
BLANK TEST	0.000	08:54

Average = 0.0790
 Std Dev = 0.0000

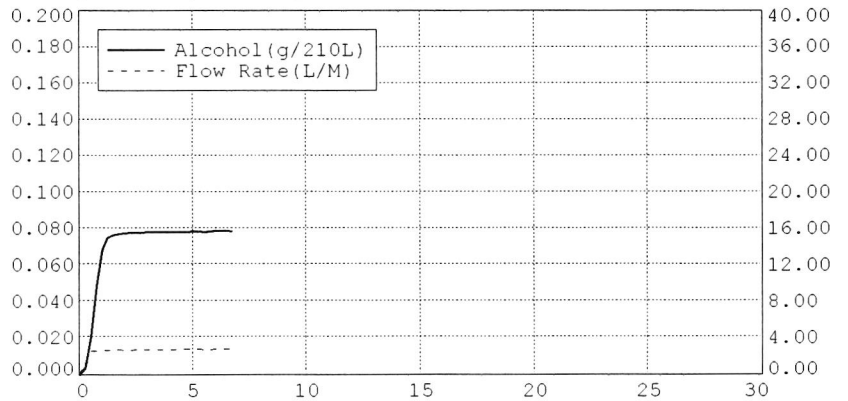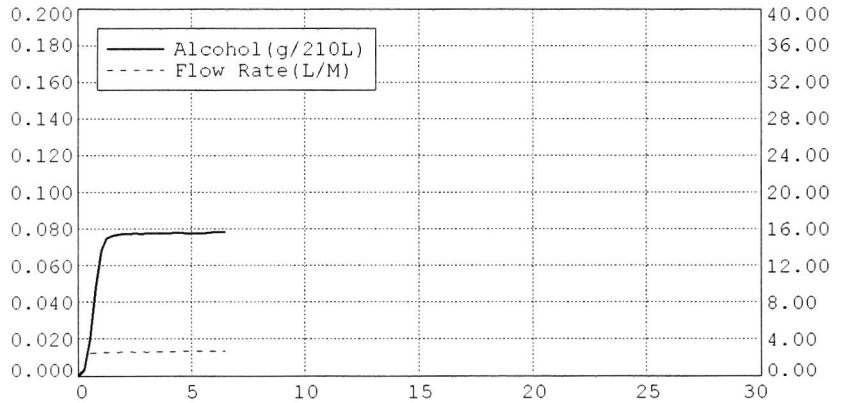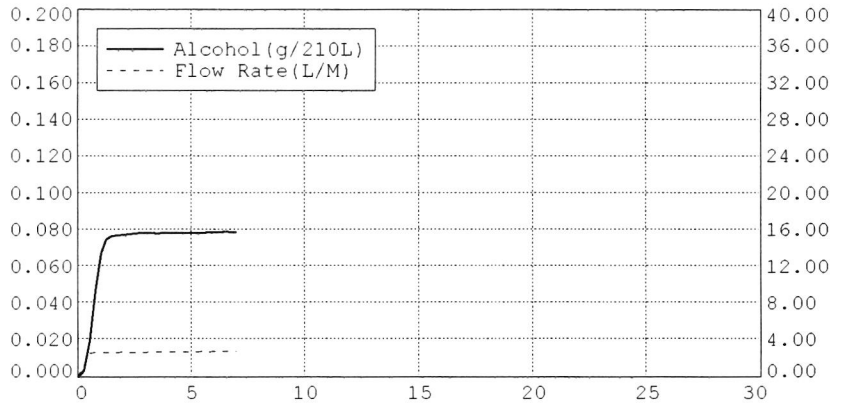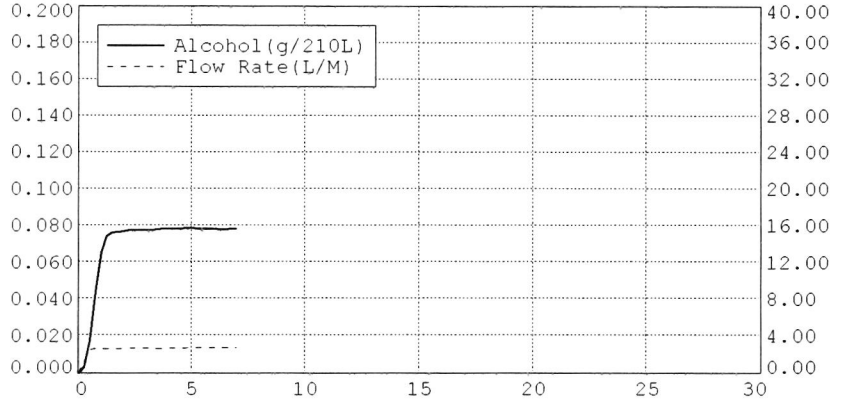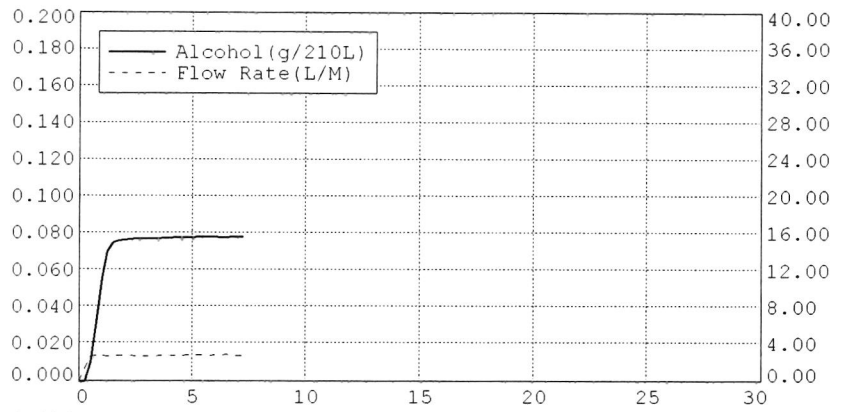

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100671






Date: 06/27/2023
 Time: 08:57:50

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.62: 0.099
 LOT #: AG211003
 EXPIRATION: 04/20/2024
 TANK PRESSURE: 917 psi

BLANK TEST	0.000	08:59
INTERNAL STANDARD	VERIFIED	08:59
EXTERNAL STANDARD	0.099	08:59
BLANK TEST	0.000	09:00
EXTERNAL STANDARD	0.099	09:00
BLANK TEST	0.000	09:01
EXTERNAL STANDARD	0.099	09:01
BLANK TEST	0.000	09:02
EXTERNAL STANDARD	0.098	09:02
BLANK TEST	0.000	09:03
EXTERNAL STANDARD	0.098	09:04
BLANK TEST	0.000	09:04

Average = 0.0986
 Std Dev = 0.0005

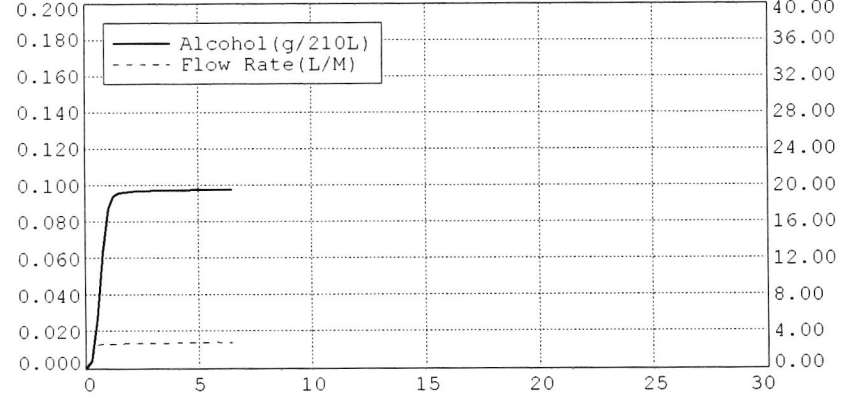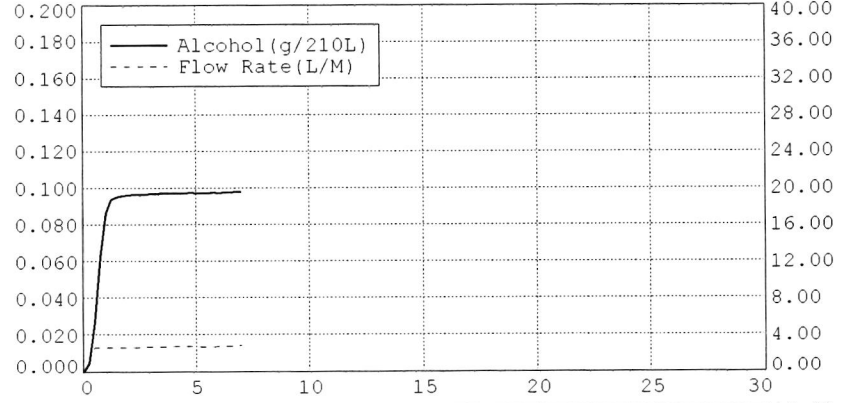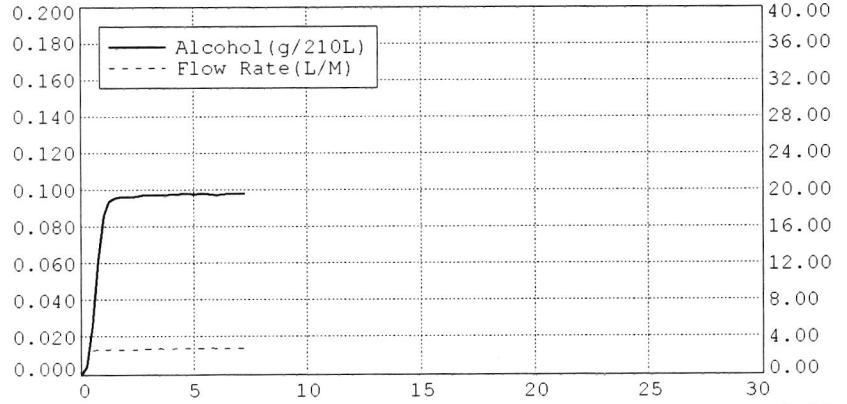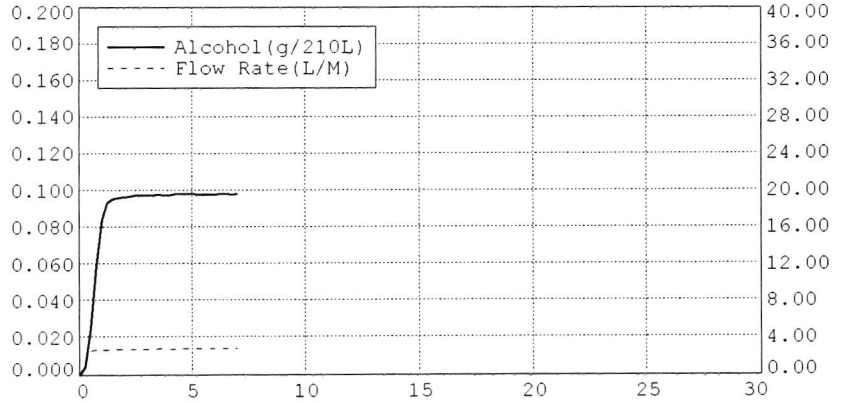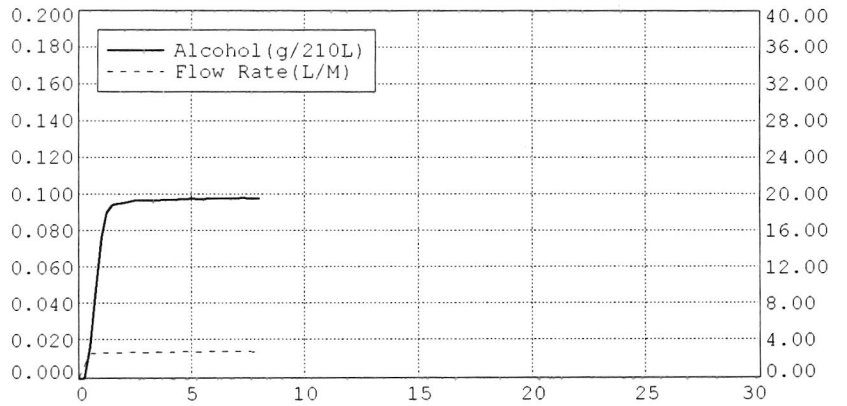

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100671






Date: 06/27/2023
Time: 09:05:47

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.61: 0.148
LOT #: AG134205
EXPIRATION: 12/08/2023
TANK PRESSURE: 573 psi

BLANK TEST	0.000	09:07
INTERNAL STANDARD	VERIFIED	09:07
EXTERNAL STANDARD	0.148	09:07
BLANK TEST	0.000	09:08
EXTERNAL STANDARD	0.148	09:08
BLANK TEST	0.000	09:09
EXTERNAL STANDARD	0.148	09:09
BLANK TEST	0.000	09:10
EXTERNAL STANDARD	0.148	09:10
BLANK TEST	0.000	09:11
EXTERNAL STANDARD	0.148	09:11
BLANK TEST	0.000	09:12

Average = 0.1480
Std Dev = 0.0000

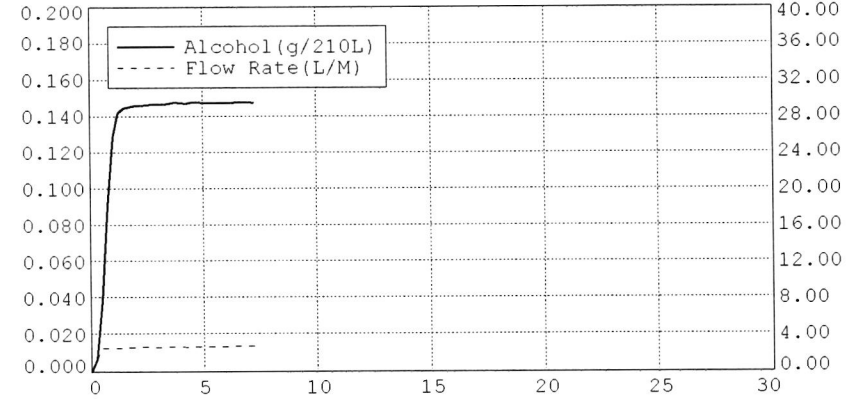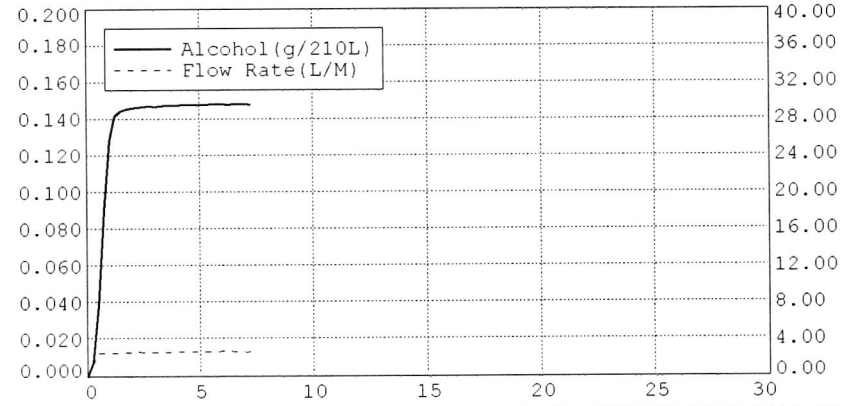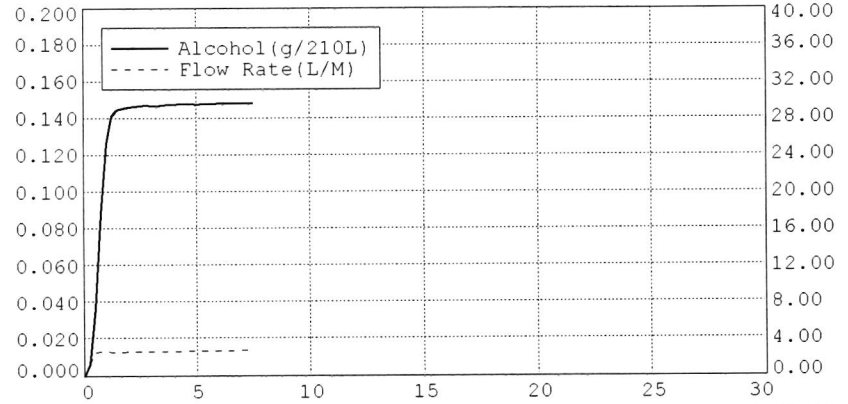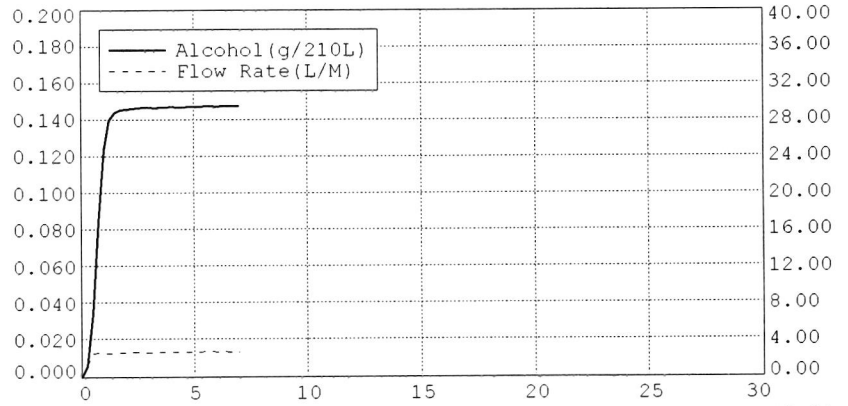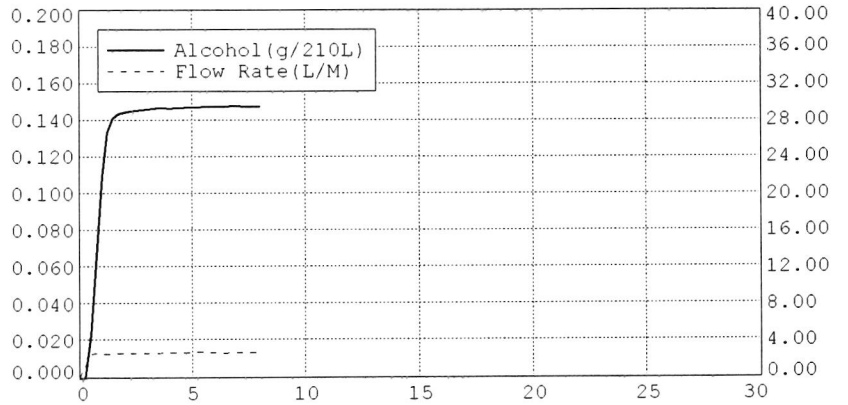

LINEARITY CHECK: Control Test 6

 Alaska Department of Public Safety
 DATAMASTER dmt: 100671






Date: 06/27/2023
 Time: 09:22:26

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 29.62: 0.297
 LOT #: AG217903
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 301 psi

BLANK TEST	0.000	09:23
INTERNAL STANDARD	VERIFIED	09:23
EXTERNAL STANDARD	0.297	09:23
BLANK TEST	0.000	09:24
EXTERNAL STANDARD	0.297	09:25
BLANK TEST	0.000	09:25
EXTERNAL STANDARD	0.298	09:26
BLANK TEST	0.000	09:27
EXTERNAL STANDARD	0.297	09:27
BLANK TEST	0.000	09:28
EXTERNAL STANDARD	0.298	09:28
BLANK TEST	0.000	09:29

Average = 0.2974
 Std Dev = 0.0005

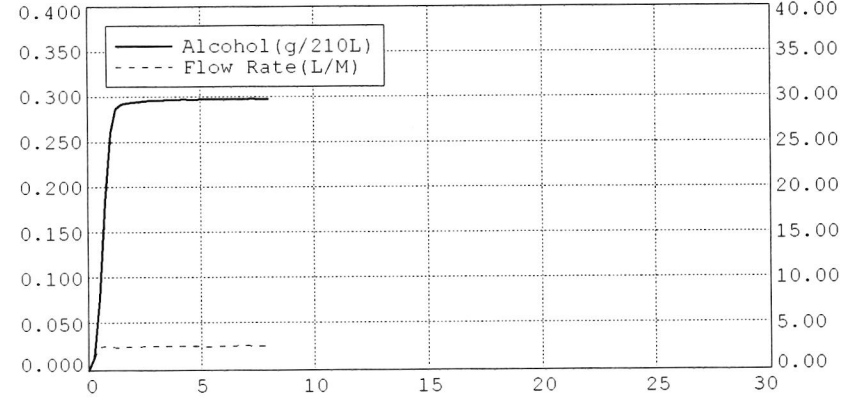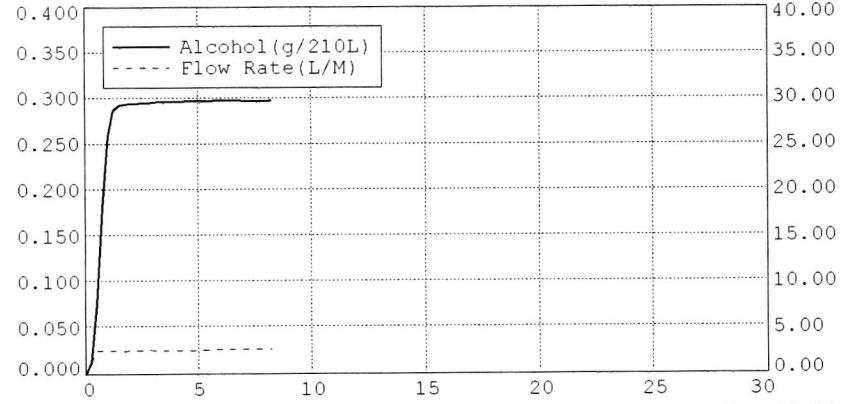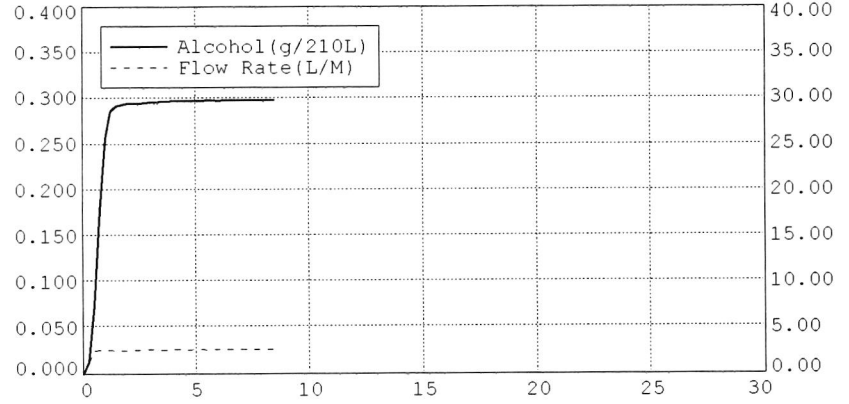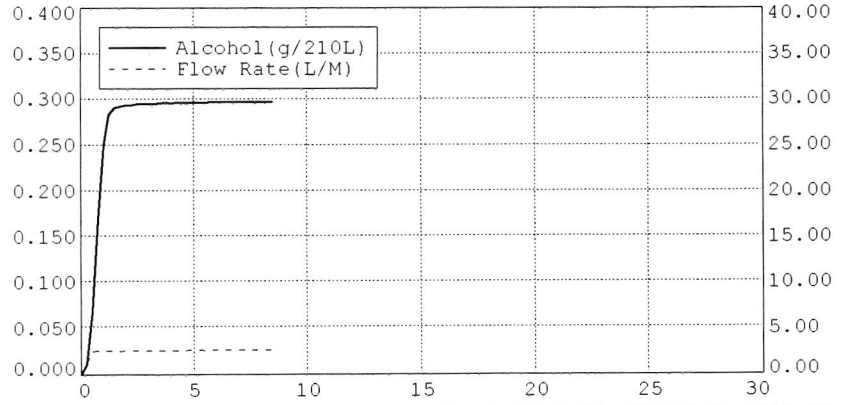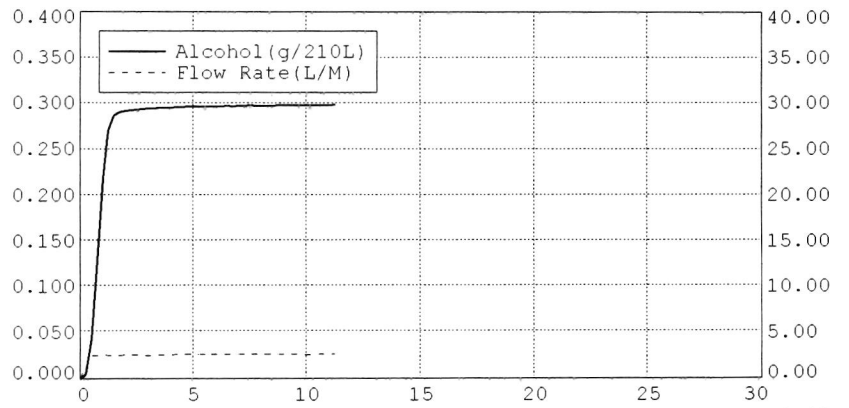

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100671

Date: 06/27/2023
Time: 10:04:51

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.62: 0.079
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	10:05
BLANK TEST	0.000	10:06
INTERNAL STANDARD	VERIFIED	10:06
EXTERNAL STANDARD	0.080	10:06
BLANK TEST	0.000	10:07
SUBJECT SAMPLE	INCOMPLETE	10:09

TJM

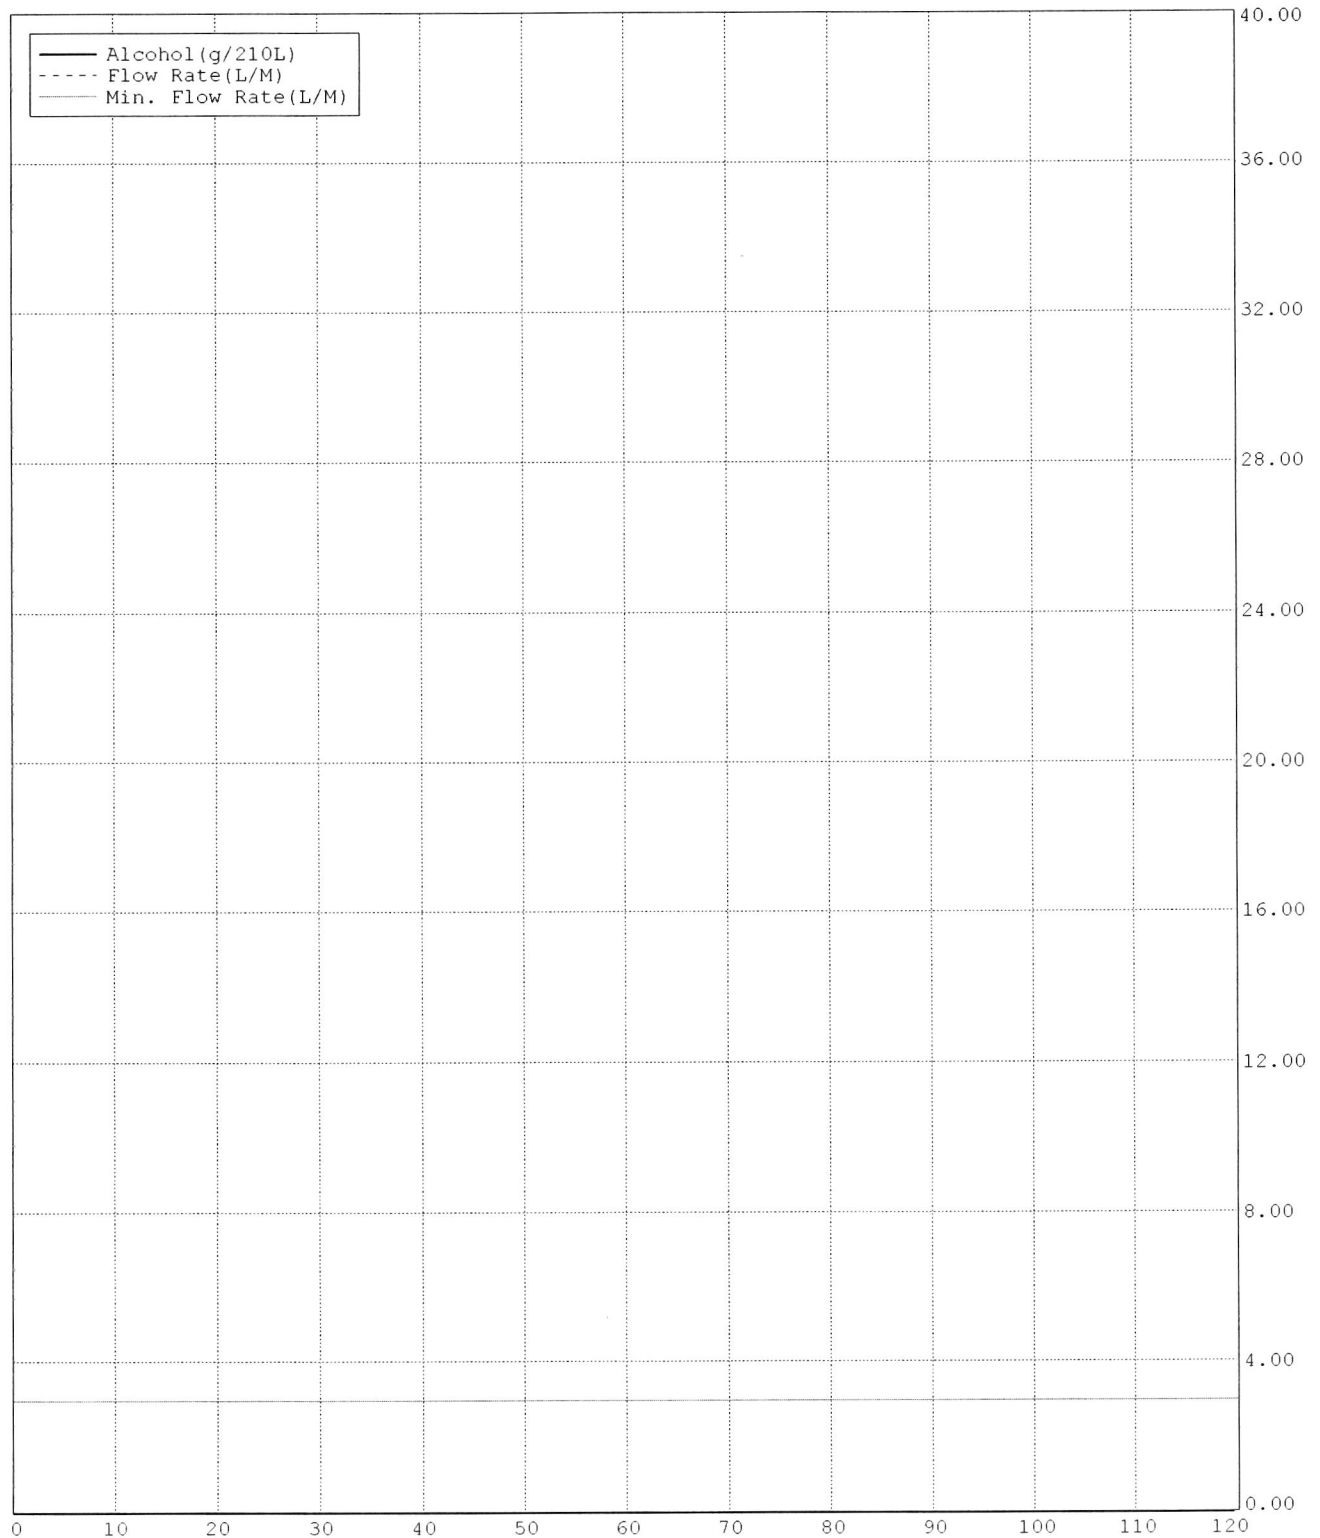

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100671

Date: 06/27/2023
Time: 10:12:56

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437


DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.62: 0.079
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	10:13
BLANK TEST	0.000	10:14
INTERNAL STANDARD	VERIFIED	10:14
EXTERNAL STANDARD	0.080	10:14
BLANK TEST	0.000	10:15
SUBJECT SAMPLE	XXX	10:15

Maximum Attempts Exceeded

TAM

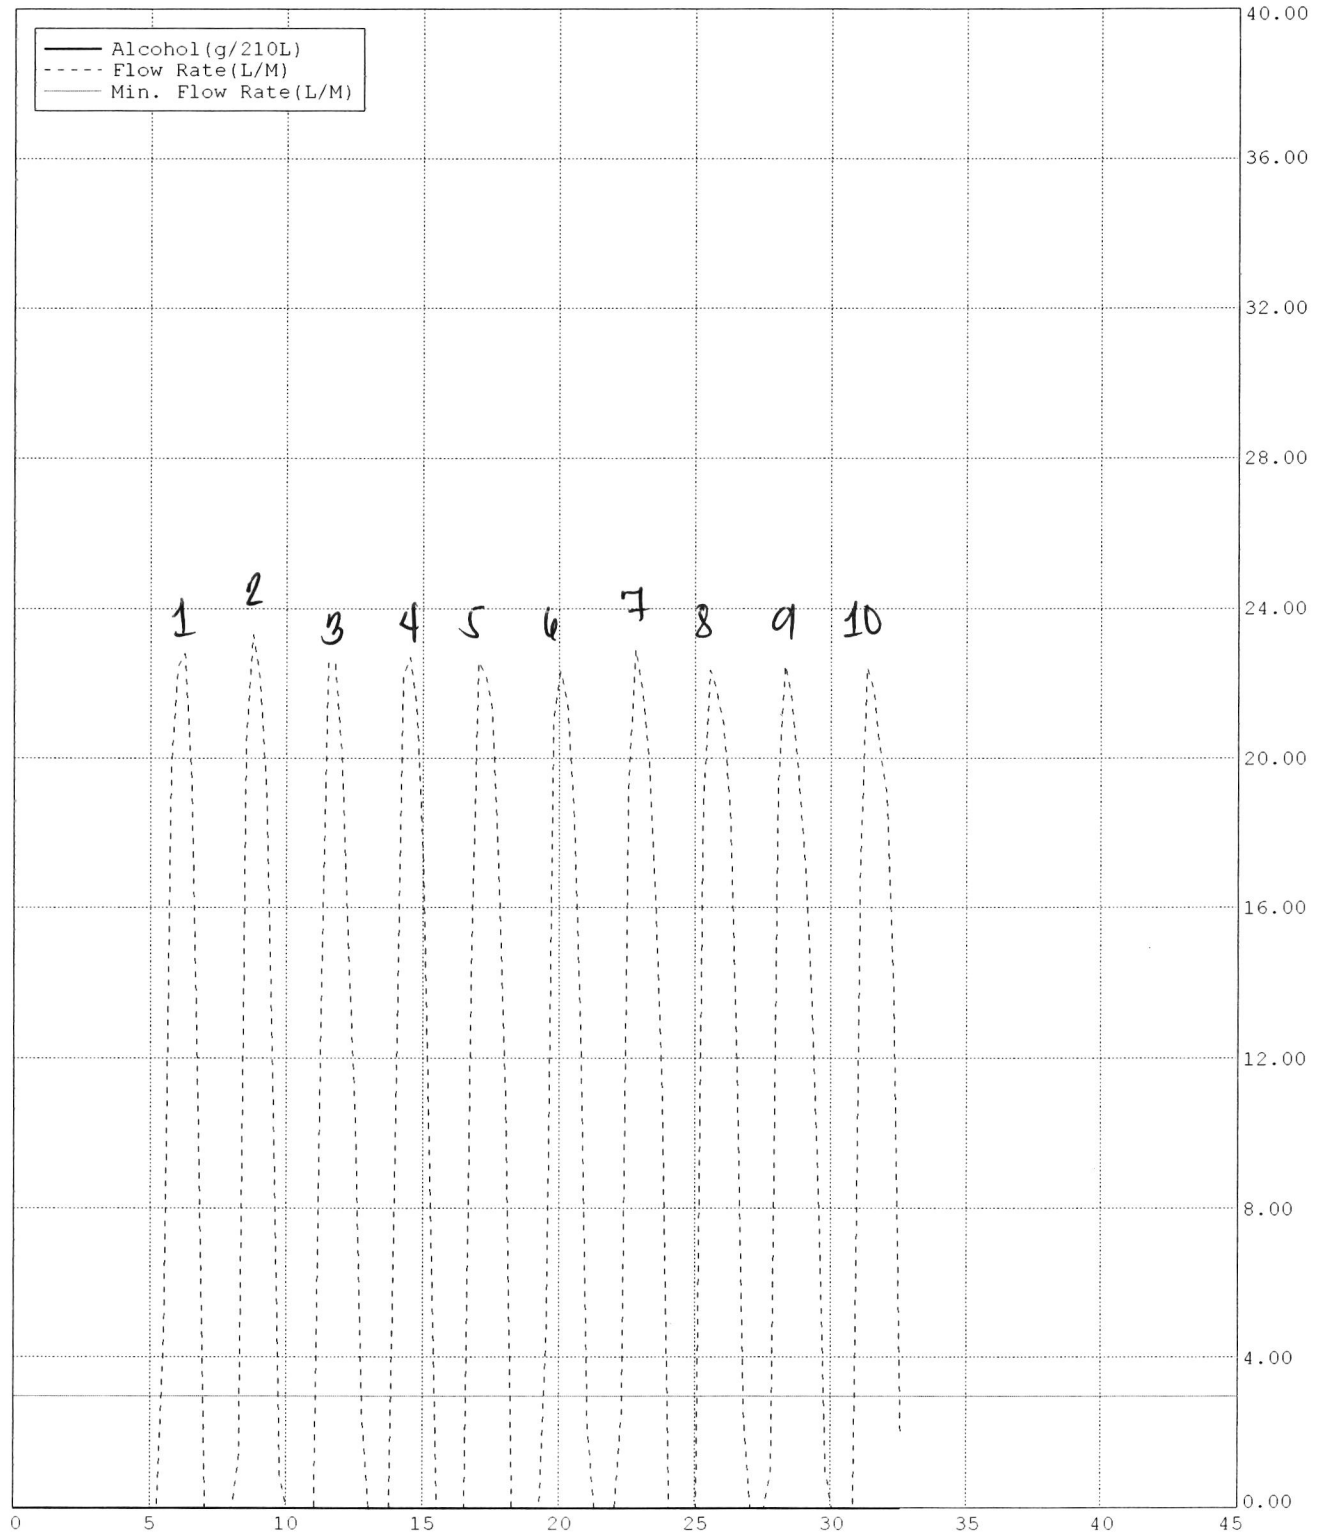

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100671

Date: 06/27/2023
Time: 10:28:44

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.62: 0.079
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	10:30
BLANK TEST	0.000	10:30
INTERNAL STANDARD	VERIFIED	10:30
EXTERNAL STANDARD	0.080	10:30
BLANK TEST	0.000	10:31
SUBJECT SAMPLE	INVALID	10:31

TAM

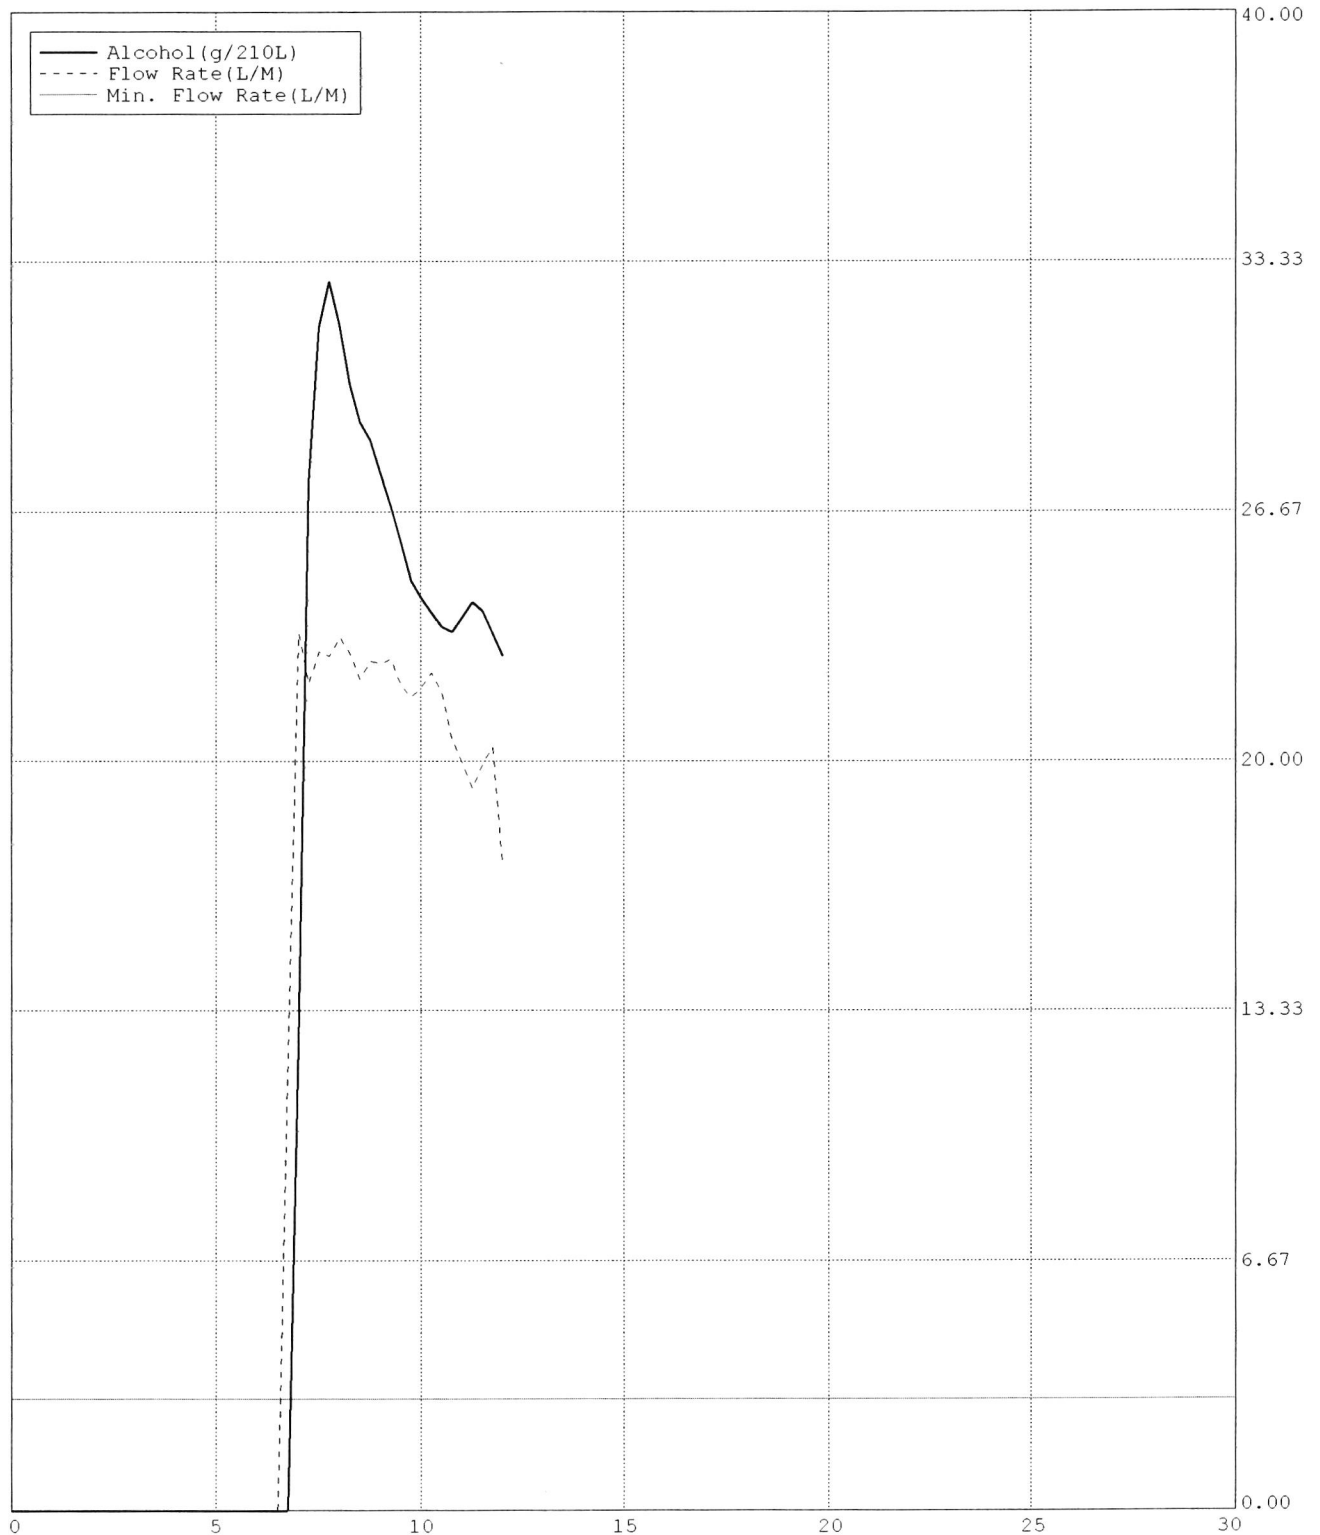

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100671

Date: 06/27/2023
Time: 11:17:45

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
RADIO FREQUENCY INTERFERENCE (RFI)
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.62: 0.079
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	11:18
BLANK TEST	0.000	11:19
INTERNAL STANDARD	VERIFIED	11:19
EXTERNAL STANDARD	0.079	11:19
BLANK TEST	0.000	11:20

RFI DETECTED

TAM



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100671

Date: 06/27/2023
Time: 10:52:19

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INTERFERENCE DETECTED - ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.62: 0.079
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	10:53
BLANK TEST	0.000	10:53
INTERNAL STANDARD	VERIFIED	10:53
Xq = 0.100 (1.15%)		
EXTERNAL STANDARD	0.079	10:53
X[1] = 0.0790 (-0.0008) (0.0023)		
BLANK TEST	0.000	10:54
SUBJECT SAMPLE	XXX	10:55
X[1] = 0.1074 (-0.0175) (0.0008)		

Interference Detected


-0.0012

Filter 2 Average: ~~-0.0016~~ TLM 07/06/2023

Filter 3 Average: 0.0023

TLM 06/27/2023

TLM

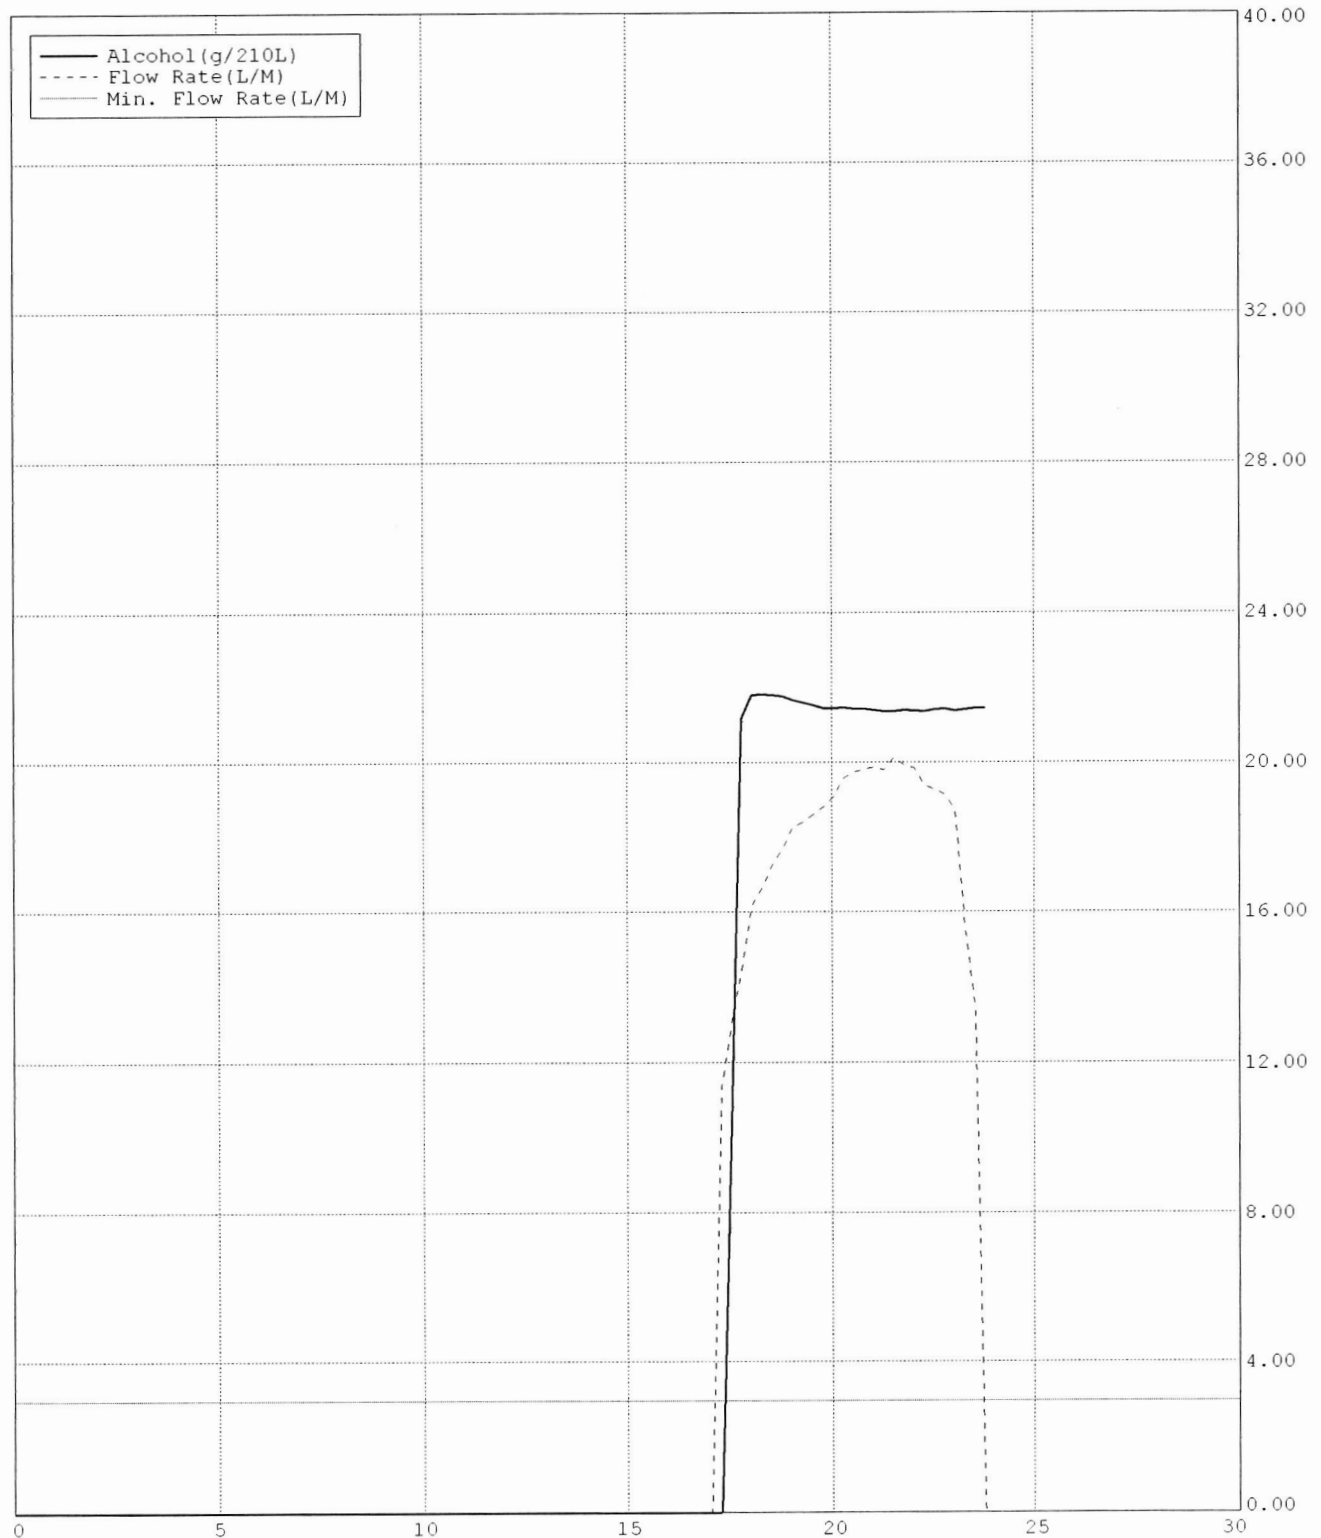

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100671

Date: 06/27/2023
Time: 10:58:39

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437


DEPT/AGENCY:
INTERFERENCE DETECTED - ISOPROPANOL
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.61: 0.079
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	11:00
BLANK TEST	0.000	11:00
INTERNAL STANDARD	VERIFIED	11:00
Xq = 0.101 (1.87%)		
EXTERNAL STANDARD	0.079	11:01
X[1] = 0.0787 (-0.0010) (0.0020)		
BLANK TEST	0.000	11:02
SUBJECT SAMPLE	XXX	11:02
X[1] = 0.1227 (-0.0327) (0.0022)		

Interference Detected

TUM

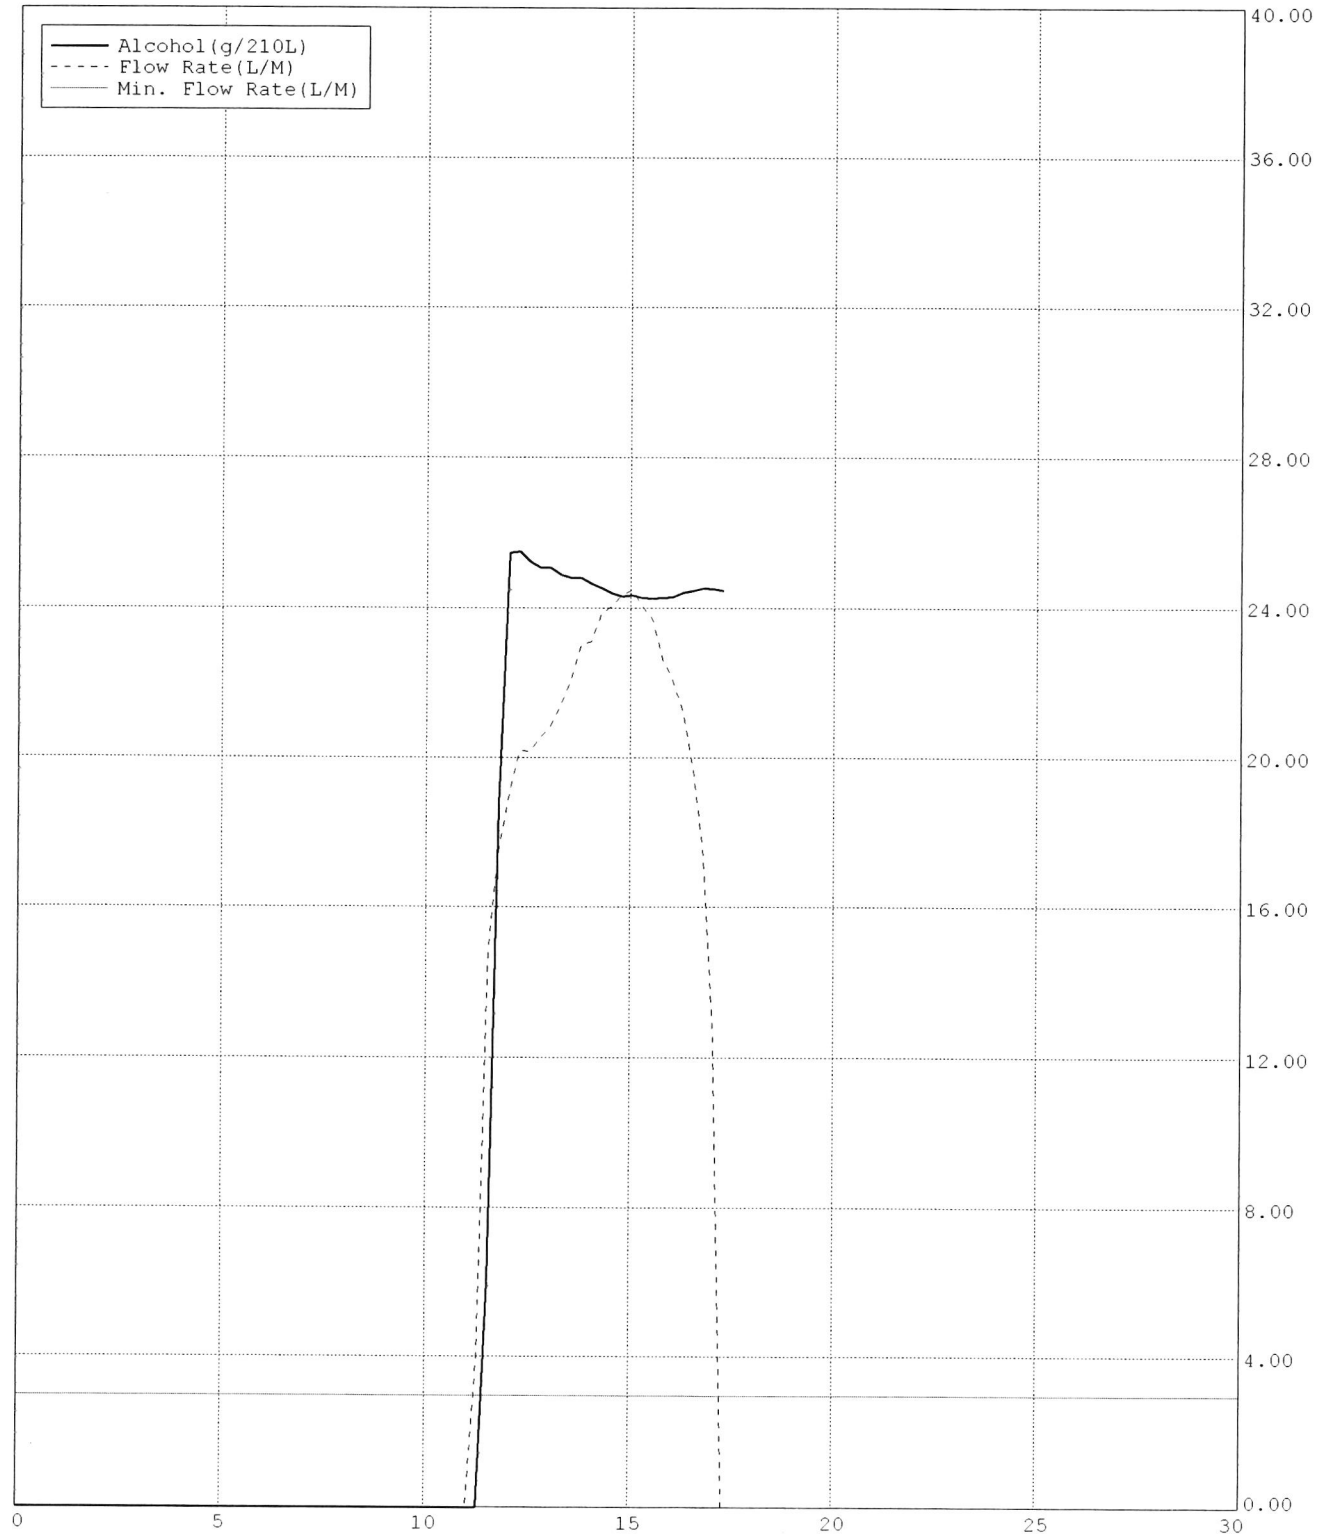

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100671

Date: 06/27/2023
Time: 10:41:48

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INTERFERENCE DETECTED - NEGATIVE CONTROL
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.61: 0.079
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	10:42
BLANK TEST	0.000	10:42
INTERNAL STANDARD	VERIFIED	10:43
Xq = 0.100 (1.51%)		
EXTERNAL STANDARD	0.079	10:43
X[1] = 0.0790 (-0.0013) (0.0031)		
BLANK TEST	0.000	10:44
SUBJECT SAMPLE (Vol=2.04L)	0.094	10:44
X[1] = 0.0945 (-0.0004) (0.0005)		
BLANK TEST	0.000	10:45
EXTERNAL STANDARD	0.078	10:45
X[1] = 0.0780 (-0.0015) (0.0017)		
BLANK TEST	0.000	10:46

Tan

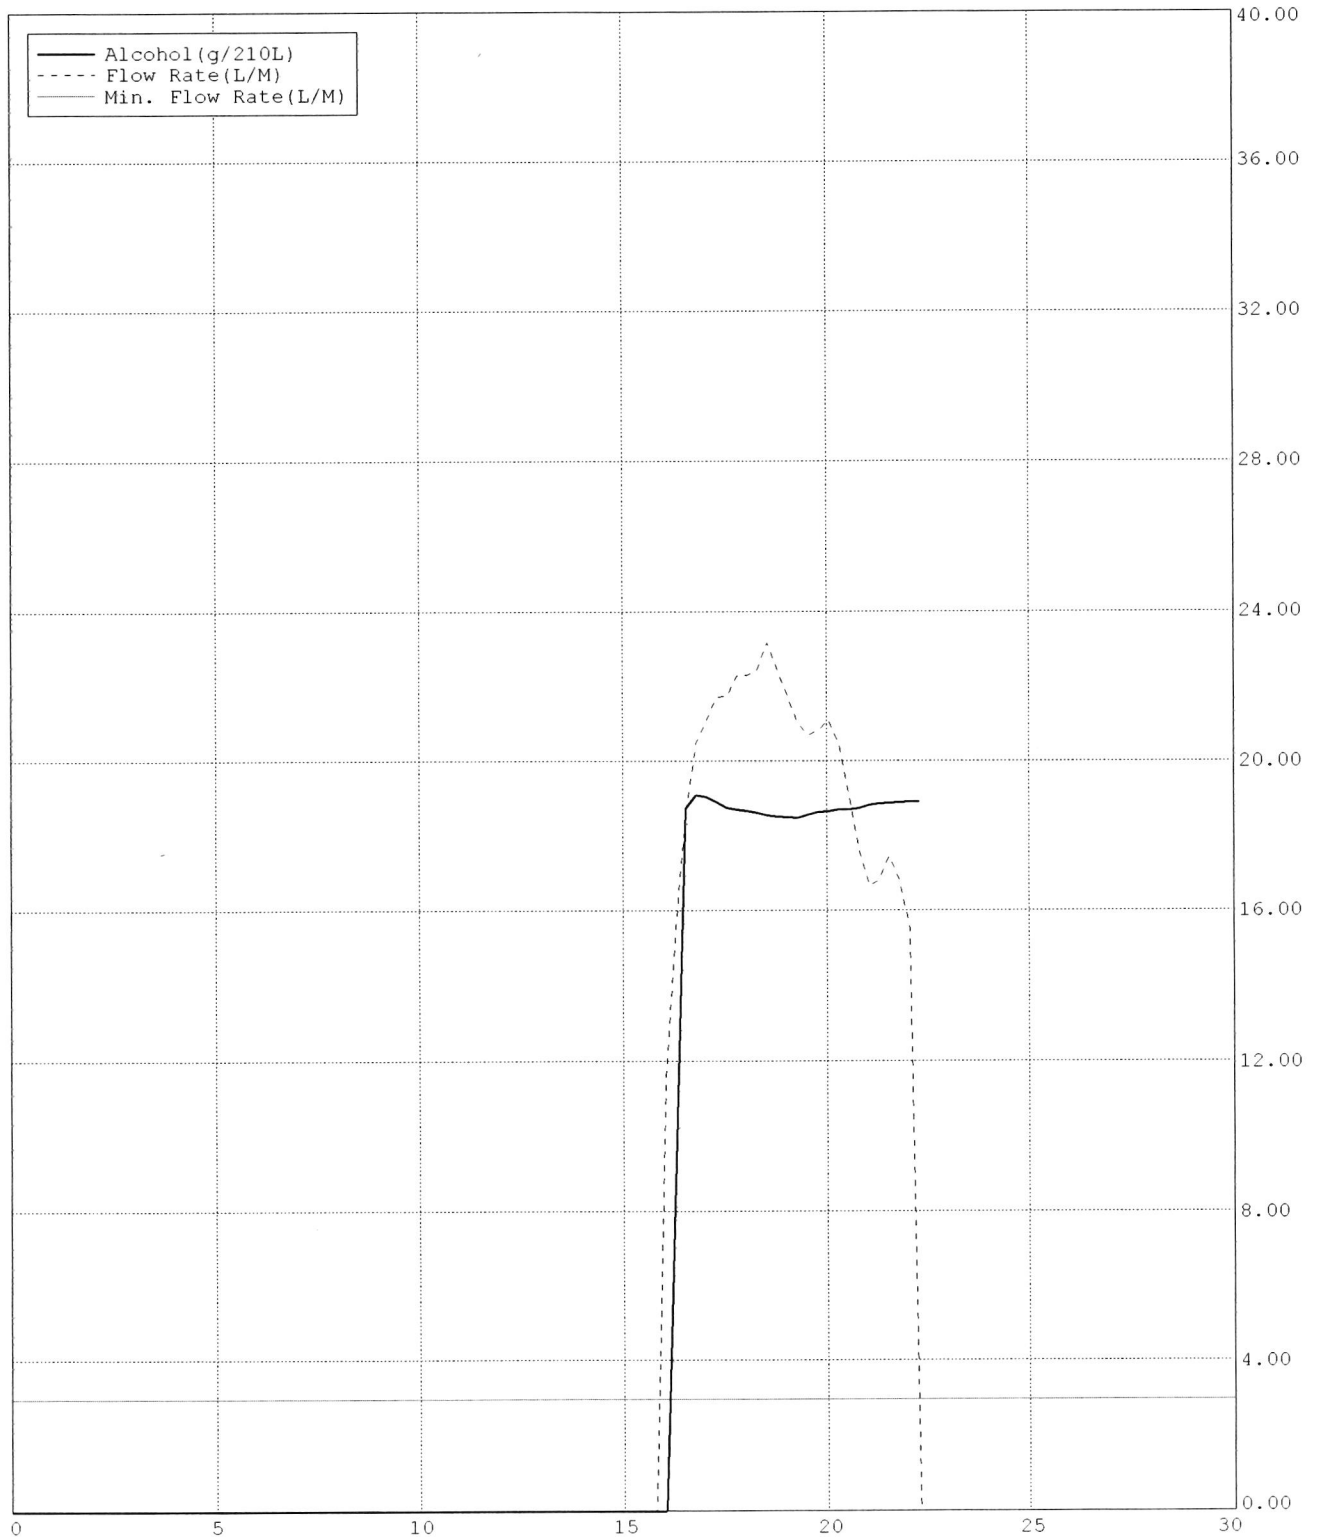

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100671

Date: 06/27/2023
Time: 12:23:50

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.62: 0.079
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	12:24
BLANK TEST	0.000	12:24
INTERNAL STANDARD	VERIFIED	12:25
EXTERNAL STANDARD	0.079	12:25
BLANK TEST	0.000	12:26
SUBJECT SAMPLE (Vol=1.89L)	0.000	12:26
BLANK TEST	0.000	12:27
EXTERNAL STANDARD	0.080	12:27
BLANK TEST	0.000	12:28

TML

