

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100681

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 12/15/2015

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 30.25: 0.081
LOT #: 01315080A3
EXPIRATION: 02/05/2017
TANK PRESSURE: 738 psi

| | | |
|-------------------|----------|-------|
| BLANK TEST | 0.000 | 11:40 |
| INTERNAL STANDARD | VERIFIED | 11:40 |
| EXTERNAL STANDARD | 0.080 | 11:40 |
| BLANK TEST | 0.000 | 11:41 |
| EXTERNAL STANDARD | 0.080 | 11:42 |
| BLANK TEST | 0.000 | 11:42 |
| EXTERNAL STANDARD | 0.080 | 11:43 |
| BLANK TEST | 0.000 | 11:44 |
| EXTERNAL STANDARD | 0.079 | 11:44 |
| BLANK TEST | 0.000 | 11:45 |
| EXTERNAL STANDARD | 0.079 | 11:45 |
| BLANK TEST | 0.000 | 11:46 |

Average = 0.0796
Std Dev = 0.0005

Diagnostic Check

VERSIONS

DMT: 3.01
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED
Breath Tube = 43.9°C PASSED

PUMP INFO

Flow Rate = 4.410 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO


Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:



- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

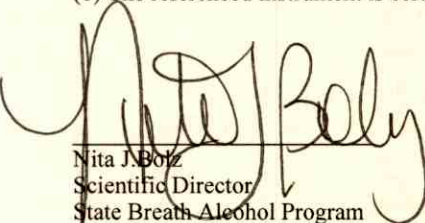
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

12/31/2015

Subscribed and sworn before me this 31st day of Dec 20 15


Nikki Roth, Notary Public
My Commission Expires With Office

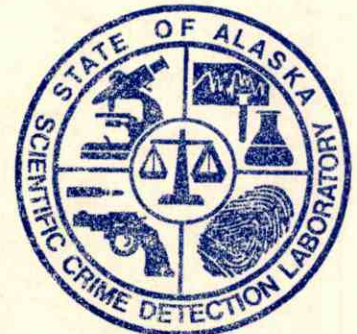

CAB 12/30/15