

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100355

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 01/29/2013

External Standard Test Values

Diagnostic Check

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 27.58: 0.073
LOT #: 02012080A1
EXPIRATION: 03/01/2014

BLANK TEST	0.000	11:35
INTERNAL STANDARD	VERIFIED	11:36
EXTERNAL STANDARD	0.073	11:36
BLANK TEST	0.000	11:37
EXTERNAL STANDARD	0.072	11:37
BLANK TEST	0.000	11:38
EXTERNAL STANDARD	0.072	11:38
BLANK TEST	0.000	11:39
EXTERNAL STANDARD	0.072	11:39
BLANK TEST	0.000	11:40
EXTERNAL STANDARD	0.072	11:40
BLANK TEST	0.000	11:41

Average = 0.0722
Std Dev = 0.0004

VERSIONS

DMT: 2.00
PIC: 3.02
Modem: 2.3
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED
Breath Tube = 47.8°C PASSED

PUMP INFO

Flow Rate = 4.234 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO

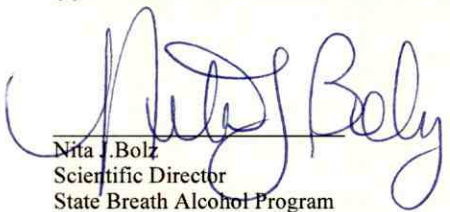
Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

2/13/2013

Subscribed and sworn before me this 13th day of Feb, 20 13


Nikki Roth, Notary Public
My Commission Expires With Office



CRF
2/11/13