




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory
4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100403

Report Issue Date: 12/01/2025
Date Received: 2025-11-17
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.022	0.022	0.022	0.022	0.023	0.022
0.080	0.079	AG335202	0.081	0.081	0.081	0.080	0.081	0.081
0.300	0.295	AG427706	0.294	0.293	0.294	0.294	0.293	0.294

As Found - Evaluation Analyst: Kaija Swisher
As Found Conditions - Barometric Pressure (inHg): 29.38 Barometer Used: VWR S/N 240680771 Temperature (C): 20.8 Relative Humidity (%): 16
As-Found Lab Activity Date Range: 11/17/2025 - 11/18/2025

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.021	0.022	0.022	0.022	0.022	0.022	+/- 0.002
0.040	0.040	AG407908	0.043	0.043	0.043	0.043	0.043	0.043	+/- 0.003
0.080	0.080	AG335202	0.082	0.082	0.082	0.082	0.082	0.082	+/- 0.004
0.100	0.100	AG333401	0.103	0.102	0.102	0.102	0.103	0.102	+/- 0.004
0.150	0.149	AG515604	0.150	0.151	0.150	0.150	0.150	0.150	+/- 0.006
0.300	0.299	AG427706	0.299	0.298	0.297	0.298	0.298	0.298	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.82 Barometer Used: VWR S/N 240680771 Temperature (C): 21.5 Relative Humidity (%): 7
As-Left Lab Activity Date Range: 11/24/2025 - 11/24/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Derek Walton on 12/01/2025

derek.walton@alaska.gov

Technically and administratively reviewed by Carlie Glaister on 12/01/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100403 Analyst or Technician Name: Derek Walton

DataMaster DMT Calibration Start Date: 11/24/2025

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 09/10/26
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.82 Temperature(C) 21.5 Relative Humidity(%) 7

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Interference (Volatiles) - *Print with View Details*
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20250722K5 Expiration Date: 12/22/2025
Simulator S/N: DR4178 Thermometer Verification Performed? ☒
2. Isopropanol Reagent Lot Number: 20250722K5 Expiration Date: 12/22/2025
Simulator S/N: DR4177 Thermometer Verification Performed? ☒
3. Negative (Ethanol Only) Lot Number: 25CP41280 Expiration Date: 12/22/2025
Simulator S/N: DR4163 Thermometer Verification Performed? ☒

Solution
03/19/27

Calibrated External Thermometer S/N: 250159297

Calibration Due Date: 03/14/2027

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 11/24/25

Data Interpretation Date (Technician): _____ (if applicable)

Data Interpretation Date (Analyst): 11/24/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100403

Date: 11/24/2025
Time: 08:07:56

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C	PASSED
(44.0°C - 52.0°C)	
Breath Tube = 40.1°C	PASSED
(38.0°C - 50.0°C)	

SETTINGS

Lamp Voltage = 1.70 V	PASSED
(1.04 V - 2.42 V)	
Cooler Voltage = 1.70 V	PASSED
(0.98 V - 2.30 V)	
Bias Voltage = 79 V	PASSED
(47 V - 111 V)	
Chopper Freq = 540 Hz	PASSED
(475 Hz - 575 Hz)	
Barometer = 29.8 in	

PUMP INFO

Flow Rate = 4.628 L/M	PASSED
(3.500 L/M - 6.500 L/M)	

DETECTOR INFO

PUMP ON	PASSED
(0.002 V <= 0.010 V)	
PUMP OFF	PASSED
(0.002 V <= 0.010 V)	

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD	PASSED
Xq = 0.076 2.10% (0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100403

Date: 11/24/2025

Time: 8:22 AM

Temperatures (°C)

Sample Cell: 49.0°C

Breath Tube: 41.3°C

Current Barometer 29.8 in ✓

Volume (Ltr) 1.55 ✓

Settings

Lamp: 1.70 V

Bias: 80 V

Cooler: 1.78 V

Chopper: 525 Hz

Voltages (V)

Flow: 1.05 V

Detector: -0.006 V ✓

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100403

Date: 05/18/2011
Time: 13:44:51

OPERATOR NAME:
COLLEEN S OBRYANT
CERTIFICATE #: 6237

LOT #: GUTH100
BOTTLE #: 10260
EXPIRATION: 10/25/2010

Ca = 0.1000
CAL = 0.986050 0.800 <= CAL < 1.200
b1 = 0.0000 0.0000 <= b1 < 0.0040
b2 = 0.0043 0.0010 <= b2 < 0.0100
b3 = 0.0000 0.0000 <= b3 < 0.0040
Xq = 0.0743 0.0500 <= Xq < 0.2000
a21 = 1.112347 1.050 <= a21 < 1.300
a31 = 0.534530 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100403

Date: 11/24/2025

Time: 08:25:45

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

DEREK WALTON

OPERATOR'S #: 9508

DEPT/AGENCY:

MINIMUM VOLUME

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080


TARGET AT 29.83: 0.080

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	08:27
BLANK TEST	0.000	08:27
INTERNAL STANDARD	VERIFIED	08:27
EXTERNAL STANDARD	0.081	08:27
BLANK TEST	0.000	08:28
SUBJECT SAMPLE (Vol=1.55L)	0.000	08:29
BLANK TEST	0.000	08:30
EXTERNAL STANDARD	0.081	08:31
BLANK TEST	0.000	08:31

dm

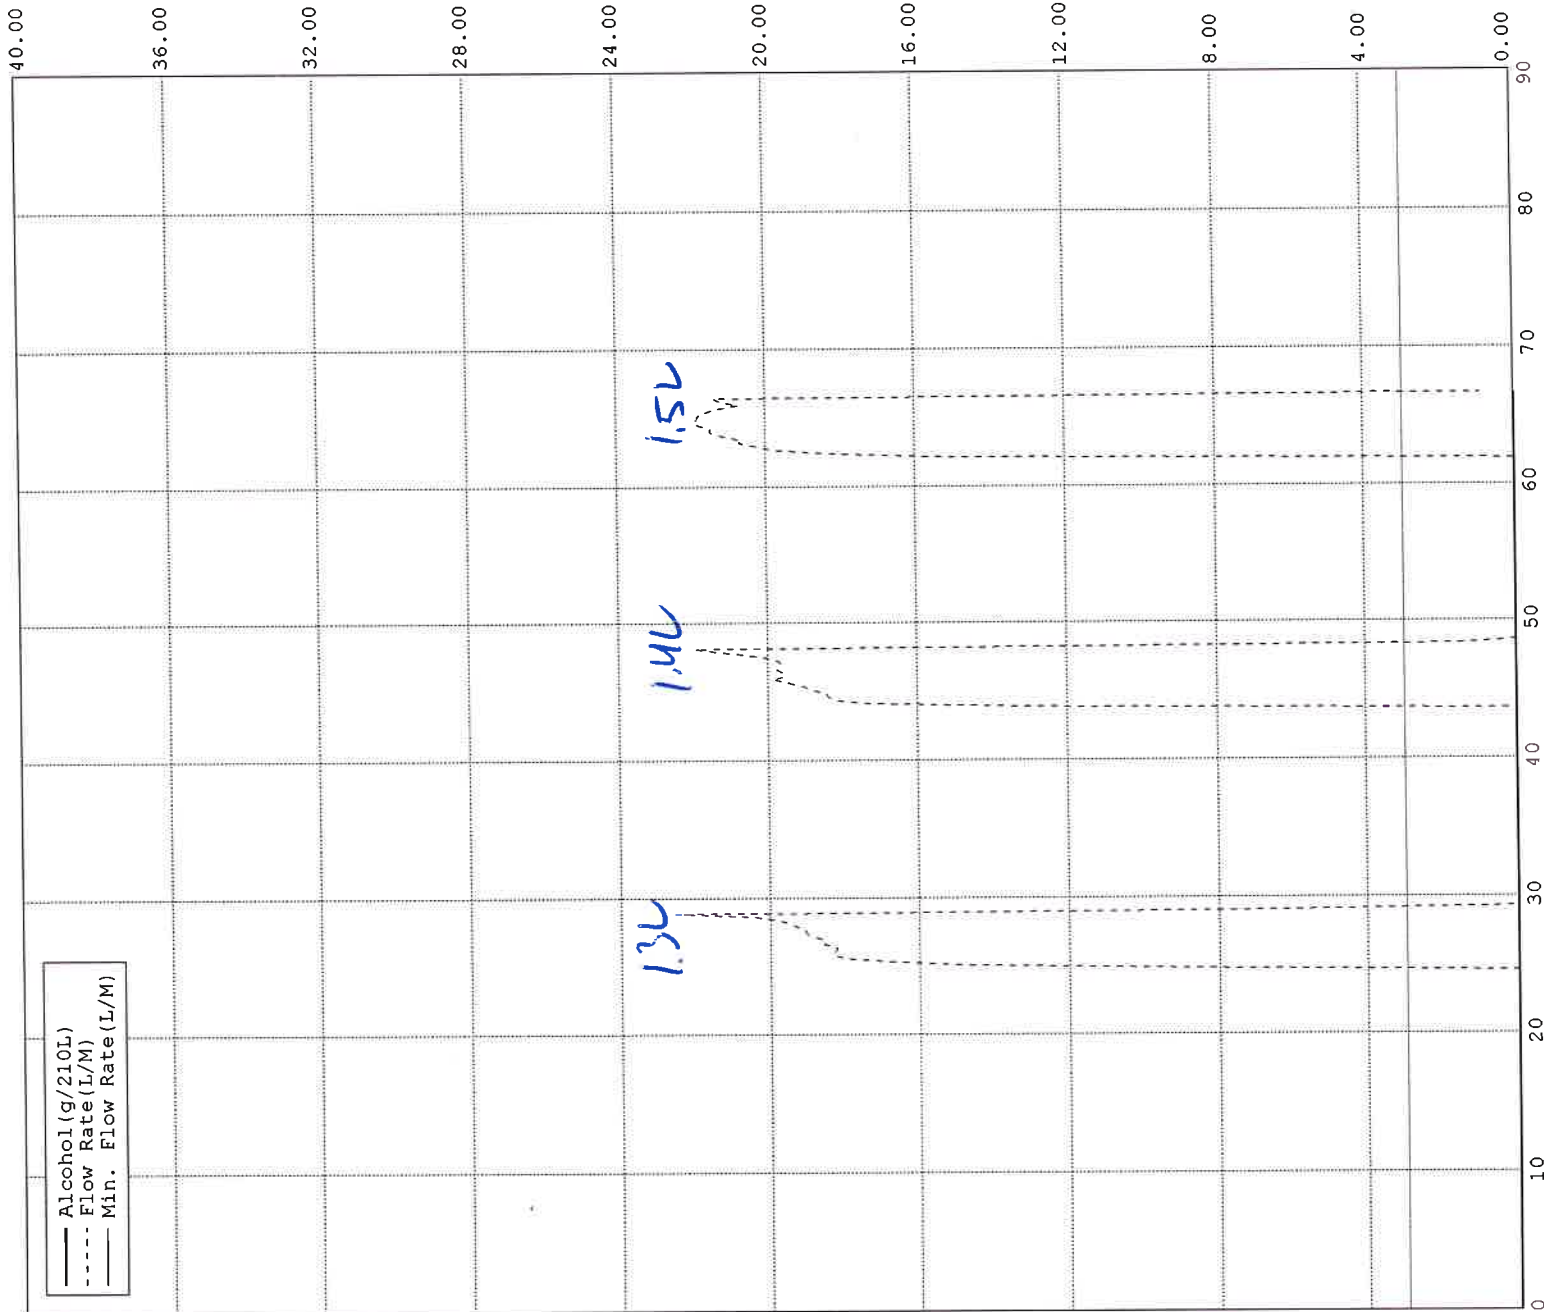

LINEARITY CHECK

Alaska Department of Public Safety

DATAMASTER dmt: 100403

Date: 11/24/2025

Time: 08:59:37


SUPERVISOR NAME:

DEREK WALTON

OPERATOR'S #: 9508

TARGET	AVERAGE	STD. DEV.
0.020	0.0218	0.0004
0.040	0.0430	0.0000
0.080	0.0820	0.0000
0.100	0.1024	0.0005
0.149	0.1502	0.0004
0.299	0.2980	0.0007

SLOPE = 0.987438
R² = 0.999967

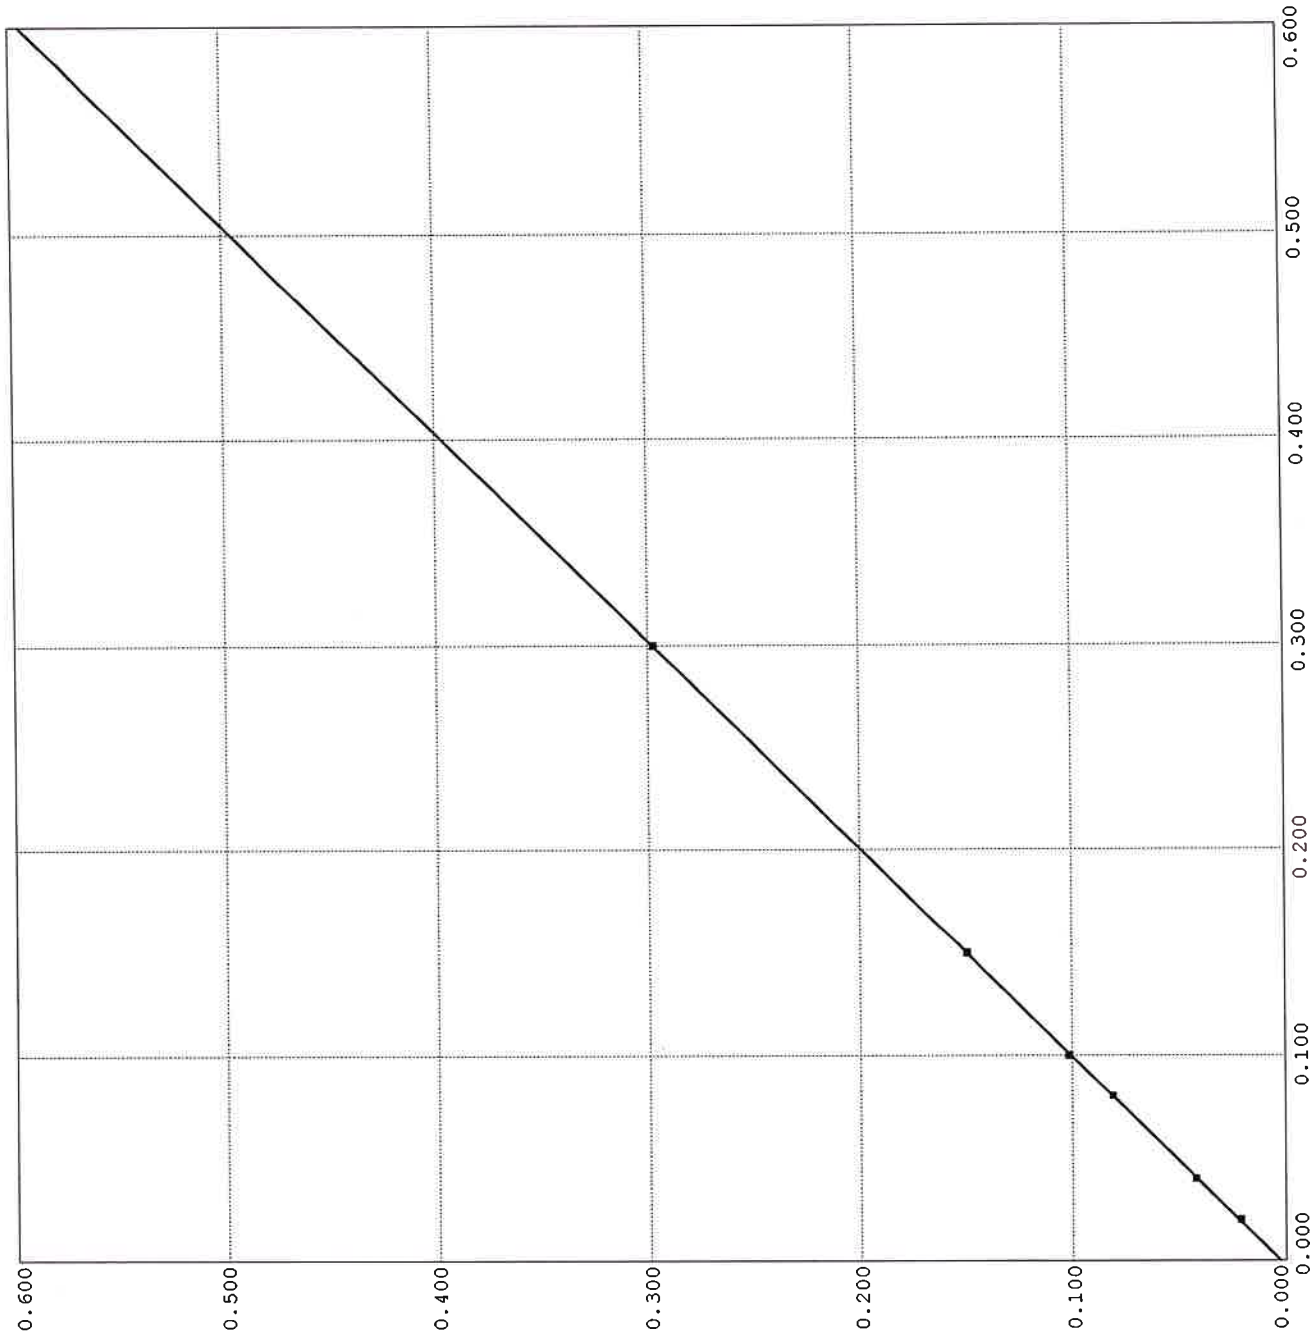

MW

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100403






Date: 11/24/2025
Time: 08:59:39

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.82: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 825 psi

BLANK TEST	0.000	09:00
INTERNAL STANDARD	VERIFIED	09:00
EXTERNAL STANDARD	0.021	09:01
BLANK TEST	0.000	09:02
EXTERNAL STANDARD	0.022	09:02
BLANK TEST	0.000	09:03
EXTERNAL STANDARD	0.022	09:03
BLANK TEST	0.000	09:04
EXTERNAL STANDARD	0.022	09:04
BLANK TEST	0.000	09:05
EXTERNAL STANDARD	0.022	09:05
BLANK TEST	0.000	09:06

Average = 0.0218
Std Dev = 0.0004

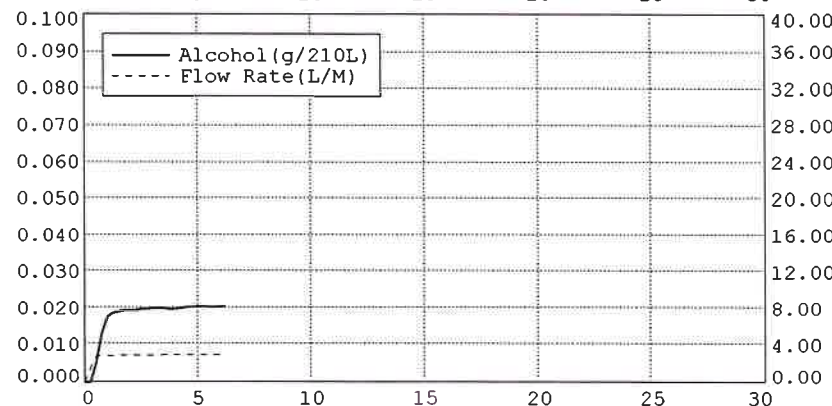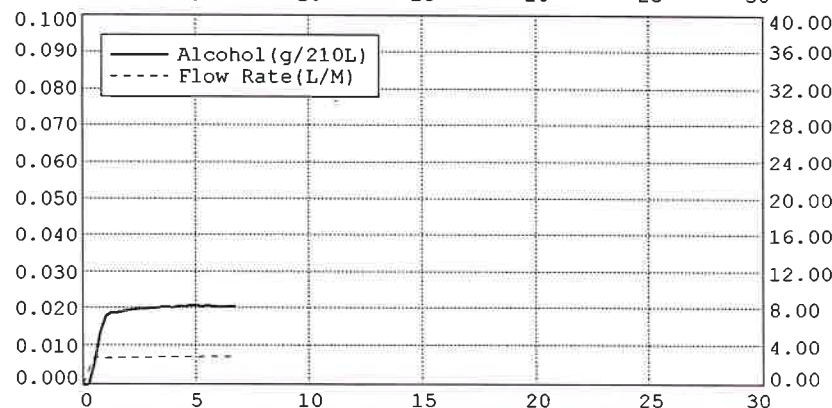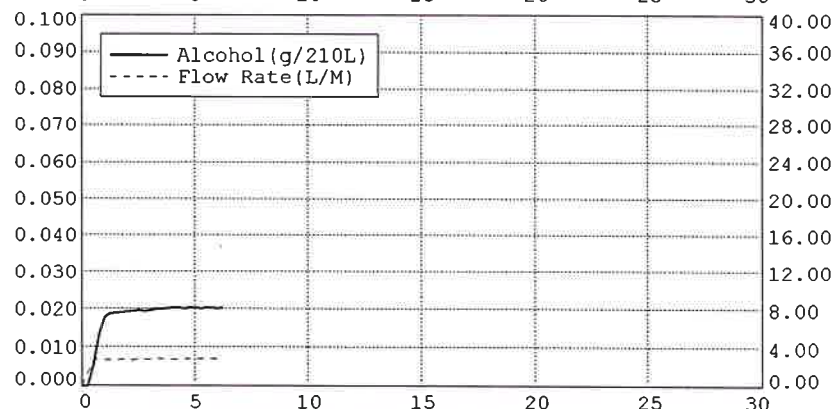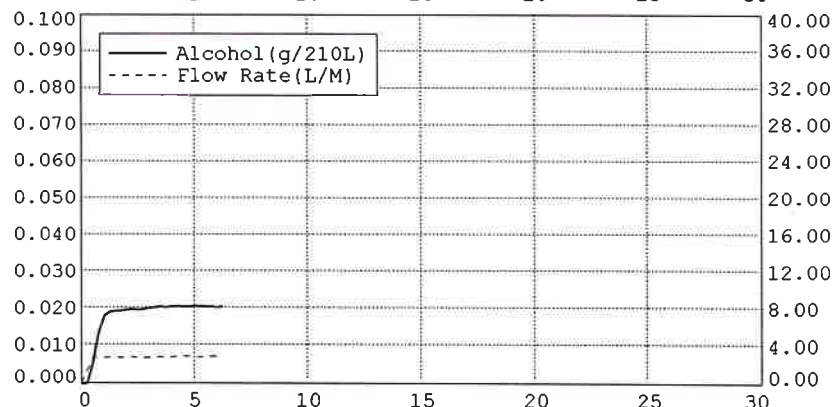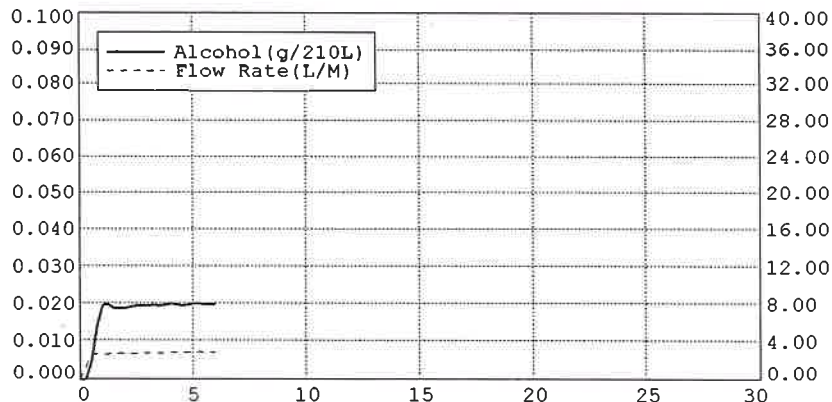

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100403






Date: 11/24/2025
Time: 09:06:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.82: 0.040
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 758 psi

BLANK TEST	0.000	09:08
INTERNAL STANDARD	VERIFIED	09:08
EXTERNAL STANDARD	0.043	09:08
BLANK TEST	0.000	09:09
EXTERNAL STANDARD	0.043	09:09
BLANK TEST	0.000	09:10
EXTERNAL STANDARD	0.043	09:10
BLANK TEST	0.000	09:11
EXTERNAL STANDARD	0.043	09:11
BLANK TEST	0.000	09:12
EXTERNAL STANDARD	0.043	09:12
BLANK TEST	0.000	09:13

Average = 0.0430
Std Dev = 0.0000

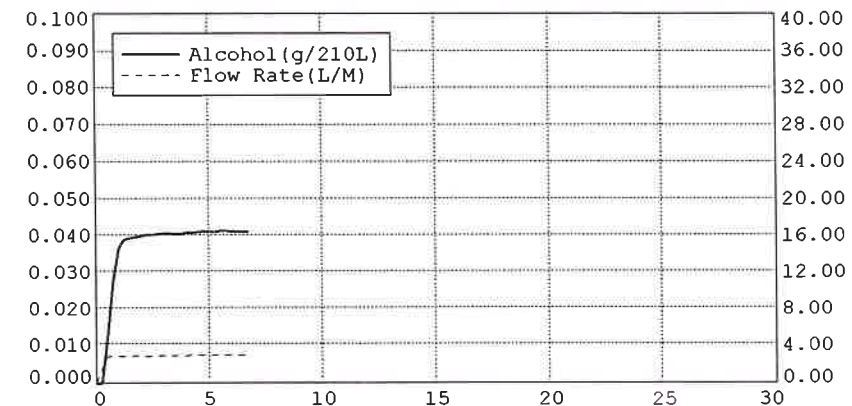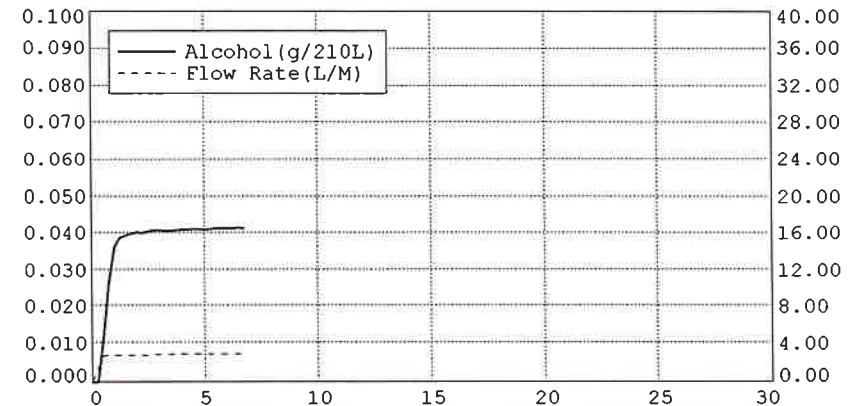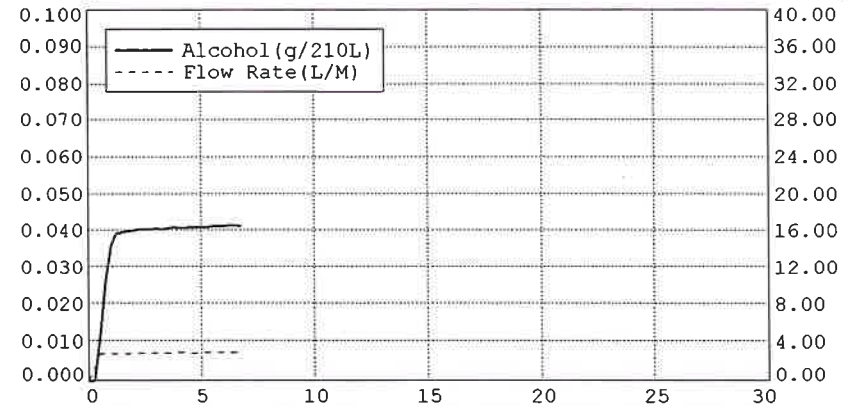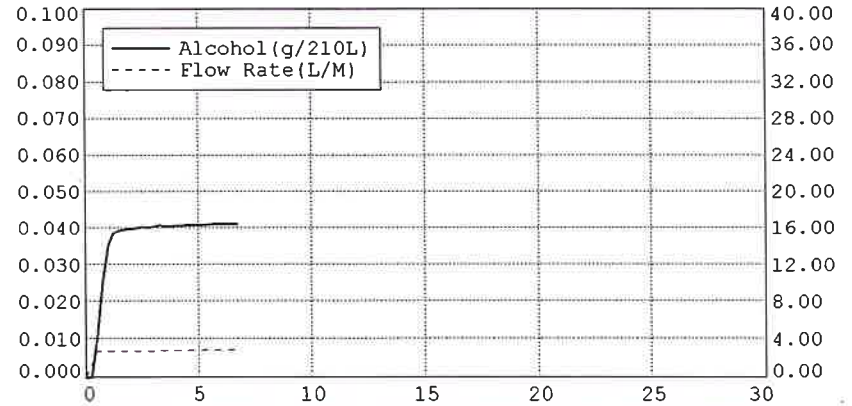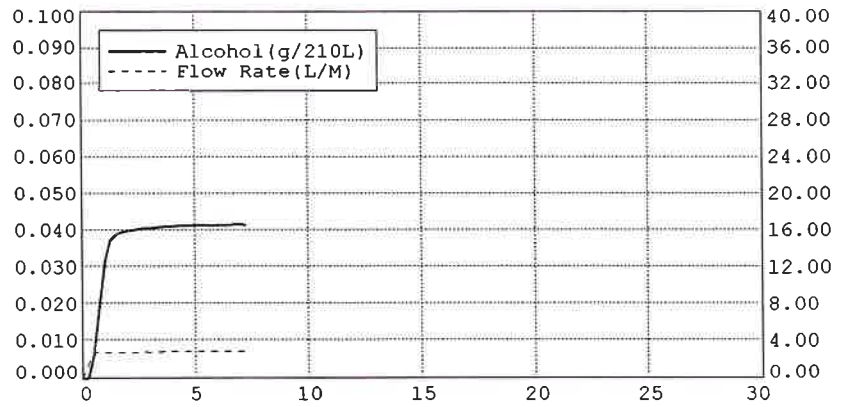

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100403






Date: 11/24/2025
Time: 09:16:39

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.82: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 1117 psi

BLANK TEST	0.000	09:17
INTERNAL STANDARD	VERIFIED	09:18
EXTERNAL STANDARD	0.082	09:18
BLANK TEST	0.000	09:19
EXTERNAL STANDARD	0.082	09:19
BLANK TEST	0.000	09:20
EXTERNAL STANDARD	0.082	09:20
BLANK TEST	0.000	09:21
EXTERNAL STANDARD	0.082	09:21
BLANK TEST	0.000	09:22
EXTERNAL STANDARD	0.082	09:22
BLANK TEST	0.000	09:23

Average = 0.0820
Std Dev = 0.0000

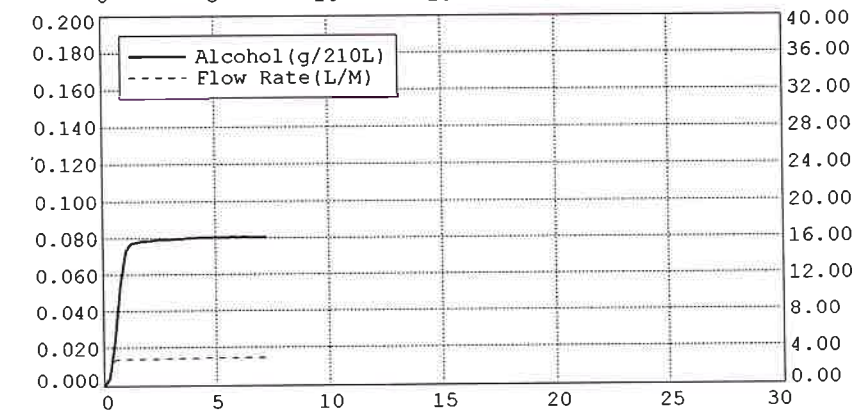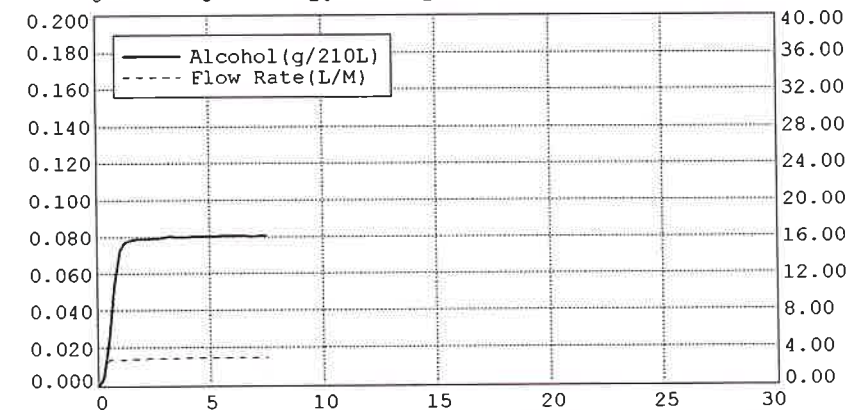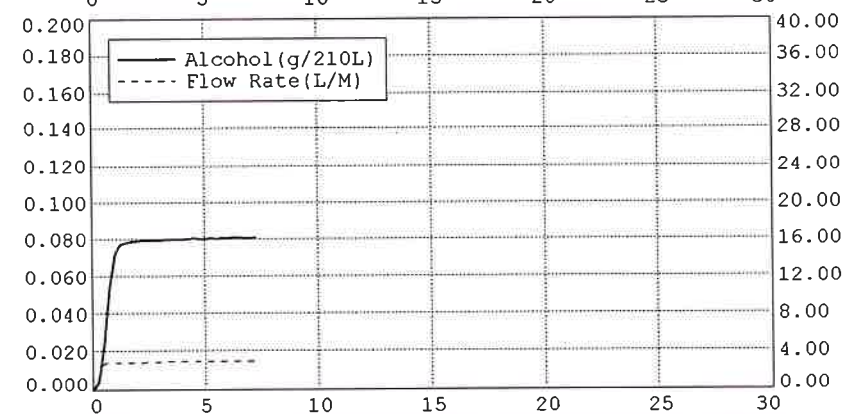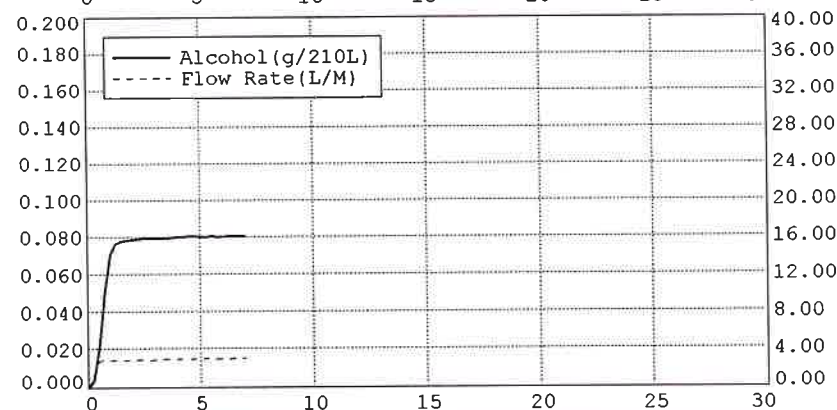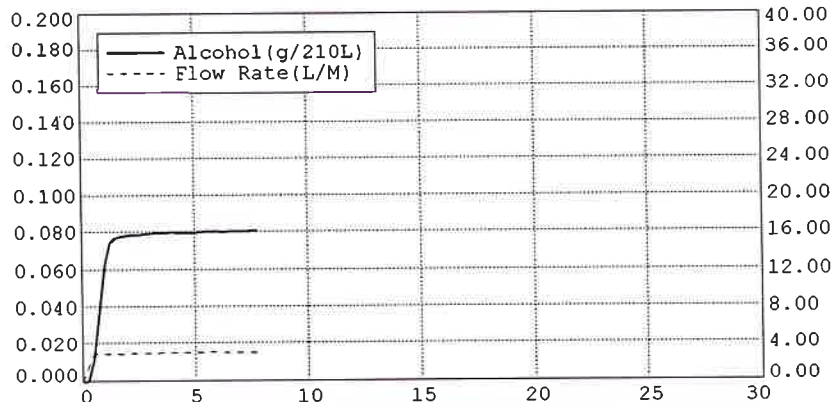

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100403






Date: 11/24/2025
Time: 09:24:41

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.83: 0.100
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 727 psi

BLANK TEST	0.000	09:25
INTERNAL STANDARD	VERIFIED	09:26
EXTERNAL STANDARD	0.103	09:26
BLANK TEST	0.000	09:27
EXTERNAL STANDARD	0.102	09:27
BLANK TEST	0.000	09:28
EXTERNAL STANDARD	0.102	09:28
BLANK TEST	0.000	09:29
EXTERNAL STANDARD	0.102	09:29
BLANK TEST	0.000	09:30
EXTERNAL STANDARD	0.103	09:30
BLANK TEST	0.000	09:31

Average = 0.1024
Std Dev = 0.0005

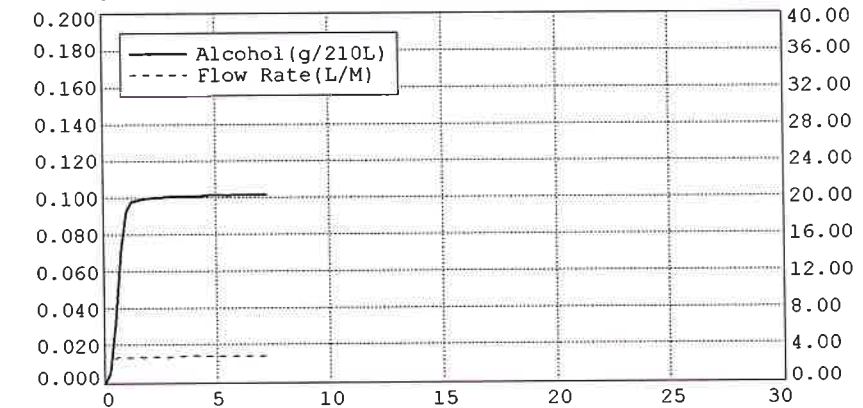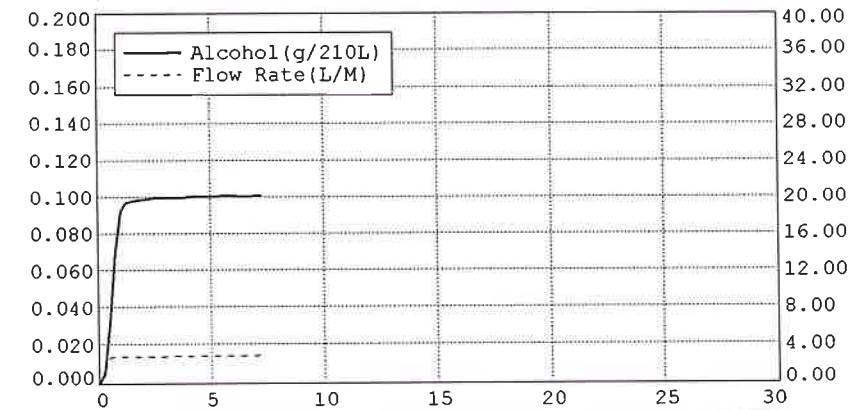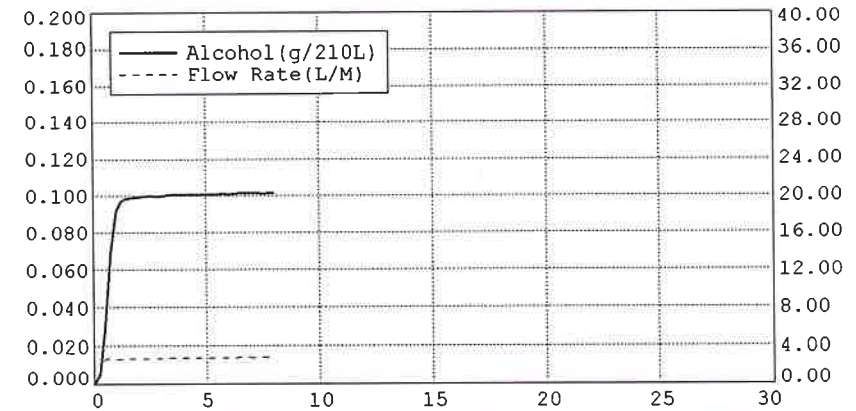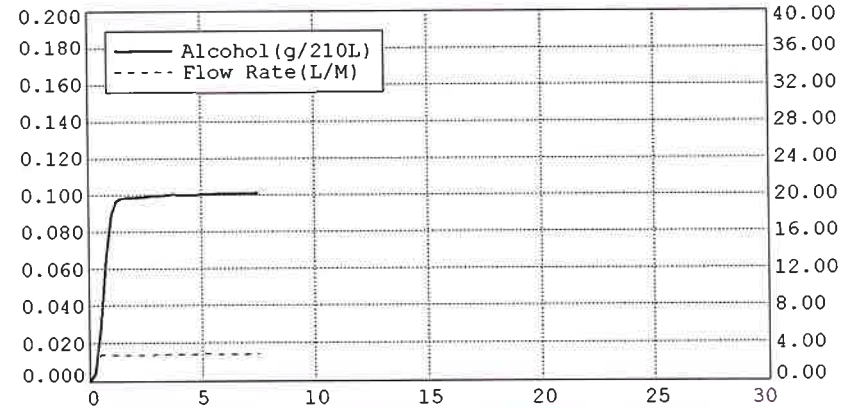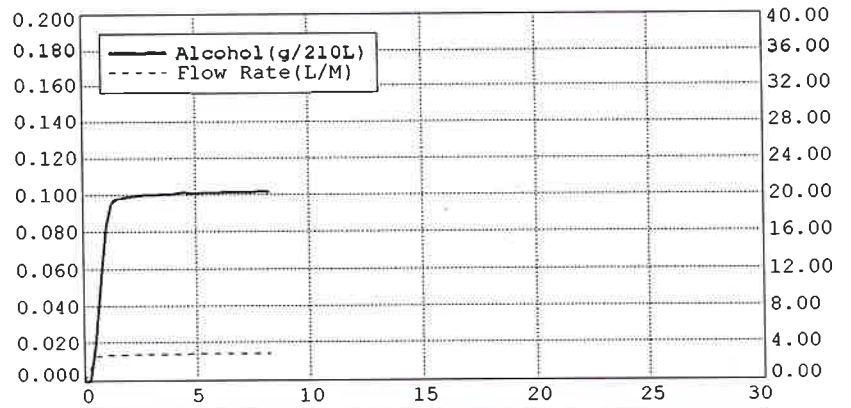

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100403






Date: 11/24/2025
Time: 09:32:35

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.83: 0.149
LOT #: AG515604
EXPIRATION: 06/05/2027
TANK PRESSURE: 756 psi

BLANK TEST	0.000	09:33
INTERNAL STANDARD	VERIFIED	09:33
EXTERNAL STANDARD	0.150	09:34
BLANK TEST	0.000	09:35
EXTERNAL STANDARD	0.151	09:35
BLANK TEST	0.000	09:36
EXTERNAL STANDARD	0.150	09:36
BLANK TEST	0.000	09:37
EXTERNAL STANDARD	0.150	09:37
BLANK TEST	0.000	09:38
EXTERNAL STANDARD	0.150	09:38
BLANK TEST	0.000	09:39

Average = 0.1502
Std Dev = 0.0004

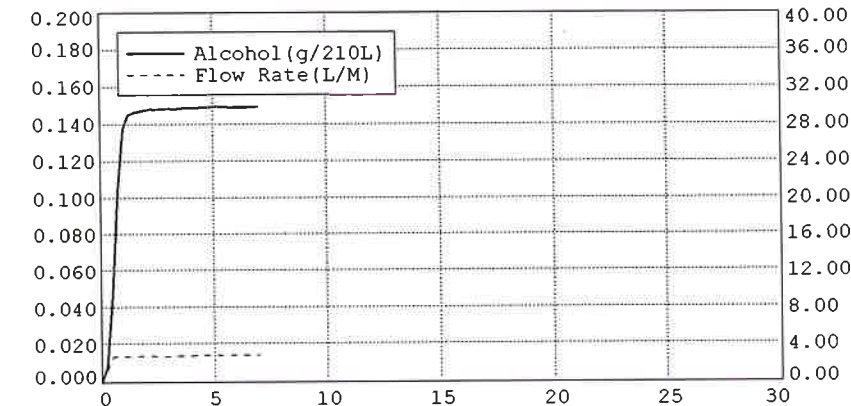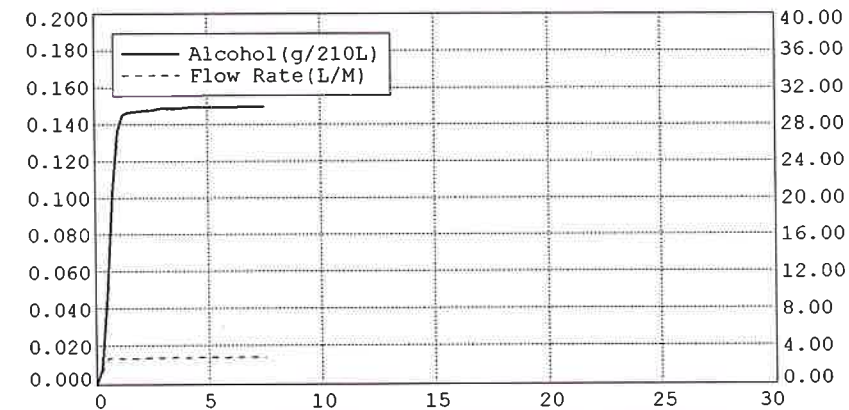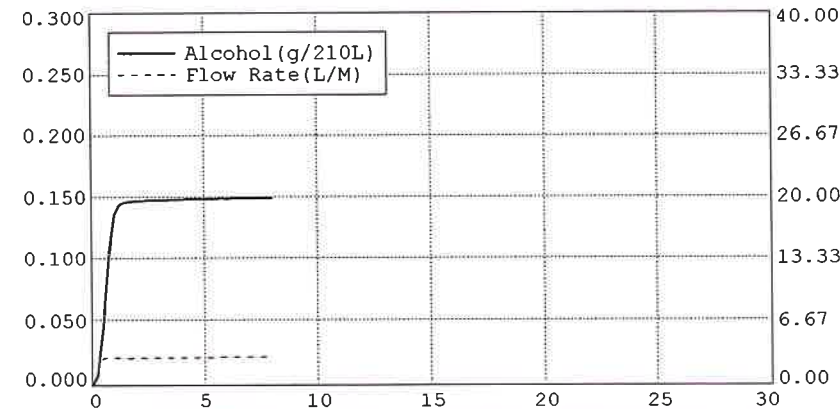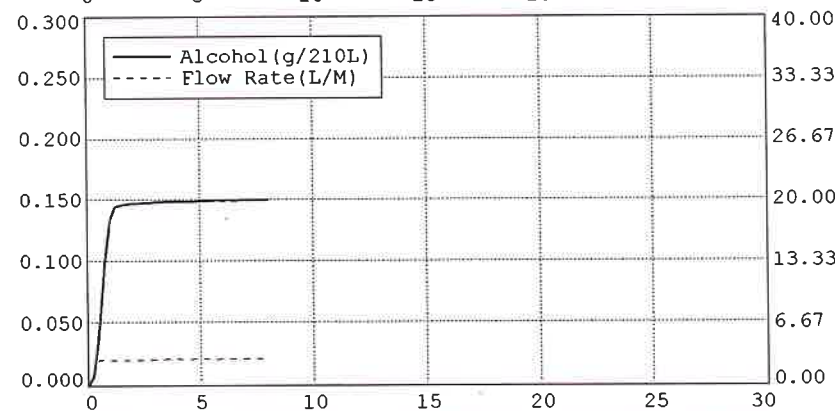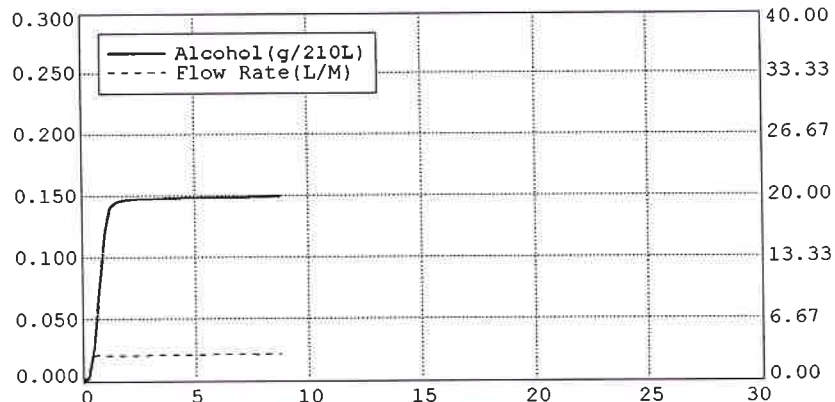

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100403






Date: 11/24/2025
Time: 09:40:59

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.83: 0.299
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 265 psi

BLANK TEST	0.000	09:42
INTERNAL STANDARD	VERIFIED	09:42
EXTERNAL STANDARD	0.299	09:42
BLANK TEST	0.000	09:43
EXTERNAL STANDARD	0.298	09:43
BLANK TEST	0.000	09:44
EXTERNAL STANDARD	0.297	09:45
BLANK TEST	0.000	09:45
EXTERNAL STANDARD	0.298	09:46
BLANK TEST	0.000	09:47
EXTERNAL STANDARD	0.298	09:47
BLANK TEST	0.000	09:48

Average = 0.2980
Std Dev = 0.0007

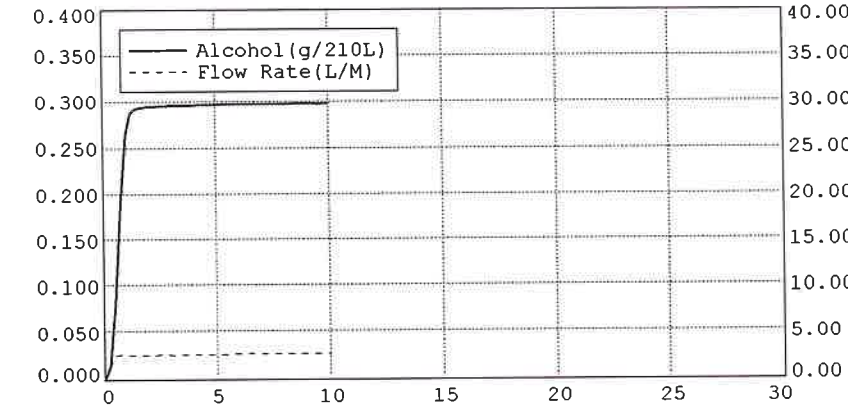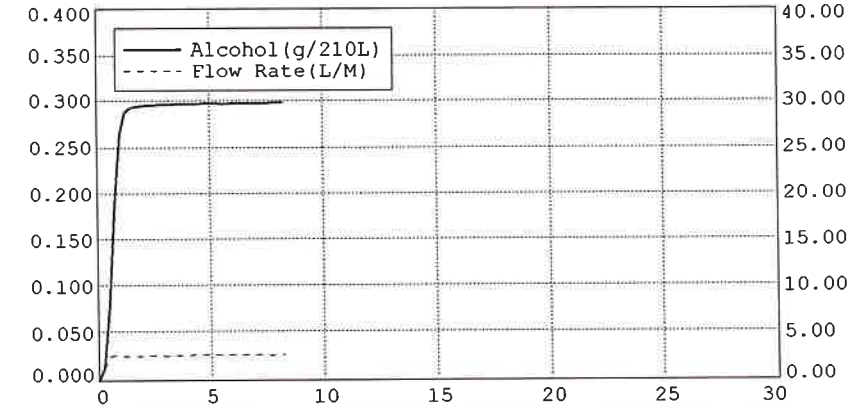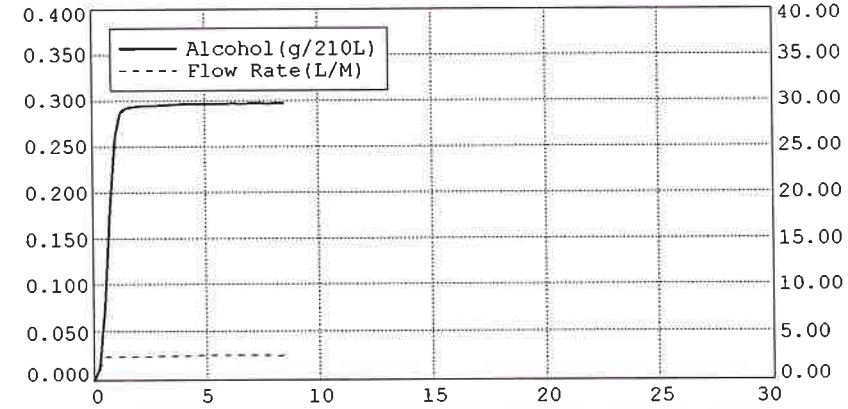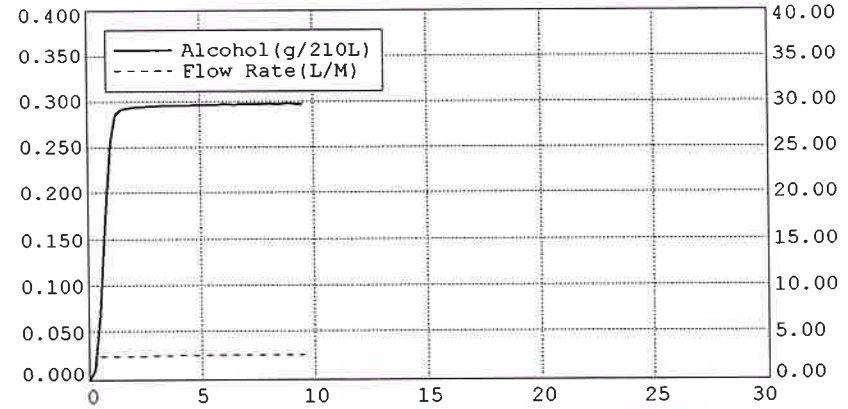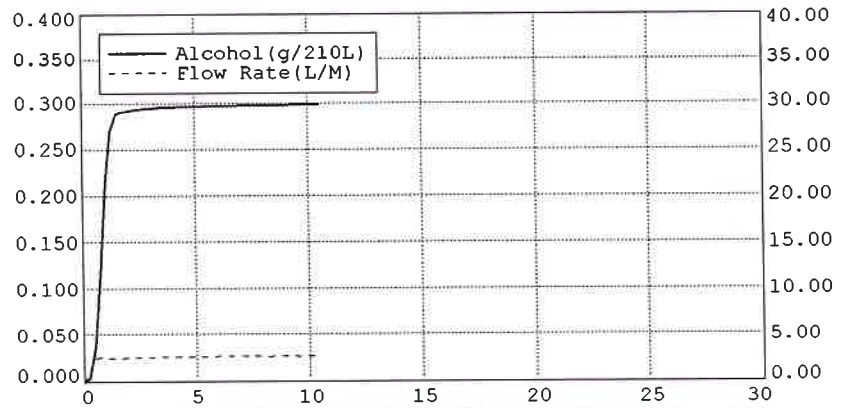

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100403

Date: 11/24/2025
Time: 09:53:49

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
DEREK WALTON
OPERATOR'S #: 9508

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.82: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	09:57
BLANK TEST	0.000	09:57
INTERNAL STANDARD	VERIFIED	09:57
EXTERNAL STANDARD	0.082	09:57
BLANK TEST	0.000	09:58
SUBJECT SAMPLE	INCOMPLETE	10:00

DMC

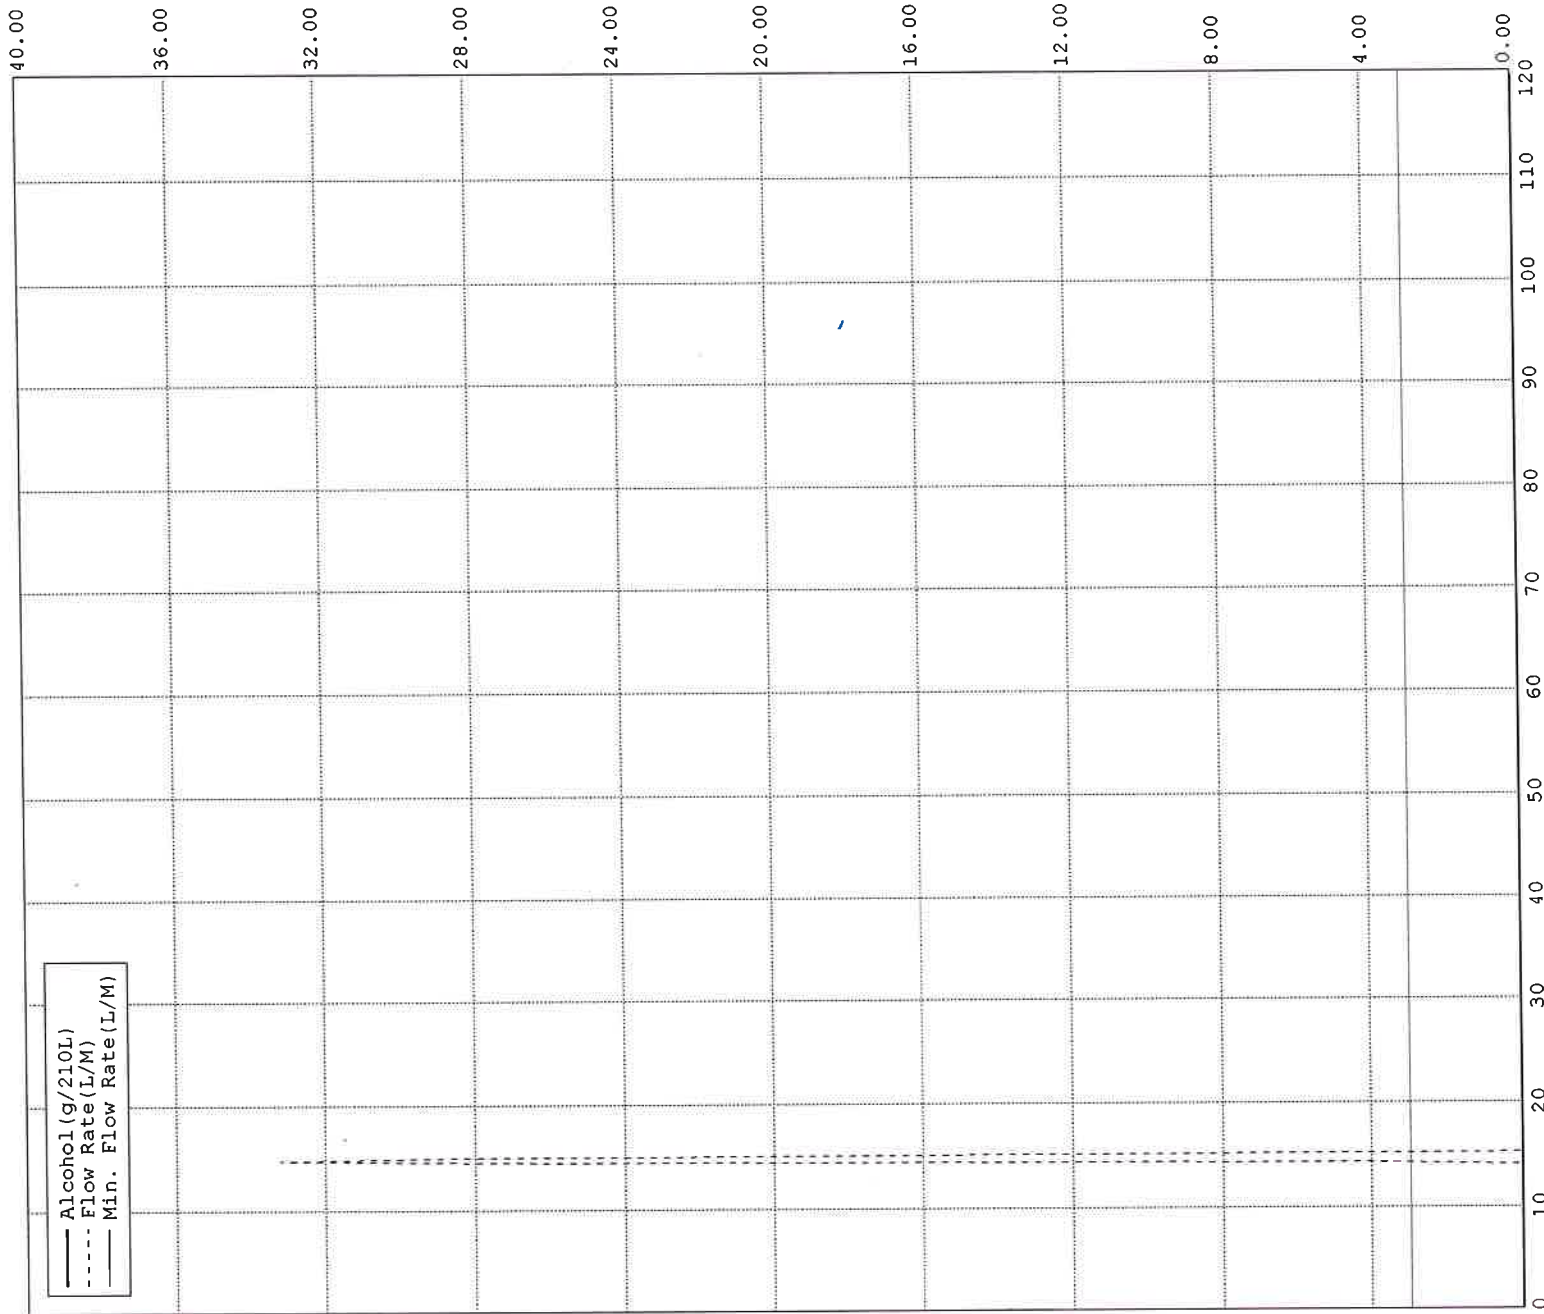

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100403

Date: 11/24/2025
Time: 10:04:40

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
DEREK WALTON
OPERATOR'S #: 9508


DEPT/AGENCY:
MAX ATTEMPTS
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.83: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:05
BLANK TEST	0.000	10:05
INTERNAL STANDARD	VERIFIED	10:05
EXTERNAL STANDARD	0.082	10:06
BLANK TEST	0.000	10:07
SUBJECT SAMPLE	XXX	10:07

Maximum Attempts Exceeded

[Handwritten signature]

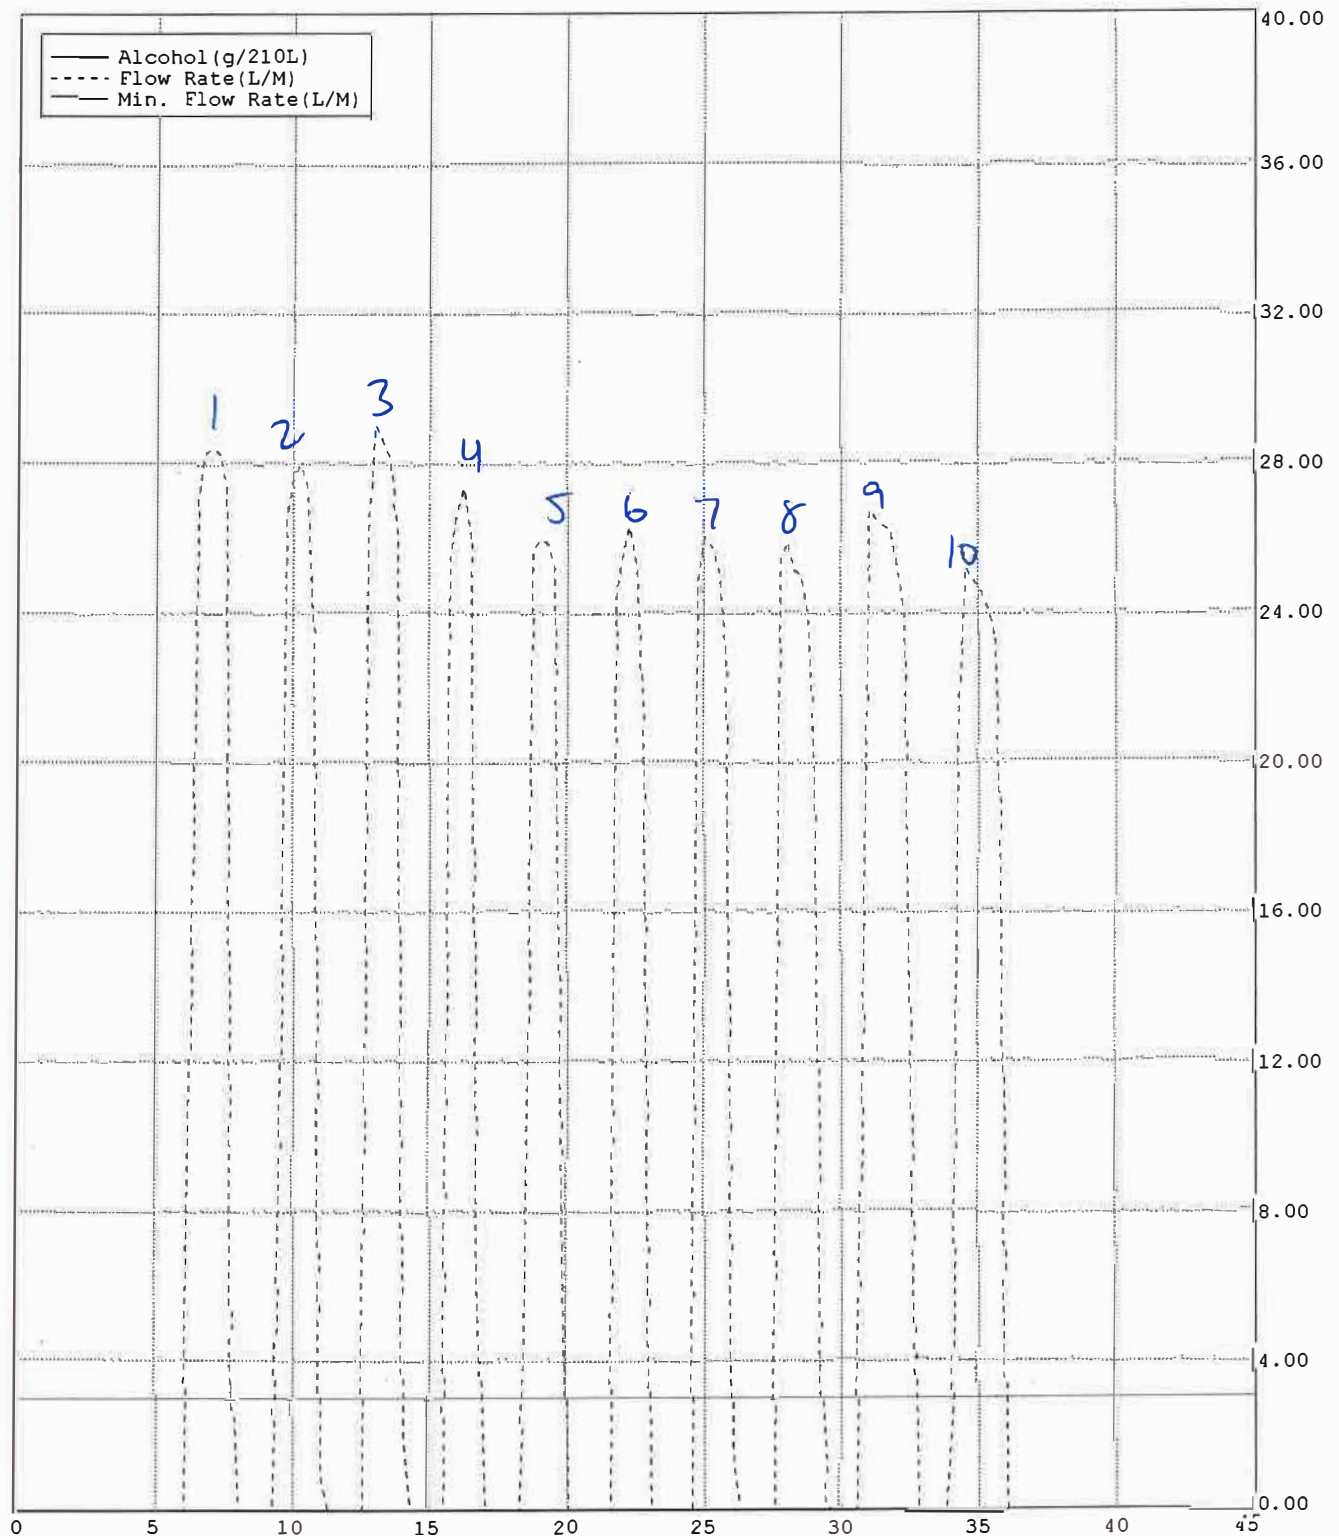

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100403

Date: 11/24/2025
 Time: 10:09:56

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXXX


OPERATOR NAME:
 DEREK WALTON
 OPERATOR'S #: 9508

DEPT/AGENCY:
 INVALID
 CASE/REPORT: XXXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.83: 0.080
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:18
BLANK TEST	0.000	10:18
INTERNAL STANDARD	VERIFIED	10:18
EXTERNAL STANDARD	0.082	10:18
BLANK TEST	0.000	10:19
SUBJECT SAMPLE	INVALID	10:20

MLC

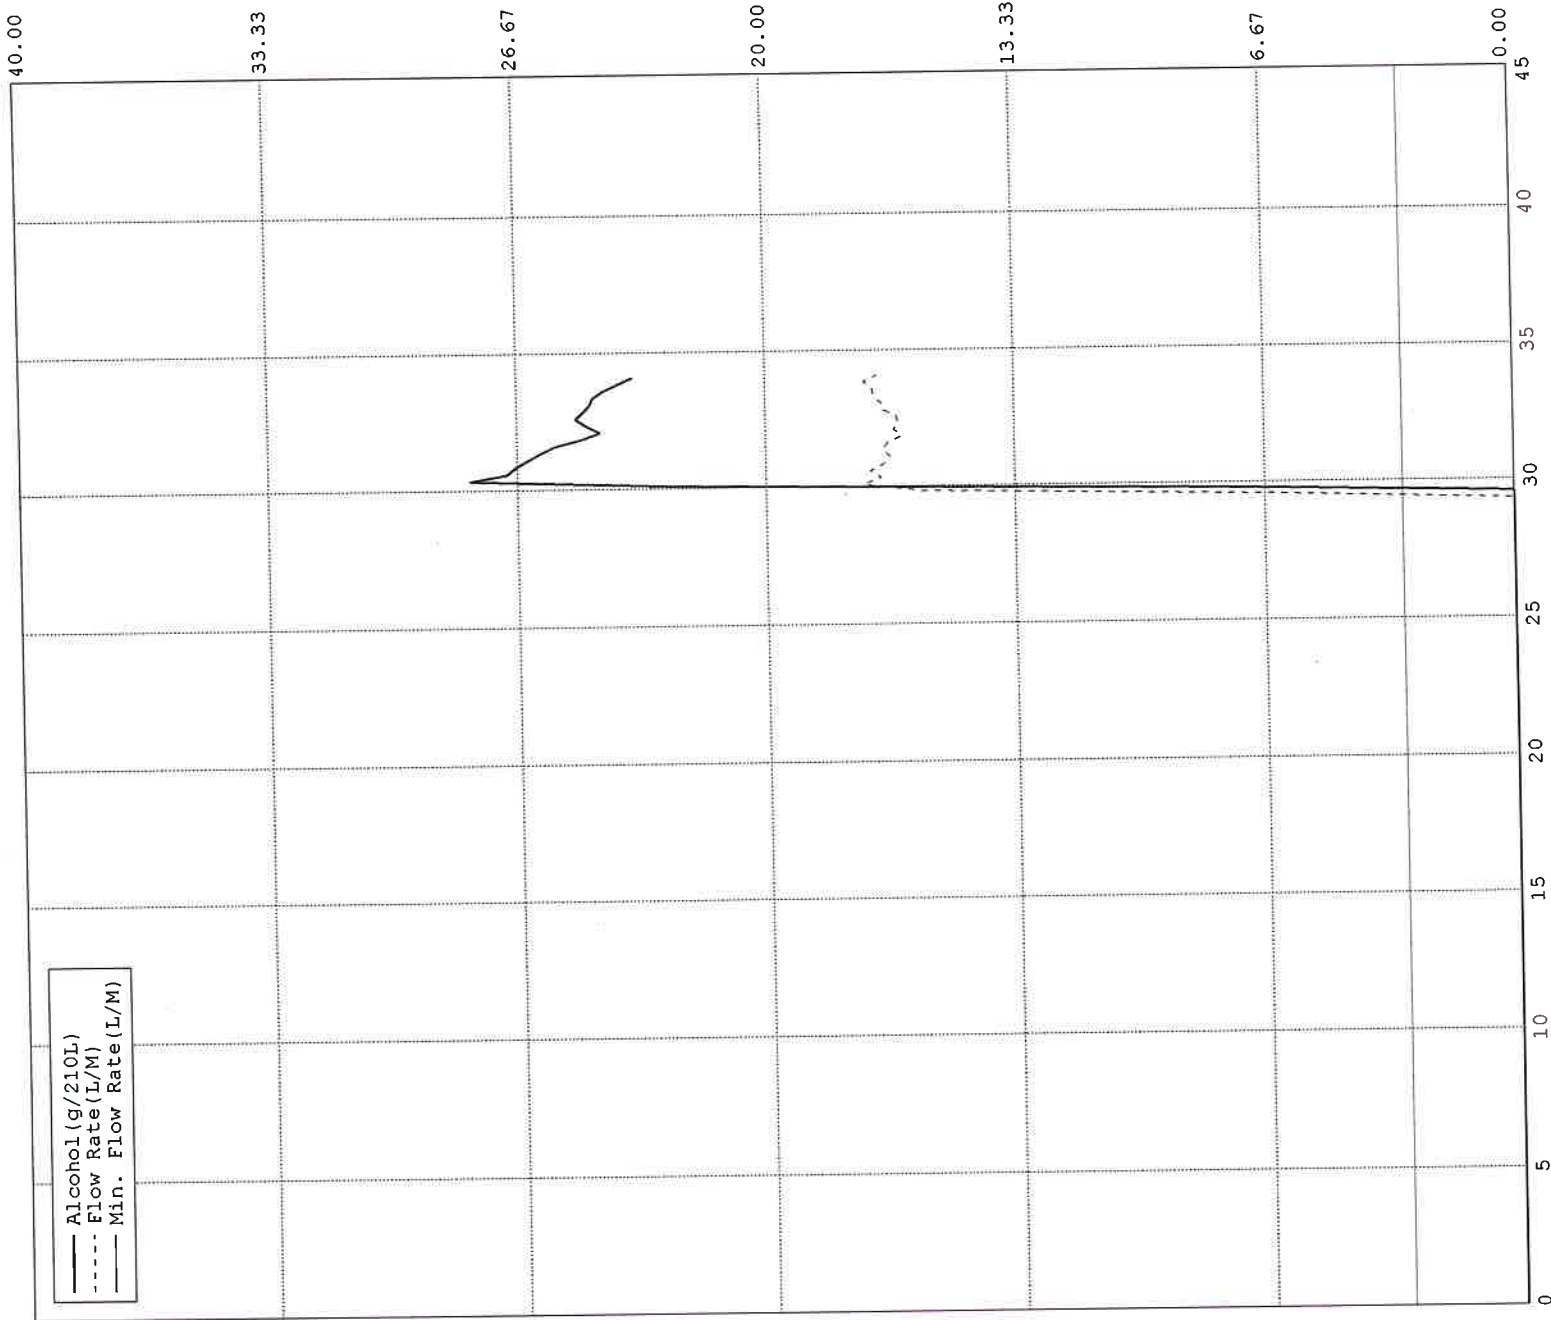

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100403

Date: 11/24/2025
Time: 10:22:36

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

DEREK WALTON

OPERATOR'S #: 9508

DEPT/AGENCY:

RADIO FREQUENCY

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.83: 0.080

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD


EXTERNAL STANDARD

BLANK TEST

PASSED 10:24
0.000 10:24
VERIFIED 10:24
0.082 10:25
0.000 10:25

RFI DETECTED

Handwritten signature

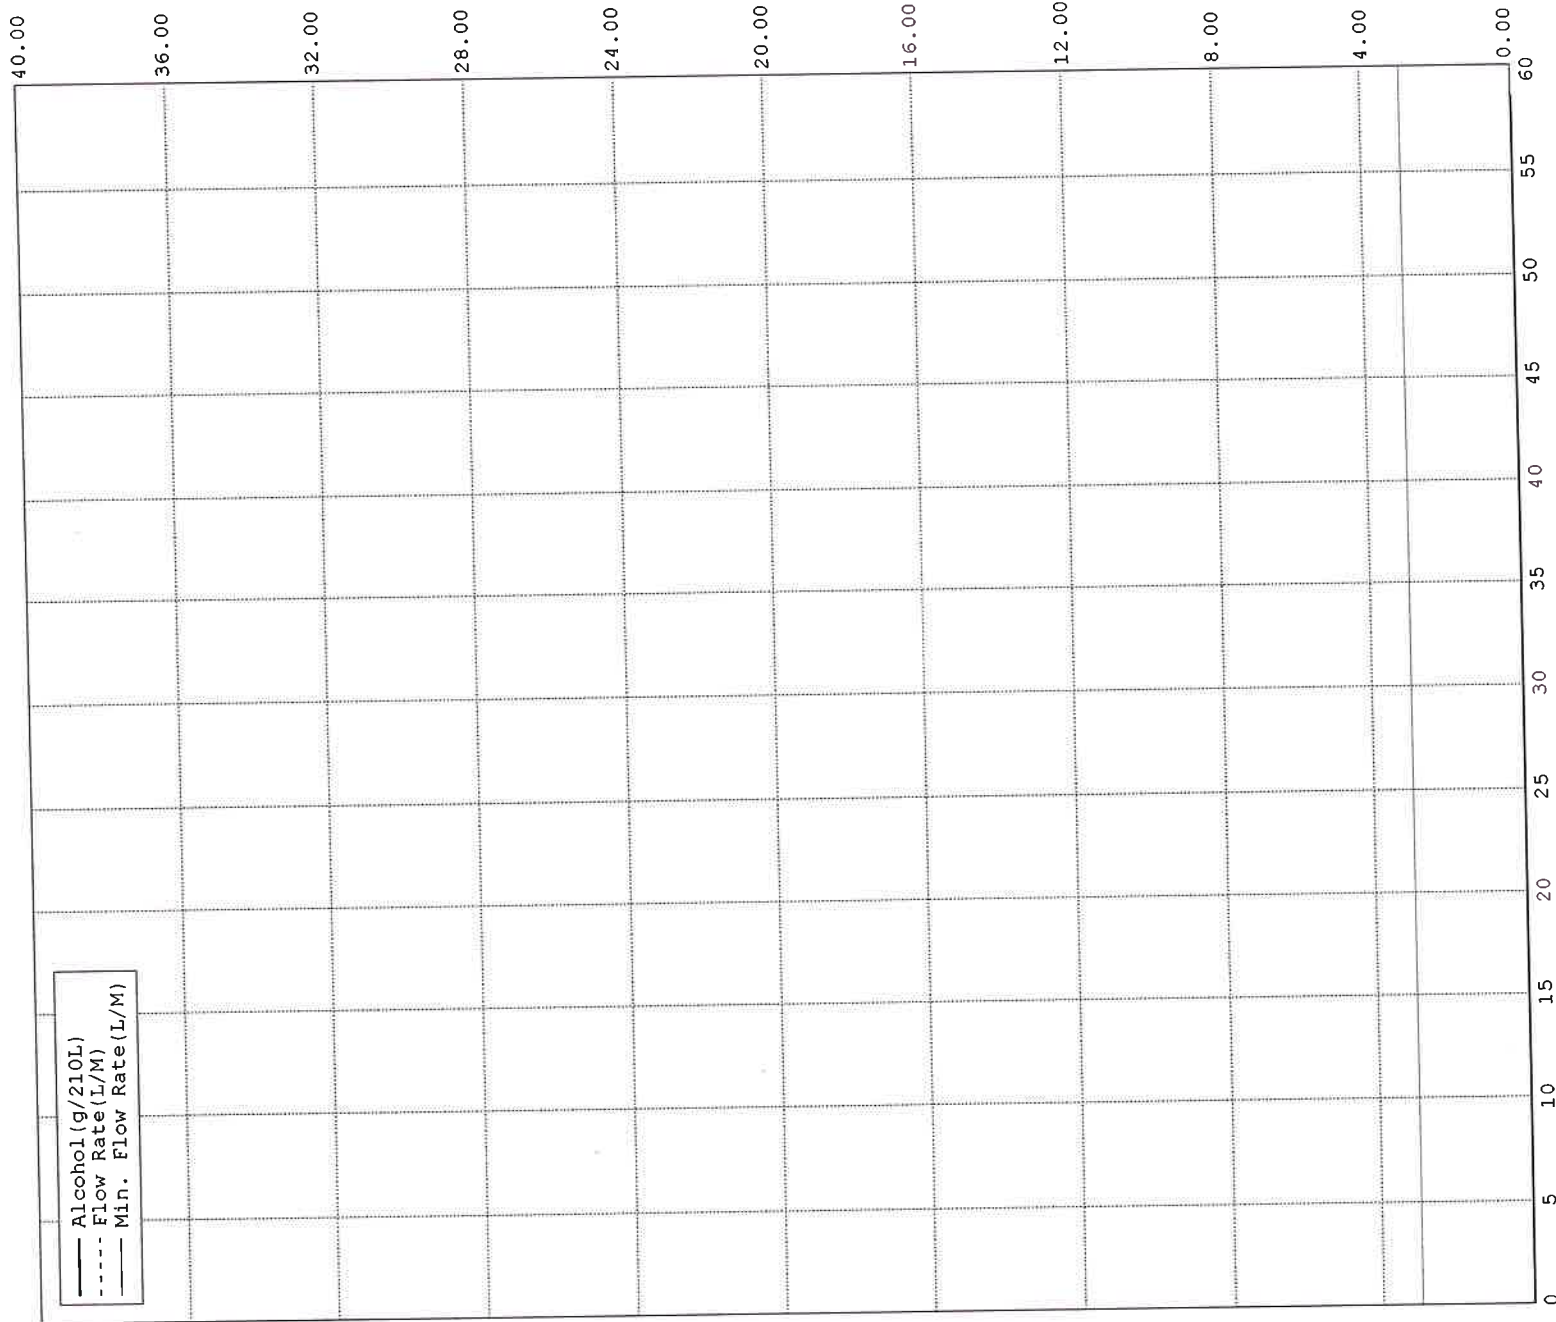

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100403

Date: 11/24/2025
Time: 10:38:59

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
DEREK WALTON
OPERATOR'S #: 9508

DEPT/AGENCY:
INTERFERENCE ACETONE
CASE/REPORT: XXXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.83: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:40
BLANK TEST	0.000	10:40
INTERNAL STANDARD	VERIFIED	10:40
Xq = 0.076 (2.45%)		
EXTERNAL STANDARD	0.082	10:41
X[1] = 0.0818 (0.0001) (0.0005)		
BLANK TEST	0.000	10:42
SUBJECT SAMPLE	XXX	10:44
X[1] = 0.1048 (-0.0192) (0.0012)		

Interference Detected

Filter 2 average: -0.0003
Filter 3 average: 0.0004
DJW 11/24/2025

DJW

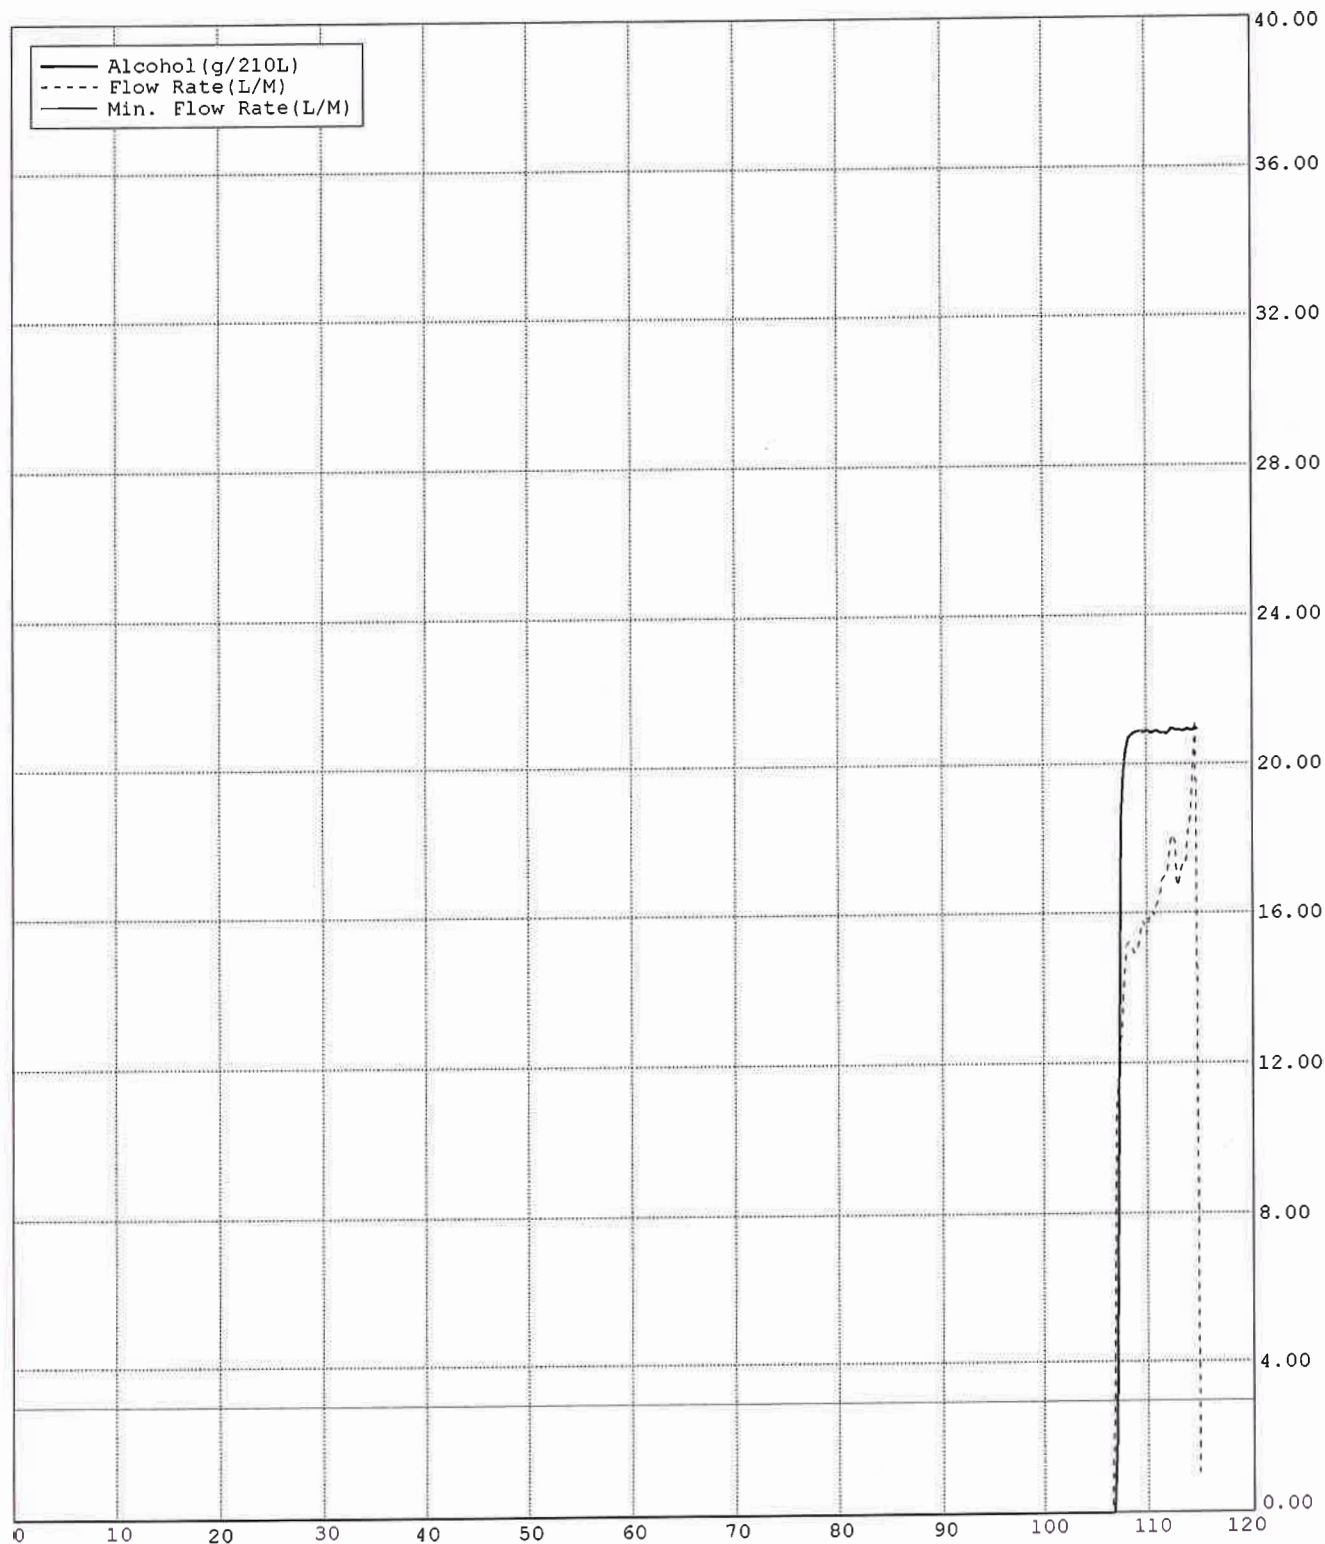

SUBJECT TEST

Alaska Department of Public Safety
 DATA MASTER dmt: 100403

Date: 11/24/2025
 Time: 10:32:02

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXXX

OPERATOR NAME:
 DEREK WALTON
 OPERATOR'S #: 9508

DEPT/AGENCY:
 INTERFERENCE ISOPROPANOL
 CASE/REPORT: XXXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.83: 0.080
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:33
BLANK TEST	0.000	10:33
INTERNAL STANDARD	VERIFIED	10:33
$X_q = 0.074$ (0.23%)		
EXTERNAL STANDARD	0.081	10:33
$X[1] = 0.0814$ (-0.0014)	(0.0007)	
BLANK TEST	0.000	10:34
SUBJECT SAMPLE	XXX	10:35
$X[1] = 0.1199$ (-0.0207)	(0.0023)	

Interference Detected

Handwritten signature



SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100403

Date: 11/24/2025
 Time: 10:47:14

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXXX


OPERATOR NAME:
 DEREK WALTON
 OPERATOR'S #: 9508

DEPT/AGENCY:
 INTERFERENCE NEGATIVE
 CASE/REPORT: XXXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.85: 0.080
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:49
BLANK TEST	0.000	10:49
INTERNAL STANDARD	VERIFIED	10:50
Xq = 0.076 (2.45%)		
EXTERNAL STANDARD	0.082	10:50
X[1] = 0.0819 (-0.0004)	(0.0004)	
BLANK TEST	0.000	10:51
SUBJECT SAMPLE (Vol=2.12L)	0.091	10:51
X[1] = 0.0913 (-0.0015)	(0.0008)	
BLANK TEST	0.000	10:52
EXTERNAL STANDARD	0.082	10:52
X[1] = 0.0819 (0.0006)	(0.0000)	
BLANK TEST	0.000	10:53

MLC

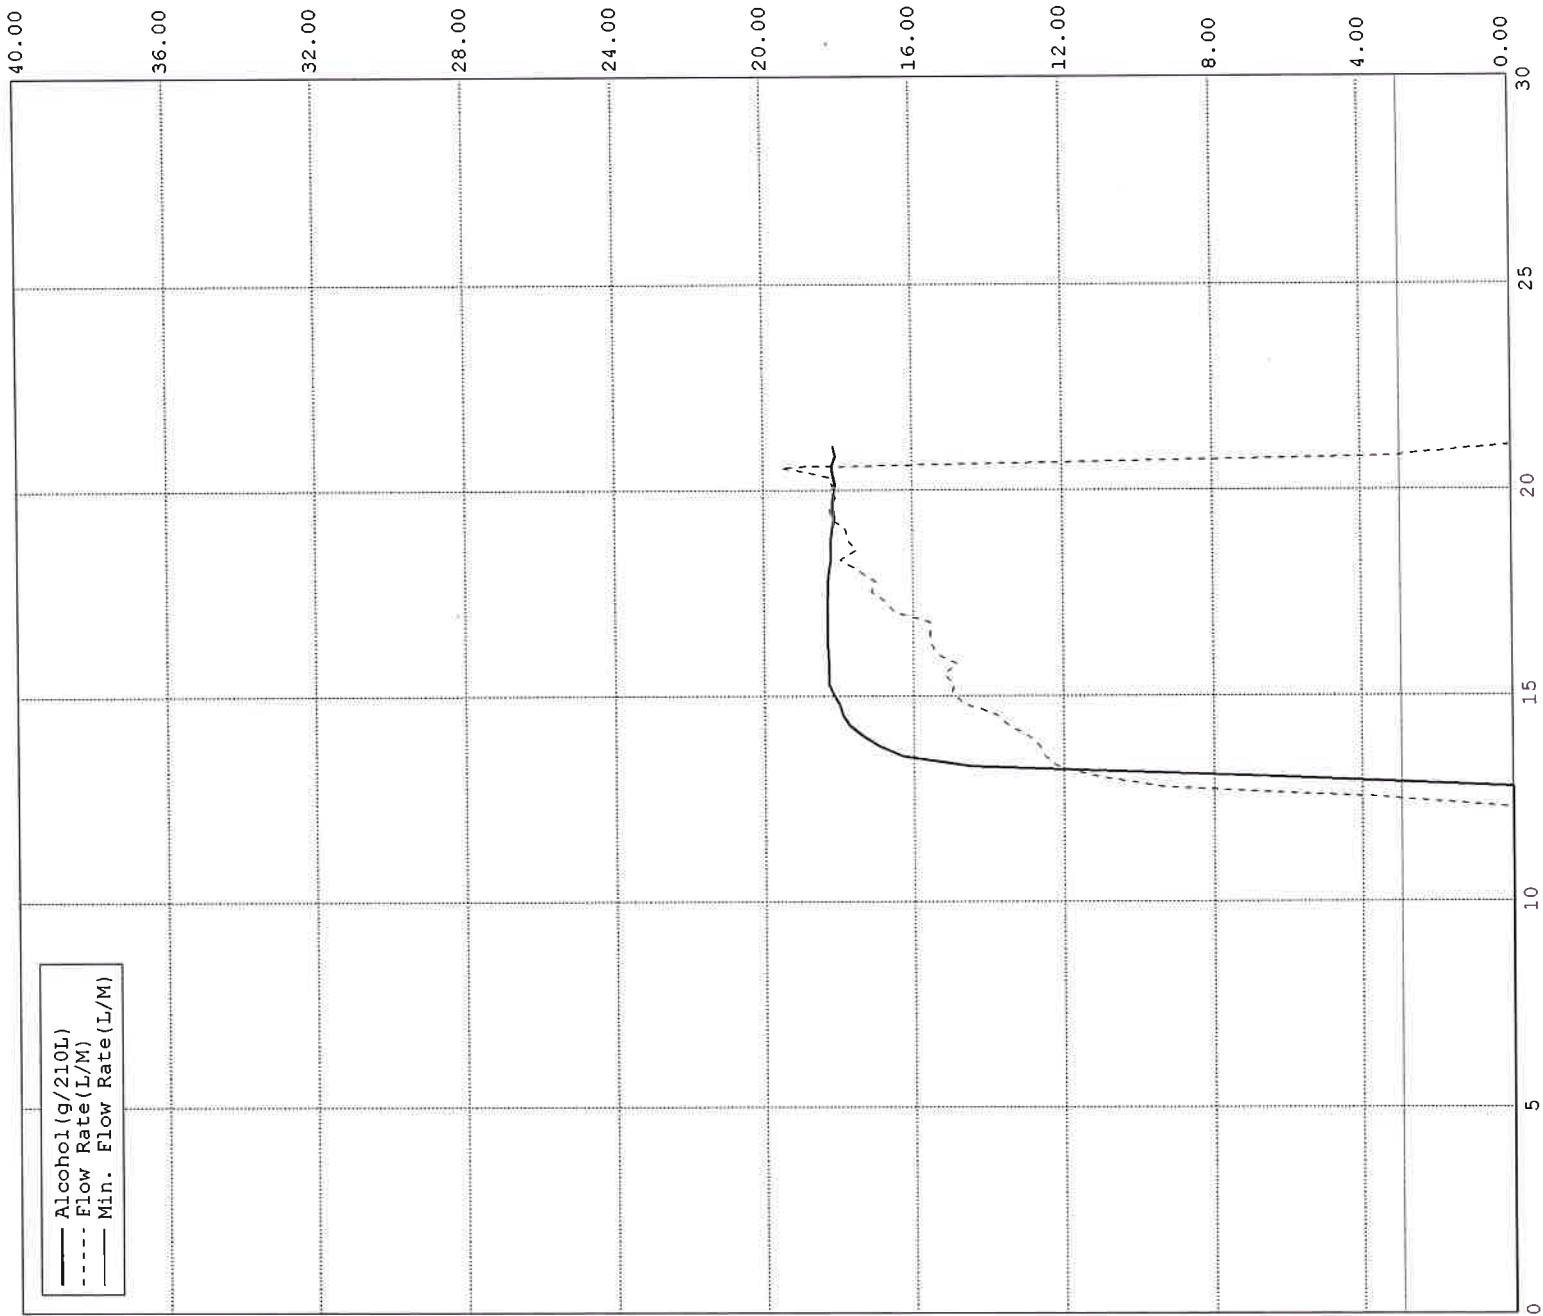

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100403

Date: 11/24/2025
Time: 11:20:27

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
DEREK WALTON
OPERATOR'S #: 9508
Non-Drinking DJW 12/01/2025
DEPT/AGENCY:
~~NON-DRINKING~~ SUBJECT
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.85: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:21
BLANK TEST	0.000	11:21
INTERNAL STANDARD	VERIFIED	11:21
EXTERNAL STANDARD	0.082	11:21
BLANK TEST	0.000	11:22
SUBJECT SAMPLE (Vol=3.26L)	0.000	11:23
BLANK TEST	0.000	11:24
EXTERNAL STANDARD	0.082	11:24
BLANK TEST	0.000	11:25

DW

