

# Alaska Scientific Crime Detection Laboratory

## Change in Instrument Status Form

Issued: 12/15/2017  
Effective: 12/15/2017

Version: CIISF 2017 R0  
Status: Active

Date: 9/13/18 Instrument Serial Number: 100395

Instrument Location: Hoonah PD

Supervisor Name and Agency: Michael Ivie / Hoonah PD

Describe the Status Change or Issue with the Instrument:

Instrument is not allowing to provide a subject sample. It keeps asking to provide a sample with the intermittent tone. It also keeps having a gas flow error status message due to a gas tube that keeps coming off.

If instrument was placed in service or removed from service, fill out the appropriate sections below.

In Service Date/Time: \_\_\_\_\_

Out of Service Date/Time: ~~9/13/18 04:35~~ 08/31/18 @ 1430.

For Use by SCDL

Additional Notes

Lt. William Mills took instrument out of service on 08/31/2018 at 1430. JMV 09/11/18

Email completed form to [dps.scdl.toxicology@alaska.gov](mailto:dps.scdl.toxicology@alaska.gov)

For questions contact the Breath Alcohol Program at 907-269-5740

# VERIFICATION OF CALIBRATION REPORT

*of DataMaster dmt Breath Test Instrument*

*State of Alaska*

Serial #: 100395

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

Date: 08/30/2018

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.81: 0.080  
LOT #: AG634001  
EXPIRATION: 12/05/2018  
TANK PRESSURE: 759 psi

BLANK TEST                      0.000    08:56  
INTERNAL STANDARD            VERIFIED   08:56

Gas Flow Error

## Diagnostic Check

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.8°C            PASSED  
Breath Tube      = 48.0°C            PASSED

PUMP INFO  
Flow Rate = 4.632 L/M                PASSED

DETECTOR INFO  
PUMP ON                                PASSED  
PUMP OFF                                PASSED

FILTER INFO  
Filter 1                                 PASSED  
Filter 2                                 PASSED  
Filter 3                                 PASSED

INTERNAL STANDARD                    PASSED

SUBJECT TEST

Alaska Department of Public Safety  
DATA MASTER dmt: 100395

Date: 08/30/2018  
Time: 08:32:04

SUBJECT NAME:  
TEST TEST  
LICENSE #: 12345

OPERATOR NAME:  
RICK C GROSHONG  
OPERATOR'S #: 2683

DEPT/AGENCY:  
HPD  
CASE/REPORT: 12345  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.81: 0.080  
LOT #: AG634001  
EXPIRATION: 12/05/2018

DIAGNOSTIC CHECK  
BLANK TEST  
INTERNAL STANDARD  
PASSED 08:33  
0.000 08:33  
VERIFIED 08:33

Gas Flow Error

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100395

Date: 09/04/2018  
Time: 04:34:49


SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXXXXXXX

OPERATOR NAME:  
MICHAEL D IVIE  
OPERATOR'S #: 8031

DEPT/AGENCY:  
HOONAH PD  
CASE/REPORT: 0000000000  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 30.14: 0.081  
LOT #: AG634001  
EXPIRATION: 12/05/2018

DIAGNOSTIC CHECK	PASSED	04:35
BIANK TEST	0.000	04:35
INTERNAL STANDARD	VERIFIED	04:36
EXTERNAL STANDARD	0.076	04:36
BIANK TEST	0.000	04:37
SUBJECT SAMPLE	INCOMPLETE	04:39

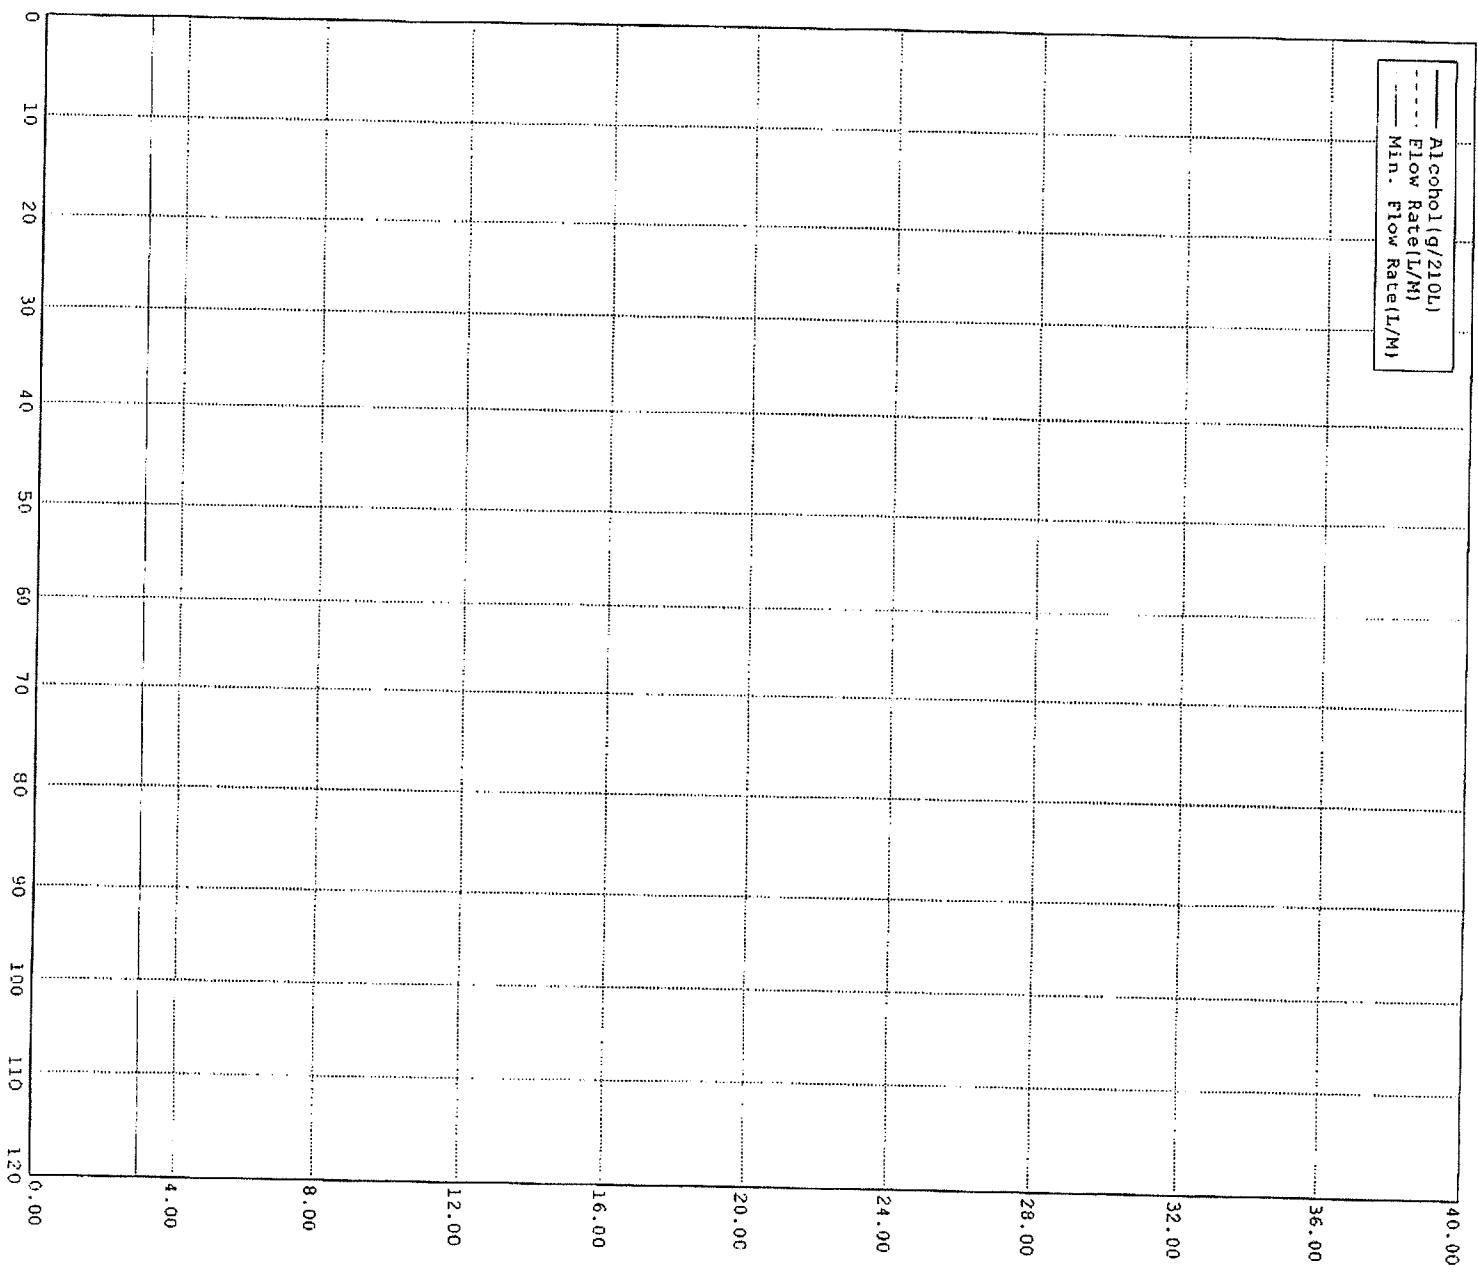

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100395

Date: 09/04/2018  
Time: 08:03:33

SUBJECT NAME:  
TEST TEST  
LICENSE #: 12345

OPERATOR NAME:  
RICK C GROSHONG  
OPERATOR'S #: 2683

DEPT/AGENCY:  
HPD1  
CASE/REPORT: 12345  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 30.15: 0.081  
LOT #: AG634001  
EXPIRATION: 12/05/2018

DIAGNOSTIC CHECK	PASSED	08:04
BLANK TEST	0.000	08:04
INTERNAL STANDARD	VERIFIED	08:04
EXTERNAL STANDARD	0.076	08:04
BLANK TEST	0.000	08:05
SUBJECT SAMPLE	INCOMPLETE	08:07

