

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Serial #: 100379

Date: 03/20/2013

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.64: 0.079
LOT #: 02012080A1
EXPIRATION: 03/01/2014

BLANK TEST	0.000	09:49
INTERNAL STANDARD	VERIFIED	09:49
EXTERNAL STANDARD	0.078	09:49
BLANK TEST	0.000	09:50
EXTERNAL STANDARD	0.077	09:50
BLANK TEST	0.000	09:51
EXTERNAL STANDARD	0.078	09:52
BLANK TEST	0.000	09:52
EXTERNAL STANDARD	0.078	09:53
BLANK TEST	0.000	09:54
EXTERNAL STANDARD	0.078	09:54
BLANK TEST	0.000	09:55

Average = 0.0778
Std Dev = 0.0004

Diagnostic Check

VERSIONS

DMT: 2.00
PIC: 3.02
Modem: 2.3
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.6°C PASSED
Breath Tube = 43.8°C PASSED

PUMP INFO

Flow Rate = 4.800 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO


Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:



- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

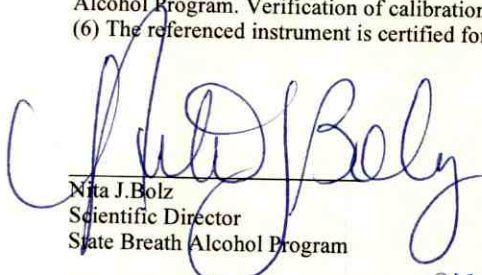
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

3/27/2013

Subscribed and sworn before me this 27 day of Mar. 20 13


Nikki Roth, Notary Public
My Commission Expires With Office

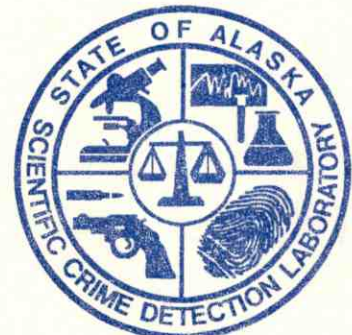

C03 3/21/13