



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100678

Report Issue Date: 05/08/2024
Date Received: 2024-02-20
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG217902	0.019	0.020	0.019	0.020	0.020	0.020
0.080	0.078	AG310901	0.078	0.078	0.078	0.078	0.078	0.078
0.300	0.294	AG327804	0.295	0.295	0.295	0.295	0.295	0.295

As Found - Evaluation Analyst: Carlie Glaister
 As Found Conditions - Barometric Pressure (inHg): 29.46 Barometer Used: Fisher S/N 230307229 Temperature (C): 22.5 Relative Humidity (%): 12
 As-Found Lab Activity Date Range: 02/22/2024 - 02/22/2024

Replaced o-ring. Blank error occurred on the first VOC, this occurred on another instrument at the same time and appears to be environmental.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.019	AG217902	0.020	0.020	0.021	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG217904	0.041	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.078	AG310901	0.079	0.079	0.079	0.079	0.079	0.079	+/- 0.004
0.100	0.097	AG333401	0.100	0.100	0.100	0.100	0.100	0.100	+/- 0.004
0.150	0.146	AG332004	0.147	0.147	0.147	0.147	0.147	0.147	+/- 0.005
0.300	0.292	AG327804	0.299	0.299	0.299	0.298	0.299	0.299	+/- 0.011

As Left Conditions - Barometric Pressure (inHg): 29.22 Barometer Used: Fisher S/N 230307229 Temperature (C): 23.6 Relative Humidity (%): 19
 As-Left Lab Activity Date Range: 02/23/2024 - 02/23/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Carlie Glaister on 02/23/2024

carlie.glaister@alaska.gov

Technically and administratively reviewed by Derek Walton on 05/08/2024

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100678 Analyst or Technician Name: Carlisle Glaister
DataMaster DMT Calibration Start Date: 2/23/24

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 230307229
Calibration Due Date: 5/2/25
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.22 Temperature(C) 23.6 Relative Humidity(%) 19
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20240214003 Expiration Date: 5/14/24
Simulator S/N: SD1088 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20240214003 Expiration Date: 5/14/24
Simulator S/N: DR4161 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 22HP41201 Expiration Date: 8/24/24
Simulator S/N: SD1177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 230631106
Calibration Due Date: 9/19/25

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 2/23/24
Data Interpretation Date (Technician): NA (if applicable)
Data Interpretation Date (Analyst): 2/23/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100678

Date: 02/23/2024
Time: 08:52:11

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 48.1°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.71 V PASSED
(1.03 V - 2.39 V)
Cooler Voltage = 1.55 V PASSED
(1.00 V - 2.34 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Freq = 517 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.6 in

PUMP INFO

Flow Rate = 4.965 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED
Xq = 0.080 0.65% (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100678

Date: 02/23/2024
Time: 9:04 AM

Temperatures (°C)
Sample Cell: 48.7°C
Breath Tube: 48.1°C

Current Barometer 29.2 in
Volume (Ltr) 1.60

Settings
Lamp: 1.76 V
Bias: 80 V
Cooler: 1.41 V
Chopper: 516 Hz

Voltages (V)
Flow: 1.06 V
Detector: 0.011 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100678

Date: 10/12/2021
Time: 14:10:04

OPERATOR NAME:
BRANDI BARNETT
CERTIFICATE #: 7038

Ca = 0.1000
CAL = 0.989964 0.800 <= CAL < 1.200
b1 = 0.0009 0.0000 <= b1 < 0.0040
b2 = 0.0042 0.0010 <= b2 < 0.0100
b3 = 0.0012 0.0000 <= b3 < 0.0040
Xq = 0.0798 0.0500 <= Xq < 0.2000
a21 = 1.102522 1.050 <= a21 < 1.300
a31 = 0.457025 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100678

Date: 02/23/2024
Time: 09:20:27


SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	09:21
BLANK TEST	0.000	09:21
INTERNAL STANDARD	VERIFIED	09:21
EXTERNAL STANDARD	0.079	09:21
BLANK TEST	0.000	09:22
SUBJECT SAMPLE (Vol=1.58L)	0.000	09:23
BLANK TEST	0.000	09:24
EXTERNAL STANDARD	0.079	09:25
BLANK TEST	0.000	09:25

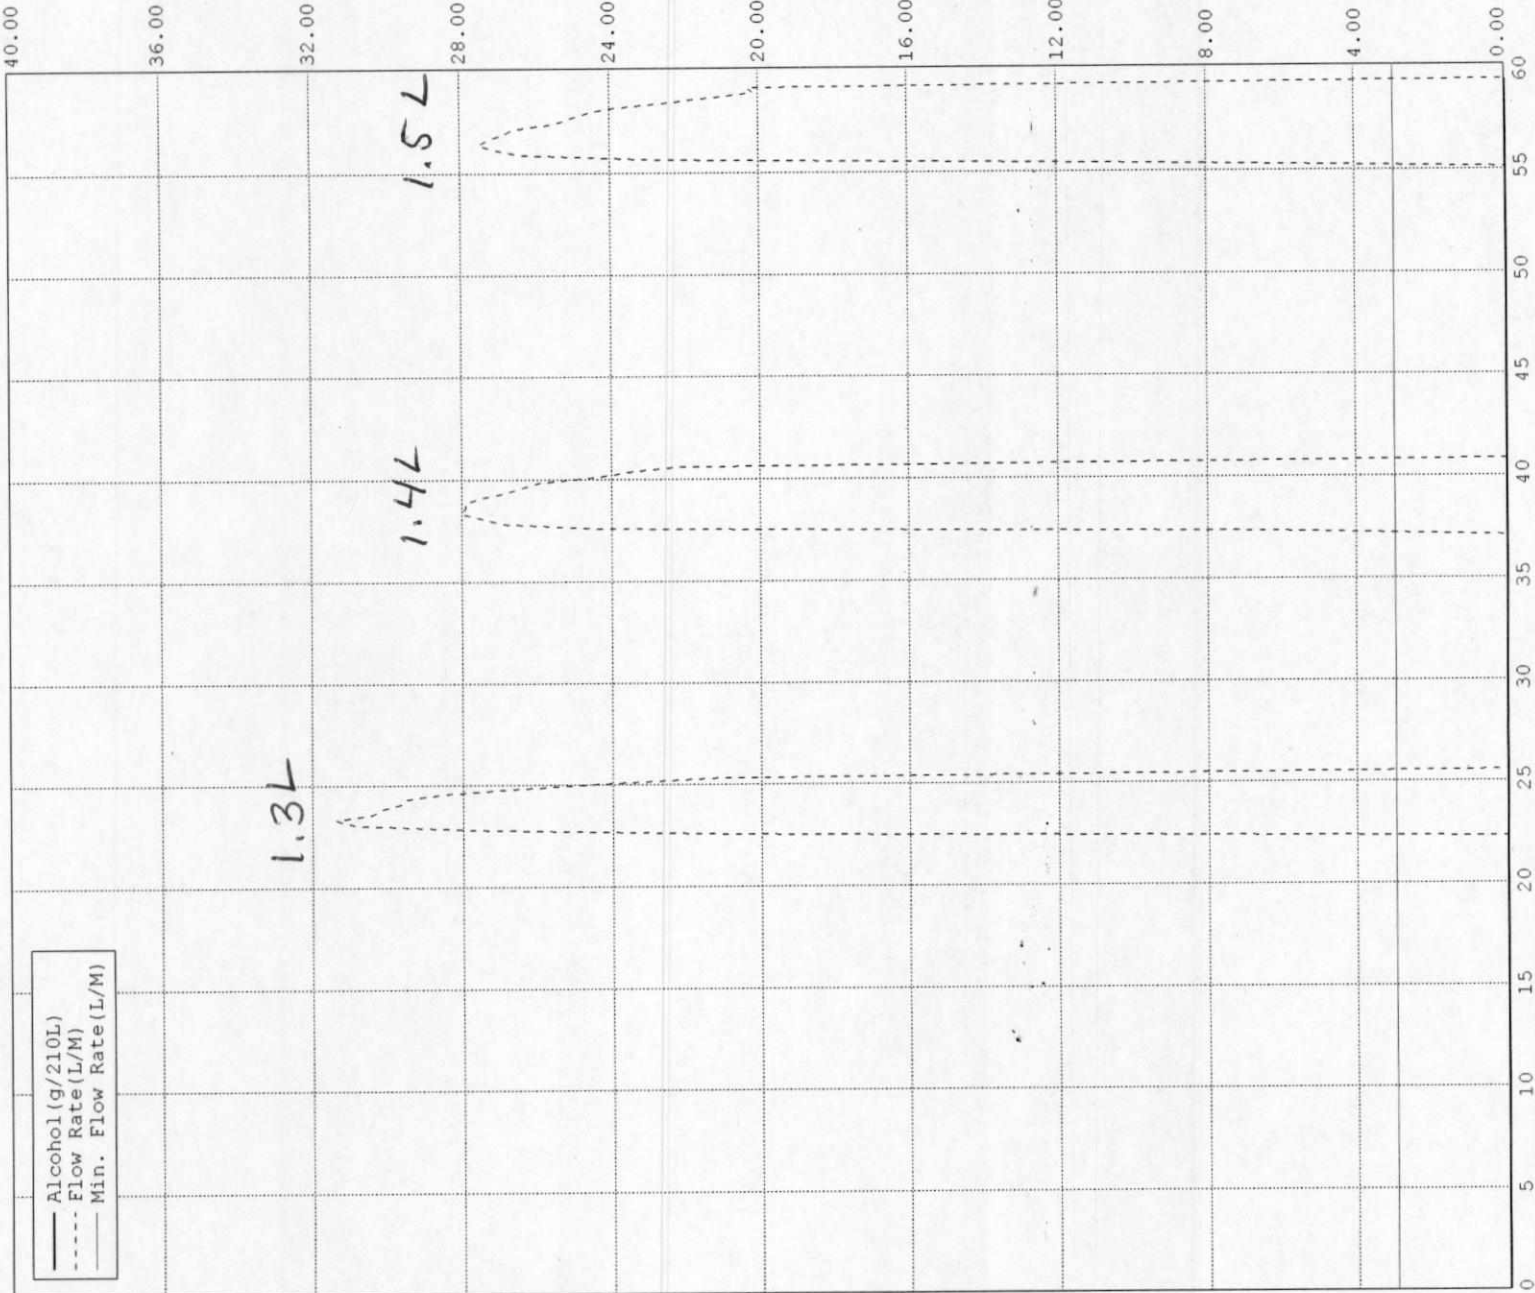

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100678

Date: 02/23/2024
 Time: 09:45:04

SUPERVISOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.019	0.0202	0.0004
0.039	0.0402	0.0004
0.078	0.0790	0.0000
0.097	0.1000	0.0000
0.146	0.1470	0.0000
0.292	0.2988	0.0004

SLOPE = 1.020079
 R² = 0.999867

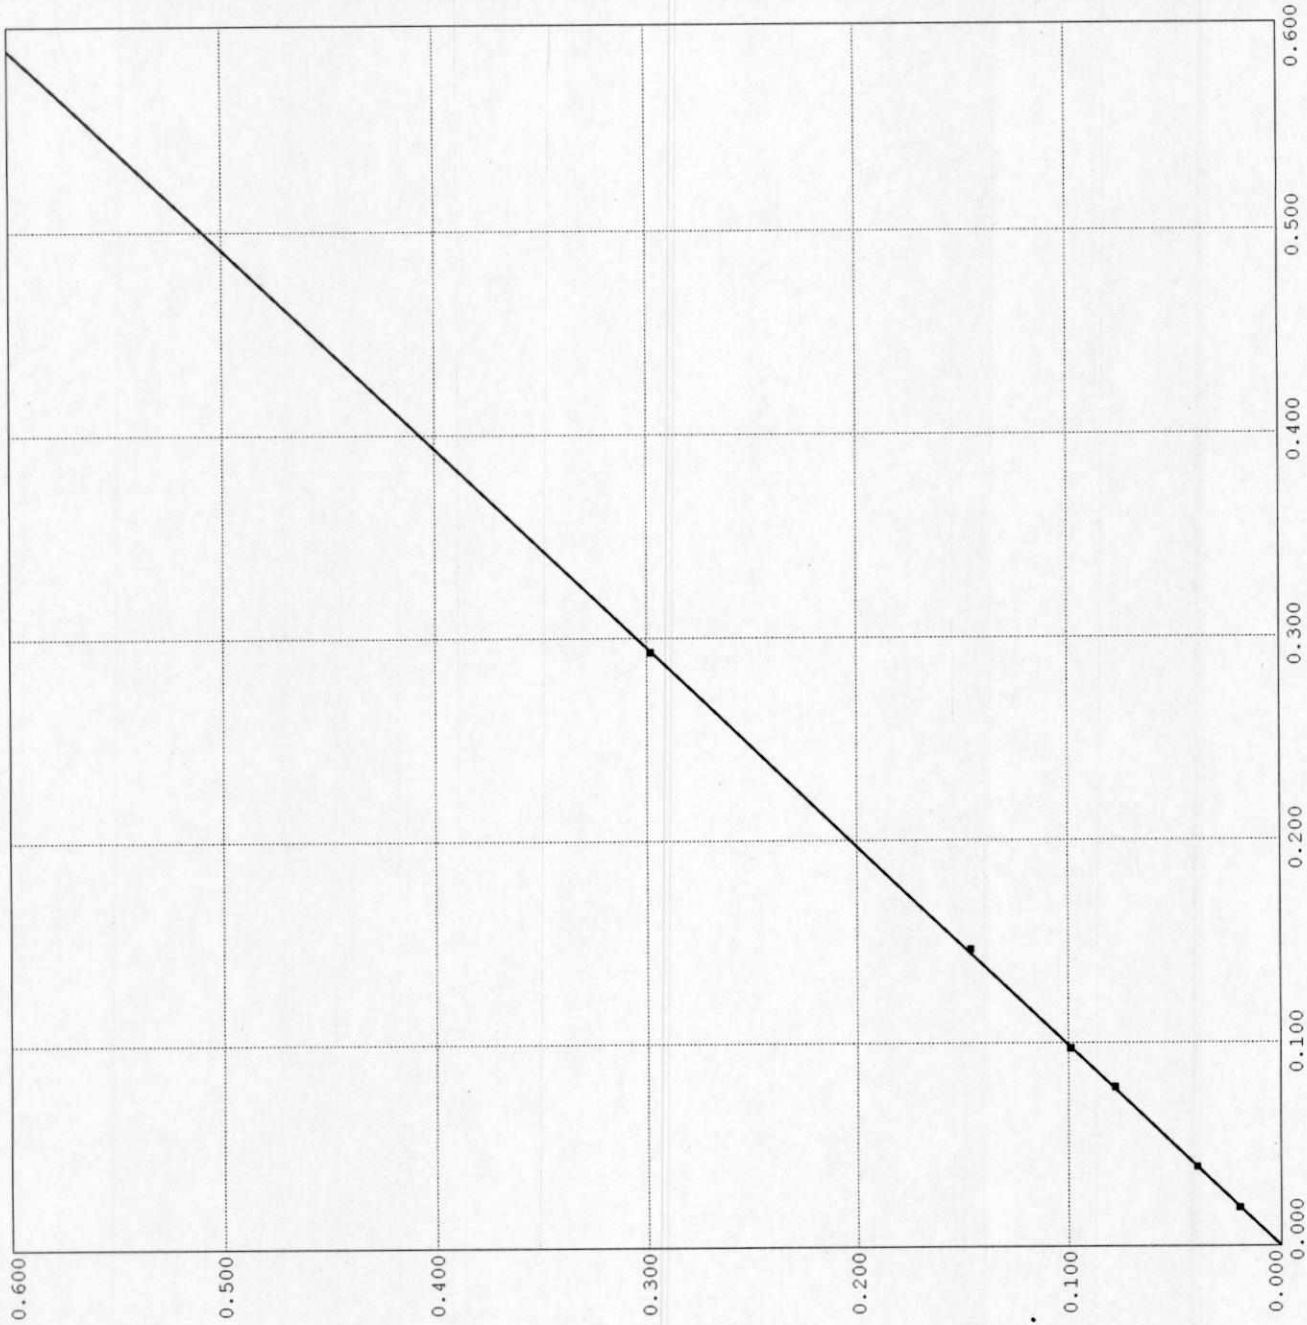

CVG

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100678






Date: 02/23/2024
Time: 09:45:07

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.17: 0.019
LOT #: AG217902
EXPIRATION: 06/28/2024
TANK PRESSURE: 508 psi

BLANK TEST	0.000	09:46
INTERNAL STANDARD	VERIFIED	09:46
EXTERNAL STANDARD	0.020	09:46
BLANK TEST	0.000	09:47
EXTERNAL STANDARD	0.020	09:47
BLANK TEST	0.000	09:48
EXTERNAL STANDARD	0.021	09:48
BLANK TEST	0.000	09:49
EXTERNAL STANDARD	0.020	09:50
BLANK TEST	0.000	09:50
EXTERNAL STANDARD	0.020	09:51
BLANK TEST	0.000	09:52

Average = 0.0202
Std Dev = 0.0004

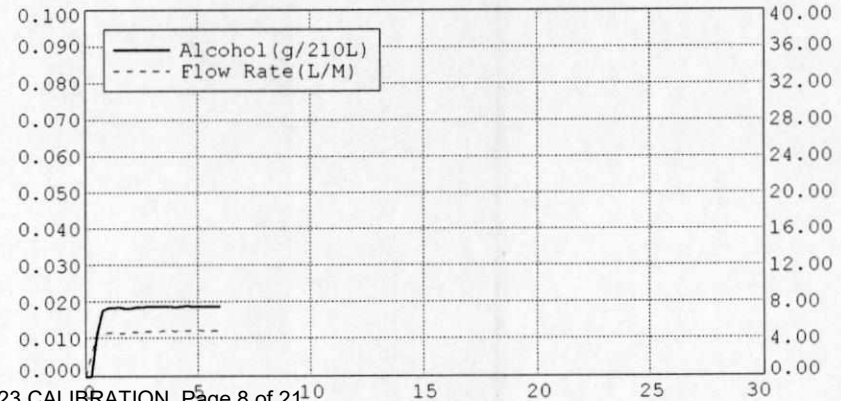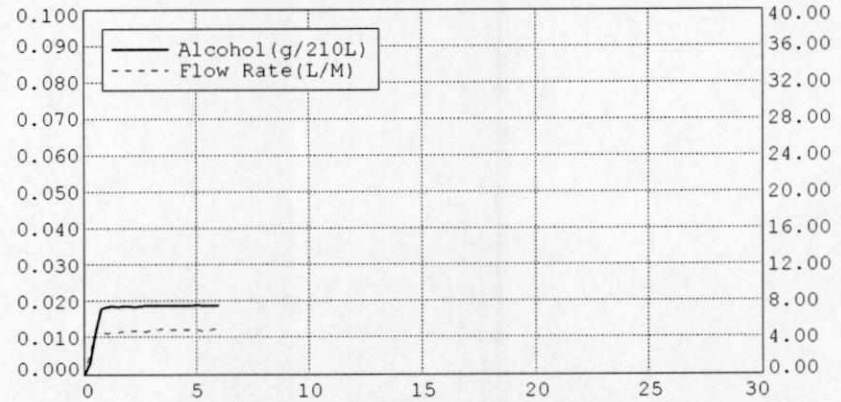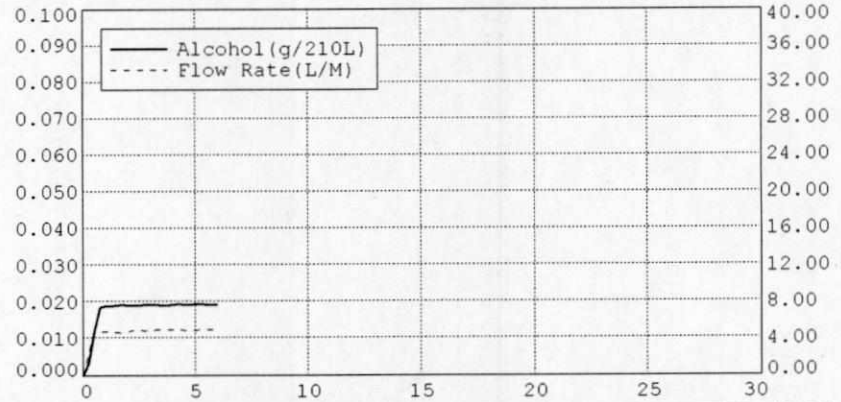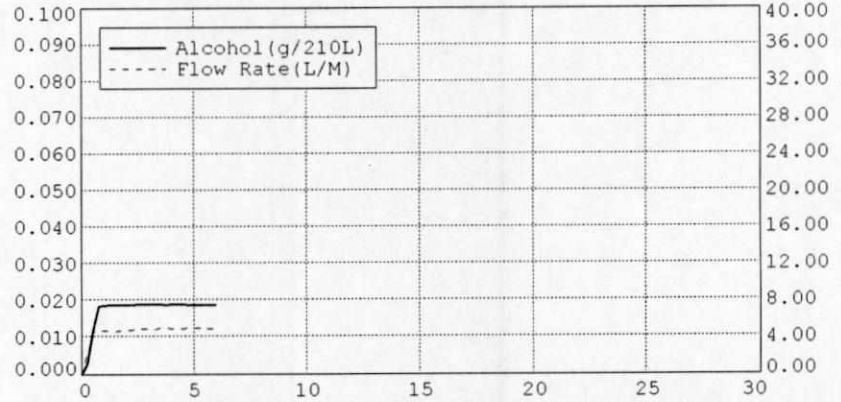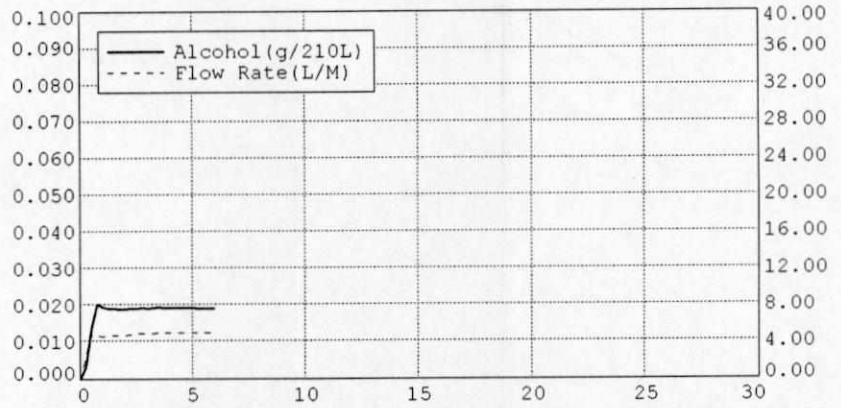

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100678






Date: 02/23/2024
 Time: 09:53:08

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 29.16: 0.039
 LOT #: AG217904
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 679 psi

BLANK TEST	0.000	09:54
INTERNAL STANDARD	VERIFIED	09:54
EXTERNAL STANDARD	0.041	09:54
BLANK TEST	0.000	09:55
EXTERNAL STANDARD	0.040	09:55
BLANK TEST	0.000	09:56
EXTERNAL STANDARD	0.040	09:57
BLANK TEST	0.000	09:57
EXTERNAL STANDARD	0.040	09:58
BLANK TEST	0.000	09:59
EXTERNAL STANDARD	0.040	09:59
BLANK TEST	0.000	10:00

Average = 0.0402
 Std Dev = 0.0004

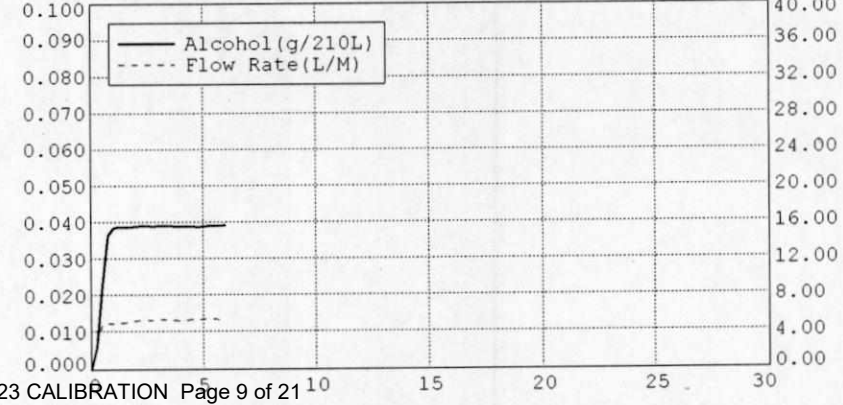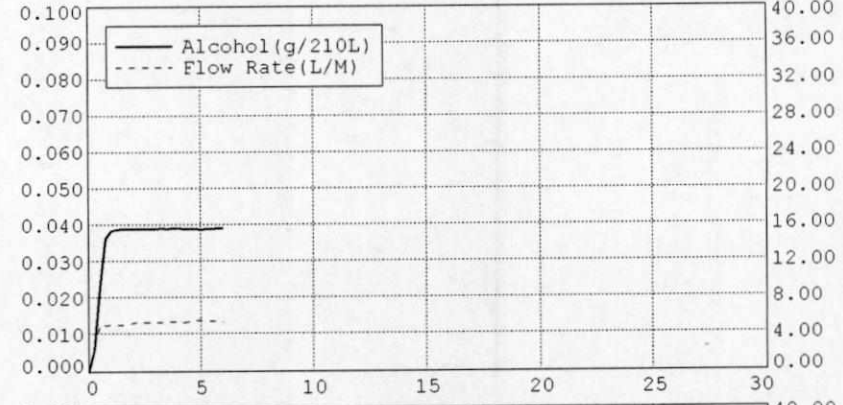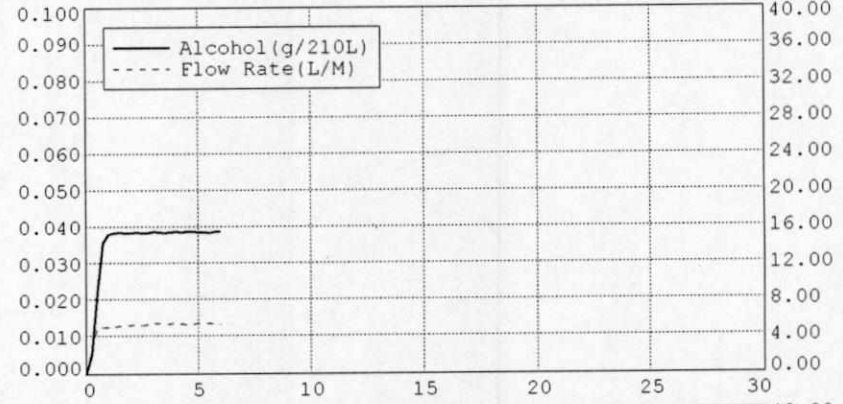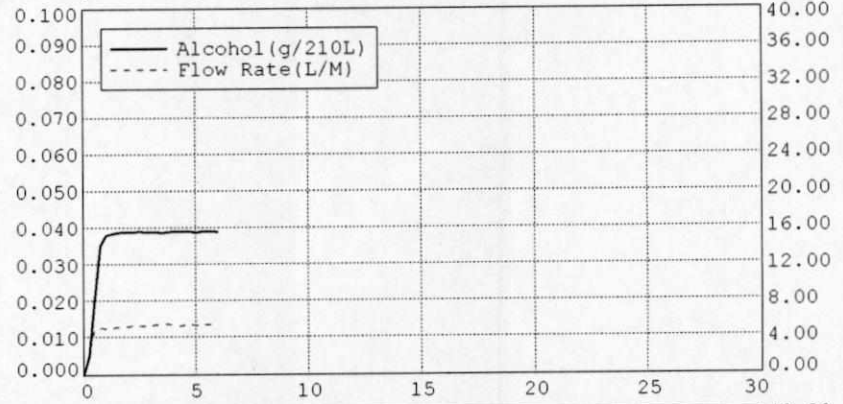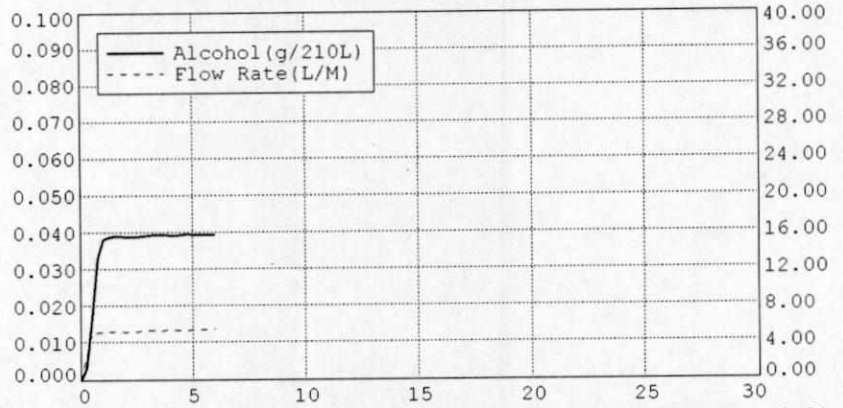

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100678






Date: 02/23/2024
 Time: 10:01:24

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.17: 0.078
 LOT #: AG310901
 EXPIRATION: 04/19/2025
 TANK PRESSURE: 275 psi

BLANK TEST	0.000	10:02
INTERNAL STANDARD	VERIFIED	10:02
EXTERNAL STANDARD	0.079	10:03
BLANK TEST	0.000	10:03
EXTERNAL STANDARD	0.079	10:04
BLANK TEST	0.000	10:05
EXTERNAL STANDARD	0.079	10:05
BLANK TEST	0.000	10:06
EXTERNAL STANDARD	0.079	10:06
BLANK TEST	0.000	10:07
EXTERNAL STANDARD	0.079	10:07
BLANK TEST	0.000	10:08

Average = 0.0790
 Std Dev = 0.0000

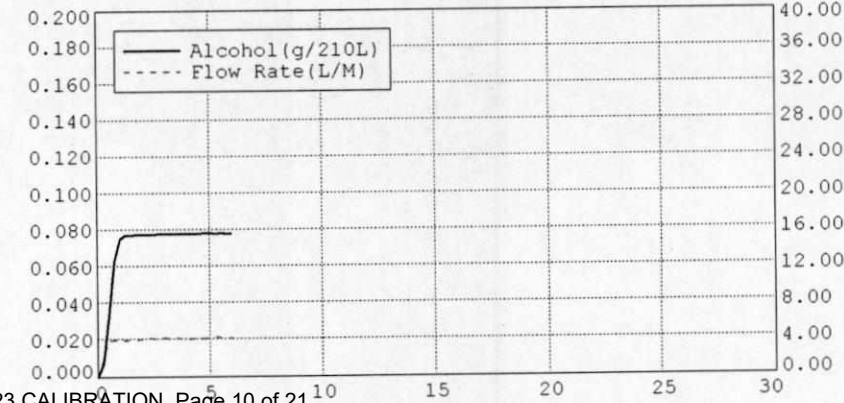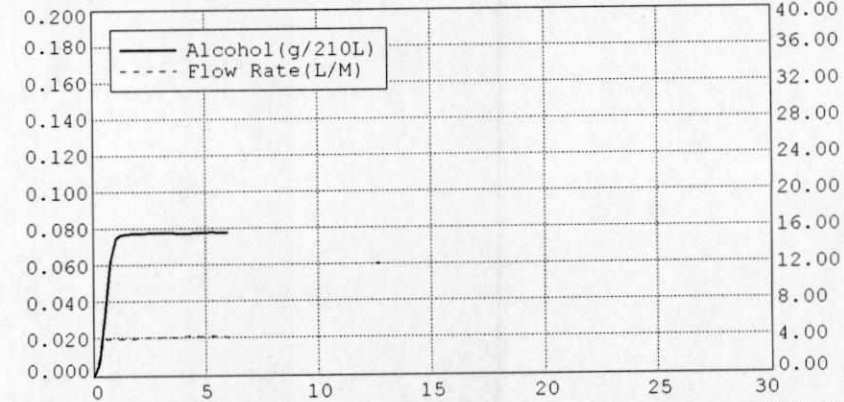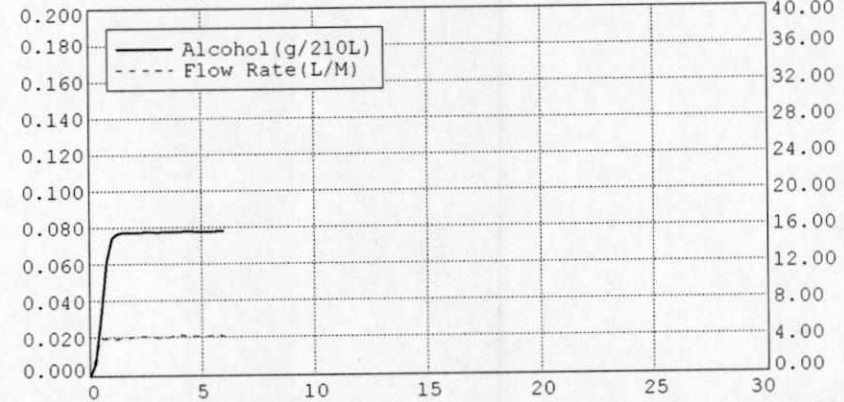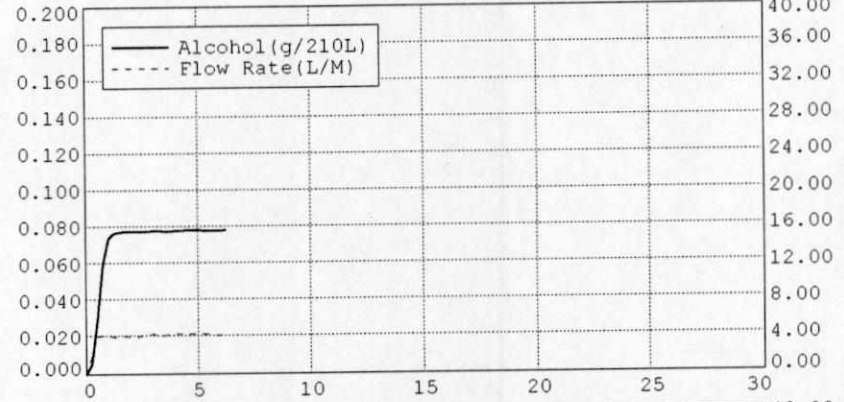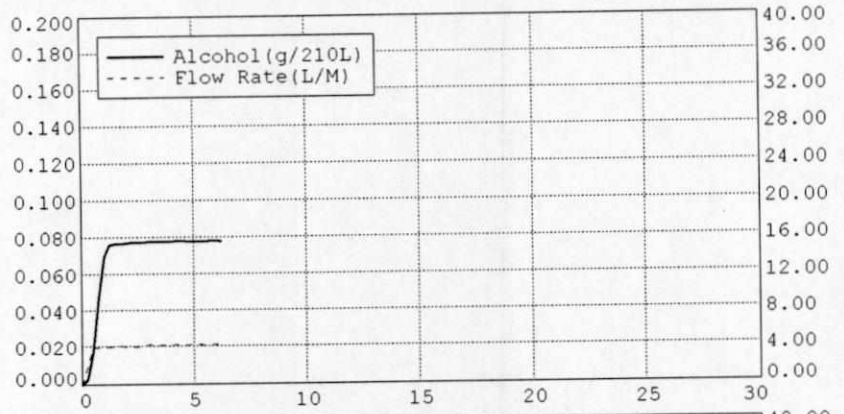

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100678






Date: 02/23/2024
 Time: 10:09:01

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.16: 0.097
 LOT #: AG333401
 EXPIRATION: 11/30/2025
 TANK PRESSURE: 1077 psi

BLANK TEST	0.000	10:10
INTERNAL STANDARD	VERIFIED	10:10
EXTERNAL STANDARD	0.100	10:10
BLANK TEST	0.000	10:11
EXTERNAL STANDARD	0.100	10:11
BLANK TEST	0.000	10:12
EXTERNAL STANDARD	0.100	10:12
BLANK TEST	0.000	10:13
EXTERNAL STANDARD	0.100	10:14
BLANK TEST	0.000	10:14
EXTERNAL STANDARD	0.100	10:15
BLANK TEST	0.000	10:16

Average = 0.1000
 Std Dev = 0.0000

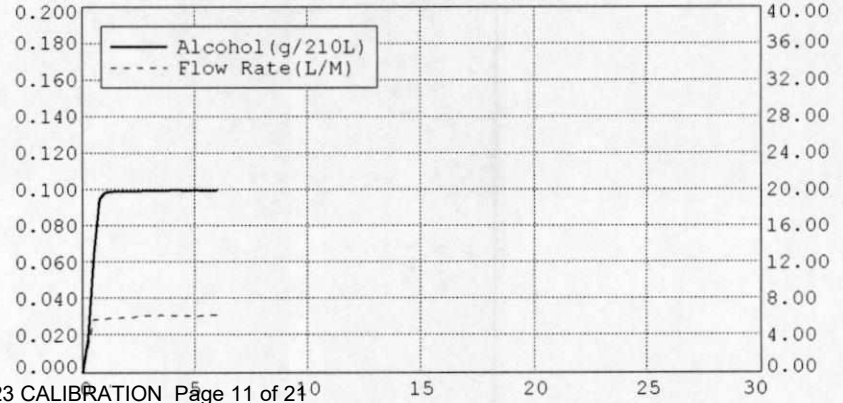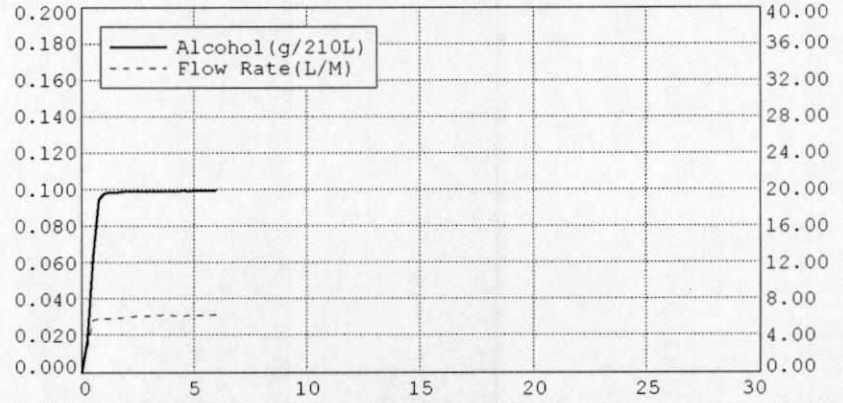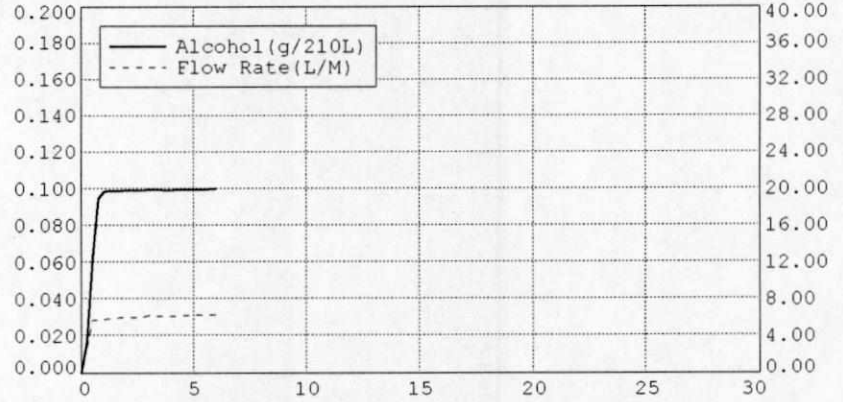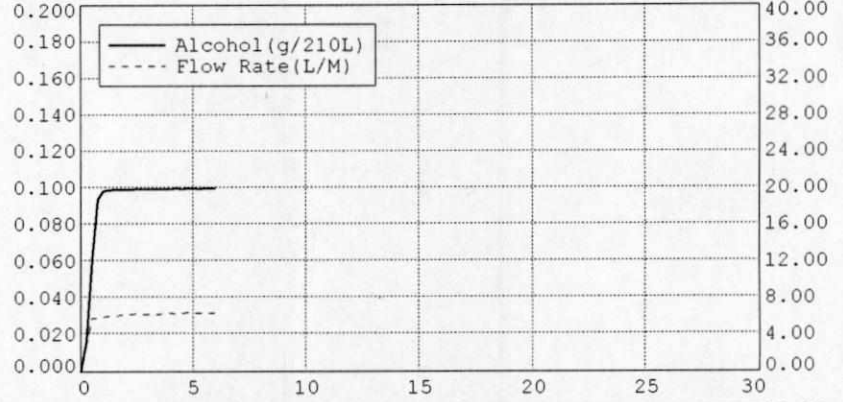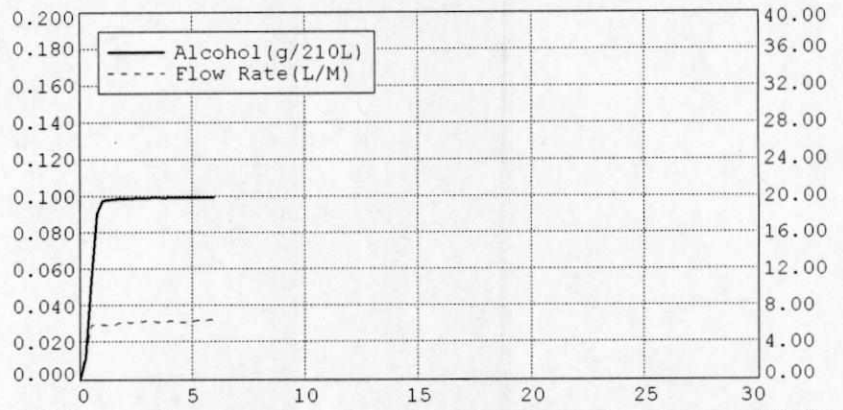

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100678






Date: 02/23/2024
 Time: 10:16:48

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 29.17: 0.146
 LOT #: AG332004
 EXPIRATION: 11/16/2025
 TANK PRESSURE: 688 psi

BLANK TEST	0.000	10:21
INTERNAL STANDARD	VERIFIED	10:21
EXTERNAL STANDARD	0.147	10:21
BLANK TEST	0.000	10:22
EXTERNAL STANDARD	0.147	10:22
BLANK TEST	0.000	10:23
EXTERNAL STANDARD	0.147	10:23
BLANK TEST	0.000	10:24
EXTERNAL STANDARD	0.147	10:24
BLANK TEST	0.000	10:25
EXTERNAL STANDARD	0.147	10:25
BLANK TEST	0.000	10:26

Average = 0.1470
 Std Dev = 0.0000

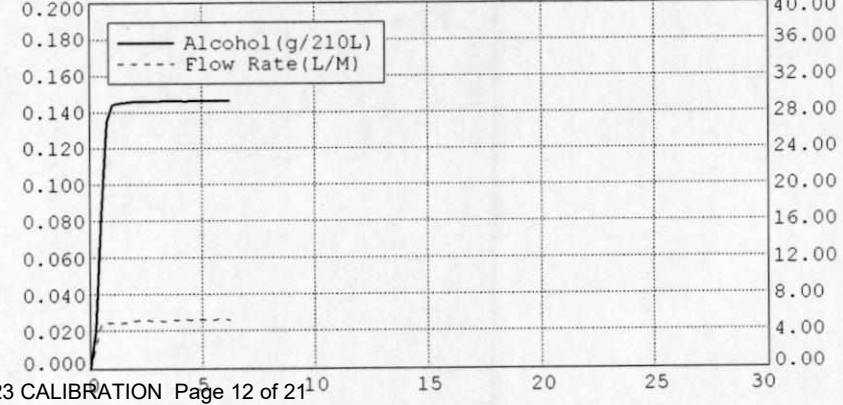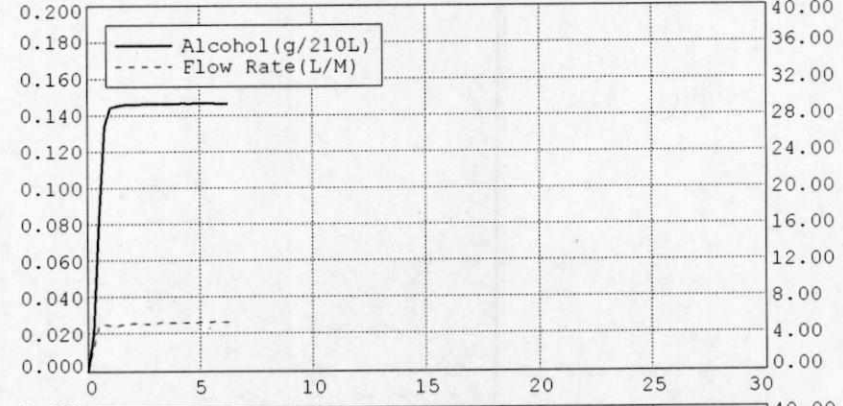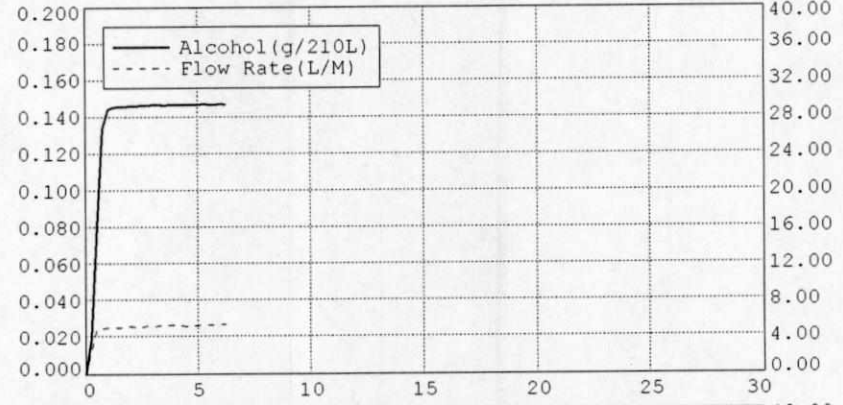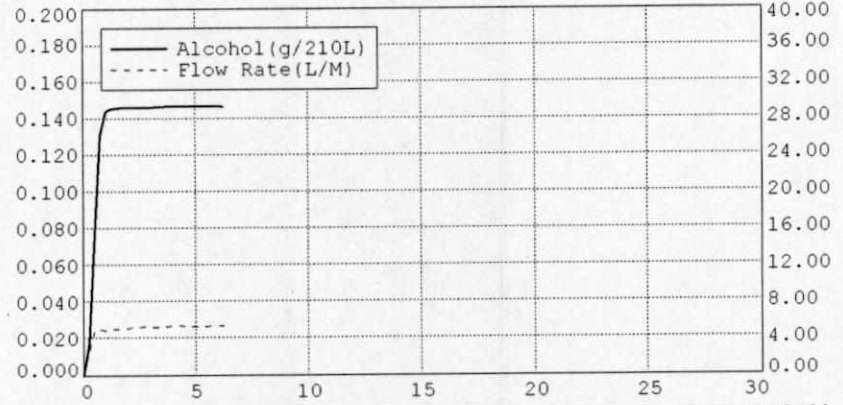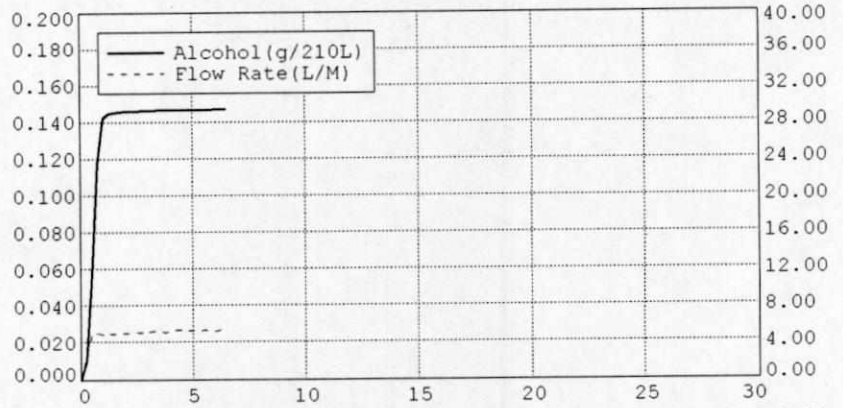

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100678






Date: 02/23/2024
Time: 10:28:52

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.16: 0.292
LOT #: AG327804
EXPIRATION: 10/05/2025
TANK PRESSURE: 172 psi

BLANK TEST	0.000	10:30
INTERNAL STANDARD	VERIFIED	10:30
EXTERNAL STANDARD	0.299	10:30
BLANK TEST	0.000	10:31
EXTERNAL STANDARD	0.299	10:31
BLANK TEST	0.000	10:32
EXTERNAL STANDARD	0.299	10:32
BLANK TEST	0.000	10:33
EXTERNAL STANDARD	0.298	10:34
BLANK TEST	0.000	10:34
EXTERNAL STANDARD	0.299	10:35
BLANK TEST	0.000	10:36

Average = 0.2988
Std Dev = 0.0004

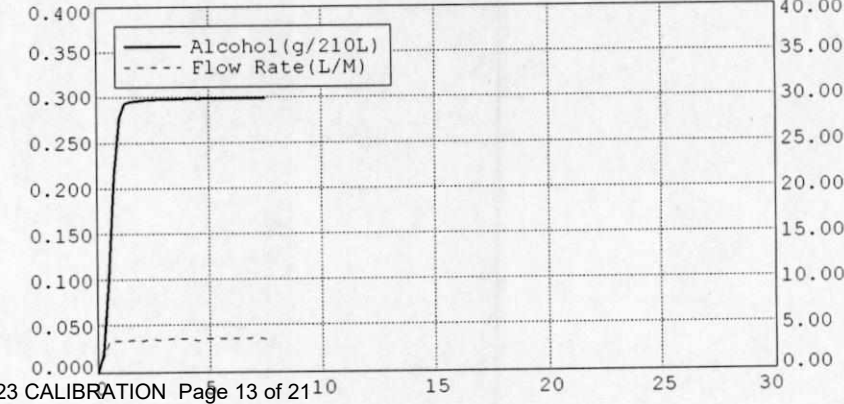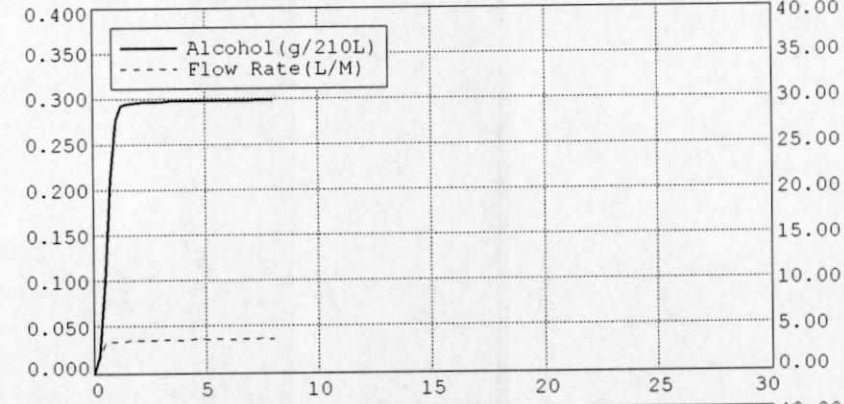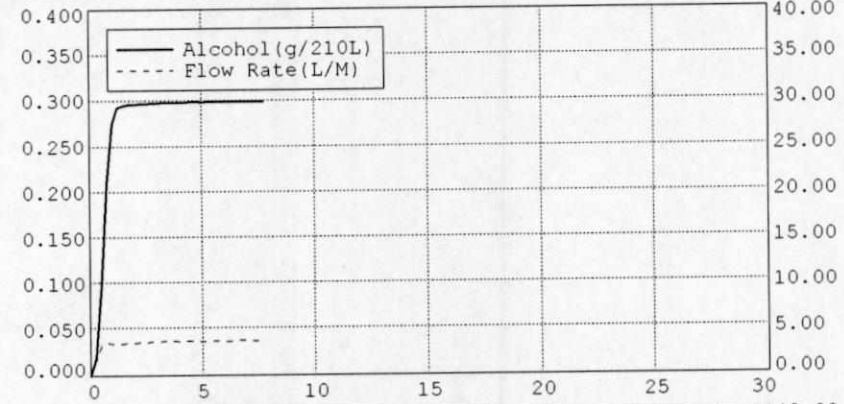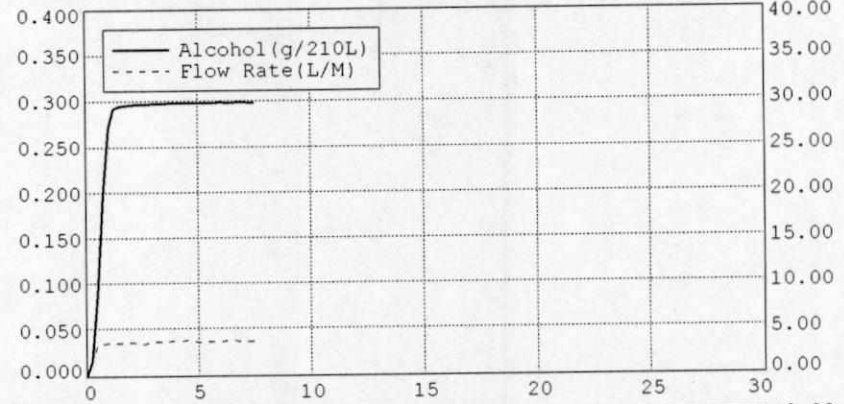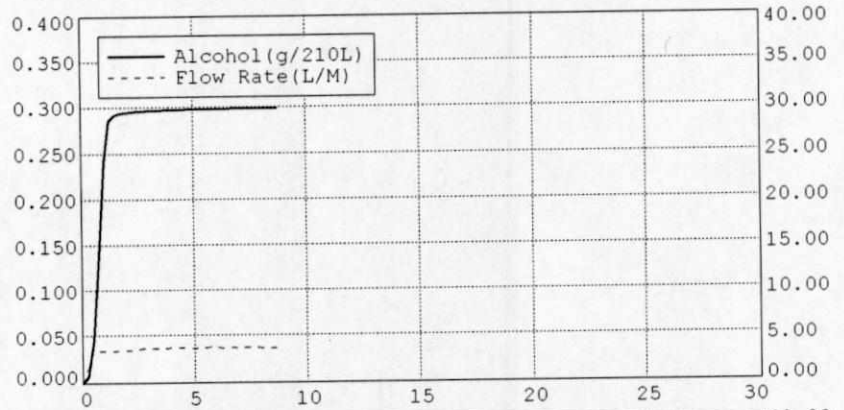

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100678

Date: 02/23/2024
Time: 10:48:01

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 10:49
BLANK TEST 0.000 10:49
INTERNAL STANDARD VERIFIED 10:49
EXTERNAL STANDARD 0.079 10:49
BLANK TEST 0.000 10:50
SUBJECT SAMPLE INCOMPLETE 10:52

Handwritten signature



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100678

Date: 02/23/2024
Time: 10:54:50

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 10:55
BLANK TEST 0.000 10:55
INTERNAL STANDARD VERIFIED 10:56
EXTERNAL STANDARD 0.079 10:56
BLANK TEST 0.000 10:57
SUBJECT SAMPLE XXX 10:57

Maximum Attempts Exceeded

OKG



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100678

Date: 02/23/2024
Time: 11:00:16

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INVALID
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 11:04
BLANK TEST 0.000 11:04
INTERNAL STANDARD VERIFIED 11:04
EXTERNAL STANDARD 0.079 11:05
BLANK TEST 0.000 11:05
SUBJECT SAMPLE INVALID 11:06

OKG

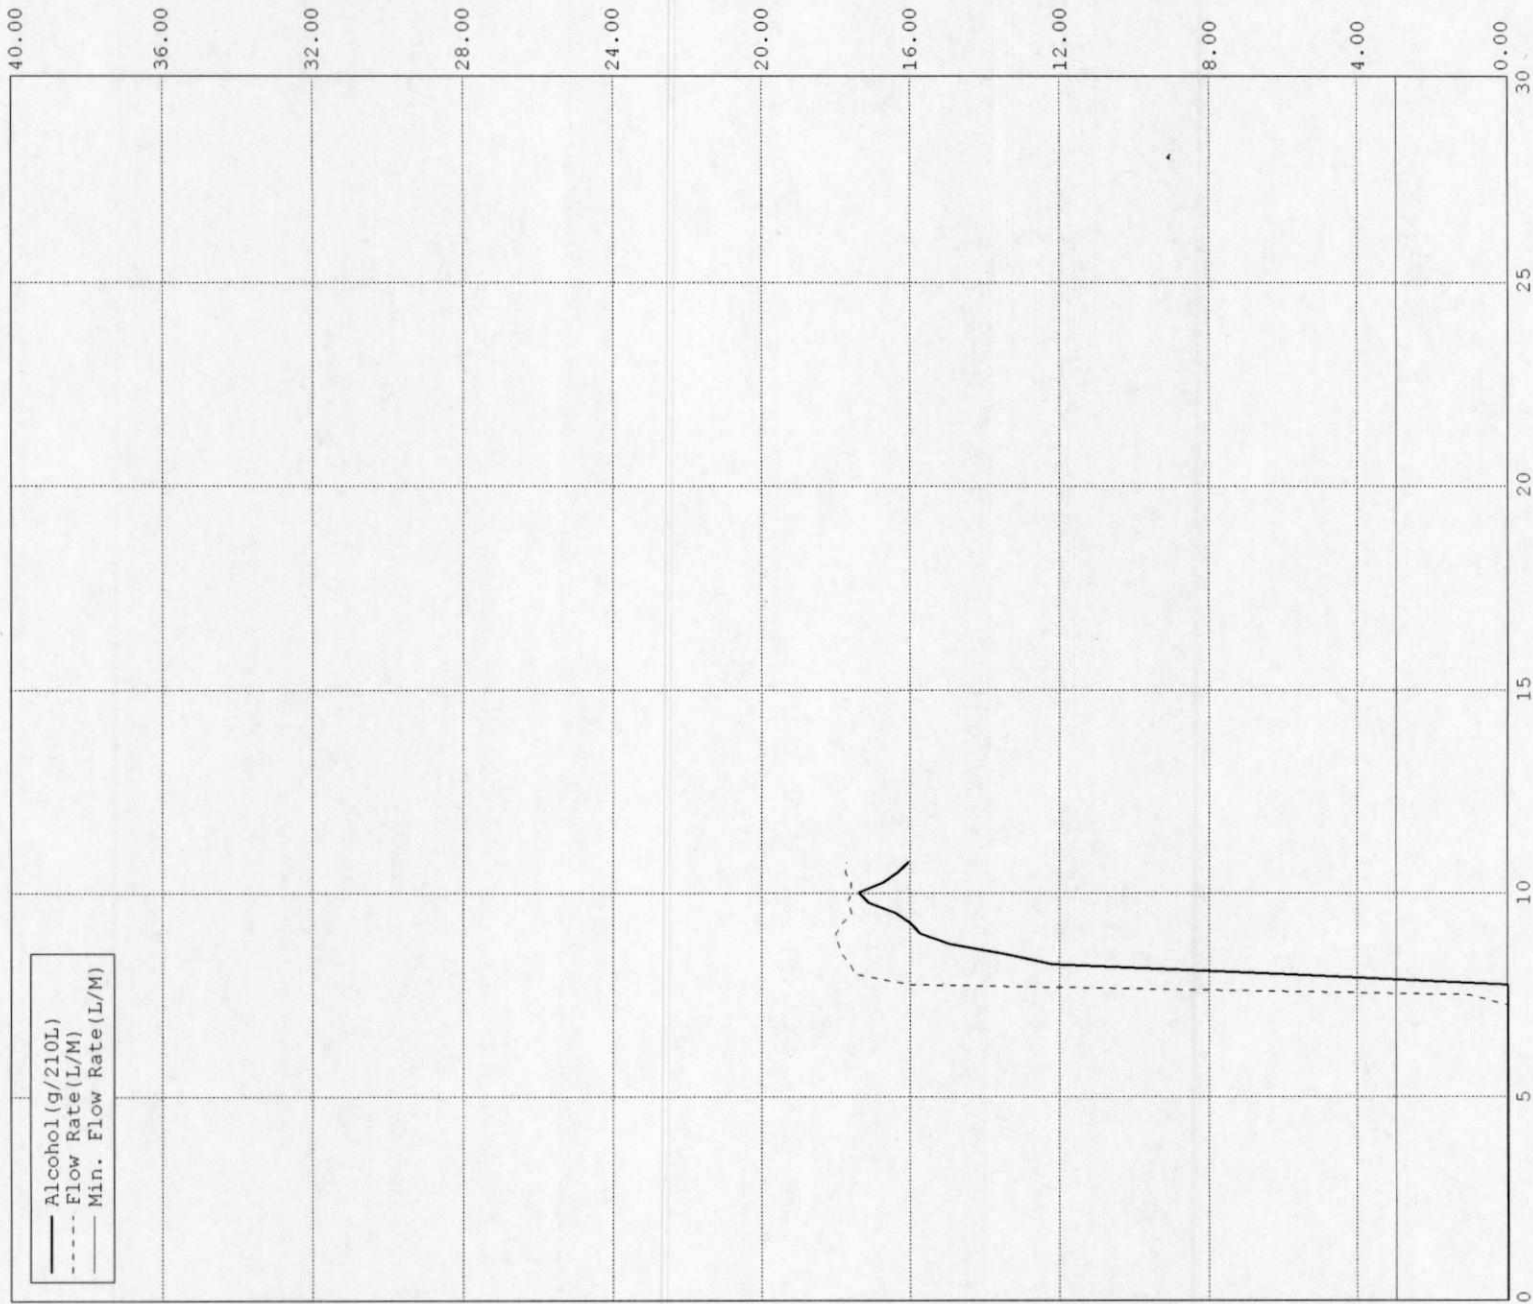

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100678

Date: 02/23/2024
Time: 11:08:57

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
RFI
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 11:10
BLANK TEST 0.000 11:10
INTERNAL STANDARD VERIFIED 11:10
EXTERNAL STANDARD 0.079 11:10
BLANK TEST 0.000 11:11

RFI DETECTED



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100678

Date: 02/23/2024
Time: 12:29:09

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE ACETONE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION


NOMINAL: 0.080
TARGET AT 29.18: 0.078
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	12:30
BLANK TEST	0.000	12:30
INTERNAL STANDARD	VERIFIED	12:30
Xq = 0.081 (0.98%)		
EXTERNAL STANDARD	0.079	12:30
X[1] = 0.0790 (-0.0010) (0.0007)		
BLANK TEST	0.000	12:31
SUBJECT SAMPLE	XXX	12:32
X[1] = 0.1101 (-0.0155) (0.0029)		

Interference Detected

Filter 2 Average: -0.0007
Filter 3 Average: 0.0014

CUG

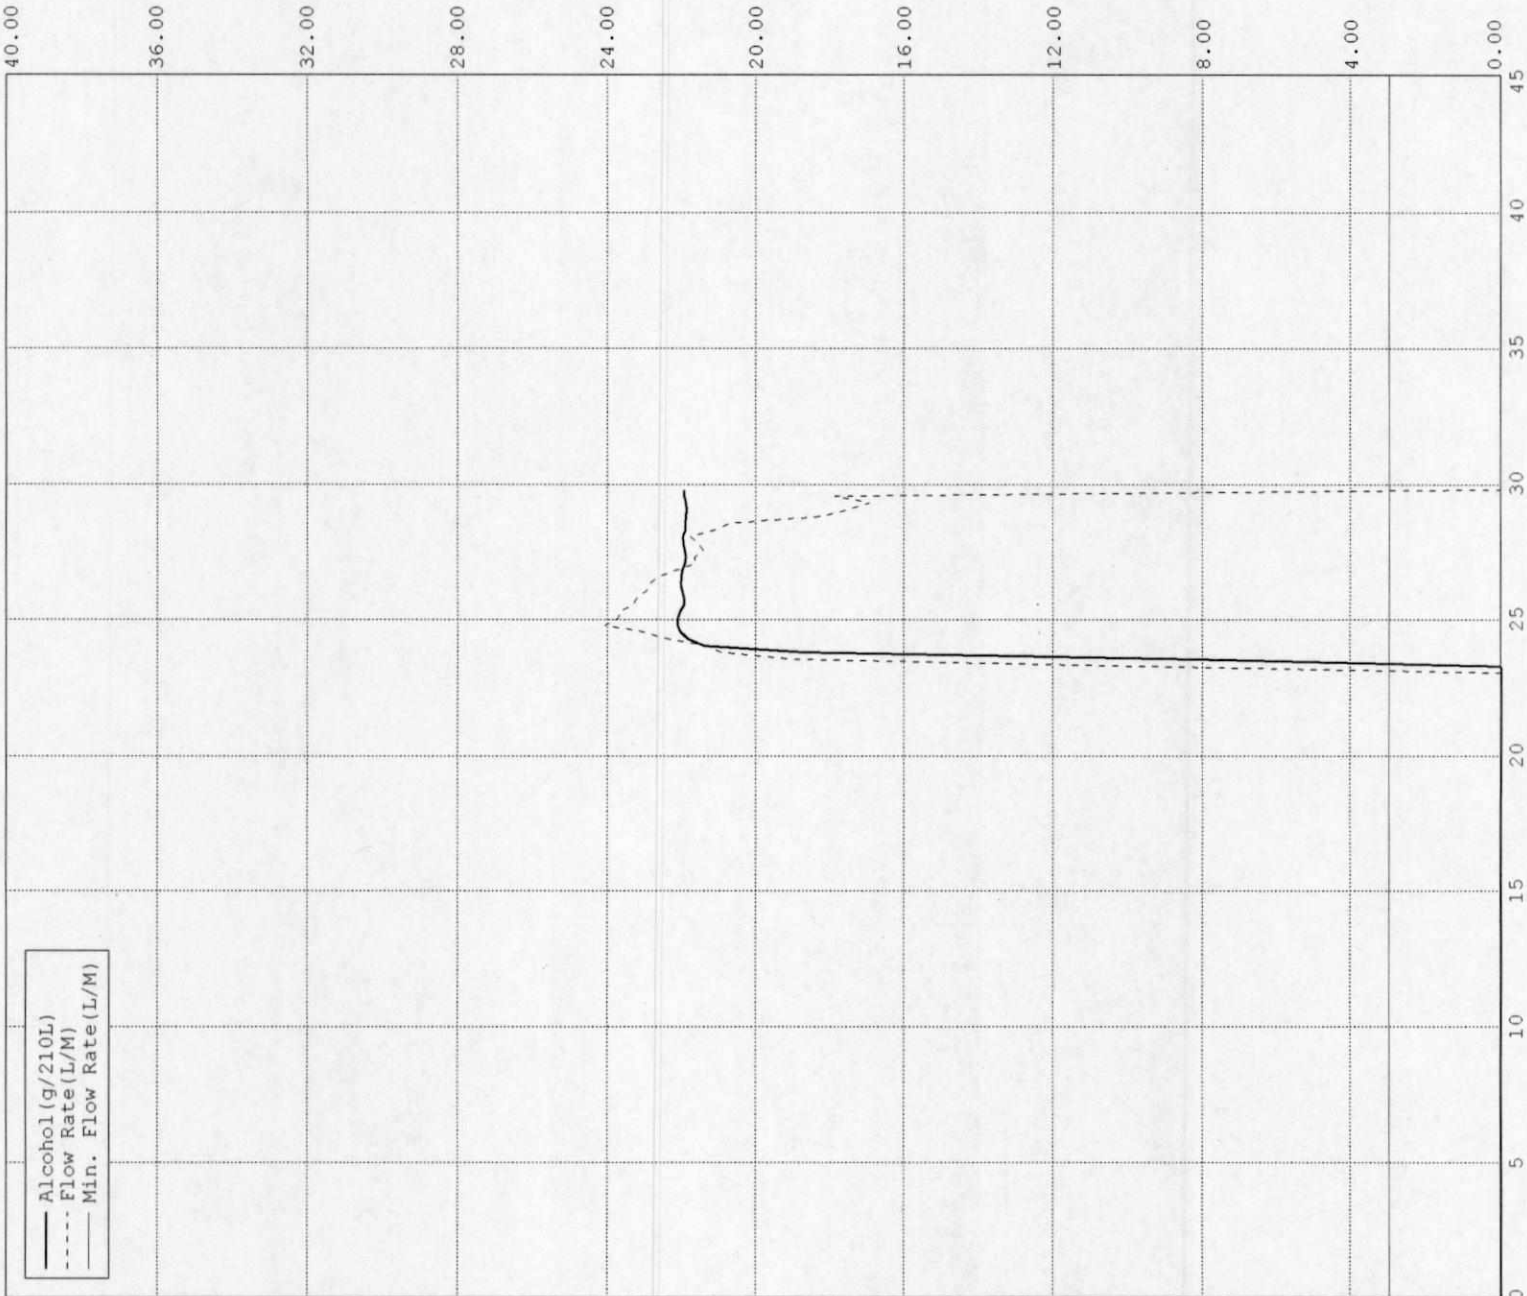

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100678

Date: 02/23/2024
Time: 12:36:39

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE IPA
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.19: 0.078
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	12:37
BLANK TEST	0.000	12:37
INTERNAL STANDARD	VERIFIED	12:37
Xq = 0.080 (0.44%)		
EXTERNAL STANDARD	0.079	12:38
X[1] = 0.0793 (-0.0003)	(0.0008)	
BLANK TEST	0.000	12:39
SUBJECT SAMPLE	XXX	12:39
X[1] = 0.1182 (-0.0184)	(0.0020)	

Interference Detected

OK



SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100678

Date: 02/23/2024
 Time: 12:17:09

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXXX


OPERATOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

DEPT/AGENCY:
 INTERFERENCE NEGATIVE
 CASE/REPORT: XXXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.19: 0.078
 LOT #: AG310901
 EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	12:19
BLANK TEST	0.000	12:19
INTERNAL STANDARD	VERIFIED	12:19
Xq = 0.080 (0.00%)		
EXTERNAL STANDARD	0.079	12:19
X[1] = 0.0788 (-0.0011)	(0.0012)	
BLANK TEST	0.000	12:20
SUBJECT SAMPLE (Vol=2.24L)	0.095	12:21
X[1] = 0.0956 (-0.0001)	(0.0003)	
BLANK TEST	0.000	12:22
EXTERNAL STANDARD	0.078	12:22
X[1] = 0.0785 (-0.0002)	(0.0028)	
BLANK TEST	0.000	12:23

CVB

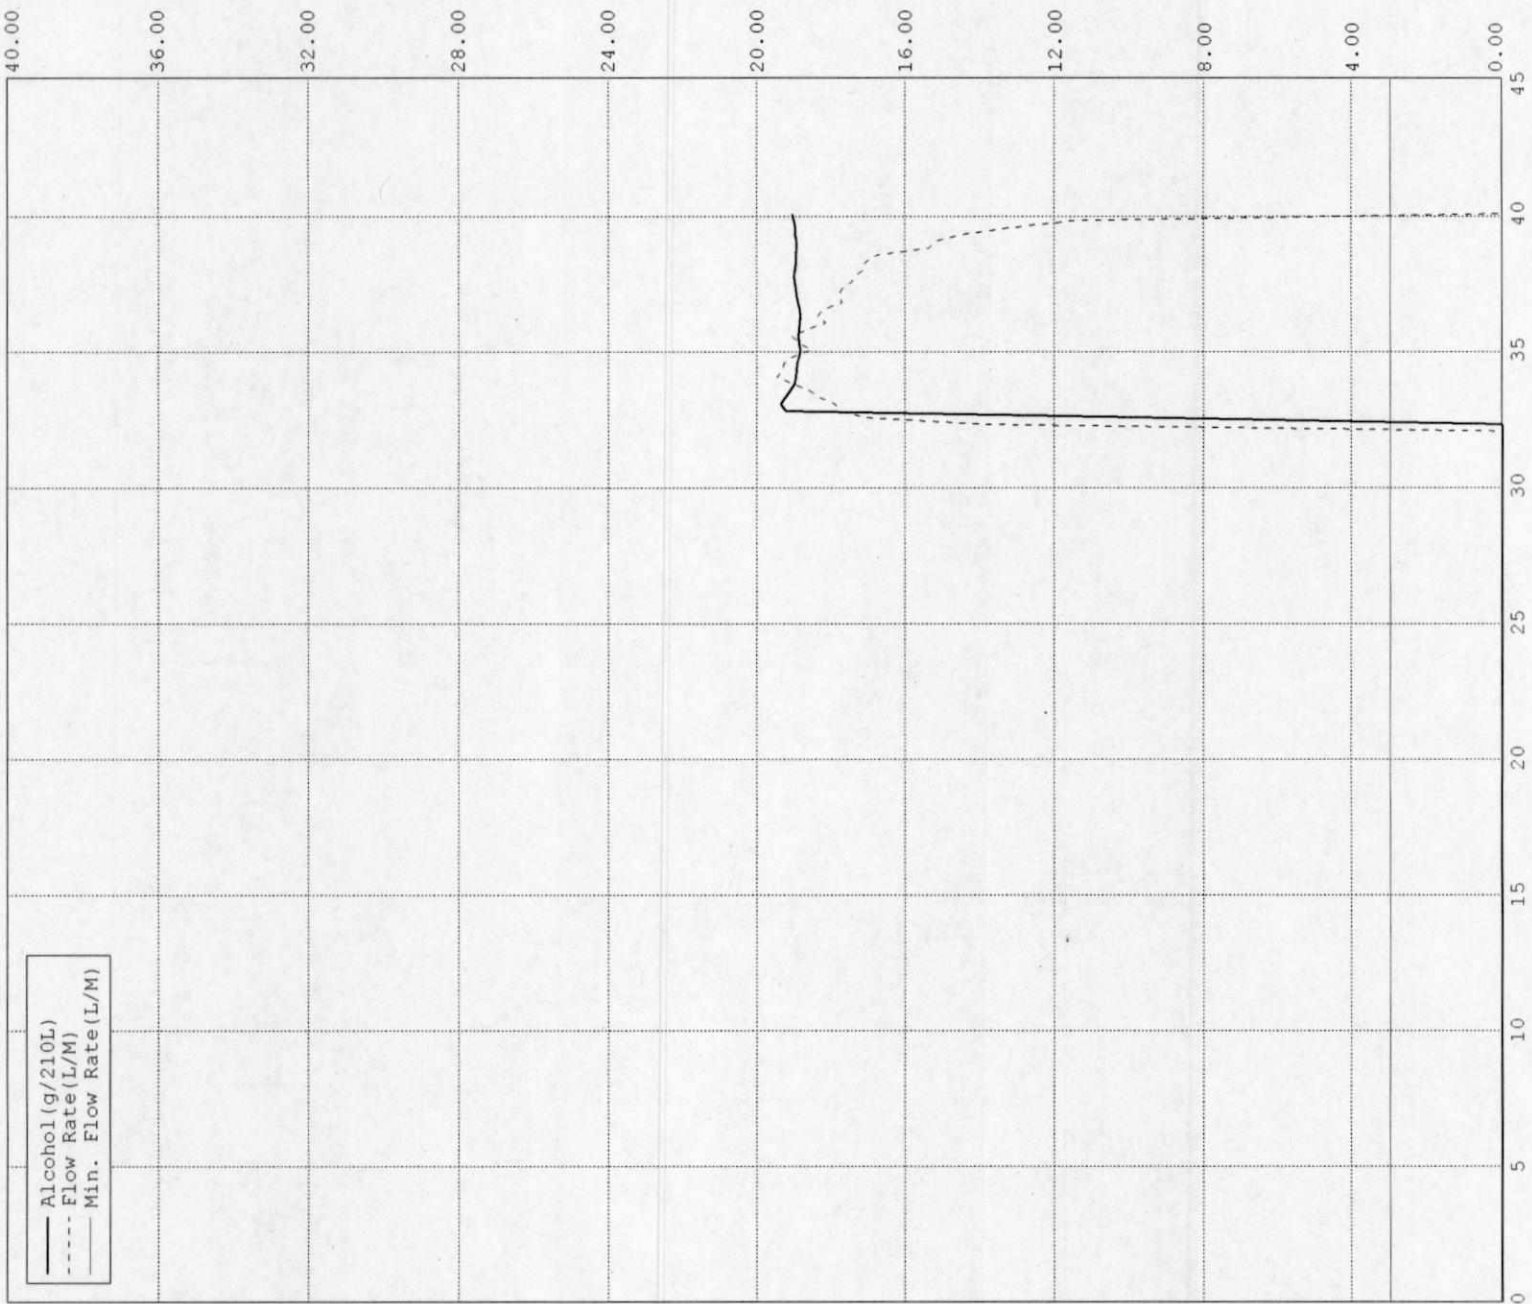

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100678

Date: 02/23/2024
Time: 13:02:41

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	13:04
BLANK TEST	0.000	13:04
INTERNAL STANDARD	VERIFIED	13:04
EXTERNAL STANDARD	0.079	13:04
BLANK TEST	0.000	13:05
SUBJECT SAMPLE (Vol=2.39L)	0.000	13:05
BLANK TEST	0.000	13:06
EXTERNAL STANDARD	0.079	13:07
BLANK TEST	0.000	13:07

CKG

