



Airgas USA LLC (LAB)
 3500 Bernard Street
 St. Louis, Mo. 63103
 Ph: (314) 533-3100
 Fax: (314) 533-7328

Certificate of Analysis

Customer Name
Exclusive Supplier
 Intoximeters, Inc.
 2081 Craig Road
 St. Louis, Mo 63146

Test Date: 19-Dec-2023

Lot # AG335202 **Model** 108


Exp Date 18-Dec-2025	Cyl. Type 108	Component Ethanol Nitrogen	Certified Concentration 0.080 ± 0.002 BrAC (208 ppm)
--------------------------------	-------------------------	---	--

Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:

RGM Serial No.	Concentration	RGM Serial No.	Concentration
EB0010581	391.8 ppm	EB0010603	392.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm	EB0010562	104.2 ppm
EB0010561	103.7 ppm	EB0010579	52.94 ppm
EB0010681	52.22 ppm		

CRM Serial No.	Concentration	CRM Serial No.	Concentration
CC727481	799.4 ppm	CC727493	389.8 ppm
CC727496	253.4 ppm	CC727498	150.2 ppm

Analytical Method: NDIR


 Approved for Release: _____
 Yusef Woods

ISO 17025:2017 A2LA accredited. Certificate Number 3082.06
ISO 17034:2016 A2LA accredited. Certificate Number 3082.07

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100375

Date: 01/17/2024
Time: 12:11:09

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 49.1°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 48.1°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.55 V PASSED
(0.92 V - 2.16 V)
Cooler Voltage = 1.57 V PASSED
(0.92 V - 2.16 V)
Bias Voltage = 80 V PASSED
(47 V - 111 V)
Chopper Freq = 540 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 30.2 in

PUMP INFO

Flow Rate = 4.027 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.092 0.67% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100375

Date: 01/17/2024
Time: 12:13 PM

Temperatures (°C)

Sample Cell: 48.7°C
Breath Tube: 48.1°C

Current Barometer 30.2 in
Volume (Ltr) 0.00

Settings

Lamp: 1.54 V
Bias: 80 V
Cooler: 1.57 V
Chopper: 539 Hz

Voltages (V)

Flow: 1.05 V
Detector: -0.008 V

LINEARITY CHECK


Alaska Department of Public Safety
DATA MASTER dmt: 100375

Date: 01/17/2024
Time: 12:20:39

SUPERVISOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0210	0.0000
0.081	0.0818	0.0004
0.303	0.3020	0.0000

SLOPE = 0.992653
R² = 0.999999

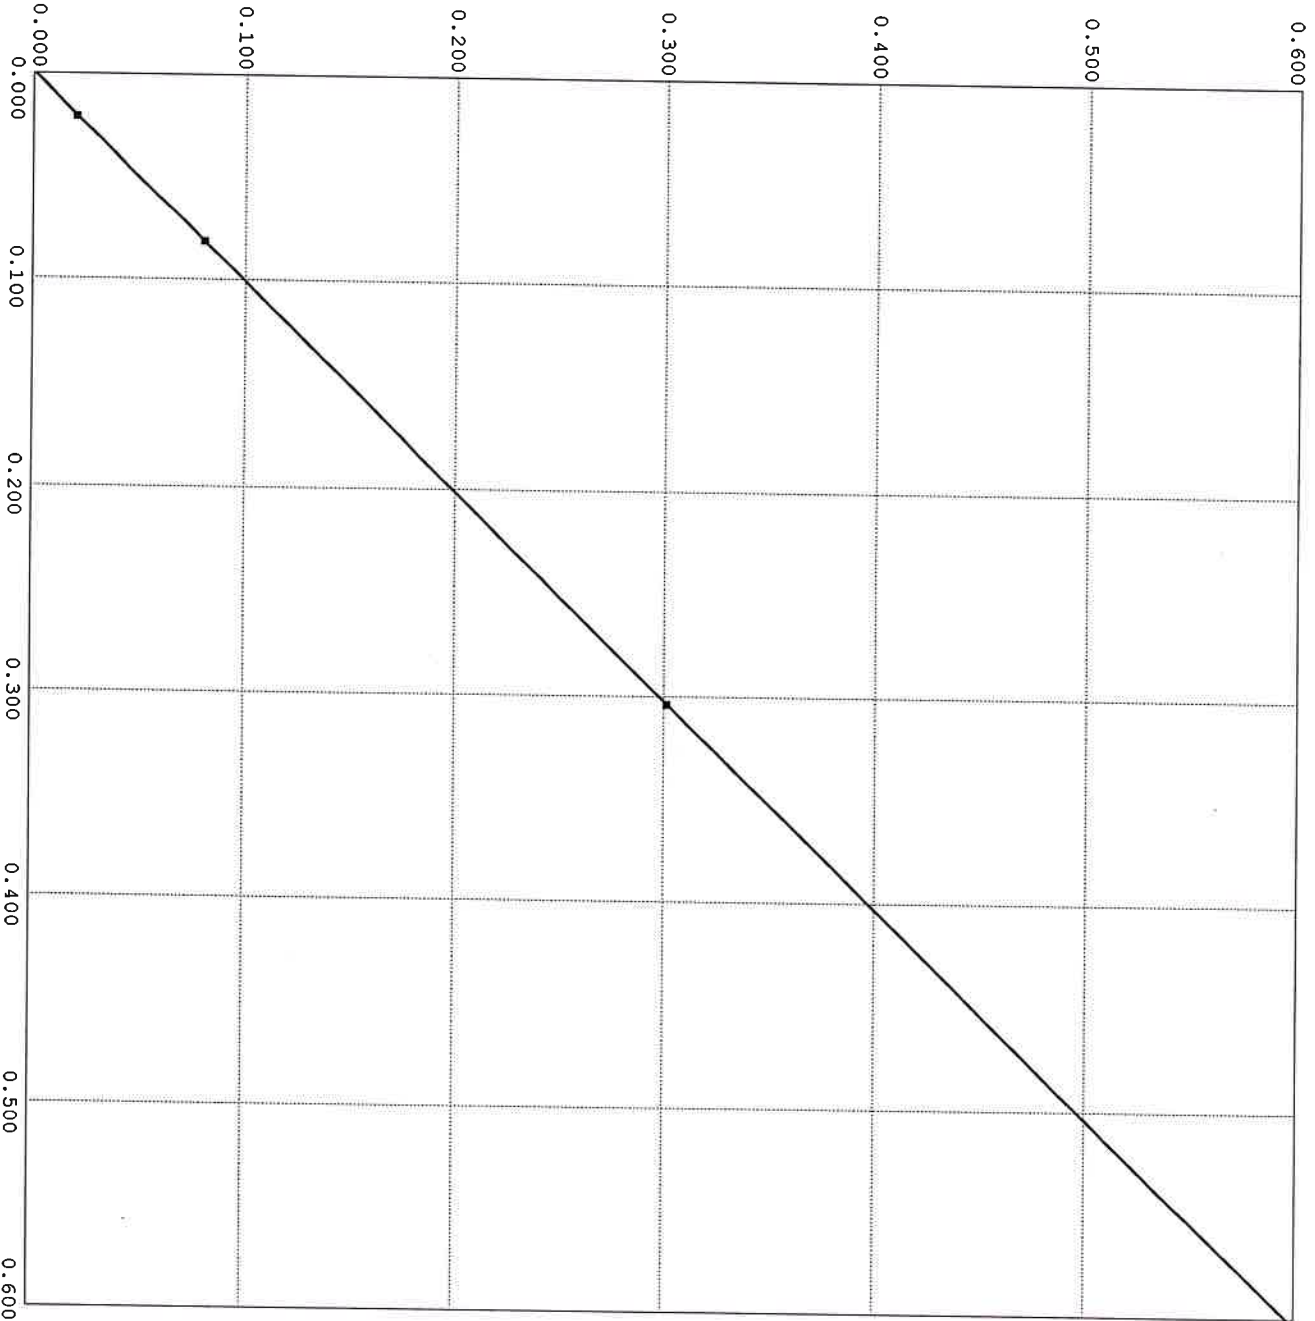

CBS

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100375






Date: 01/17/2024
Time: 12:20:41

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 30.24: 0.020
LOT #: AG217902
EXPIRATION: 06/28/2024
TANK PRESSURE: 437 psi

BLANK TEST	0.000	12:22
INTERNAL STANDARD	VERIFIED	12:22
EXTERNAL STANDARD	0.021	12:22
BLANK TEST	0.000	12:23
EXTERNAL STANDARD	0.021	12:23
BLANK TEST	0.000	12:24
EXTERNAL STANDARD	0.021	12:24
BLANK TEST	0.000	12:25
EXTERNAL STANDARD	0.021	12:25
BLANK TEST	0.000	12:26
EXTERNAL STANDARD	0.021	12:26
BLANK TEST	0.000	12:27

Average = 0.0210
Std Dev = 0.0000

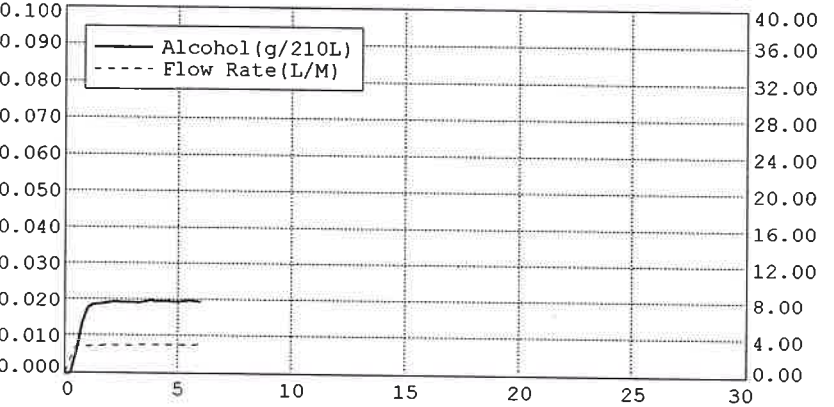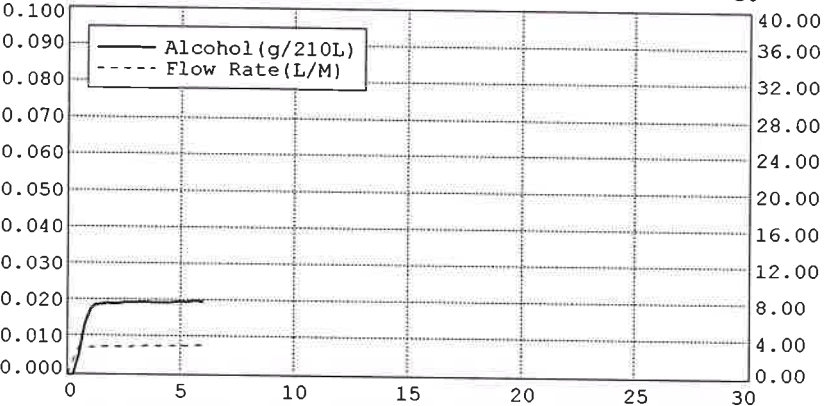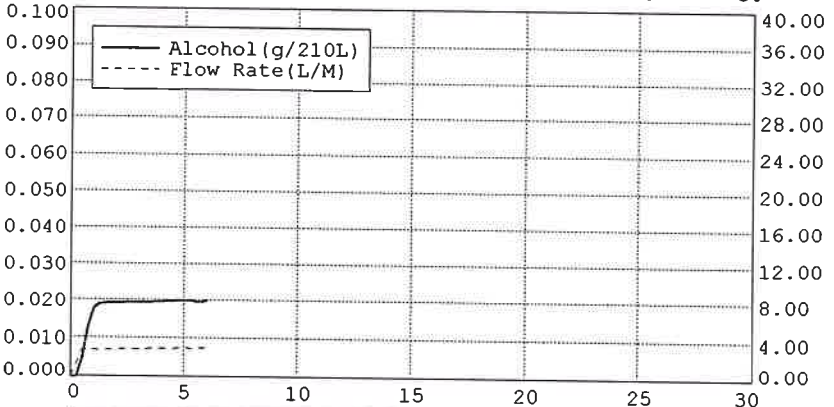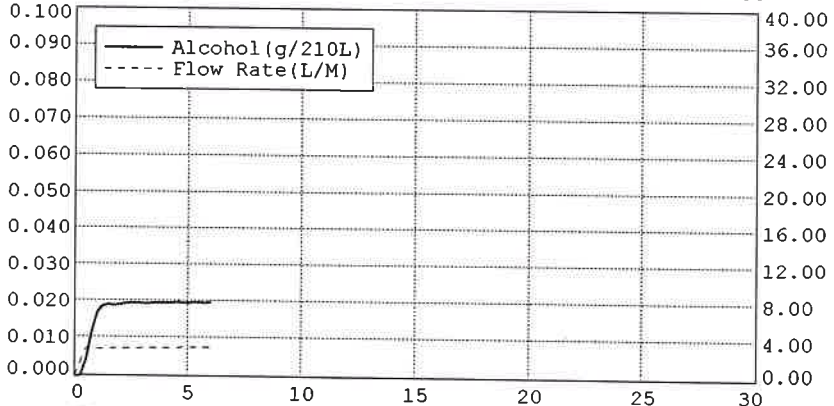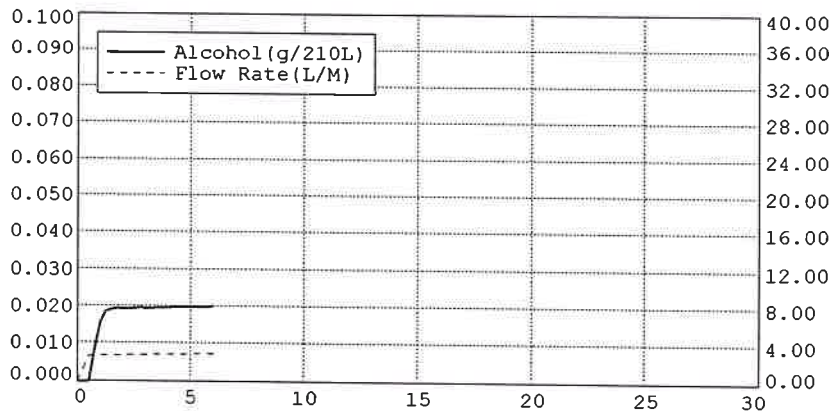

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100375






Date: 01/17/2024
 Time: 12:28:28

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 30.24: 0.081
 LOT #: 09523080A1
 EXPIRATION: 05/05/2025
 TANK PRESSURE: 571 psi

BLANK TEST	0.000	12:29
INTERNAL STANDARD	VERIFIED	12:30
EXTERNAL STANDARD	0.082	12:30
BLANK TEST	0.000	12:31
EXTERNAL STANDARD	0.081	12:31
BLANK TEST	0.000	12:32
EXTERNAL STANDARD	0.082	12:32
BLANK TEST	0.000	12:33
EXTERNAL STANDARD	0.082	12:33
BLANK TEST	0.000	12:34
EXTERNAL STANDARD	0.082	12:34
BLANK TEST	0.000	12:35

Average = 0.0818
 Std Dev = 0.0004

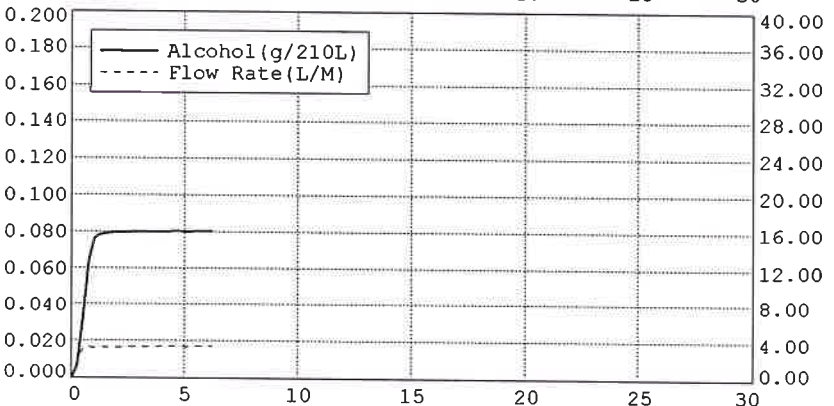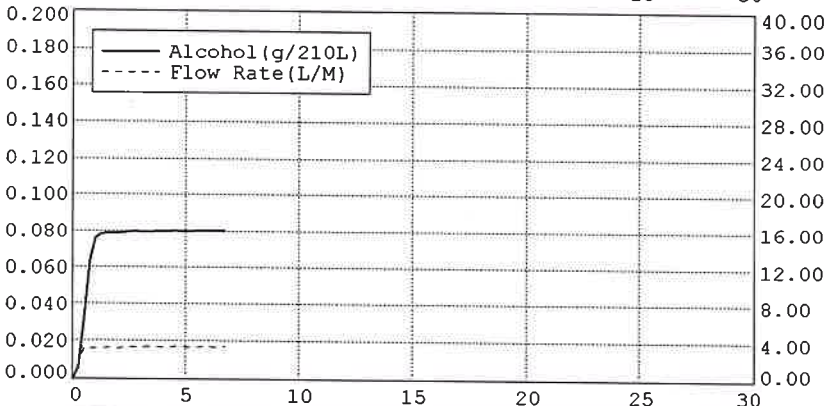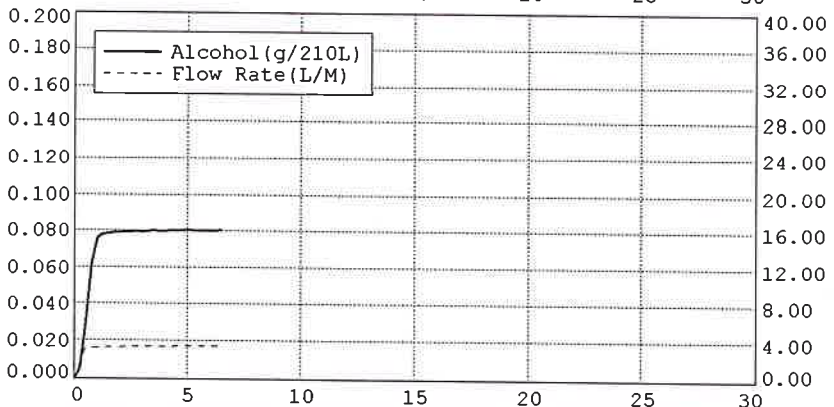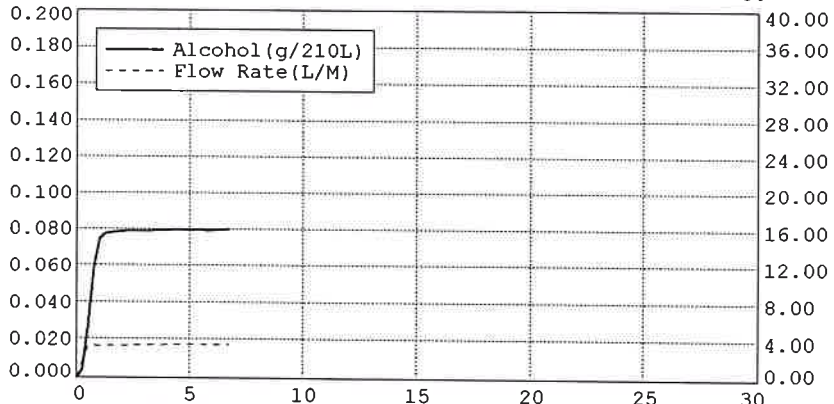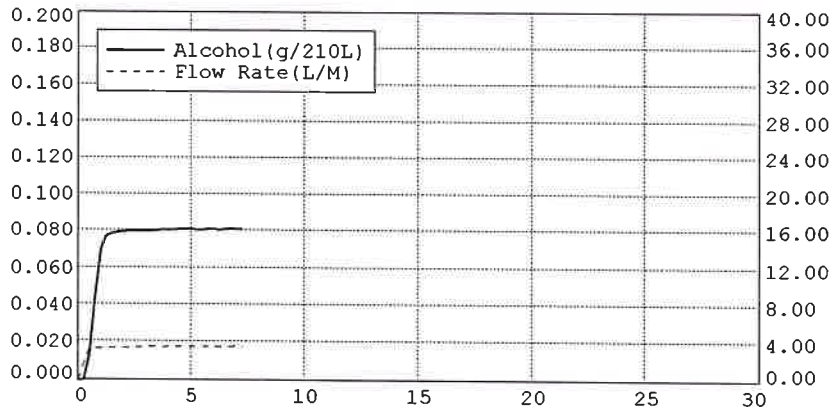

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100375






Date: 01/17/2024
Time: 12:37:45

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 30.24: 0.303
LOT #: AG327804
EXPIRATION: 10/05/2025
TANK PRESSURE: 354 psi

BLANK TEST	0.000	12:38
INTERNAL STANDARD	VERIFIED	12:38
EXTERNAL STANDARD	0.302	12:39
BLANK TEST	0.000	12:40
EXTERNAL STANDARD	0.302	12:40
BLANK TEST	0.000	12:41
EXTERNAL STANDARD	0.302	12:41
BLANK TEST	0.000	12:42
EXTERNAL STANDARD	0.302	12:42
BLANK TEST	0.000	12:43
EXTERNAL STANDARD	0.302	12:43
BLANK TEST	0.000	12:44

Average = 0.3020
Std Dev = 0.0000

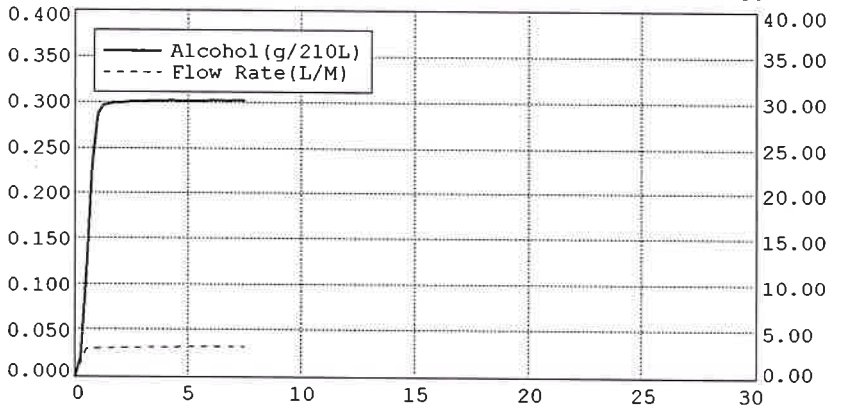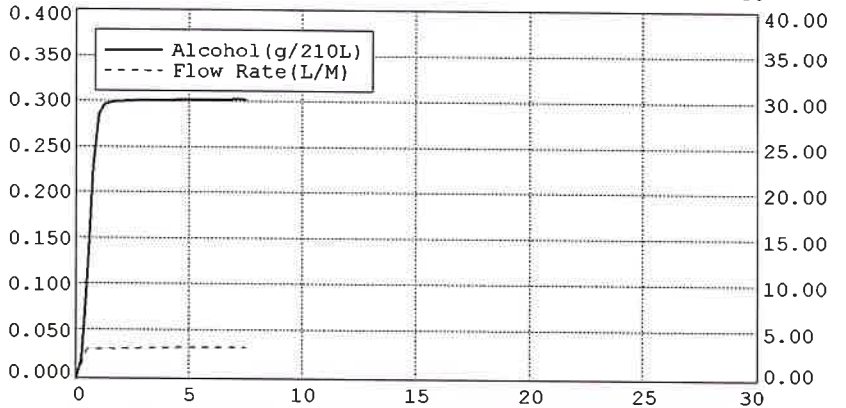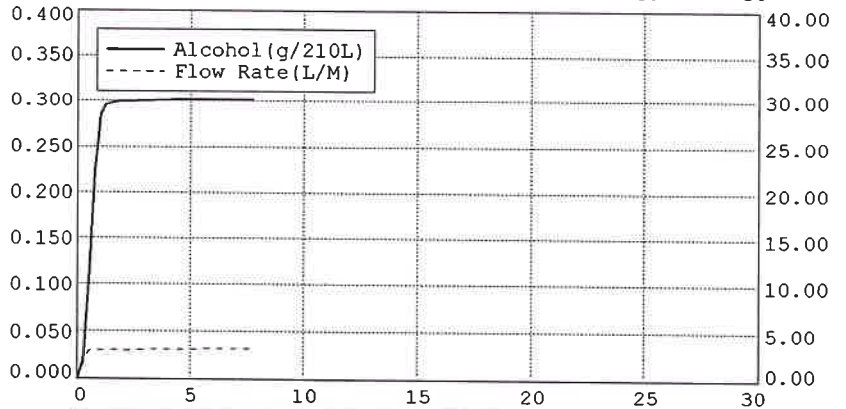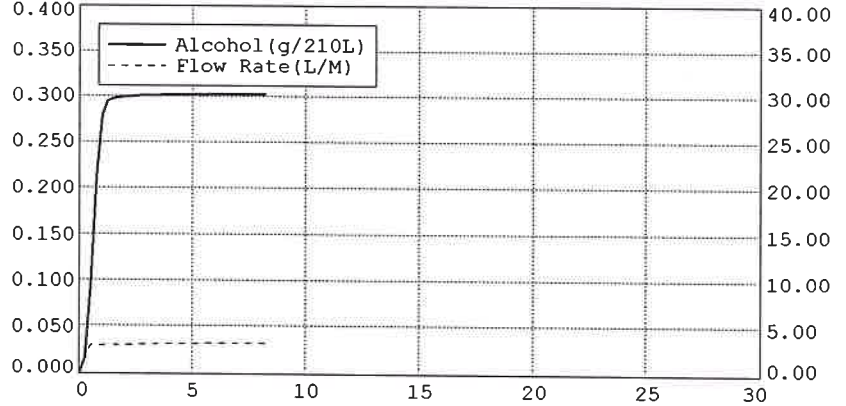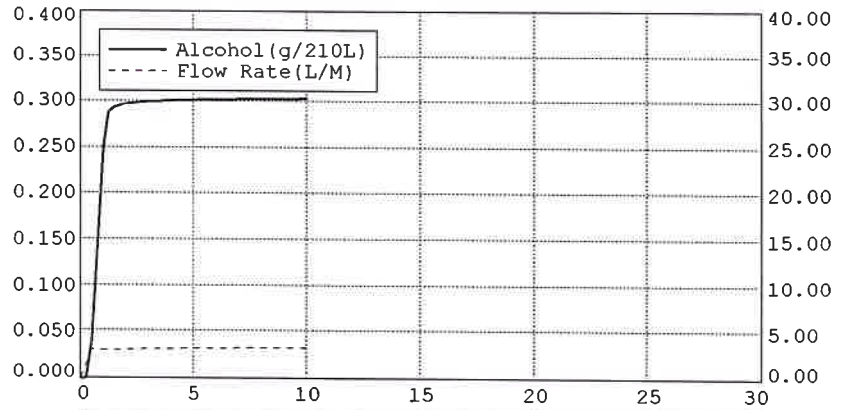

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100397

Date: 01/17/2024
Time: 11:51:05

VERSIONS
DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 48.1°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.77 V PASSED
(1.01 V - 2.37 V)
Cooler Voltage = 1.59 V PASSED
(1.04 V - 2.44 V)
Bias Voltage = 81 V PASSED
(49 V - 113 V)
Chopper Freq = 527 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 30.3 in

PUMP INFO

Flow Rate = 4.288 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED
Xq = 0.093 1.11% (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100397

Date: 01/17/2024
Time: 11:54 AM

Temperatures (°C)

Sample Cell: 48.9°C
Breath Tube: 48.1°C

Current Barometer 30.2 in
Volume (Ltr) 0.00

Settings

Lamp: 1.77 V
Bias: 81 V
Cooler: 1.64 V
Chopper: 525 Hz

Voltages (V)

Flow: 1.06 V
Detector: 0.046 V

LINEARITY CHECK


Alaska Department of Public Safety
DATAMASTER dmt: 100397

Date: 01/17/2024
Time: 12:05:16

SUPERVISOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.081	0.0800	0.0000
0.303	0.3020	0.0007

SLOPE = 0.997415
R² = 0.999992

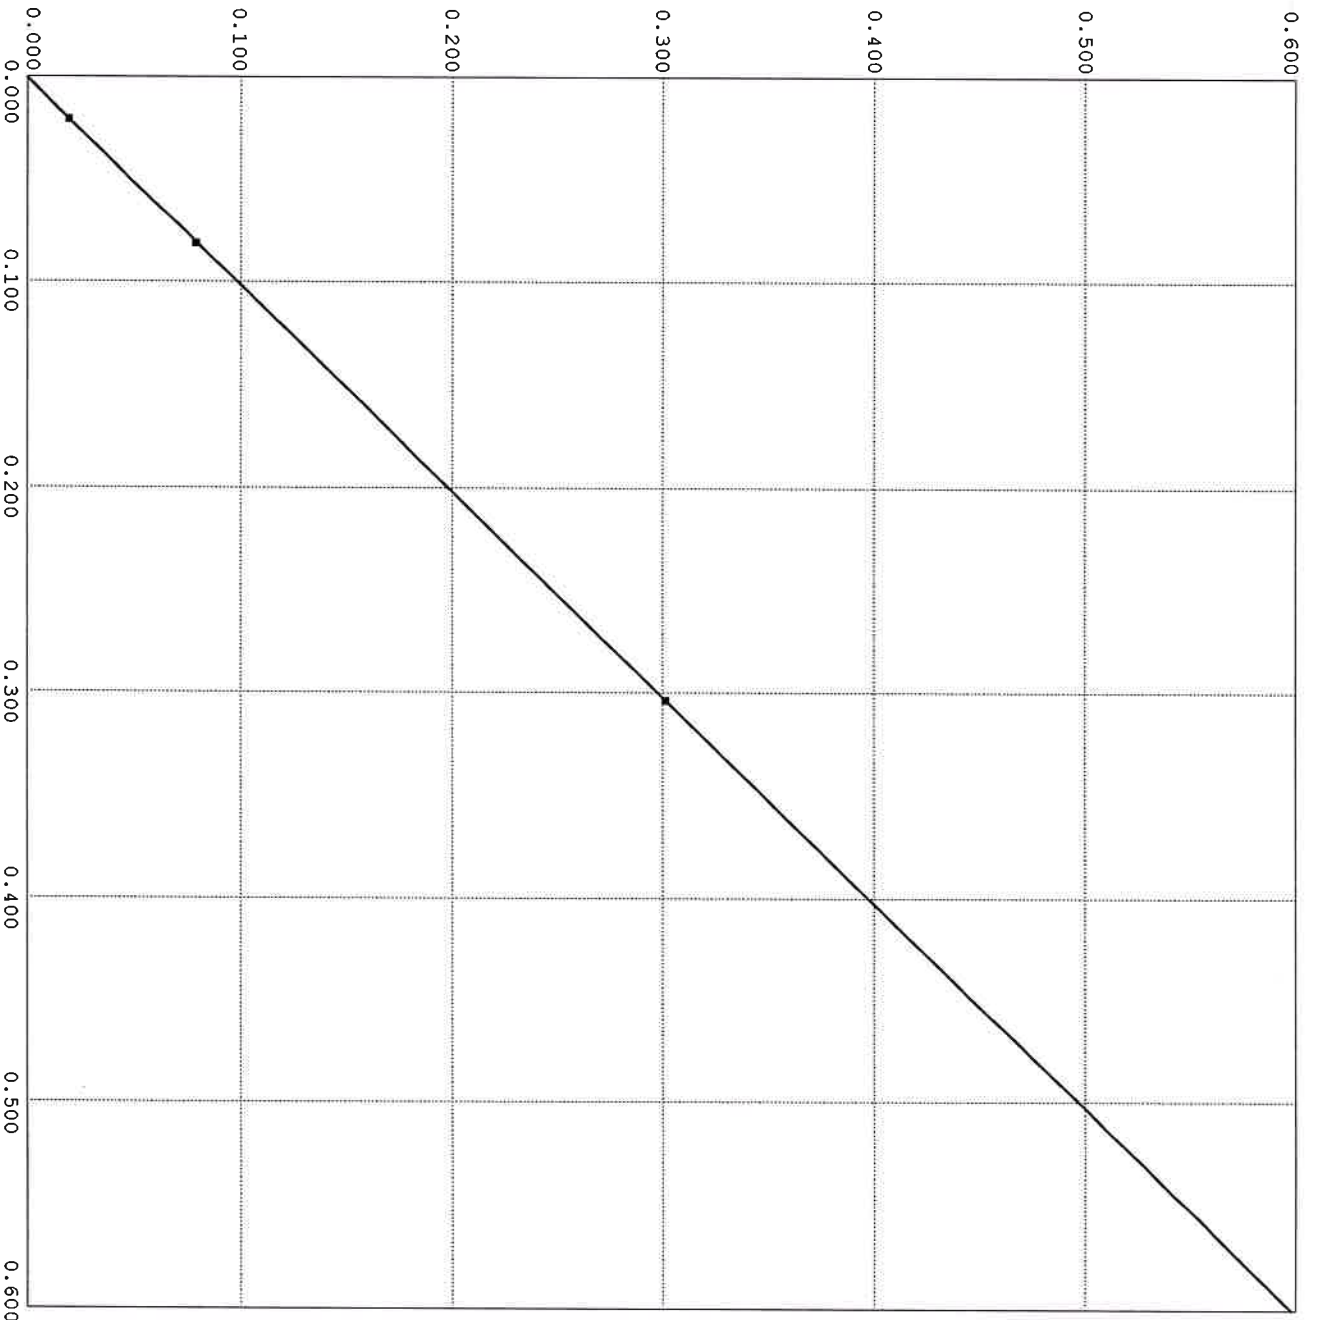

CRB

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100397






Date: 01/17/2024
Time: 12:05:18

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 30.25: 0.020
LOT #: AG217902
EXPIRATION: 06/28/2024
TANK PRESSURE: 407 psi

BLANK TEST	0.000	12:09
INTERNAL STANDARD	VERIFIED	12:09
EXTERNAL STANDARD	0.020	12:09
BLANK TEST	0.000	12:10
EXTERNAL STANDARD	0.020	12:10
BLANK TEST	0.000	12:11
EXTERNAL STANDARD	0.020	12:12
BLANK TEST	0.000	12:12
EXTERNAL STANDARD	0.020	12:13
BLANK TEST	0.000	12:14
EXTERNAL STANDARD	0.020	12:14
BLANK TEST	0.000	12:15

Average = 0.0200
Std Dev = 0.0000

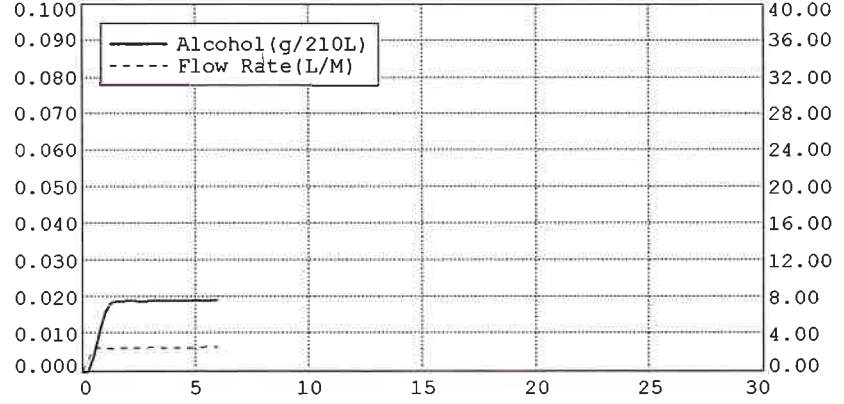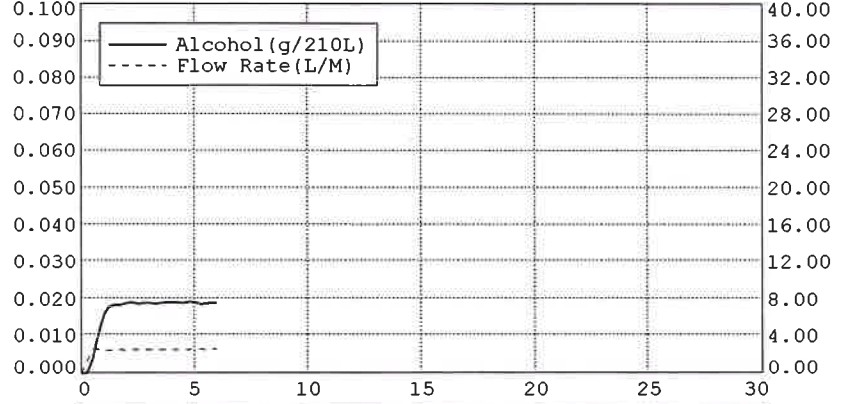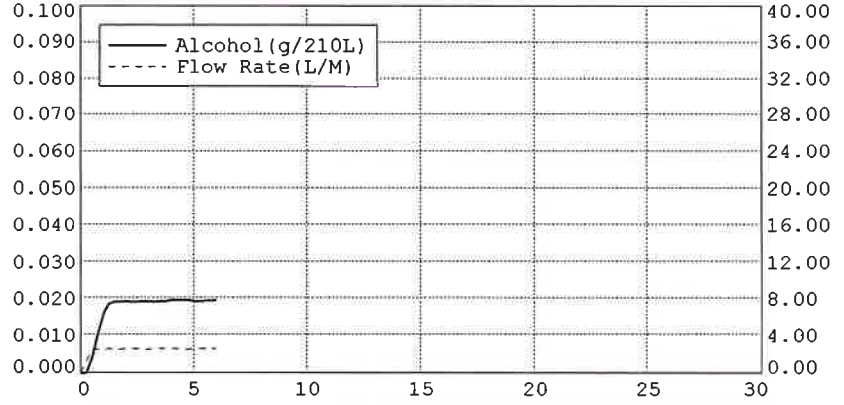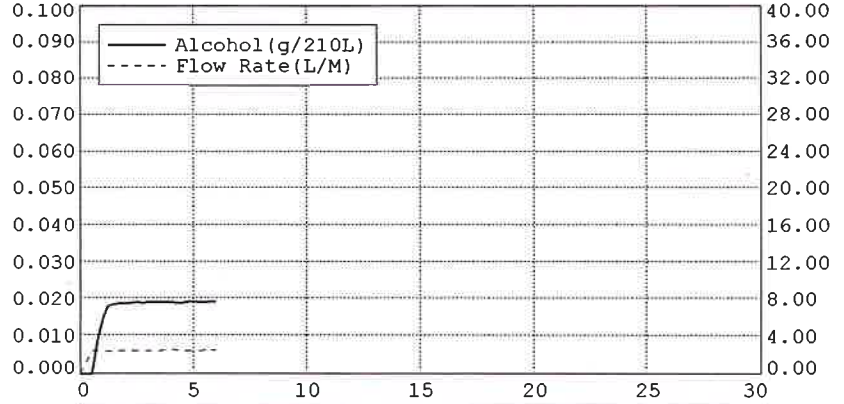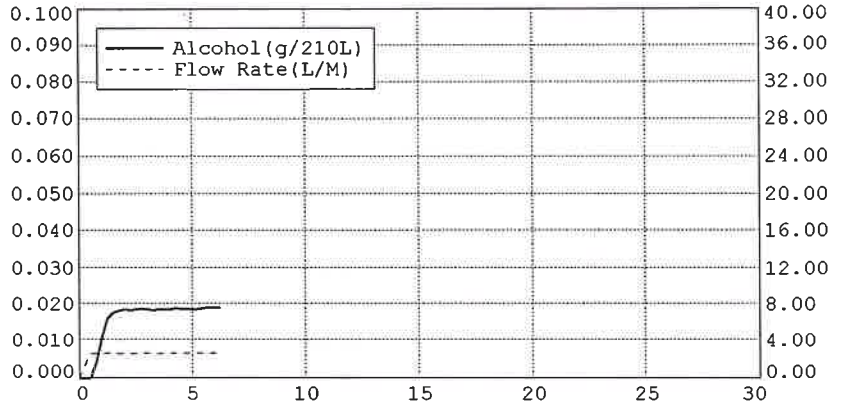

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100397






Date: 01/17/2024
 Time: 12:16:06

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 30.25: 0.081
 LOT #: 09523080A1
 EXPIRATION: 05/05/2025
 TANK PRESSURE: 546 psi

BLANK TEST	0.000	12:18
INTERNAL STANDARD	VERIFIED	12:18
EXTERNAL STANDARD	0.080	12:18
BLANK TEST	0.000	12:19
EXTERNAL STANDARD	0.080	12:19
BLANK TEST	0.000	12:20
EXTERNAL STANDARD	0.080	12:21
BLANK TEST	0.000	12:21
EXTERNAL STANDARD	0.080	12:22
BLANK TEST	0.000	12:23
EXTERNAL STANDARD	0.080	12:23
BLANK TEST	0.000	12:24

Average = 0.0800
 Std Dev = 0.0000

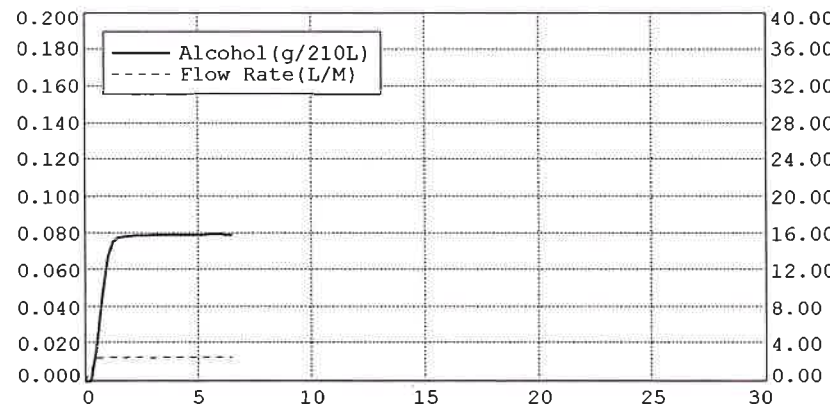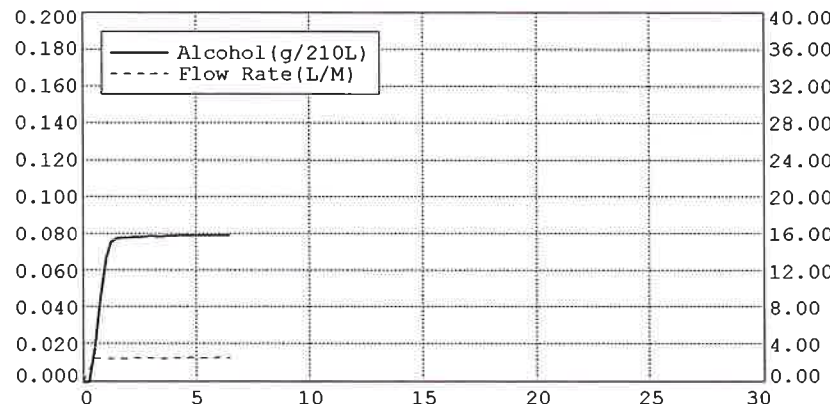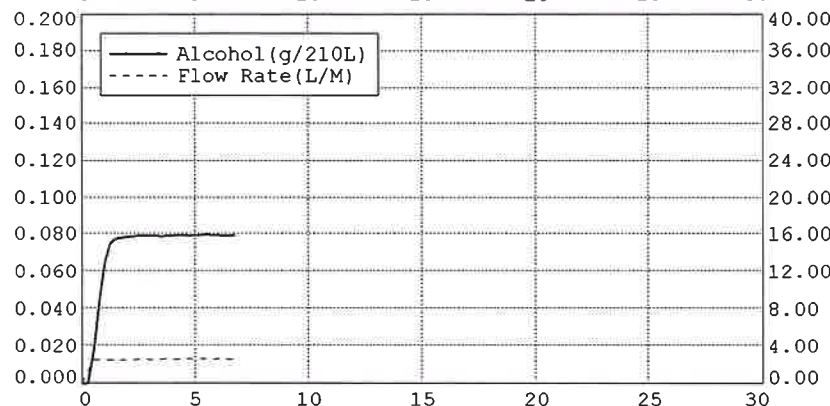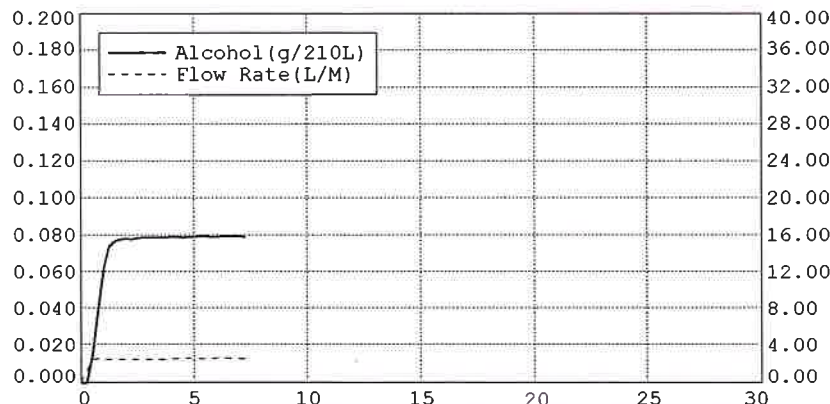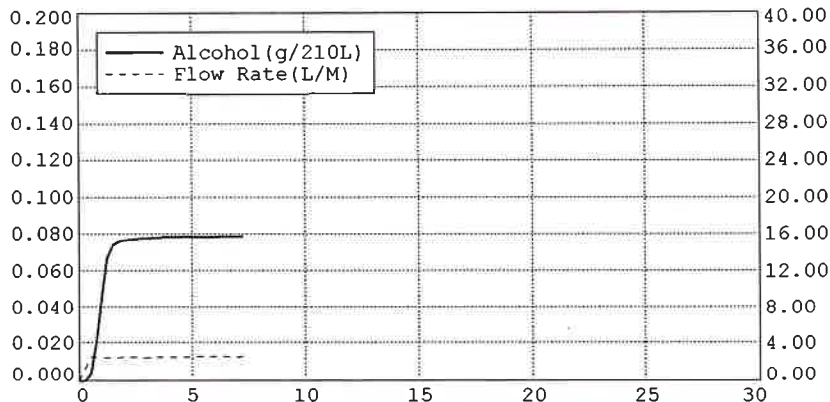

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100397






Date: 01/17/2024
 Time: 12:26:41

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 30.25: 0.303
 LOT #: AG327804
 EXPIRATION: 10/05/2025
 TANK PRESSURE: 312 psi

BLANK TEST	0.000	12:27
INTERNAL STANDARD	VERIFIED	12:28
EXTERNAL STANDARD	0.301	12:28
BLANK TEST	0.000	12:29
EXTERNAL STANDARD	0.302	12:29
BLANK TEST	0.000	12:30
EXTERNAL STANDARD	0.303	12:30
BLANK TEST	0.000	12:31
EXTERNAL STANDARD	0.302	12:31
BLANK TEST	0.000	12:32
EXTERNAL STANDARD	0.302	12:32
BLANK TEST	0.000	12:33

Average = 0.3020
 Std Dev = 0.0007

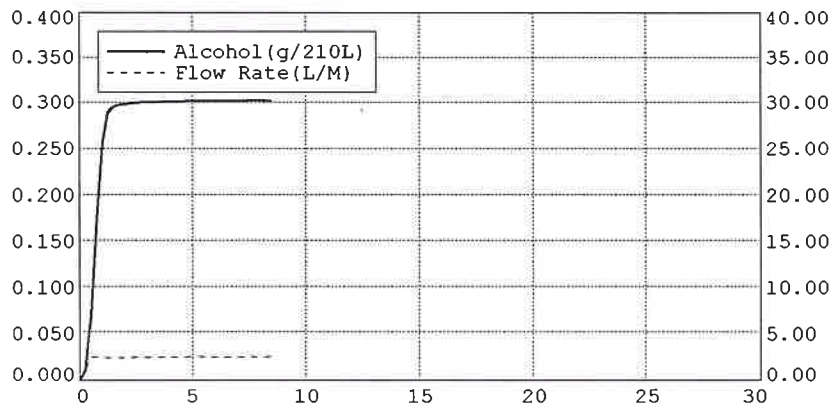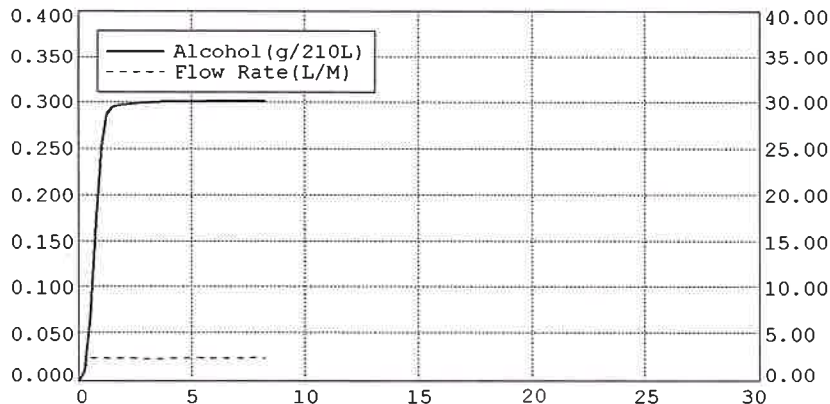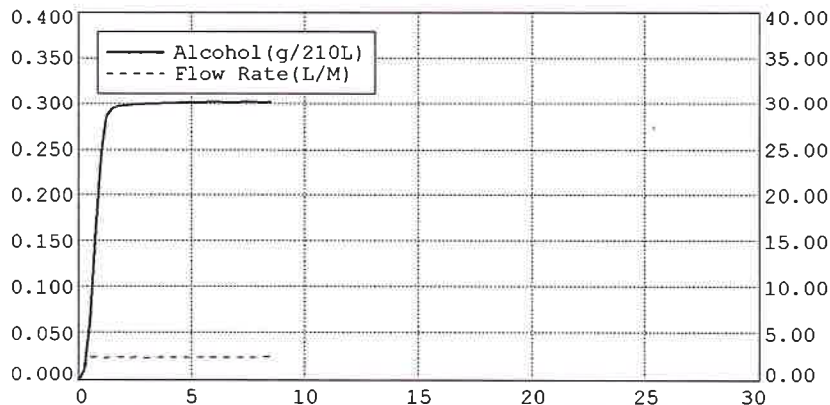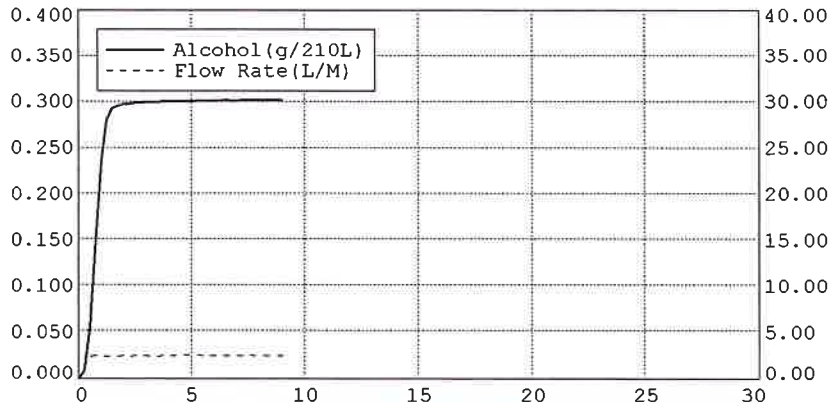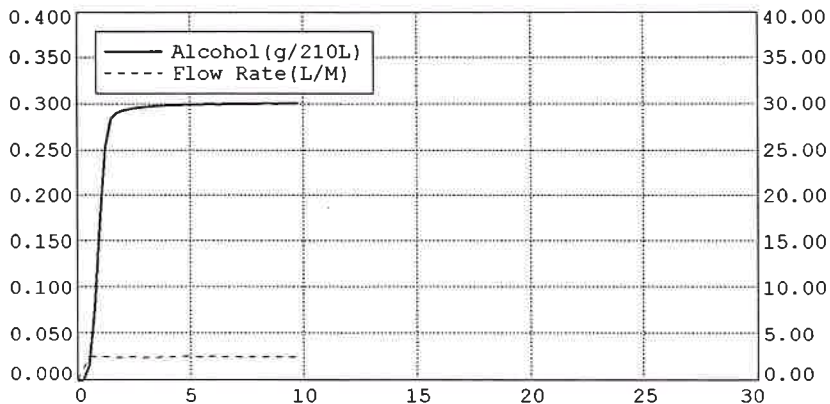

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100399

Date: 01/17/2024
Time: 11:48:38

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 48.1°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.79 V PASSED
(1.00 V - 2.32 V)
Cooler Voltage = 1.58 V PASSED
(0.99 V - 2.31 V)
Bias Voltage = 81 V PASSED
(49 V - 113 V)
Chopper Freq = 525 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 30.2 in

PUMP INFO

Flow Rate = 4.701 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED
Xq = 0.086 1.44% (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100399

Date: 01/17/2024
Time: 11:52 AM

Temperatures (°C)
Sample Cell: 48.9°C
Breath Tube: 48.1°C

Current Barometer 30.2 in
Volume (Ltr) 0.00

Settings
Lamp: 1.79 V
Bias: 81 V
Cooler: 1.58 V
Chopper: 524 Hz

Voltages (V)
Flow: 1.06 V
Detector: -0.033 V

LINEARITY CHECK

Alaska Department of Public Safety
DATAMASTER dmt: 100399


Date: 01/17/2024
Time: 12:06:54

SUPERVISOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0192	0.0013
0.081	0.0800	0.0000
0.303	0.3040	0.0000

SLOPE = 1.007072
R² = 0.999995

MR

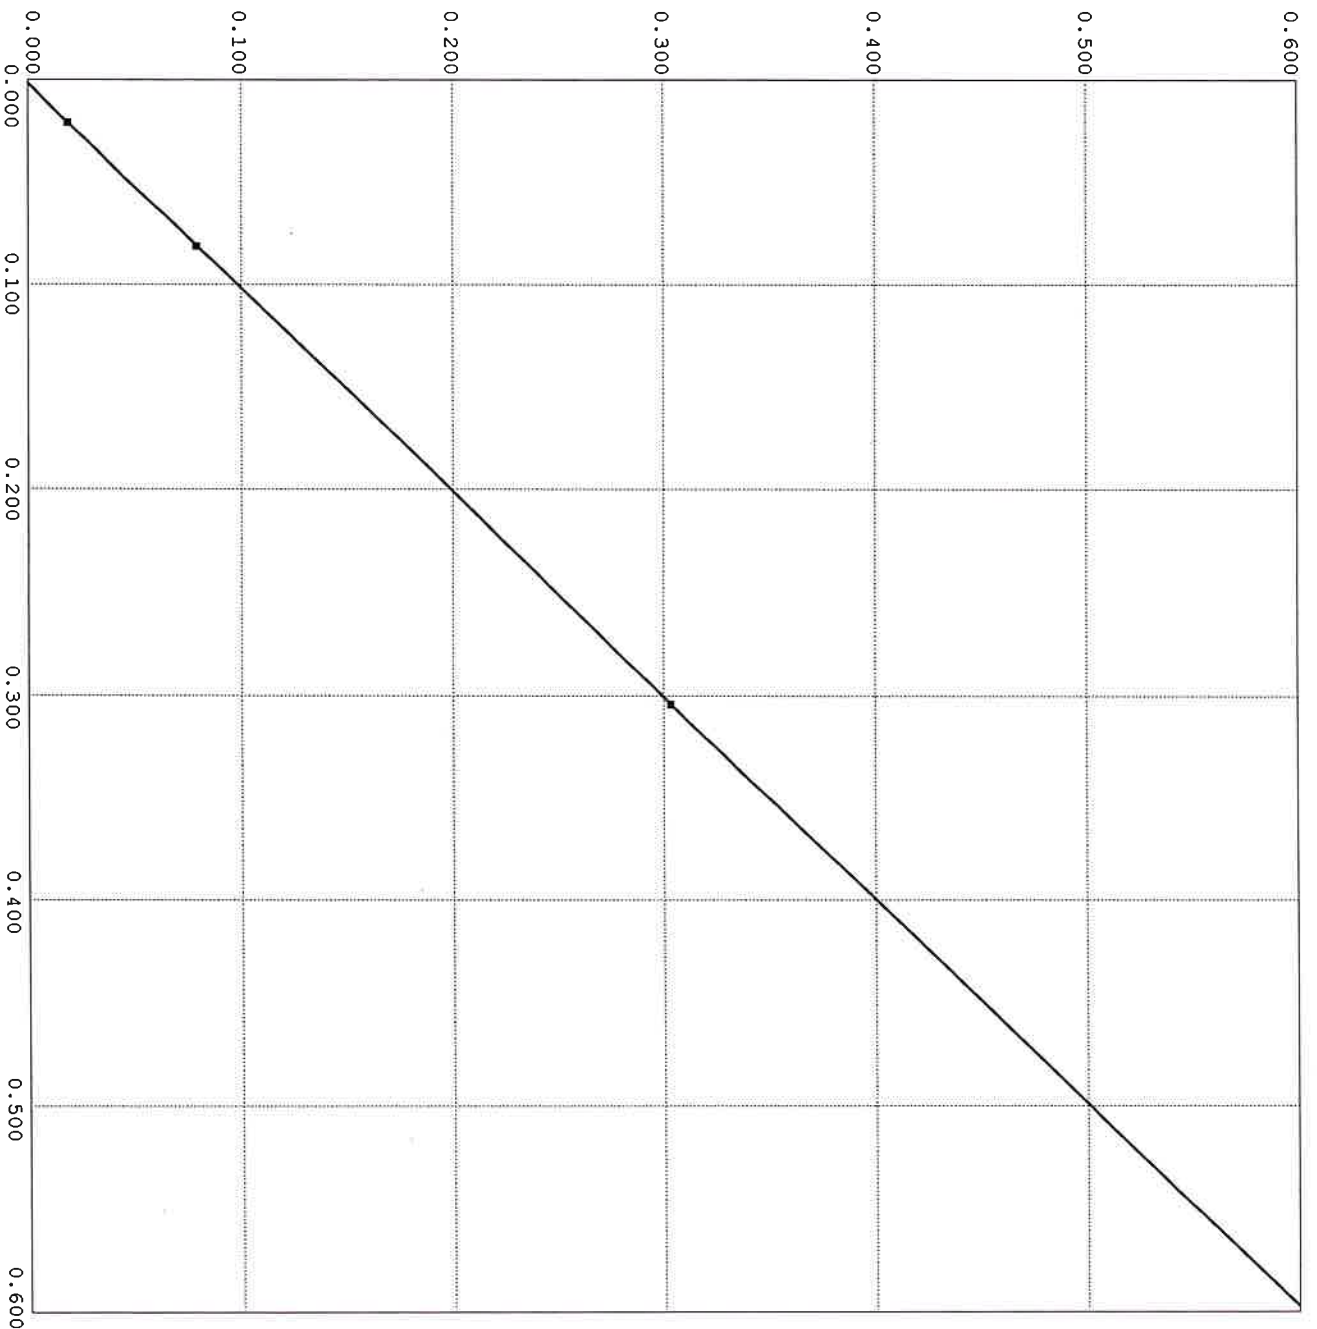

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100399






Date: 01/17/2024
 Time: 12:06:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 30.23: 0.020
 LOT #: AG217902
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 400 psi

BLANK TEST	0.000	12:14
INTERNAL STANDARD	VERIFIED	12:14
EXTERNAL STANDARD	0.019	12:14
BLANK TEST	0.000	12:15
EXTERNAL STANDARD	0.017	12:15
BLANK TEST	0.000	12:16
EXTERNAL STANDARD	0.020	12:16
BLANK TEST	0.000	12:17
EXTERNAL STANDARD	0.020	12:17
BLANK TEST	0.000	12:18
EXTERNAL STANDARD	0.020	12:18
BLANK TEST	0.000	12:19

Average = 0.0192
 Std Dev = 0.0013

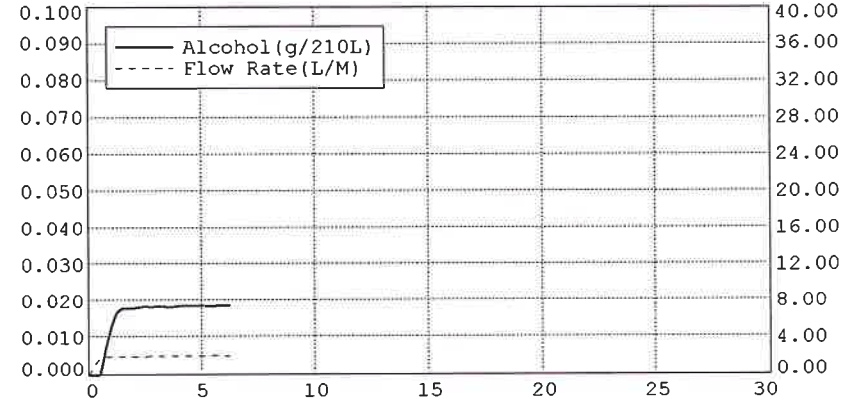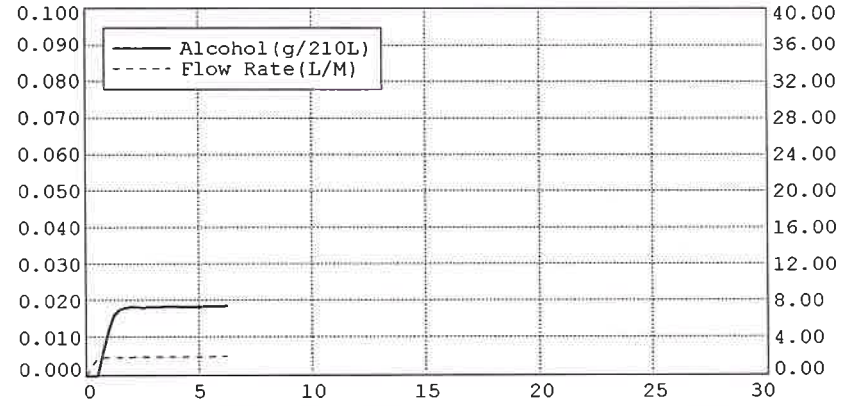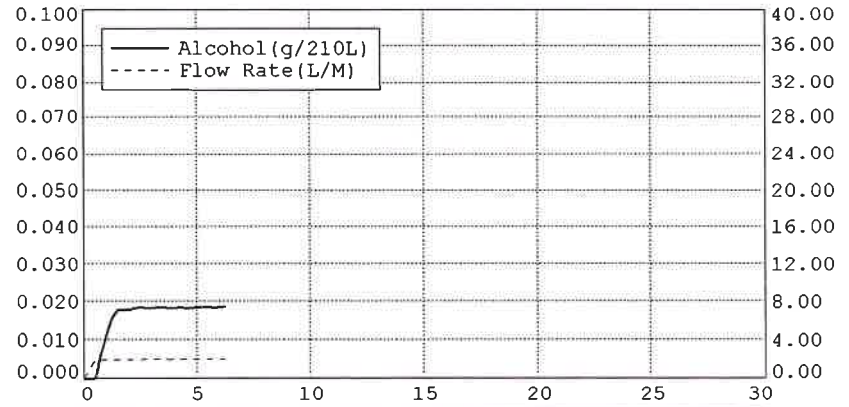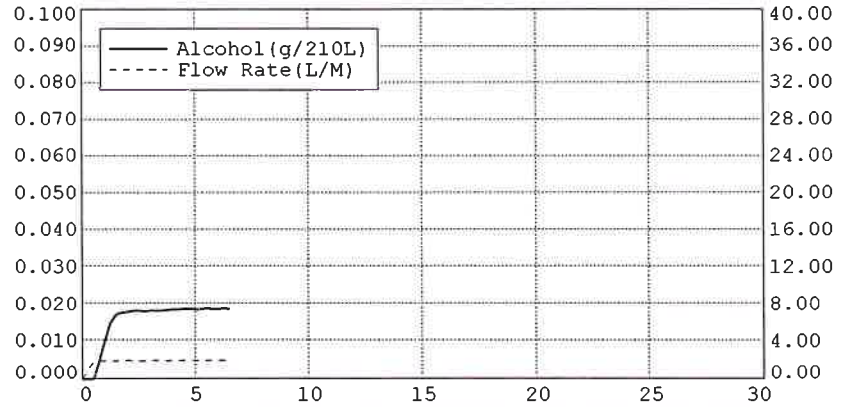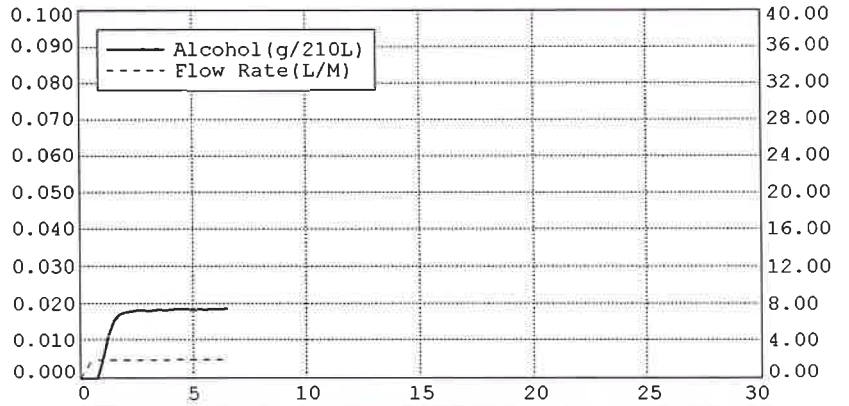

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100399






Date: 01/17/2024
Time: 12:25:52

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 30.23: 0.081
LOT #: AG310901
EXPIRATION: 04/19/2025
TANK PRESSURE: 278 psi

BLANK TEST	0.000	12:27
INTERNAL STANDARD	VERIFIED	12:27
EXTERNAL STANDARD	0.080	12:27
BLANK TEST	0.000	12:28
EXTERNAL STANDARD	0.080	12:28
BLANK TEST	0.000	12:29
EXTERNAL STANDARD	0.080	12:29
BLANK TEST	0.000	12:30
EXTERNAL STANDARD	0.080	12:30
BLANK TEST	0.000	12:31
EXTERNAL STANDARD	0.080	12:31
BLANK TEST	0.000	12:32

Average = 0.0800
Std Dev = 0.0000

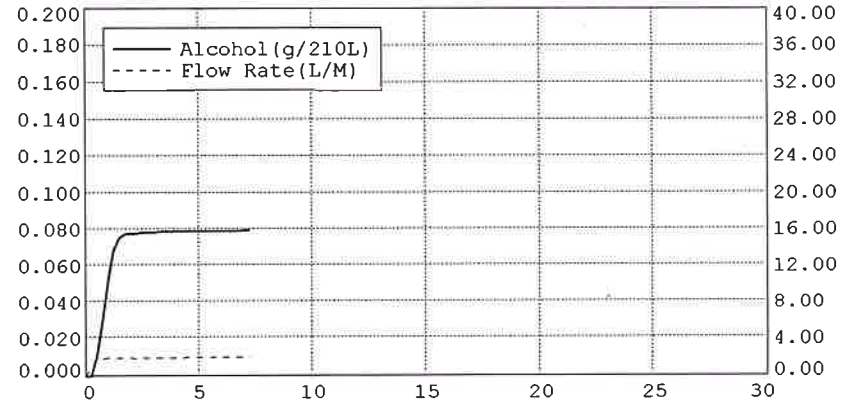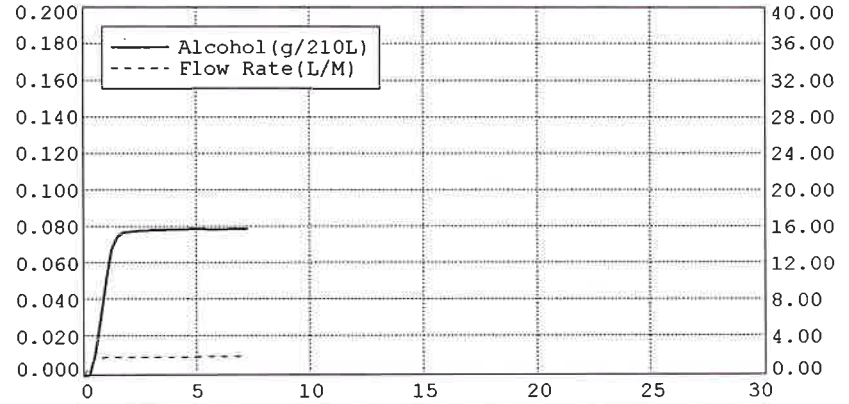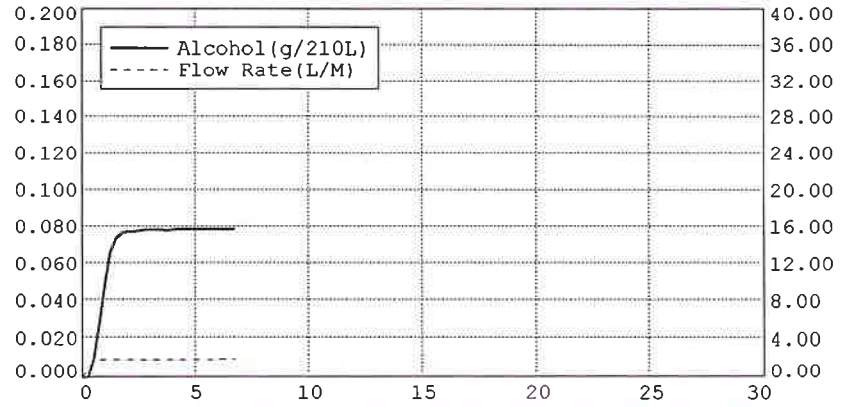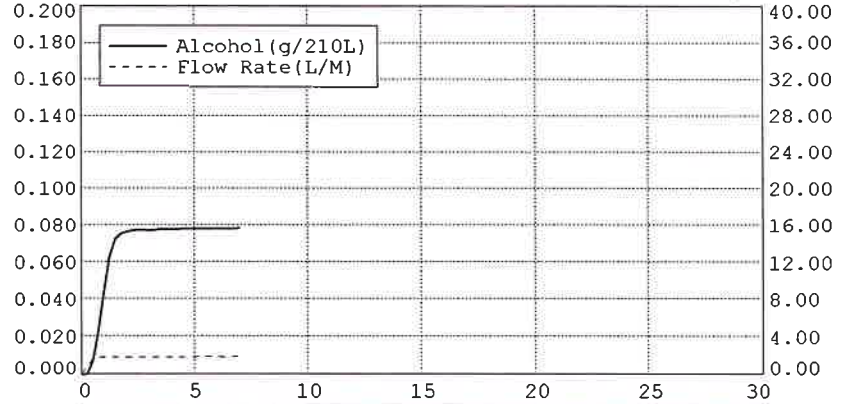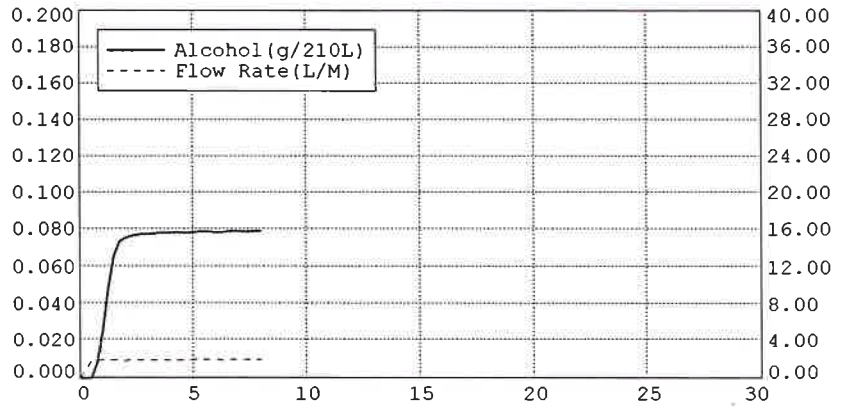

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100399






Date: 01/17/2024
Time: 12:38:29

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 30.23: 0.303
LOT #: AG327804
EXPIRATION: 10/05/2025
TANK PRESSURE: 293 psi

BLANK TEST	0.000	12:40
INTERNAL STANDARD	VERIFIED	12:40
EXTERNAL STANDARD	0.304	12:40
BLANK TEST	0.000	12:41
EXTERNAL STANDARD	0.304	12:41
BLANK TEST	0.000	12:42
EXTERNAL STANDARD	0.304	12:42
BLANK TEST	0.000	12:43
EXTERNAL STANDARD	0.304	12:44
BLANK TEST	0.000	12:44
EXTERNAL STANDARD	0.304	12:45
BLANK TEST	0.000	12:46

Average = 0.3040
Std Dev = 0.0000

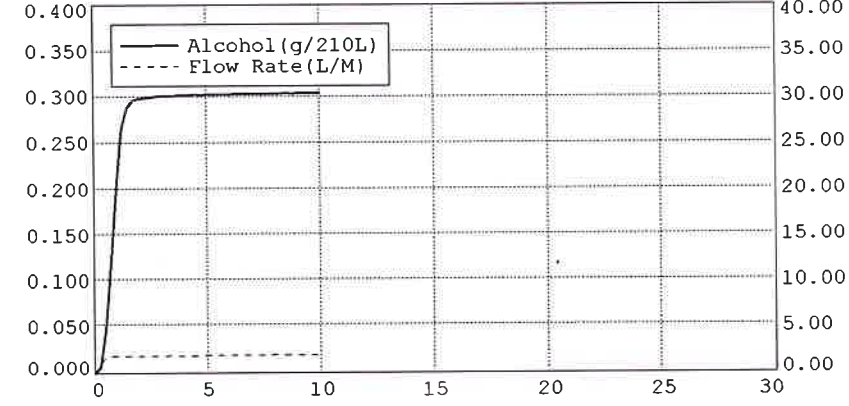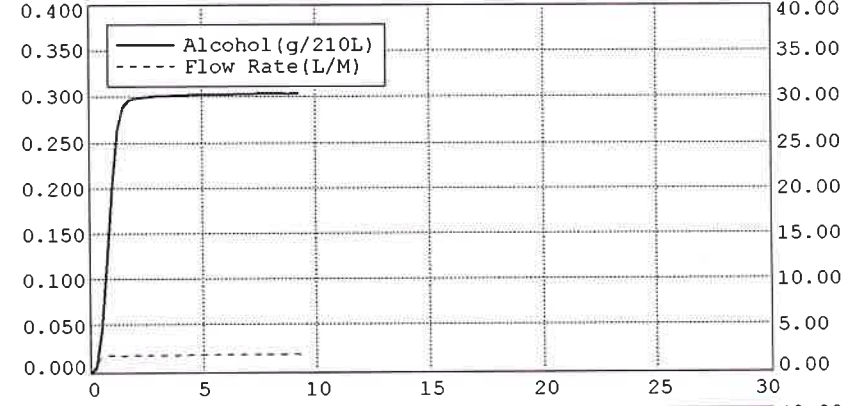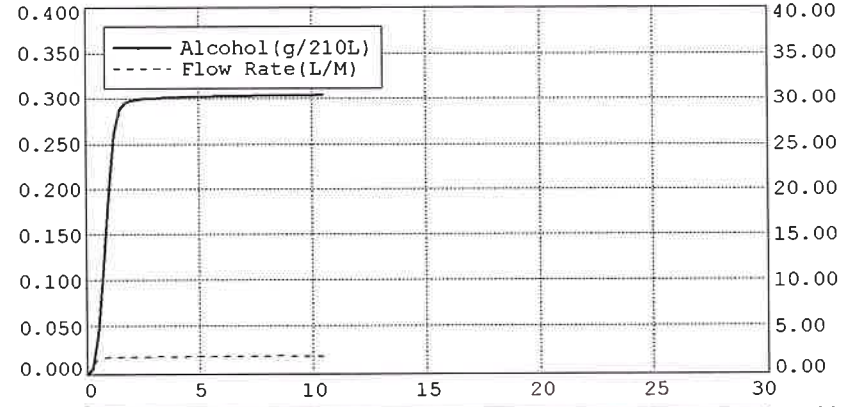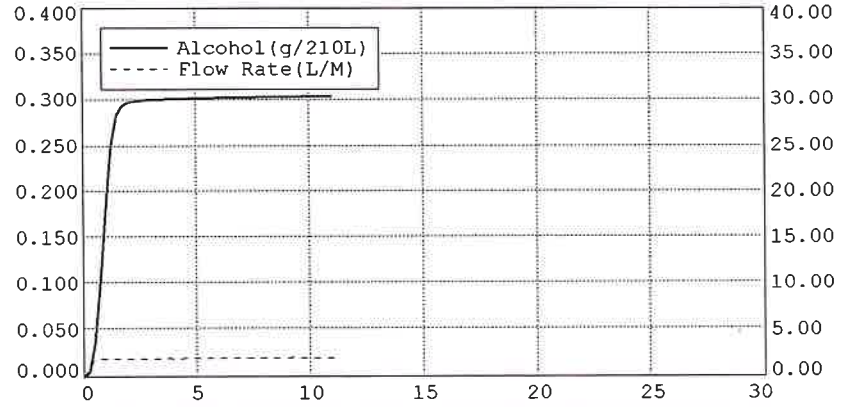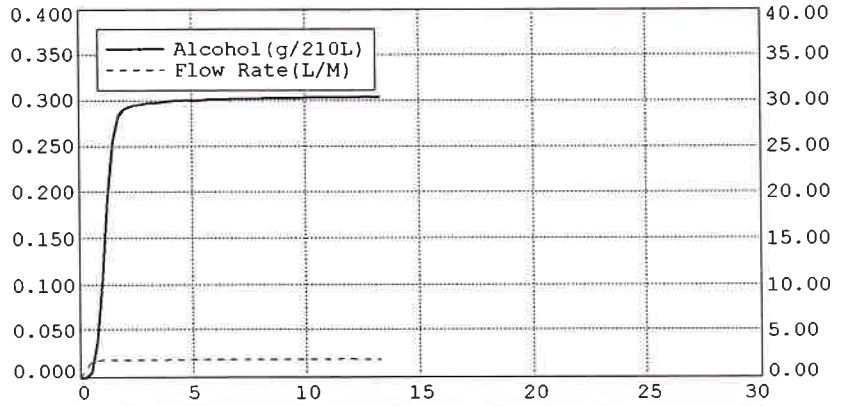

SUPERVISOR TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100375

Date: 01/17/2024
Time: 12:54:37

SUPERVISOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.24: 0.081
TANK PRESSURE: 1238 psi






BLANK TEST	0.000	12:55
INTERNAL STANDARD	VERIFIED	12:55
EXTERNAL STANDARD	0.081	12:55
BLANK TEST	0.000	12:56
EXTERNAL STANDARD	0.081	12:57
BLANK TEST	0.000	12:57
EXTERNAL STANDARD	0.082	12:58
BLANK TEST	0.000	12:59
EXTERNAL STANDARD	0.081	12:59
BLANK TEST	0.000	13:00
EXTERNAL STANDARD	0.081	13:00
BLANK TEST	0.000	13:01

Average = 0.0812
Std Dev = 0.0004

Lot A6335202
Exp 12/18/25
Tank 016

COB
1/17/24

Tank 016 Average: 0.081
COB 2024.01.18

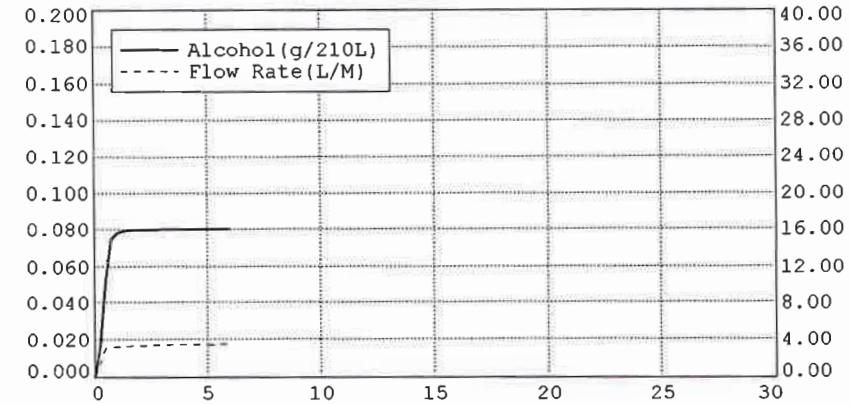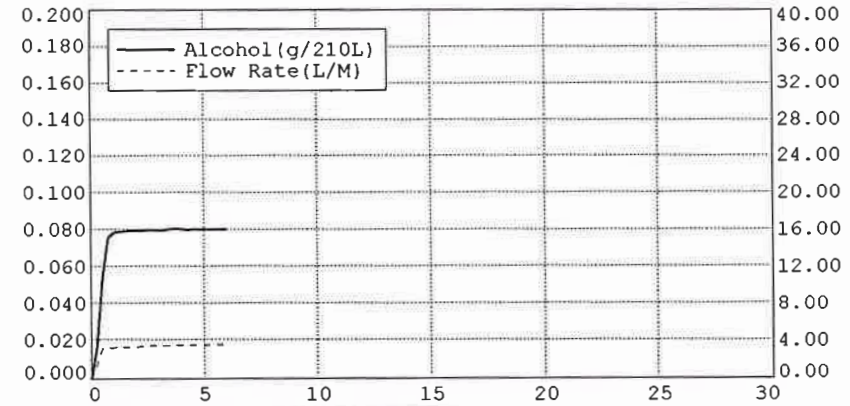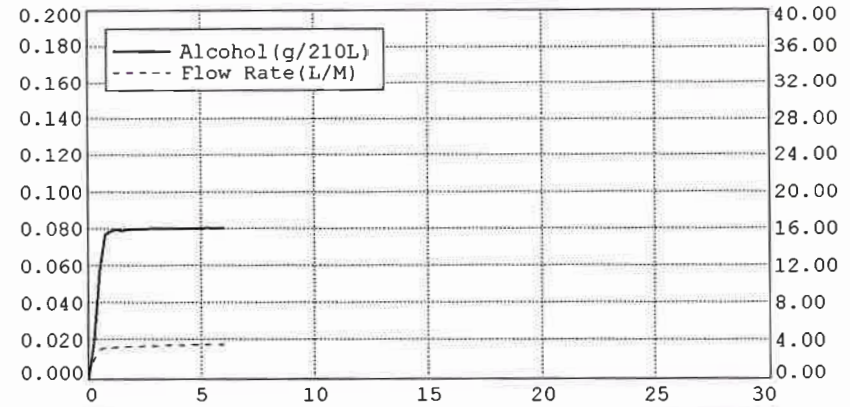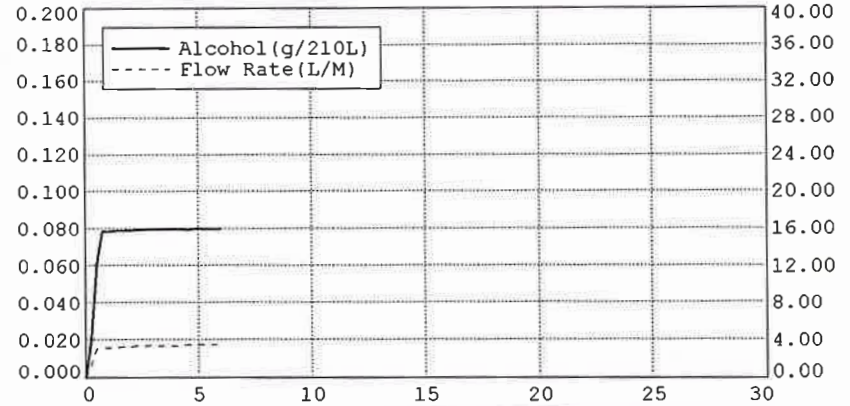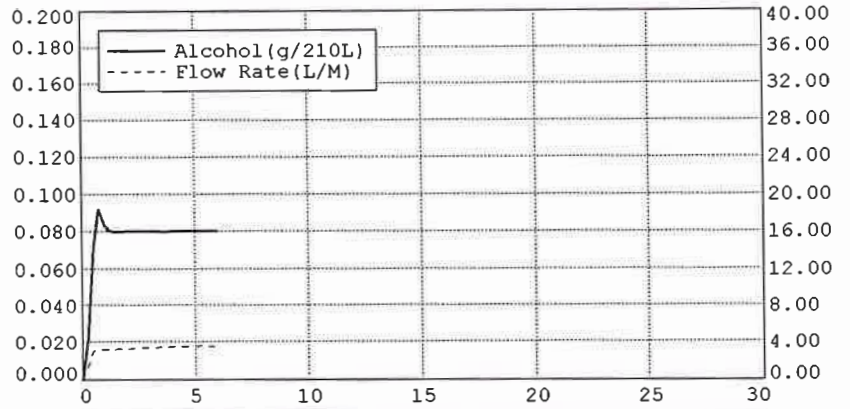

SUPERVISOR TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100397

Date: 01/17/2024
Time: 12:43:12

SUPERVISOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.24: 0.081
TANK PRESSURE: 1209 psi






BLANK TEST	0.000	12:44
INTERNAL STANDARD	VERIFIED	12:44
EXTERNAL STANDARD	0.081	12:44
BLANK TEST	0.000	12:45
EXTERNAL STANDARD	0.081	12:45
BLANK TEST	0.000	12:46
EXTERNAL STANDARD	0.081	12:46
BLANK TEST	0.000	12:47
EXTERNAL STANDARD	0.081	12:48
BLANK TEST	0.000	12:48
EXTERNAL STANDARD	0.080	12:49
BLANK TEST	0.000	12:50

Average = 0.0808
Std Dev = 0.0004

Lot # 35202
Exp 12/18/25

Tank 016

COB
1/17/24

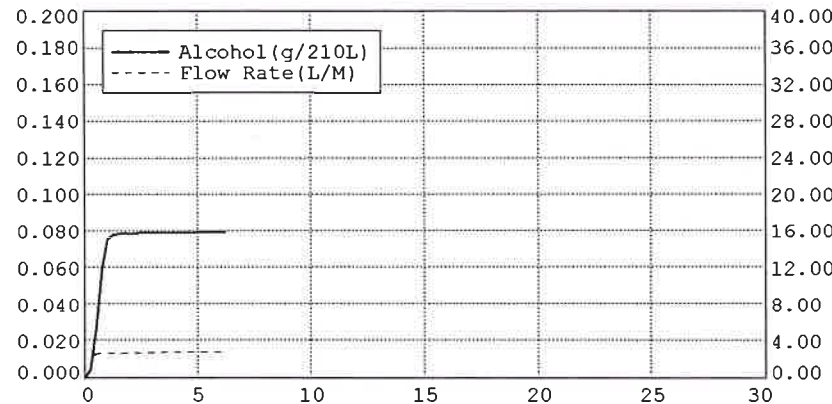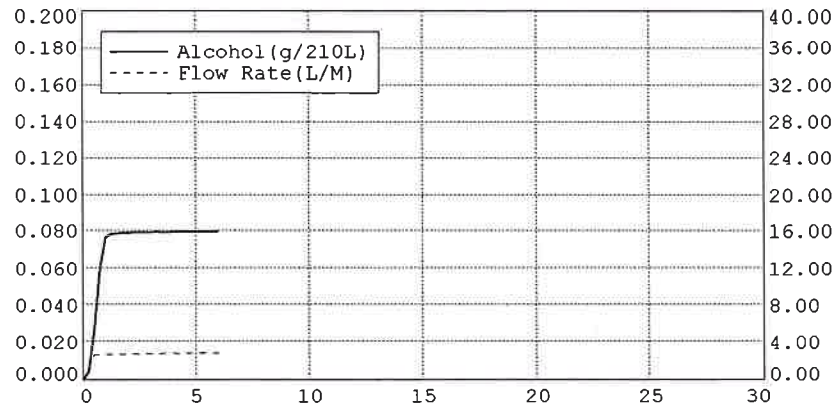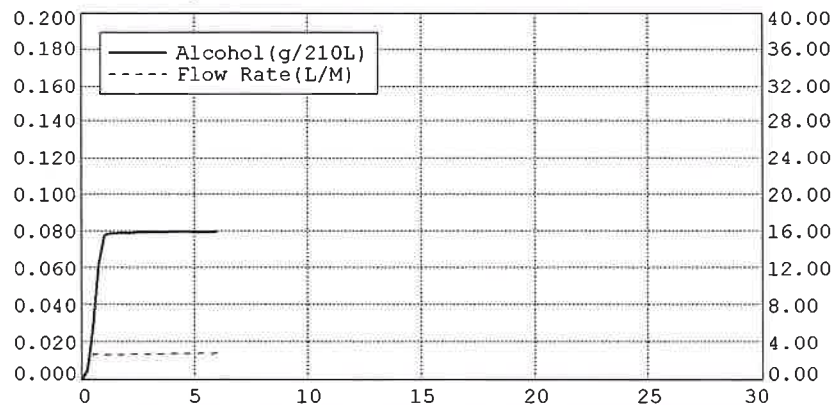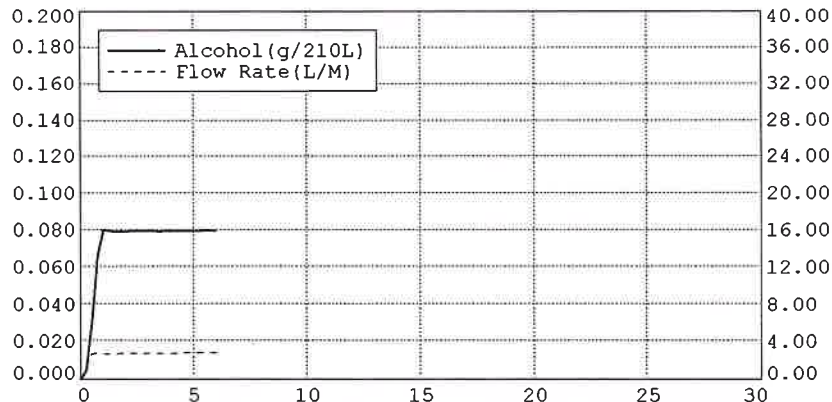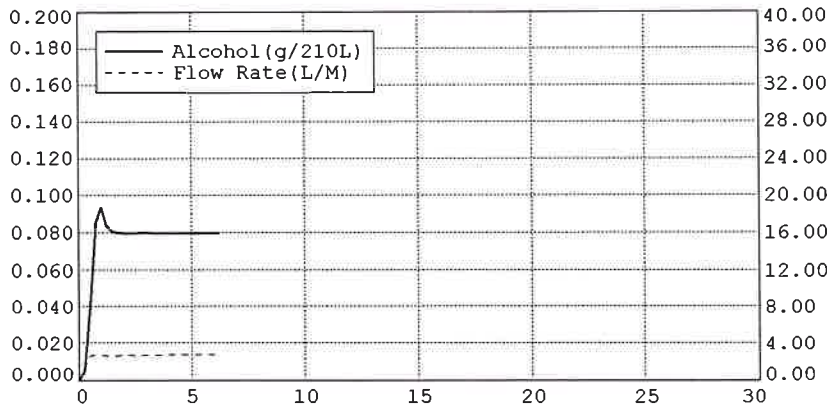

SUPERVISOR TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100399

Date: 01/17/2024
Time: 12:51:11

SUPERVISOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.23: 0.081
TANK PRESSURE: 1221 psi






BLANK TEST	0.000	12:52
INTERNAL STANDARD	VERIFIED	12:52
EXTERNAL STANDARD	0.082	12:52
BLANK TEST	0.000	12:53
EXTERNAL STANDARD	0.081	12:53
BLANK TEST	0.000	12:54
EXTERNAL STANDARD	0.082	12:55
BLANK TEST	0.000	12:55
EXTERNAL STANDARD	0.081	12:56
BLANK TEST	0.000	12:57
EXTERNAL STANDARD	0.081	12:57
BLANK TEST	0.000	12:58

Average = 0.0814
Std Dev = 0.0005

Lot AG33500
Exp 12/18/25

Tank 016

COB
1/17/24

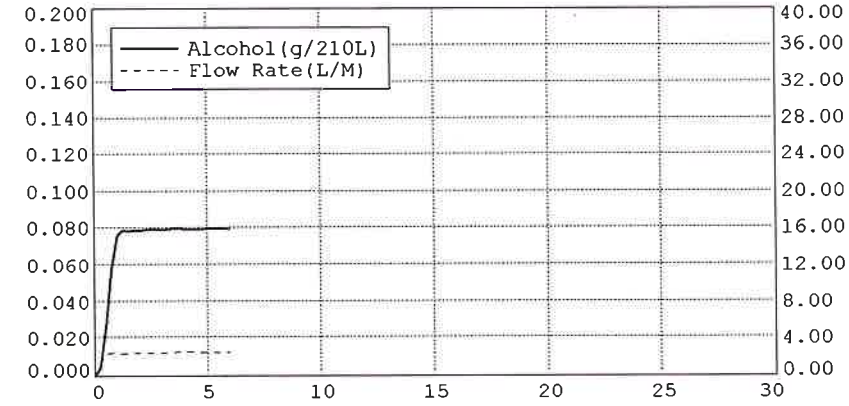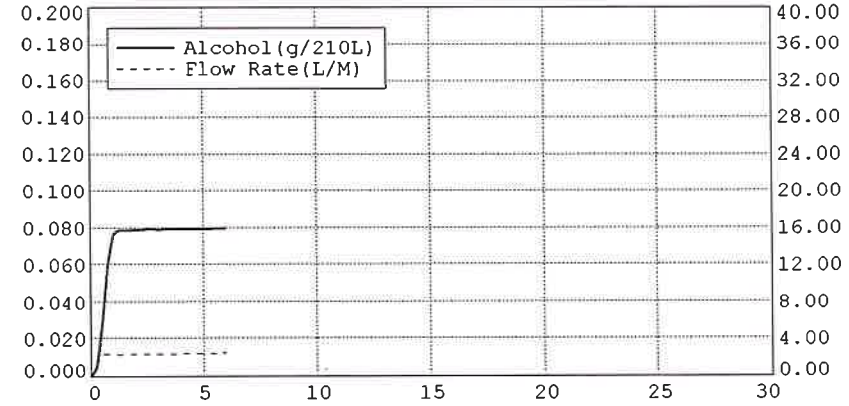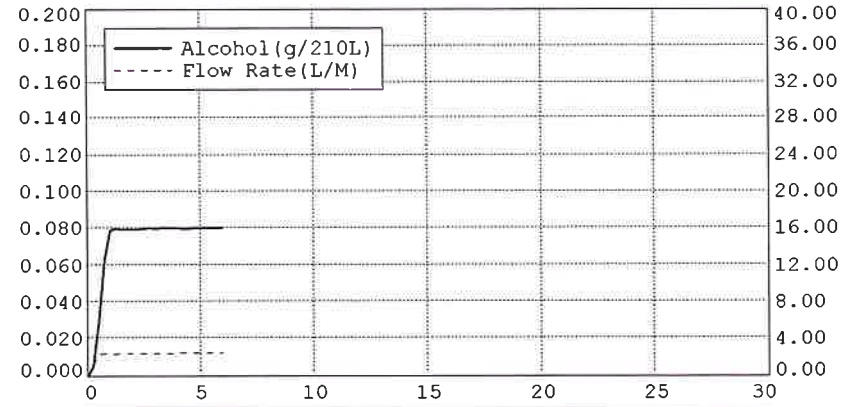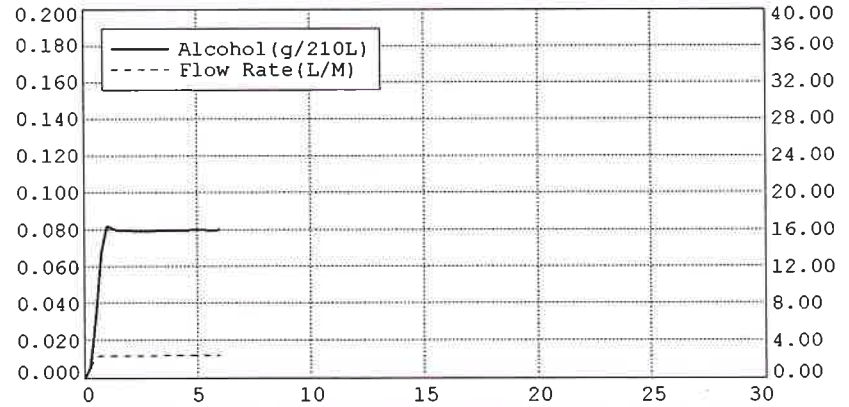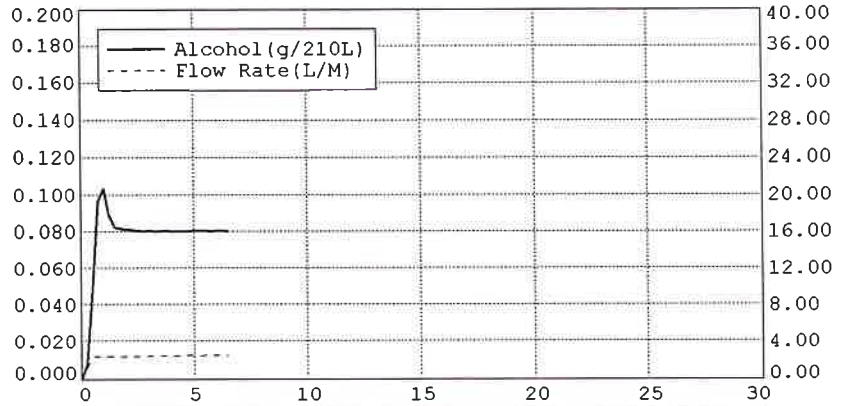

SUPERVISOR TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100375

Date: 01/17/2024
 Time: 13:03:31

SUPERVISOR NAME:
 COLLEEN S OBRYANT
 OPERATOR'S #: 6237

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 30.23: 0.081
 TANK PRESSURE: 1243 psi

BLANK TEST	0.000	13:04
INTERNAL STANDARD	VERIFIED	13:04
EXTERNAL STANDARD	0.082	13:04
BLANK TEST	0.000	13:05
EXTERNAL STANDARD	0.082	13:06
BLANK TEST	0.000	13:06
EXTERNAL STANDARD	0.082	13:07
BLANK TEST	0.000	13:08
EXTERNAL STANDARD	0.082	13:08
BLANK TEST	0.000	13:09
EXTERNAL STANDARD	0.081	13:09
BLANK TEST	0.000	13:10






Average = 0.0818
 Std Dev = 0.0004

*Lot AG335002
 Exp 12/18/25*

Tank 017

*COB
 1/17/24*

**Tank 017 Average: 0.082
 COB 2024.01.18**

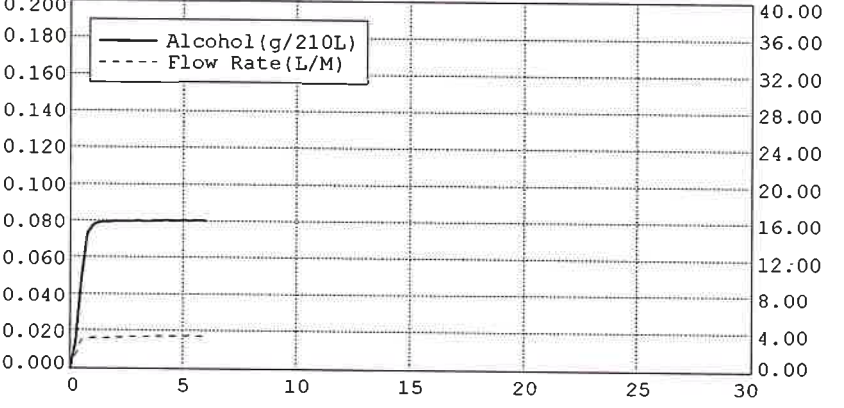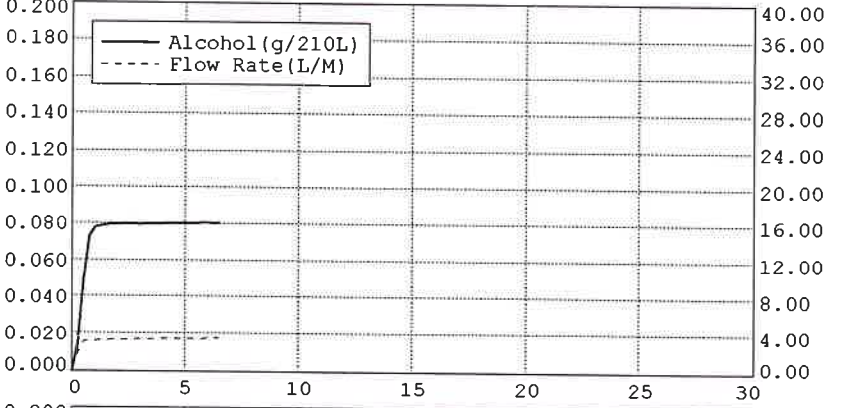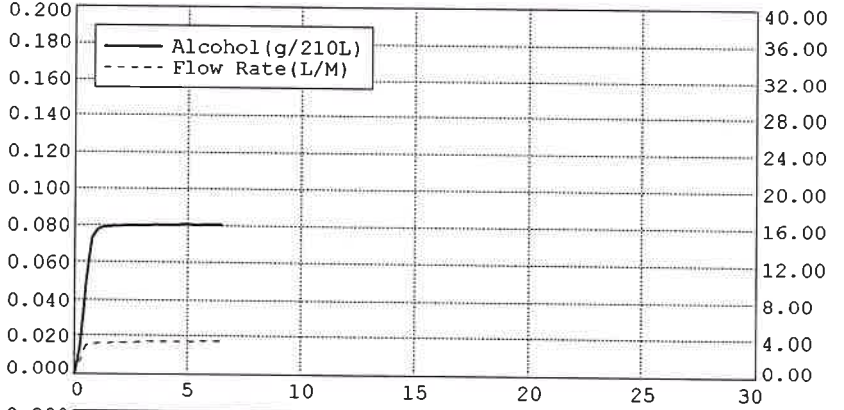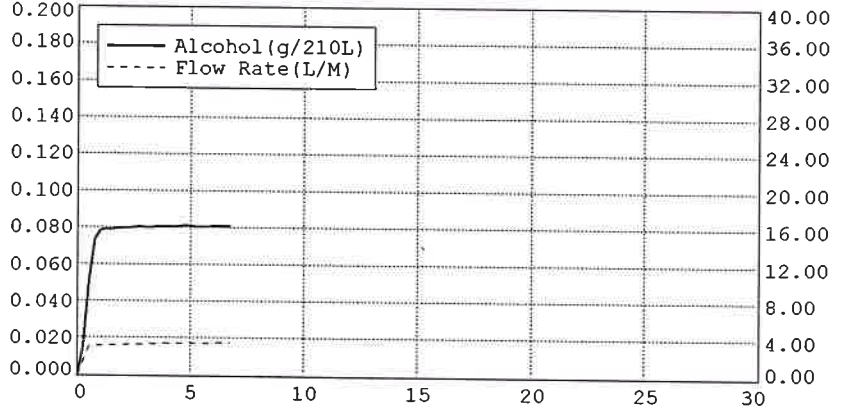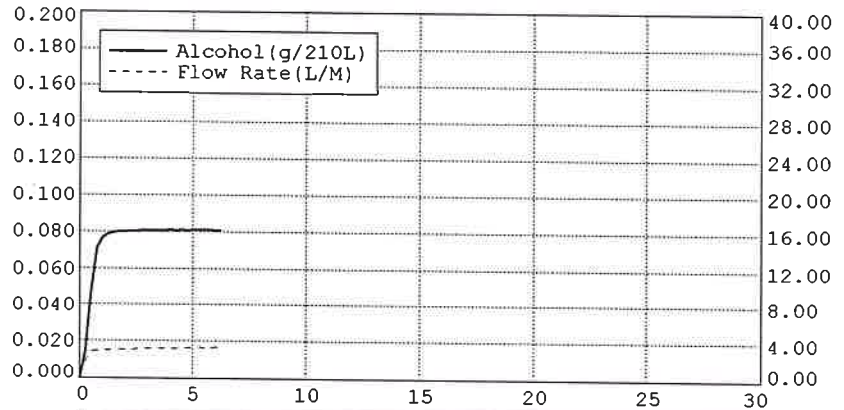

SUPERVISOR TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100397

Date: 01/17/2024
 Time: 12:52:23

SUPERVISOR NAME:
 COLLEEN S OBYRYANT
 OPERATOR'S #: 6237

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 30.25: 0.081
 TANK PRESSURE: 1217 psi






BLANK TEST	0.000	12:53
INTERNAL STANDARD	VERIFIED	12:53
EXTERNAL STANDARD	0.081	12:53
BLANK TEST	0.000	12:54
EXTERNAL STANDARD	0.081	12:54
BLANK TEST	0.000	12:55
EXTERNAL STANDARD	0.081	12:55
BLANK TEST	0.000	12:56
EXTERNAL STANDARD	0.081	12:57
BLANK TEST	0.000	12:57
EXTERNAL STANDARD	0.081	12:58
BLANK TEST	0.000	12:59

Average = 0.0810
 Std Dev = 0.0000

Lot A6335202
Exp 10/18/05

Tank 017

COB
1/17/24

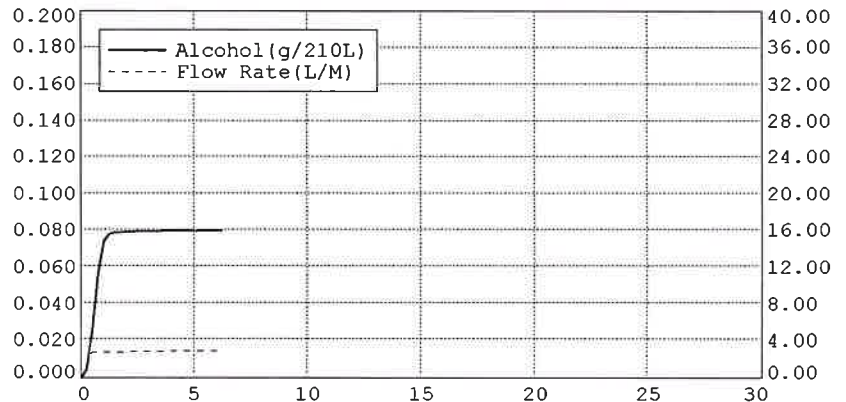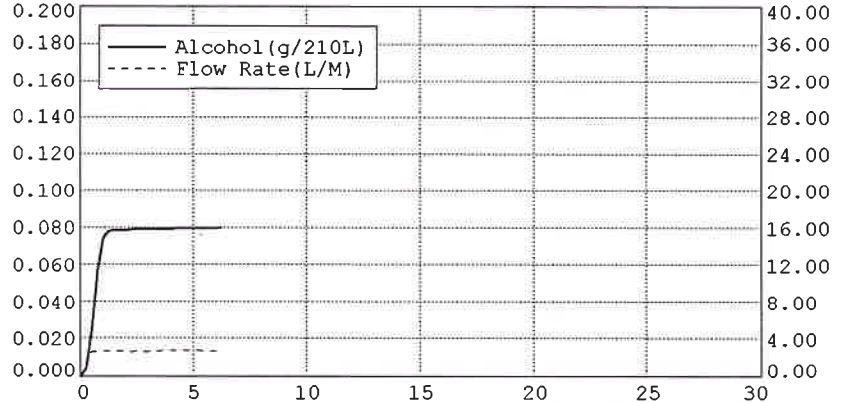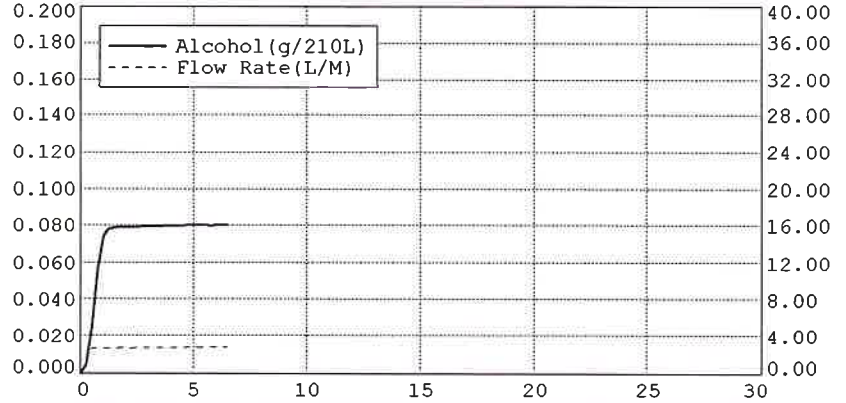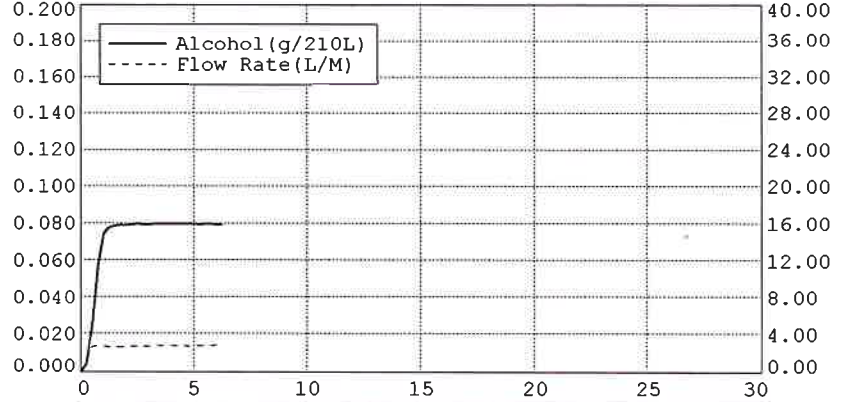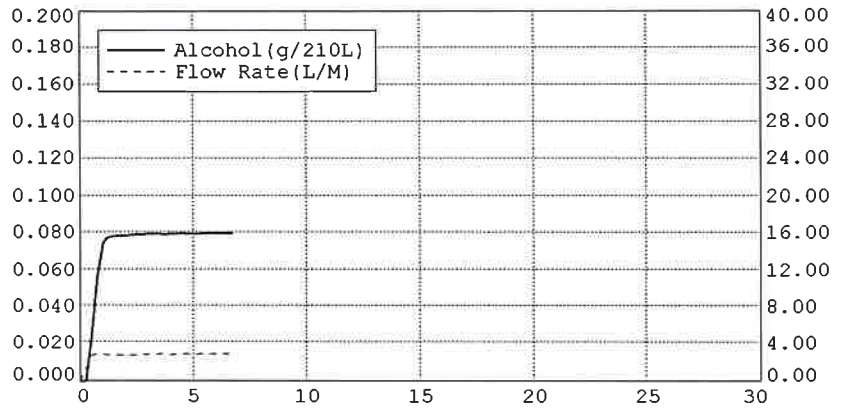

SUPERVISOR TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100399

Date: 01/17/2024
Time: 12:59:34

SUPERVISOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.23: 0.081
TANK PRESSURE: 1227 psi






BLANK TEST	0.000	13:00
INTERNAL STANDARD	VERIFIED	13:00
EXTERNAL STANDARD	0.084	13:01
BLANK TEST	0.000	13:02
EXTERNAL STANDARD	0.083	13:02
BLANK TEST	0.000	13:03
EXTERNAL STANDARD	0.083	13:03
BLANK TEST	0.000	13:04
EXTERNAL STANDARD	0.081	13:04
BLANK TEST	0.000	13:05
EXTERNAL STANDARD	0.081	13:05
BLANK TEST	0.000	13:06

Average = 0.0824
Std Dev = 0.0013

Lot AG335002
Exp 12/18/25

Tank 017

COB
1/17/24

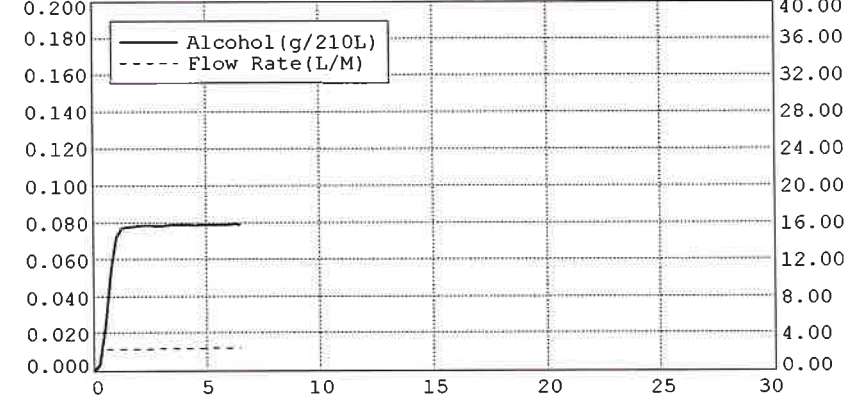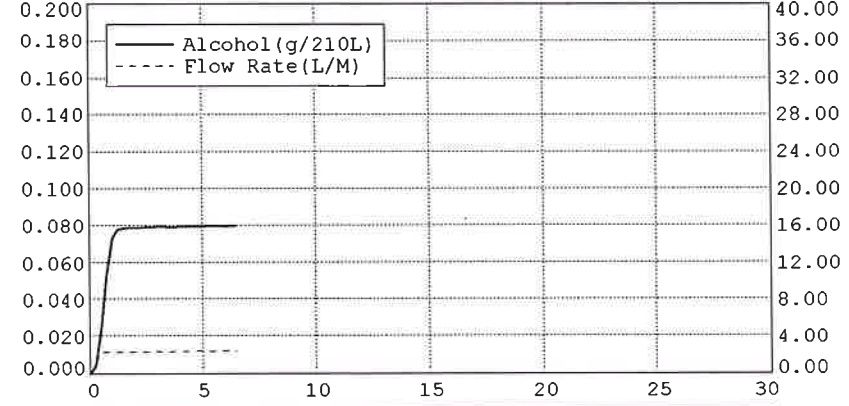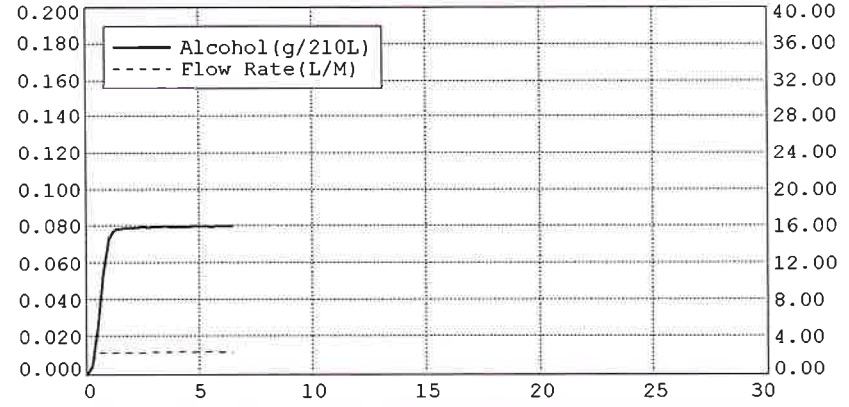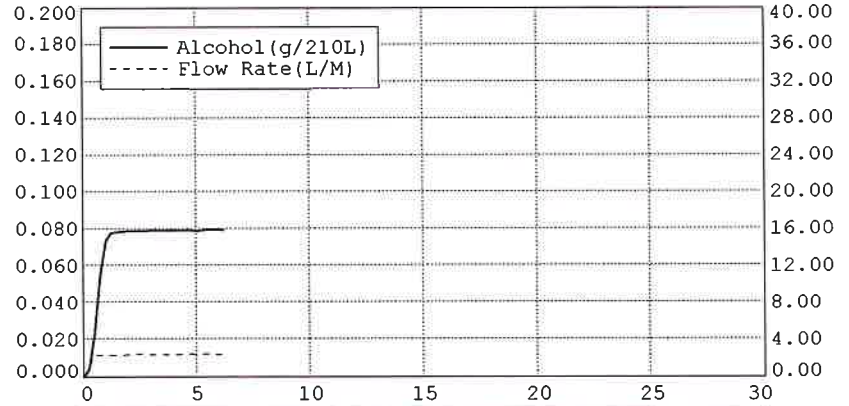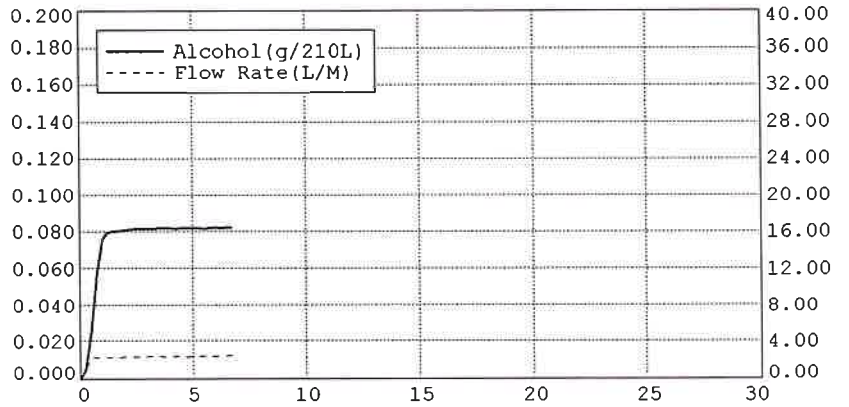

SUPERVISOR TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100375

Date: 01/17/2024
Time: 13:13:04

SUPERVISOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.24: 0.081
TANK PRESSURE: 1242 psi

BLANK TEST	0.000	13:14
INTERNAL STANDARD	VERIFIED	13:14
EXTERNAL STANDARD	0.082	13:14
BLANK TEST	0.000	13:15
EXTERNAL STANDARD	0.081	13:15
BLANK TEST	0.000	13:16
EXTERNAL STANDARD	0.081	13:16
BLANK TEST	0.000	13:17
EXTERNAL STANDARD	0.082	13:17
BLANK TEST	0.000	13:18
EXTERNAL STANDARD	0.082	13:18
BLANK TEST	0.000	13:19






Average = 0.0816
Std Dev = 0.0005

*Lot AG335002
Exp 12/18/25*

Tank 018

*COB
1/17/24*

**Tank 018 Average: 0.081
COB 2024.01.18**

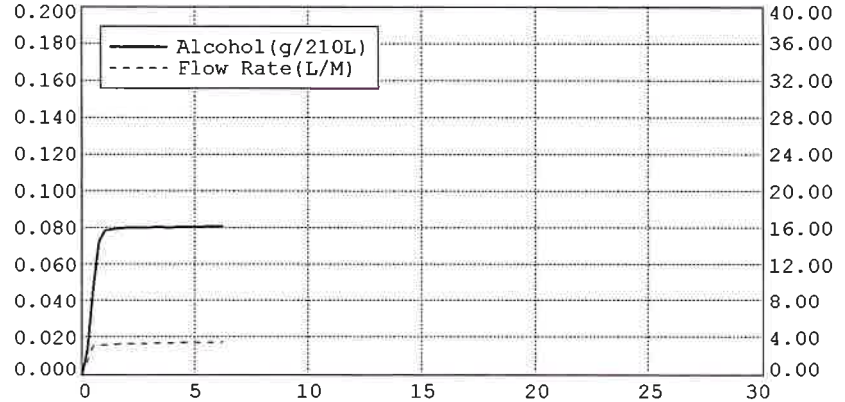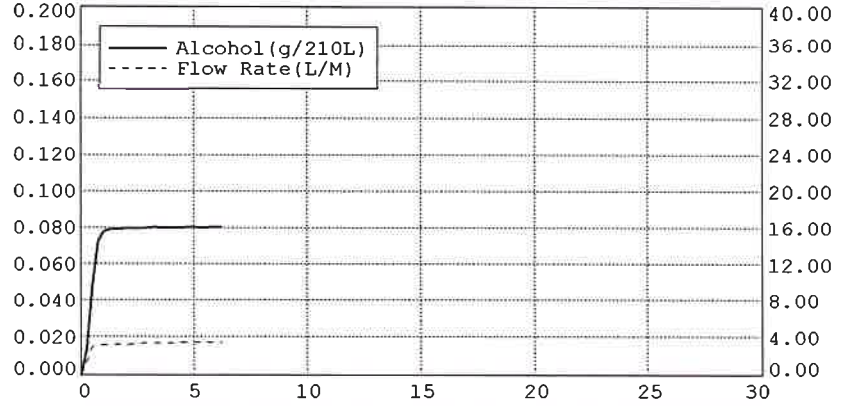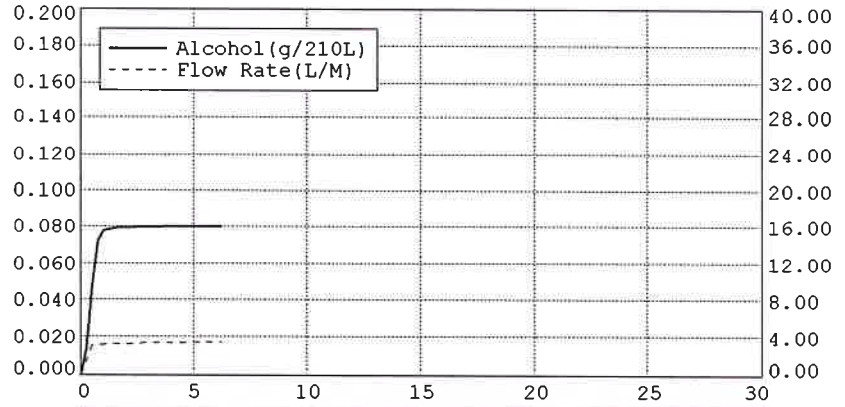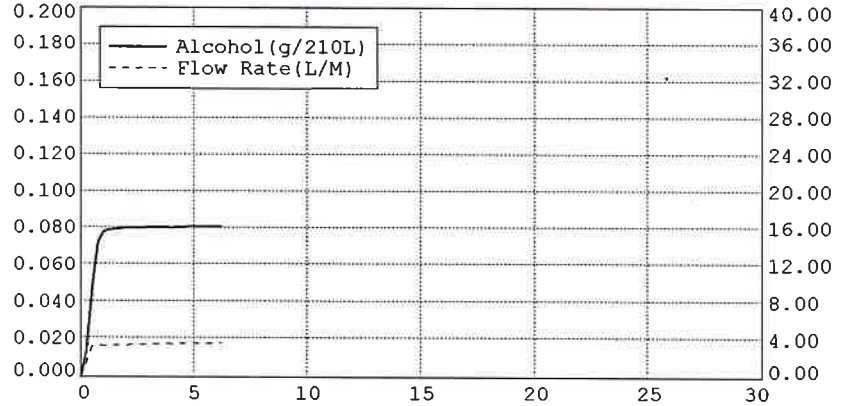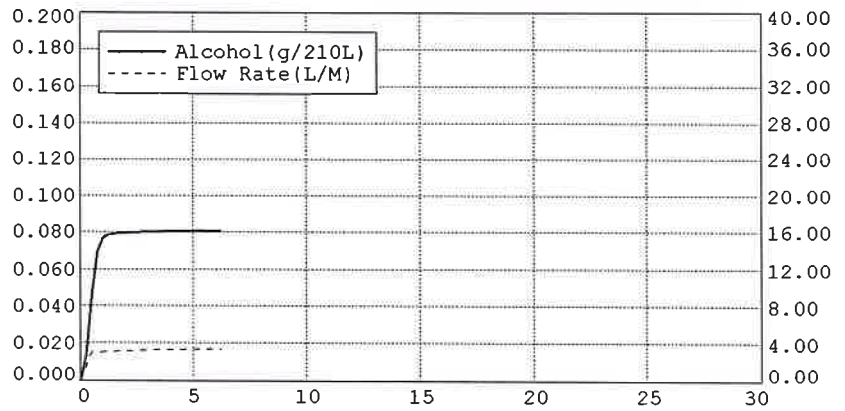

SUPERVISOR TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100397

Date: 01/17/2024
Time: 13:01:33

SUPERVISOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.24: 0.081
TANK PRESSURE: 1210 psi






BLANK TEST	0.000	13:02
INTERNAL STANDARD	VERIFIED	13:02
EXTERNAL STANDARD	0.080	13:02
BLANK TEST	0.000	13:03
EXTERNAL STANDARD	0.080	13:04
BLANK TEST	0.000	13:04
EXTERNAL STANDARD	0.081	13:05
BLANK TEST	0.000	13:06
EXTERNAL STANDARD	0.081	13:06
BLANK TEST	0.000	13:07
EXTERNAL STANDARD	0.081	13:07
BLANK TEST	0.000	13:08

Average = 0.0806
Std Dev = 0.0005

Lot AG385202
Exp 12/18/25

Tank 018

COB
1/17/24

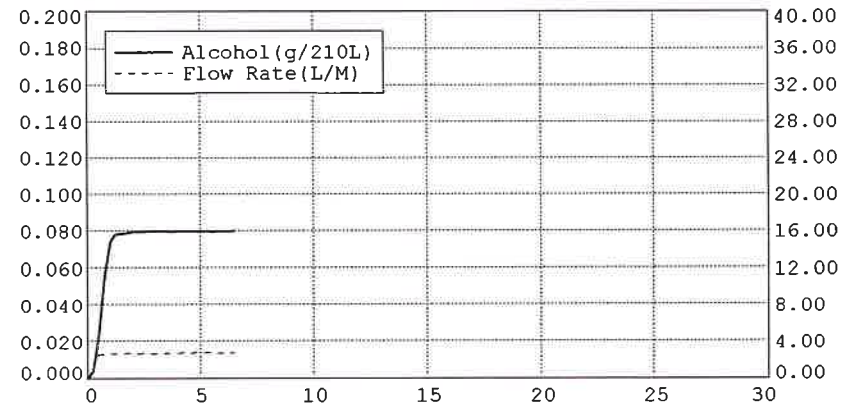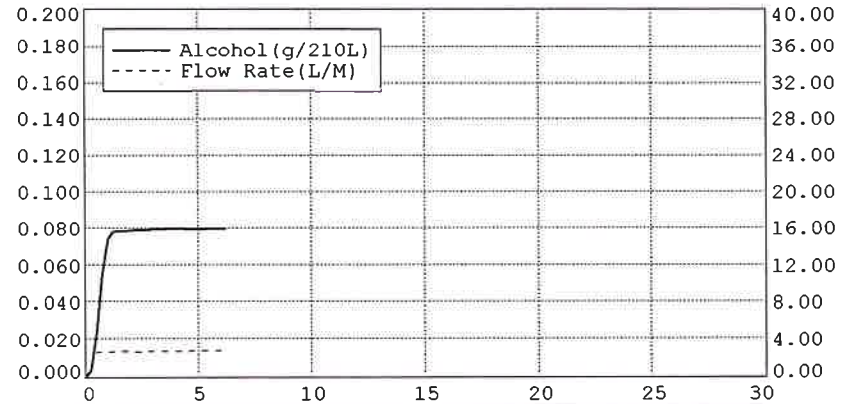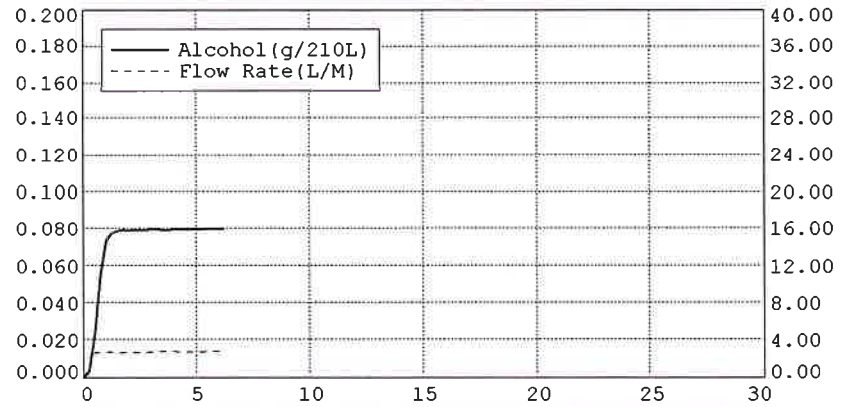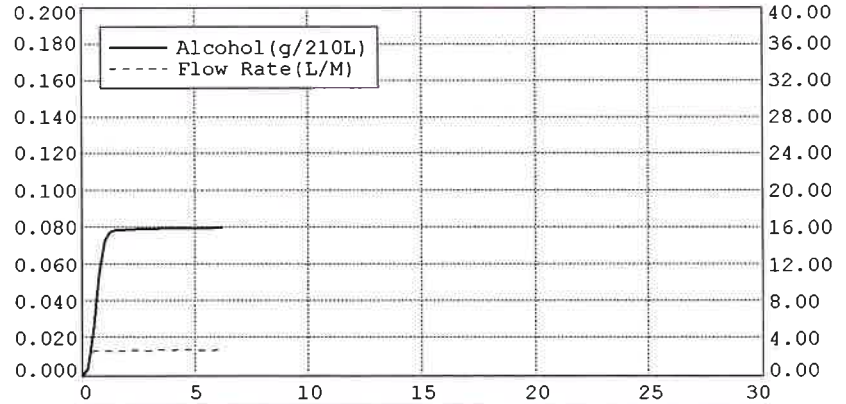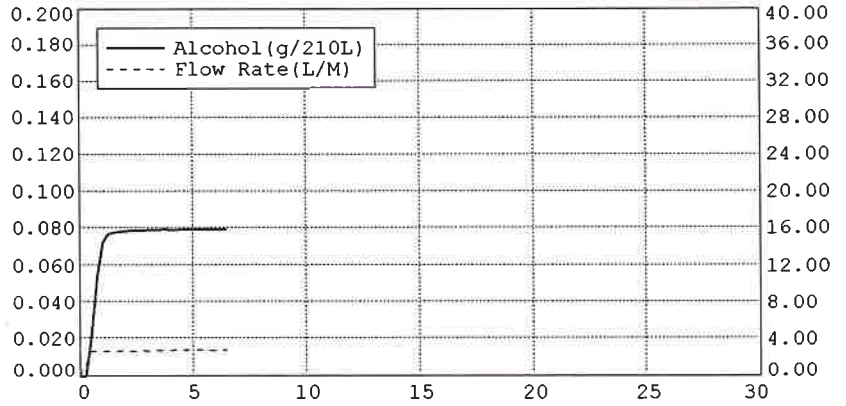

SUPERVISOR TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100399

Date: 01/17/2024
 Time: 13:17:59

SUPERVISOR NAME:
 COLLEEN S OBRYANT
 OPERATOR'S #: 6237

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 30.23: 0.081
 TANK PRESSURE: 1191 psi

BLANK TEST	0.000	13:21
INTERNAL STANDARD	VERIFIED	13:21
EXTERNAL STANDARD	0.082	13:21
BLANK TEST	0.000	13:22
EXTERNAL STANDARD	0.082	13:22
BLANK TEST	0.000	13:23
EXTERNAL STANDARD	0.081	13:23
BLANK TEST	0.000	13:24
EXTERNAL STANDARD	0.081	13:24
BLANK TEST	0.000	13:25
EXTERNAL STANDARD	0.083	13:26
BLANK TEST	0.000	13:26

Average = 0.0818
 Std Dev = 0.0008

AG 335200-20t
Exp 12/18/25

Tank 018

COB
1/17/24

