




State of Alaska  
Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
Anchorage, Alaska 99507  
David Kanaris, Chief, Forensic Laboratories



**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100349

**Report Issue Date:** 12/01/2025  
**Date Received:** 2025-10-13  
**Condition of Item:** No apparent damage

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

| As-Found Data              |                           |            |                  |       |       |       |       |                  |
|----------------------------|---------------------------|------------|------------------|-------|-------|-------|-------|------------------|
| Nominal Values<br>(g/210L) | Target Values<br>(g/210L) | Lot Number | Results (g/210L) |       |       |       |       | Mean<br>(g/210L) |
| 0.020                      | 0.020                     | AG408002   | 0.021            | 0.020 | 0.020 | 0.020 | 0.020 | 0.020            |
| 0.080                      | 0.078                     | AG335202   | 0.078            | 0.078 | 0.078 | 0.078 | 0.078 | 0.078            |
| 0.300                      | 0.293                     | AG427706   | 0.291            | 0.291 | 0.291 | 0.291 | 0.291 | 0.291            |

As Found - Evaluation Analyst: Colleen O'Bryant

As Found Conditions - Barometric Pressure (inHg): 29.45 Barometer Used: VWR S/N 240680771 Temperature (C): 21.4 Relative Humidity (%): 26

As-Found Lab Activity Date Range: 10/13/2025 - 10/15/2025

Removed from agency for lack of breath test operators.

| As-Left Data               |                           |            |                  |       |       |       |       |                  |                         |
|----------------------------|---------------------------|------------|------------------|-------|-------|-------|-------|------------------|-------------------------|
| Nominal Values<br>(g/210L) | Target Values<br>(g/210L) | Lot Number | Results (g/210L) |       |       |       |       | Mean<br>(g/210L) | Uncertainty<br>(g/210L) |
| 0.020                      | 0.020                     | AG408002   | 0.020            | 0.020 | 0.021 | 0.021 | 0.021 | 0.021            | +/- 0.002               |
| 0.040                      | 0.040                     | AG407908   | 0.040            | 0.040 | 0.040 | 0.040 | 0.040 | 0.040            | +/- 0.003               |
| 0.080                      | 0.080                     | AG335202   | 0.079            | 0.079 | 0.078 | 0.079 | 0.079 | 0.079            | +/- 0.004               |
| 0.100                      | 0.100                     | AG333401   | 0.099            | 0.099 | 0.099 | 0.099 | 0.099 | 0.099            | +/- 0.004               |
| 0.150                      | 0.150                     | AG515604   | 0.148            | 0.147 | 0.147 | 0.147 | 0.147 | 0.147            | +/- 0.006               |
| 0.300                      | 0.299                     | AG427706   | 0.297            | 0.297 | 0.297 | 0.298 | 0.297 | 0.297            | +/- 0.012               |

As Left Conditions - Barometric Pressure (inHg): 29.82 Barometer Used: VWR S/N 240680771 Temperature (C): 21.2 Relative Humidity (%): 7

As-Left Lab Activity Date Range: 11/24/2025 - 11/24/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Derek Walton on 11/24/2025

[derek.walton@alaska.gov](mailto:derek.walton@alaska.gov)

Technically and administratively reviewed by Carlie Glaister on 12/01/2025

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100549 Analyst or Technician Name: Derek Walton

DataMaster DMT Calibration Start Date: 11/24/2025

### Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value  $\leq$  3.00%

### Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer  
Barometer/Thermometer/Hygrometer S/N: 240680771  
Calibration Due Date: 09/10/26
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

### Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 29.82 Temperature(C) 21.2 Relative Humidity(%) 7

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Interference (Volatiles) - *Print with View Details*
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20250922K5 Expiration Date: 12/22/25  
Simulator S/N: DR4178 Thermometer Verification Performed? ☒
2. Isopropanol Reagent Lot Number: 20250922K5 Expiration Date: 12/22/25  
Simulator S/N: DR4177 Thermometer Verification Performed? ☒
3. Negative (Ethanol Only) Lot Number: 25CP41280 Expiration Date: 12/22/25  
Simulator S/N: DR4163 Thermometer Verification Performed? ☒

Solution  
03/19/27

Calibrated External Thermometer S/N: 250159297

Calibration Due Date: 03/14/2027

### Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

### Completion

Lab Work End Date: 11/24/25

Data Interpretation Date (Technician): \_\_\_\_\_ (if applicable)

Data Interpretation Date (Analyst): 11/24/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

# DIAGNOSTIC RECORD

Alaska Department of Public Safety  
DATAMASTER dmt: 100349

Date: 11/24/2025  
Time: 09:05:39

## VERSIONS

DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

## TEMPERATURES

|                         |        |
|-------------------------|--------|
| Sample Chamber = 48.7°C | PASSED |
| (44.0°C - 52.0°C)       |        |
| Breath Tube = 46.9°C    | PASSED |
| (38.0°C - 50.0°C)       |        |

## SETTINGS

|                         |        |
|-------------------------|--------|
| Lamp Voltage = 1.75 V   | PASSED |
| (1.05 V - 2.45 V)       |        |
| Cooler Voltage = 1.73 V | PASSED |
| (1.04 V - 2.42 V)       |        |
| Bias Voltage = 80 V     | PASSED |
| (48 V - 112 V)          |        |
| Chopper Freq = 527 Hz   | PASSED |
| (475 Hz - 575 Hz)       |        |
| Barometer = 29.6 in     |        |

## PUMP INFO

|                         |        |
|-------------------------|--------|
| Flow Rate = 4.588 L/M   | PASSED |
| (3.500 L/M - 6.500 L/M) |        |

## DETECTOR INFO

|                      |        |
|----------------------|--------|
| PUMP ON              | PASSED |
| (0.002 V <= 0.010 V) |        |
| PUMP OFF             | PASSED |
| (0.002 V <= 0.010 V) |        |

## FILTER INFO

|          |        |
|----------|--------|
| Filter 1 | PASSED |
| Filter 2 | PASSED |
| Filter 3 | PASSED |

## INTERNAL STANDARD

|                  |        |
|------------------|--------|
| Xq = 0.079 1.34% | PASSED |
| (0.00% - 4.00%)  |        |

# Technician Screen

-----  
DATAMASTER dmt: 100349  
-----

Date: 11/24/2025  
Time: 9:13 AM

Temperatures (°C)  
Sample Cell: 48.8°C  
Breath Tube: 46.4°C

Current Barometer 29.8 in  
Volume (Ltr) 1.52 ✓

Settings  
Lamp: 1.75 V  
Bias: 80 V  
Cooler: 1.73 V  
Chopper: 526 Hz

Voltages (V)  
Flow: 1.05 V  
Detector: -0.028 V ✓

# CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100349  
-----

Date: 04/29/2024  
Time: 12:41:52

OPERATOR NAME:  
KAIJA SWISHER  
CERTIFICATE #: 10746

|     |   |          |        |                |
|-----|---|----------|--------|----------------|
| Ca  | = | 0.1000   |        |                |
| CAL | = | 0.980299 | 0.800  | <= CAL < 1.200 |
| b1  | = | 0.0005   | 0.0000 | <= b1 < 0.0040 |
| b2  | = | 0.0057   | 0.0010 | <= b2 < 0.0100 |
| b3  | = | 0.0009   | 0.0000 | <= b3 < 0.0040 |
| Xq  | = | 0.0777   | 0.0500 | <= Xq < 0.2000 |
| a21 | = | 1.191043 | 1.050  | <= a21 < 1.300 |
| a31 | = | 0.569042 | 0.300  | <= a31 < 0.800 |

# SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100349

Date: 11/24/2025

Time: 09:18:26

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

DEREK WALTON

OPERATOR'S #: 9508

DEPT/AGENCY:

MINIMUM VOLUME

CASE/REPORT: XXXX

TEST TYPE: TEST

## EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080


TARGET AT 29.82: 0.080

LOT #: AG335202

EXPIRATION: 12/18/2025

|                            |          |       |
|----------------------------|----------|-------|
| DIAGNOSTIC CHECK           | PASSED   | 09:19 |
| BLANK TEST                 | 0.000    | 09:19 |
| INTERNAL STANDARD          | VERIFIED | 09:19 |
| EXTERNAL STANDARD          | 0.079    | 09:19 |
| BLANK TEST                 | 0.000    | 09:20 |
| SUBJECT SAMPLE (Vol=1.52L) | 0.000    | 09:21 |
| BLANK TEST                 | 0.000    | 09:22 |
| EXTERNAL STANDARD          | 0.079    | 09:22 |
| BLANK TEST                 | 0.000    | 09:23 |

*[Handwritten signature]*

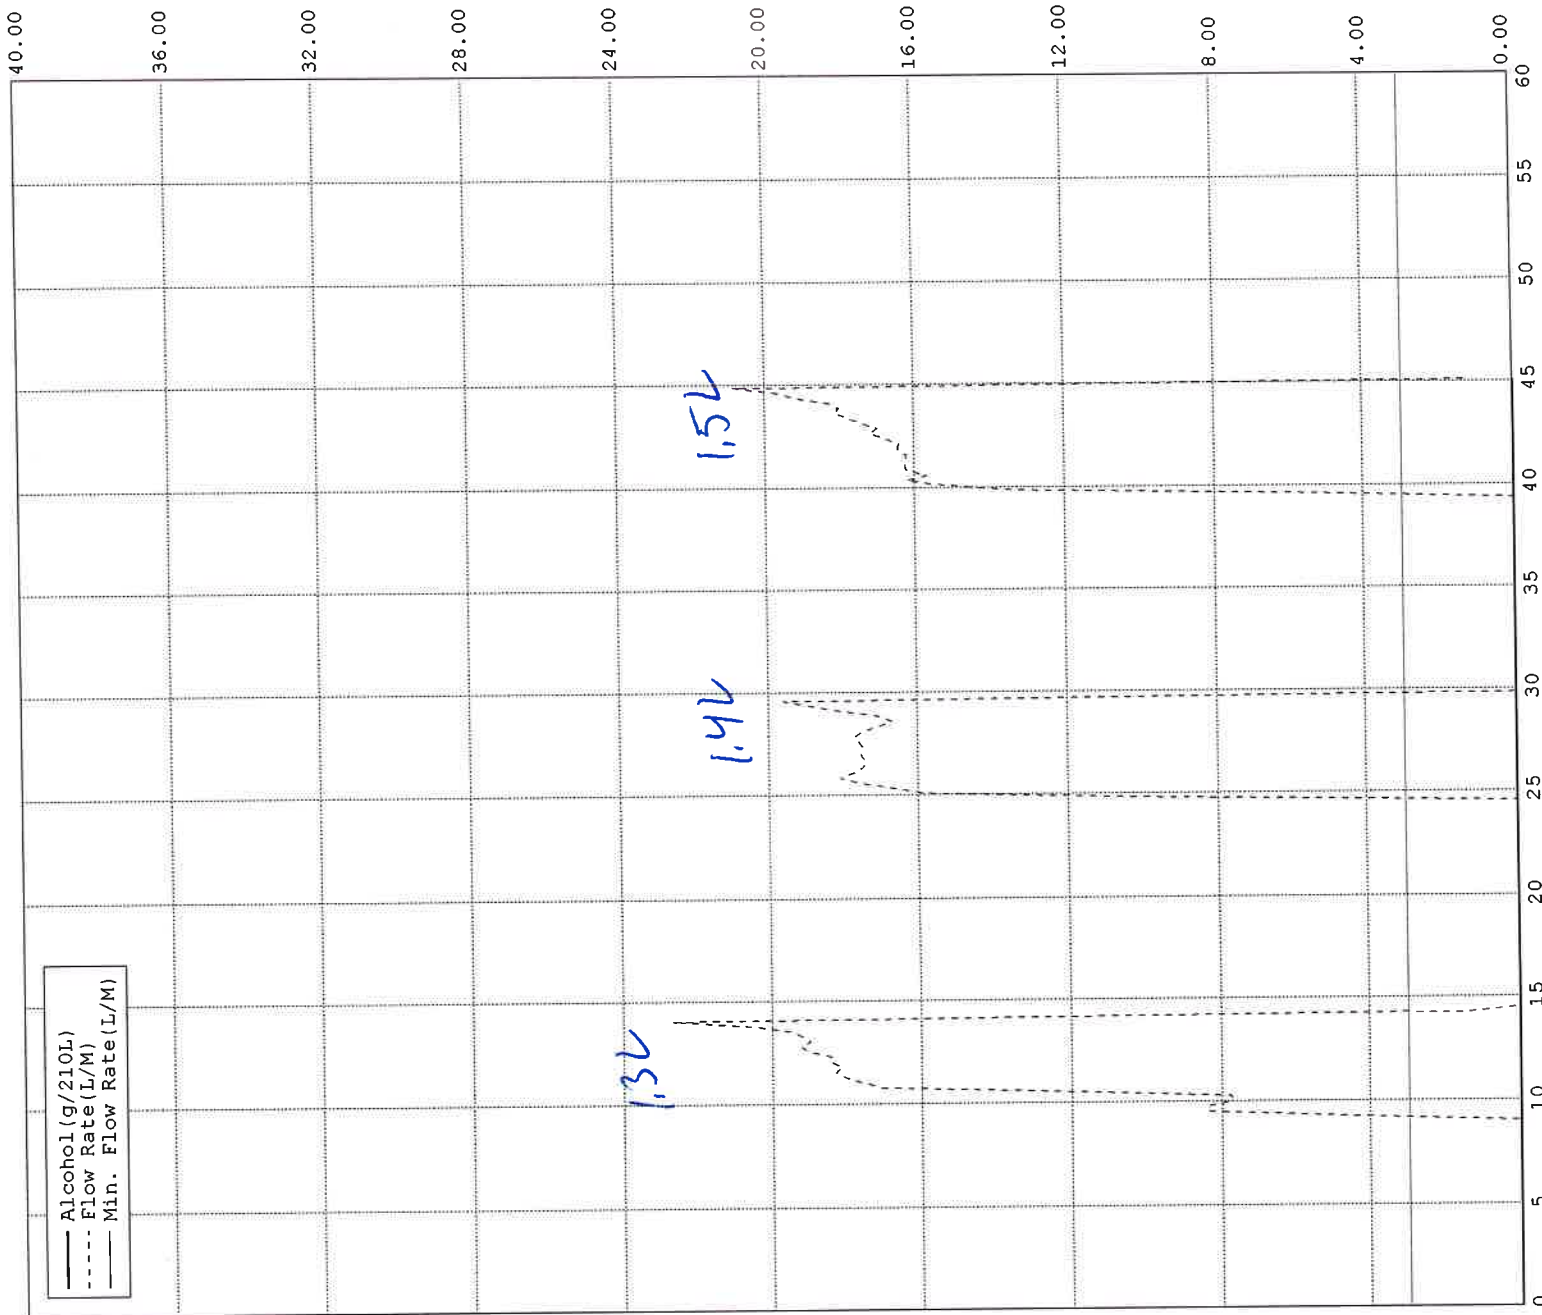

# LINEARITY CHECK


Alaska Department of Public Safety  
 DATAMASTER dmt: 100349

Date: 11/24/2025  
 Time: 09:27:55

SUPERVISOR NAME:  
 DEREK WALTON  
 OPERATOR'S #: 9508

| TARGET | AVERAGE | STD. DEV. |
|--------|---------|-----------|
| 0.020  | 0.0206  | 0.0005    |
| 0.040  | 0.0400  | 0.0000    |
| 0.080  | 0.0788  | 0.0004    |
| 0.100  | 0.0990  | 0.0000    |
| 0.150  | 0.1472  | 0.0004    |
| 0.299  | 0.2972  | 0.0004    |

SLOPE = 0.991594  
 R<sup>2</sup> = 0.999923

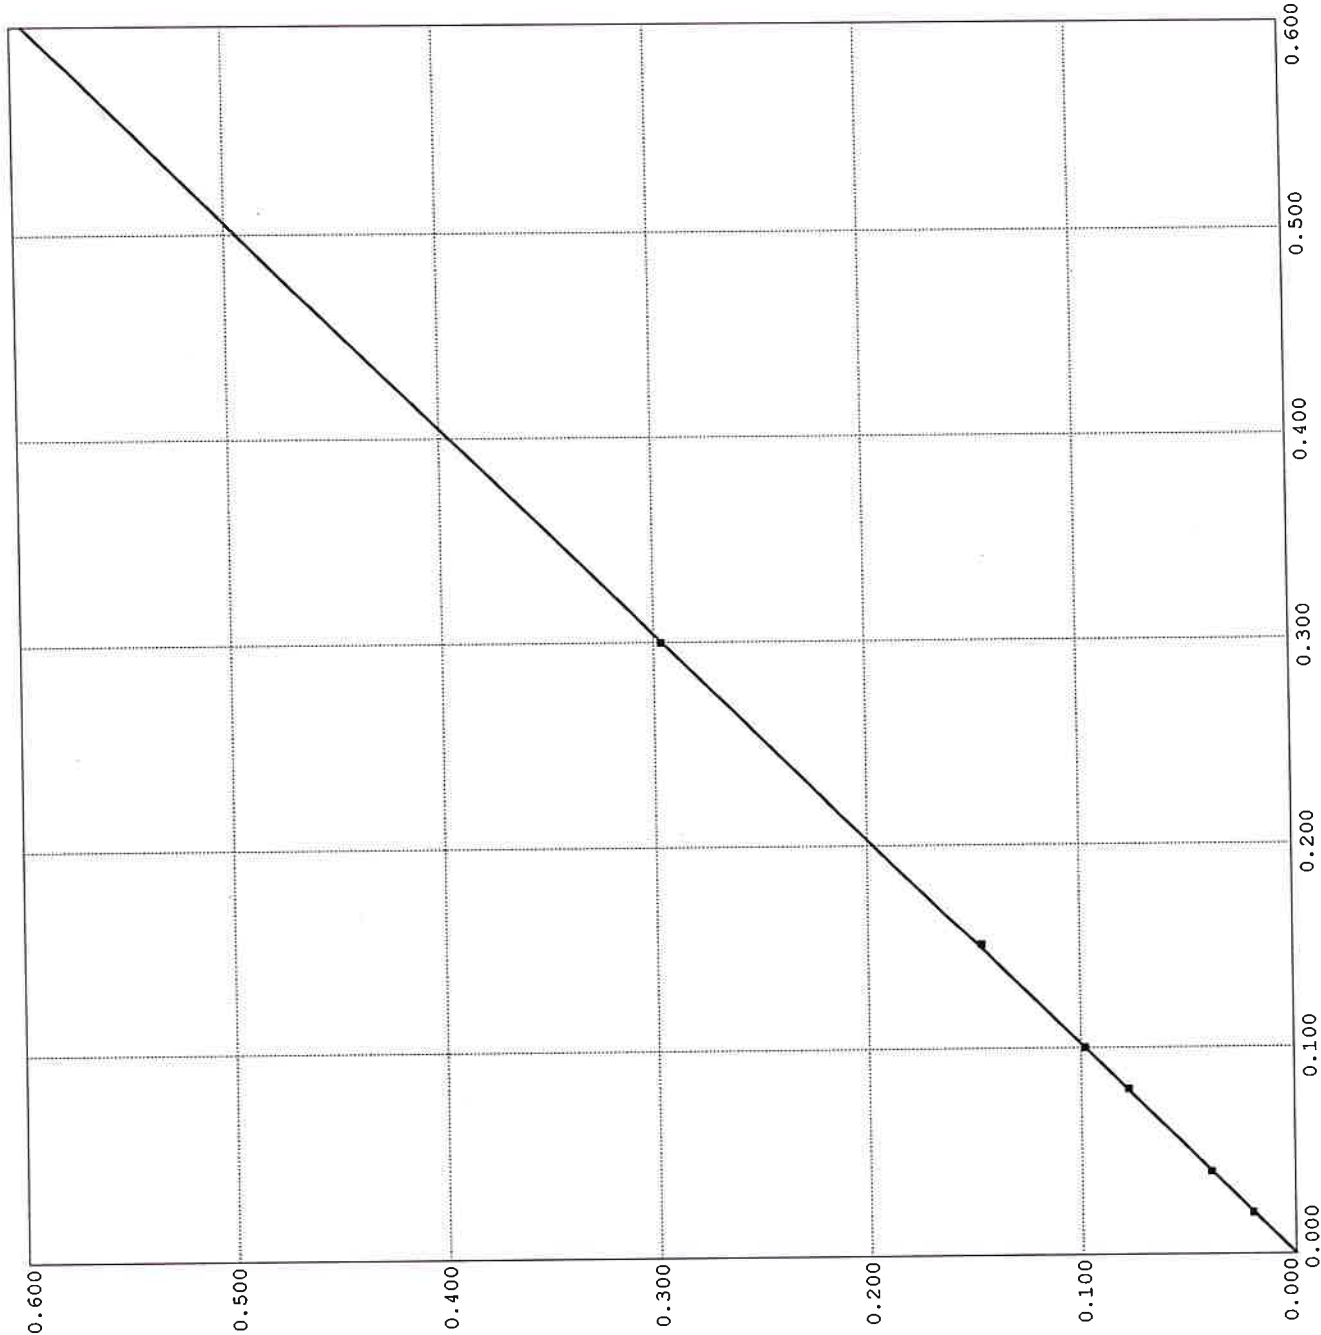

*DM*

# LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100349






Date: 11/24/2025  
Time: 09:27:58

## EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 29.81: 0.020  
LOT #: AG408002  
EXPIRATION: 03/20/2026  
TANK PRESSURE: 254 psi

|                   |          |       |
|-------------------|----------|-------|
| BLANK TEST        | 0.000    | 10:03 |
| INTERNAL STANDARD | VERIFIED | 10:03 |
| EXTERNAL STANDARD | 0.020    | 10:03 |
| BLANK TEST        | 0.000    | 10:04 |
| EXTERNAL STANDARD | 0.020    | 10:04 |
| BLANK TEST        | 0.000    | 10:05 |
| EXTERNAL STANDARD | 0.021    | 10:05 |
| BLANK TEST        | 0.000    | 10:06 |
| EXTERNAL STANDARD | 0.021    | 10:06 |
| BLANK TEST        | 0.000    | 10:07 |
| EXTERNAL STANDARD | 0.021    | 10:07 |
| BLANK TEST        | 0.000    | 10:08 |

Average = 0.0206  
Std Dev = 0.0005

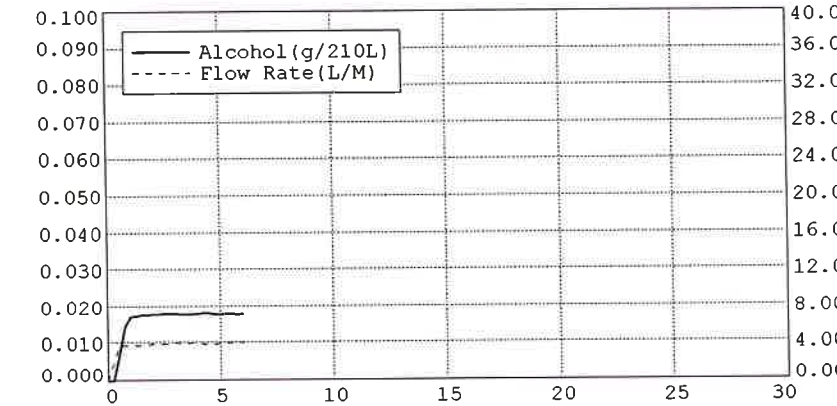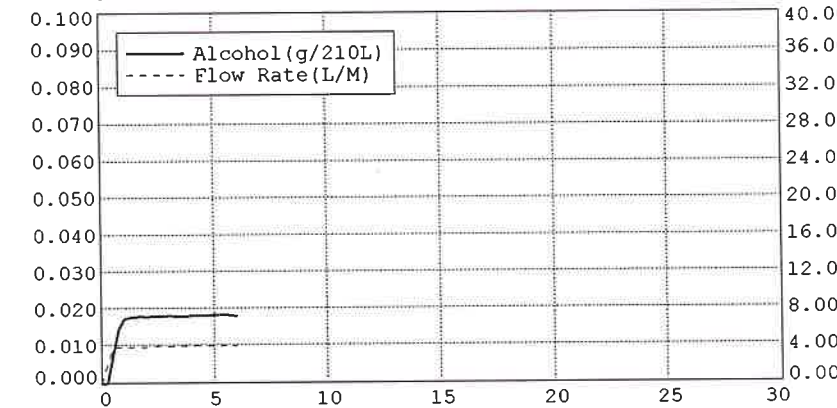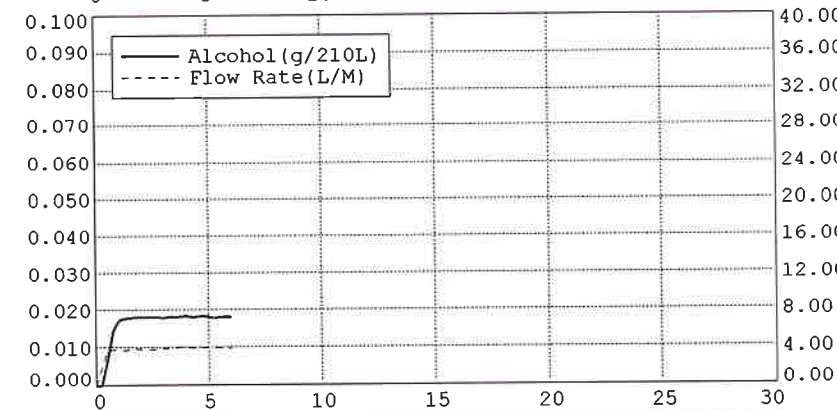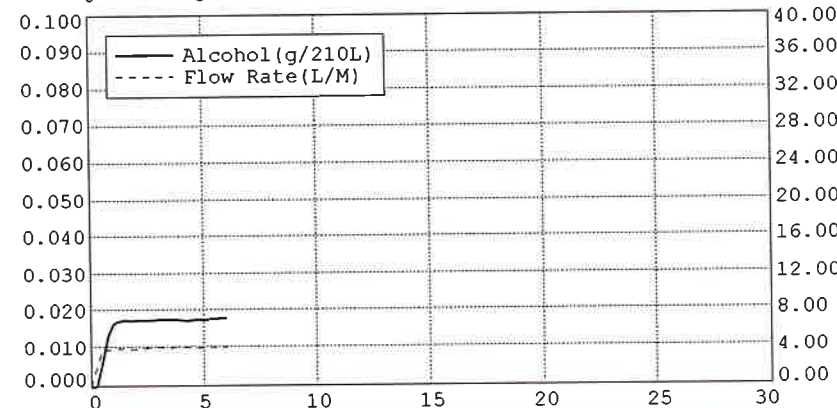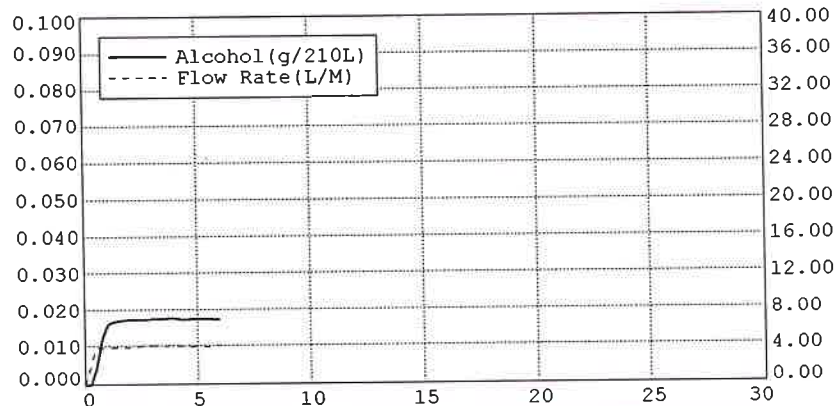

# LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
DATAMASTER dmt: 100349






Date: 11/24/2025  
Time: 10:10:25

## EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
TARGET AT 29.81: 0.040  
LOT #: AG407908  
EXPIRATION: 03/19/2026  
TANK PRESSURE: 571 psi

|                   |          |       |
|-------------------|----------|-------|
| BLANK TEST        | 0.000    | 10:11 |
| INTERNAL STANDARD | VERIFIED | 10:12 |
| EXTERNAL STANDARD | 0.040    | 10:12 |
| BLANK TEST        | 0.000    | 10:13 |
| EXTERNAL STANDARD | 0.040    | 10:13 |
| BLANK TEST        | 0.000    | 10:14 |
| EXTERNAL STANDARD | 0.040    | 10:14 |
| BLANK TEST        | 0.000    | 10:15 |
| EXTERNAL STANDARD | 0.040    | 10:15 |
| BLANK TEST        | 0.000    | 10:16 |
| EXTERNAL STANDARD | 0.040    | 10:16 |
| BLANK TEST        | 0.000    | 10:17 |

Average = 0.0400  
Std Dev = 0.0000

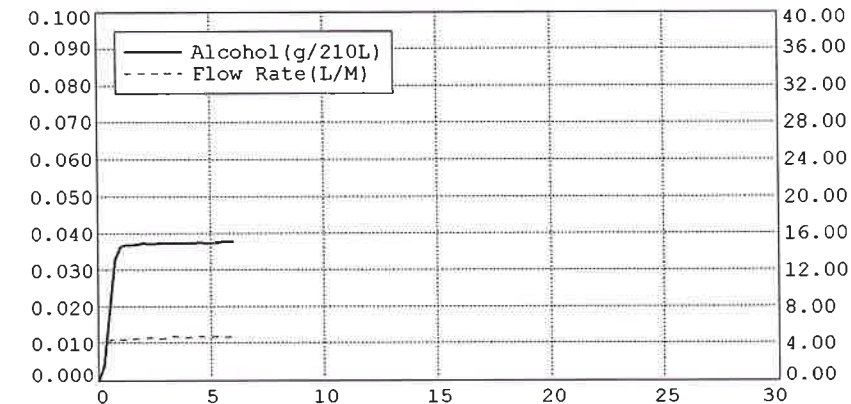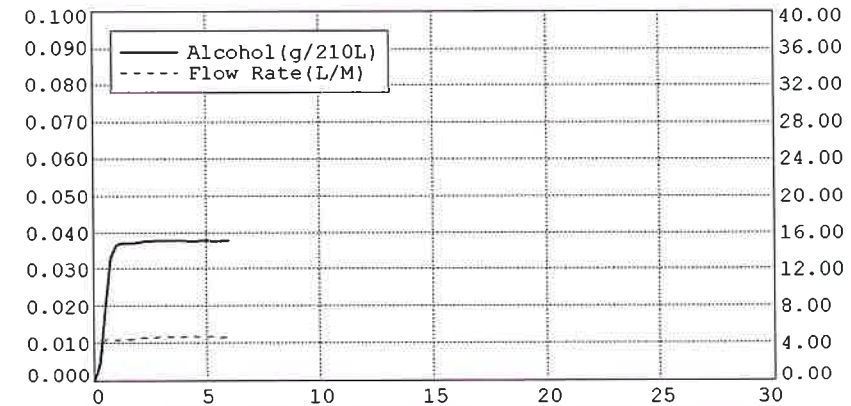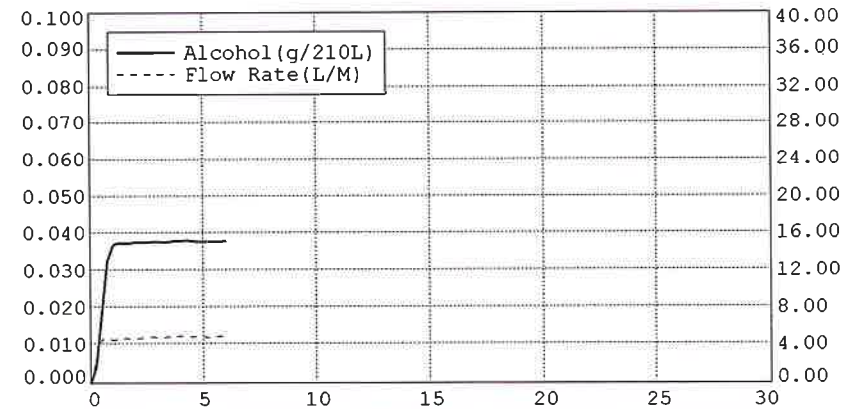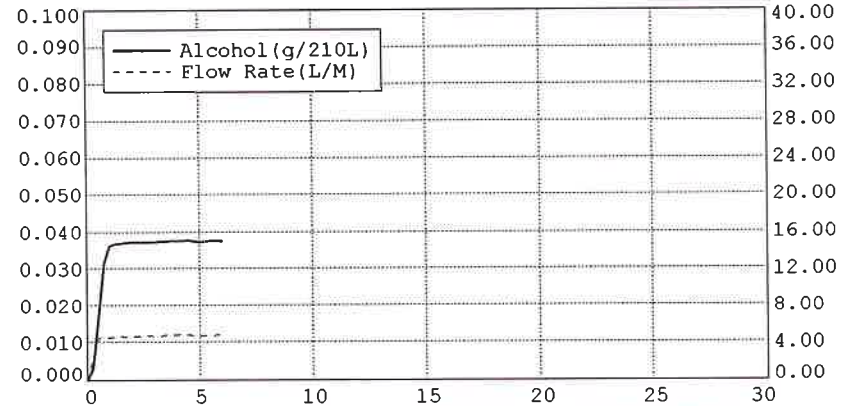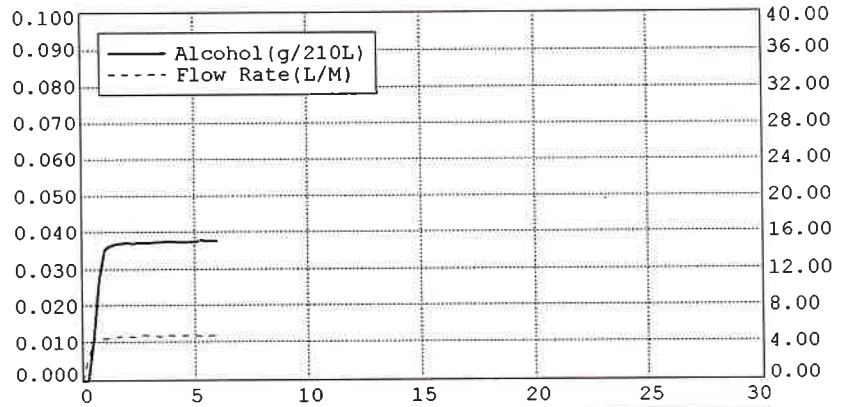

# LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
DATAMASTER dmt: 100349






Date: 11/24/2025  
Time: 10:19:12

## EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.81: 0.080  
LOT #: AG335202  
EXPIRATION: 12/18/2025  
TANK PRESSURE: 482 psi

|                   |          |       |
|-------------------|----------|-------|
| BLANK TEST        | 0.000    | 10:20 |
| INTERNAL STANDARD | VERIFIED | 10:20 |
| EXTERNAL STANDARD | 0.079    | 10:20 |
| BLANK TEST        | 0.000    | 10:21 |
| EXTERNAL STANDARD | 0.079    | 10:21 |
| BLANK TEST        | 0.000    | 10:22 |
| EXTERNAL STANDARD | 0.078    | 10:23 |
| BLANK TEST        | 0.000    | 10:23 |
| EXTERNAL STANDARD | 0.079    | 10:24 |
| BLANK TEST        | 0.000    | 10:25 |
| EXTERNAL STANDARD | 0.079    | 10:25 |
| BLANK TEST        | 0.000    | 10:26 |

Average = 0.0788  
Std Dev = 0.0004

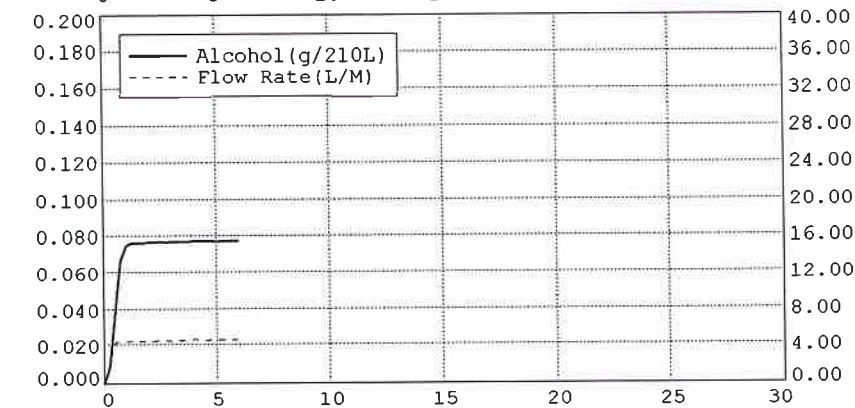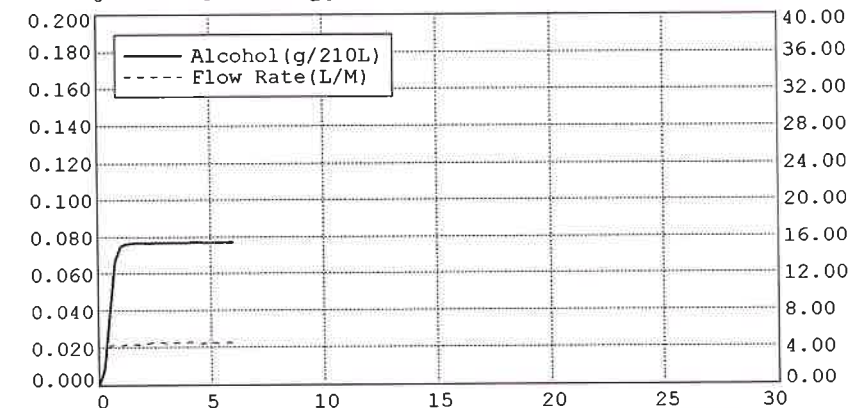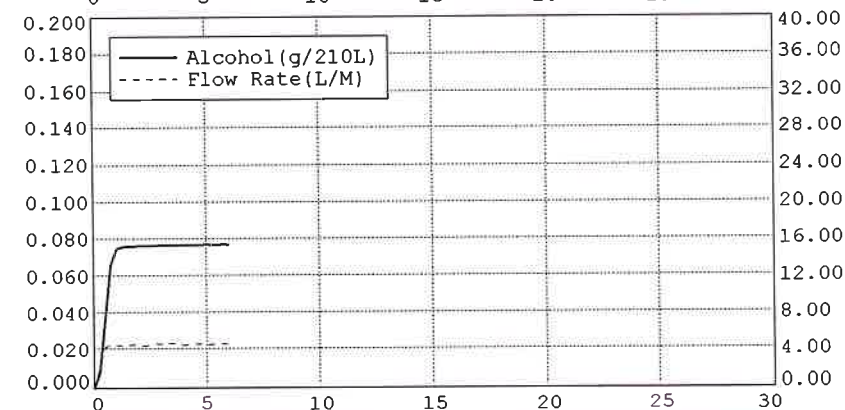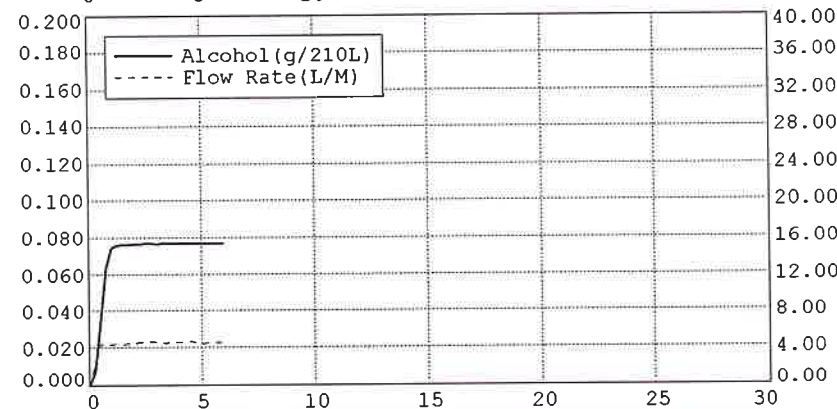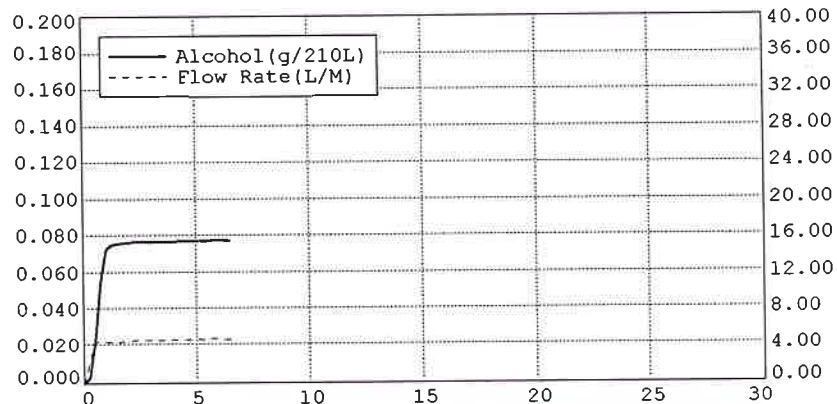

# LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
DATAMASTER dmt: 100349






Date: 11/24/2025  
Time: 10:27:41

## EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
TARGET AT 29.82: 0.100  
LOT #: AG333401  
EXPIRATION: 11/30/2025  
TANK PRESSURE: 805 psi

|                   |          |       |
|-------------------|----------|-------|
| BLANK TEST        | 0.000    | 10:28 |
| INTERNAL STANDARD | VERIFIED | 10:29 |
| EXTERNAL STANDARD | 0.099    | 10:29 |
| BLANK TEST        | 0.000    | 10:30 |
| EXTERNAL STANDARD | 0.099    | 10:30 |
| BLANK TEST        | 0.000    | 10:31 |
| EXTERNAL STANDARD | 0.099    | 10:31 |
| BLANK TEST        | 0.000    | 10:32 |
| EXTERNAL STANDARD | 0.099    | 10:32 |
| BLANK TEST        | 0.000    | 10:33 |
| EXTERNAL STANDARD | 0.099    | 10:33 |
| BLANK TEST        | 0.000    | 10:34 |

Average = 0.0990  
Std Dev = 0.0000

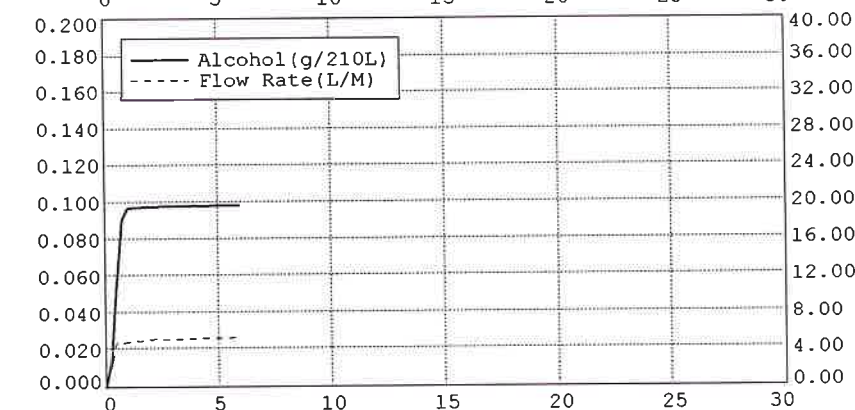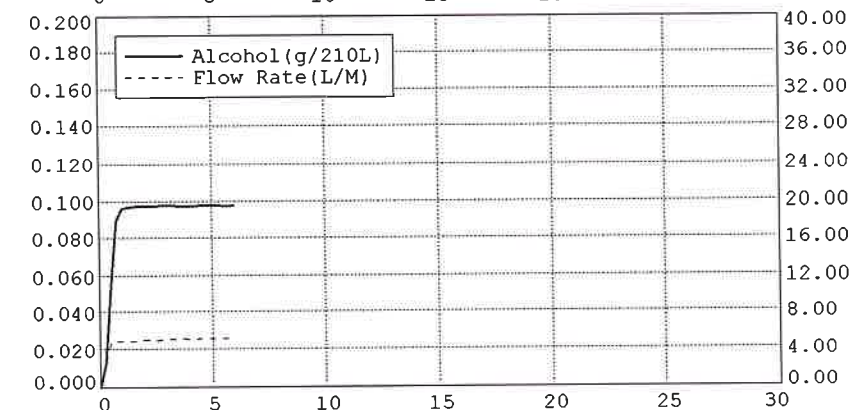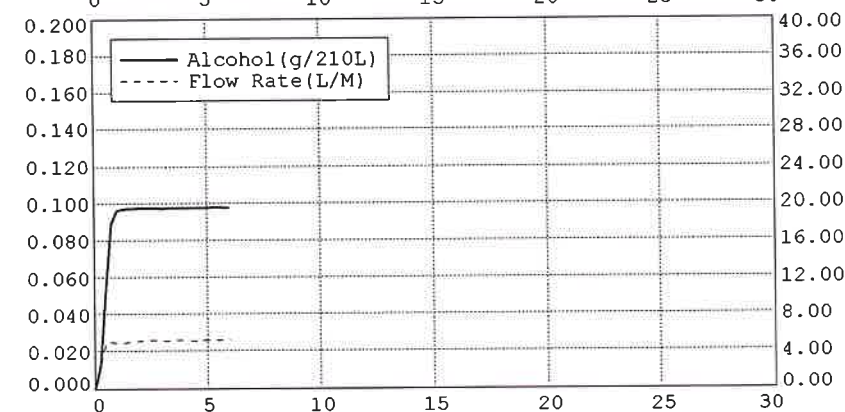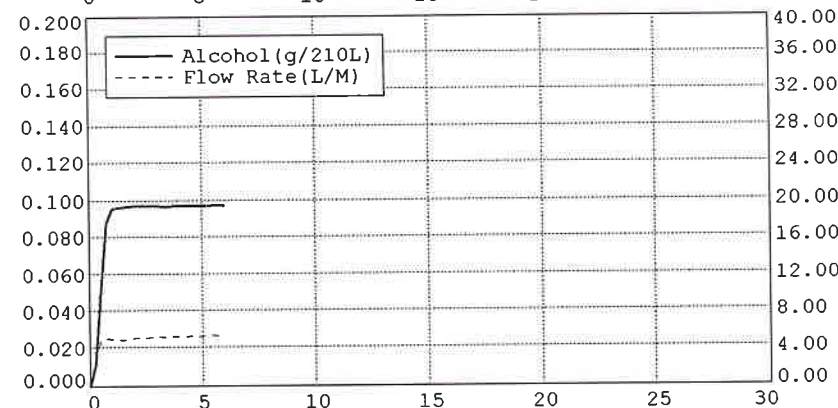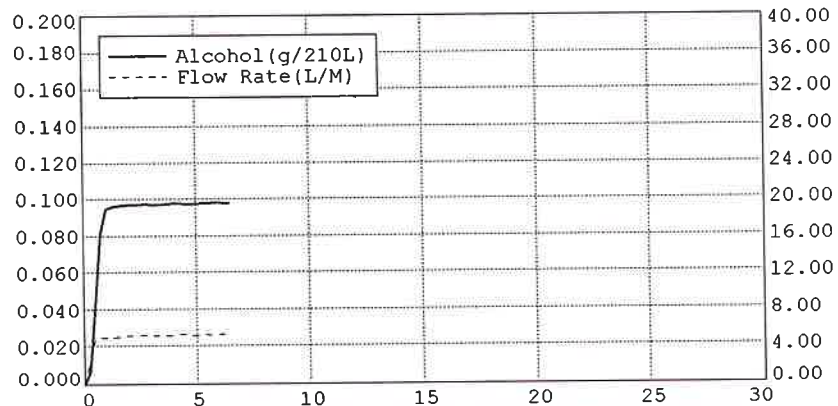

# LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
DATAMASTER dmt: 100349






Date: 11/24/2025  
Time: 10:37:27

## EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
TARGET AT 29.83: 0.150  
LOT #: AG515604  
EXPIRATION: 06/05/2027  
TANK PRESSURE: 692 psi

|                   |          |       |
|-------------------|----------|-------|
| BLANK TEST        | 0.000    | 10:38 |
| INTERNAL STANDARD | VERIFIED | 10:38 |
| EXTERNAL STANDARD | 0.148    | 10:39 |
| BLANK TEST        | 0.000    | 10:40 |
| EXTERNAL STANDARD | 0.147    | 10:40 |
| BLANK TEST        | 0.000    | 10:41 |
| EXTERNAL STANDARD | 0.147    | 10:41 |
| BLANK TEST        | 0.000    | 10:42 |
| EXTERNAL STANDARD | 0.147    | 10:42 |
| BLANK TEST        | 0.000    | 10:43 |
| EXTERNAL STANDARD | 0.147    | 10:43 |
| BLANK TEST        | 0.000    | 10:44 |

Average = 0.1472  
Std Dev = 0.0004

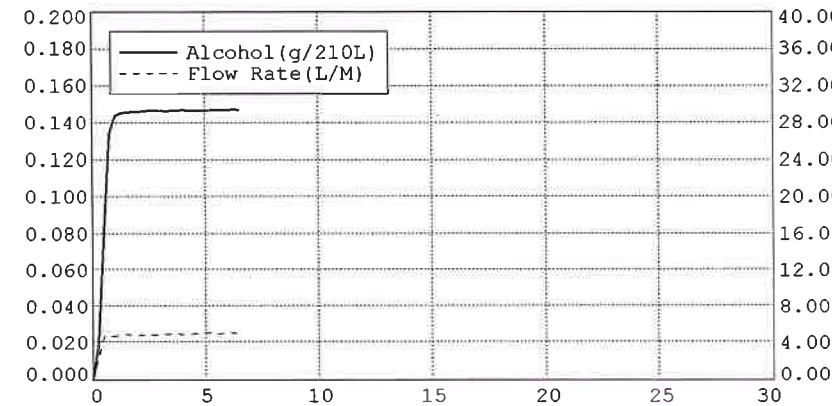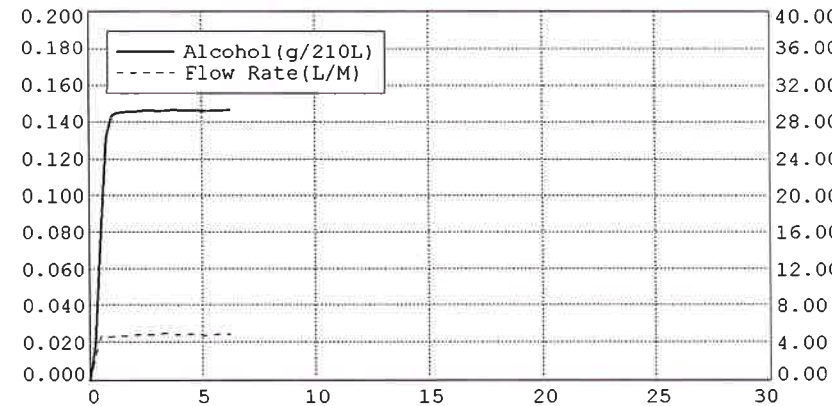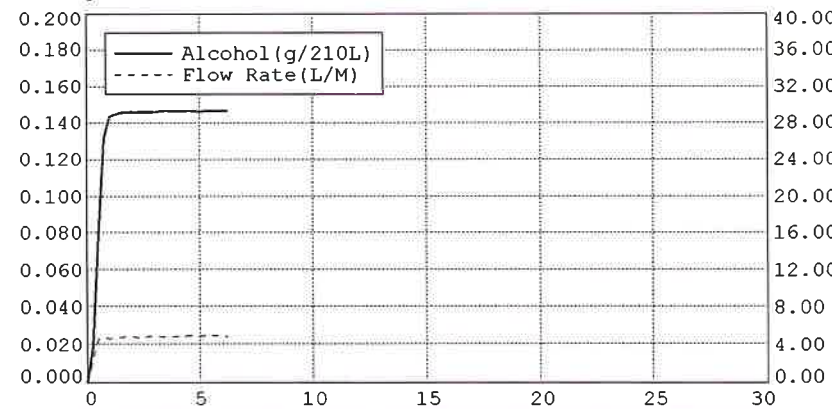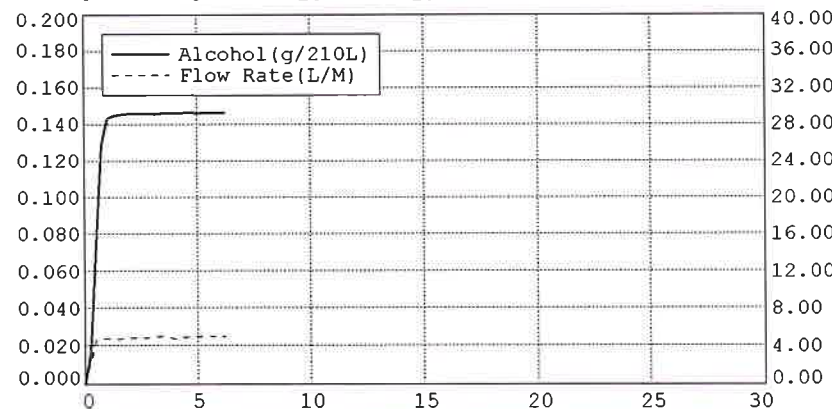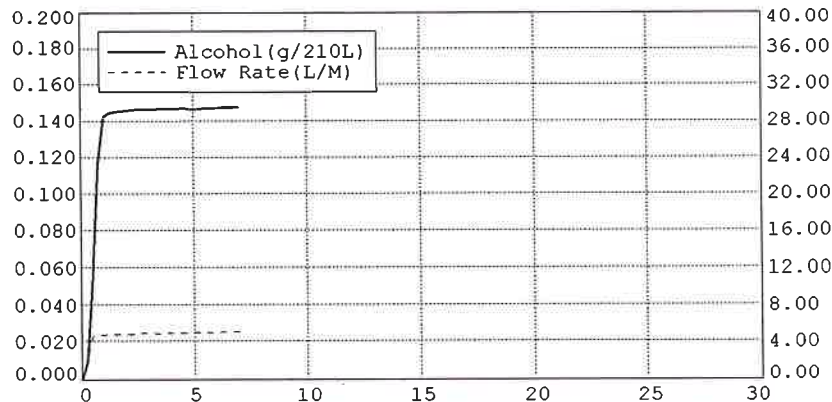

# LINEARITY CHECK: Control Test 6






Alaska Department of Public Safety  
DATAMASTER dmt: 100349

Date: 11/24/2025  
Time: 10:46:15

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.300  
TARGET AT 29.83: 0.299  
LOT #: AG427706  
EXPIRATION: 10/03/2026  
TANK PRESSURE: 428 psi

|                   |          |       |
|-------------------|----------|-------|
| BLANK TEST        | 0.000    | 10:47 |
| INTERNAL STANDARD | VERIFIED | 10:47 |
| EXTERNAL STANDARD | 0.297    | 10:47 |
| BLANK TEST        | 0.000    | 10:48 |
| EXTERNAL STANDARD | 0.297    | 10:48 |
| BLANK TEST        | 0.000    | 10:49 |
| EXTERNAL STANDARD | 0.297    | 10:50 |
| BLANK TEST        | 0.000    | 10:51 |
| EXTERNAL STANDARD | 0.298    | 10:51 |
| BLANK TEST        | 0.000    | 10:52 |
| EXTERNAL STANDARD | 0.297    | 10:52 |
| BLANK TEST        | 0.000    | 10:53 |

Average = 0.2972  
Std Dev = 0.0004

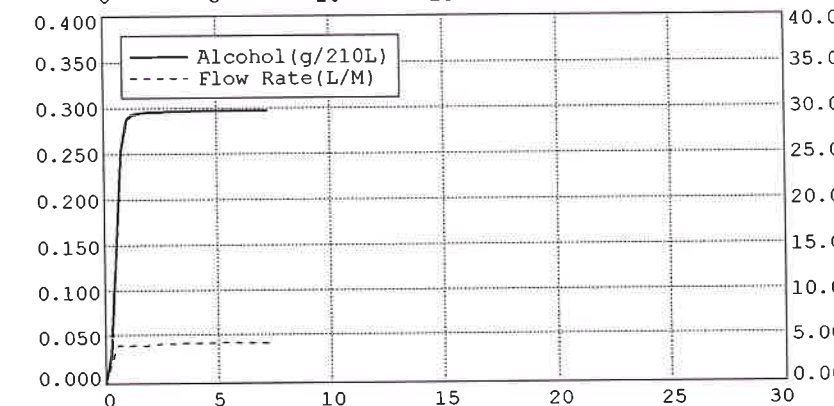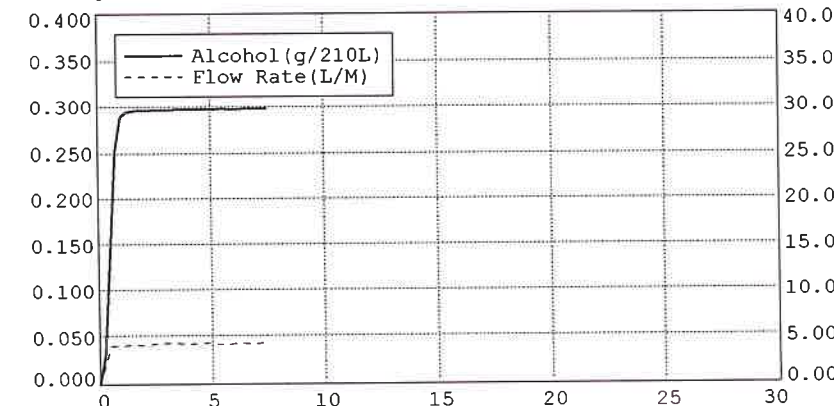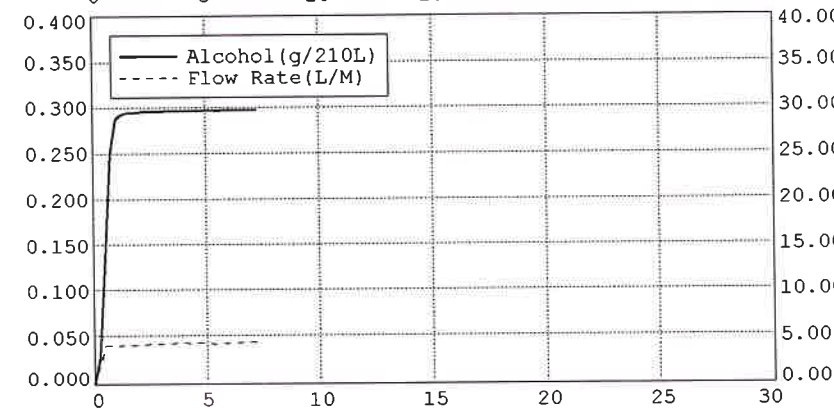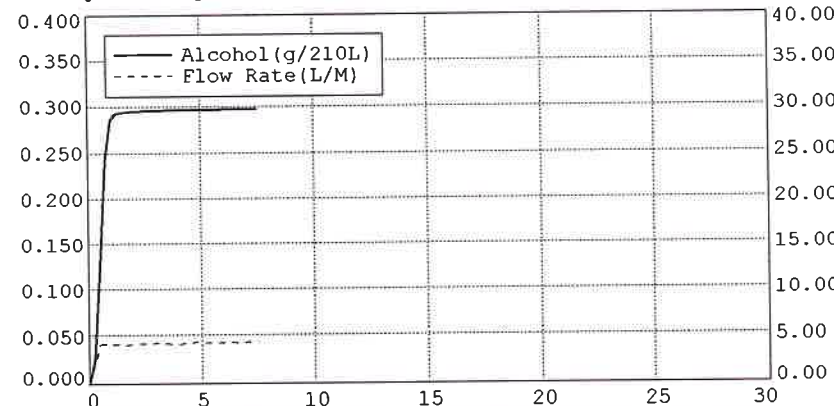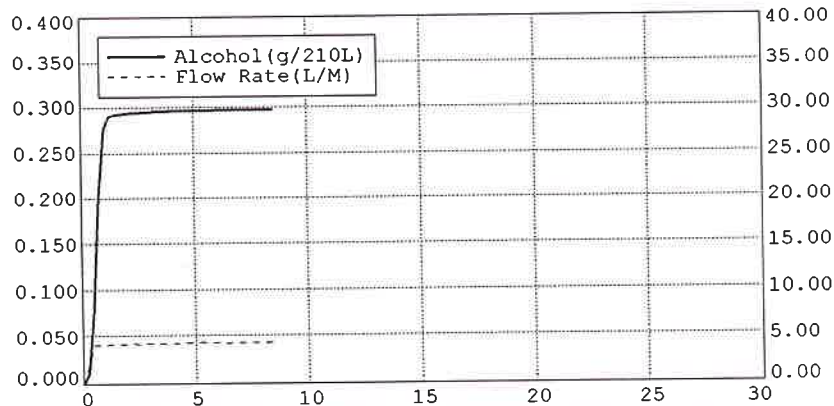

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100349

Date: 11/24/2025

Time: 11:01:21

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

DEREK WALTON

OPERATOR'S #: 9508

DEPT/AGENCY:

INCOMPLETE

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.83: 0.080

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED

0.000

VERIFIED

0.079

0.000

INCOMPLETE

11:03

11:03


11:03

11:03

11:04

11:06

MAC

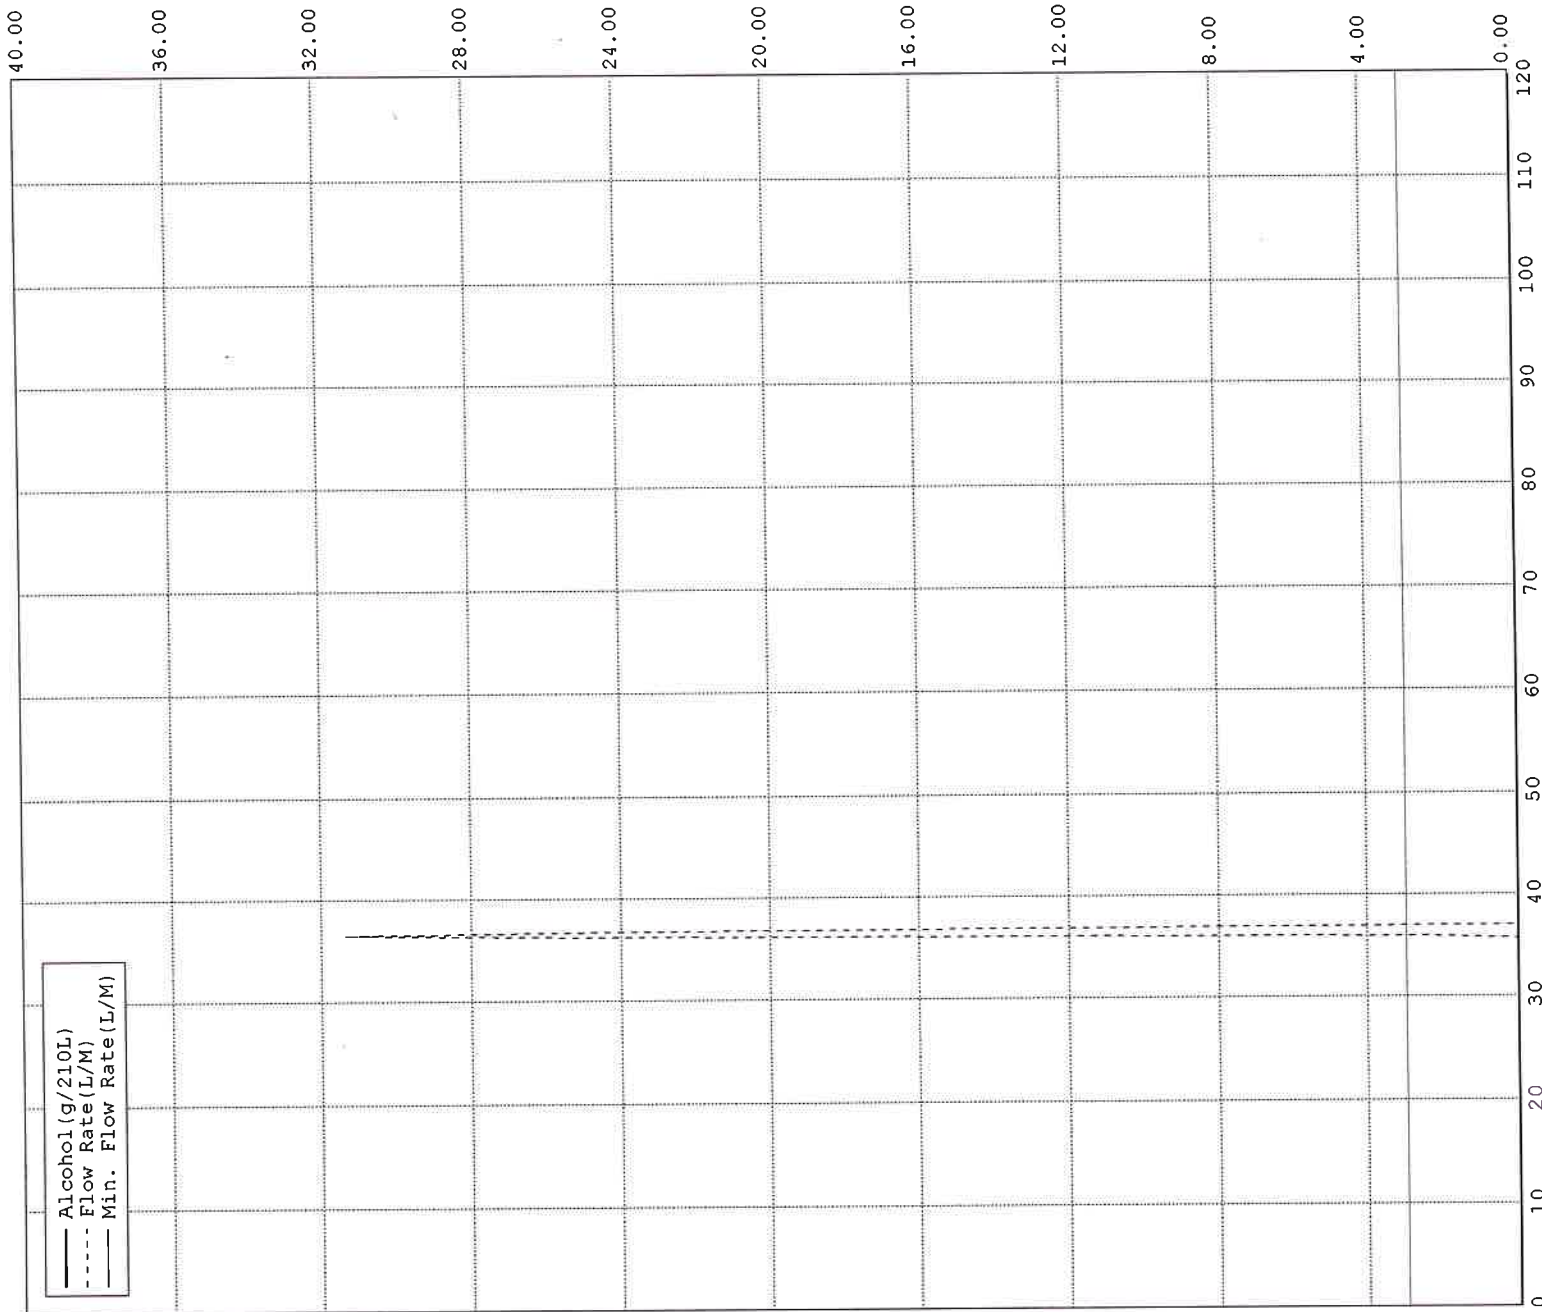

# SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100349

Date: 11/24/2025  
Time: 11:08:40

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508


DEPT/AGENCY:  
MAX ATTEMPTS  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.83: 0.080  
LOT #: AG335202  
EXPIRATION: 12/18/2025

|                   |          |       |
|-------------------|----------|-------|
| DIAGNOSTIC CHECK  | PASSED   | 11:10 |
| BLANK TEST        | 0.000    | 11:10 |
| INTERNAL STANDARD | VERIFIED | 11:10 |
| EXTERNAL STANDARD | 0.079    | 11:11 |
| BLANK TEST        | 0.000    | 11:12 |
| SUBJECT SAMPLE    | XXX      | 11:12 |

Maximum Attempts Exceeded

*DMW*

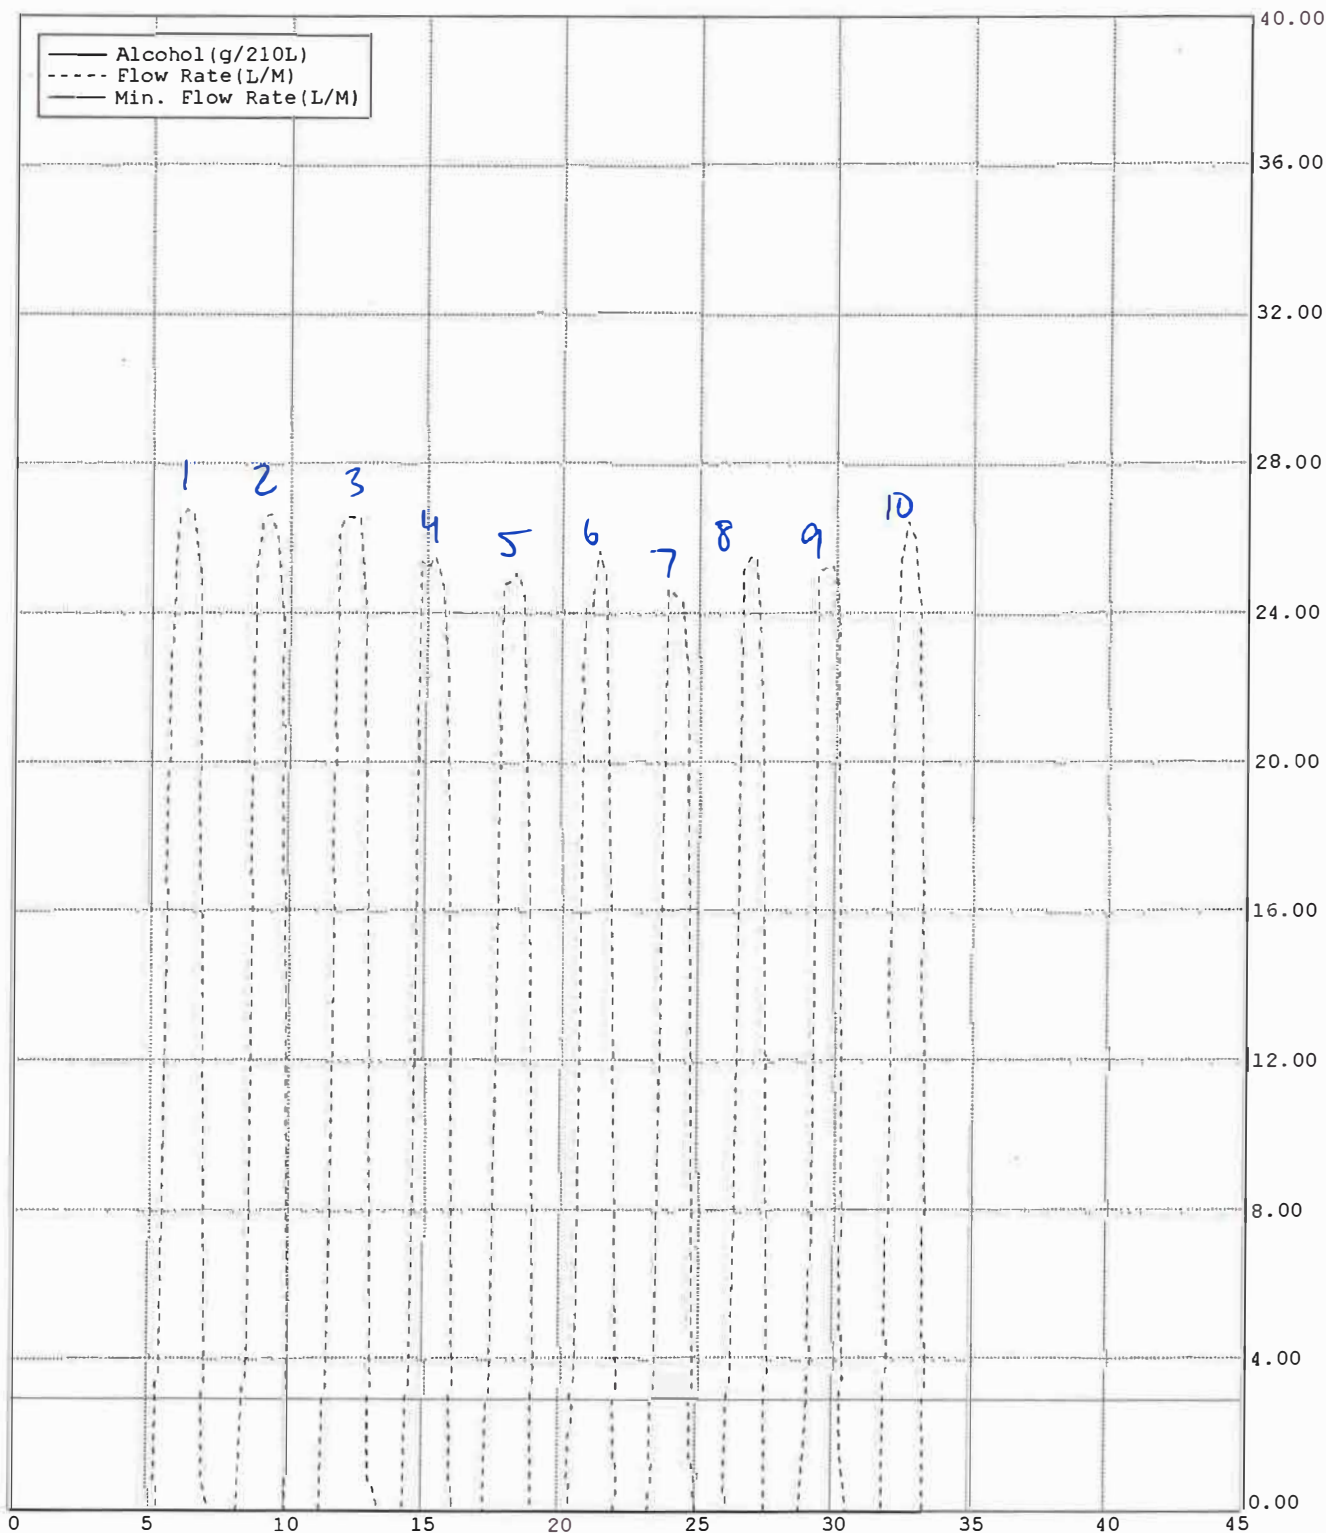

# SUBJECT TEST

Alaska Department of Public Safety  
 DATAMASTER dmt: 100349

Date: 11/24/2025  
 Time: 11:14:48

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXXX


OPERATOR NAME:  
 DEREK WALTON  
 OPERATOR'S #: 9508

DEPT/AGENCY:  
 INVALID  
 CASE/REPORT: XXXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.080  
 TARGET AT 29.83: 0.080  
 LOT #: AG335202  
 EXPIRATION: 12/18/2025

|                   |          |       |
|-------------------|----------|-------|
| DIAGNOSTIC CHECK  | PASSED   | 11:15 |
| BLANK TEST        | 0.000    | 11:15 |
| INTERNAL STANDARD | VERIFIED | 11:16 |
| EXTERNAL STANDARD | 0.079    | 11:16 |
| BLANK TEST        | 0.000    | 11:17 |
| SUBJECT SAMPLE    | INVALID  | 11:17 |

*DM*

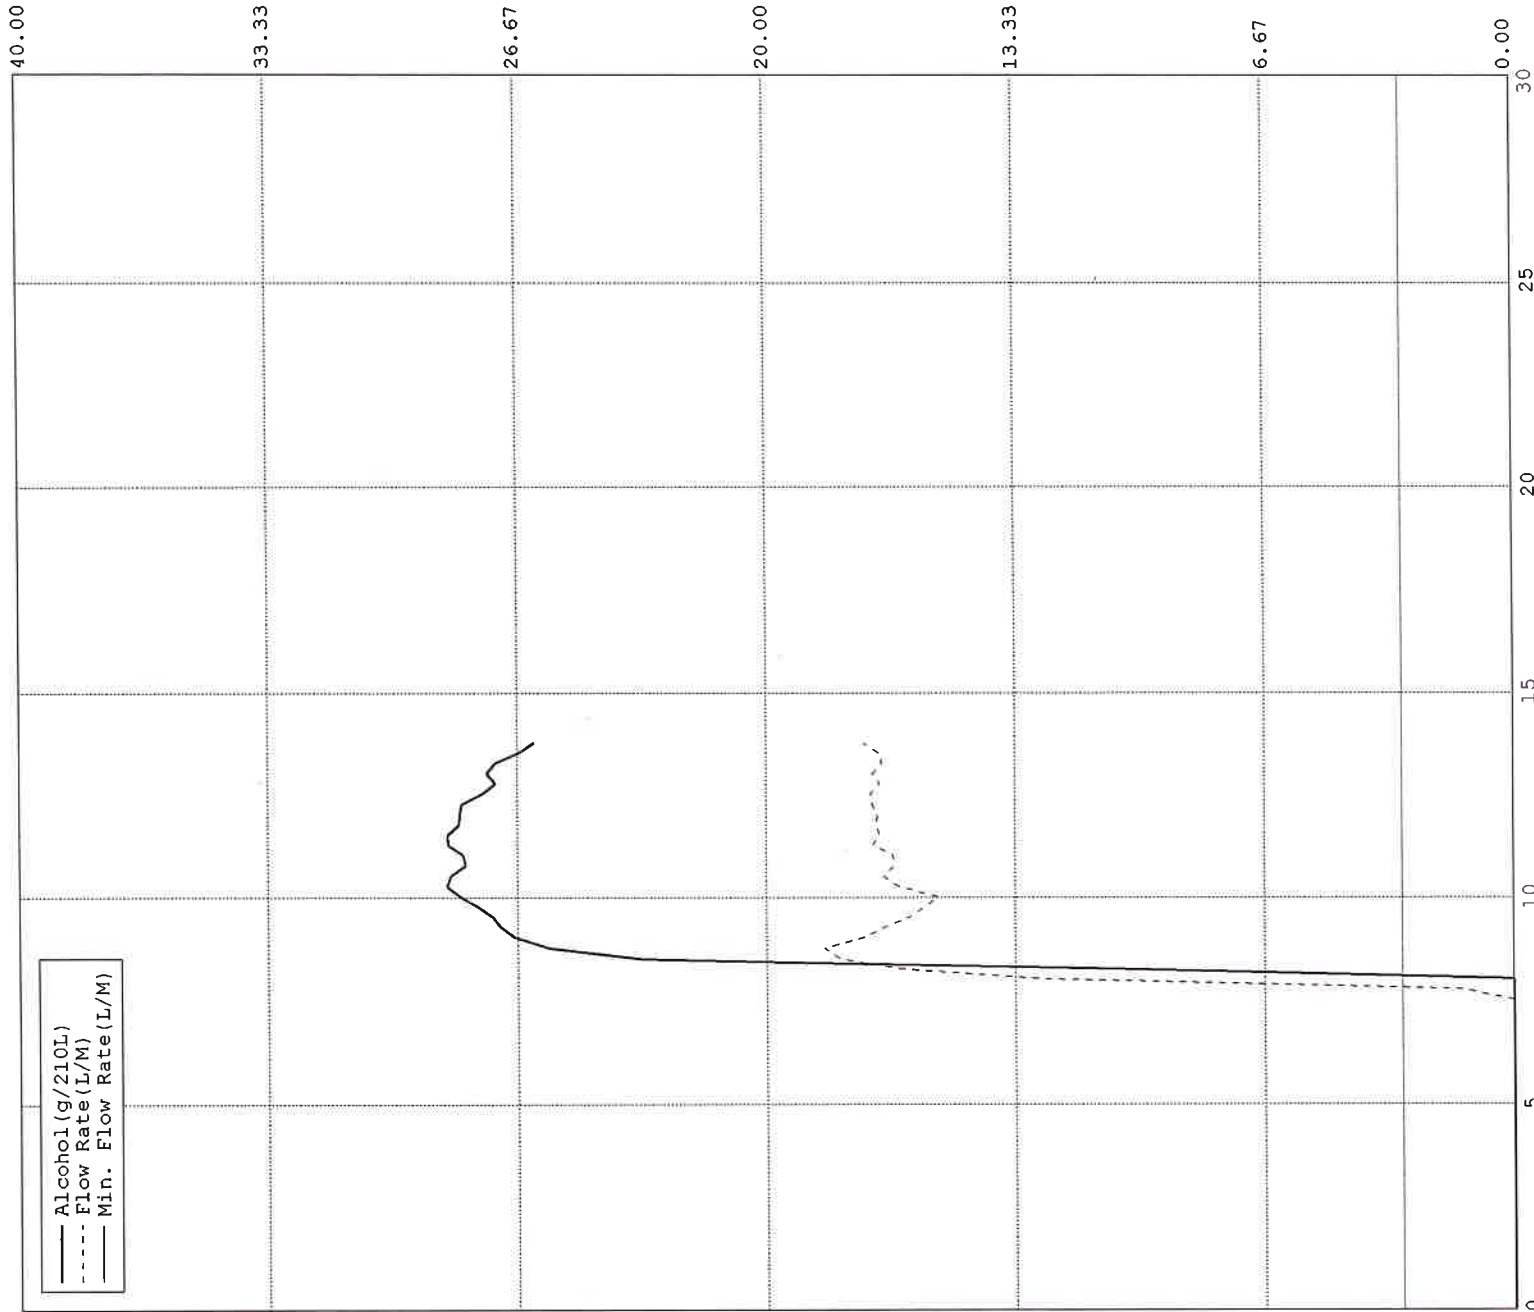

Alaska Department of Public Safety  
DATAMASTER dmt: 100349

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

DEPT/AGENCY:   
RADIO FREQUENCY   
CASE/REPORT: XXXX   
TEST TYPE: TEST

NOMINAL: 0.080  
TARGET AT 29.83: 0.080  
LOT #: AG335202  
EXPIRATION: 12/18/2025

|                   |          |       |
|-------------------|----------|-------|
| DIAGNOSTIC CHECK  | PASSED   | 11:22 |
| BLANK TEST        | 0.000    | 11:23 |
| INTERNAL STANDARD | VERIFIED | 11:23 |
| EXTERNAL STANDARD | 0.078    | 11:23 |
| BLANK TEST        | 0.000    | 11:24 |

ME



# SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100349

Date: 11/24/2025  
Time: 11:29:02

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508

DEPT/AGENCY:  
INTERFERENCE ACETONE  
CASE/REPORT: XXXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.83: 0.080  
LOT #: AG335202  
EXPIRATION: 12/18/2025

|                                  |          |       |
|----------------------------------|----------|-------|
| DIAGNOSTIC CHECK                 | PASSED   | 11:30 |
| BLANK TEST                       | 0.000    | 11:30 |
| INTERNAL STANDARD                | VERIFIED | 11:30 |
| Xq = 0.078 (0.89%)               |          |       |
| EXTERNAL STANDARD                | 0.079    | 11:30 |
| X[1] = 0.0792 (0.0002) (0.0026)  |          |       |
| BLANK TEST                       | 0.000    | 11:31 |
| SUBJECT SAMPLE                   | XXX      | 11:33 |
| X[1] = 0.1049 (-0.0194) (0.0023) |          |       |

Interference Detected

Filter 2 average: -0.0007  
Filter 3 average: 0.0021  
DJW 11/24/2025

*[Handwritten signature]*

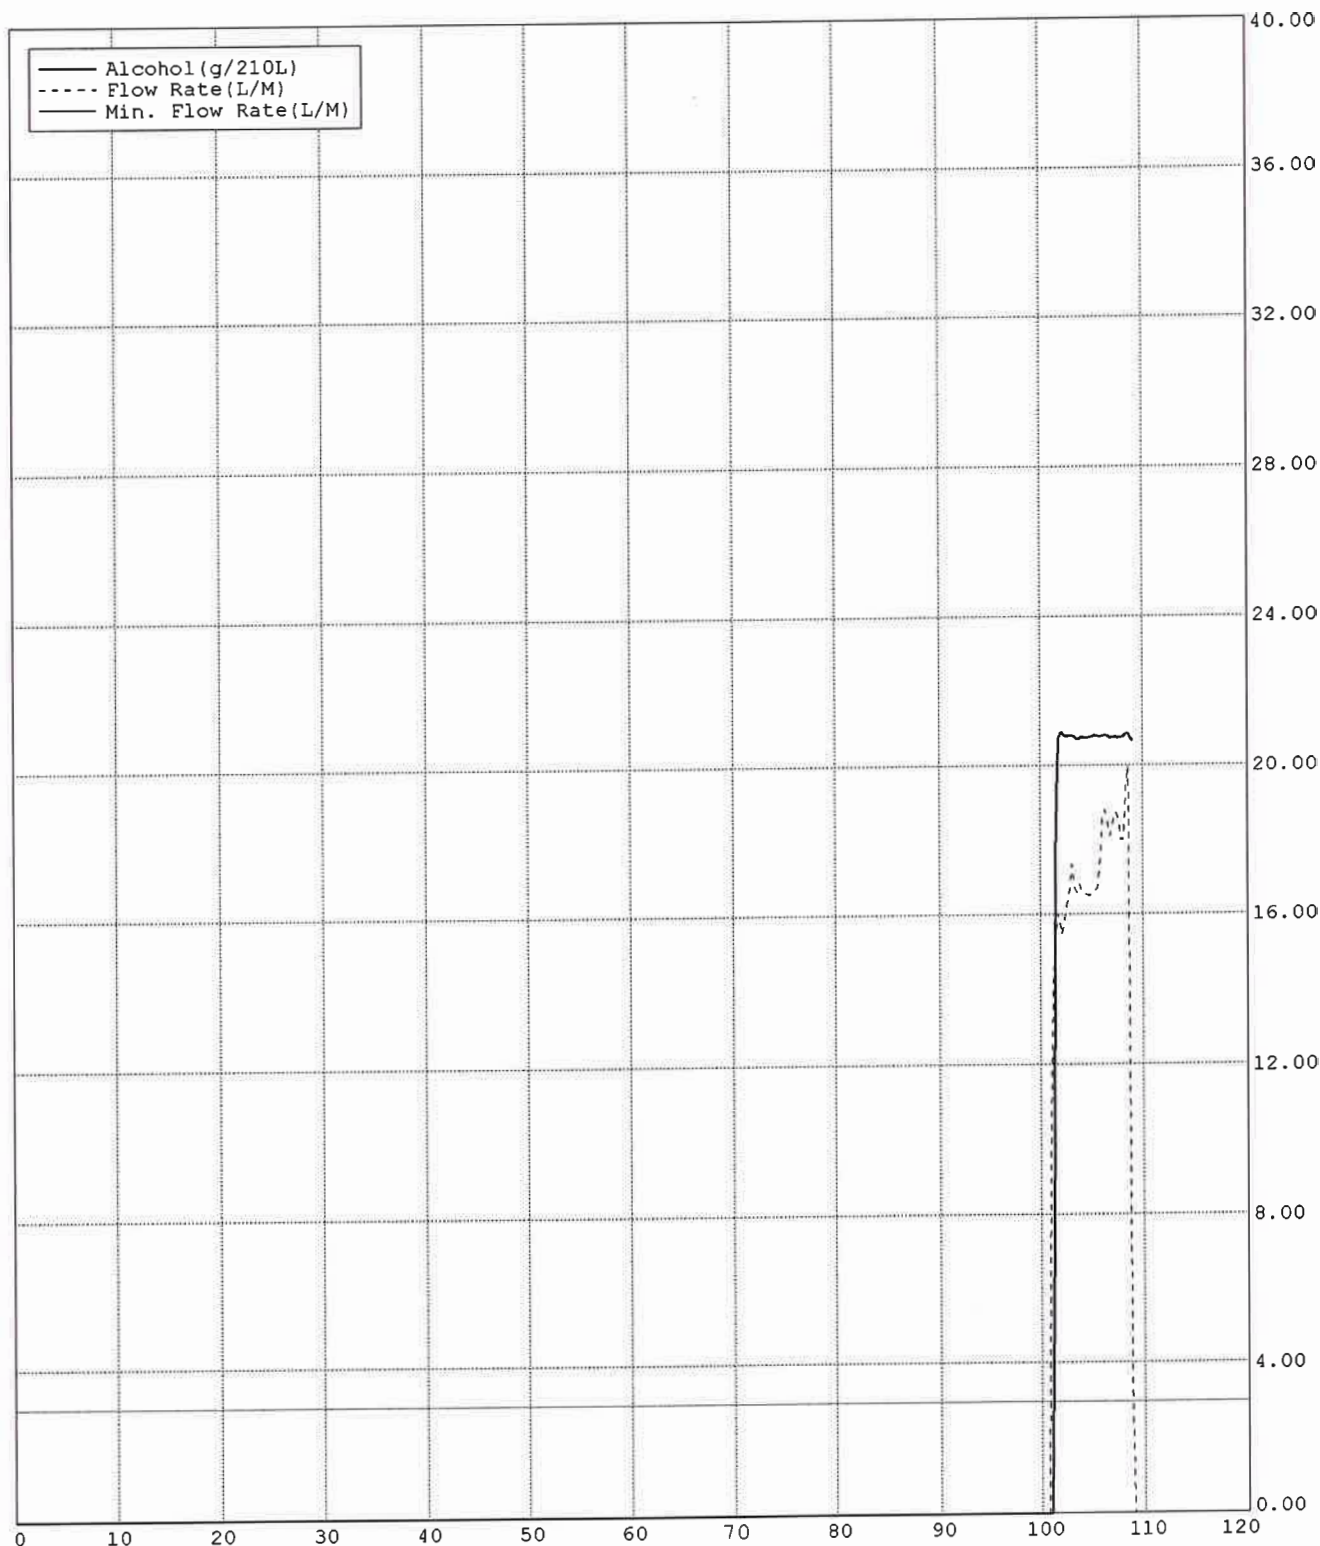

# SUBJECT TEST

Alaska Department of Public Safety  
 DATA MASTER dmt: 100349

Date: 11/24/2025  
 Time: 11:44:26

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXXX

OPERATOR NAME:  
 DEREK WALTON  
 OPERATOR'S #: 9508


DEPT/AGENCY:  
 INTERFERENCE ISOPROPANOL  
 CASE/REPORT: XXXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.080  
 TARGET AT 29.83: 0.080  
 LOT #: AG335202  
 EXPIRATION: 12/18/2025

|                         |          |       |
|-------------------------|----------|-------|
| DIAGNOSTIC CHECK        | PASSED   | 11:45 |
| BLANK TEST              | 0.000    | 11:45 |
| INTERNAL STANDARD       | VERIFIED | 11:46 |
| Xq = 0.079 (1.45%)      |          |       |
| EXTERNAL STANDARD       | 0.079    | 11:46 |
| X[1] = 0.0790 (-0.0011) | (0.0019) |       |
| BLANK TEST              | 0.000    | 11:47 |
| SUBJECT SAMPLE          | XXX      | 11:47 |
| X[1] = 0.1170 (-0.0289) | (0.0016) |       |

Interference Detected

*Handwritten signature/initials*

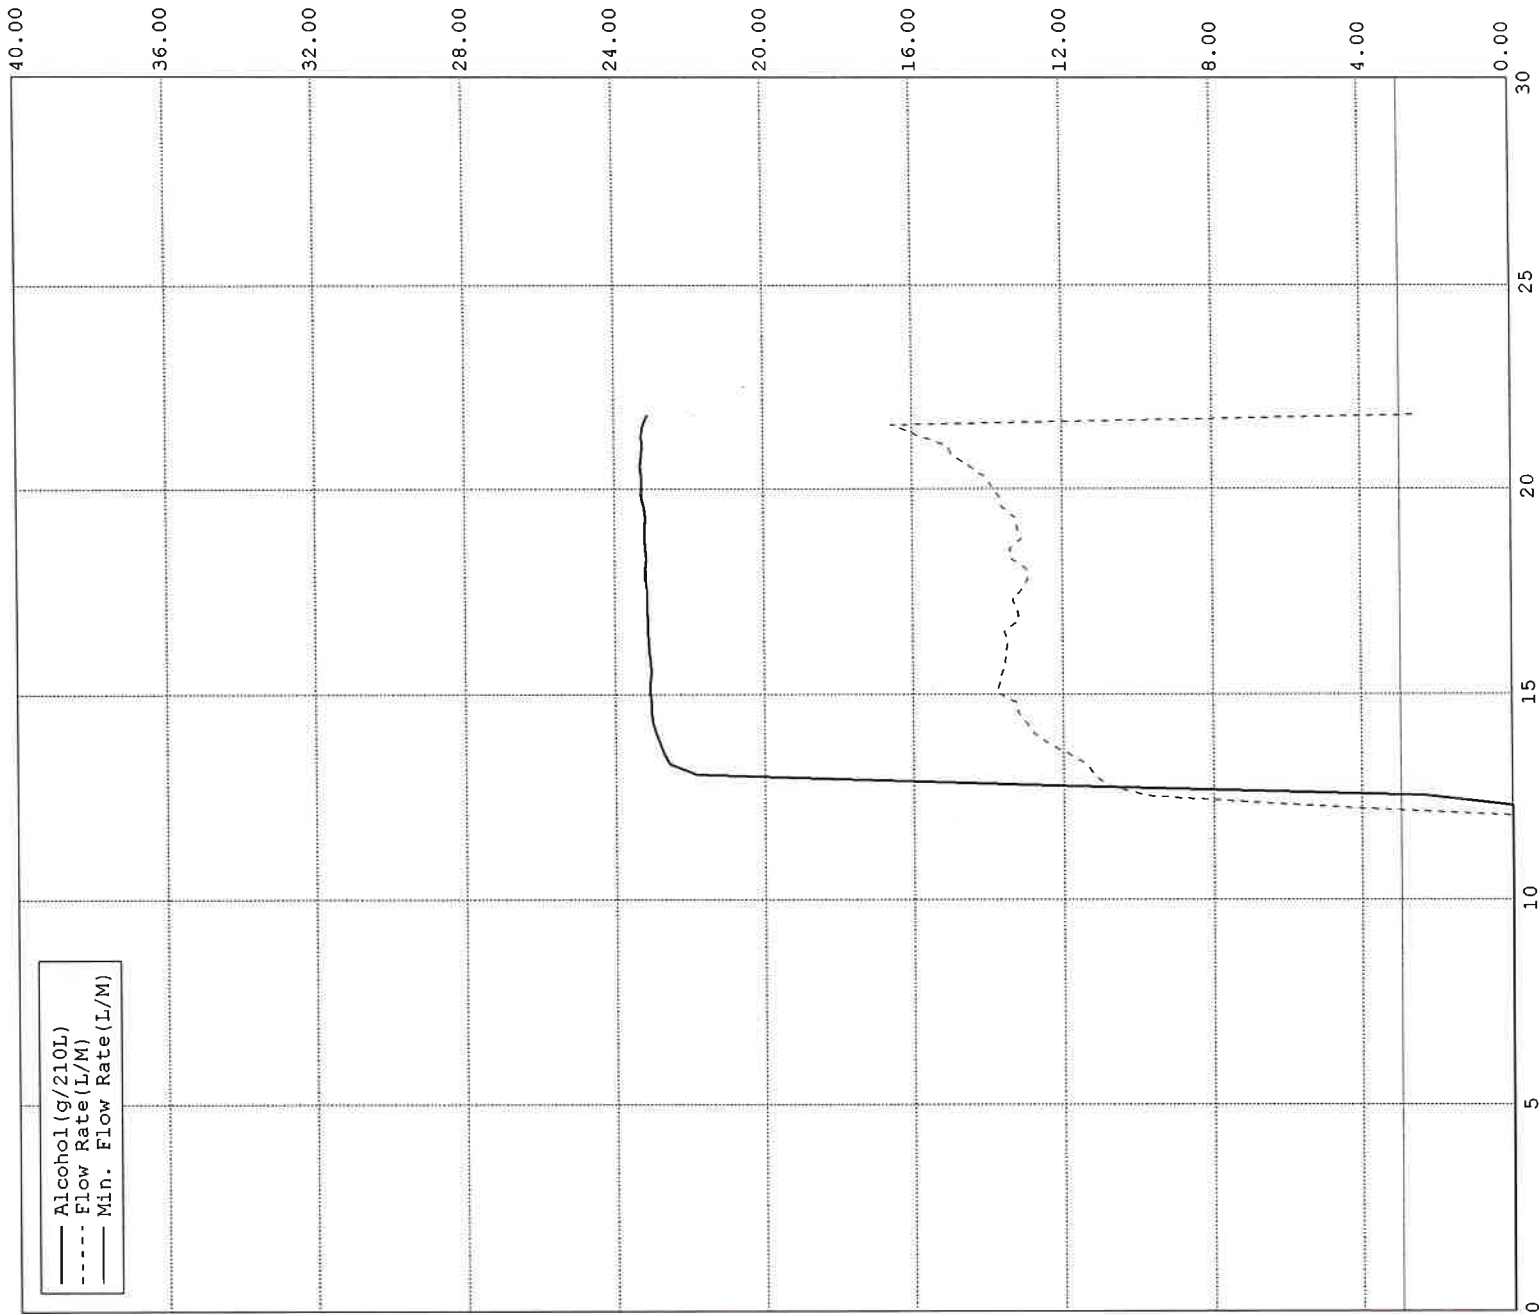

# SUBJECT TEST

Alaska Department of Public Safety  
 DATAMASTER dmt: 100349

Date: 11/24/2025  
 Time: 11:36:46

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXXX


OPERATOR NAME:  
 DEREK WALTON  
 OPERATOR'S #: 9508

DEPT/AGENCY:  
 INTERFERENCE NEGATIVE  
 CASE/REPORT: XXXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.080  
 TARGET AT 29.84: 0.080  
 LOT #: AG335202  
 EXPIRATION: 12/18/2025

|                            |          |       |
|----------------------------|----------|-------|
| DIAGNOSTIC CHECK           | PASSED   | 11:37 |
| BLANK TEST                 | 0.000    | 11:38 |
| INTERNAL STANDARD          | VERIFIED | 11:38 |
| Xq = 0.079 (1.12%)         |          |       |
| EXTERNAL STANDARD          | 0.078    | 11:38 |
| X[1] = 0.0783 (-0.0011)    | (0.0022) |       |
| BLANK TEST                 | 0.000    | 11:39 |
| SUBJECT SAMPLE (Vol=2.02L) | 0.091    | 11:40 |
| X[1] = 0.0910 (0.0003)     | (0.0018) |       |
| BLANK TEST                 | 0.000    | 11:41 |
| EXTERNAL STANDARD          | 0.079    | 11:41 |
| X[1] = 0.0786 (-0.0007)    | (0.0017) |       |
| BLANK TEST                 | 0.000    | 11:42 |

*DMC*

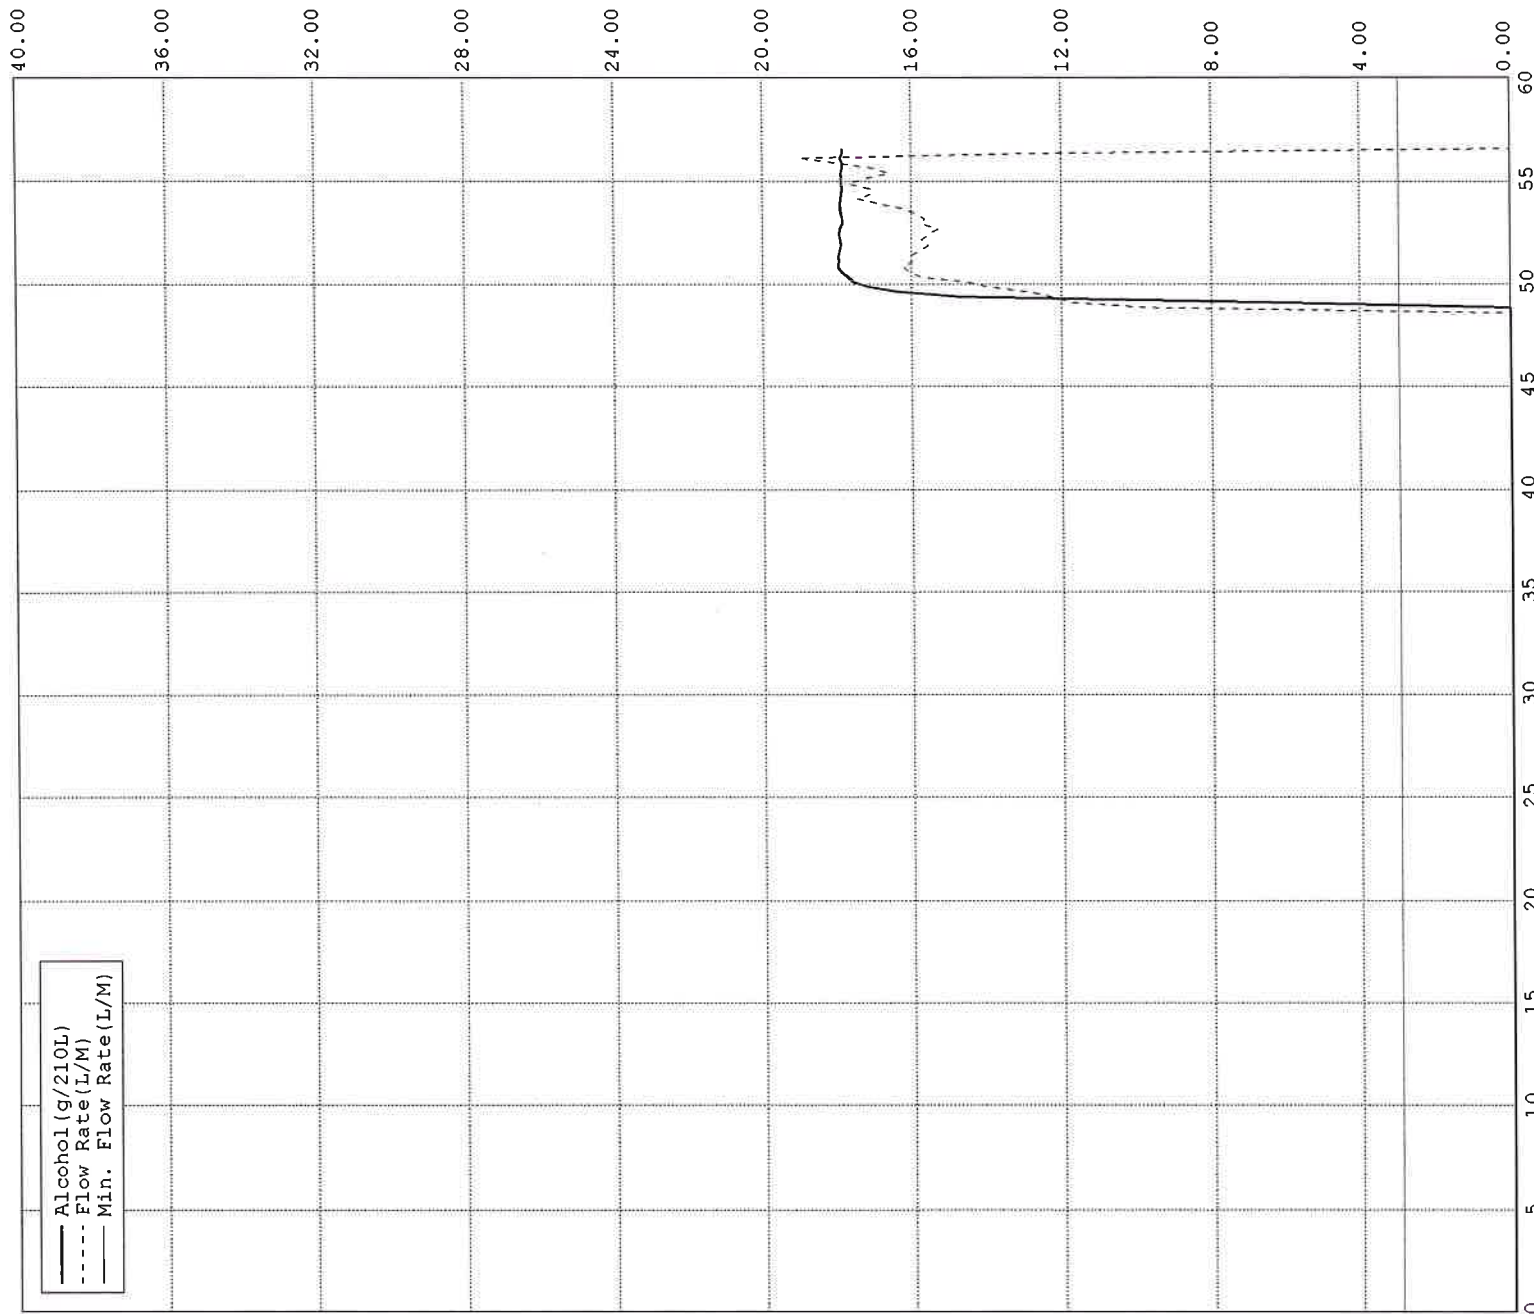

# SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100349

Date: 11/24/2025

Time: 12:12:40

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

DEREK WALTON

OPERATOR'S #: 9508

DEPT/AGENCY:

NON-DRINKING SUBJECT

CASE/REPORT: XXXX

TEST TYPE: TEST

## EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.84: 0.080

LOT #: AG335202

EXPIRATION: 12/18/2025

|                            |          |       |
|----------------------------|----------|-------|
| DIAGNOSTIC CHECK           | PASSED   | 12:13 |
| BLANK TEST                 | 0.000    | 12:13 |
| INTERNAL STANDARD          | VERIFIED | 12:13 |
| EXTERNAL STANDARD          | 0.079    | 12:14 |
| BLANK TEST                 | 0.000    | 12:15 |
| SUBJECT SAMPLE (Vol=3.85L) | 0.000    | 12:15 |
| BLANK TEST                 | 0.000    | 12:16 |
| EXTERNAL STANDARD          | 0.079    | 12:16 |
| BLANK TEST                 | 0.000    | 12:17 |

DMV

