



7 Eastgate Dr. • P.O. Box 790 • Jacksonville, IL 62651-0790
217-245-2183 • Fax: 217-243-7634 • www.ilmoproducts.com

Certificate of Analysis


Certificate ID: 2697
Part #: BAC105L080T
Cylinder Size: 105L
Lot Number: 02012080A1
Expiration: 3/1/2014

0.080 BAC (For use with breath alcohol testing instruments)

Contents: 105 Liters @ 1000 psig 70°F (21°C)


Component:	Concentration:	Accuracy:	Method:
Ethanol	208.4 ppm	+/- 0.002 or 2%	NDIR
Nitrogen	Balance	BAC whichever is greater	

*NIST Standard Reference Material
Certification of NTRM Batch No. 091602
Nominal 210 µmol/mol Ethanol in Nitrogen
for ILMO Products Co., Jacksonville, IL


Specialty Gas Lab Tech

01-24-12
Date

Distributed by: CMI Inc.
316 East Ninth Street
Owensboro, KY 42303
Phone 866-835-0690
www.alcoholtest.com

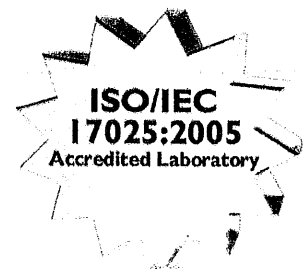

SUPERVISOR TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100362

Date: 03/02/2012
 Time: 13:03:21

SUPERVISOR NAME:
 CHARLES FOSTER
 OPERATOR'S #: 7734

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.22: 0.078

BLANK TEST	0.000	13:04
INTERNAL STANDARD	VERIFIED	13:05
EXTERNAL STANDARD	0.077	13:05
BLANK TEST	0.000	13:06
EXTERNAL STANDARD	0.077	13:06
BLANK TEST	0.000	13:07
EXTERNAL STANDARD	0.078	13:07
BLANK TEST	0.000	13:08
EXTERNAL STANDARD	0.077	13:08
BLANK TEST	0.000	13:09
EXTERNAL STANDARD	0.077	13:09
BLANK TEST	0.000	13:10






Average = 0.0778
 Std Dev = 0.0003

ILMO 0.080 BAC

Lot #: 02012080A1

Expiration: 3/1/2014

*Combined average of
 three instruments = 0.078*

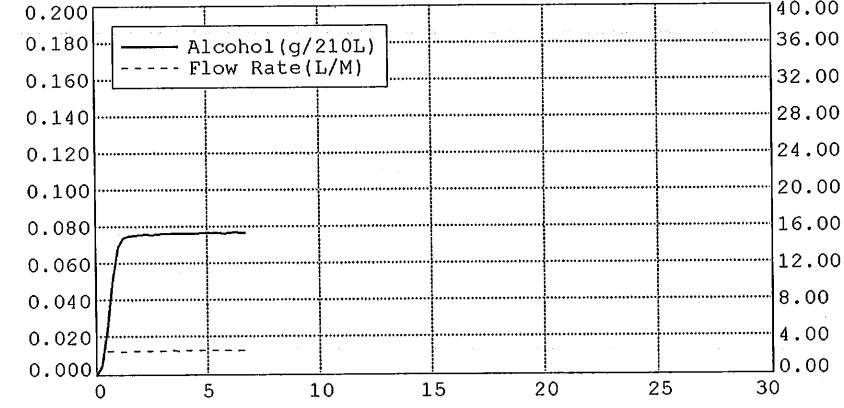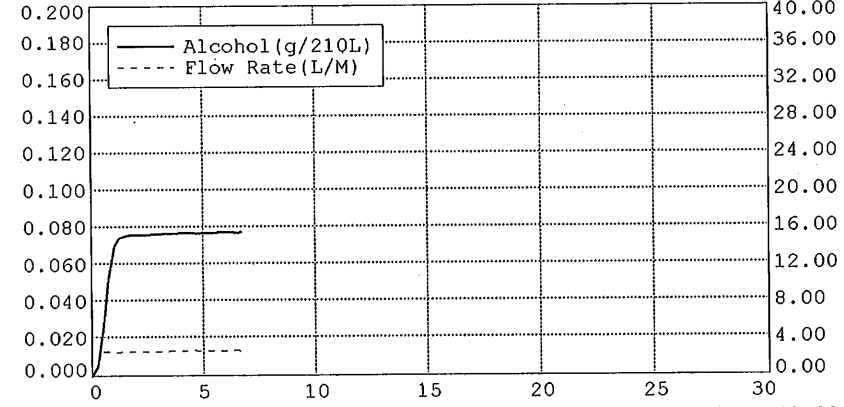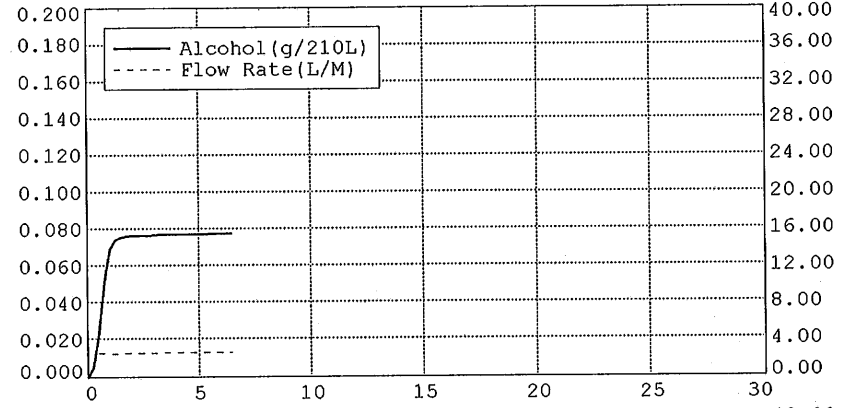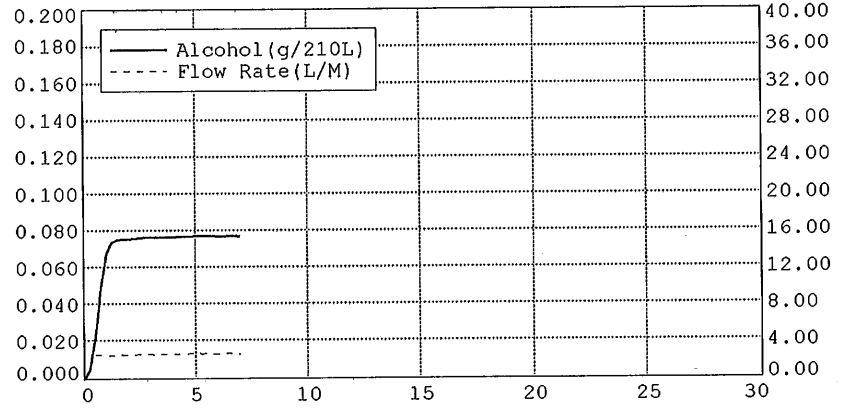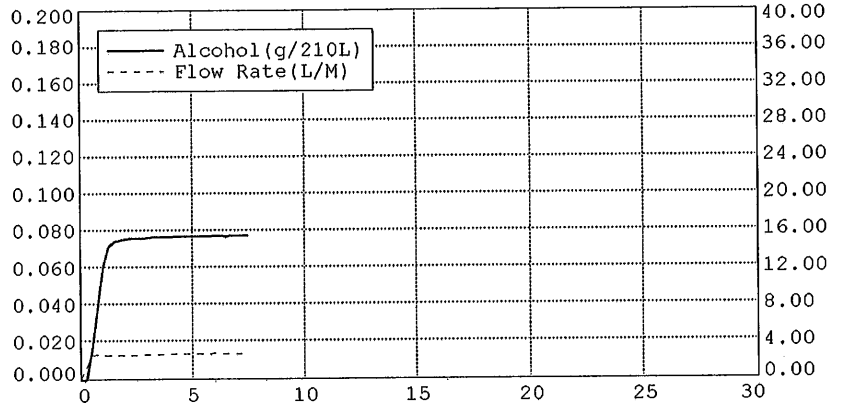

SUPERVISOR TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100669






Date: 03/02/2012
 Time: 12:42:31

SUPERVISOR NAME:
 CHARLES FOSTER
 OPERATOR'S #: 7734

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.22: 0.078

BLANK TEST	0.000	12:44
INTERNAL STANDARD	VERIFIED	12:44
EXTERNAL STANDARD	0.078	12:44
BLANK TEST	0.000	12:45
EXTERNAL STANDARD	0.078	12:45
BLANK TEST	0.000	12:46
EXTERNAL STANDARD	0.078	12:46
BLANK TEST	0.000	12:47
EXTERNAL STANDARD	0.078	12:48
BLANK TEST	0.000	12:48
EXTERNAL STANDARD	0.078	12:49
BLANK TEST	0.000	12:50

Average = 0.0786
 Std Dev = 0.0003

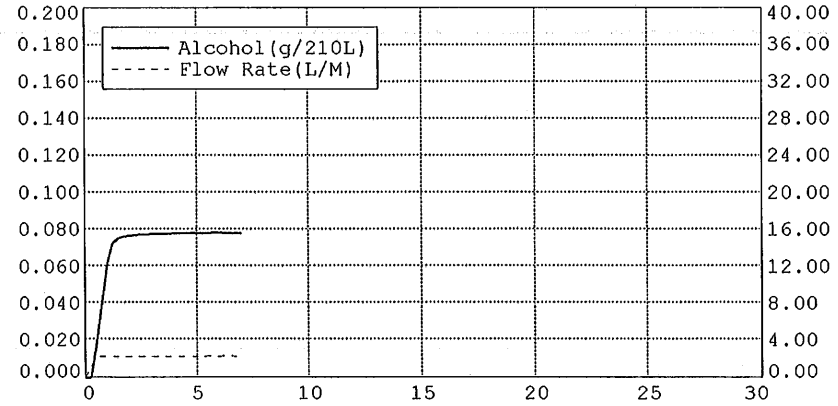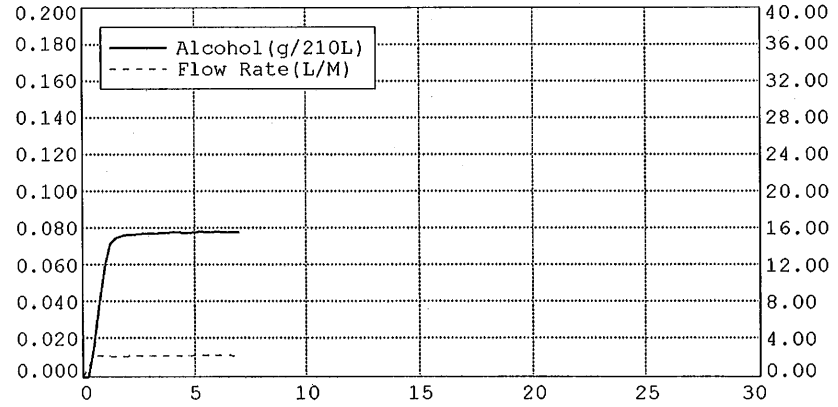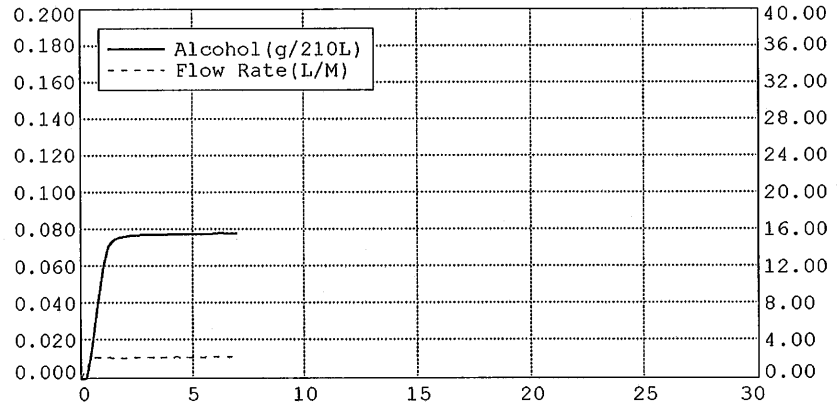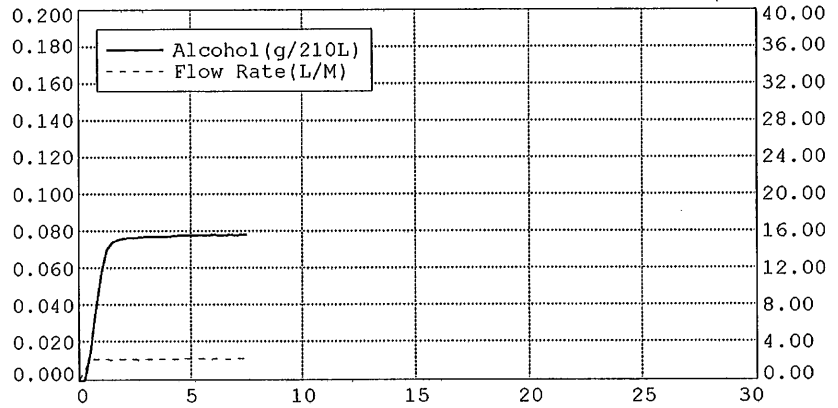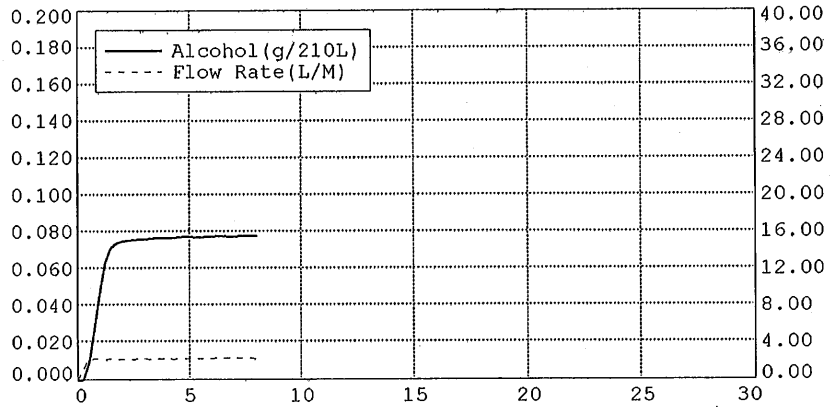

SUPERVISOR TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100668

Date: 03/02/2012
Time: 12:54:22

SUPERVISOR NAME:
CHARLES FOSTER
OPERATOR'S #: 7734

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.21: 0.078

BLANK TEST	0.000	12:56
INTERNAL STANDARD	VERIFIED 0.078	12:56
EXTERNAL STANDARD	0.078	12:56
BLANK TEST	0.000	12:57
EXTERNAL STANDARD	0.078	12:57
BLANK TEST	0.000	12:58
EXTERNAL STANDARD	0.078	12:58
BLANK TEST	0.000	12:59
EXTERNAL STANDARD	0.078	12:59
BLANK TEST	0.000	13:00
EXTERNAL STANDARD	0.078	13:00
BLANK TEST	0.000	13:01

Average = 0.0785
Std Dev = 0.0002

