



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories



**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100398

**Report Issue Date:** 04/25/2024  
**Date Received:** 2023-08-14  
**Condition of Item:** Needs Repair

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

As-Found Data				
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)	Mean (g/210L)
0.020				
0.080				
0.300				

As Found - Evaluation Analyst: Tatiana Malnoske  
 As Found Conditions - Barometric Pressure (inHg): 29.84 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.7 Relative Humidity (%): 39%  
 As-Found Lab Activity Date Range: 08/17/2023 - 08/17/2023

Unable to screw a tank in. I tried different tanks then changed the O-ring twice and was still having issues. I was unable to perform linearity testing due to this issue.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.040	AG217904	0.040	0.040	0.039	0.039	0.039	0.039	+/- 0.003
0.080	0.079	AG310901	0.079	0.078	0.079	0.078	0.078	0.078	+/- 0.004
0.100	0.099	AG211003	0.098	0.098	0.098	0.098	0.098	0.098	+/- 0.004
0.150	0.148	AG332004	0.145	0.146	0.145	0.145	0.145	0.145	+/- 0.005
0.300	0.297	AG327804	0.296	0.296	0.295	0.295	0.295	0.295	+/- 0.011

As Left Conditions - Barometric Pressure (inHg): 29.60 Barometer Used: Fisher S/N 230307229 Temperature (C): 20.1 Relative Humidity (%): 25  
 As-Left Lab Activity Date Range: 03/28/2024 - 03/29/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Carlie Glaister on 04/25/2024

[carlie.glaister@alaska.gov](mailto:carlie.glaister@alaska.gov)

Technically and administratively reviewed by Brandi Barnett on 04/25/2024

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100399 Analyst or Technician Name: Megan C.

DataMaster DMT Calibration Start Date: 3/28/24 Supervised by Carlise Glaister

### Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value  $\leq$  3.00%

### Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer  
Barometer/Thermometer/Hygrometer S/N: 230307229  
Calibration Due Date: 5/2/2025
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

### Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.7 liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 29.60 Temperature(C) 20.1 Relative Humidity(%) 25  
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20240214C08 Expiration Date: 5/14/24  
Simulator S/N: SD10886 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20240214C08 Expiration Date: 5/14/24  
Simulator S/N: DR4161 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 22HP41201 Expiration Date: 8/24/24  
Simulator S/N: SD1177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 230631106  
Calibration Due Date: 9/19/2025

### Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

### Completion

Lab Work End Date: 3/28/24  
Data Interpretation Date (Technician): 3/29/24 MNC (if applicable)  
Data Interpretation Date (Analyst): 3/29/24 supervised by CLK

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100398  
-----

Date: 03/28/2024  
Time: 09:00:34

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 49.2°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 48.1°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.82 V PASSED  
(1.09 V - 2.55 V)  
Cooler Voltage = 1.76 V PASSED  
(1.06 V - 2.46 V)  
Bias Voltage = 80 V PASSED  
(48 V - 112 V)  
Chopper Freq = 536 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.6 in

PUMP INFO

Flow Rate = 4.278 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.002 v <= 0.010 v)  
PUMP OFF PASSED  
(0.002 v <= 0.010 v)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.081 1.63% (0.00% - 4.00%) PASSED

Technician Screen

-----  
DATAMASTER dmt: 100398  
-----

Date: 03/28/2024  
Time: 9:10 AM

Temperatures (°C)  
Sample Cell: 48.9°C  
Breath Tube: 47.6°C

Current Barometer 29.6 in  
Volume (Ltr) 1.44

Settings  
Lamp: 1.85 V  
Bias: 80 V  
Cooler: 1.66 V  
Chopper: 534 Hz

Voltages (V)  
Flow: 1.03 V  
Detector: -0.055 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100398  
-----

Date: 01/18/2024  
Time: 07:38:48

OPERATOR NAME:  
INTOX I METERS  
CERTIFICATE #: INTOXIMETERS

Ca = 0.0990  
CAL = 0.986540    0.800 <= CAL < 1.200  
b1 = 0.0007    0.0000 <= b1 < 0.0040  
b2 = 0.0099    0.0010 <= b2 < 0.0100  
b3 = 0.0006    0.0000 <= b3 < 0.0040  
Xq = 0.0797    0.0500 <= Xq < 0.2000  
a21 = 1.232388    1.050 <= a21 < 1.300  
a31 = 0.463748    0.300 <= a31 < 0.800

INTOX

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100398

Date: 03/28/2024

Time: 09:15:15

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CROUSE

OPERATOR'S #: 10747

DEPT/AGENCY:

MINIMUM VOLUME TEST

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080


TARGET AT 29.60: 0.079

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	09:16
BLANK TEST	0.000	09:16
INTERNAL STANDARD	VERIFIED	09:16
EXTERNAL STANDARD	0.079	09:17
BLANK TEST	0.000	09:17
SUBJECT SAMPLE (Vol=1.58L)	0.000	09:19
BLANK TEST	0.000	09:20
EXTERNAL STANDARD	0.078	09:20
BLANK TEST	0.000	09:21

MVC

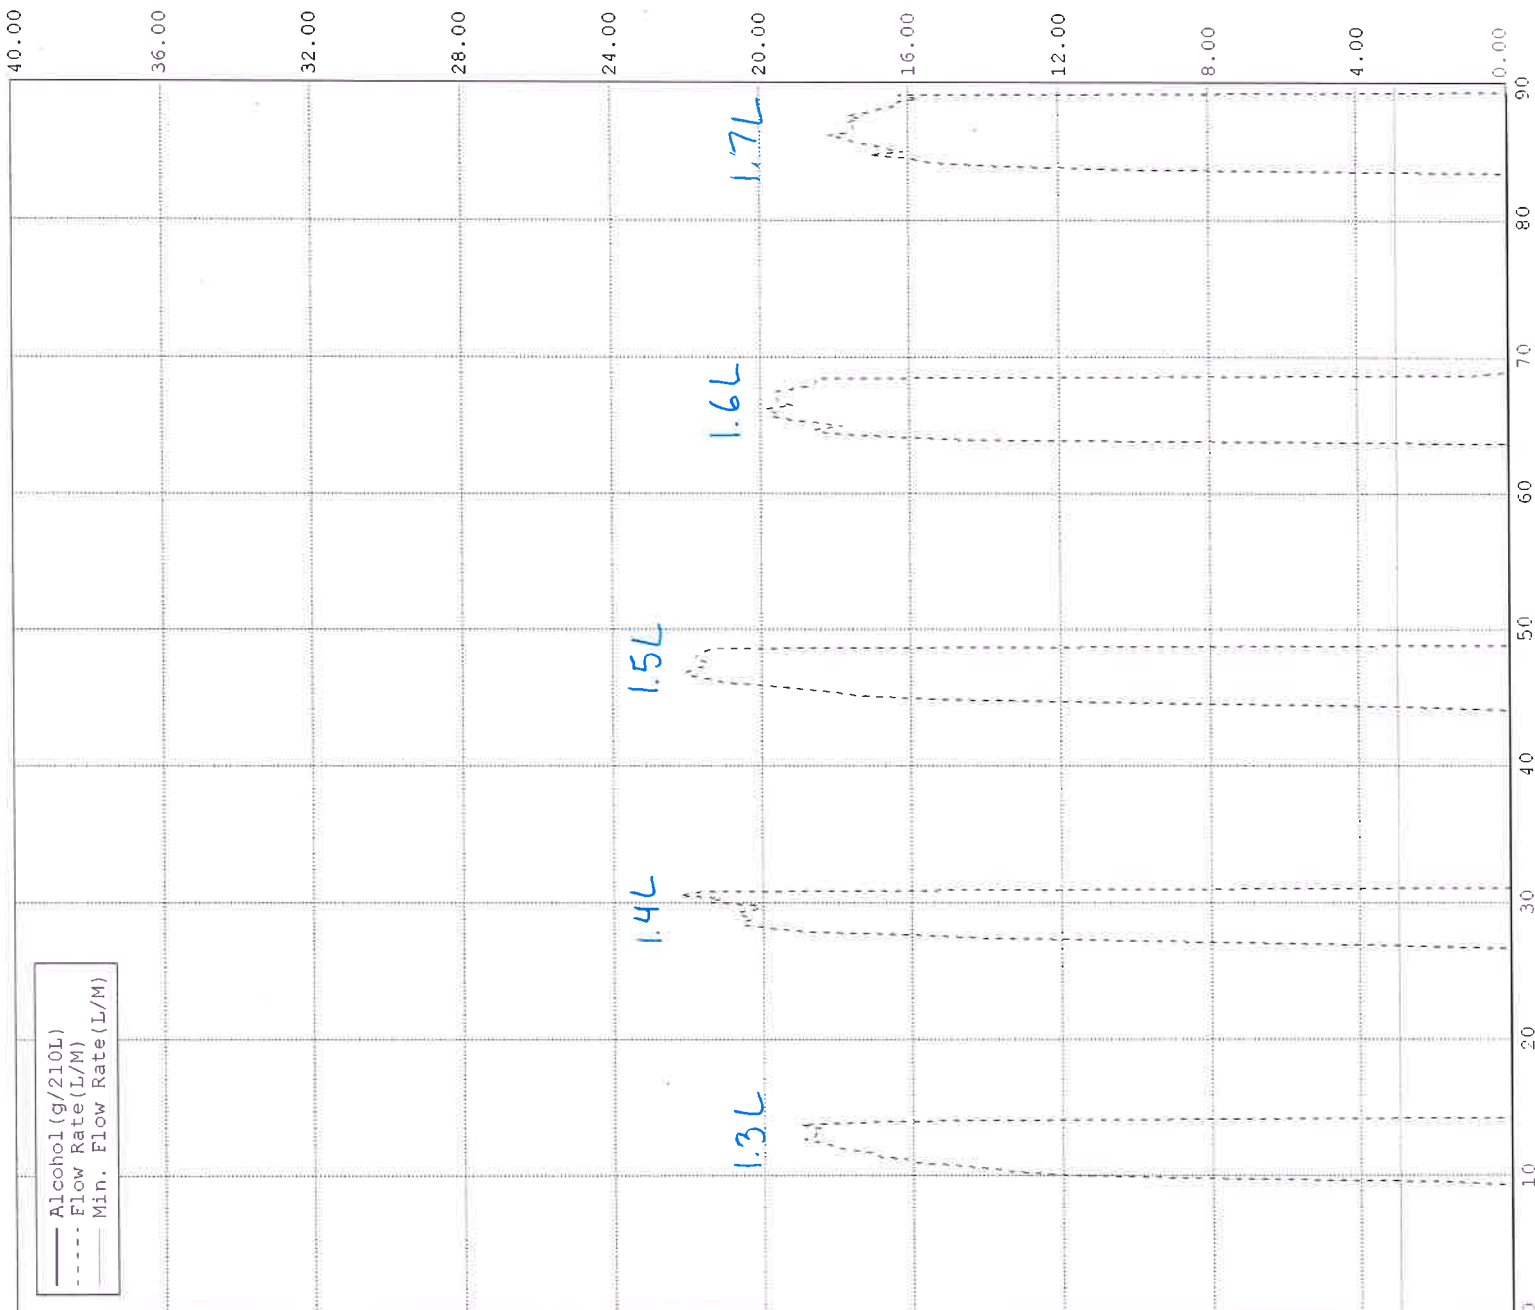

LINEARITY CHECK


-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100398  
 -----

Date: 03/28/2024  
 Time: 09:37:07

SUPERVISOR NAME:  
 MEGAN CROUSE  
 OPERATOR'S #: 10747

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.040	0.0394	0.0005
0.079	0.0784	0.0005
0.099	0.0980	0.0000
0.148	0.1452	0.0004
0.297	0.2954	0.0005

SLOPE = 0.993876  
 R<sup>2</sup> = 0.999940

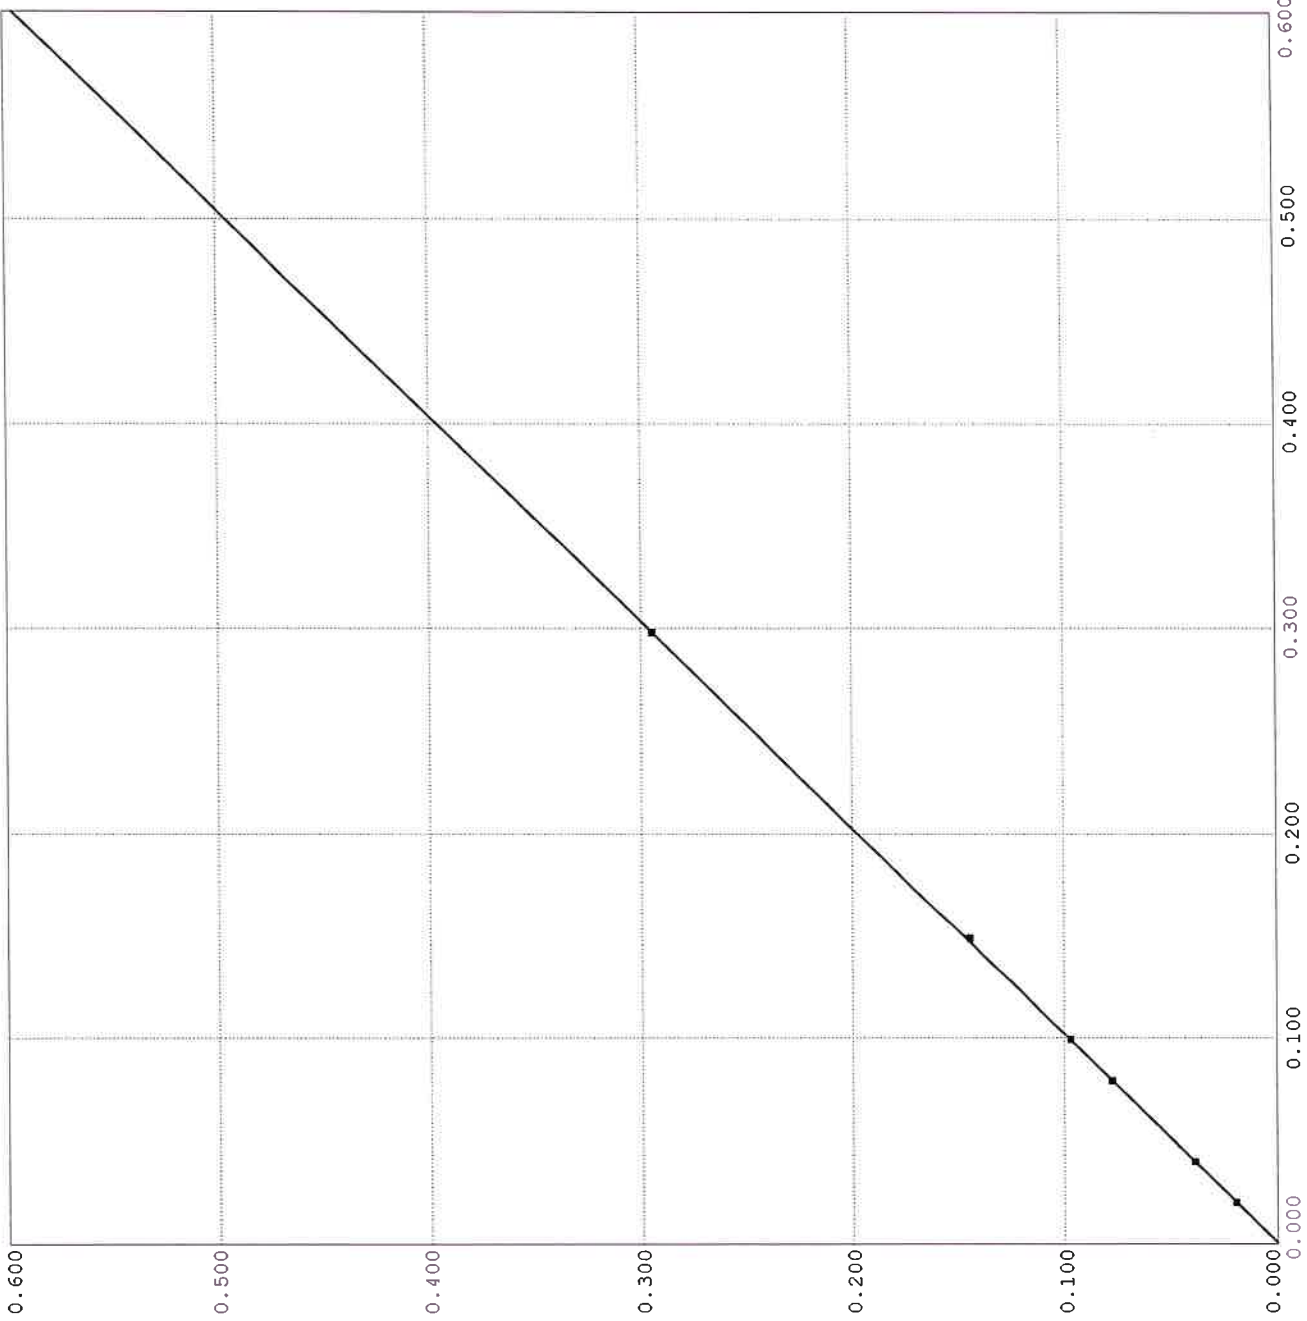

MNC



LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100398






Date: 03/28/2024  
Time: 09:37:09

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 29.60: 0.020  
LOT #: AG217902  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 630 psi

BLANK TEST	0.000	09:41
INTERNAL STANDARD	VERIFIED	09:41
EXTERNAL STANDARD	0.020	09:41
BLANK TEST	0.000	09:42
EXTERNAL STANDARD	0.020	09:42
BLANK TEST	0.000	09:43
EXTERNAL STANDARD	0.020	09:43
BLANK TEST	0.000	09:44
EXTERNAL STANDARD	0.020	09:44
BLANK TEST	0.000	09:45
EXTERNAL STANDARD	0.020	09:45
BLANK TEST	0.000	09:46

Average = 0.0200  
Std Dev = 0.0000

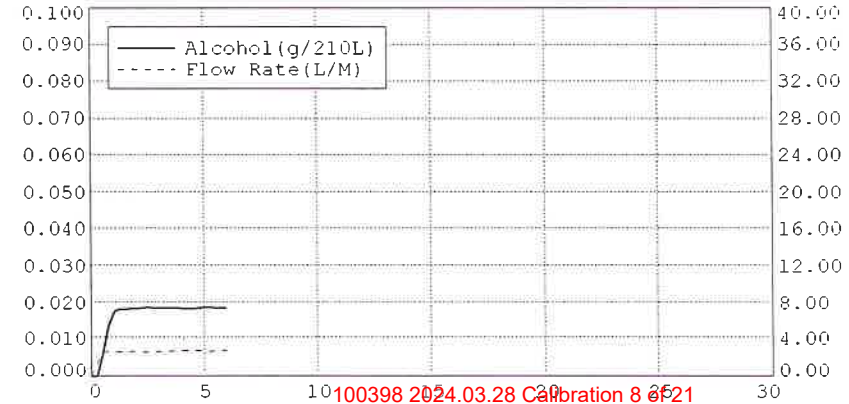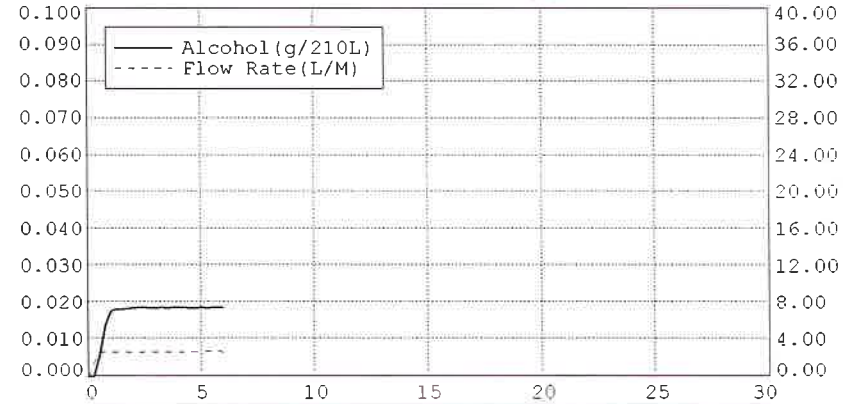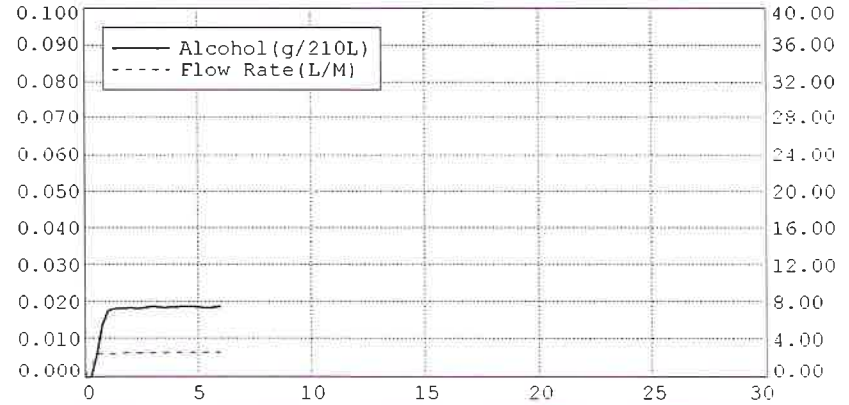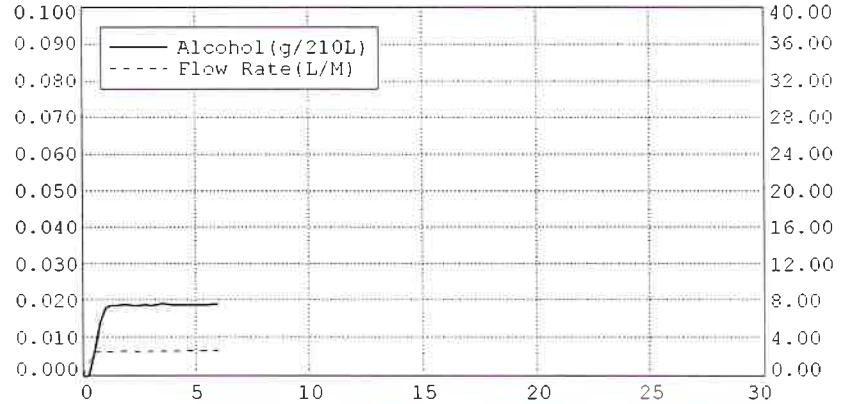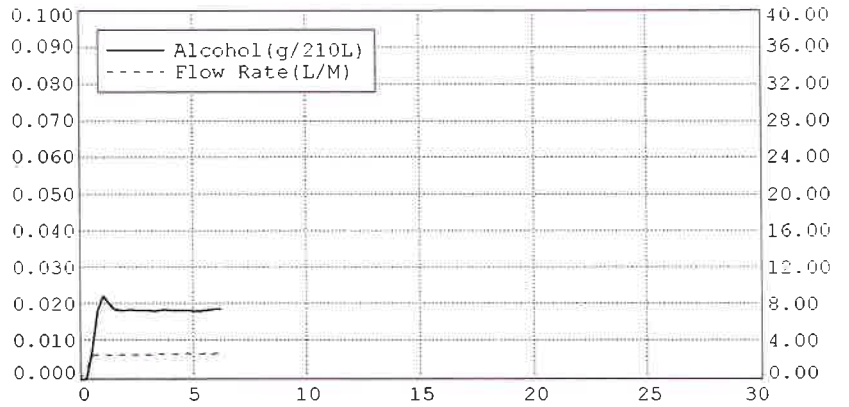



LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100398






Date: 03/28/2024  
 Time: 09:50:11

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 29.59: 0.040  
 LOT #: AG217904  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 831 psi

BLANK TEST	0.000	09:51
INTERNAL STANDARD	VERIFIED	09:51
EXTERNAL STANDARD	0.040	09:51
BLANK TEST	0.000	09:52
EXTERNAL STANDARD	0.040	09:52
BLANK TEST	0.000	09:53
EXTERNAL STANDARD	0.039	09:53
BLANK TEST	0.000	09:54
EXTERNAL STANDARD	0.039	09:54
BLANK TEST	0.000	09:55
EXTERNAL STANDARD	0.039	09:55
BLANK TEST	0.000	09:56

Average = 0.0394  
 Std Dev = 0.0005

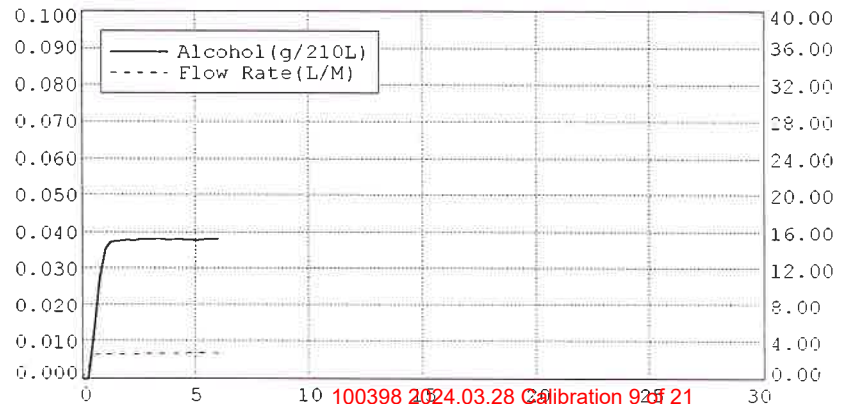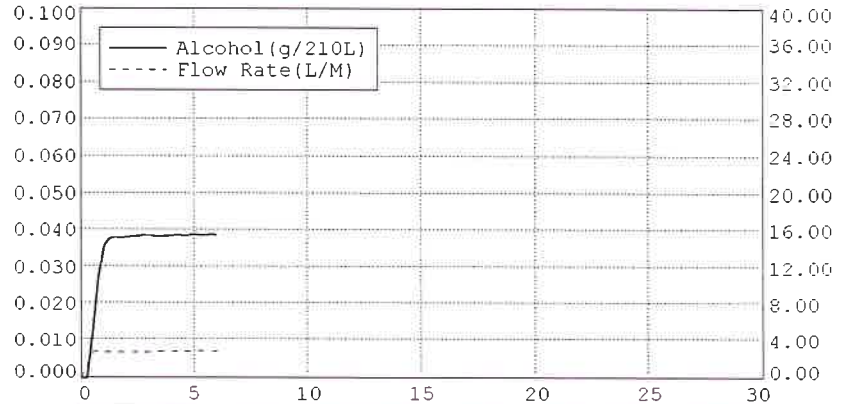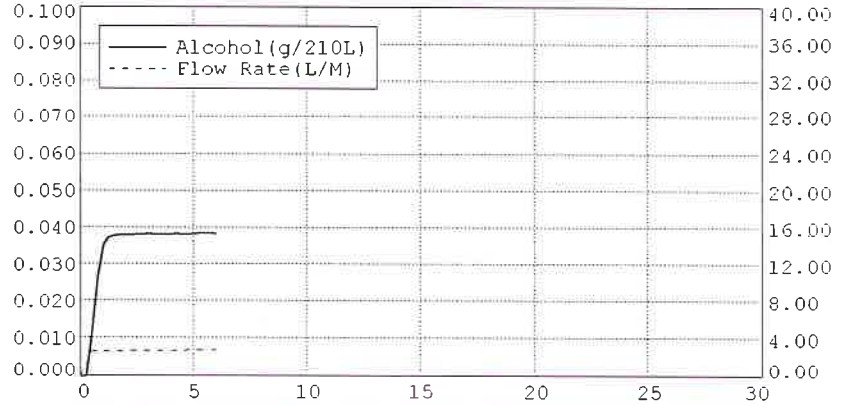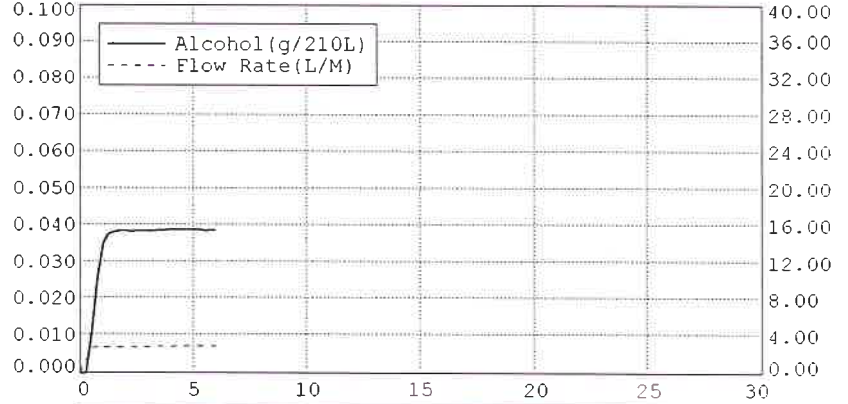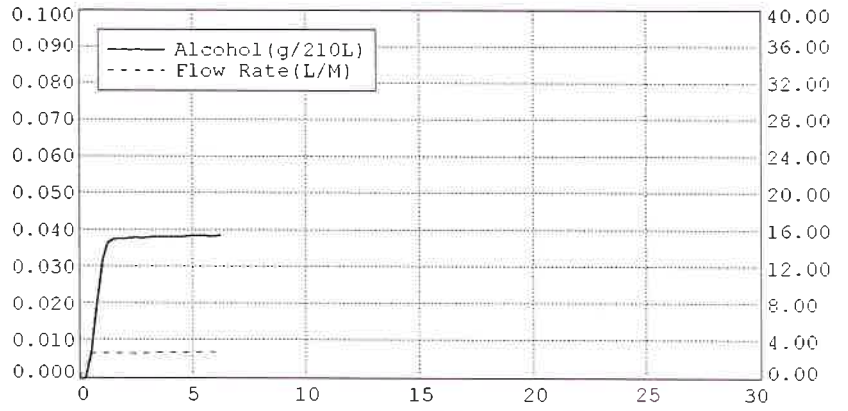

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100398






Date: 03/28/2024  
 Time: 09:57:50

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.60: 0.079  
 LOT #: AG310901  
 EXPIRATION: 04/19/2025  
 TANK PRESSURE: 888 psi

BLANK TEST	0.000	09:58
INTERNAL STANDARD	VERIFIED	09:59
EXTERNAL STANDARD	0.079	09:59
BLANK TEST	0.000	10:00
EXTERNAL STANDARD	0.078	10:00
BLANK TEST	0.000	10:01
EXTERNAL STANDARD	0.079	10:01
BLANK TEST	0.000	10:02
EXTERNAL STANDARD	0.078	10:02
BLANK TEST	0.000	10:03
EXTERNAL STANDARD	0.078	10:03
BLANK TEST	0.000	10:04

Average = 0.0784  
 Std Dev = 0.0005

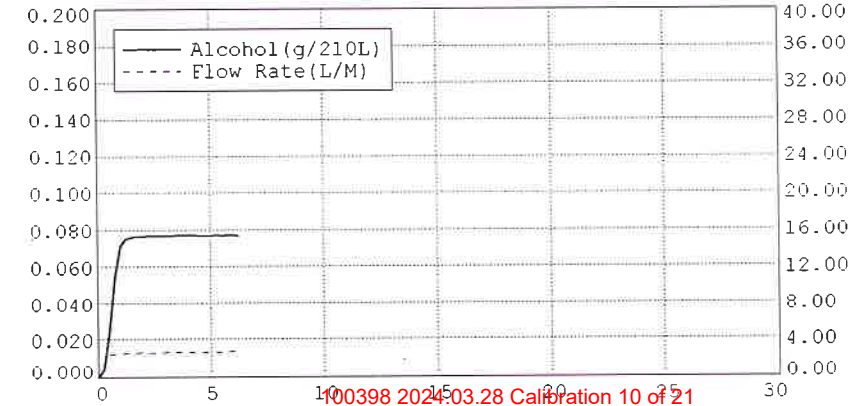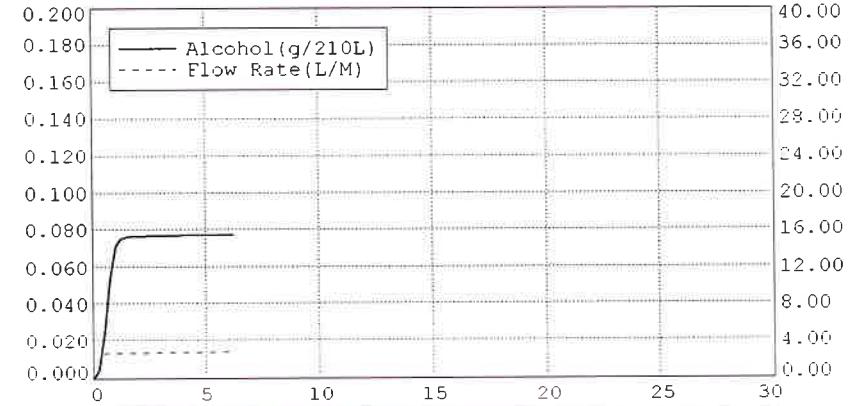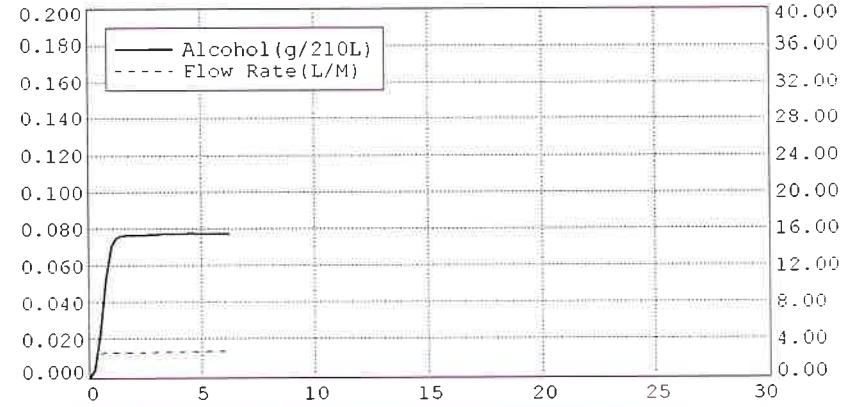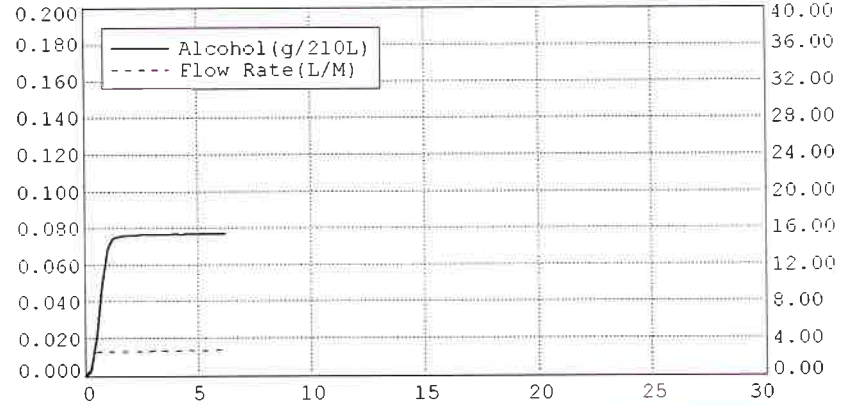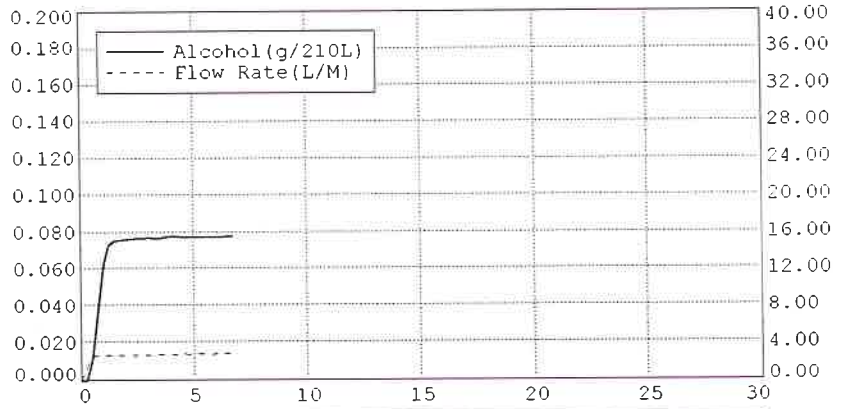

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100398






Date: 03/28/2024  
 Time: 10:07:28

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.60: 0.099  
 LOT #: AG211003  
 EXPIRATION: 04/20/2024  
 TANK PRESSURE: 412 psi

BLANK TEST	0.000	10:08
INTERNAL STANDARD	VERIFIED	10:08
EXTERNAL STANDARD	0.098	10:08
BLANK TEST	0.000	10:09
EXTERNAL STANDARD	0.098	10:09
BLANK TEST	0.000	10:10
EXTERNAL STANDARD	0.098	10:11
BLANK TEST	0.000	10:11
EXTERNAL STANDARD	0.098	10:12
BLANK TEST	0.000	10:13
EXTERNAL STANDARD	0.098	10:13
BLANK TEST	0.000	10:14

Average = 0.0980  
 Std Dev = 0.0000

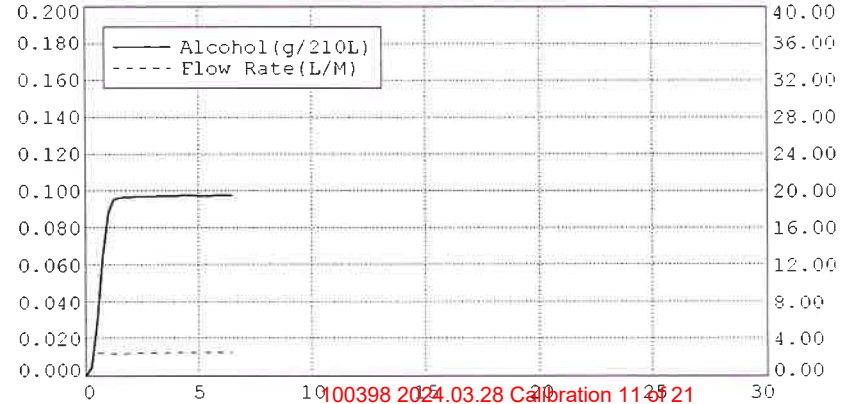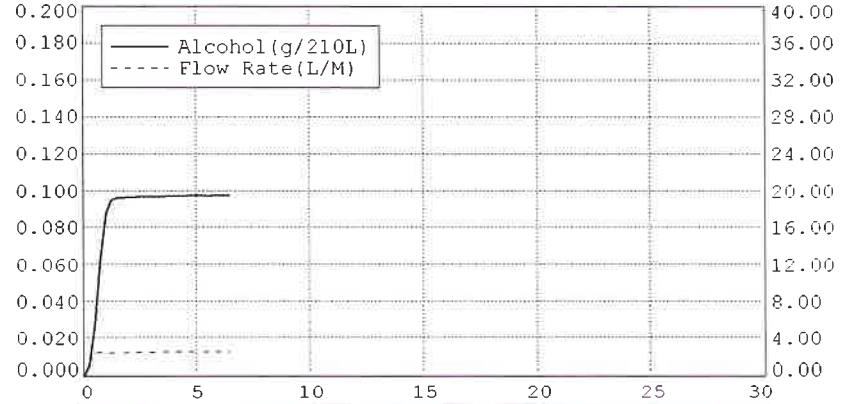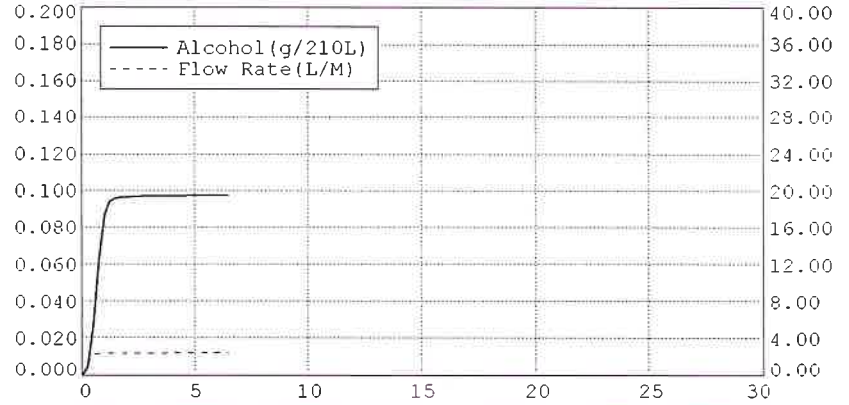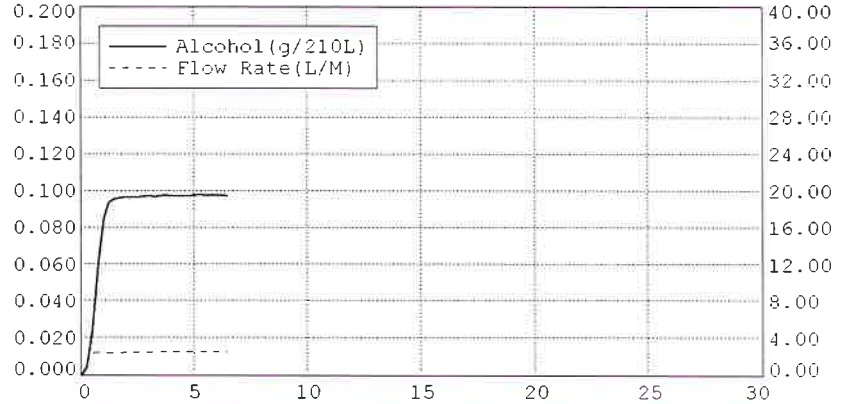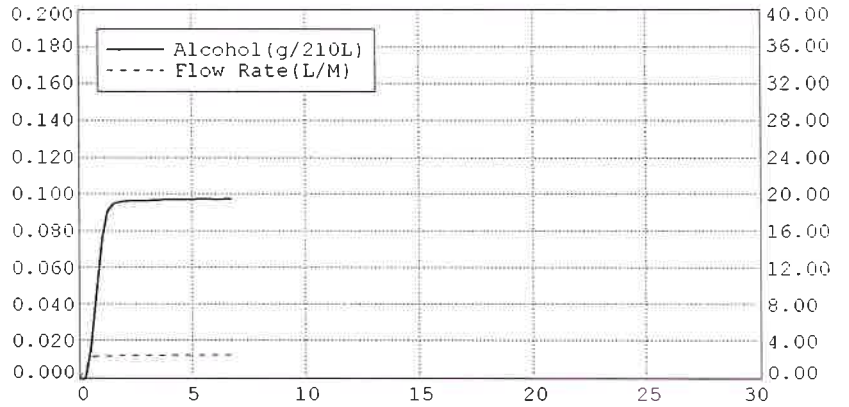



LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100398






Date: 03/28/2024  
 Time: 10:15:36

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.59: 0.148  
 LOT #: AG332004  
 EXPIRATION: 11/16/2025  
 TANK PRESSURE: 627 psi

BLANK TEST	0.000	10:16
INTERNAL STANDARD	VERIFIED	10:16
EXTERNAL STANDARD	0.145	10:17
BLANK TEST	0.000	10:17
EXTERNAL STANDARD	0.146	10:18
BLANK TEST	0.000	10:19
EXTERNAL STANDARD	0.145	10:19
BLANK TEST	0.000	10:20
EXTERNAL STANDARD	0.145	10:20
BLANK TEST	0.000	10:21
EXTERNAL STANDARD	0.145	10:21
BLANK TEST	0.000	10:22

Average = 0.1452  
 Std Dev = 0.0004

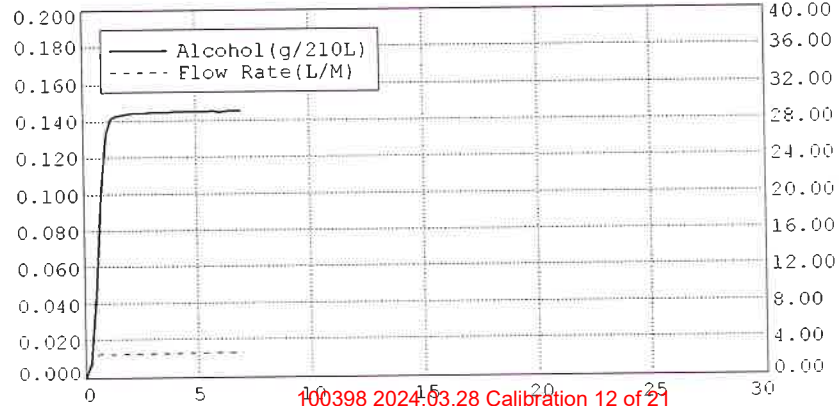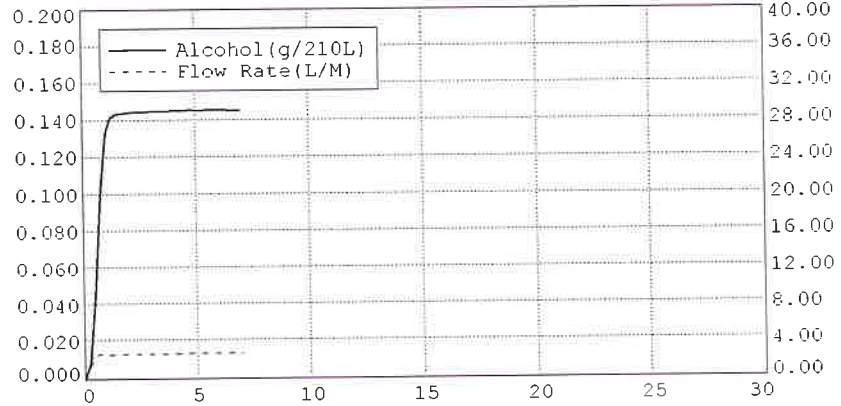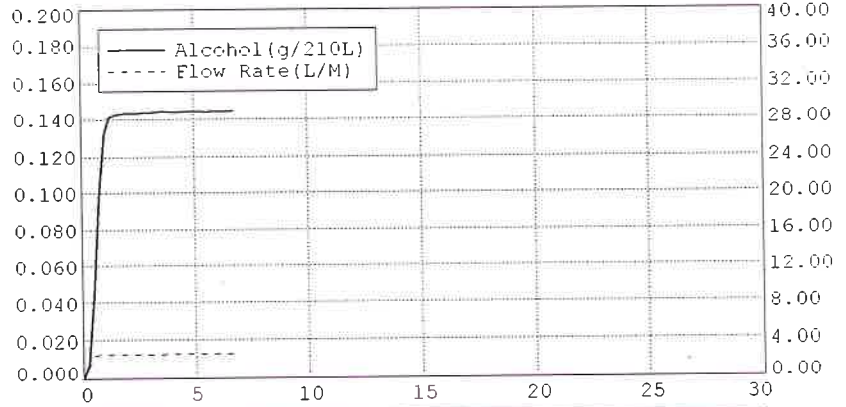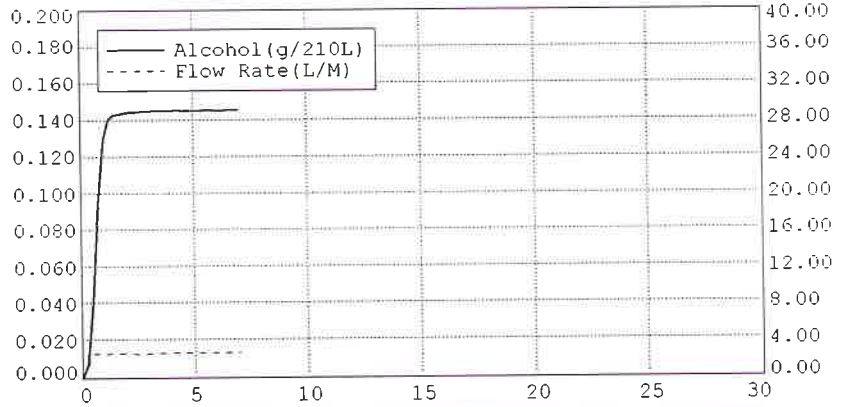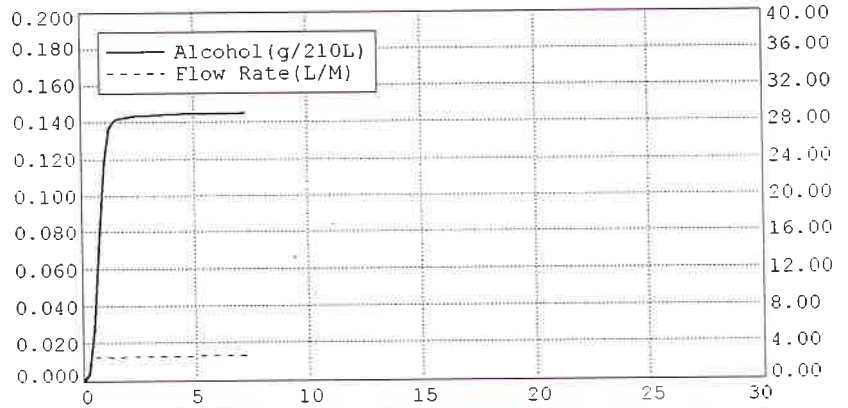

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100398






Date: 03/28/2024  
 Time: 10:24:31

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.60: 0.297  
 LOT #: AG327804  
 EXPIRATION: 10/05/2025  
 TANK PRESSURE: 132 psi

BLANK TEST	0.000	10:25
INTERNAL STANDARD	VERIFIED	10:25
EXTERNAL STANDARD	0.296	10:26
BLANK TEST	0.000	10:26
EXTERNAL STANDARD	0.296	10:27
BLANK TEST	0.000	10:28
EXTERNAL STANDARD	0.295	10:28
BLANK TEST	0.000	10:29
EXTERNAL STANDARD	0.295	10:29
BLANK TEST	0.000	10:30
EXTERNAL STANDARD	0.295	10:30
BLANK TEST	0.000	10:31

Average = 0.2954  
 Std Dev = 0.0005

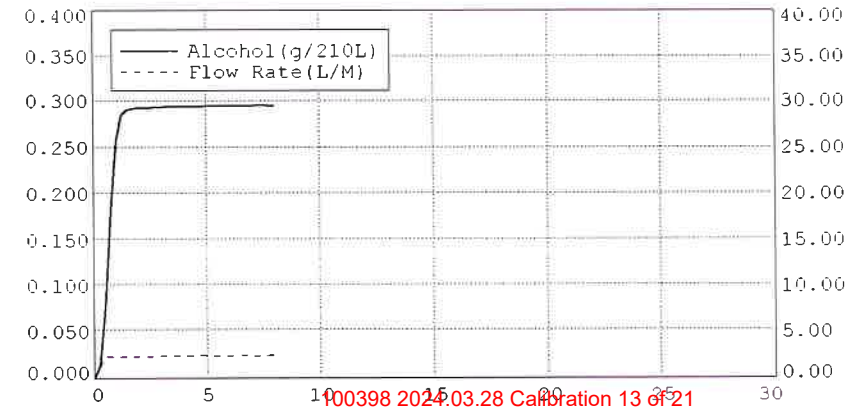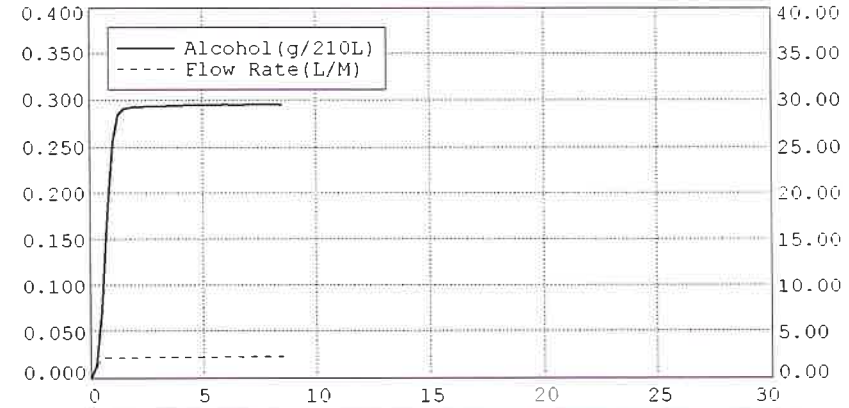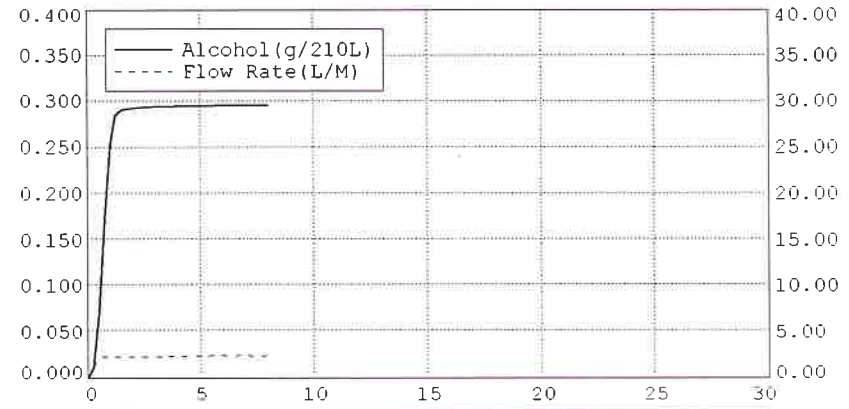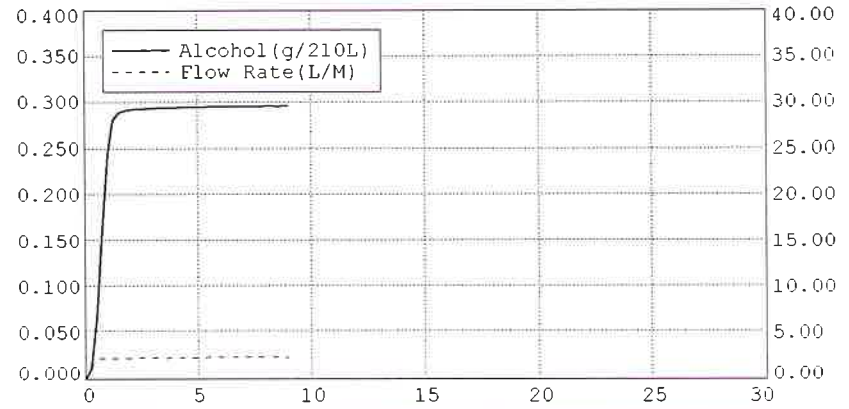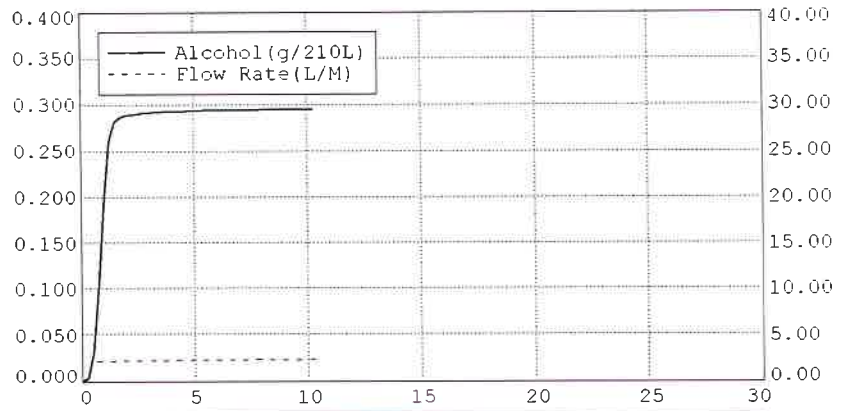

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100398

Date: 03/28/2024

Time: 10:44:12

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CROUSE

OPERATOR'S #: 10747

DEPT/AGENCY:

INCOMPLETE

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.60: 0.079

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD


EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 10:45  
0.000 10:45  
VERIFIED 10:45  
0.079 10:45  
0.000 10:46  
INCOMPLETE 10:48

MNC

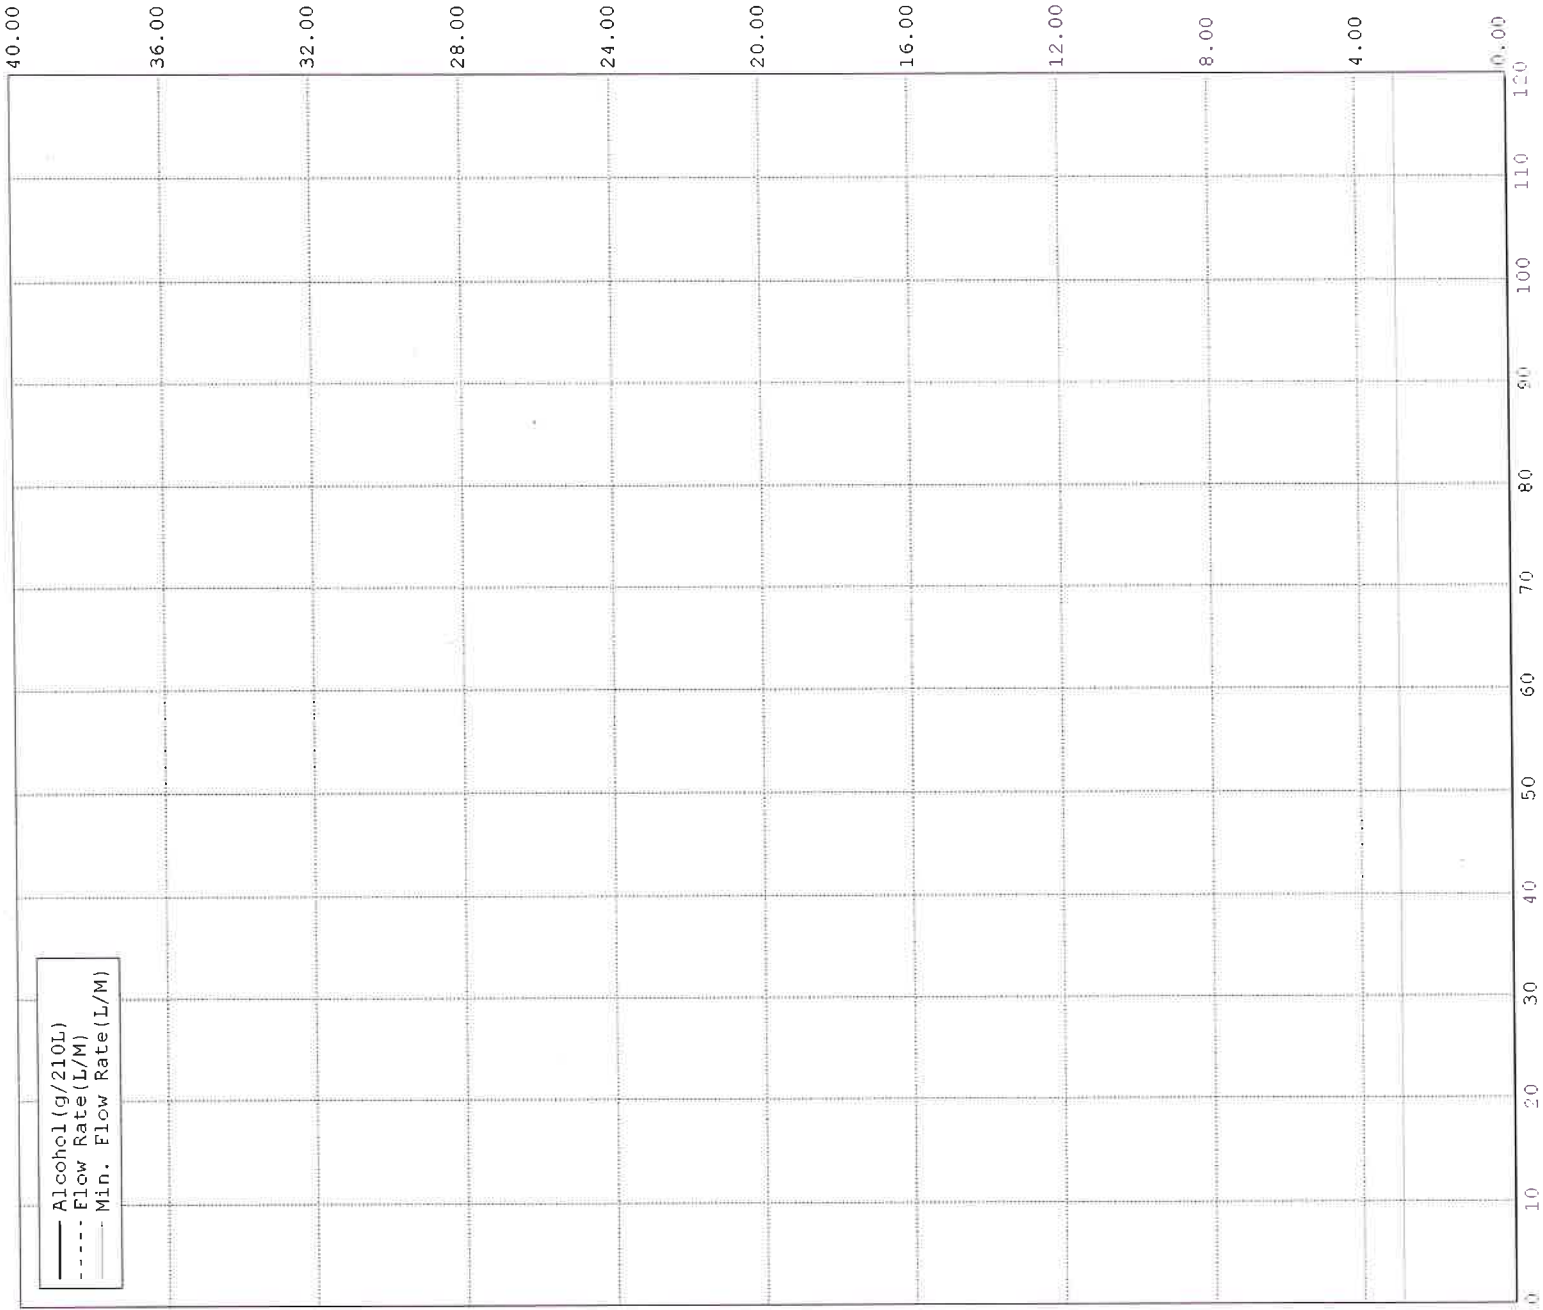



SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100398

Date: 03/28/2024

Time: 10:55:22

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CROUSE

OPERATOR'S #: 10747

DEPT/AGENCY:

MAXIMUM ATTEMPTS EXCEEDED

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.60: 0.079

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

PASSED 10:56

BLANK TEST 0.000 10:56

INTERNAL STANDARD

VERIFIED 10:56

EXTERNAL STANDARD


0.079 10:56

BLANK TEST 0.000 10:57

SUBJECT SAMPLE XXX 10:58

Maximum Attempts Exceeded

MNC

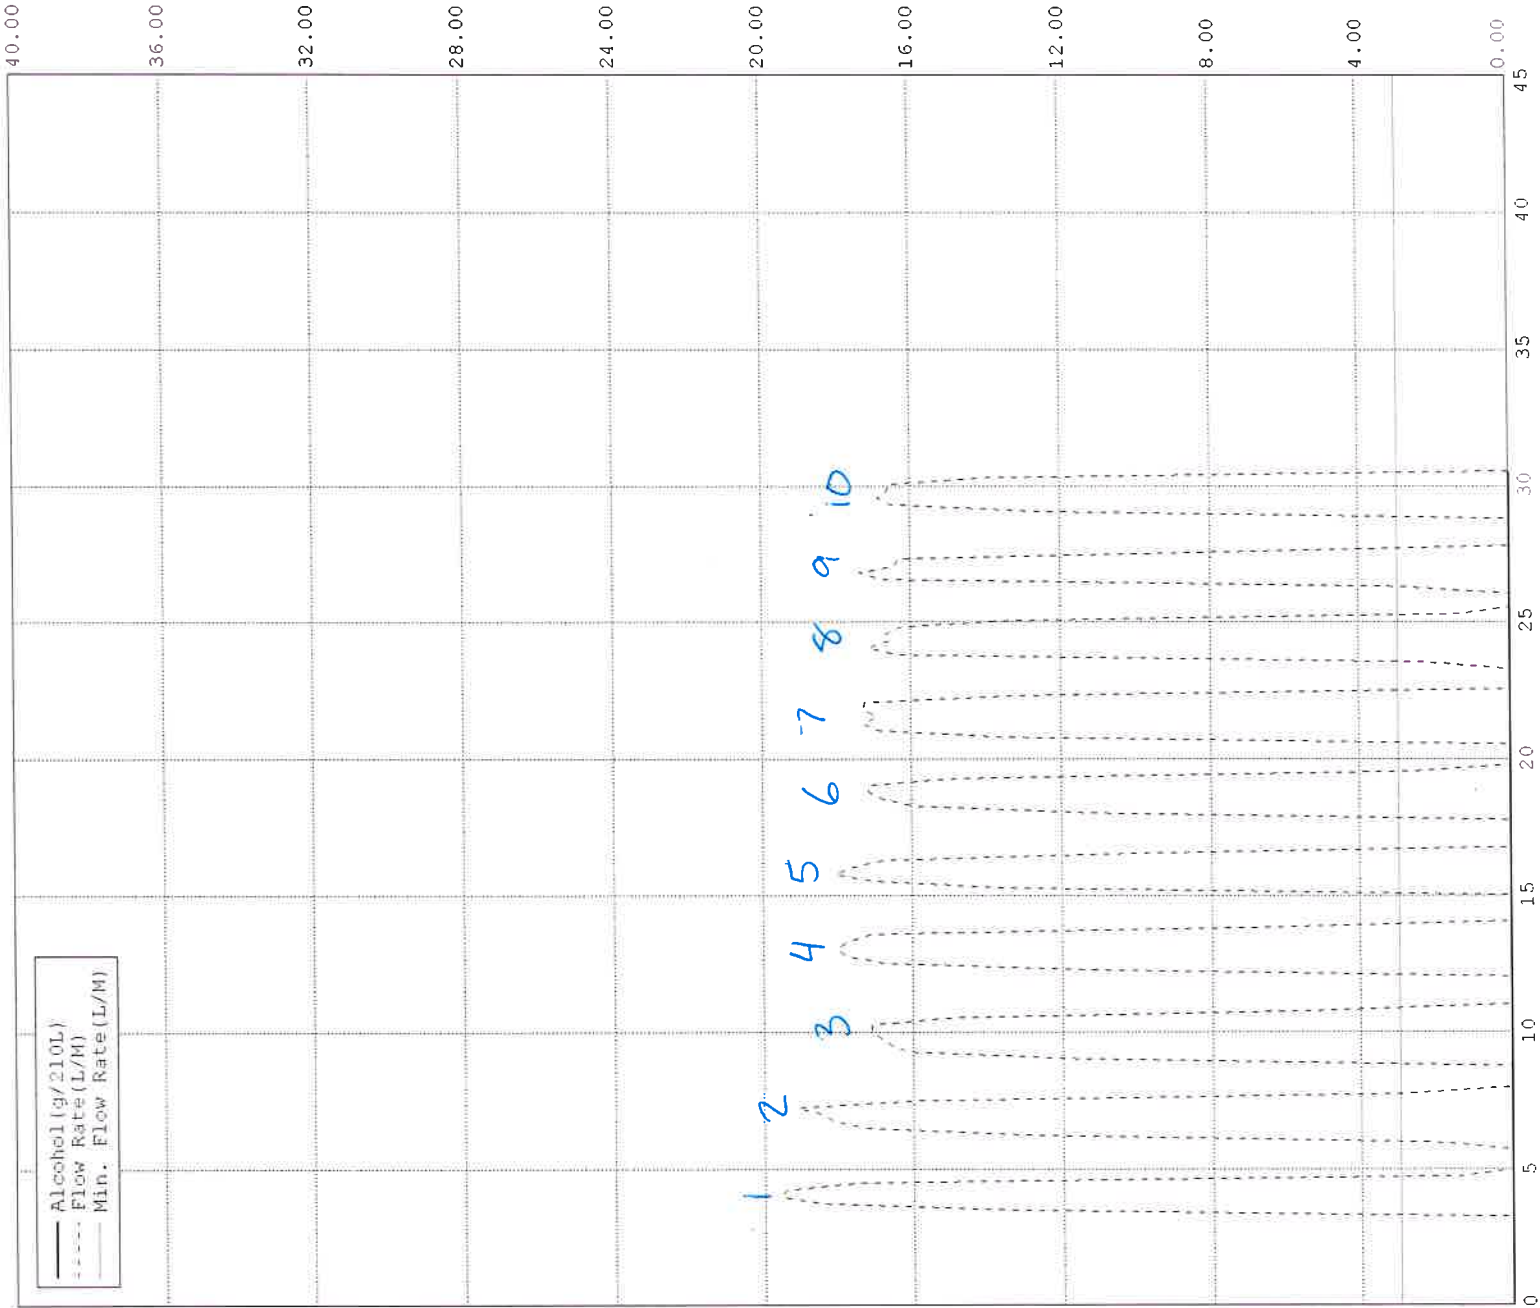

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100398

Date: 03/28/2024

Time: 11:14:35

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CROUSE

OPERATOR'S #: 10747

DEPT/AGENCY:

INVALID

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.60: 0.079

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

PASSED 11:16

BLANK TEST

0.000 11:16

INTERNAL STANDARD

VERIFIED 11:16

EXTERNAL STANDARD

0.079 11:16


BLANK TEST

0.000 11:17

SUBJECT SAMPLE

INVALID 11:18

MNC

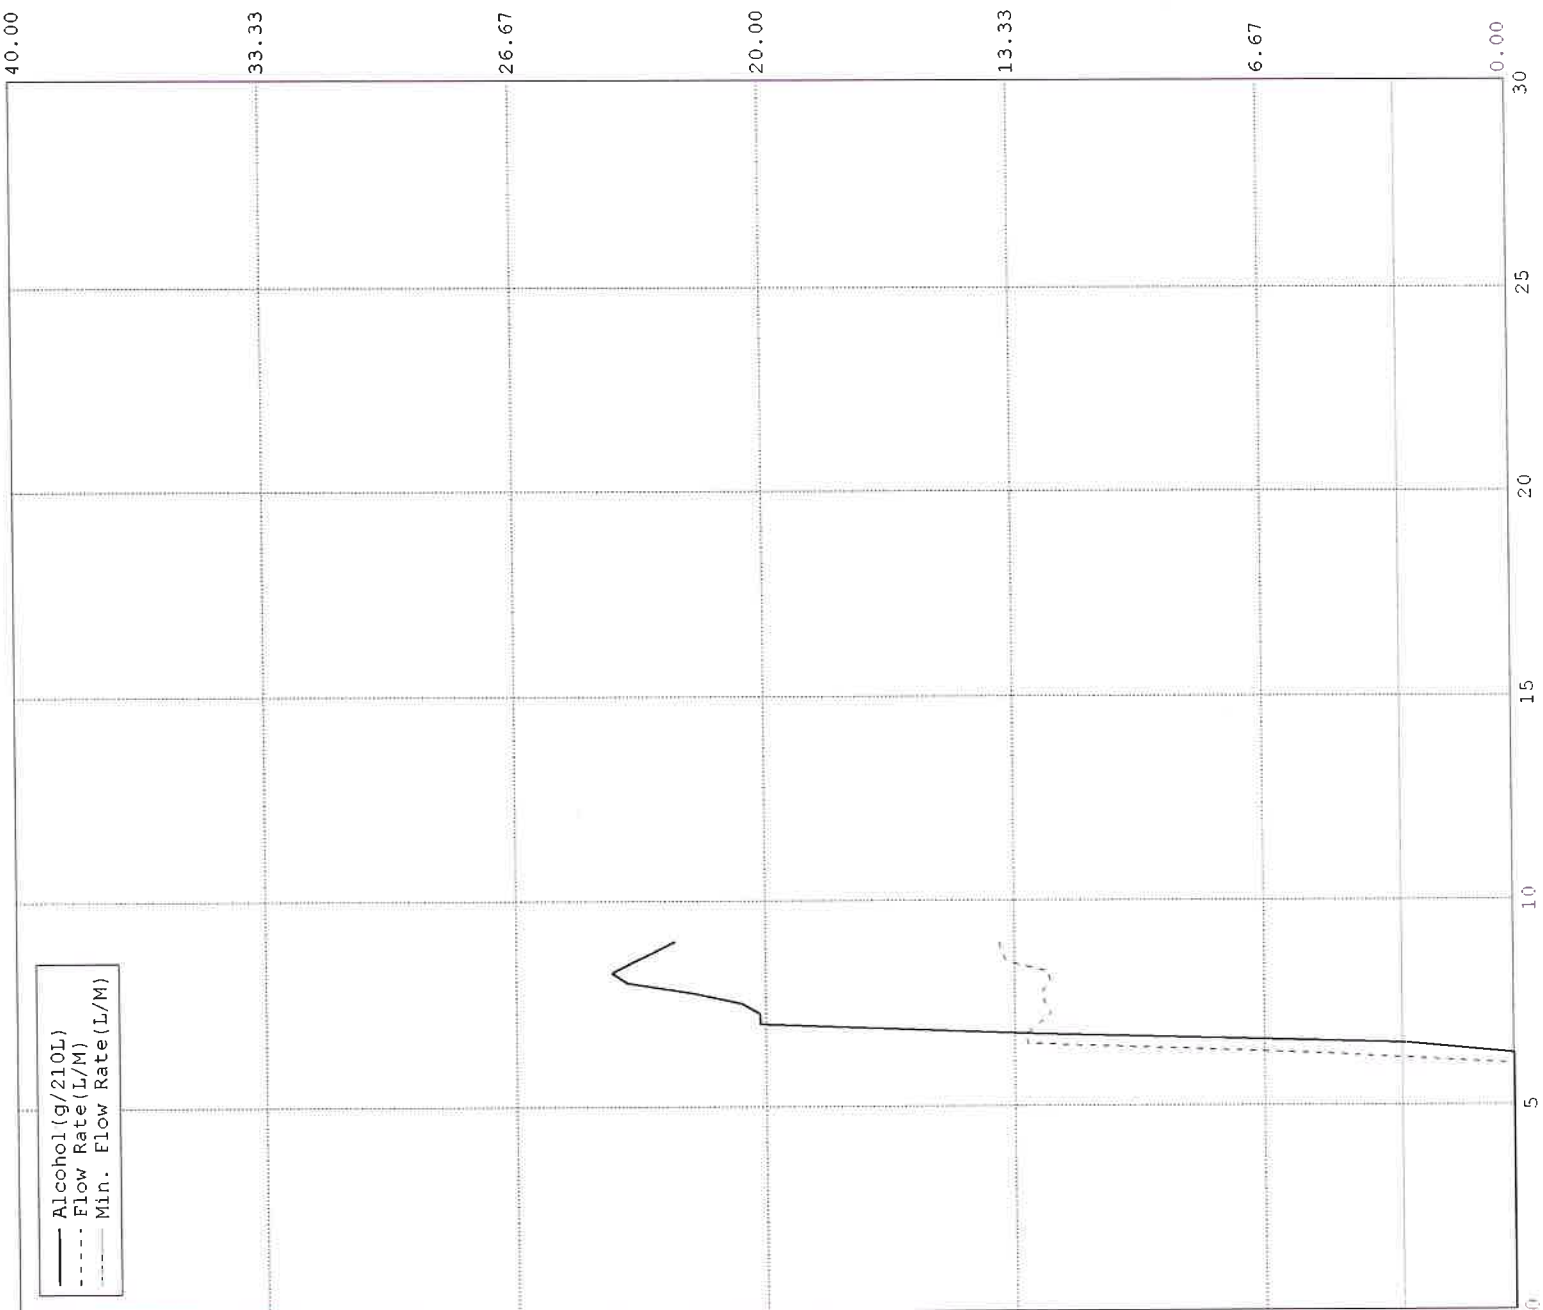

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100398

Date: 03/28/2024

Time: 11:19:31

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CROUSE

OPERATOR'S #: 10747

DEPT/AGENCY:

RFI

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.60: 0.079

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD


EXTERNAL STANDARD

BLANK TEST

PASSED 11:21  
0.000 11:21  
VERIFIED 11:21  
0.079 11:21  
0.000 11:22

RFI DETECTED

MNC

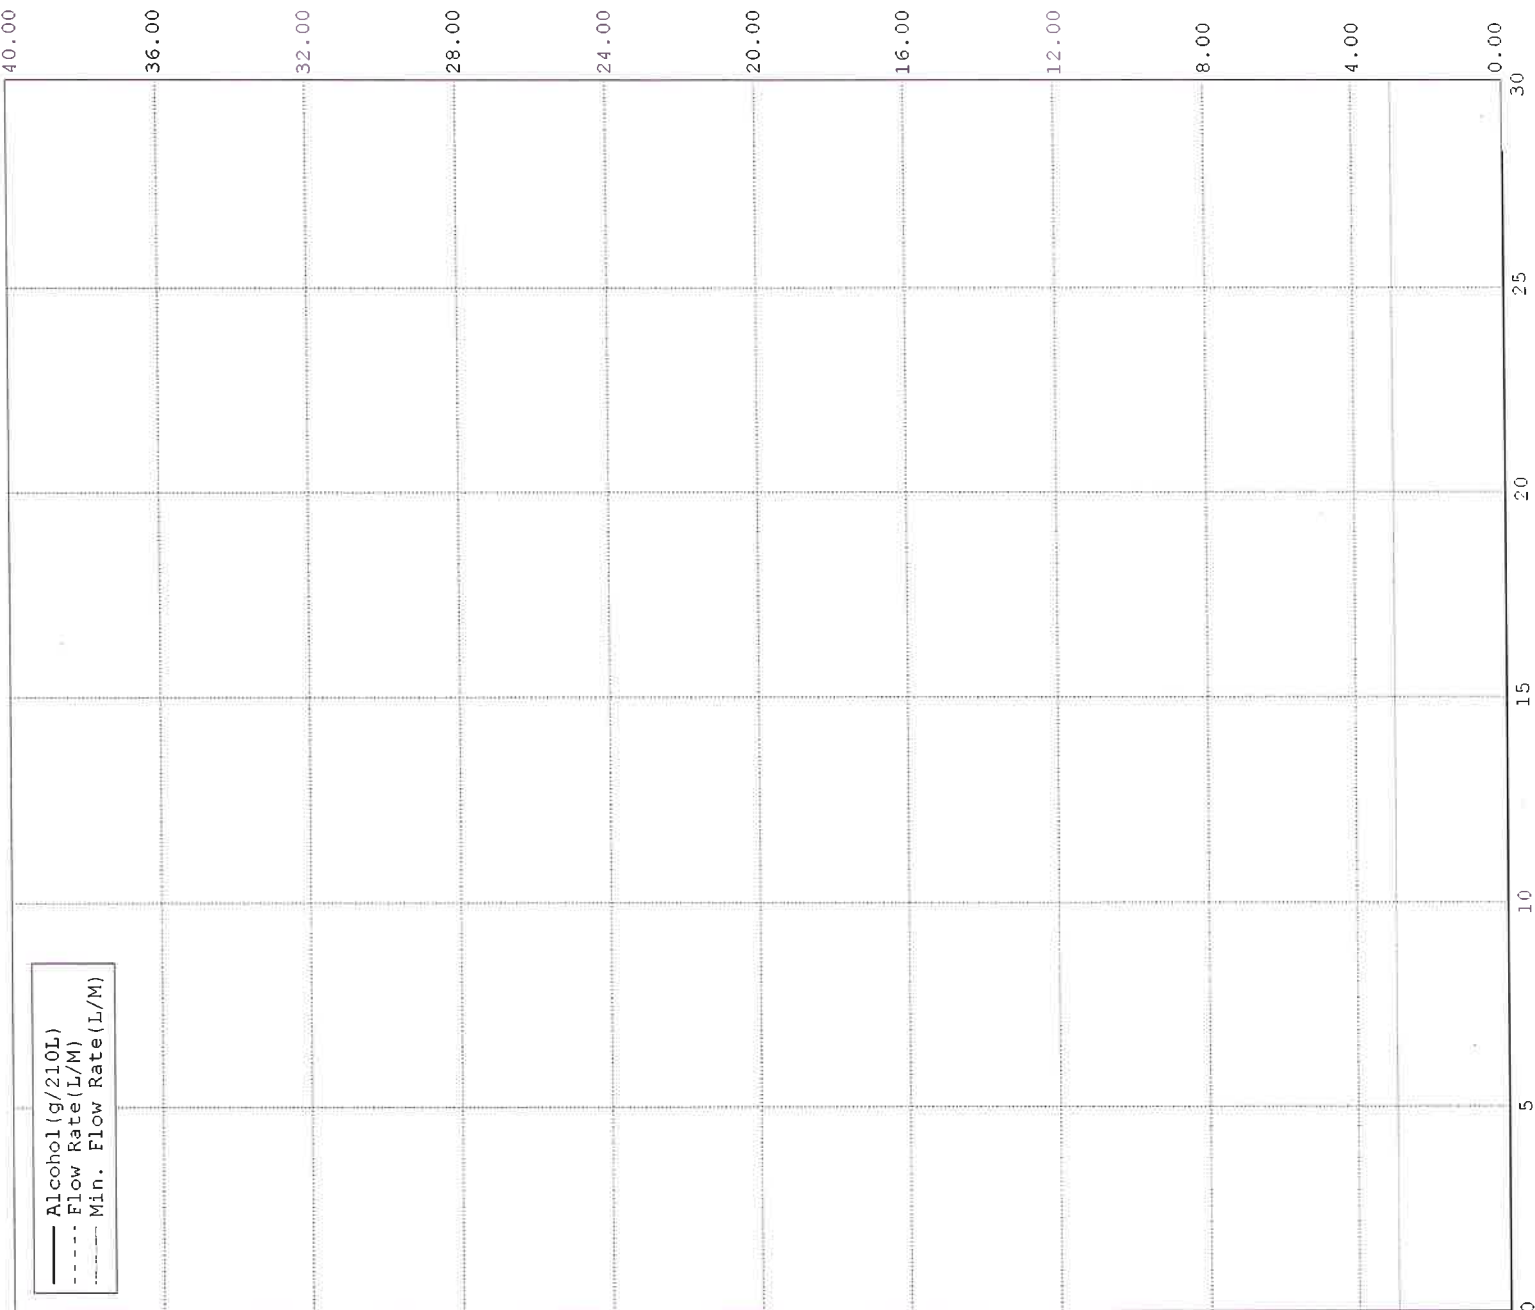

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100398

Date: 03/28/2024  
Time: 13:27:49

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
MEGAN CROUSE  
OPERATOR'S #: 10747

DEPT/AGENCY:  
INTERFERENCE - ACETONE  
CASE/REPORT: XXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.61: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 13:28  
BLANK TEST 0.000 13:28  
INTERNAL STANDARD VERIFIED 13:29  
Xg = 0.082 (2.29%)  
EXTERNAL STANDARD 0.079 13:29  
X[f] = 0.0789 (-0.0030) (0.0000)  
BLANK TEST 0.000 13:30  
SUBJECT SAMPLE XXX 13:30  
X[1] = 0.1068 (-0.0199) (-0.0023)

Interference Detected

Filter 2 Average: -0.0031 MNC 3/29/24  
Filter 3 Average: 0.0002  
MNC 3/29/24

MNC

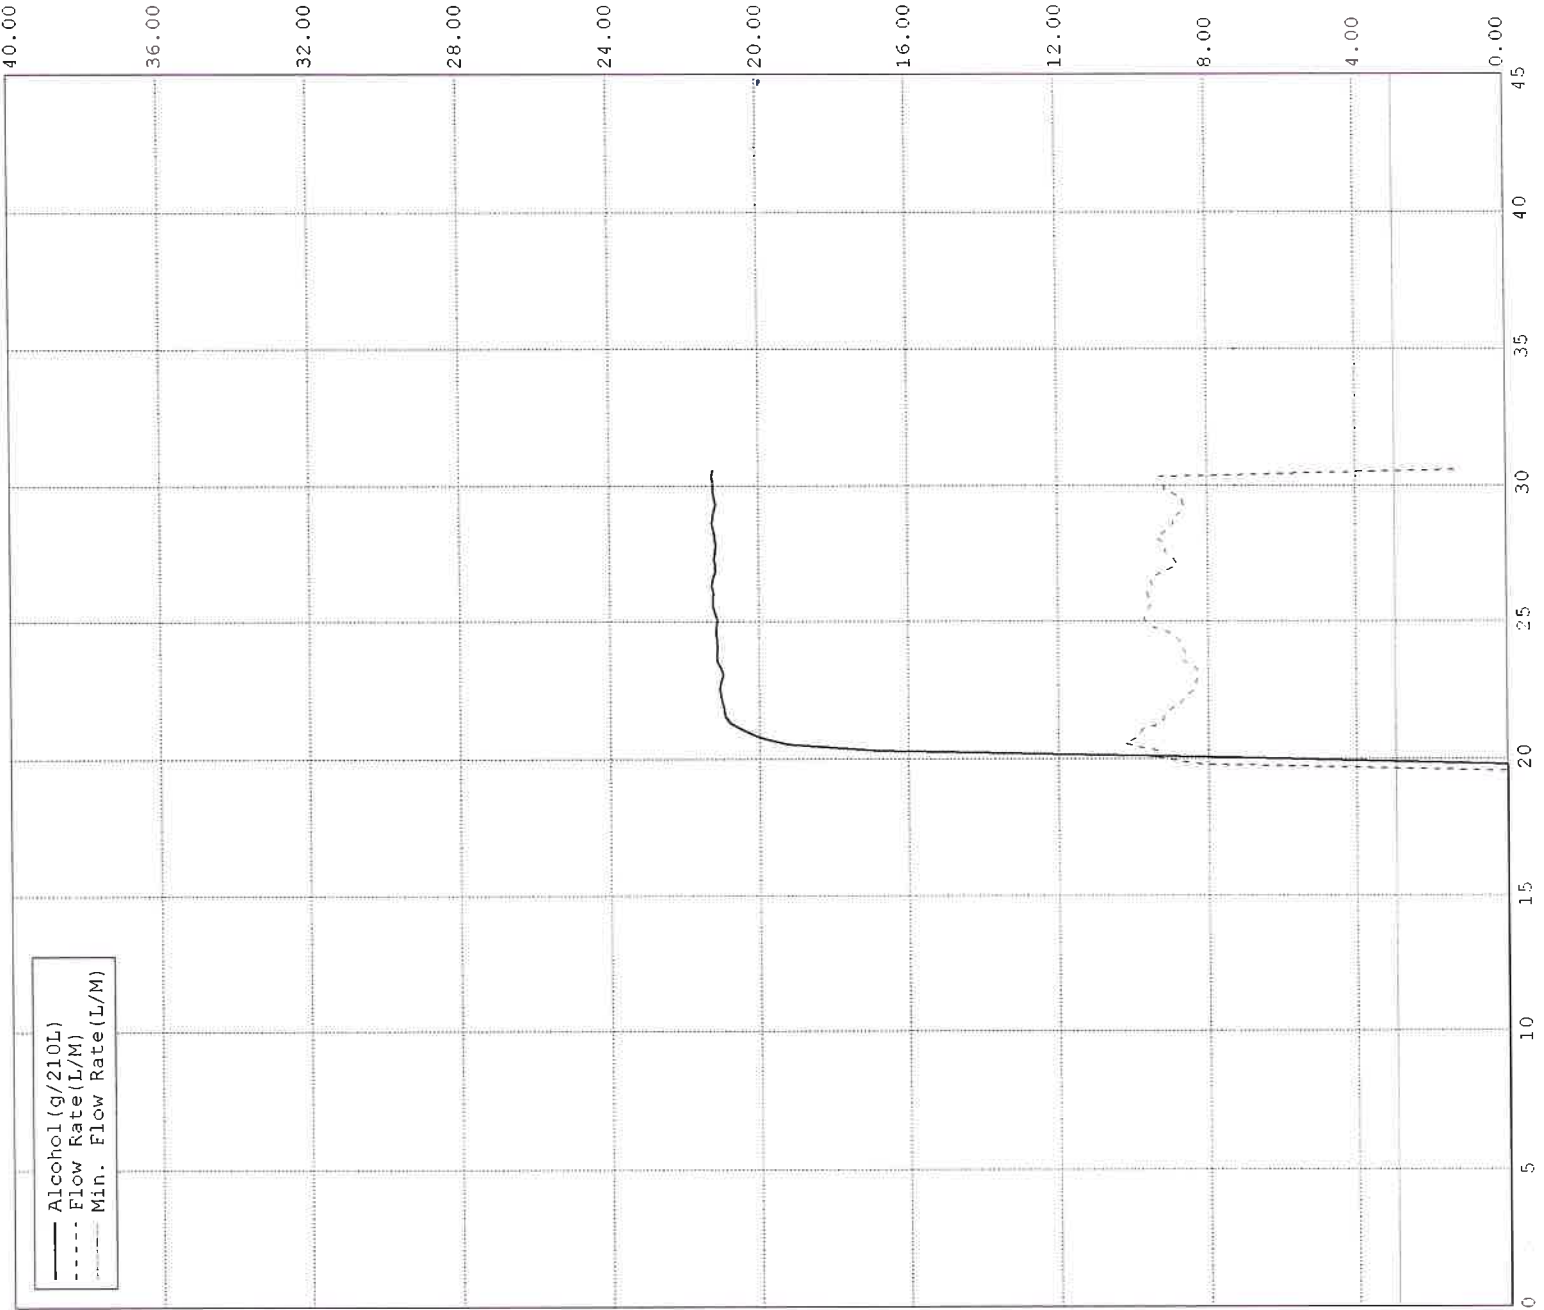

SUBJECT TEST

Alaska Department of Public Safety  
DATA MASTER dmt: 100398

Date: 03/28/2024  
Time: 13:32:55

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
MEGAN CROUSE  
OPERATOR'S #: 10747


DEPT/AGENCY:  
INTERFERENCE - IPA  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.60: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 13:33  
BLANK TEST 0.000 13:34  
INTERNAL STANDARD VERIFIED 13:34  
Xq = 0.082 (2.51%) 0.079 13:34  
EXTERNAL STANDARD (0.0005)  
X[1] = 0.0790 (-0.0030) 0.000 13:35  
BLANK TEST XXX 13:36  
SUBJECT SAMPLE X[1] = 0.1191 (-0.0288) (-0.0008)

Interference Detected

MNC

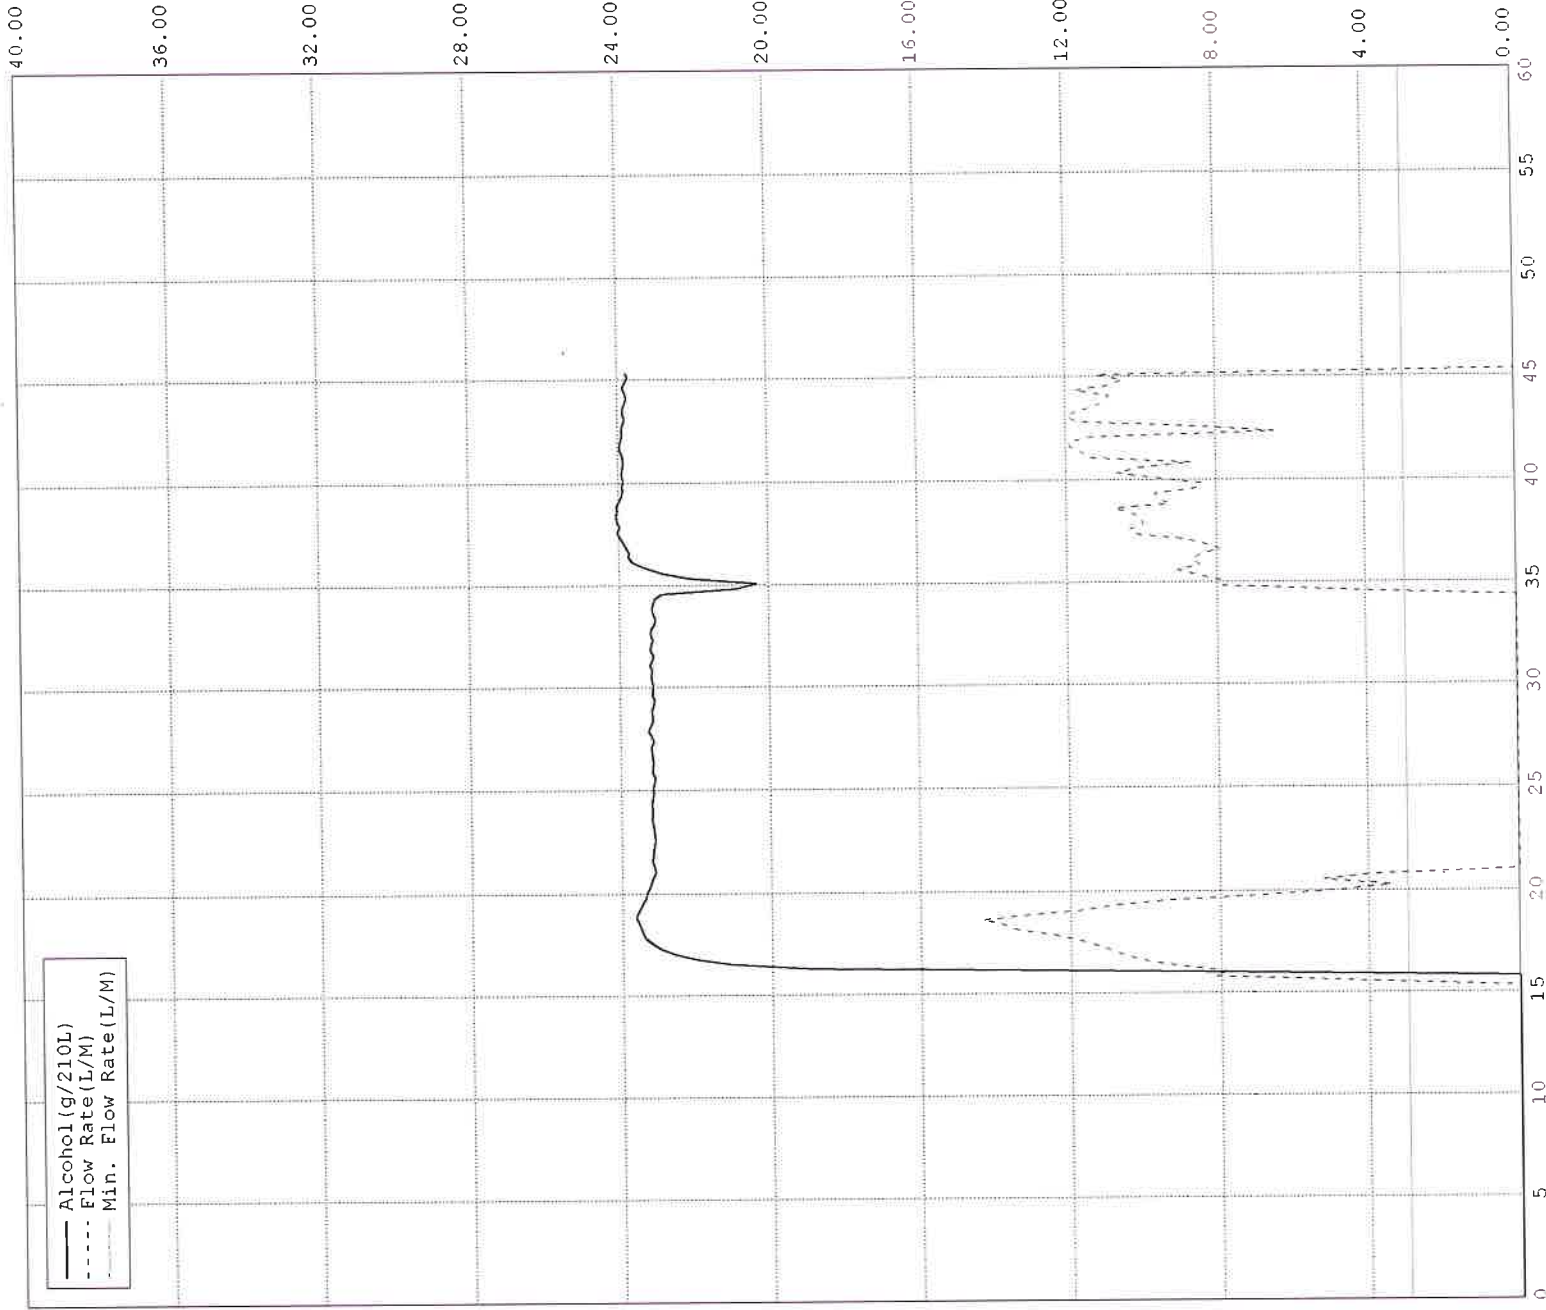



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100398

Date: 03/28/2024  
Time: 13:20:26

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
MEGAN CROUSE  
OPERATOR'S #: 10747

DEPT/AGENCY:  
INTERFERENCE - NEGATIVE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.60: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 13:21  
BLANK TEST 0.000 13:21  
INTERNAL STANDARD VERIFIED 13:21  
Xg = 0.081 (1.53%)  
EXTERNAL STANDARD 0.079 13:21  
X[1] = 0.0788 (-0.0033) (0.0002)  
BLANK TEST 0.000 13:22  
SUBJECT SAMPLE (Vol=1.95L) 0.094 13:23  
X[1] = 0.0943 (0.0019) (-0.0011)  
BLANK TEST 0.000 13:24  
EXTERNAL STANDARD 0.078 13:24  
X[1] = 0.0783 (-0.0030) (-0.0001)  
BLANK TEST 0.000 13:25

MNC

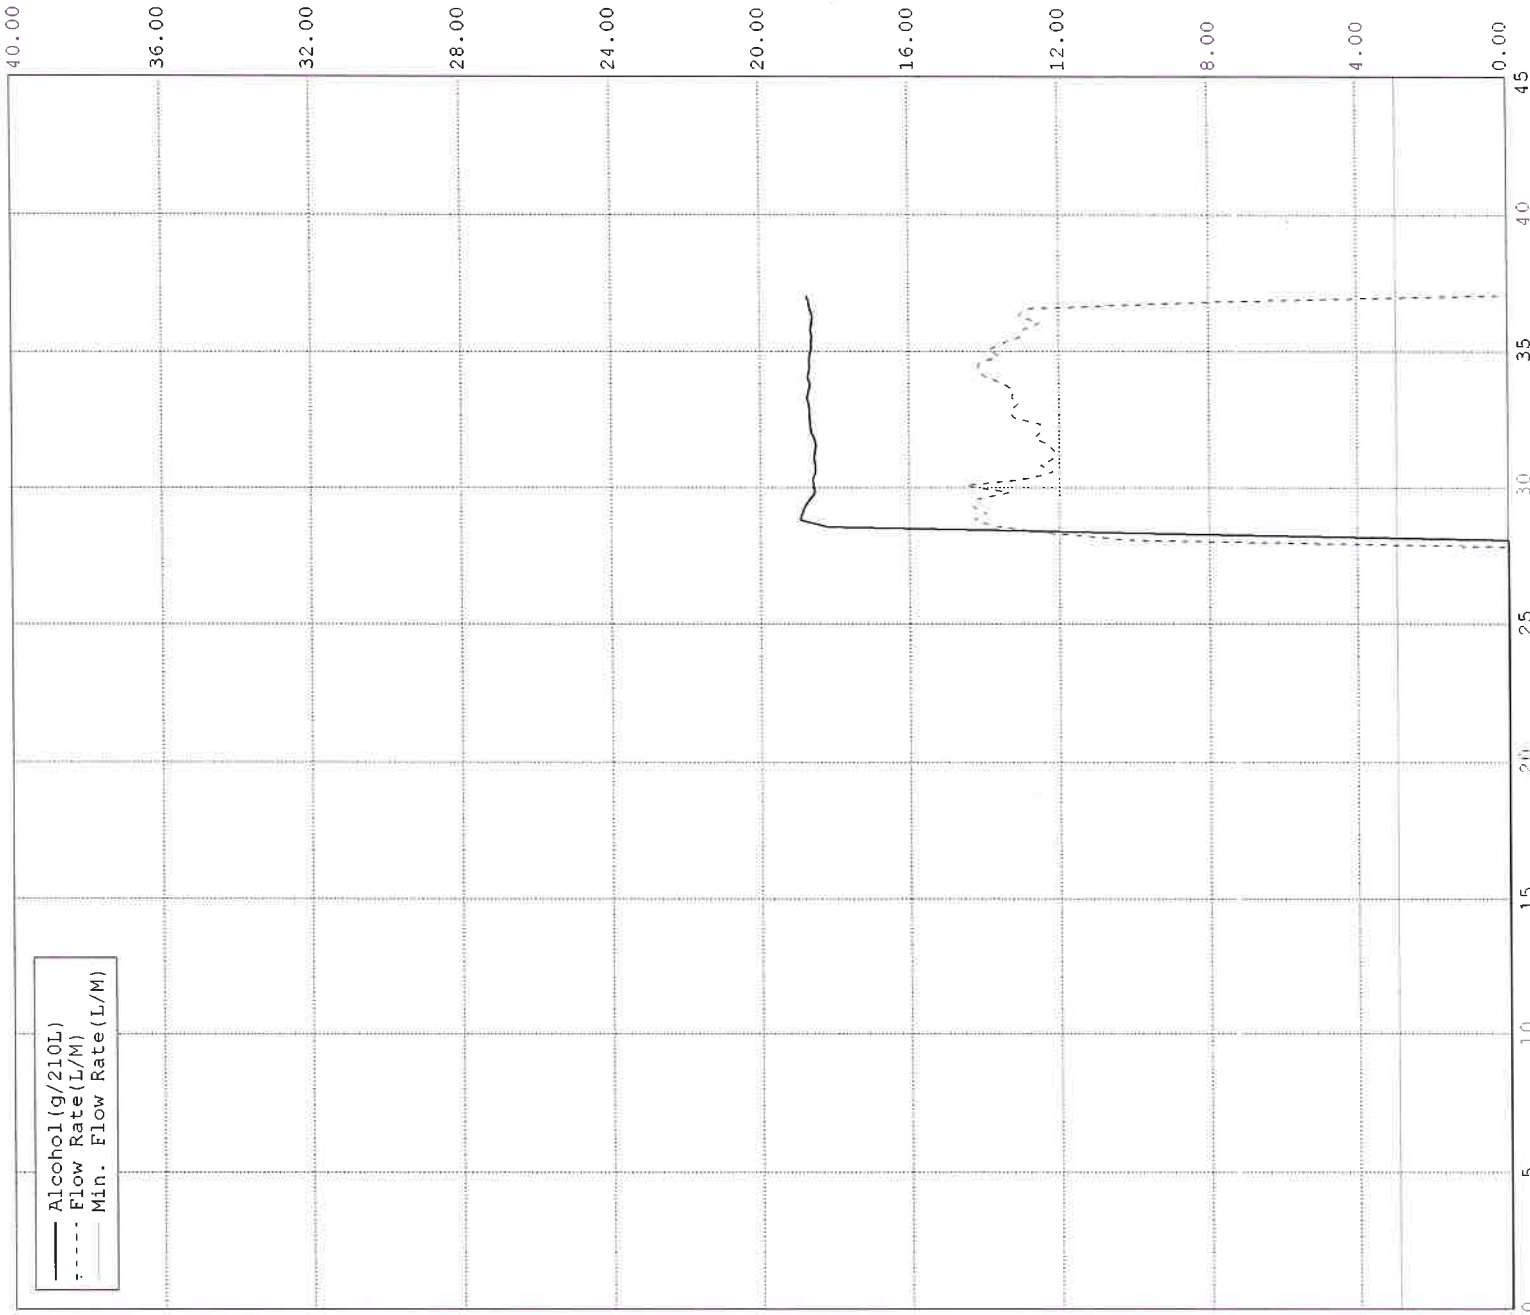



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100398

Date: 03/28/2024  
Time: 13:58:01

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
MEGAN CROUSE  
OPERATOR'S #: 10747

DEPT/AGENCY:  
NON-DRINKING SUBJECT TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.61: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	13:59
BLANK TEST	0.000	13:59
INTERNAL STANDARD	VERIFIED	13:59
EXTERNAL STANDARD	0.079	13:59
BLANK TEST	0.000	14:00
SUBJECT SAMPLE (Vol=1.68L)	0.000	14:00
BLANK TEST	0.000	14:01
EXTERNAL STANDARD	0.079	14:02
BLANK TEST	0.000	14:02

MNC

