



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories

Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100348

Report Issue Date: 12/05/2022
Date Received: 2022-09-07
Condition of Item: Good

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

Start Date 11/09/2022 - As Found - **End Date 11/09/2022** As Found - Evaluation Analyst: Derek Walton
 As Found Conditions - Barometric Pressure (inHg): 29.34 Barometer Used: Fisher S/N 221250180 Temperature (C): 21.8
 Relative Humidity (%): 21

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG100401	0.019	0.019	0.020	0.020	0.020	0.020	0.020
0.080	0.078	AG113402	0.076	0.076	0.076	0.076	0.076	0.076	0.076
0.300	0.294	AG130502	0.286	0.286	0.286	0.286	0.286	0.286	0.286

Start Date 11/14/2022 - As Left - **End Date 11/14/2022**
 As Left Conditions - Barometric Pressure (inHg): 29.97 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.7 Relative
 Humidity (%): 21

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.020	AG100401	0.019	0.020	0.020	0.020	0.020	0.020	+/- 0.002	
0.040	0.040	AG111710	0.039	0.039	0.039	0.039	0.039	0.039	+/- 0.003	
0.080	0.080	AG113402	0.077	0.078	0.078	0.077	0.078	0.078	+/- 0.003	
0.100	0.100	AG211003	0.098	0.098	0.098	0.098	0.098	0.098	+/- 0.003	
0.150	0.150	AG134205	0.147	0.147	0.147	0.147	0.147	0.147	+/- 0.004	
0.300	0.301	AG130502	0.297	0.296	0.296	0.296	0.296	0.296	+/- 0.008	

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Technically and administratively reviewed by Brandi Barnett on 12/05/2022

Results authorized by Colleen O'Bryant on 12/05/2022
colleen.obryant@alaska.gov

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100348 Analyst: C.O Bryant Start Date: 11/14/23

- Diagnostic Test (attached)
- Adjust voltages, if needed
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Internal Standard value \leq 3.00%
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.5 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 29.97 Temperature (C): 22.7 Relative Humidity (%): 21

Linearity Test (attached)

0.020g/210L Mnf: <u>Argas</u>	Lot: <u>AG100401</u>	Exp: <u>1/4/23</u>
0.040g/210L Mnf: <u>Argas</u>	Lot: <u>AG111710</u>	Exp: <u>4/27/23</u>
0.080g/210L Mnf: <u>Argas</u>	Lot: <u>AG113402</u>	Exp: <u>5/14/23</u>
0.100g/210L Mnf: <u>Argas</u>	Lot: <u>AG108404</u> ^{AG211003}	Exp: <u>3/25/23</u> ^{4/20/24} ^{11/14/23}
0.150g/210L Mnf: <u>Argas</u>	Lot: <u>AG134205</u>	Exp: <u>12/8/23</u>
0.300g/210L Mnf: <u>Argas</u>	Lot: <u>AG130502</u>	Exp: <u>11/01/23</u>

Functional Tests (attached)

- Incomplete
- Invalid
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)
- Interference (Volatiles)

Acetone Mnf: Lifeloc Lot: 21DP41158 Level: 0.100 Exp: 4/29/23

Simulator S/N: SD1200 Verification Performed?

Isopropanol Mnf: Lifeloc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: DP4176 Verification Performed?

Neg. Control Mnf: Lifeloc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: DB4162 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 210958384 Calibration Due Date: 11/9/23

- Verify stylus is calibrated
- Non-Drinking Subject Test
- Reset Options
- Upload
- Clear Memory
- Remove Tank Prior to Shutdown
- Verification of Calibration (VOC)
- Calibration End Date: 11/14/23

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100348

Date: 11/14/2022
Time: 12:14:23

VERSIONS
DMT: 3.02 ✓
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 44.5°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.71 V PASSED
(1.01 V - 2.35 V)
Cooler Voltage = 1.71 V PASSED
(1.04 V - 2.44 V)
Bias Voltage = 79 V PASSED
(48 V - 112 V)
Chopper Freq = 540 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.9 in

PUMP INFO

Flow Rate = 4.379 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.001 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.091 1.47% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100348

Date: 11/14/2022
Time: 1:51 PM

Temperatures (°C)

Sample Cell: 48.9°C
Breath Tube: 44.5°C

Current Barometer 30.0 in
Volume (Ltr) 1.48

Settings

Lamp: 1.74 V
Bias: 80 V
Cooler: 1.82 V
Chopper: 538 Hz

Voltages (V)

Flow: 1.03 V
Detector: 0.023 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100348

Date: 09/20/2018
Time: 14:41:22

OPERATOR NAME:
DEREK WALTON
CERTIFICATE #: 9508

Ca = 0.1000
CAL = 0.951429 0.800 <= CAL < 1.200
b1 = 0.0003 0.0000 <= b1 < 0.0040
b2 = 0.0052 0.0010 <= b2 < 0.0100
b3 = 0.0004 0.0000 <= b3 < 0.0040
Xq = 0.0893 0.0500 <= Xq < 0.2000
a21 = 1.182097 1.050 <= a21 < 1.300
a31 = 0.540738 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100348

Date: 11/14/2022
Time: 13:54:33


SUBJECT NAME:
TEST TEST
LICENSE #: MIN VOLUME

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 22-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080	TARGET AT 29.98: 0.080	LOT #: AG113402	EXPIRATION: 05/14/2023
DIAGNOSTIC CHECK	PASSED	13:56	
INTERNAL STANDARD	0.000	13:56	
EXTERNAL STANDARD	VERIFIED	13:56	
INTERNAL STANDARD	0.077	13:56	
EXTERNAL STANDARD	0.000	13:57	
INTERNAL STANDARD	0.000	13:58	
EXTERNAL STANDARD	0.000	13:59	
INTERNAL STANDARD	0.078	13:59	
EXTERNAL STANDARD	0.000	14:00	

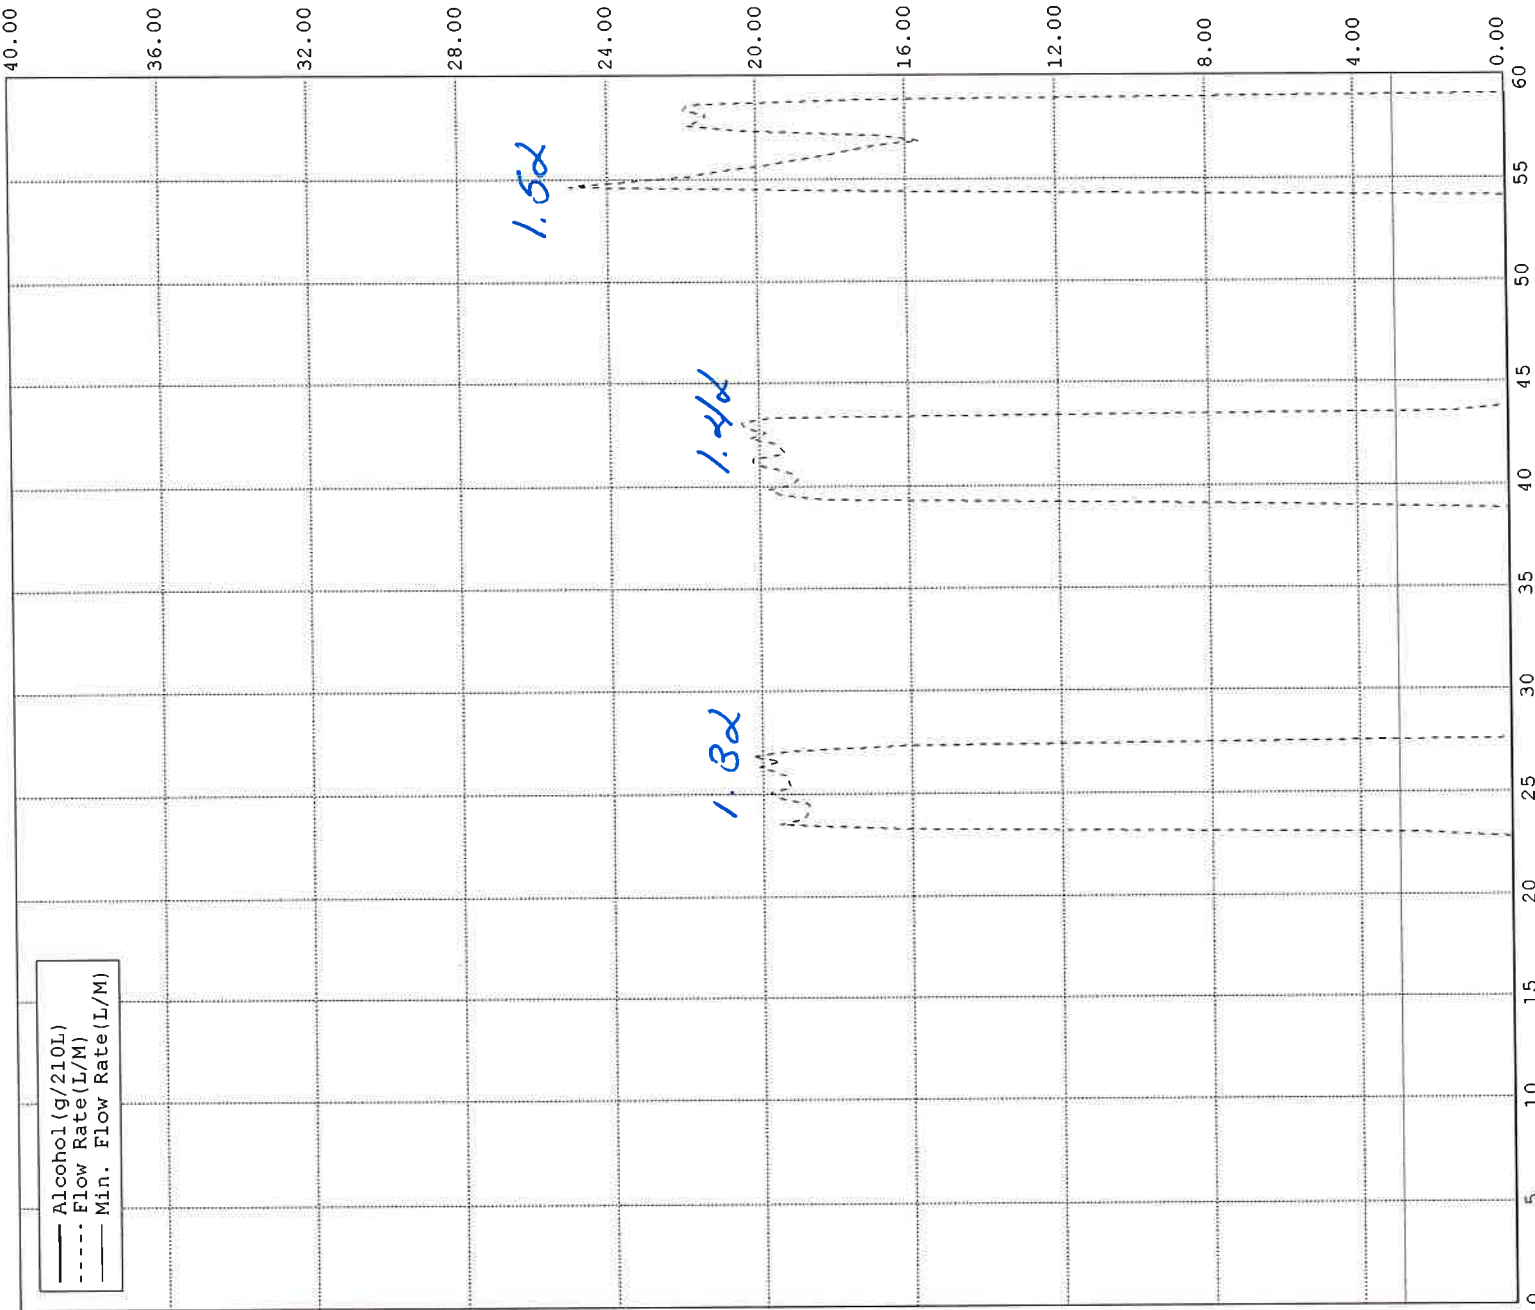

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100348

Date: 11/14/2022
 Time: 14:08:56

SUPERVISOR NAME:
 COLLEEN S OBRyant
 OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0198	0.0004
0.040	0.0390	0.0000
0.080	0.0776	0.0005
0.100	0.0980	0.0000
0.150	0.1470	0.0000
0.301	0.2962	0.0004

SLOPE = 0.984831
 R² = 0.999981

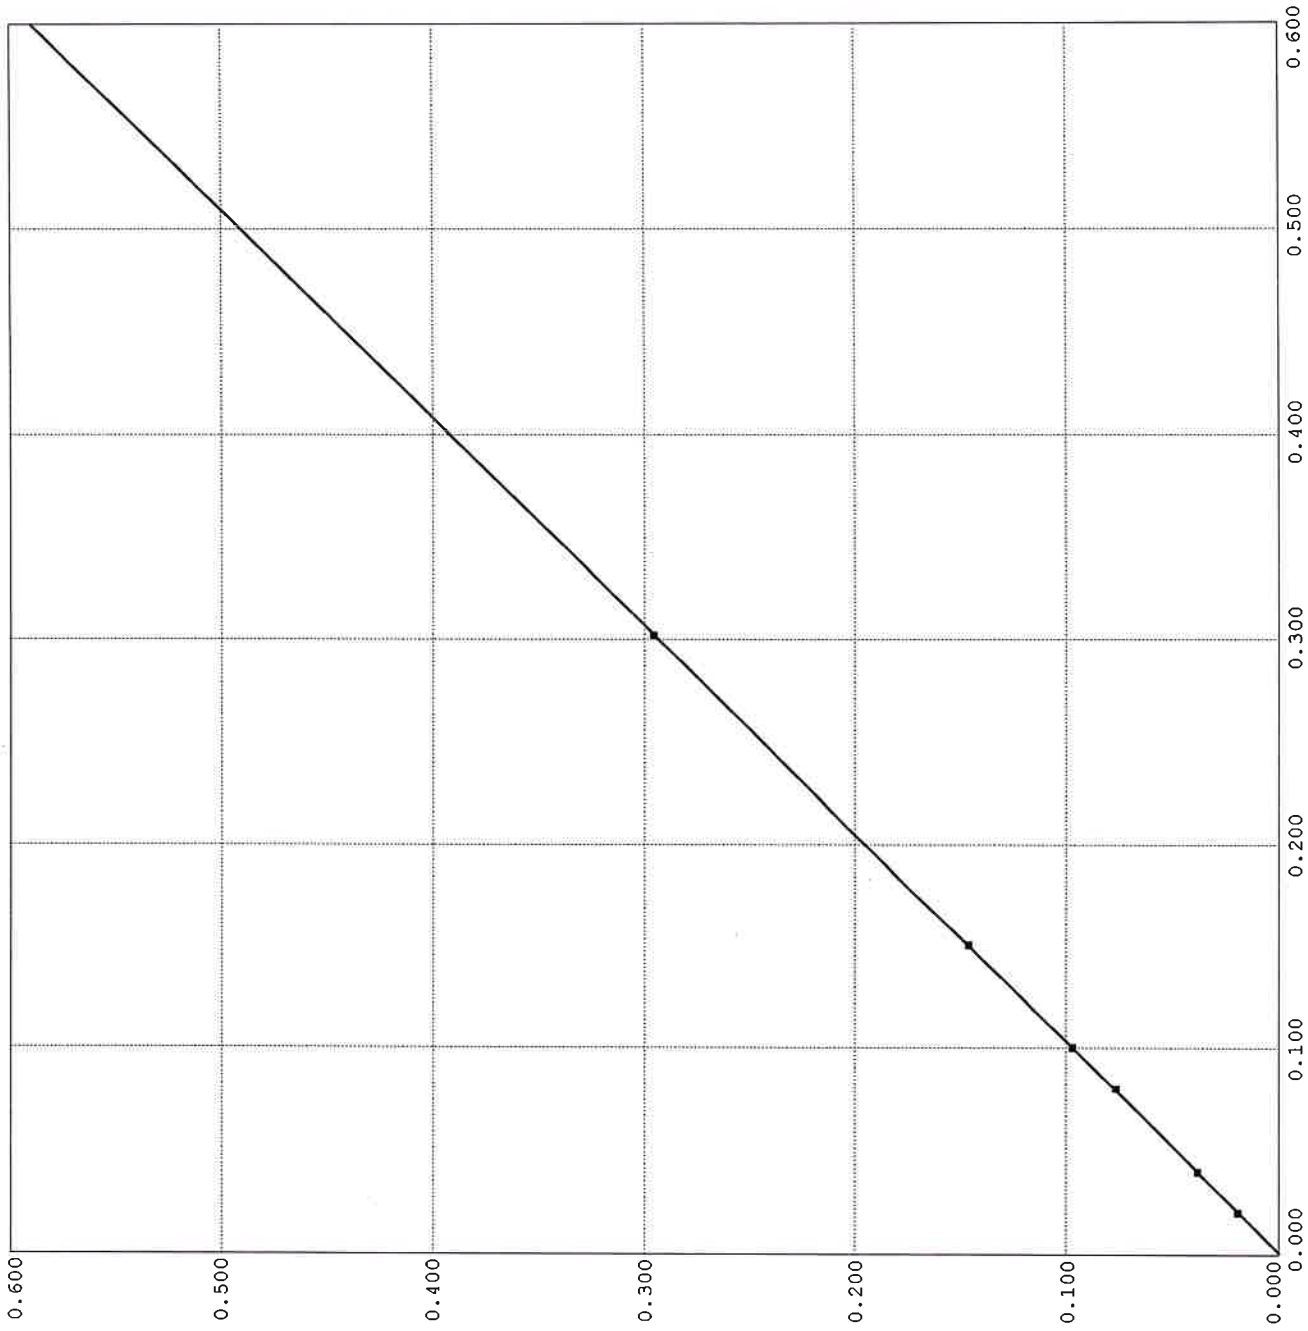

CS

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100348






Date: 11/14/2022
 Time: 14:20:27

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 30.00: 0.020
 LOT #: AG100401
 EXPIRATION: 01/04/2023
 TANK PRESSURE: 419 psi

BLANK TEST	0.000	14:21
INTERNAL STANDARD	VERIFIED	14:21
EXTERNAL STANDARD	0.019	14:21
BLANK TEST	0.000	14:22
EXTERNAL STANDARD	0.020	14:22
BLANK TEST	0.000	14:23
EXTERNAL STANDARD	0.020	14:24
BLANK TEST	0.000	14:24
EXTERNAL STANDARD	0.020	14:25
BLANK TEST	0.000	14:26
EXTERNAL STANDARD	0.020	14:26
BLANK TEST	0.000	14:27

Average = 0.0198
 Std Dev = 0.0004

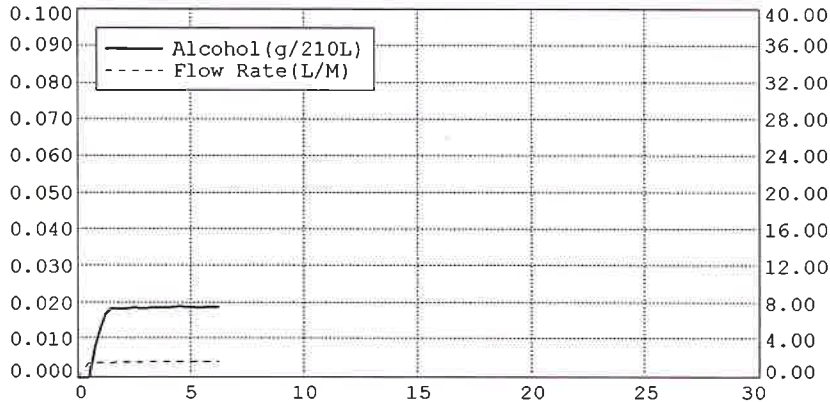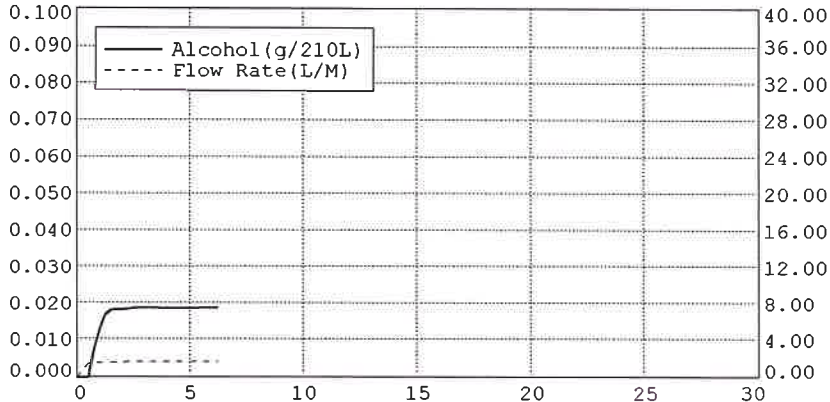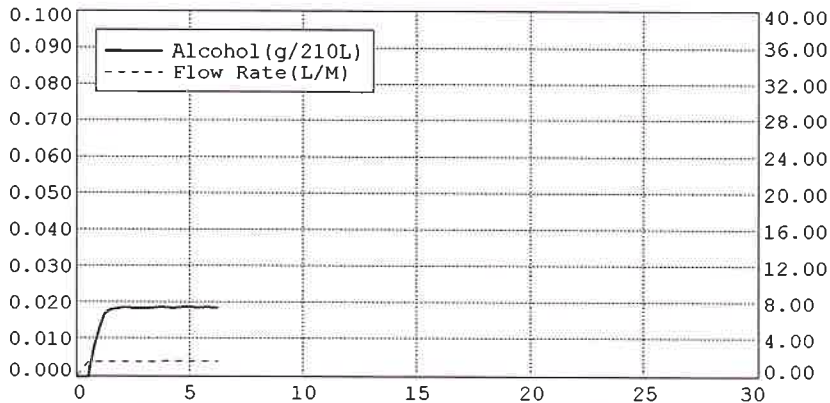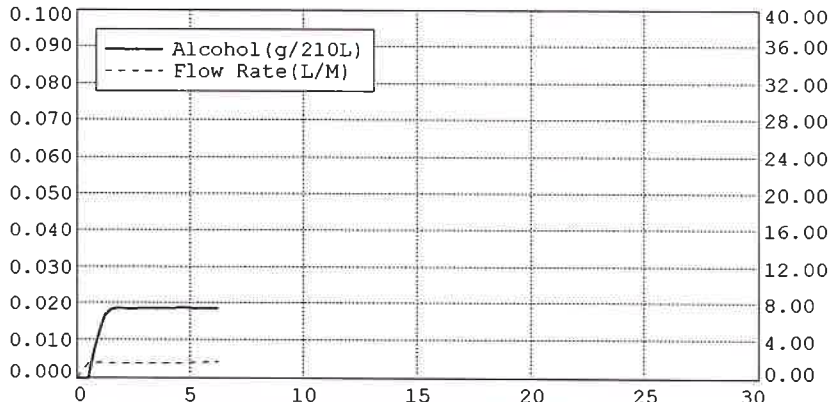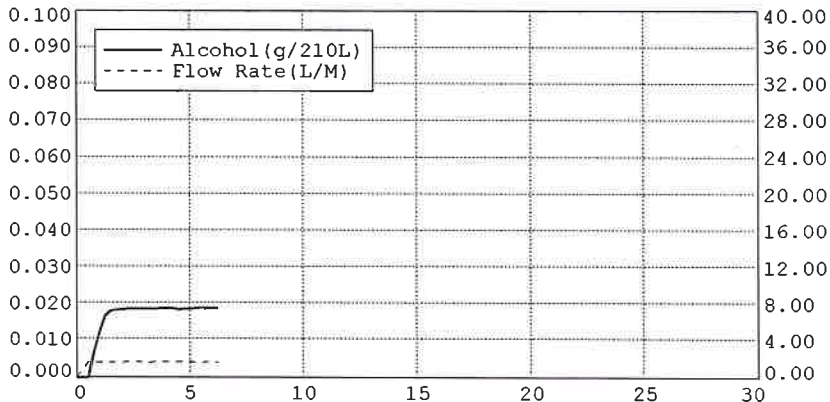

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100348






Date: 11/14/2022
 Time: 14:27:34

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 29.99: 0.040
 LOT #: AG111710
 EXPIRATION: 04/27/2023
 TANK PRESSURE: 399 psi

BLANK TEST	0.000	14:28
INTERNAL STANDARD	VERIFIED	14:28
EXTERNAL STANDARD	0.039	14:29
BLANK TEST	0.000	14:30
EXTERNAL STANDARD	0.039	14:30
BLANK TEST	0.000	14:31
EXTERNAL STANDARD	0.039	14:31
BLANK TEST	0.000	14:32
EXTERNAL STANDARD	0.039	14:32
BLANK TEST	0.000	14:33
EXTERNAL STANDARD	0.039	14:33
BLANK TEST	0.000	14:34

Average = 0.0390
 Std Dev = 0.0000

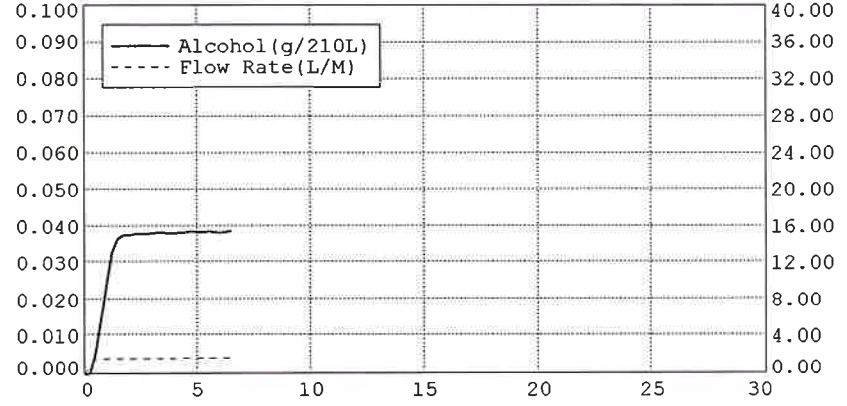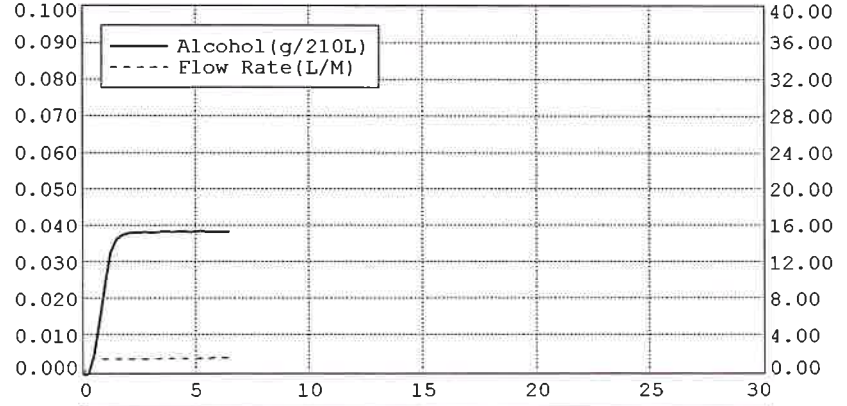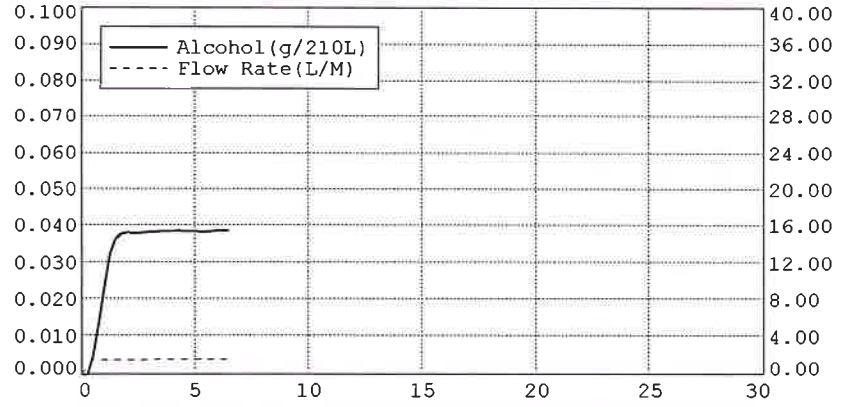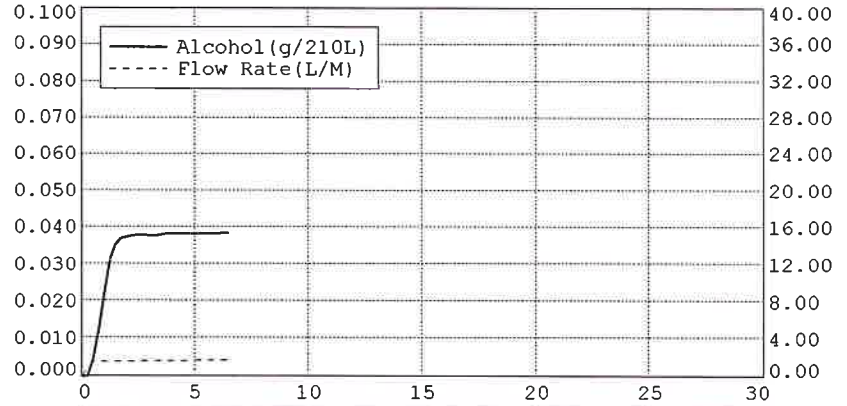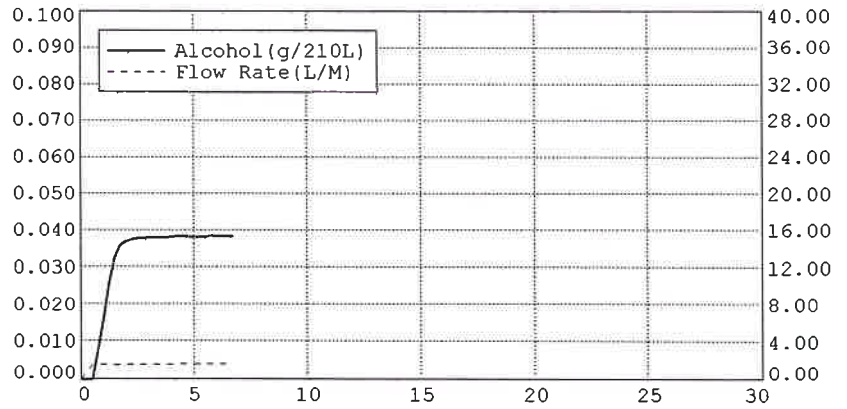

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100348






Date: 11/14/2022
 Time: 14:35:11

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 30.00: 0.080
 LOT #: AG113402
 EXPIRATION: 05/14/2023
 TANK PRESSURE: 872 psi

BLANK TEST	0.000	14:36
INTERNAL STANDARD	VERIFIED	14:36
EXTERNAL STANDARD	0.077	14:36
BLANK TEST	0.000	14:37
EXTERNAL STANDARD	0.078	14:37
BLANK TEST	0.000	14:38
EXTERNAL STANDARD	0.078	14:38
BLANK TEST	0.000	14:39
EXTERNAL STANDARD	0.077	14:39
BLANK TEST	0.000	14:40
EXTERNAL STANDARD	0.078	14:41
BLANK TEST	0.000	14:41

Average = 0.0776
 Std Dev = 0.0005

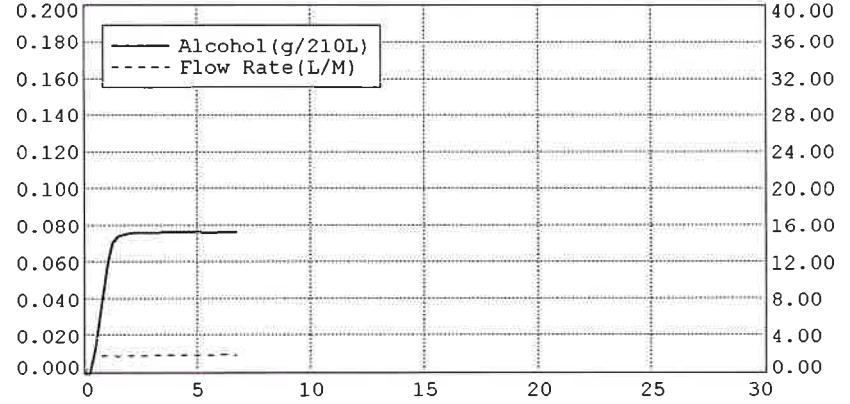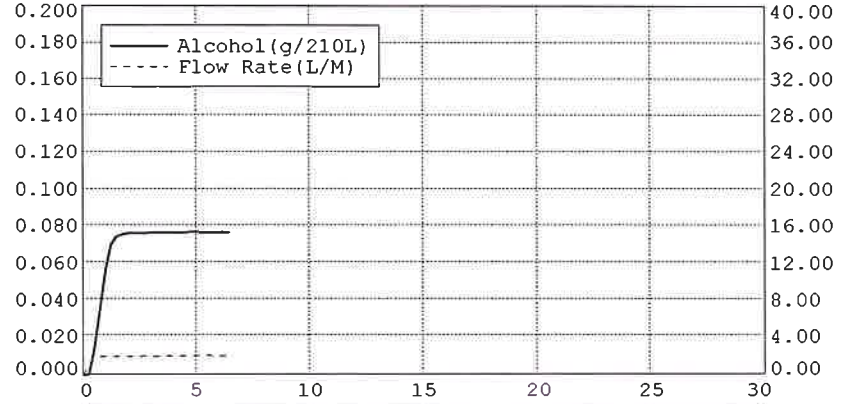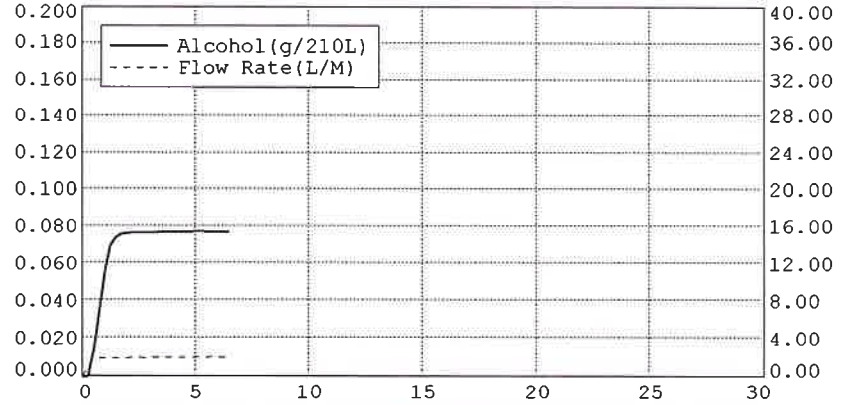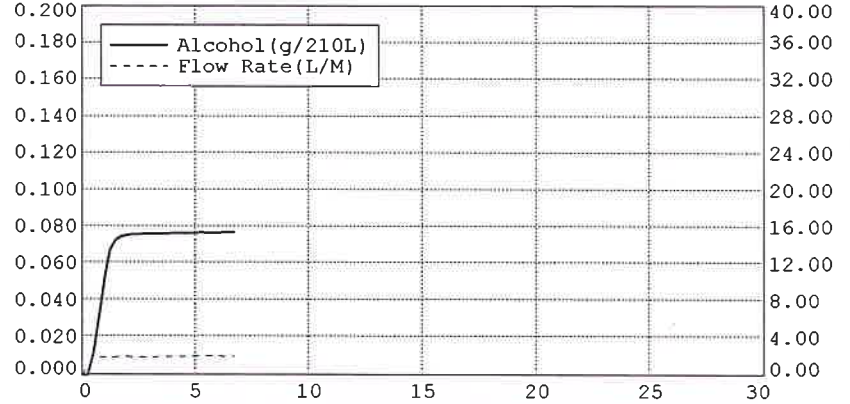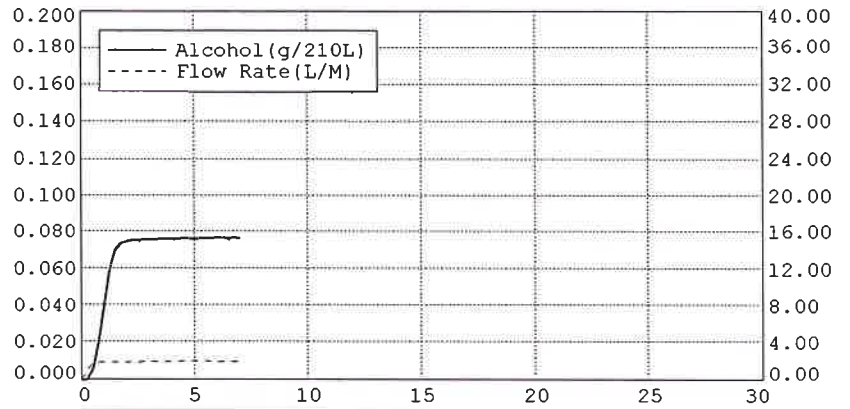

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100348






Date: 11/14/2022
 Time: 14:45:31

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 30.00: 0.100
 LOT #: AG211003
 EXPIRATION: 04/20/2024
 TANK PRESSURE: 1049 psi

BLANK TEST	0.000	14:48
INTERNAL STANDARD	VERIFIED	14:48
EXTERNAL STANDARD	0.098	14:48
BLANK TEST	0.000	14:49
EXTERNAL STANDARD	0.098	14:49
BLANK TEST	0.000	14:50
EXTERNAL STANDARD	0.098	14:50
BLANK TEST	0.000	14:51
EXTERNAL STANDARD	0.098	14:51
BLANK TEST	0.000	14:52
EXTERNAL STANDARD	0.098	14:52
BLANK TEST	0.000	14:53

Average = 0.0980
 Std Dev = 0.0000

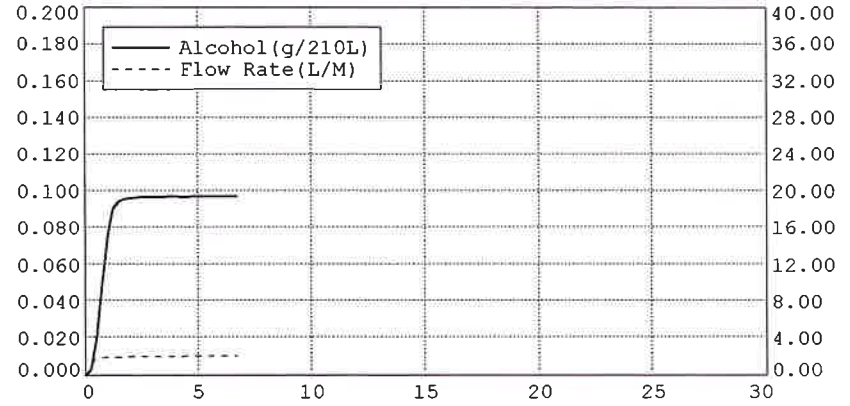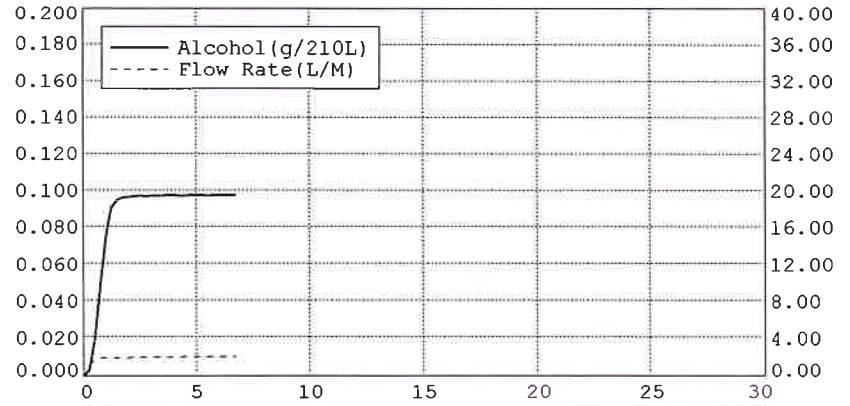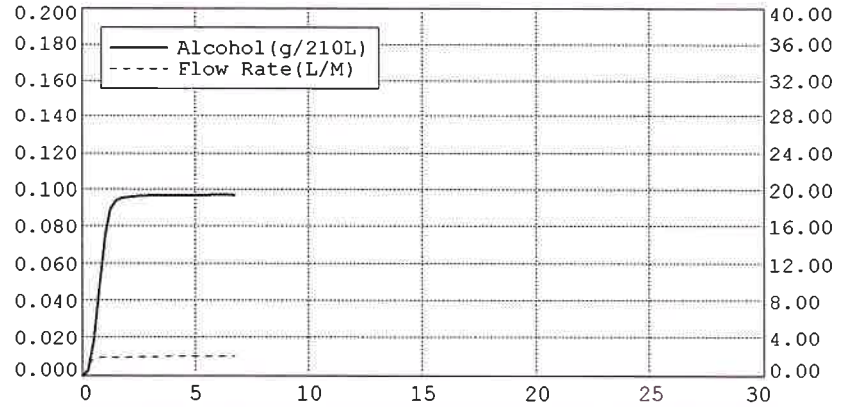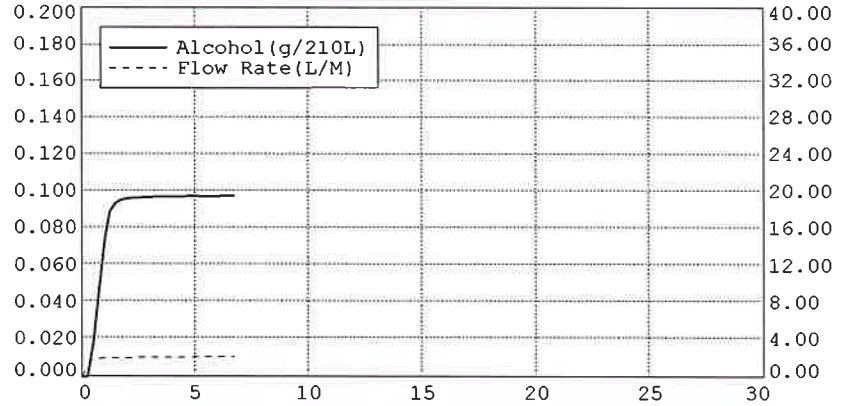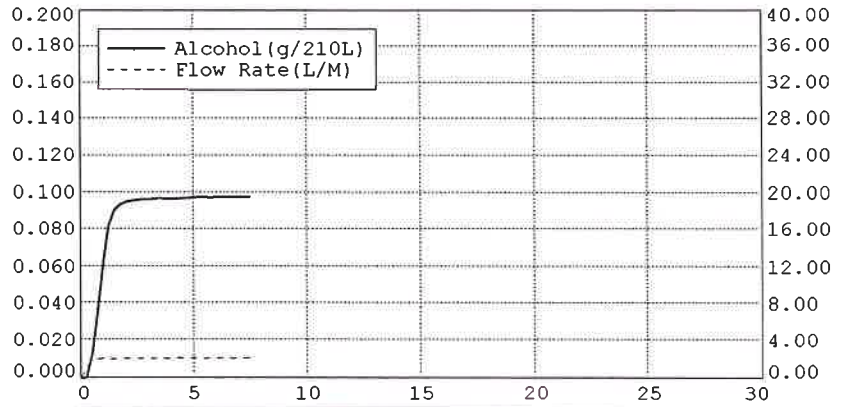

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100348






Date: 11/14/2022
 Time: 14:55:01

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 30.00: 0.150
 LOT #: AG134205
 EXPIRATION: 12/08/2023
 TANK PRESSURE: 692 psi

BLANK TEST	0.000	14:56
INTERNAL STANDARD	VERIFIED	14:56
EXTERNAL STANDARD	0.147	14:57
BLANK TEST	0.000	14:57
EXTERNAL STANDARD	0.147	14:58
BLANK TEST	0.000	14:59
EXTERNAL STANDARD	0.147	14:59
BLANK TEST	0.000	15:00
EXTERNAL STANDARD	0.147	15:00
BLANK TEST	0.000	15:01
EXTERNAL STANDARD	0.147	15:01
BLANK TEST	0.000	15:02

Average = 0.1470
 Std Dev = 0.0000

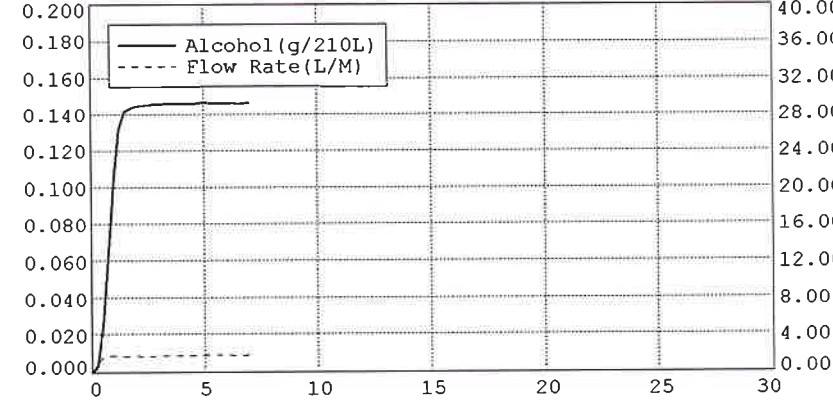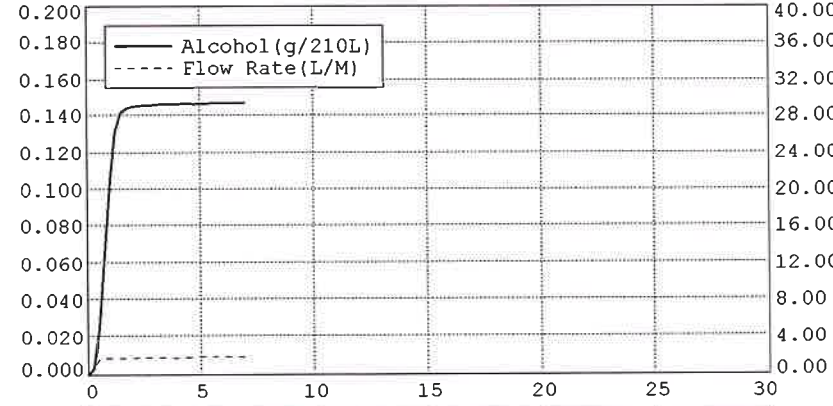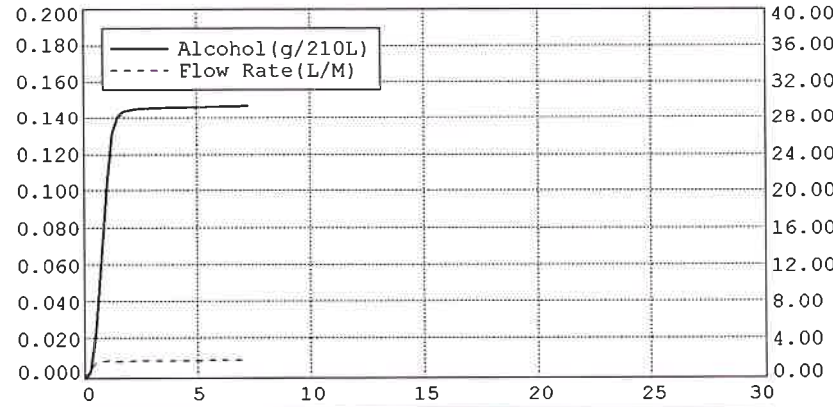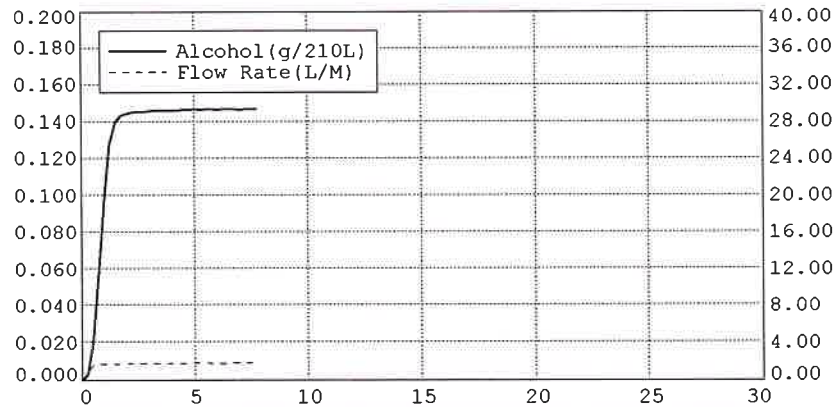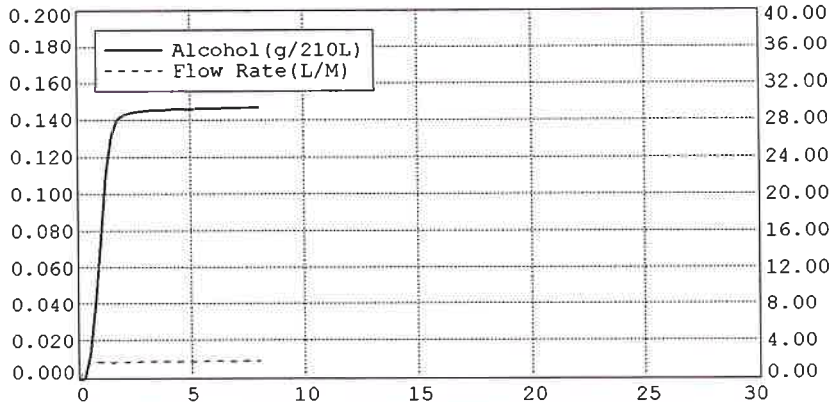

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100348






Date: 11/14/2022
 Time: 15:09:33

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 30.01: 0.301
 LOT #: AG130502
 EXPIRATION: 11/01/2023
 TANK PRESSURE: 531 psi

BLANK TEST	0.000	15:10
INTERNAL STANDARD	VERIFIED	15:10
EXTERNAL STANDARD	0.297	15:10
BLANK TEST	0.000	15:11
EXTERNAL STANDARD	0.296	15:12
BLANK TEST	0.000	15:13
EXTERNAL STANDARD	0.296	15:13
BLANK TEST	0.000	15:14
EXTERNAL STANDARD	0.296	15:14
BLANK TEST	0.000	15:15
EXTERNAL STANDARD	0.296	15:15
BLANK TEST	0.000	15:16

Average = 0.2962
 Std Dev = 0.0004

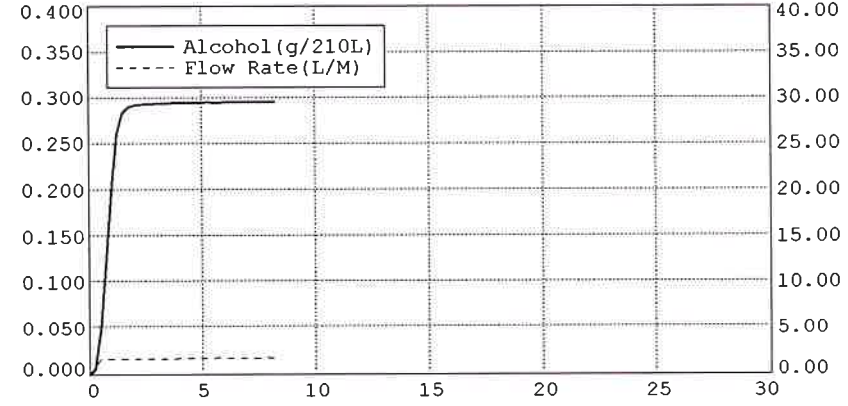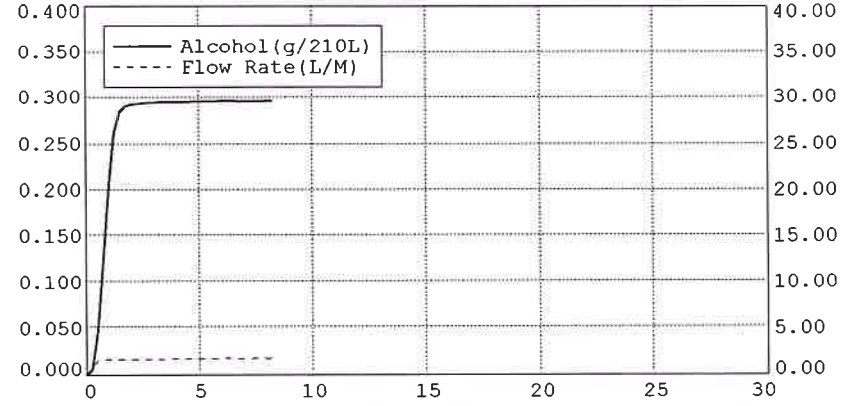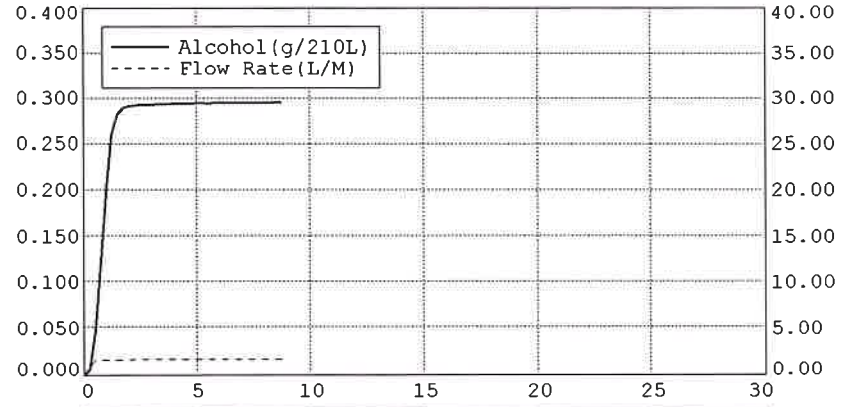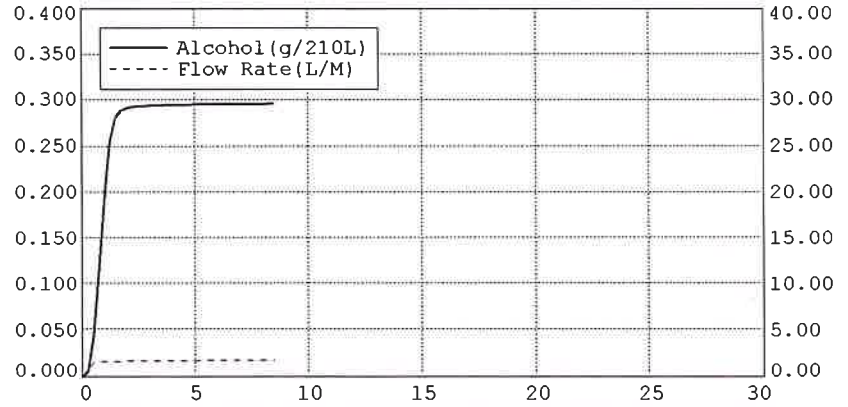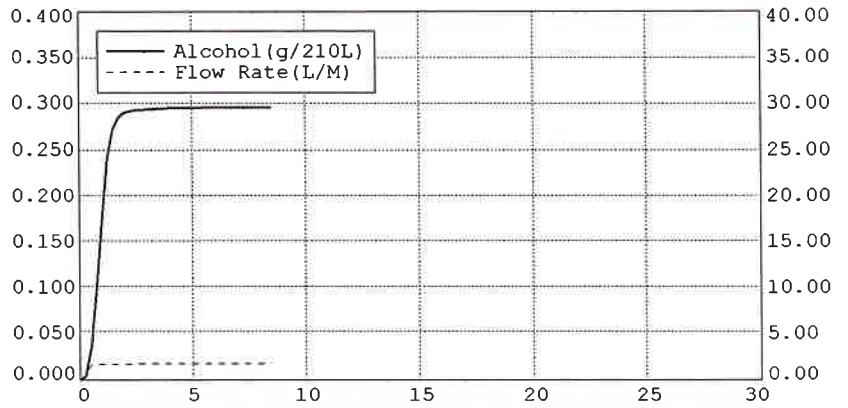

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100348

Date: 11/14/2022
Time: 15:23:44


SUBJECT NAME:
TEST TEST
LICENSE #: INCOMPLETE

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 22-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.02: 0.080
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK PASSED 15:24
BLANK TEST 0.000 15:24
INTERNAL STANDARD VERIFIED 15:25
EXTERNAL STANDARD 0.079 15:25
BLANK TEST 0.000 15:26
SUBJECT SAMPLE INCOMPLETE 15:28

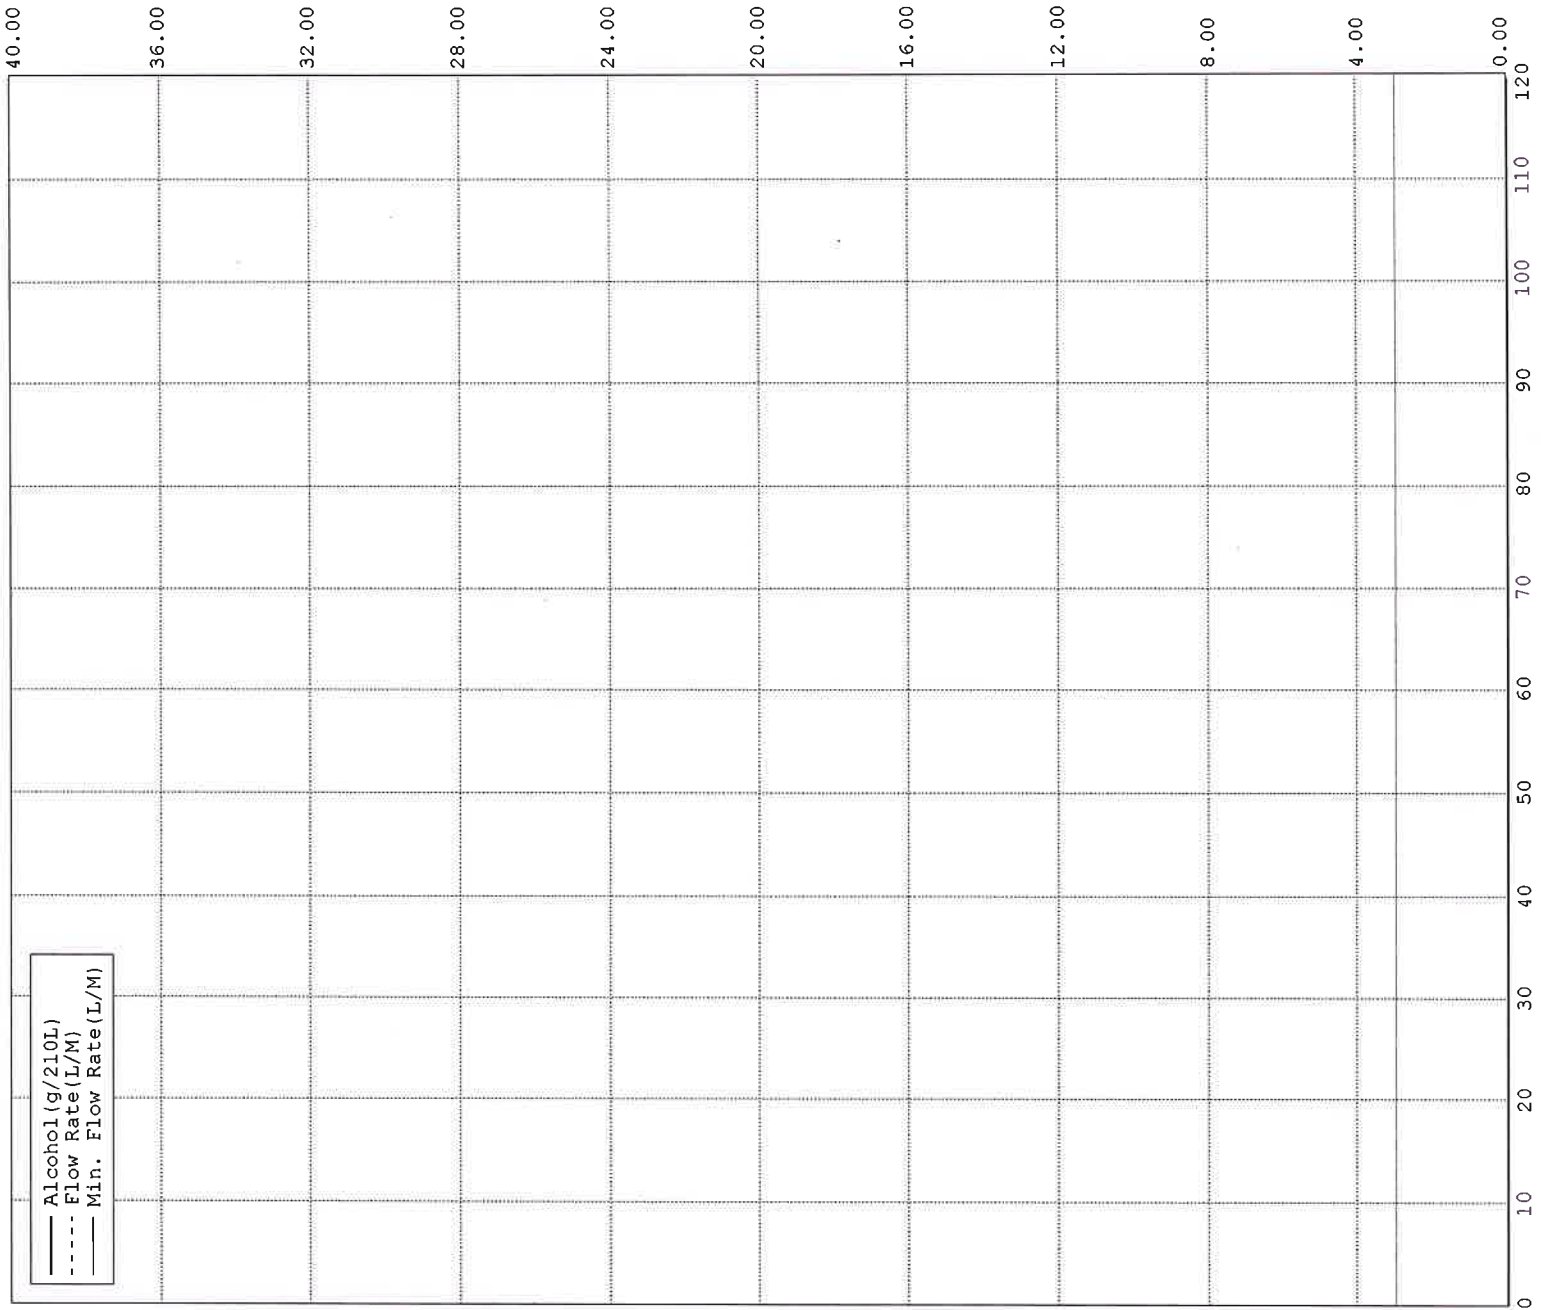

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100348

Date: 11/14/2022
Time: 15:52:32

SUBJECT NAME:
TEST TEST
LICENSE #: MAX ATTEMPTS


OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 22-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.02: 0.080
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK PASSED 15:55
BLANK TEST 0.000 15:55
INTERNAL STANDARD VERIFIED 15:55
EXTERNAL STANDARD 0.078 15:55
BLANK TEST 0.000 15:56
SUBJECT SAMPLE XXX 15:57

Maximum Attempts Exceeded

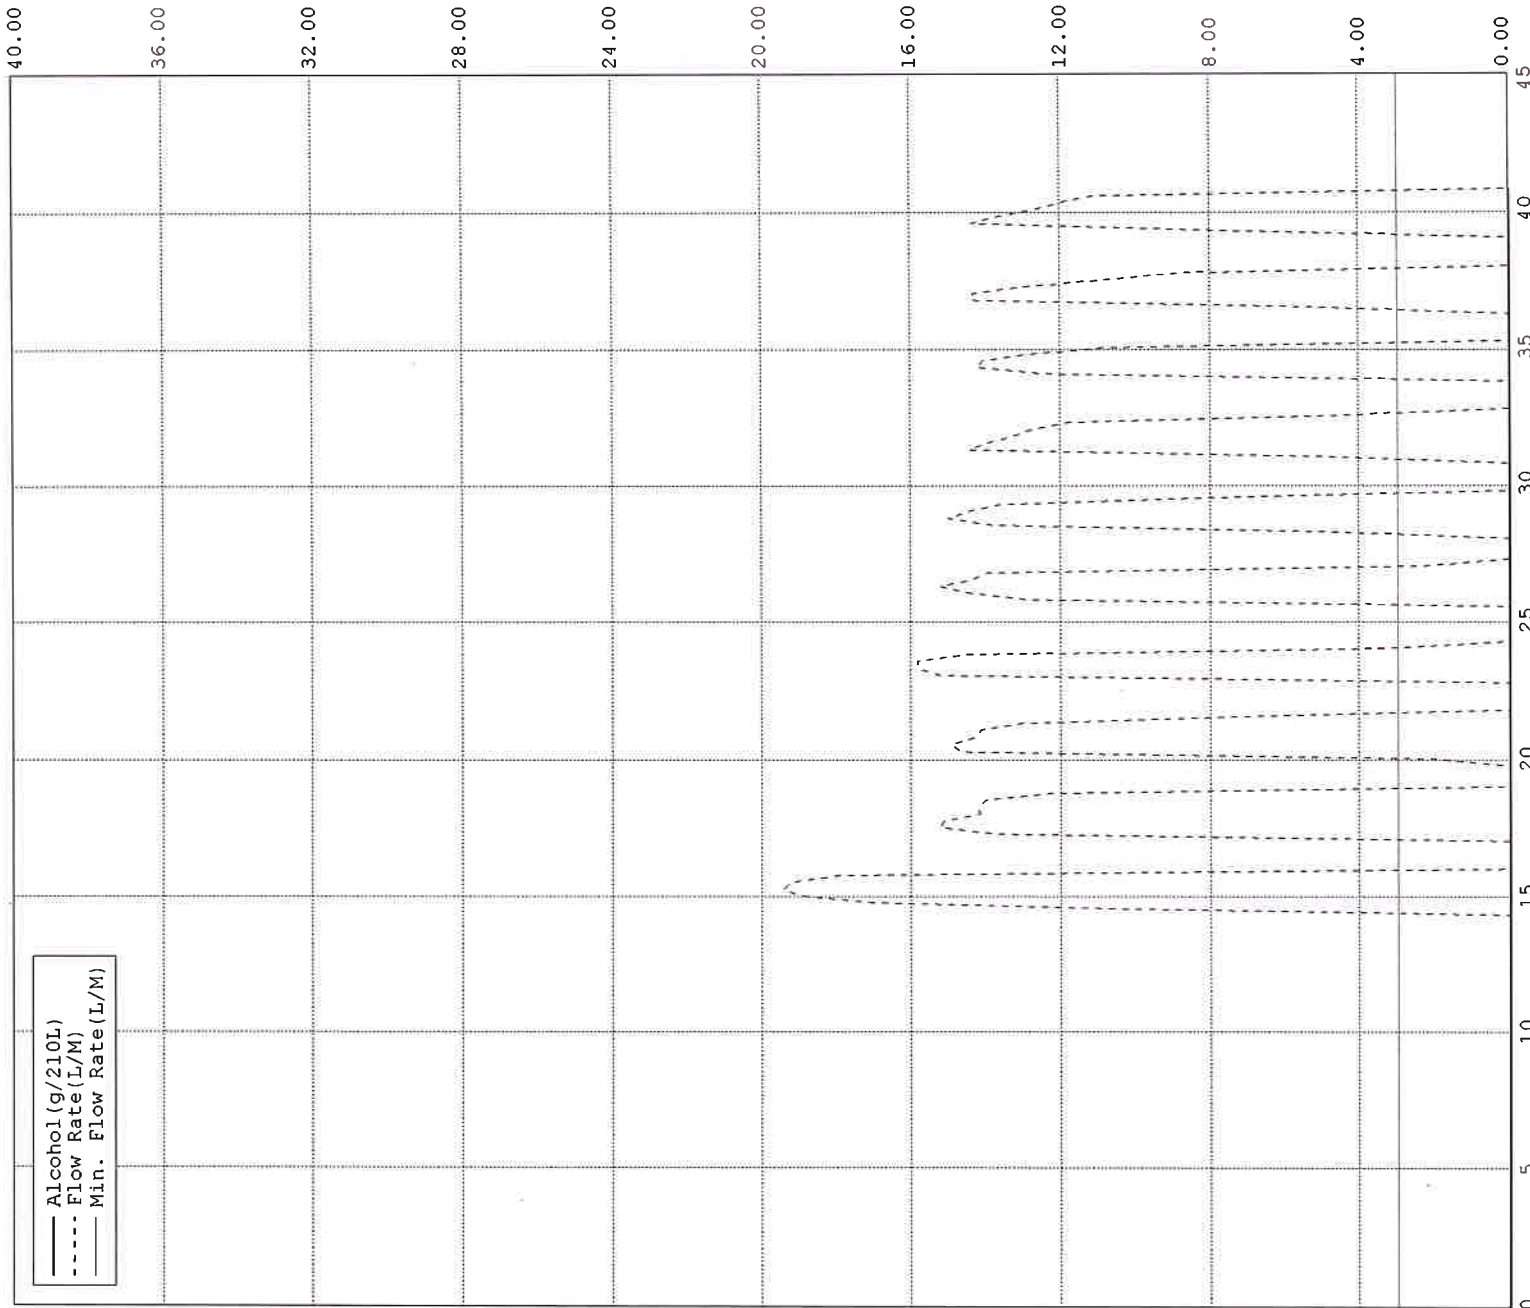

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100348

Date: 11/14/2022
Time: 15:30:07

SUBJECT NAME:
TEST TEST
LICENSE #: INT-ACETONE

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 22-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.02: 0.080
LOT #: AG113402
EXPIRATION: 05/14/2023


DIAGNOSTIC CHECK	PASSED	15:31
BLANK TEST	0.000	15:32
INTERNAL STANDARD	VERIFIED	15:32
Xq = 0.091 (2.15%)		
EXTERNAL STANDARD	0.079	15:32
X[1] = 0.0786 (-0.0004) (0.0033)		
BLANK TEST	0.000	15:33
SUBJECT SAMPLE	XXX	15:33
X[1] = 0.1054 (-0.0169) (0.0024)		

Interference Detected

Filter Avg = -0.0004

Filter Avg = 0.0034

CS

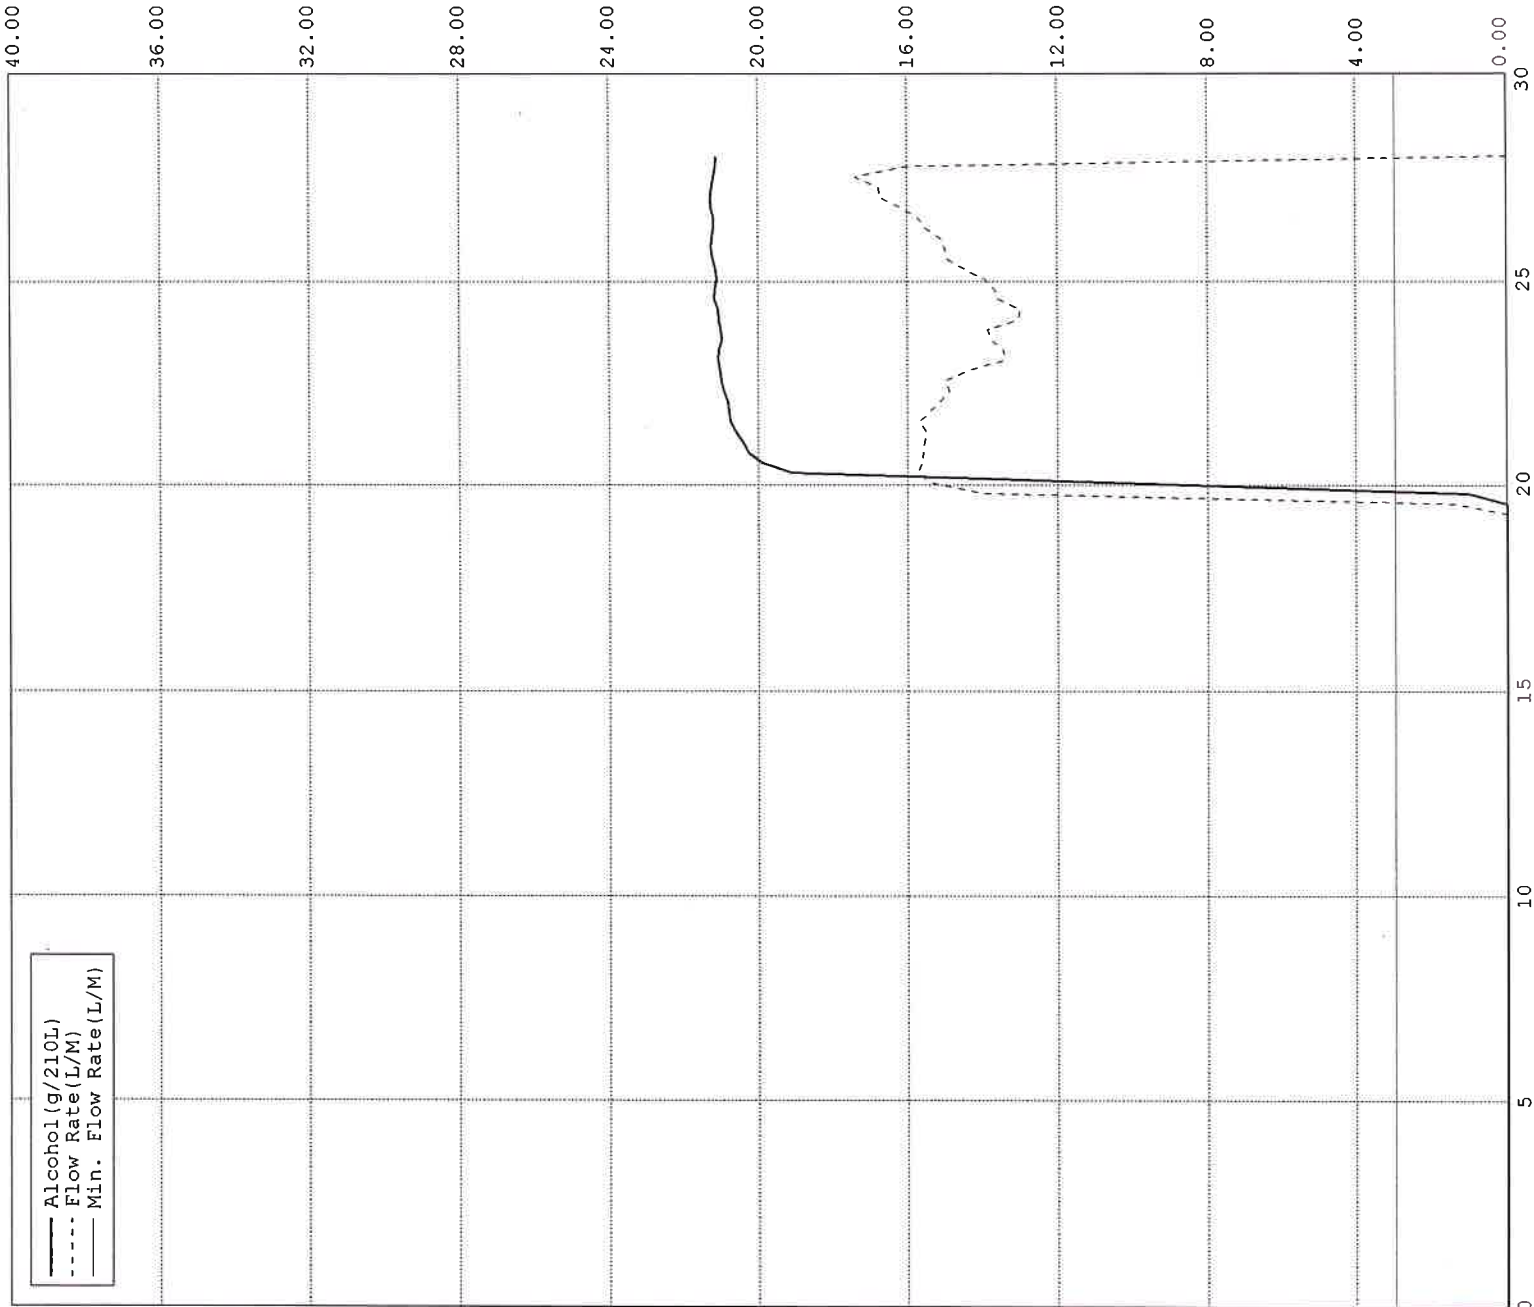

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100348

Date: 11/14/2022
Time: 15:38:19

SUBJECT NAME:
TEST TEST
LICENSE #: INT=IPA

OPERATOR NAME:
COLLEEN S OBRyant
OPERATOR'S #: 6237


DEPT/AGENCY:
AAA1
CASE/REPORT: 22-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.01: 0.080
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK PASSED 15:39
BLANK TEST 0.000 15:39
INTERNAL STANDARD VERIFIED 15:39
Xq = 0.091 (1.86%)
EXTERNAL STANDARD 0.078 15:40
X[1] = 0.0781 (0.0001) (0.0037)
BLANK TEST 0.000 15:41
SUBJECT SAMPLE XXX 15:41
X[1] = 0.1140 (-0.0264) (0.0029)

Interference Detected

COB

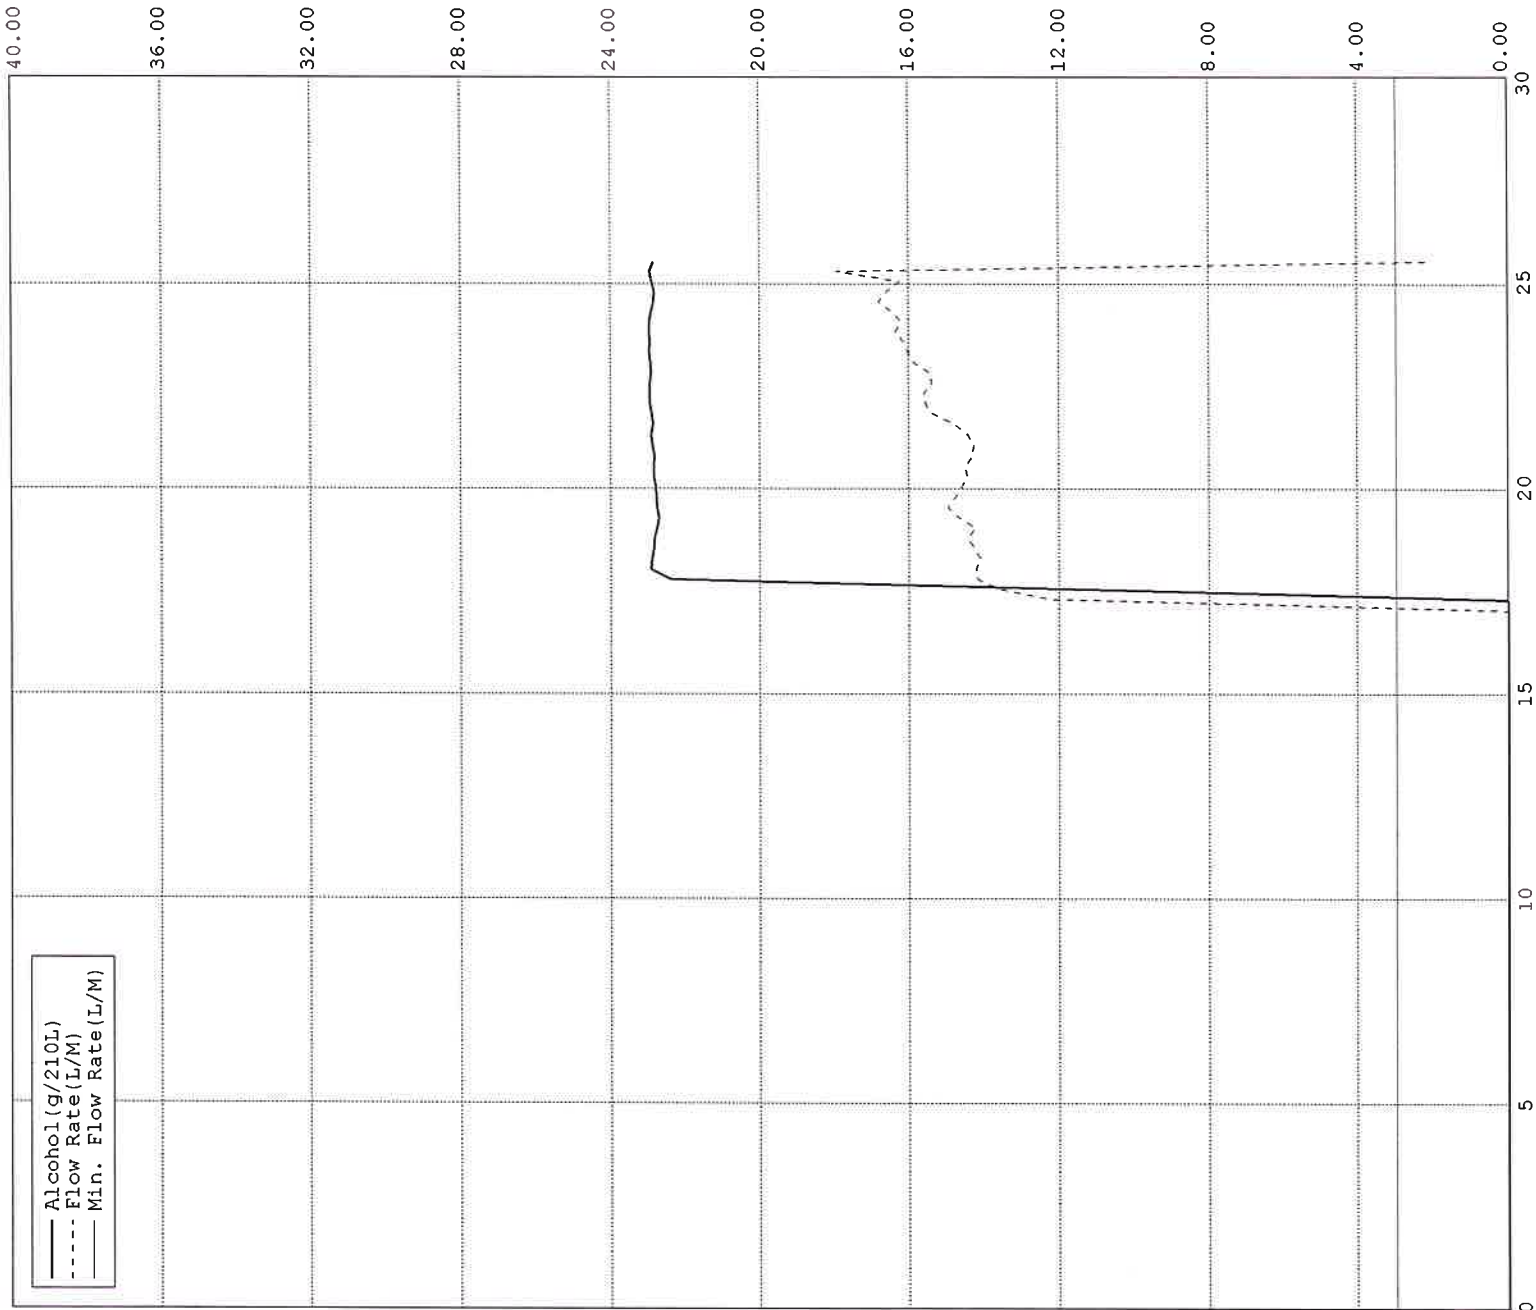

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100348

Date: 11/14/2022

Time: 15:44:55

SUBJECT NAME:

TEST TEST

LICENSE #: INT-NEGATIVE

OPERATOR NAME:

COLLEEN S O'BRYAN

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 22-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 30.02: 0.080

LOT #: AG113402

EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK

PASSED 15:46

BLANK TEST

0.000 15:46

INTERNAL STANDARD

VERIFIED 15:46

Xq = 0.091 (1.47%)

EXTERNAL STANDARD

0.078 15:46

X[1] = 0.0776 (-0.0007) (0.0036)

BLANK TEST

0.000 15:47

SUBJECT SAMPLE (Vol=1.90L)

0.089 15:48

X[1] = 0.0892 (0.0001) (0.0016)

BLANK TEST

0.000 15:49

EXTERNAL STANDARD


0.078 15:49

X[1] = 0.0776 (-0.0006) (0.0028)

BLANK TEST

0.000 15:50

CRB

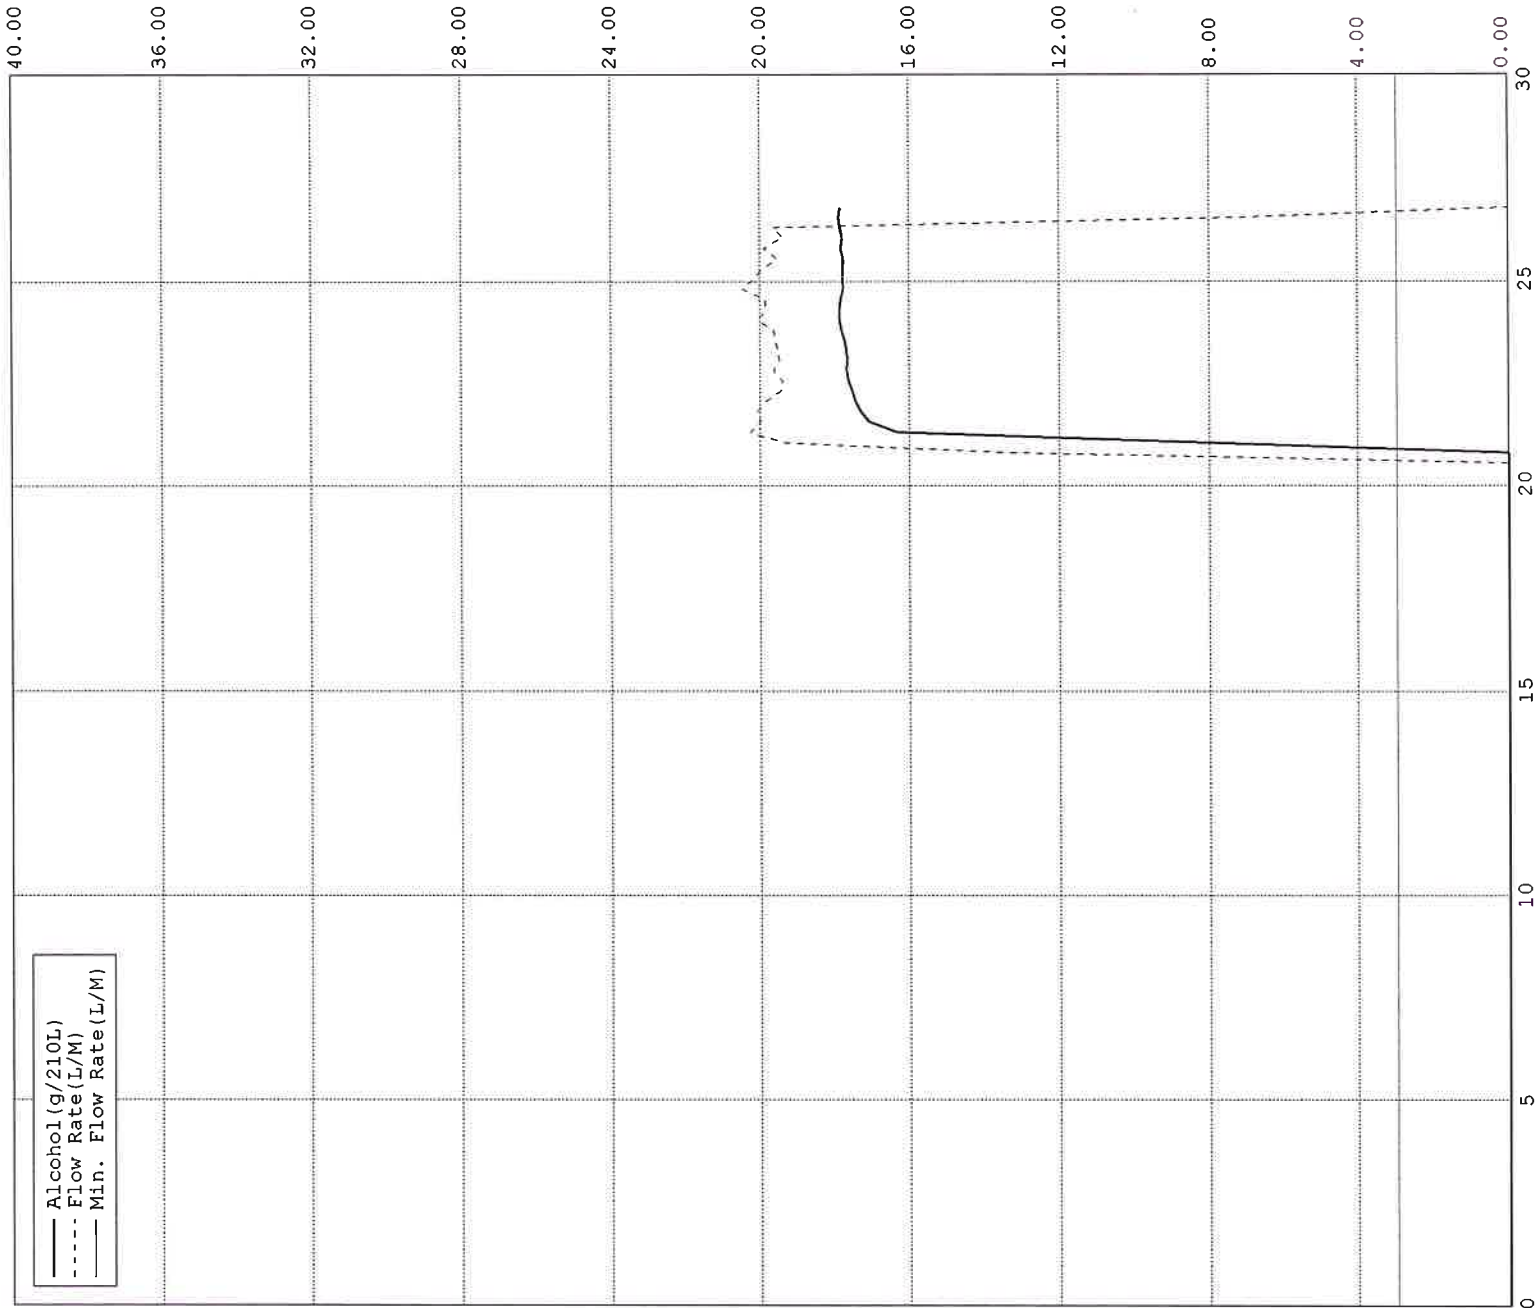

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100348

Date: 11/14/2022
Time: 16:01:13

SUBJECT NAME:
TEST TEST
LICENSE #: INVALID


OPERATOR NAME:
COLLEEN S OBRyant
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 22-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 30.03: 0.080
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	16:02
BLANK TEST	0.000	16:02
INTERNAL STANDARD	VERIFIED	16:02
EXTERNAL STANDARD	0.077	16:03
BLANK TEST	0.000	16:04
SUBJECT SAMPLE	INVALID	16:04

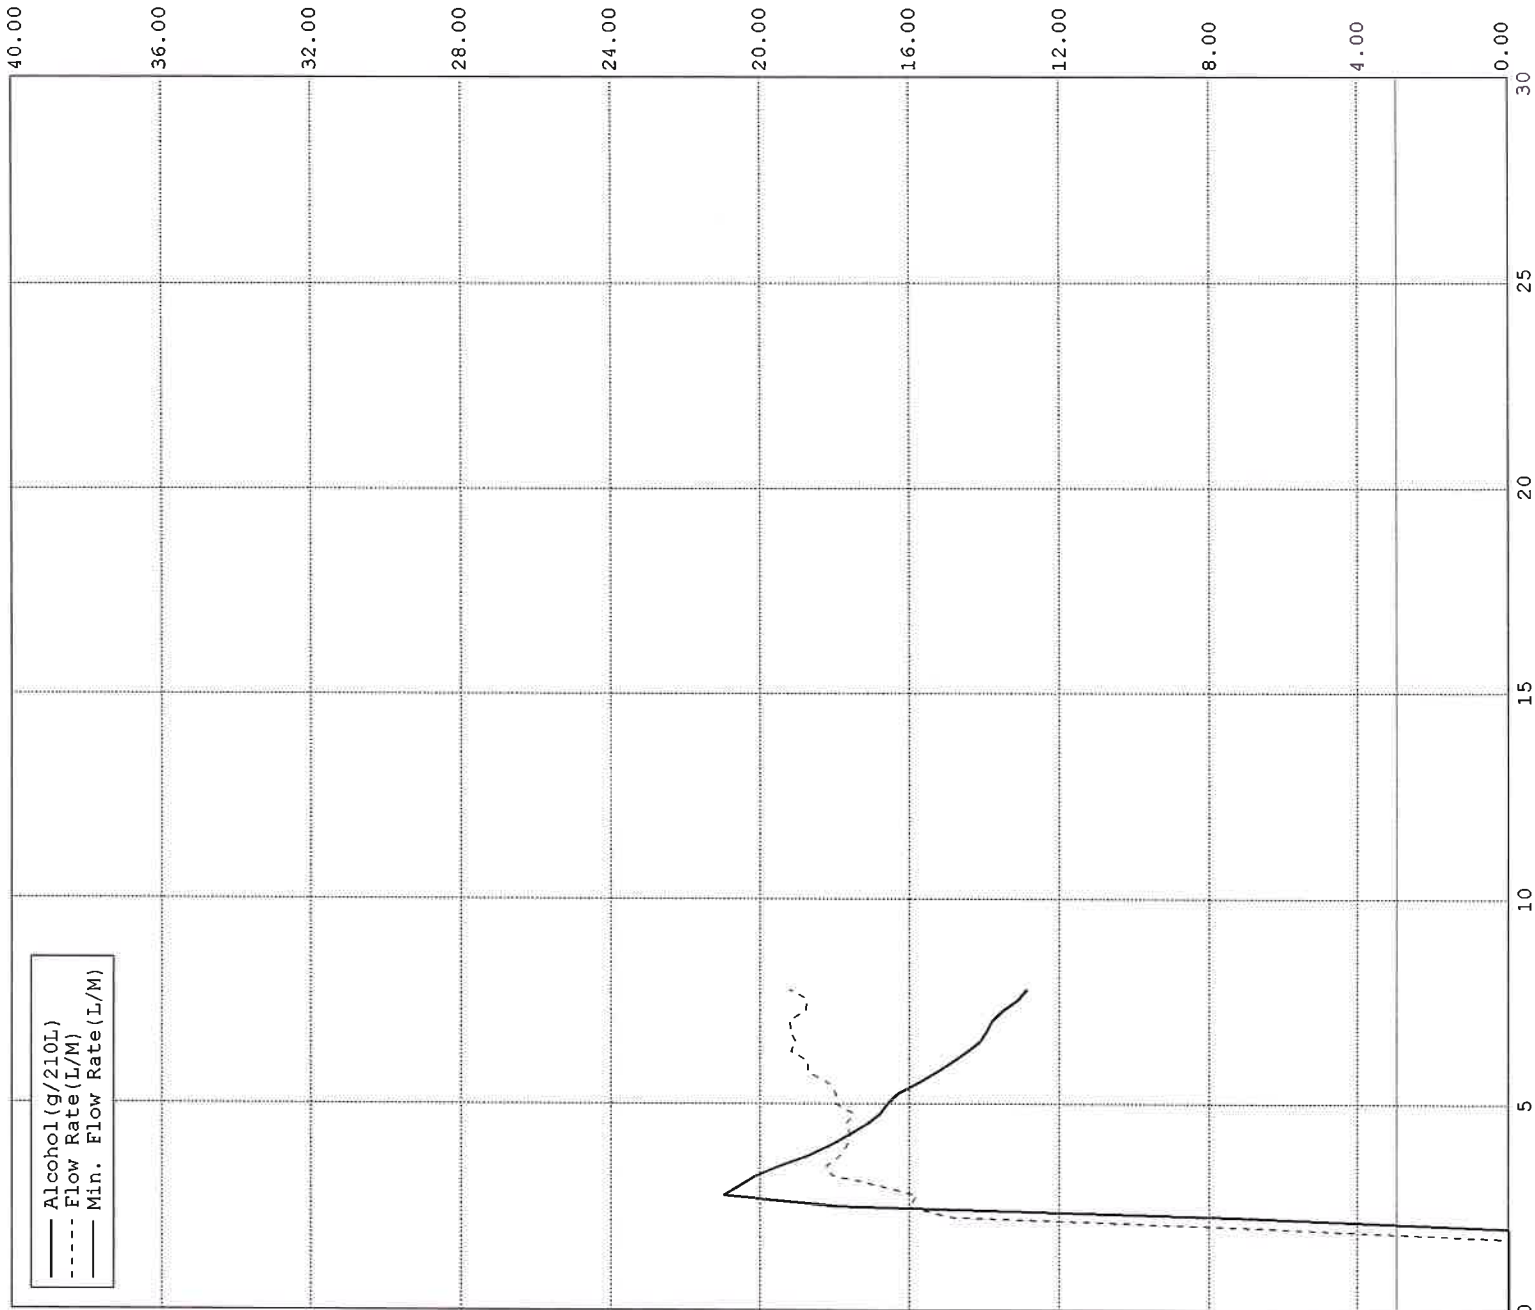

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100348

Date: 11/14/2022
Time: 16:06:05

SUBJECT NAME:
TEST TEST
LICENSE #: RFI

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237


DEPT/AGENCY:
AAA1
CASE/REPORT: 22-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.03: 0.080
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK PASSED 16:07
BLANK TEST 0.000 16:07
INTERNAL STANDARD VERIFIED 16:07
EXTERNAL STANDARD 0.078 16:07
BLANK TEST 0.000 16:08

RFI DETECTED

COB

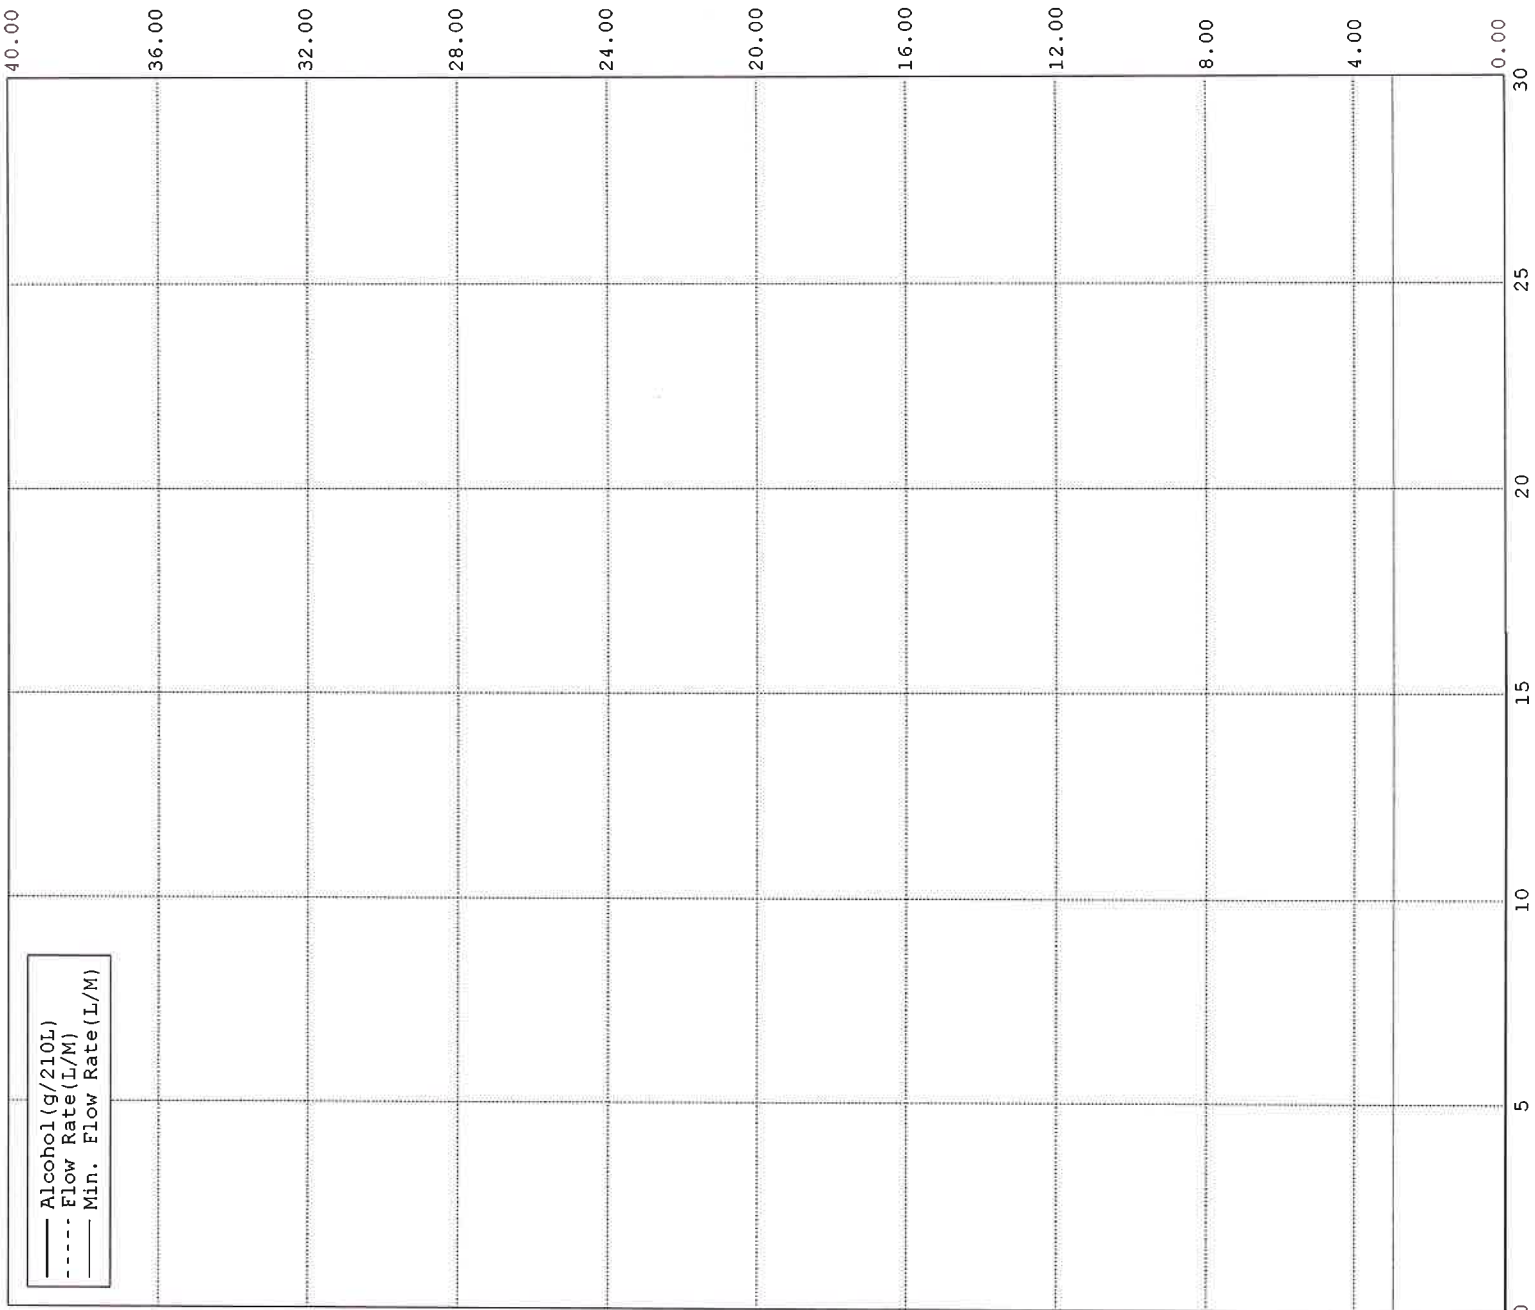

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100348

Date: 11/14/2022

Time: 16:24:53

SUBJECT NAME:

TEST TEST

LICENSE #: NON-DRINKING

OPERATOR NAME:

COLLEEN S O'BRYAN

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 22-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 30.06: 0.080

LOT #: AG113402

EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	16:25
BLANK TEST	0.000	16:26
INTERNAL STANDARD	VERIFIED	16:26
EXTERNAL STANDARD	0.078	16:26
BLANK TEST	0.000	16:27
SUBJECT SAMPLE (Vol=1.87L)	0.000	16:27
BLANK TEST	0.000	16:28
EXTERNAL STANDARD	0.078	16:29
BLANK TEST	0.000	16:29

