

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100669

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 12/10/2019

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 27.93: 0.075
LOT #: AG923401
EXPIRATION: 08/22/2021
TANK PRESSURE: 1221 psi

BLANK TEST	0.000	11:13
INTERNAL STANDARD	VERIFIED	11:13
EXTERNAL STANDARD	0.074	11:13
BLANK TEST	0.000	11:14
EXTERNAL STANDARD	0.074	11:14
BLANK TEST	0.000	11:15
EXTERNAL STANDARD	0.074	11:15
BLANK TEST	0.000	11:16
EXTERNAL STANDARD	0.074	11:16
BLANK TEST	0.000	11:17
EXTERNAL STANDARD	0.074	11:18
BLANK TEST	0.000	11:18

Average = 0.0740
Std Dev = 0.0000

Diagnostic Check

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 49.1°C PASSED
Breath Tube = 46.6°C PASSED

PUMP INFO

Flow Rate = 4.321 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

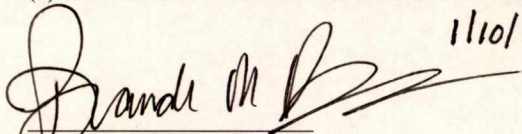
FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED

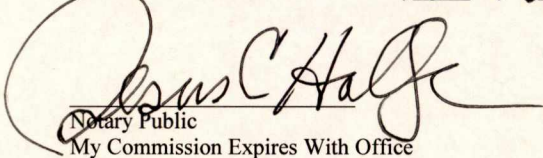
I, Brandi M. Barnett, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

 1/10/20

Brandi M. Barnett
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 10 day of Jan, 2020


Notary Public
My Commission Expires With Office



DW 12/26/19