

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100369

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 12/27/2017

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.36: 0.079
LOT #: AG608504
EXPIRATION: 03/25/2018
TANK PRESSURE: 914 psi

BLANK TEST	0.000	20:49
INTERNAL STANDARD	VERIFIED	20:49
EXTERNAL STANDARD	0.077	20:50
BLANK TEST	0.000	20:51
EXTERNAL STANDARD	0.077	20:51
BLANK TEST	0.000	20:52
EXTERNAL STANDARD	0.077	20:52
BLANK TEST	0.000	20:53
EXTERNAL STANDARD	0.077	20:53
BLANK TEST	0.000	20:54
EXTERNAL STANDARD	0.077	20:54
BLANK TEST	0.000	20:55

Average = 0.0770
Std Dev = 0.0000

Diagnostic Check

VERSIONS

DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
Breath Tube = 39.4°C PASSED

PUMP INFO

Flow Rate = 5.310 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO


Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED

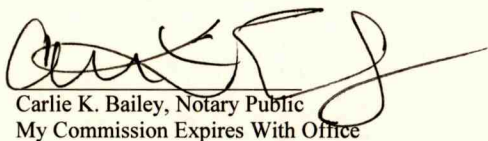
I, Charles R. Foster, after being first duly sworn, depose and state as follows:

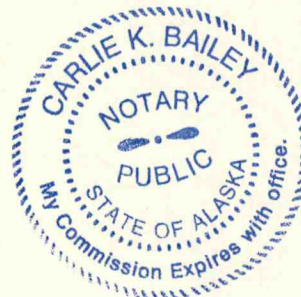
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


 3/8/18

Charles R. Foster
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 08 day of 03, 2018


Carlie K. Bailey, Notary Public
My Commission Expires With Office




3/2/18