

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument  
State of Alaska

Serial #: 100364

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 12/27/2015

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.59: 0.079  
LOT #: 09214080A2  
EXPIRATION: 05/01/2016  
TANK PRESSURE: 112 psi

BLANK TEST	0.000	05:49
INTERNAL STANDARD	VERIFIED	05:49
EXTERNAL STANDARD	0.079	05:49
BLANK TEST	0.000	05:50
EXTERNAL STANDARD	0.079	05:50
BLANK TEST	0.000	05:51
EXTERNAL STANDARD	0.079	05:51
BLANK TEST	0.000	05:52
EXTERNAL STANDARD	0.079	05:53
BLANK TEST	0.000	05:53
EXTERNAL STANDARD	0.080	05:54
BLANK TEST	0.000	05:55

Average = 0.0792  
Std Dev = 0.0004

## Diagnostic Check

### VERSIONS

DMT: 3.01  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.9°C PASSED  
Breath Tube = 44.6°C PASSED

### PUMP INFO

Flow Rate = 4.496 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED

### FILTER INFO

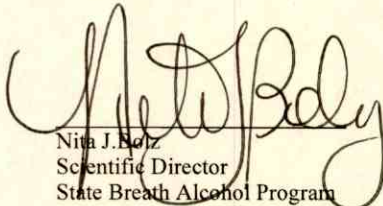
Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

### INTERNAL STANDARD


PASSED

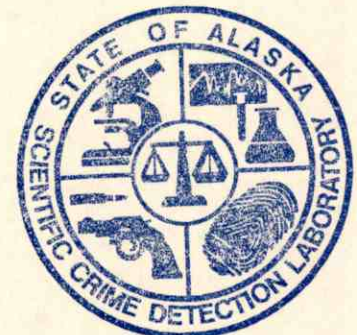
I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

 1/20/2016  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 20<sup>th</sup> day of Jan, 20 16

  
Nikki Roth, Notary Public  
My Commission Expires With Office



003/12/16