



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories

Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100378

Report Issue Date: 03/28/2024
Date Received: 2024-02-21
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

Start Date 02/22/2024 - As Found - **End Date 02/23/2024** As Found - Evaluation Analyst: Carlie Glaister
 As Found Conditions - Barometric Pressure (inHg): 29.46 Barometer Used: Fisher S/N 230307229 Temperature (C): 22.5
 Relative Humidity (%): 12

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG217902	0.019	0.020	0.020	0.019	0.020	0.020
0.080	0.078	AG310901	0.076	0.076	0.077	0.076	0.077	0.076
0.300	0.294	AG327804	0.290	0.290	0.290	0.290	0.290	0.290

Replaced O-ring. Reinstalled software 3.02. Blank error occurred during first VOC simultaneously with another nearby instrument. Appears to be environmental. Screen freezing did not occur during evaluation.

Start Date 02/23/2024 - As Left - **End Date 02/23/2024**

As Left Conditions - Barometric Pressure (inHg): 29.22 Barometer Used: Fisher S/N 230307229 Temperature (C): 23.6 Relative Humidity (%): 19

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.019	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG217904	0.039	0.040	0.039	0.040	0.040	0.040	+/- 0.003
0.080	0.078	AG310901	0.078	0.077	0.078	0.077	0.077	0.077	+/- 0.004
0.100	0.097	AG211003	0.099	0.098	0.098	0.098	0.098	0.098	+/- 0.004
0.150	0.146	AG332004	0.145	0.144	0.145	0.144	0.145	0.145	+/- 0.005
0.300	0.293	AG327804	0.294	0.294	0.294	0.293	0.294	0.294	+/- 0.011

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.



State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories

Serial Number: 100378

Results authorized by Carlie Glaister on 03/28/2024

carlie.glaister@alaska.gov

Technically and administratively reviewed by Colleen O'Bryant on 03/28/2024

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100378

Analyst or Technician Name: Carlie Glaister

DataMaster DMT Calibration Start Date: 2/23/24

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 230307229
Calibration Due Date: 5/2/25
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.22 Temperature(C) 23.6 Relative Humidity(%) 19

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20240214COB Expiration Date: 5/14/24
Simulator S/N: SD1088 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20270214COB Expiration Date: 5/14/24
Simulator S/N: DR4161 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 20710214COB Expiration Date: 5/14/24
Simulator S/N: SD1177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: 9/19/25

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 2/23/24

Data Interpretation Date (Technician): NA (if applicable)

Data Interpretation Date (Analyst): 2/23/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100378

Date: 02/23/2024
Time: 08:31:45

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 48.1°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.55 V PASSED
(0.93 V - 2.17 V)
Cooler Voltage = 1.57 V PASSED
(0.94 V - 2.20 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Freq = 527 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.6 in

PUMP INFO

Flow Rate = 4.552 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED

Xq = 0.087 0.20% (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100378

Date: 02/23/2024
Time: 8:48 AM

Temperatures (°C)

Sample Cell: 48.7°C
Breath Tube: 47.6°C

Current Barometer 29.2 in
Volume (Ltr) 1.55

Settings

Lamp: 1.56 V
Bias: 80 V
Cooler: 1.62 V
Chopper: 527 Hz

Voltages (V)

Flow: 1.06 V
Detector: -0.046 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100378

Date: 05/19/2021
Time: 12:20:25

OPERATOR NAME:
CARLIE BAILEY
CERTIFICATE #: 10436

Ca = 0.1000
CAL = 0.957976 0.800 <= CAL < 1.200
b1 = 0.0008 0.0000 <= b1 < 0.0040
b2 = 0.0058 0.0010 <= b2 < 0.0100
b3 = 0.0012 0.0000 <= b3 < 0.0040
Xq = 0.0869 0.0500 <= Xq < 0.2000
a21 = 1.178345 1.050 <= a21 < 1.300
a31 = 0.448135 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100378

Date: 02/23/2024

Time: 09:04:50

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

MINIMUM VOLUME TEST

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080


TARGET AT 29.17: 0.078

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	09:05
BLANK TEST	0.000	09:05
INTERNAL STANDARD	VERIFIED	09:06
EXTERNAL STANDARD	0.077	09:06
BLANK TEST	0.000	09:07
SUBJECT SAMPLE (Vol=1.53L)	0.000	09:08
BLANK TEST	0.000	09:09
EXTERNAL STANDARD	0.078	09:09
BLANK TEST	0.000	09:10

OK

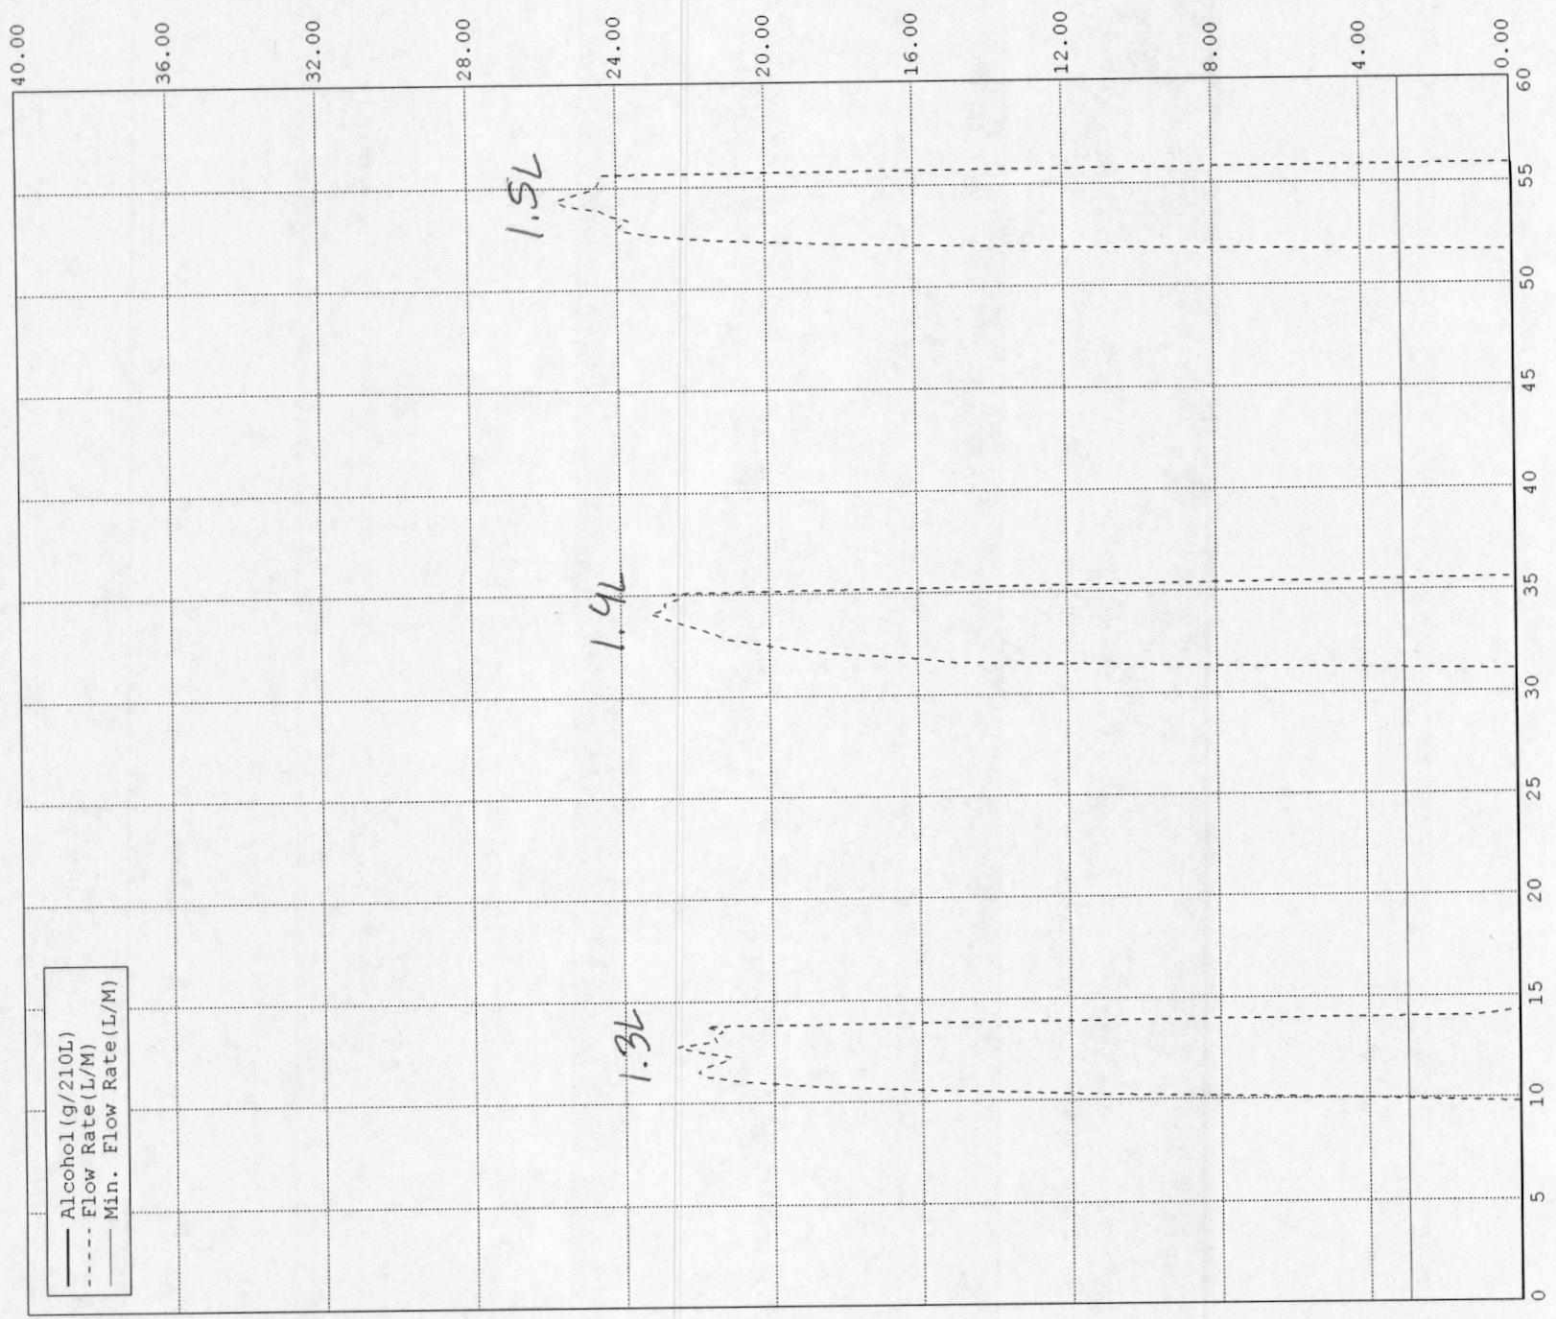

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100378

Date: 02/23/2024
 Time: 09:24:27

SUPERVISOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.019	0.0200	0.0000
0.039	0.0396	0.0005
0.078	0.0774	0.0005
0.097	0.0982	0.0004
0.146	0.1446	0.0005
0.293	0.2938	0.0004

SLOPE = 0.999245
 = 0.999892

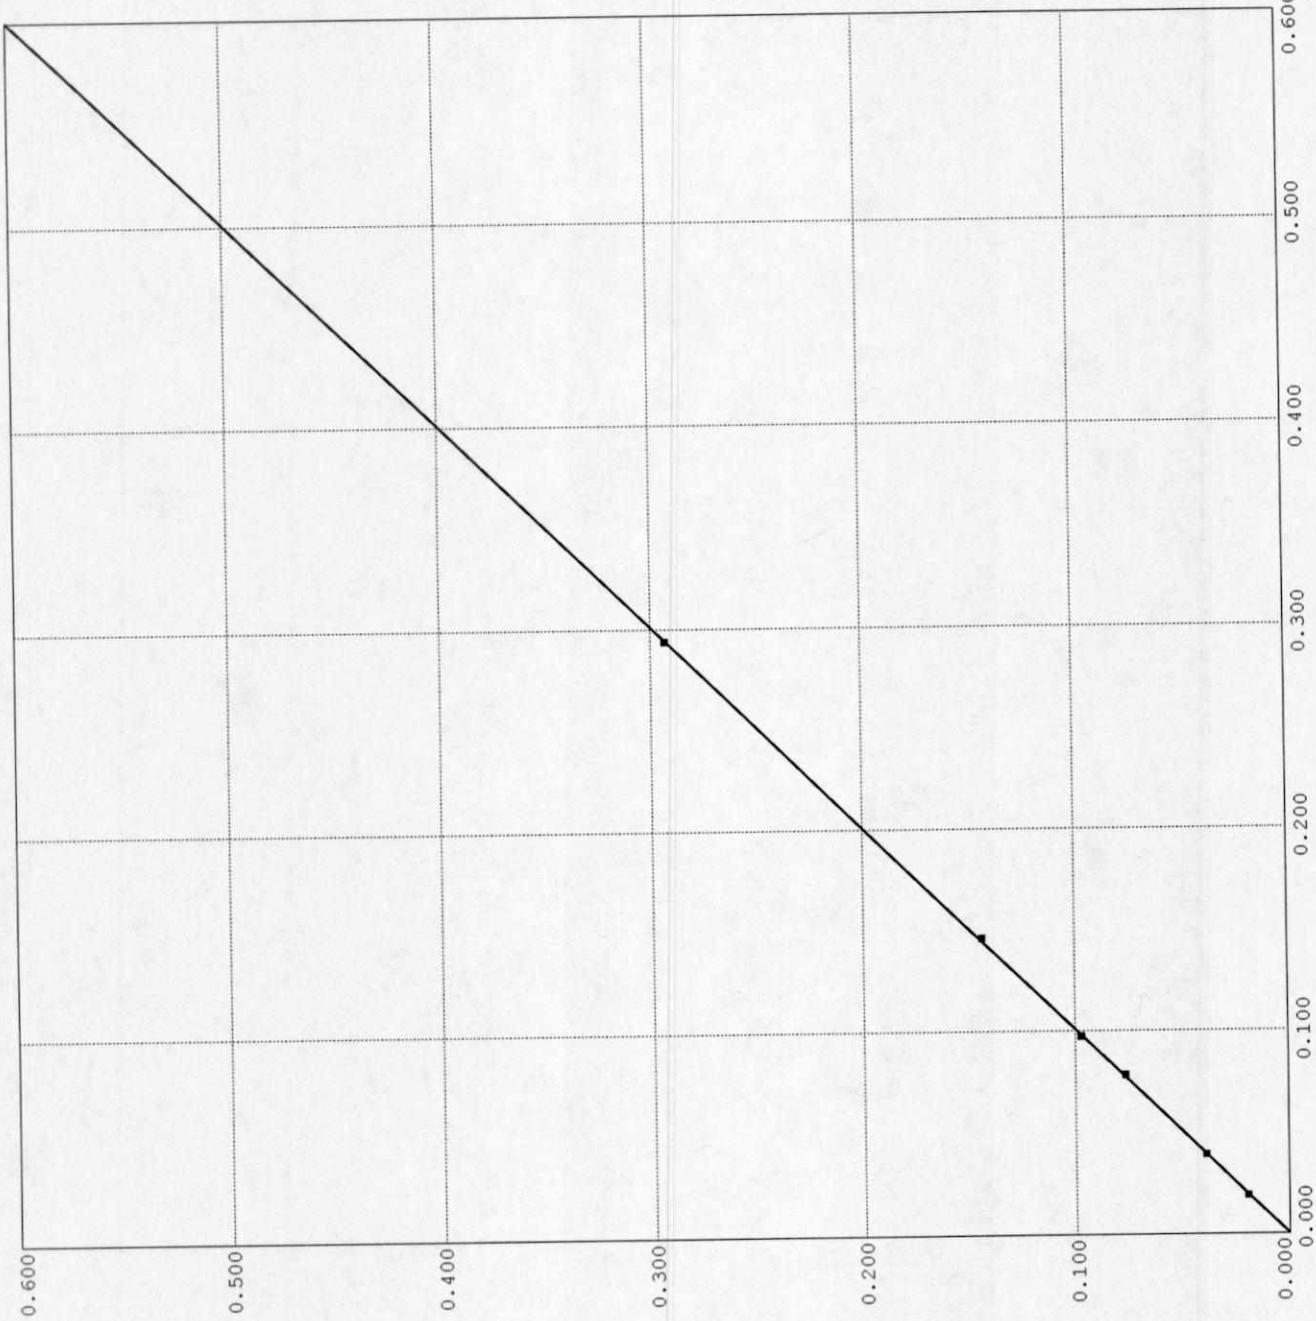

CKG

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100378






Date: 02/23/2024
Time: 09:24:29

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.17: 0.019
LOT #: AG217902
EXPIRATION: 06/28/2024
TANK PRESSURE: 662 psi

BLANK TEST	0.000	09:26
INTERNAL STANDARD	VERIFIED	09:26
EXTERNAL STANDARD	0.020	09:26
BLANK TEST	0.000	09:27
EXTERNAL STANDARD	0.020	09:27
BLANK TEST	0.000	09:28
EXTERNAL STANDARD	0.020	09:28
BLANK TEST	0.000	09:29
EXTERNAL STANDARD	0.020	09:29
BLANK TEST	0.000	09:30
EXTERNAL STANDARD	0.020	09:30
BLANK TEST	0.000	09:31

Average = 0.0200
Std Dev = 0.0000

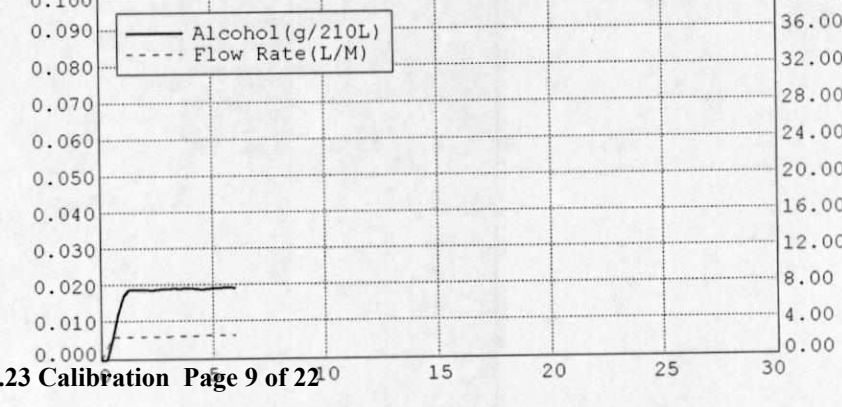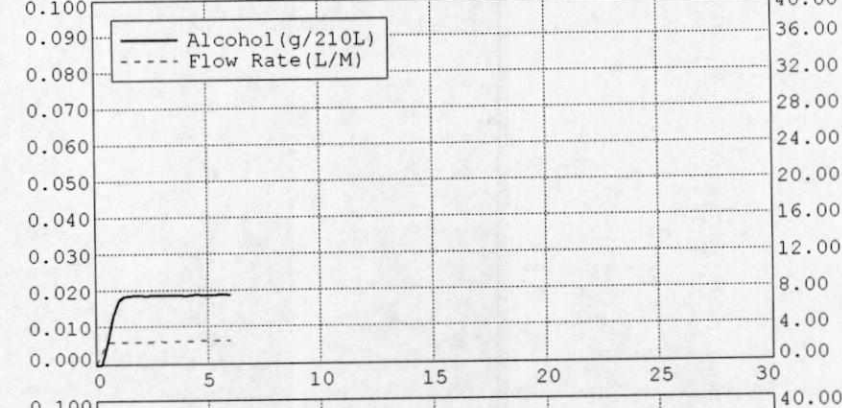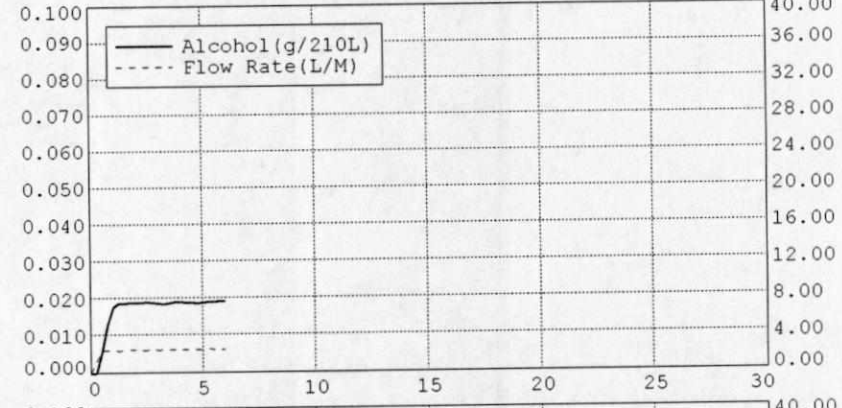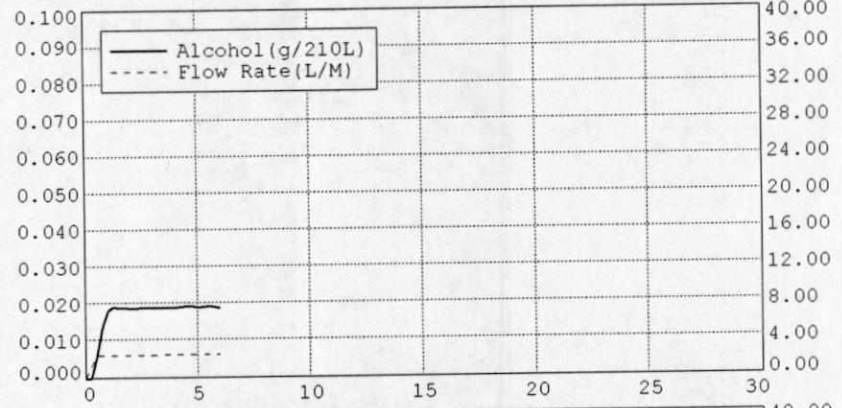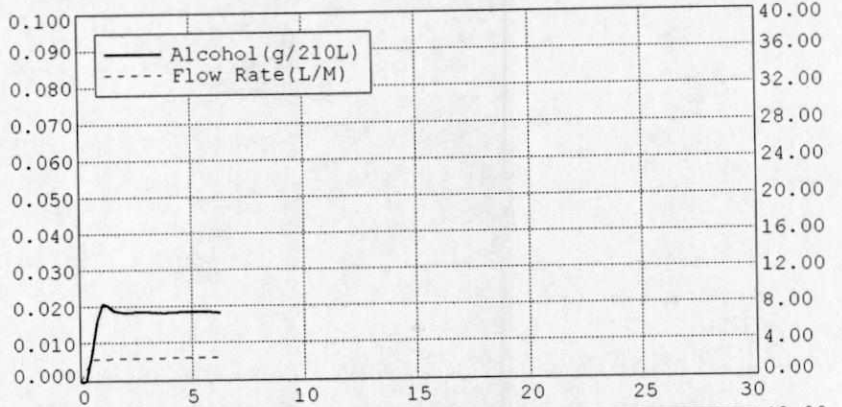

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100378






Date: 02/23/2024
 Time: 09:32:58

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 29.17: 0.039
 LOT #: AG217904
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 789 psi

BLANK TEST	0.000	09:34
INTERNAL STANDARD	VERIFIED	09:34
EXTERNAL STANDARD	0.039	09:34
BLANK TEST	0.000	09:35
EXTERNAL STANDARD	0.040	09:35
BLANK TEST	0.000	09:36
EXTERNAL STANDARD	0.039	09:36
BLANK TEST	0.000	09:37
EXTERNAL STANDARD	0.040	09:38
BLANK TEST	0.000	09:38
EXTERNAL STANDARD	0.040	09:39
BLANK TEST	0.000	09:40

Average = 0.0396
 Std Dev = 0.0005

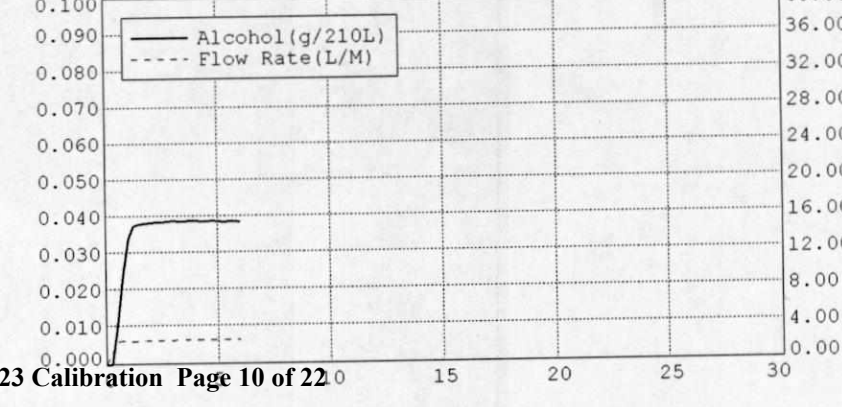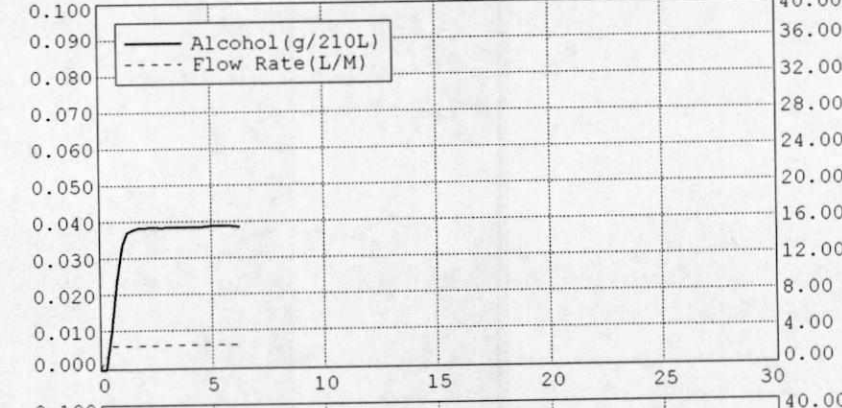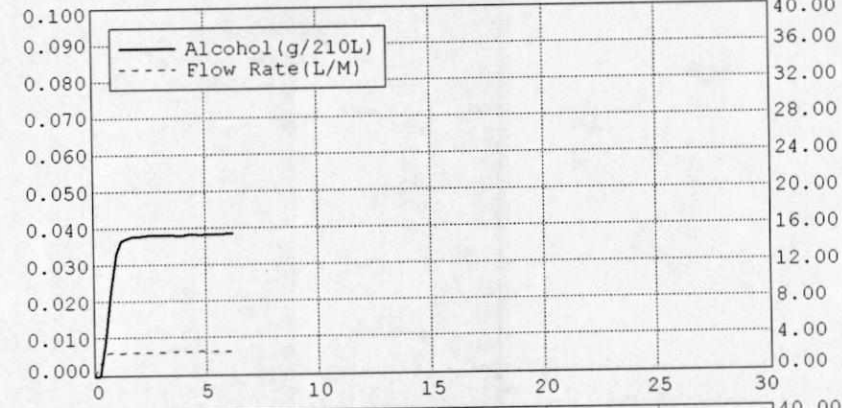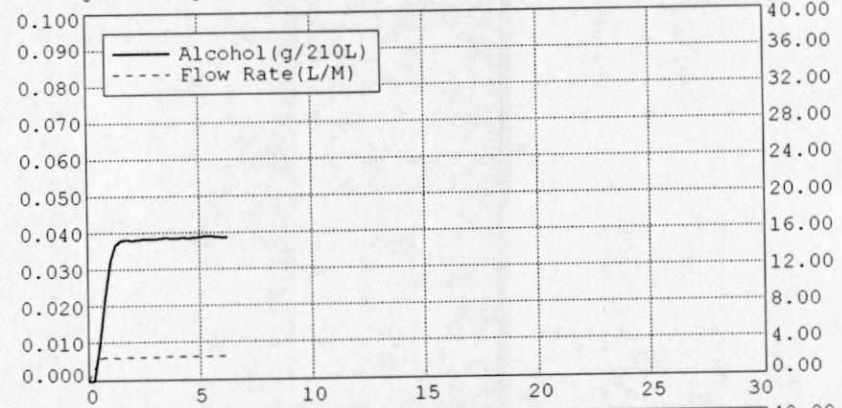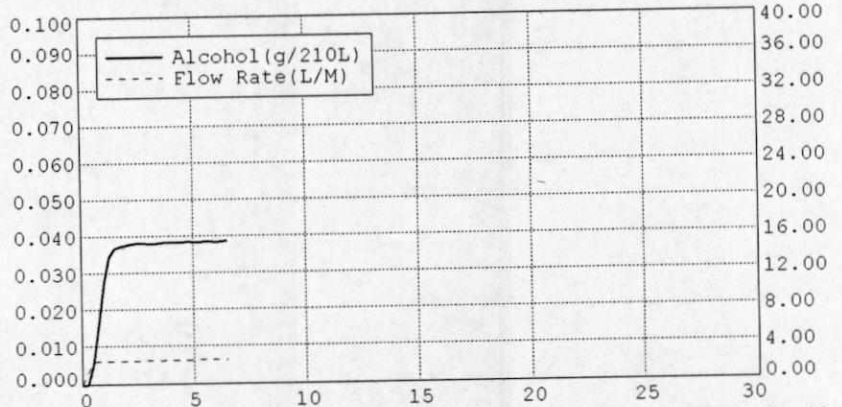

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100378






Date: 02/23/2024
 Time: 09:40:44

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.17: 0.078
 LOT #: AG310901
 EXPIRATION: 04/19/2025
 TANK PRESSURE: 631 psi

BLANK TEST	0.000	09:42
INTERNAL STANDARD	VERIFIED	09:42
EXTERNAL STANDARD	0.078	09:42
BLANK TEST	0.000	09:43
EXTERNAL STANDARD	0.077	09:43
BLANK TEST	0.000	09:44
EXTERNAL STANDARD	0.078	09:44
BLANK TEST	0.000	09:45
EXTERNAL STANDARD	0.077	09:45
BLANK TEST	0.000	09:46
EXTERNAL STANDARD	0.077	09:46
BLANK TEST	0.000	09:47

Average = 0.0774
 Std Dev = 0.0005

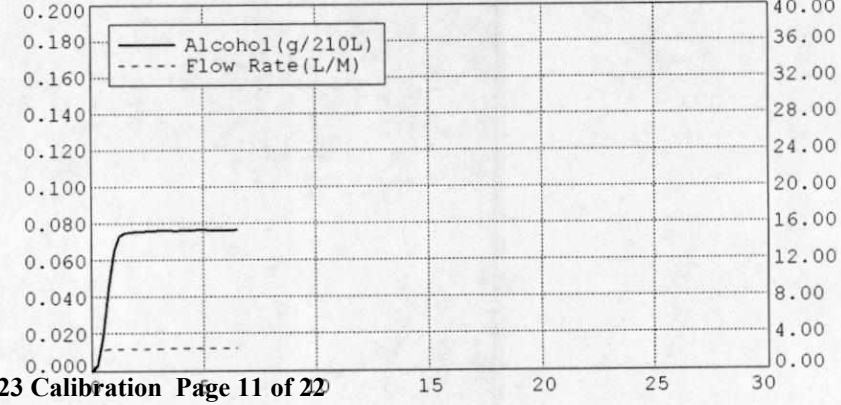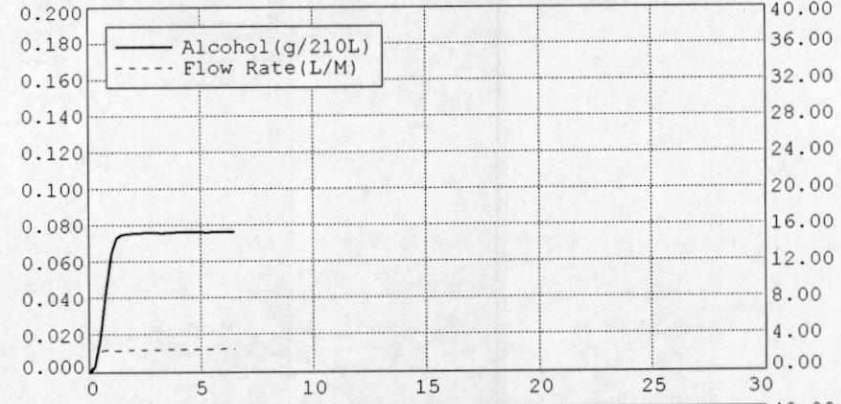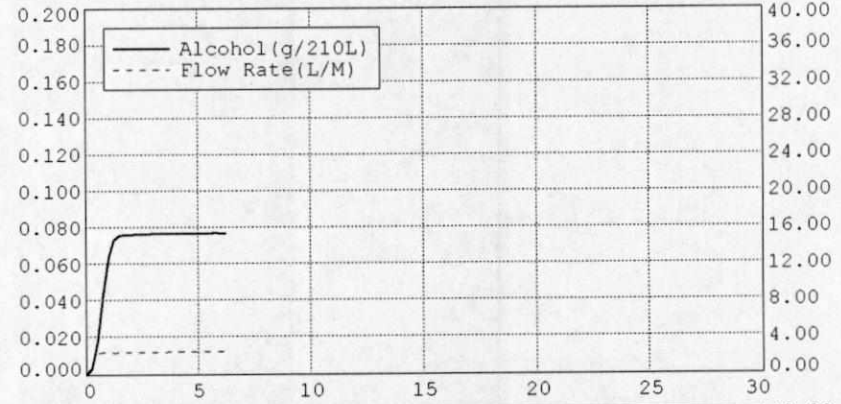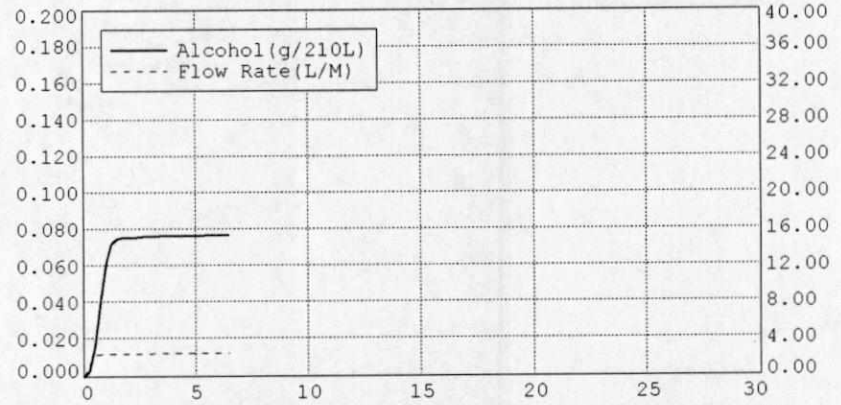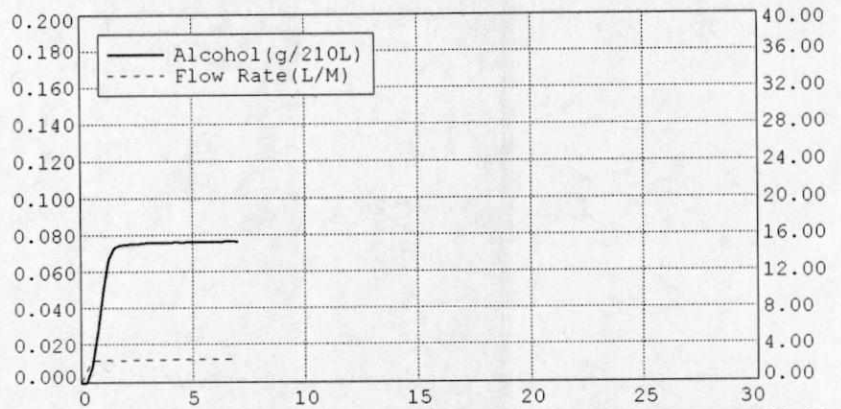

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100378






Date: 02/23/2024
Time: 09:48:19

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.16: 0.097
LOT #: AG2111003
EXPIRATION: 04/20/2024
TANK PRESSURE: 441 psi

BLANK TEST	0.000	09:49
INTERNAL STANDARD	VERIFIED	09:49
EXTERNAL STANDARD	0.099	09:50
BLANK TEST	0.000	09:51
EXTERNAL STANDARD	0.098	09:51
BLANK TEST	0.000	09:52
EXTERNAL STANDARD	0.098	09:52
BLANK TEST	0.000	09:53
EXTERNAL STANDARD	0.098	09:53
BLANK TEST	0.000	09:54
EXTERNAL STANDARD	0.098	09:54
BLANK TEST	0.000	09:55

Average = 0.0982
Std Dev = 0.0004

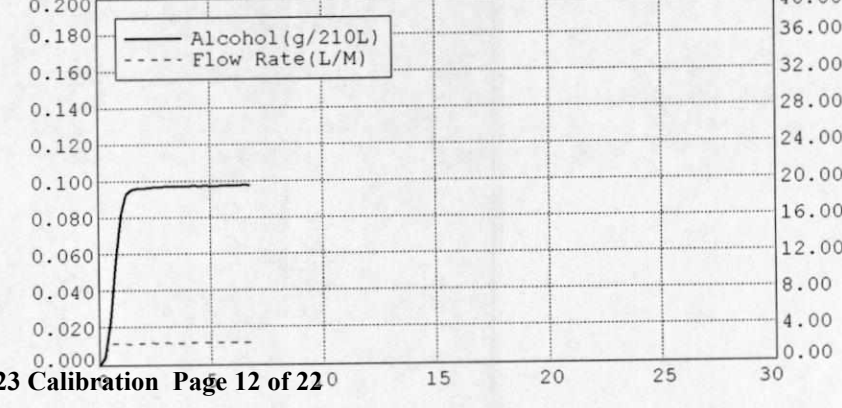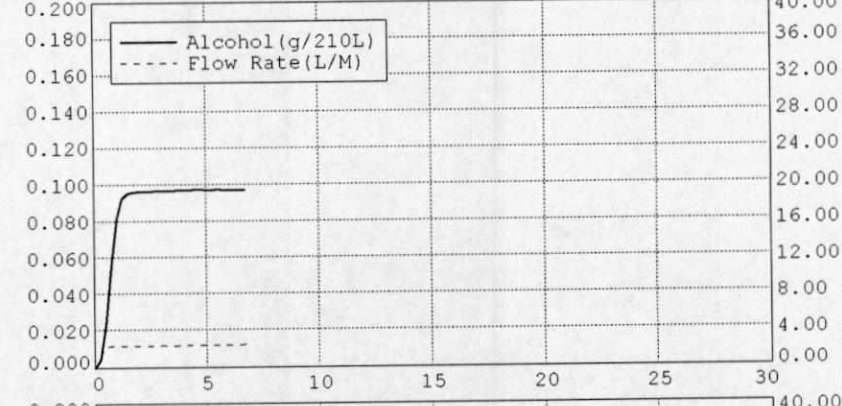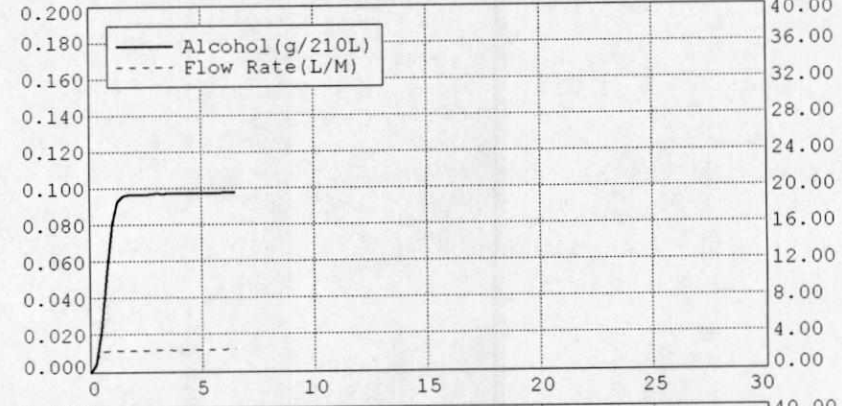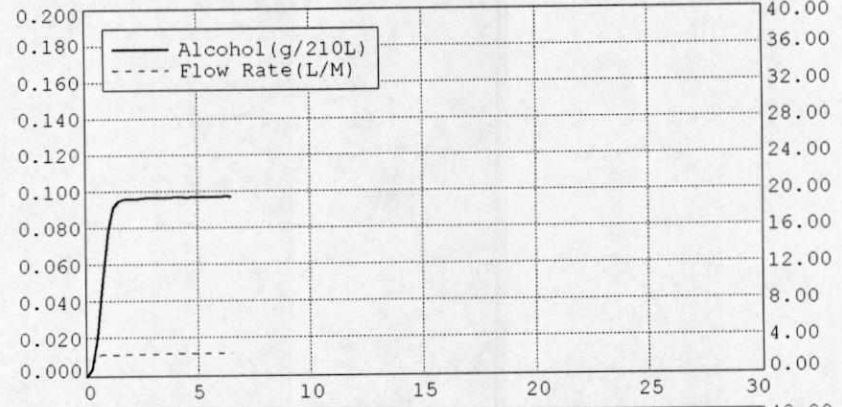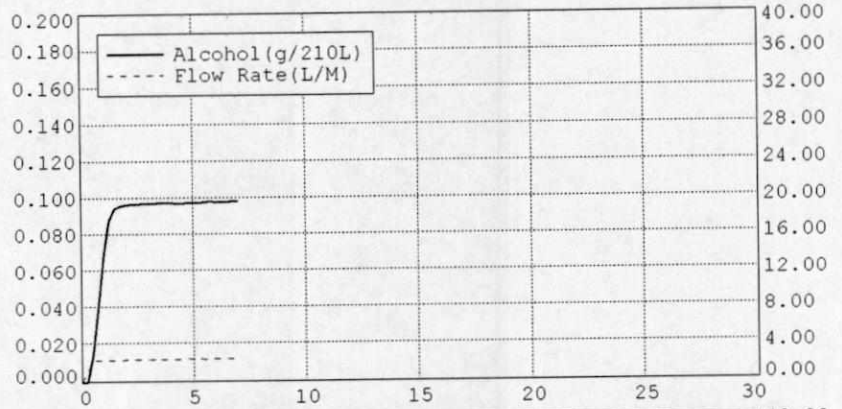

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100378






Date: 02/23/2024
 Time: 09:56:09

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 29.17: 0.146
 LOT #: AG332004
 EXPIRATION: 11/16/2025
 TANK PRESSURE: 700 psi

BLANK TEST	0.000	09:57
INTERNAL STANDARD	VERIFIED	09:57
EXTERNAL STANDARD	0.145	09:58
BLANK TEST	0.000	09:58
EXTERNAL STANDARD	0.144	09:59
BLANK TEST	0.000	10:00
EXTERNAL STANDARD	0.145	10:00
BLANK TEST	0.000	10:01
EXTERNAL STANDARD	0.144	10:01
BLANK TEST	0.000	10:02
EXTERNAL STANDARD	0.145	10:02
BLANK TEST	0.000	10:03

Average = 0.1446
 Std Dev = 0.0005

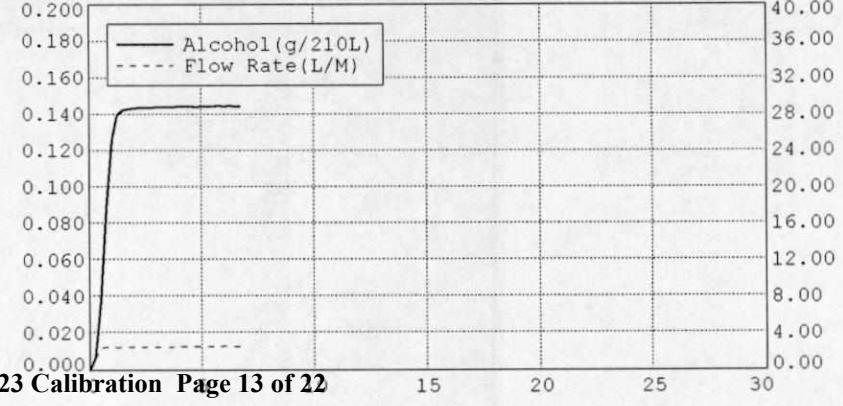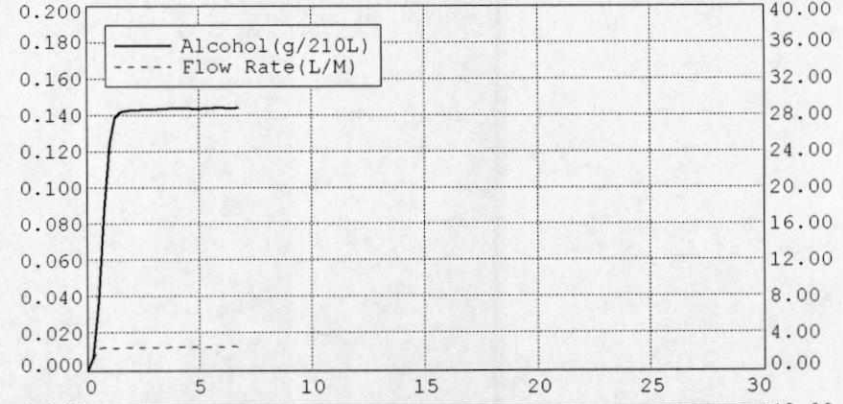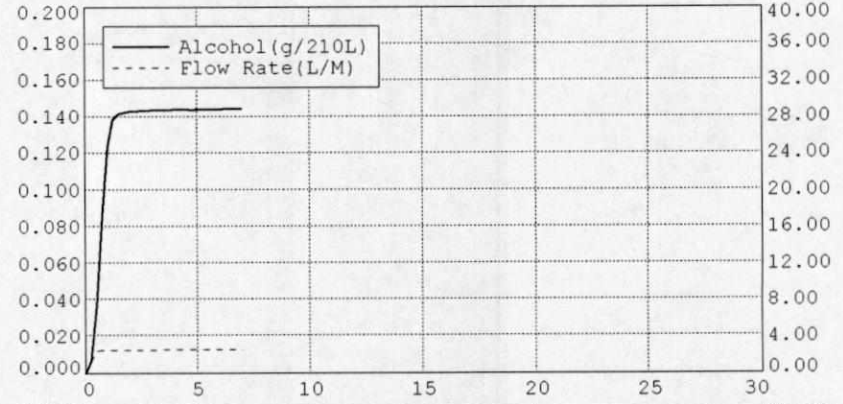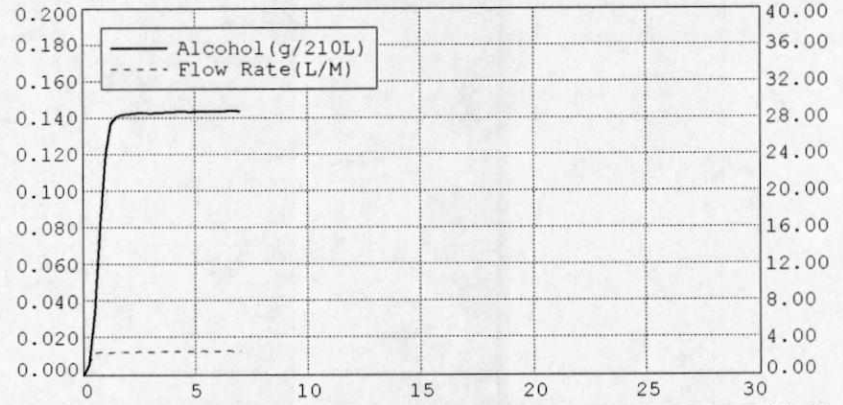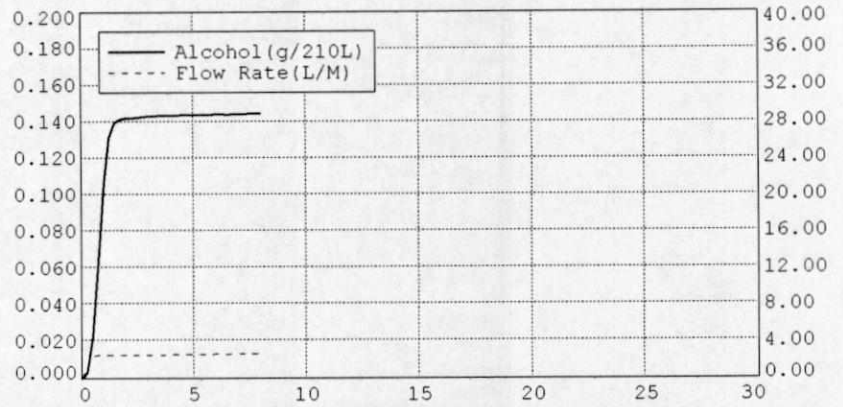

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100378






Date: 02/23/2024
Time: 10:04:07

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.17: 0.293
LOT #: AG327804
EXPIRATION: 10/05/2025
TANK PRESSURE: 313 psi

BLANK TEST	0.000	10:05
INTERNAL STANDARD	VERIFIED	10:05
EXTERNAL STANDARD	0.294	10:06
BLANK TEST	0.000	10:06
EXTERNAL STANDARD	0.294	10:07
BLANK TEST	0.000	10:08
EXTERNAL STANDARD	0.294	10:08
BLANK TEST	0.000	10:09
EXTERNAL STANDARD	0.293	10:09
BLANK TEST	0.000	10:10
EXTERNAL STANDARD	0.294	10:10
BLANK TEST	0.000	10:11

Average = 0.2938
Std Dev = 0.0004

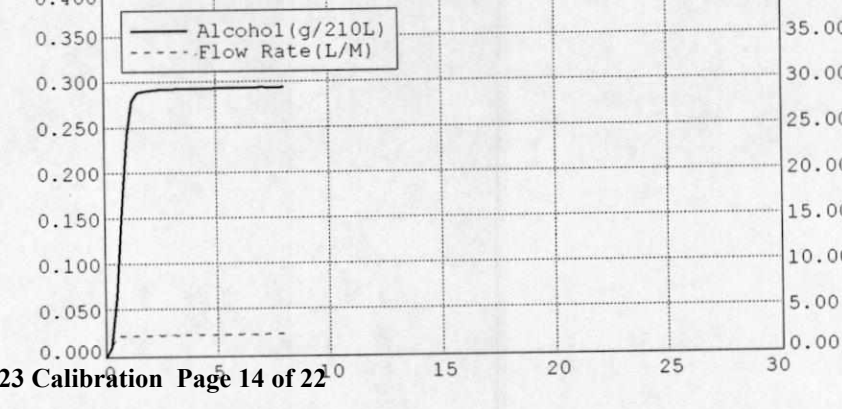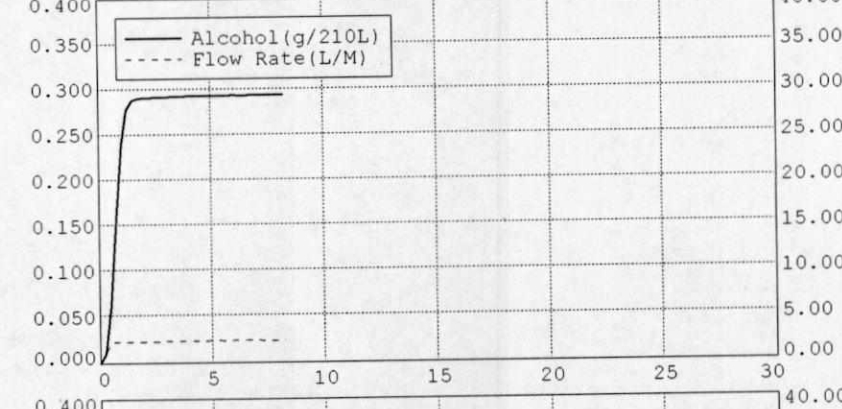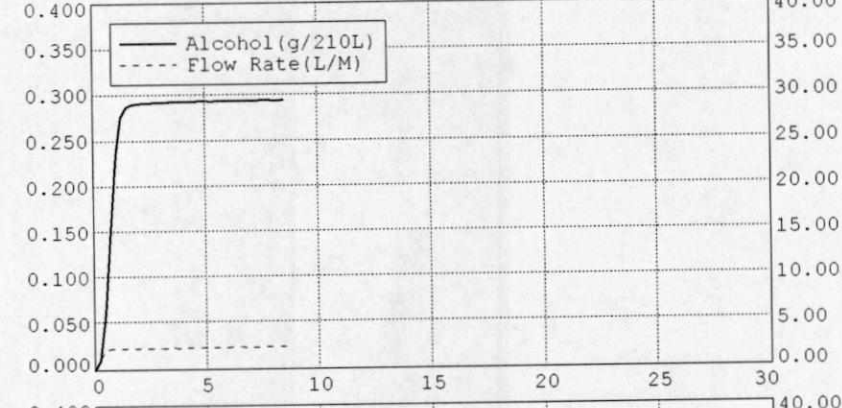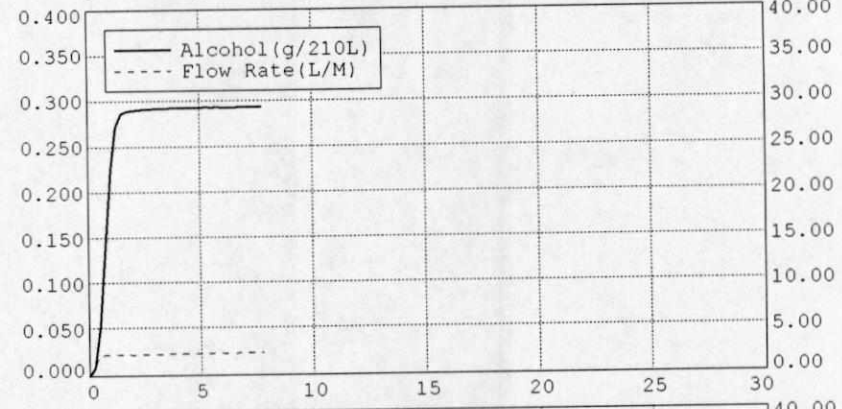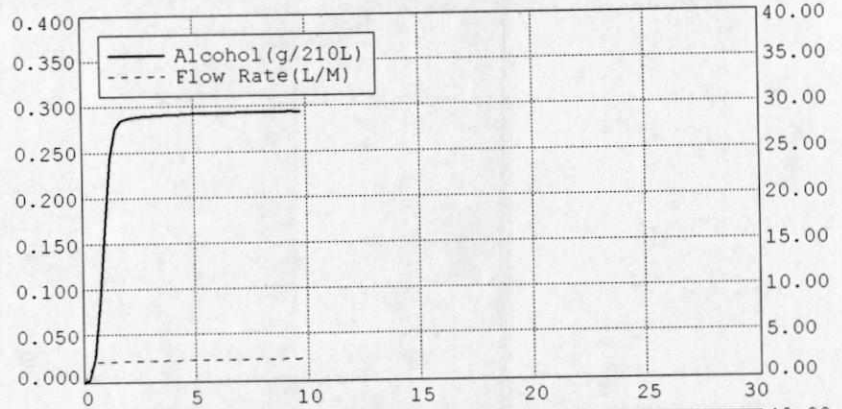

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100378

Date: 02/23/2024

Time: 10:29:25

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INCOMPLETE

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.17: 0.078

DIAGNOSTIC CHECK

PASSED 10:30

0.000 10:30

BLANK TEST

VERIFIED 10:30

0.078 10:31

INTERNAL STANDARD

0.000 10:32

BLANK TEST

INCOMPLETE 10:34

SUBJECT SAMPLE

CKG



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100378

Date: 02/23/2024
Time: 10:36:29

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
MAX ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078

DIAGNOSTIC CHECK PASSED 10:37
BLANK TEST 0.000 10:37
INTERNAL STANDARD VERIFIED 10:37
EXTERNAL STANDARD 0.077 10:37
BLANK TEST 0.000 10:38
SUBJECT SAMPLE XXX 10:39

Maximum Attempts Exceeded

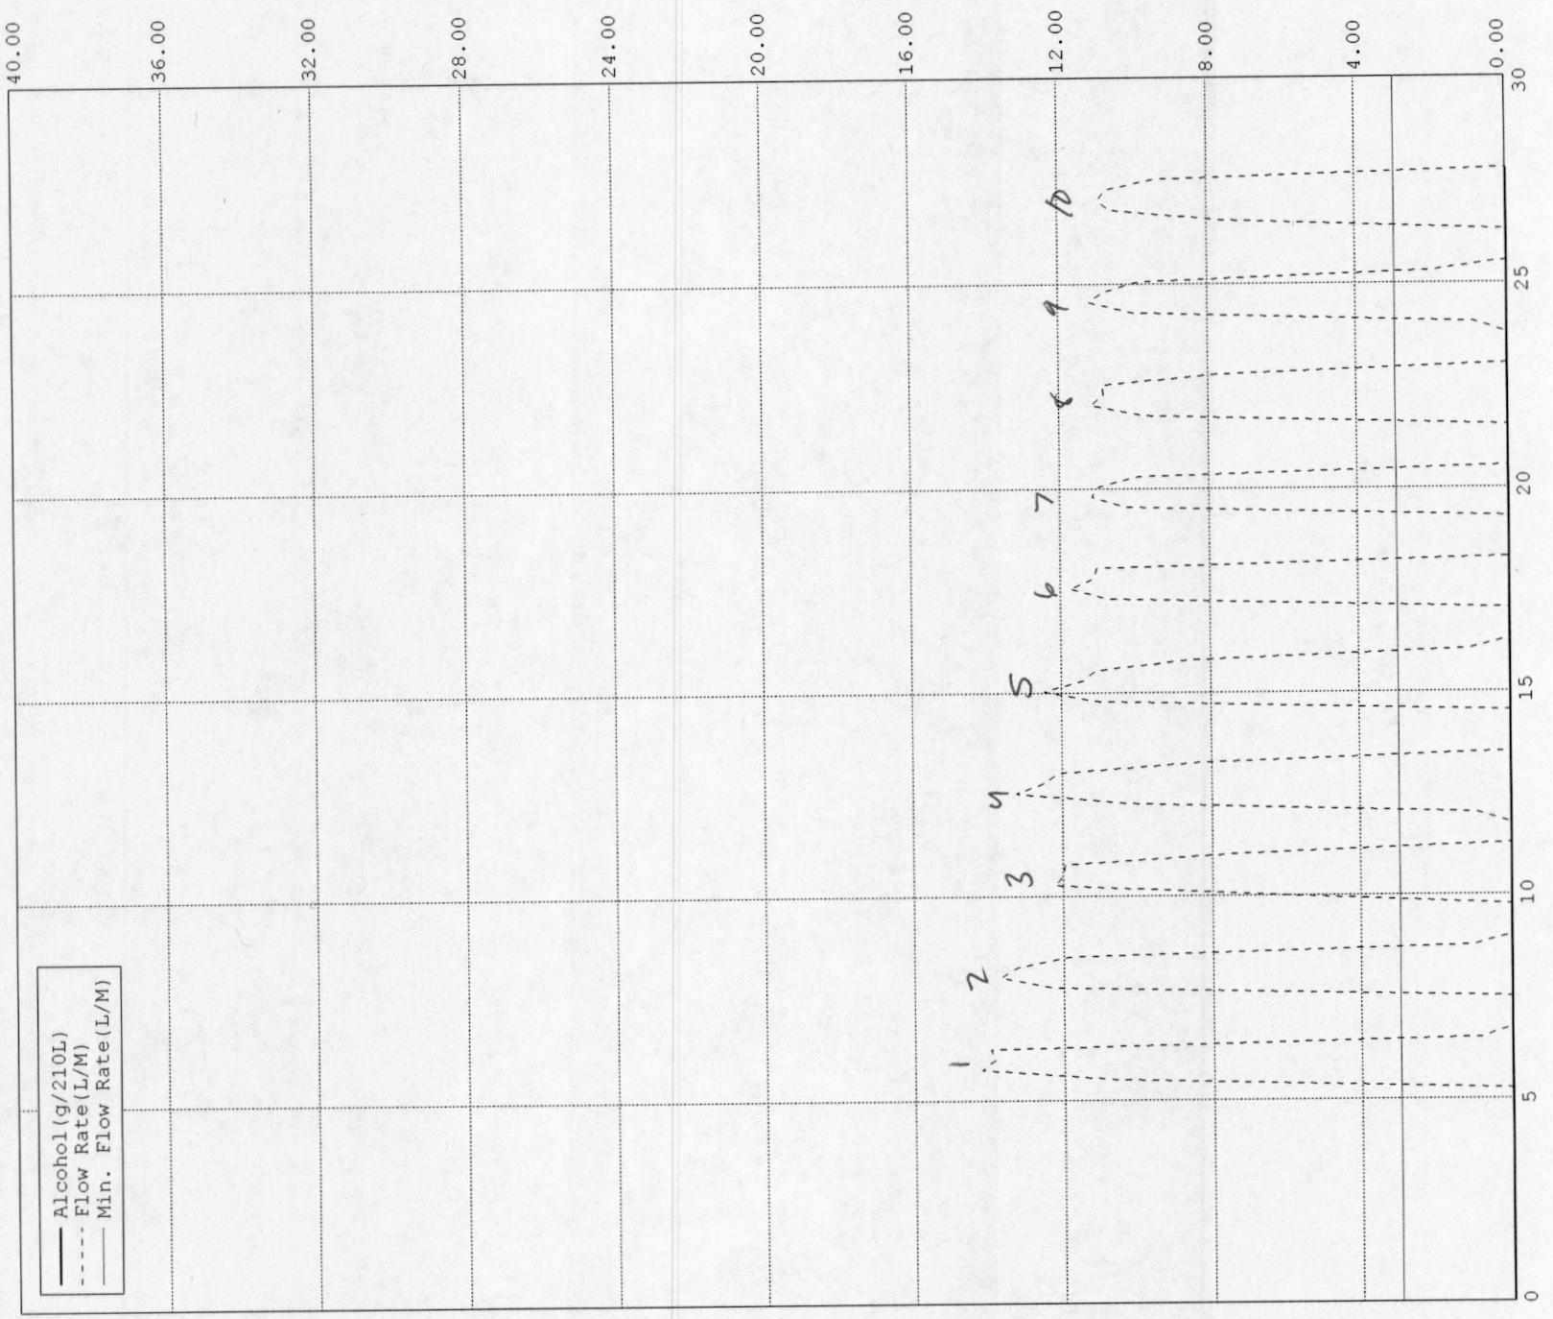

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100378

Date: 02/23/2024
Time: 10:41:23

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INVALID


CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.18: 0.078
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK
PASSED 10:43
BLANK TEST 0.000 10:43
INTERNAL STANDARD VERIFIED 10:44
EXTERNAL STANDARD 0.077 10:44
BLANK TEST 0.000 10:45
SUBJECT SAMPLE INVALID 10:45

OKG

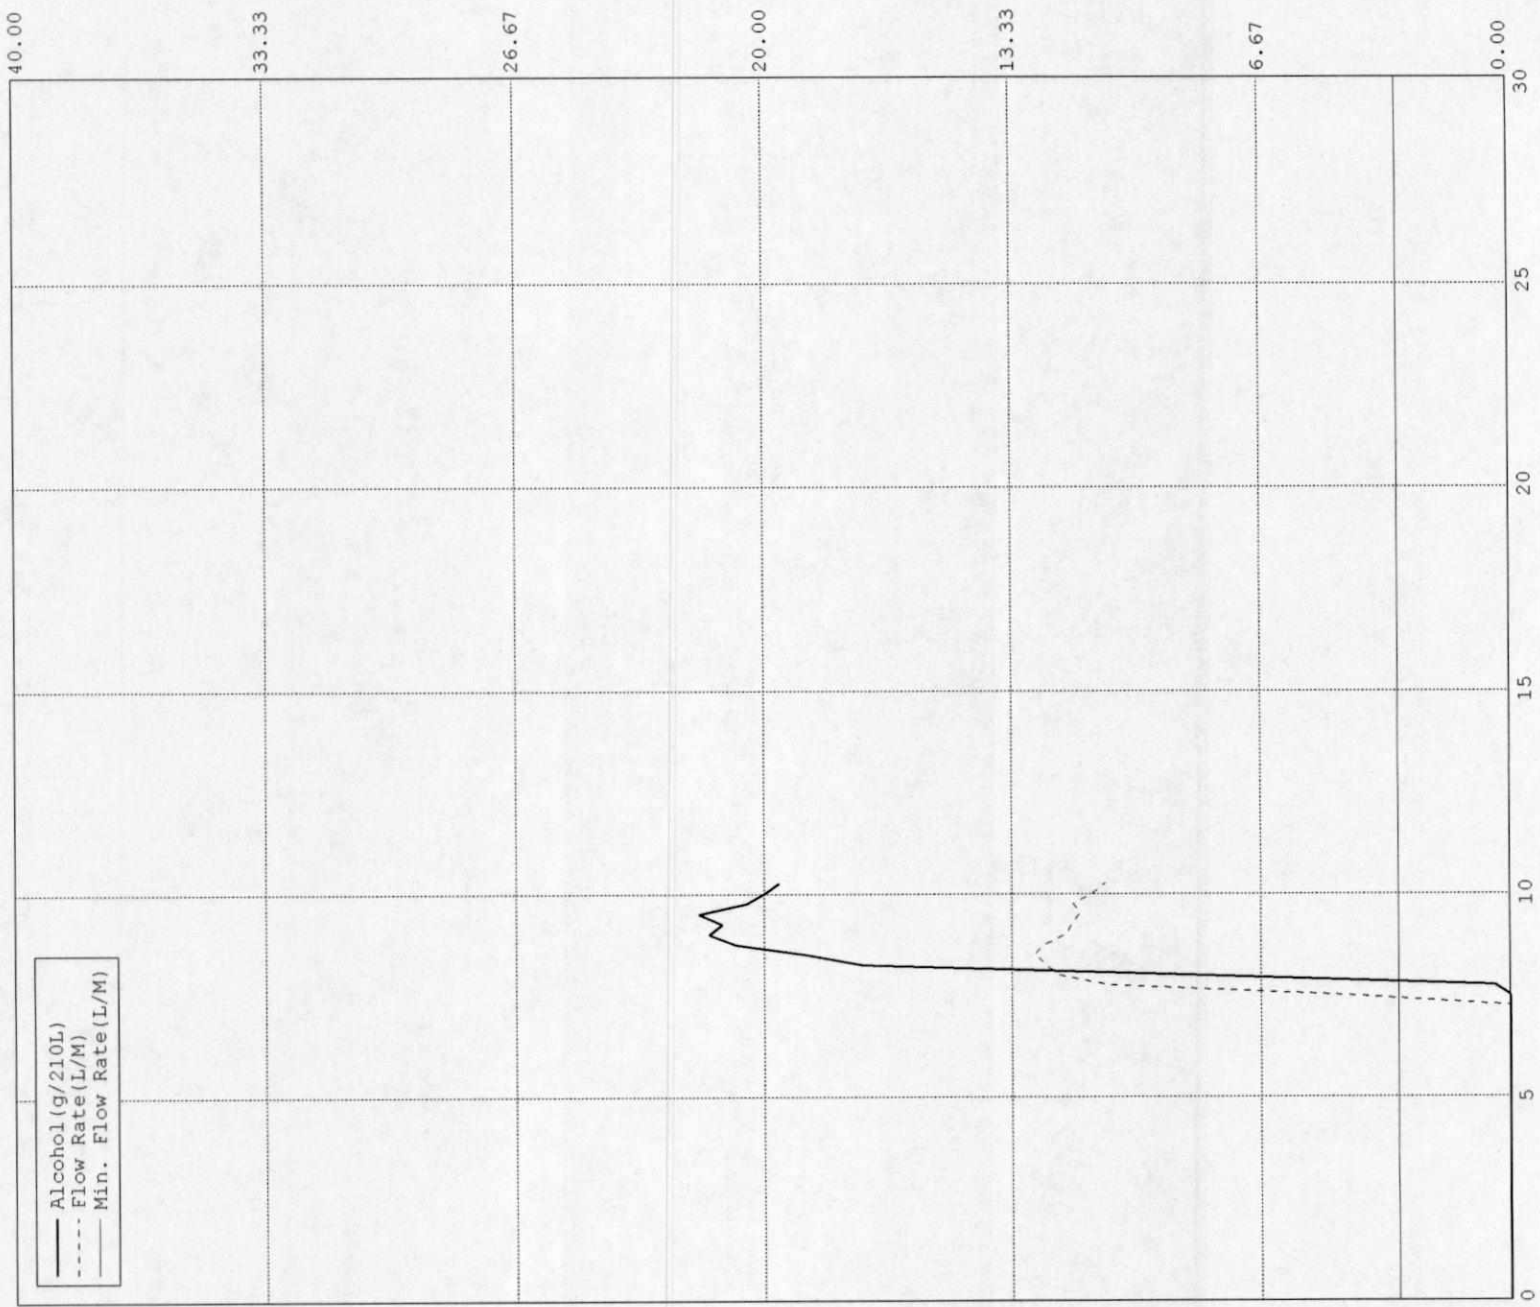

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100378

Date: 02/23/2024
Time: 10:48:14

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
RFI

CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 10:49
BLANK TEST 0.000 10:49
INTERNAL STANDARD VERIFIED 10:49
EXTERNAL STANDARD 0.078 10:49
BLANK TEST 0.000 10:50

RFI DETECTED



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100378

Date: 02/23/2024
Time: 11:55:57

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE ACETONE
BASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.19: 0.078
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	11:57
BLANK TEST	0.000	11:57
INTERNAL STANDARD	VERIFIED	11:57
Xq = 0.088 (1.30%)		
EXTERNAL STANDARD	0.078	11:57
X[1] = 0.0777 (-0.0014)	(0.0008)	
BLANK TEST	0.000	11:58
SUBJECT SAMPLE	XXX	11:59
X[1] = 0.1079 (-0.0170)	(0.0003)	

Interference Detected

filter 2 ave: ~~-0.0017~~ -0.0019 corrected on 3/28/2024 CKG
filter 3 ave: 0.0009

UUG-2123124

CKG



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100378

Date: 02/23/2024
Time: 12:03:04

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE IPA
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.19: 0.078

DIAGNOSTIC CHECK	PASSED	12:04
BLANK TEST	0.000	12:04
INTERNAL STANDARD	VERIFIED	12:04
Xq = 0.087	(0.00%)	
EXTERNAL STANDARD	0.077	12:04
X[1] = 0.0769	(-0.0025)	(0.0010)
BLANK TEST	0.000	12:05
SUBJECT SAMPLE	XXX	12:06
X[1] = 0.1151	(-0.0270)	(-0.0001)

Interference Detected

OKG



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100378

Date: 02/23/2024
Time: 12:08:37

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE NEGATIVE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.19: 0.078

DIAGNOSTIC CHECK	PASSED	12:09
BLANK TEST	0.000	12:09
INTERNAL STANDARD	VERIFIED	12:09
$X_q = 0.087$ (0.30%)		
EXTERNAL STANDARD	0.077	12:10
$X[1] = 0.0771$ (-0.0017)	(0.0013)	
BLANK TEST	0.000	12:11
SUBJECT SAMPLE (Vol=2.19L)	0.092	12:11
$X[1] = 0.0920$ (-0.0010)	(0.0006)	
BLANK TEST	0.000	12:12
EXTERNAL STANDARD	0.077	12:12
$X[1] = 0.0770$ (-0.0018)	(0.0003)	
BLANK TEST	0.000	12:13

CYG



SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100378

Date: 02/23/2024

Time: 12:42:14

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

NON DRINKING SUBJECT TEST

LEASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.18: 0.078

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	12:43
BLANK TEST	0.000	12:43
INTERNAL STANDARD	VERIFIED	12:43
EXTERNAL STANDARD	0.077	12:43
BLANK TEST	0.000	12:44
SUBJECT SAMPLE (Vol=1.64L)	0.000	12:45
BLANK TEST	0.000	12:46
EXTERNAL STANDARD	0.078	12:46
BLANK TEST	0.000	12:47

Handwritten signature/initials

