

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100382

Analyst or Technician Name: Carlie Glaister

DataMaster DMT Calibration Start Date: 12/8/25

Diagnostic Test

☒ Perform Diagnostic Test (View Details)

☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

☒ Adjust Voltages (if needed)

- Lamp (2.60 V Maximum)

- Bias

- Cooler (2.00 V Maximum)

☒ Set RFI Sensitivity

☒ Adjust internal barometer reading to match NIST-traceable barometer

Barometer/Thermometer/Hygrometer S/N: 240680771

Calibration Due Date: 9/10/26

☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed

☒ Print Technician Screen

☒ Print "Cal Factors"

Minimum Volume Test

☒ Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.28 Temperature(C) 22.0 Relative Humidity(%) 4

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

☒ Incomplete

☒ Invalid

☒ Maximum Attempts Exceeded

☒ Radio Frequency Interference (RFI)

☐ Interference (Volatiles) - Print with View Details

1. Acetone Reagent Lot Number: 20250922KS Expiration Date: 12/22/25

Simulator S/N: DR4178 Thermometer Verification Performed? ☒

2. Isopropanol Reagent Lot Number: 20250922KS Expiration Date: 12/22/25

Simulator S/N: DR4177 Thermometer Verification Performed? ☒

3. Negative (Ethanol Only) Lot Number: _____ Expiration Date: _____

Simulator S/N: _____ Thermometer Verification Performed? ☒

Calibrated External Thermometer S/N: 250159297

Calibration Due Date: 3/14/27

Administrative

☒ Verify Stylus Calibration

☐ Reset Options

☐ Clear Memory

☐ Verification of Calibration (VOC)

☐ Perform Non-Drinking Subject Test

☐ Upload Instrument

☐ Remove Dry Gas Tank Before Shutdown

☐ Add Ready for Tech Review Note

Completion

Lab Work End Date: 12/8/25

Data Interpretation Date (Technician): NA (if applicable)

Data Interpretation Date (Analyst): 12/8/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100382

Date: 12/08/2025
Time: 10:53:00

VERSIONS
DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 42.9°C PASSED
(38.0°C - 50.0°C)

SETTINGS
Lamp Voltage = 1.75 V PASSED
(1.05 V - 2.45 V)
Cooler Voltage = 1.62 V PASSED
(0.97 V - 2.27 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Freq = 510 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.3 in

PUMP INFO
Flow Rate = 4.460 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO
PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO
Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED
Xq = 0.081 0.22% (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100382

Date: 12/08/2025

Time: 10:57 AM

Temperatures (°C)

Sample Cell: 48.9°C

Breath Tube: 42.5°C

Current Barometer 29.3 in

Volume (Ltr) 1.49

Settings

Lamp: 1.83 V

Bias: 79 V

Cooler: 1.90 V

Chopper: 511 Hz

Voltages (V)

Flow: 1.04 V

Detector: -0.019 V

Rejected

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100382

Date: 10/20/2025
Time: 12:59:07

OPERATOR NAME:
DEREK WALTON
CERTIFICATE #: 9508

Ca	=	0.1000		
CAL	=	0.982484	0.800	<= CAL < 1.200
b1	=	0.0003	0.0000	<= b1 < 0.0040
b2	=	0.0059	0.0010	<= b2 < 0.0100
b3	=	0.0005	0.0000	<= b3 < 0.0040
Xq	=	0.0803	0.0500	<= Xq < 0.2000
a21	=	1.169428	1.050	<= a21 < 1.300
a31	=	0.464902	0.300	<= a31 < 0.800

Rejected

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100382

Date: 12/08/2025
 Time: 11:00:40

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXXX


OPERATOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

DEPT/AGENCY:
 MINIMUM VOLUME TEST
 CASE/REPORT: XXXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.26: 0.078
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:01
BLANK TEST	0.000	11:01
INTERNAL STANDARD	VERIFIED	11:01
EXTERNAL STANDARD	0.078	11:02
BLANK TEST	0.000	11:03
SUBJECT SAMPLE (Vol=1.51L)	0.000	11:04
BLANK TEST	0.000	11:05
EXTERNAL STANDARD	0.078	11:05
BLANK TEST	0.000	11:06

0865

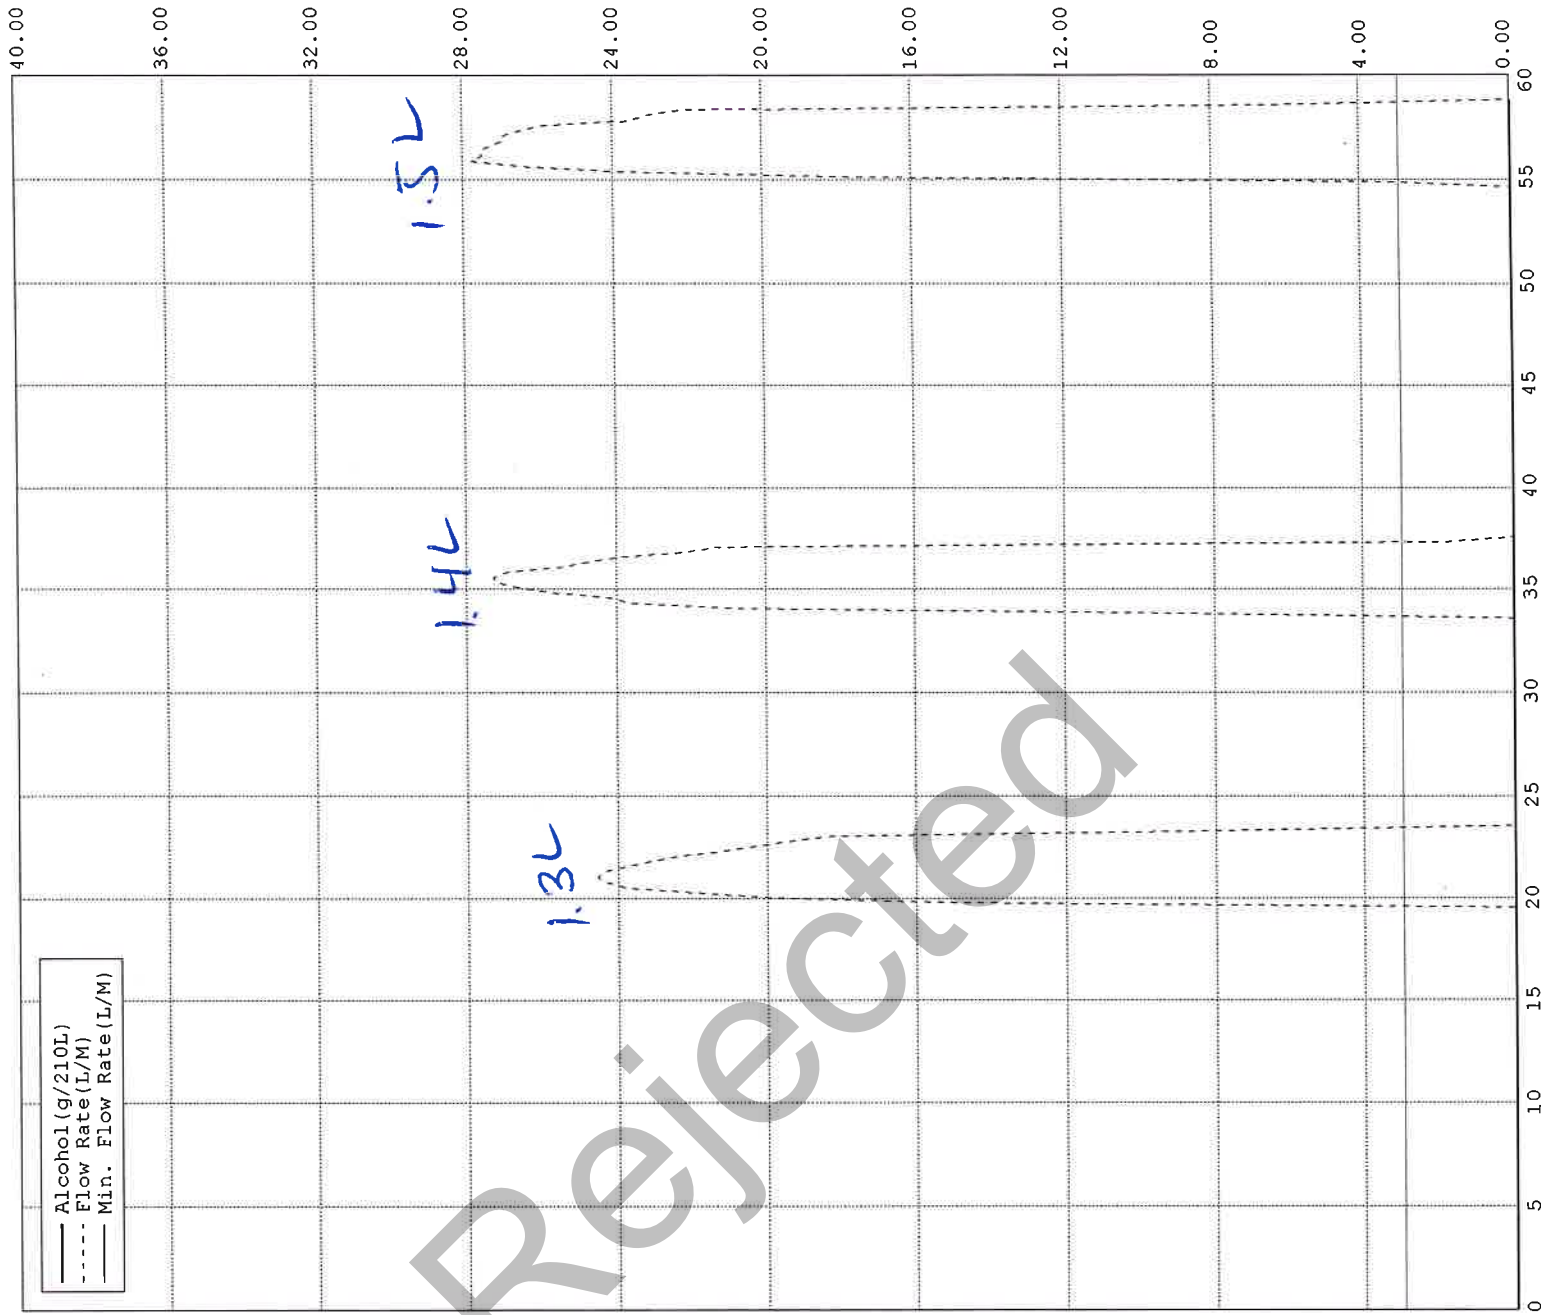

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100382

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 12/08/2025

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 295 psi

BLANK TEST	0.000	11:27
INTERNAL STANDARD	VERIFIED	11:27
EXTERNAL STANDARD	0.078	11:27
BLANK TEST	0.000	11:28
EXTERNAL STANDARD	0.078	11:28
BLANK TEST	0.000	11:29
EXTERNAL STANDARD	0.077	11:29
BLANK TEST	0.000	11:30
EXTERNAL STANDARD	0.078	11:30
BLANK TEST	0.000	11:31
EXTERNAL STANDARD	0.078	11:32
BLANK TEST	0.000	11:32

Average = 0.0778
Std Dev = 0.0004

Diagnostic Check

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C	PASSED
Breath Tube = 43.3°C	PASSED

PUMP INFO

Flow Rate = 4.452 L/M	PASSED
-----------------------	--------

DETECTOR INFO

PUMP ON	PASSED
PUMP OFF	PASSED

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD

PASSED

VOC post software reinstall OK 12/8/25

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100382

Date: 12/08/2025
Time: 12:34:19

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C	PASSED
(44.0°C - 52.0°C)	
Breath Tube = 44.1°C	PASSED
(38.0°C - 50.0°C)	

SETTINGS

Lamp Voltage = 1.83 V	PASSED
(1.05 V - 2.45 V)	
Cooler Voltage = 1.90 V	PASSED
(0.97 V - 2.27 V)	
Bias Voltage = 79 V	PASSED
(48 V - 112 V)	
Chopper Freq = 516 Hz	PASSED
(475 Hz - 575 Hz)	
Barometer = 29.3 in	

PUMP INFO

Flow Rate = 4.521 L/M	PASSED
(3.500 L/M - 6.500 L/M)	

DETECTOR INFO

PUMP ON	PASSED
(0.002 V <= 0.010 V)	
PUMP OFF	PASSED
(0.002 V <= 0.010 V)	

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD

Xq = 0.081 0.87%	PASSED
(0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100382

Date: 12/08/2025

Time: 12:43 PM

Temperatures (°C)

Sample Cell: 48.9°C

Breath Tube: 43.6°C

Current Barometer 29.3 in

Volume (Ltr) 1.42

Settings

Lamp: 1.83 V

Bias: 79 V

Cooler: 1.92 V

Chopper: 515 Hz

Voltages (V)

Flow: 1.03 V

Detector: 0.044 V

Rejected

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100382

Date: 12/08/2025
Time: 12:44:51

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.29: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:45
BLANK TEST	0.000	12:46
INTERNAL STANDARD	VERIFIED	12:46
EXTERNAL STANDARD	0.078	12:46
BLANK TEST	0.000	12:47
SUBJECT SAMPLE (Vol=1.63L)	XXX	12:48

Blank Error

Blank error occurred -
test re performed OMB
12/18/25

OMB

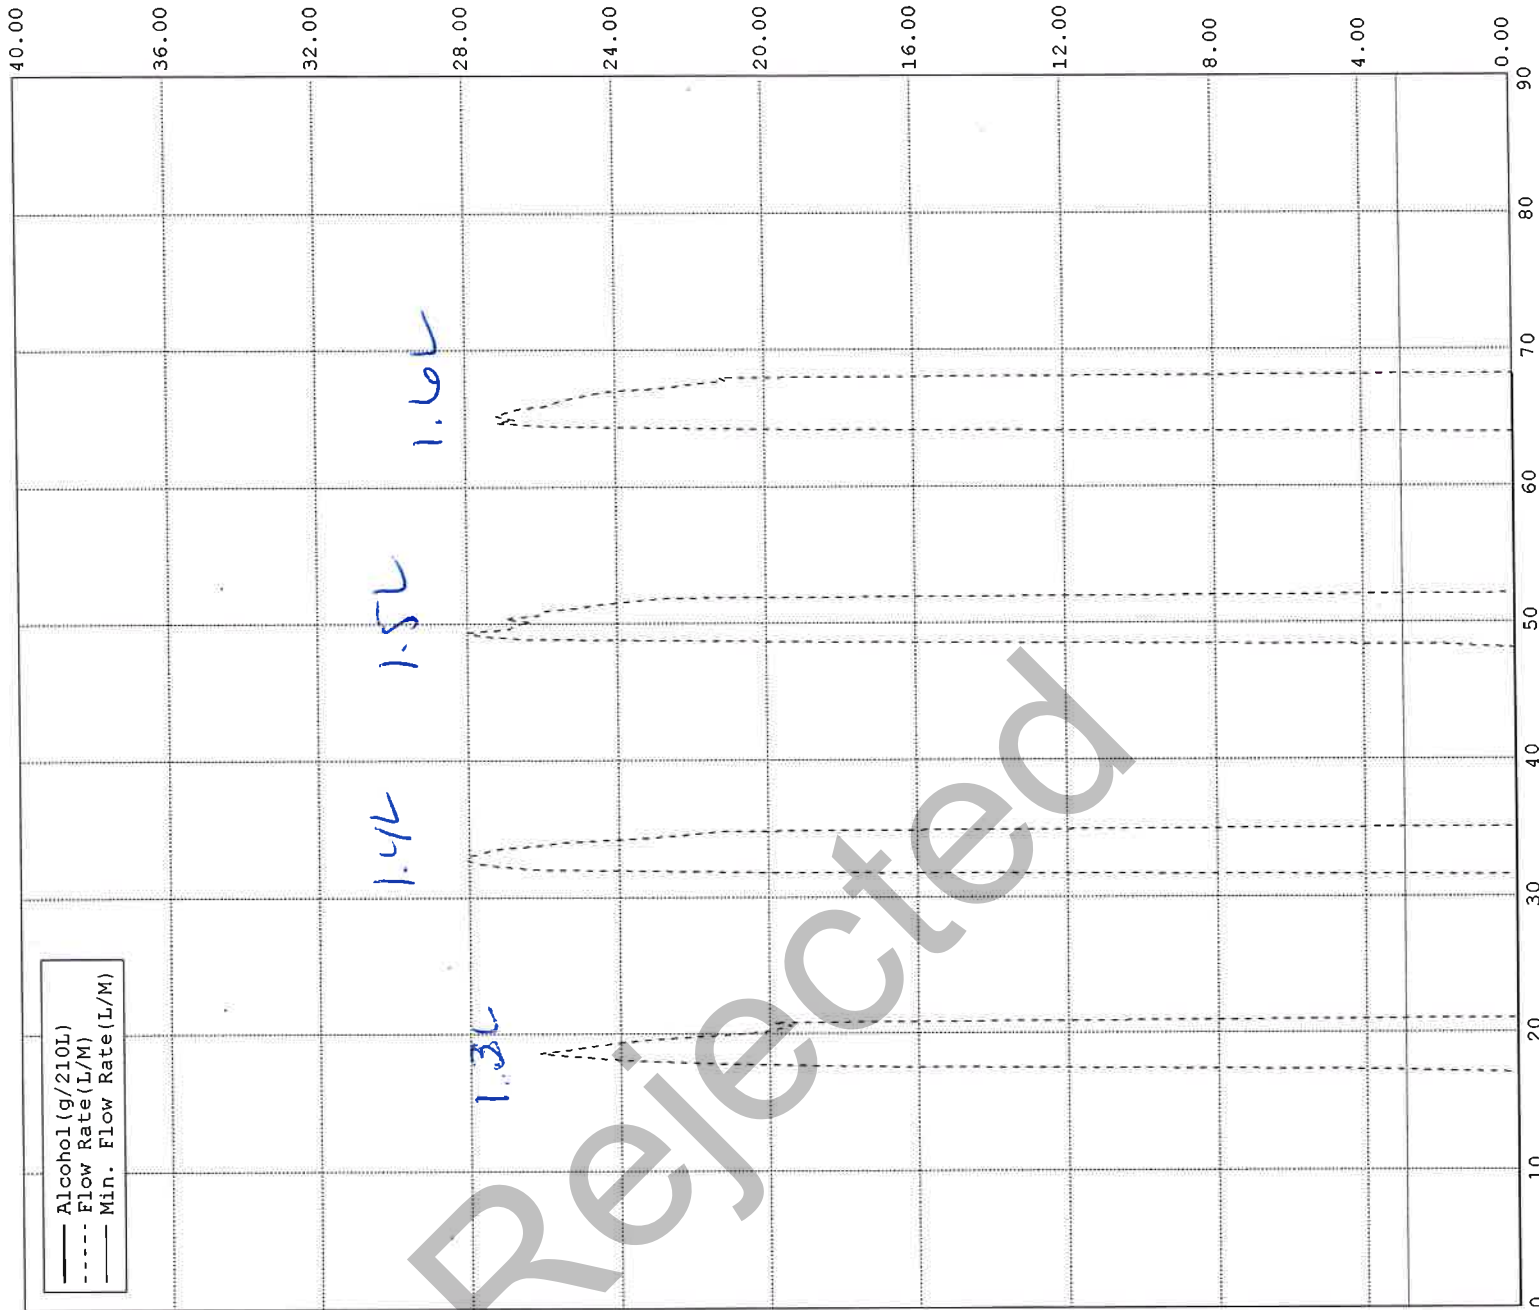

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100382

Date: 12/08/2025

Time: 12:52:18

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

MINIMUM VOLUME TEST

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080


TARGET AT 29.28: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:53
BLANK TEST	0.000	12:53
INTERNAL STANDARD	VERIFIED	12:53
EXTERNAL STANDARD	0.078	12:54
BLANK TEST	0.000	12:54
SUBJECT SAMPLE (Vol=1.63L)	0.000	12:55
BLANK TEST	0.000	12:56
EXTERNAL STANDARD	0.078	12:57
BLANK TEST	0.000	12:57

CARLIE

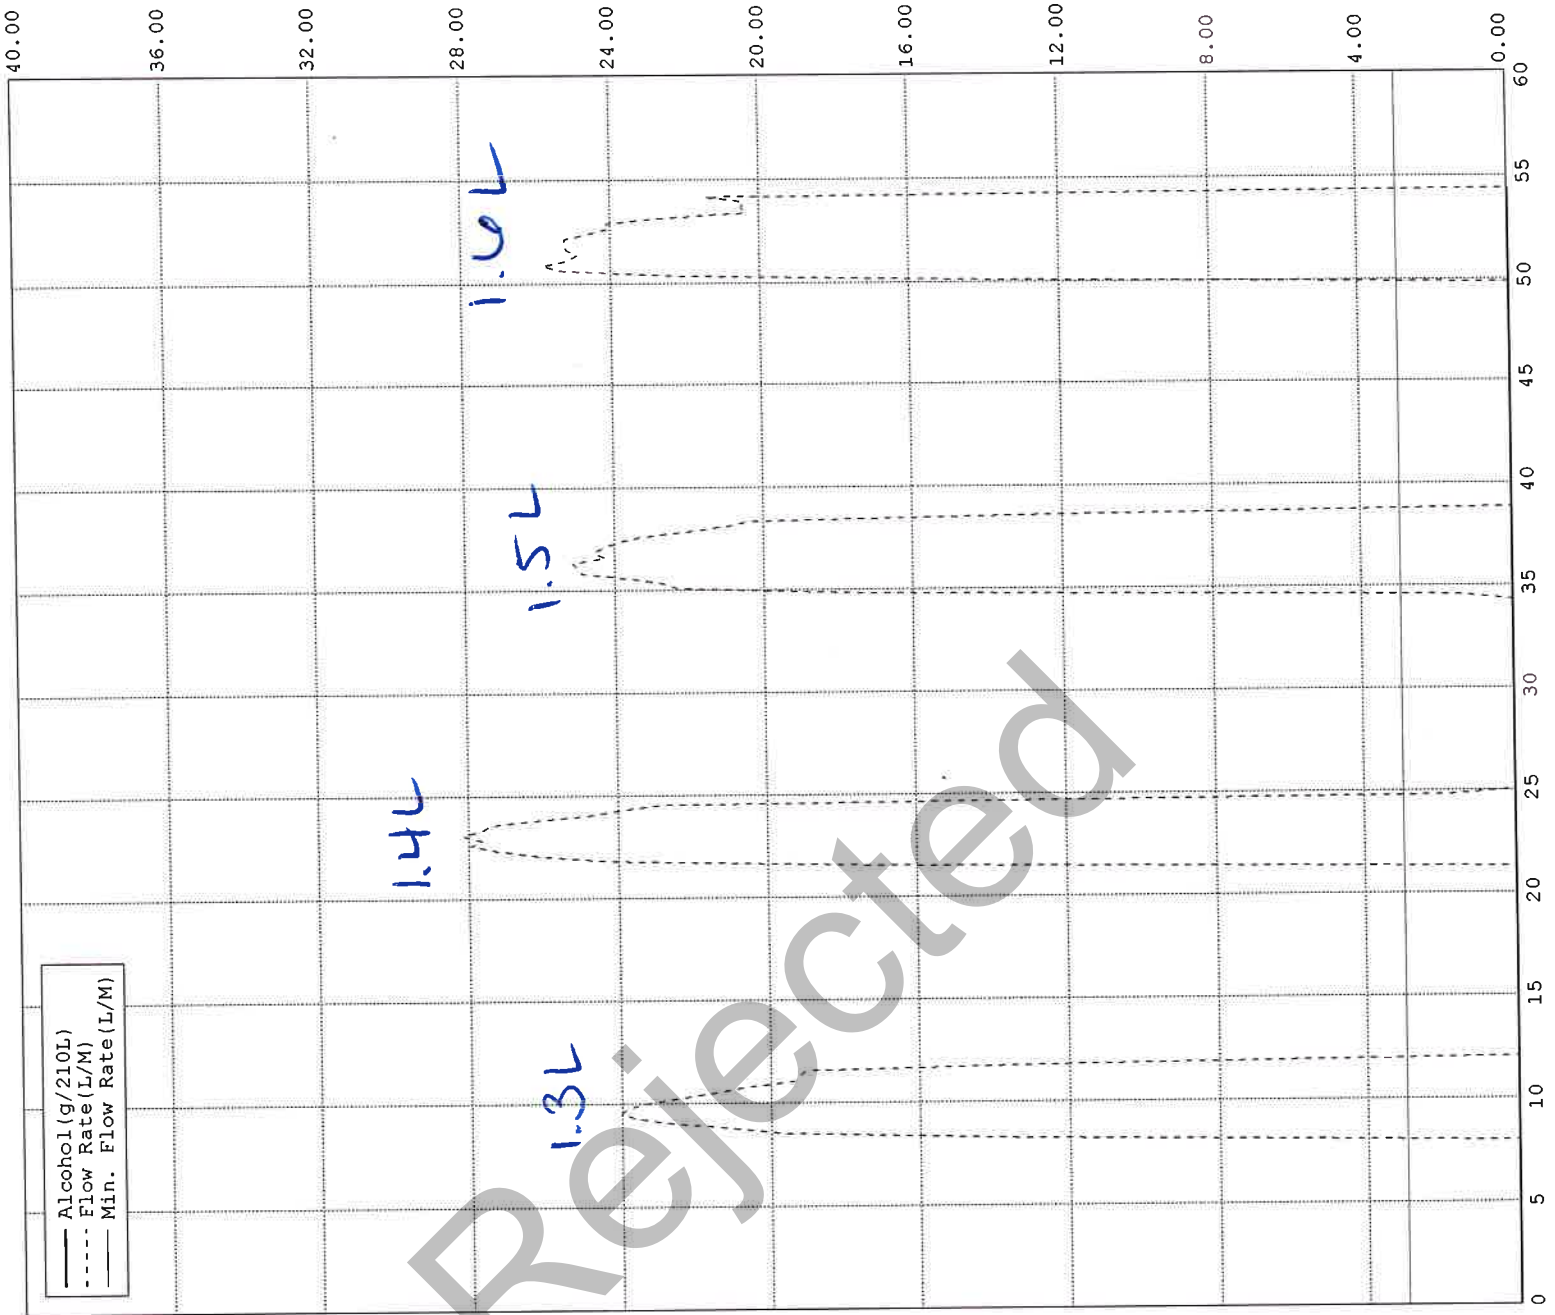

LINEARITY CHECK


Alaska Department of Public Safety
 DATAMASTER dmt: 100382

Date: 12/08/2025
 Time: 13:00:26

SUPERVISOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.039	0.0396	0.0005
0.078	0.0772	0.0004
0.098	0.0970	0.0000
0.147	0.1456	0.0005
0.294	0.2910	0.0007

SLOPE = 0.988001
 R² = 0.999987

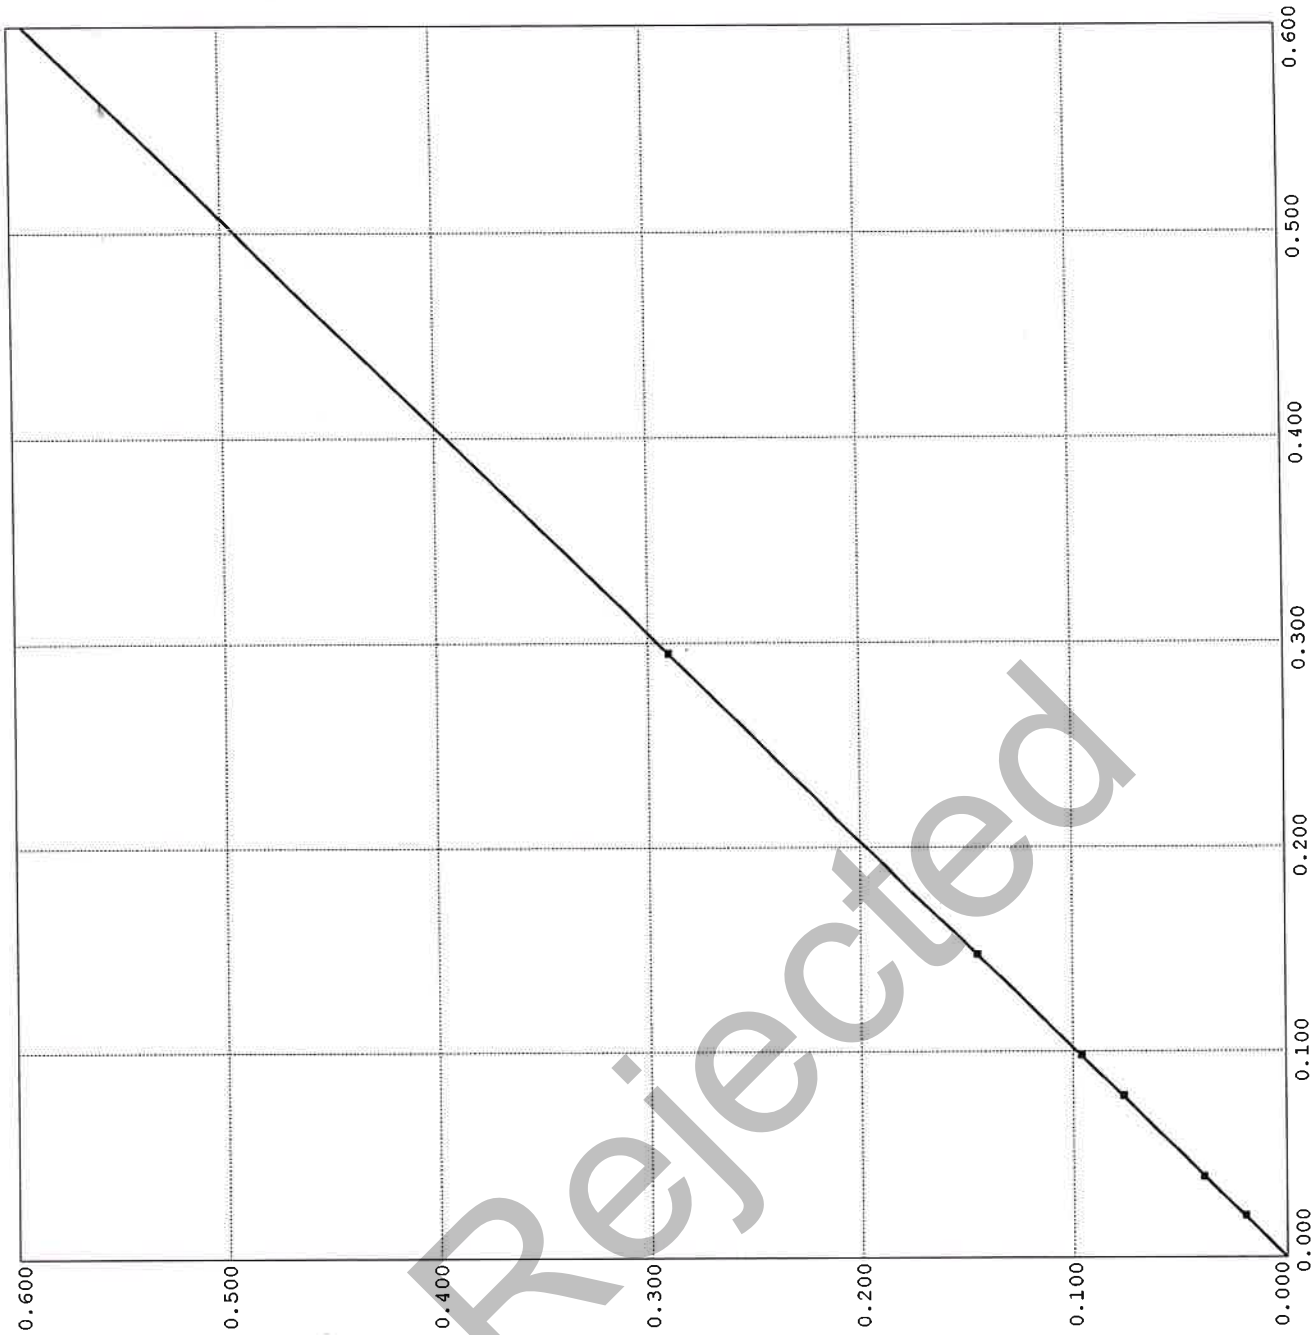

OK

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100382






Date: 12/08/2025
Time: 13:00:28

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.28: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 759 psi

TEST TYPE	Value	Time
BLANK TEST	0.000	13:01
INTERNAL STANDARD	VERIFIED	13:01
EXTERNAL STANDARD	0.020	13:02
BLANK TEST	0.000	13:02
EXTERNAL STANDARD	0.020	13:03
BLANK TEST	0.000	13:04
EXTERNAL STANDARD	0.020	13:04
BLANK TEST	0.000	13:05
EXTERNAL STANDARD	0.020	13:05
BLANK TEST	0.000	13:06
EXTERNAL STANDARD	0.020	13:06
BLANK TEST	0.000	13:07

Average = 0.0200
Std Dev = 0.0000

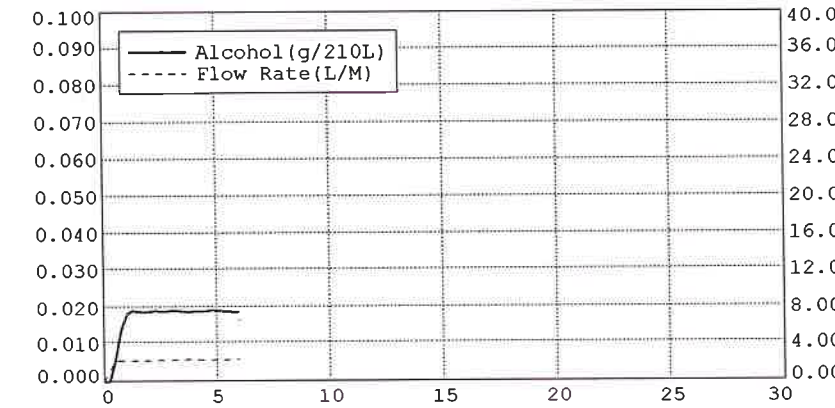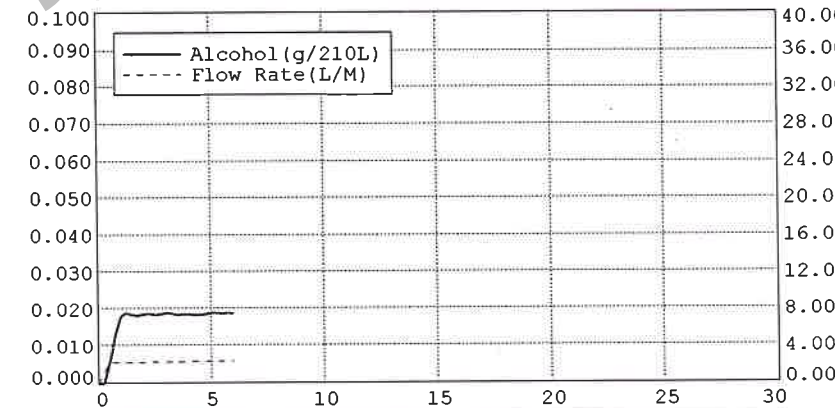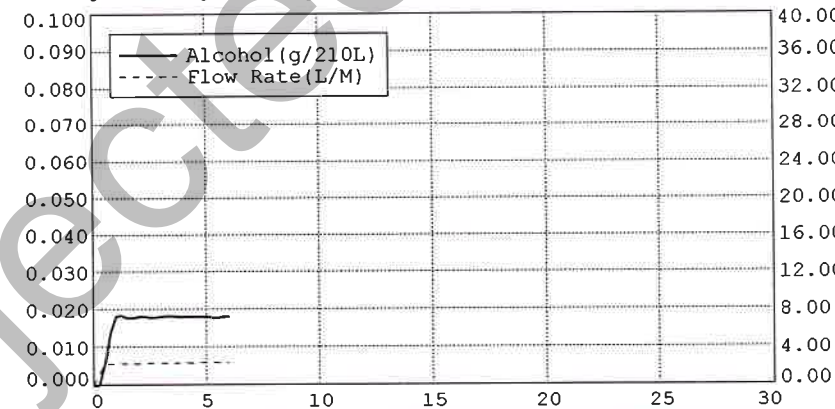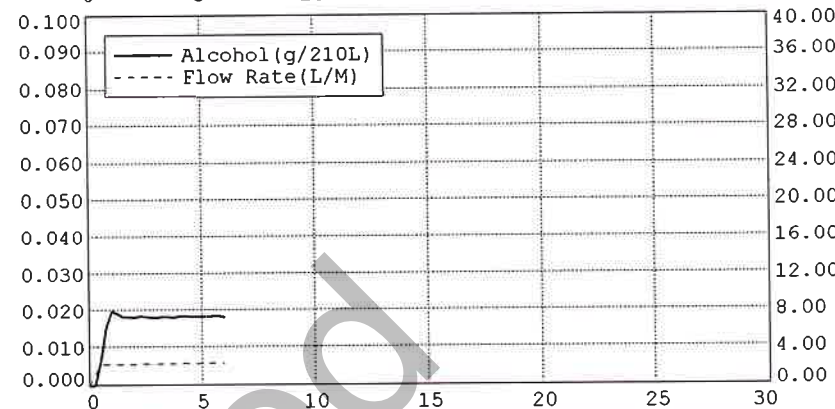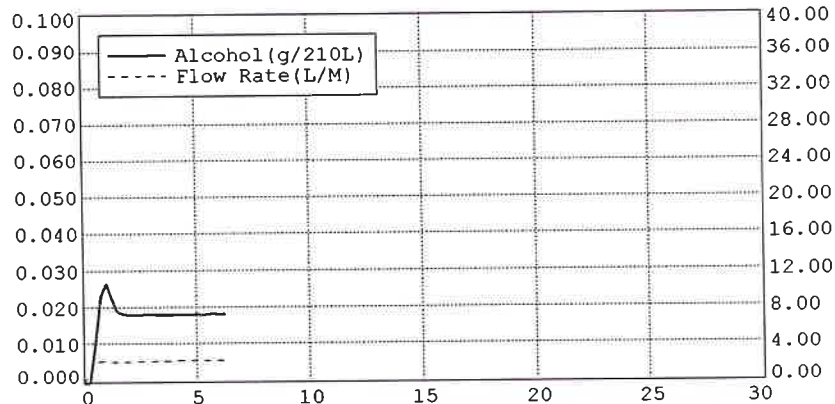

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100382






Date: 12/08/2025
Time: 13:08:23

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.28: 0.039
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 681 psi

BLANK TEST	0.000	13:09
INTERNAL STANDARD	VERIFIED	13:09
EXTERNAL STANDARD	0.040	13:09
BLANK TEST	0.000	13:10
EXTERNAL STANDARD	0.040	13:11
BLANK TEST	0.000	13:11
EXTERNAL STANDARD	0.040	13:12
BLANK TEST	0.000	13:13
EXTERNAL STANDARD	0.039	13:13
BLANK TEST	0.000	13:14
EXTERNAL STANDARD	0.039	13:14
BLANK TEST	0.000	13:15

Average = 0.0396
Std Dev = 0.0005

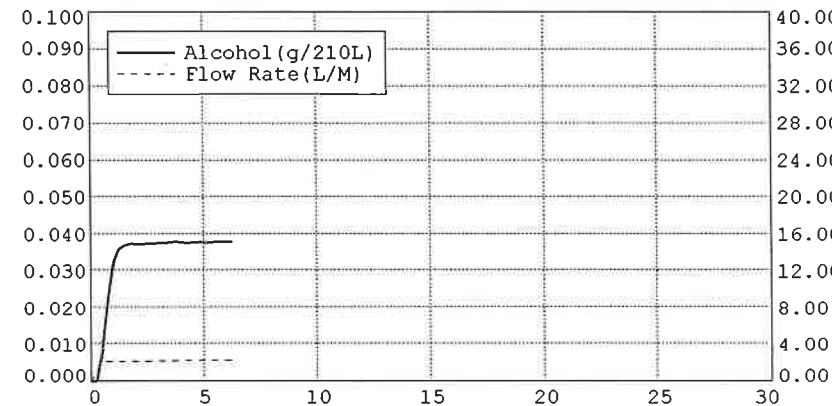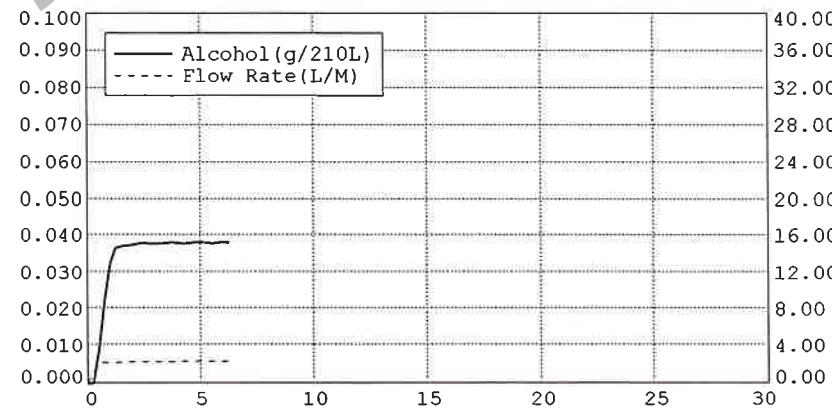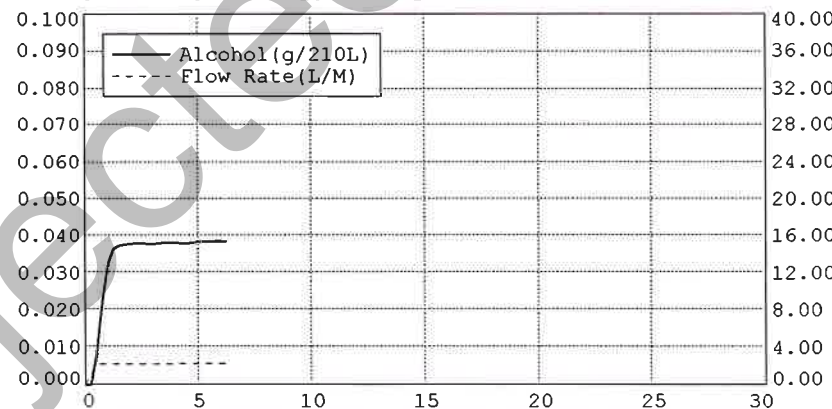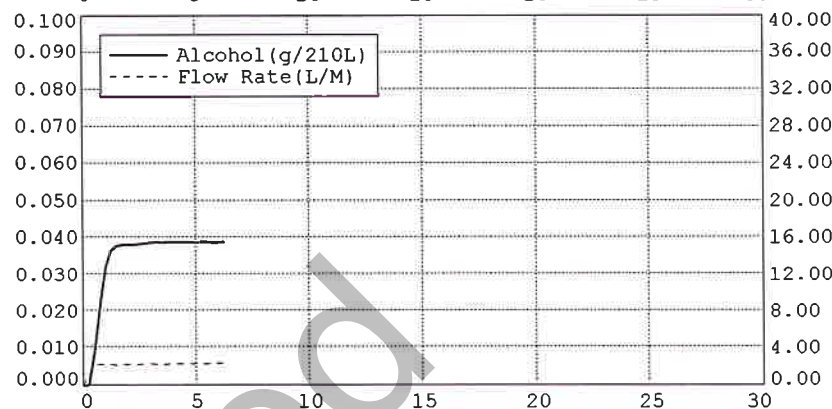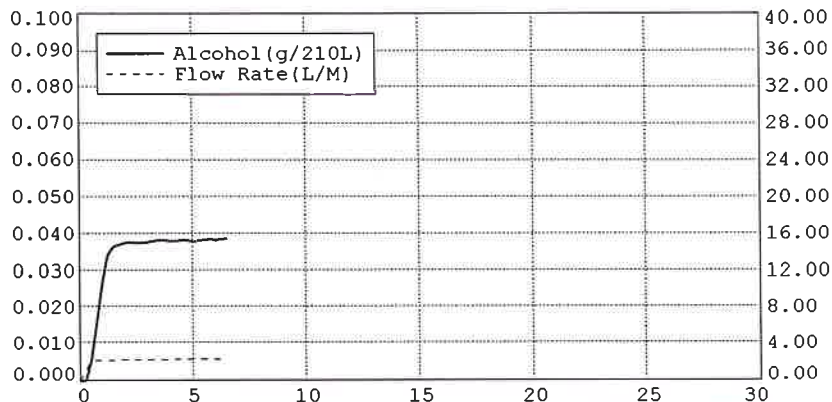

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100382






Date: 12/08/2025
Time: 13:17:10

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 270 psi

TEST TYPE	VALUE	TIME
BLANK TEST	0.000	13:18
INTERNAL STANDARD	VERIFIED	13:18
EXTERNAL STANDARD	0.077	13:18
BLANK TEST	0.000	13:19
EXTERNAL STANDARD	0.077	13:19
BLANK TEST	0.000	13:20
EXTERNAL STANDARD	0.077	13:20
BLANK TEST	0.000	13:21
EXTERNAL STANDARD	0.077	13:22
BLANK TEST	0.000	13:22
EXTERNAL STANDARD	0.078	13:23
BLANK TEST	0.000	13:24

Average = 0.0772
Std Dev = 0.0004

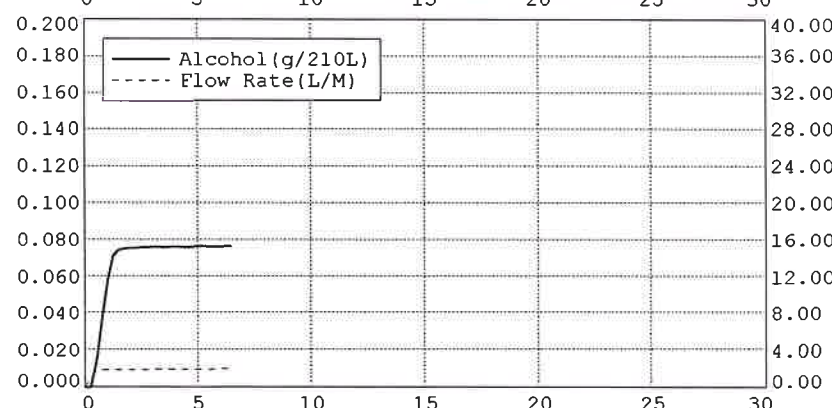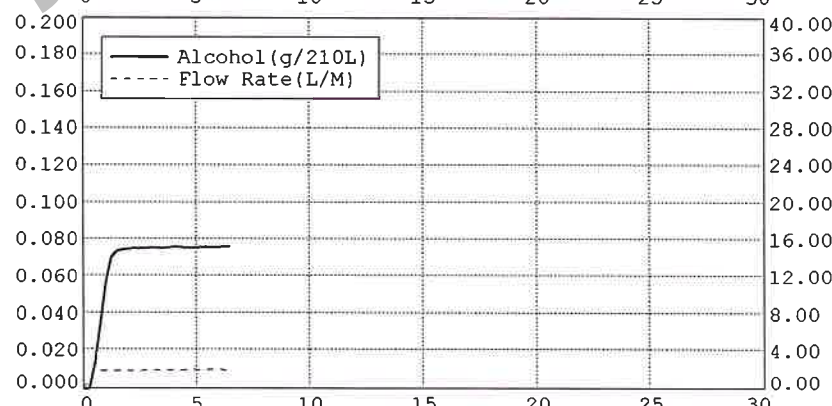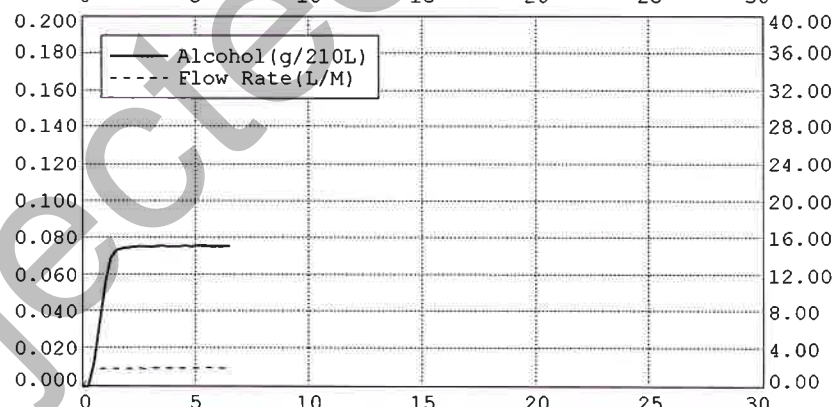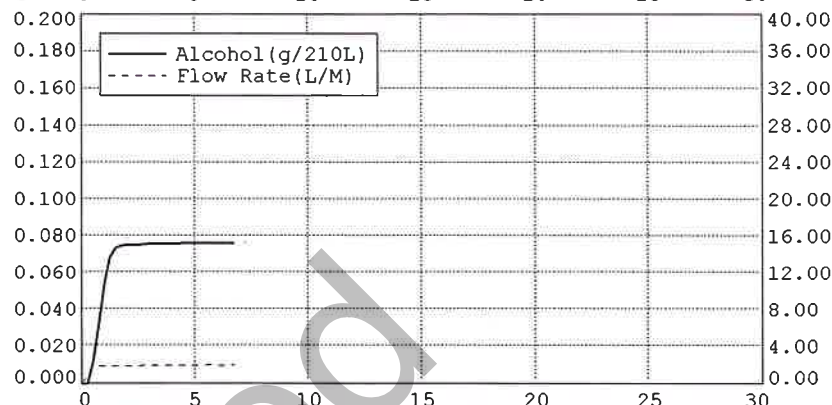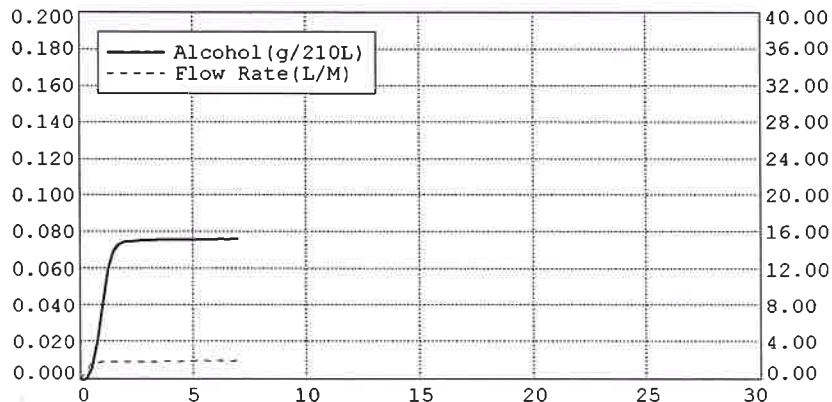

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100382






Date: 12/08/2025
Time: 13:24:44

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.28: 0.098
LOT #: AG516101
EXPIRATION: 06/10/2027
TANK PRESSURE: 1162 psi

TEST TYPE	CONCENTRATION (g/210L)	TIME
BLANK TEST	0.000	13:25
INTERNAL STANDARD	VERIFIED	13:25
EXTERNAL STANDARD	0.097	13:26
BLANK TEST	0.000	13:27
EXTERNAL STANDARD	0.097	13:27
BLANK TEST	0.000	13:28
EXTERNAL STANDARD	0.097	13:28
BLANK TEST	0.000	13:29
EXTERNAL STANDARD	0.097	13:29
BLANK TEST	0.000	13:30
EXTERNAL STANDARD	0.097	13:30
BLANK TEST	0.000	13:31

Average = 0.0970
Std Dev = 0.0000

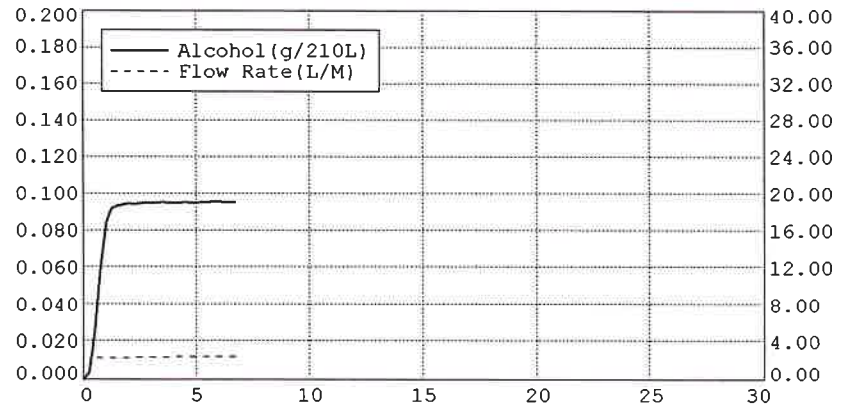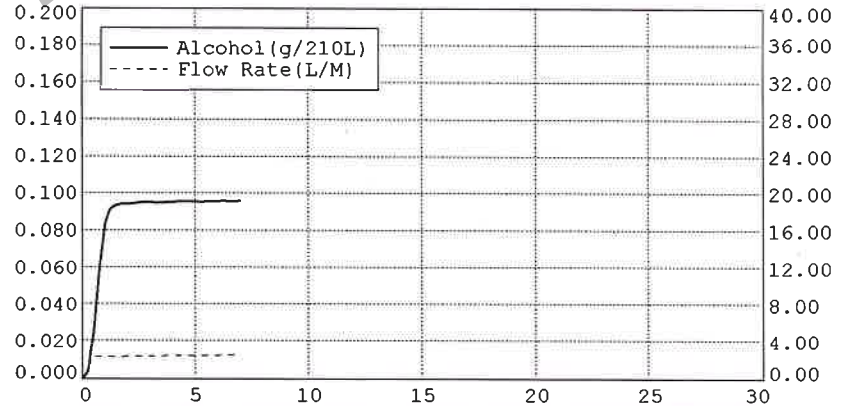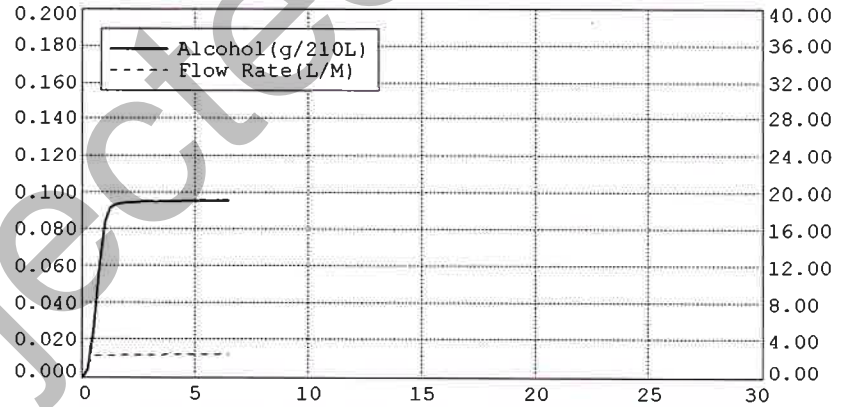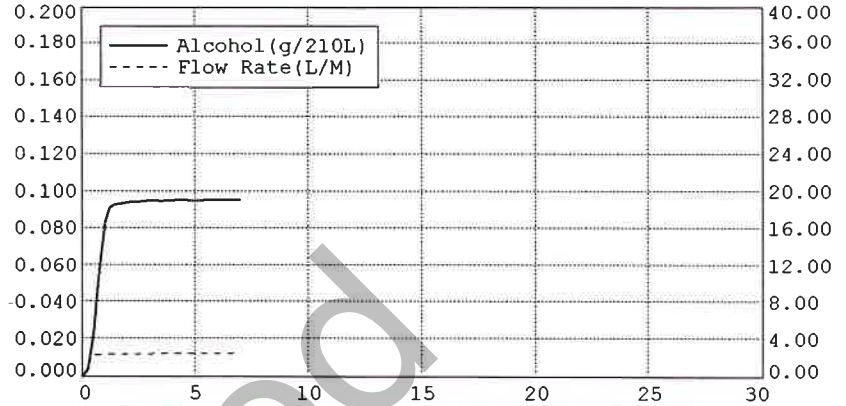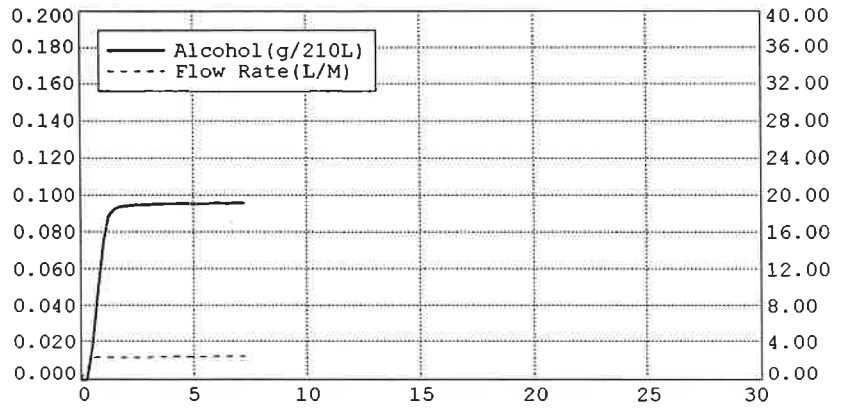

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100382






Date: 12/08/2025
Time: 13:32:10

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.28: 0.147
LOT #: AG515604
EXPIRATION: 06/05/2027
TANK PRESSURE: 673 psi

TEST TYPE	Value	Time
BLANK TEST	0.000	13:33
INTERNAL STANDARD	VERIFIED	13:33
EXTERNAL STANDARD	0.146	13:33
BLANK TEST	0.000	13:34
EXTERNAL STANDARD	0.146	13:34
BLANK TEST	0.000	13:35
EXTERNAL STANDARD	0.146	13:35
BLANK TEST	0.000	13:36
EXTERNAL STANDARD	0.145	13:37
BLANK TEST	0.000	13:37
EXTERNAL STANDARD	0.145	13:38
BLANK TEST	0.000	13:39

Average = 0.1456
Std Dev = 0.0005

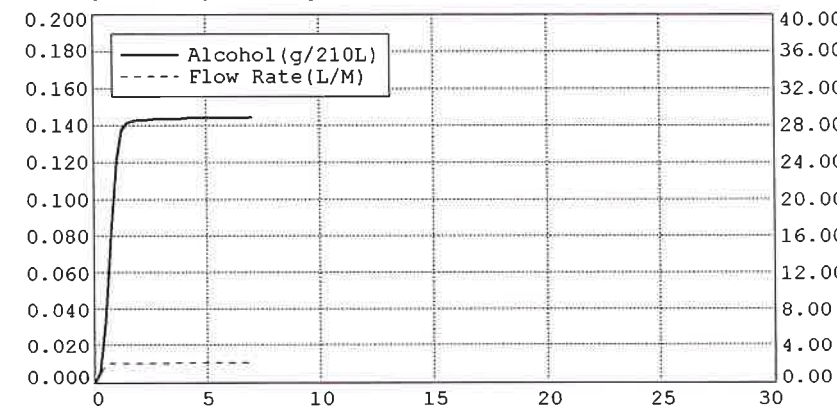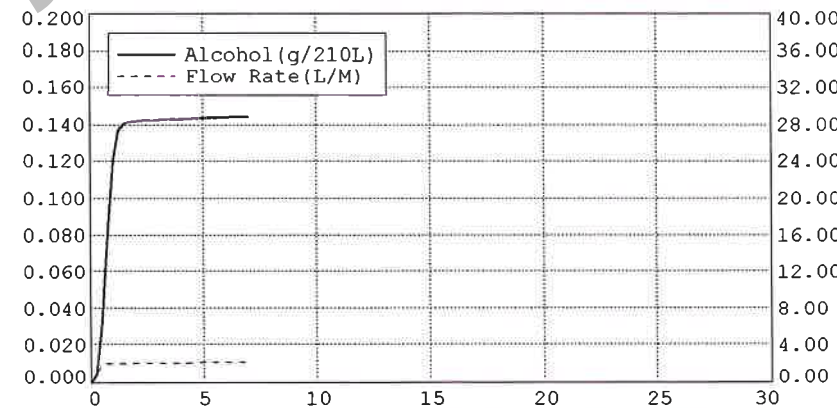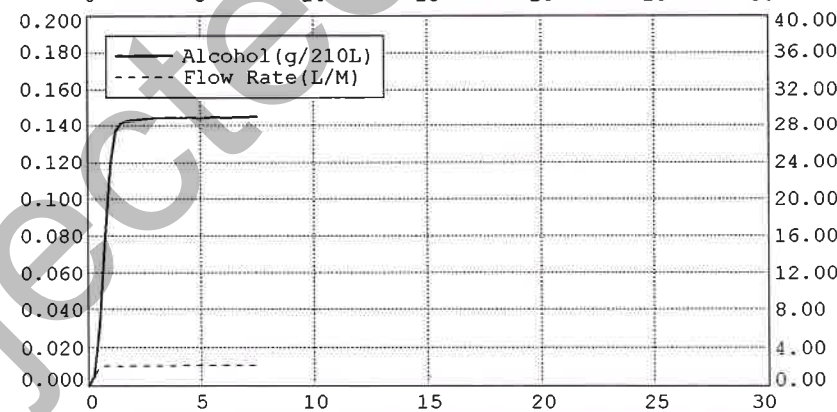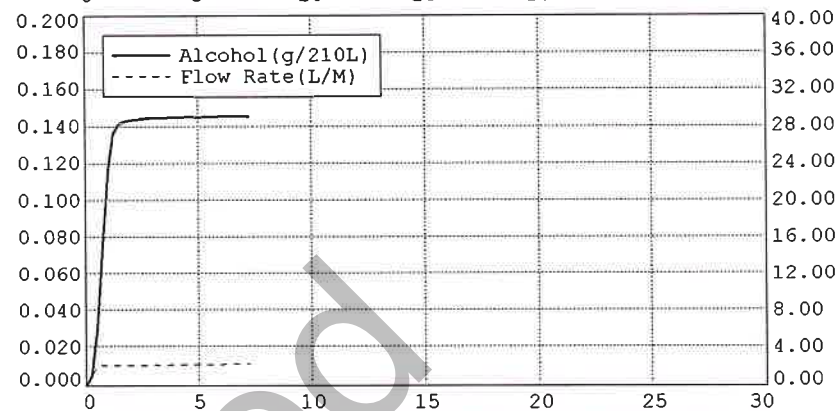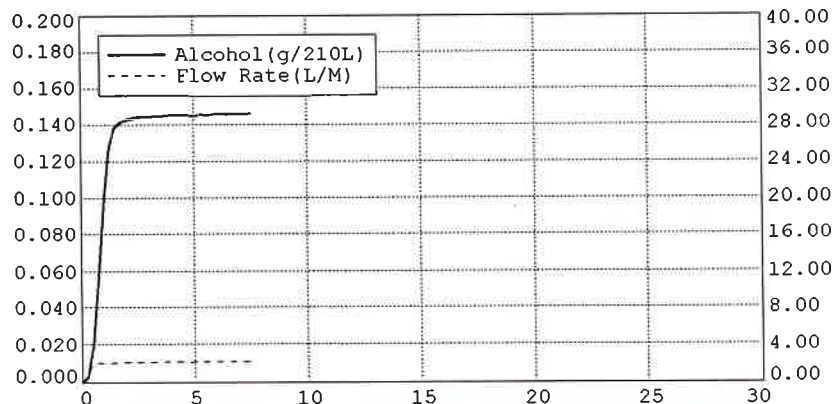

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100382






Date: 12/08/2025
Time: 13:39:35

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.27: 0.294
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 174 psi

BLANK TEST	0.000	13:40
INTERNAL STANDARD	VERIFIED	13:40
EXTERNAL STANDARD	0.292	13:41
BLANK TEST	0.000	13:42
EXTERNAL STANDARD	0.290	13:42
BLANK TEST	0.000	13:43
EXTERNAL STANDARD	0.291	13:43
BLANK TEST	0.000	13:44
EXTERNAL STANDARD	0.291	13:44
BLANK TEST	0.000	13:45
EXTERNAL STANDARD	0.291	13:45
BLANK TEST	0.000	13:46

Average = 0.2910
Std Dev = 0.0007

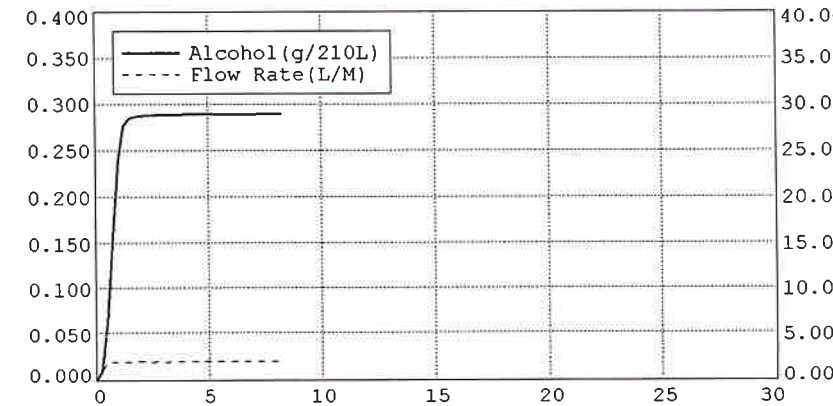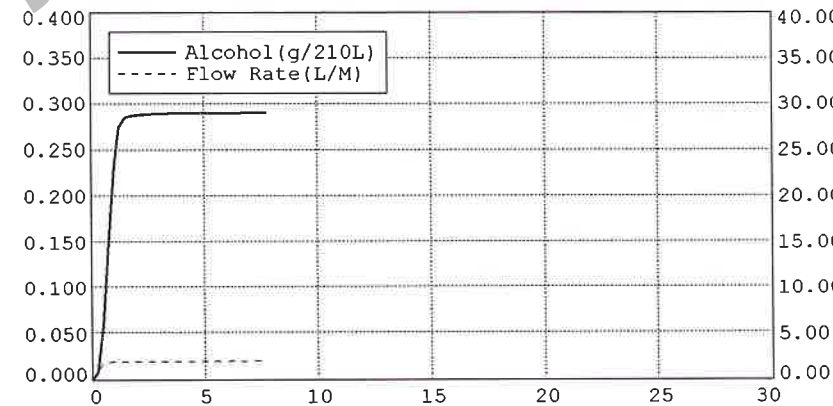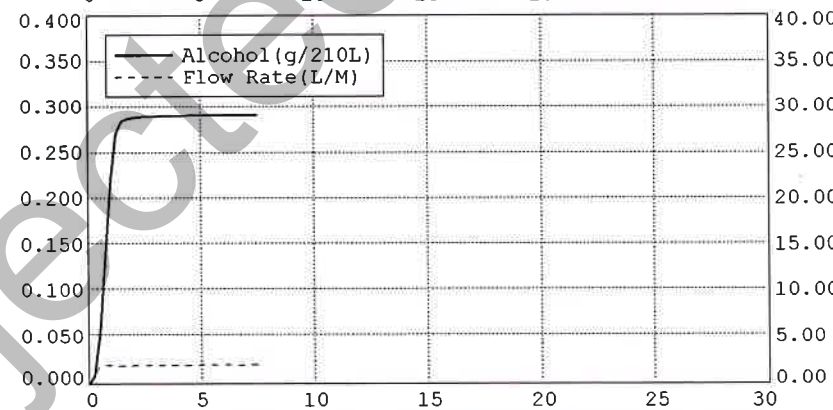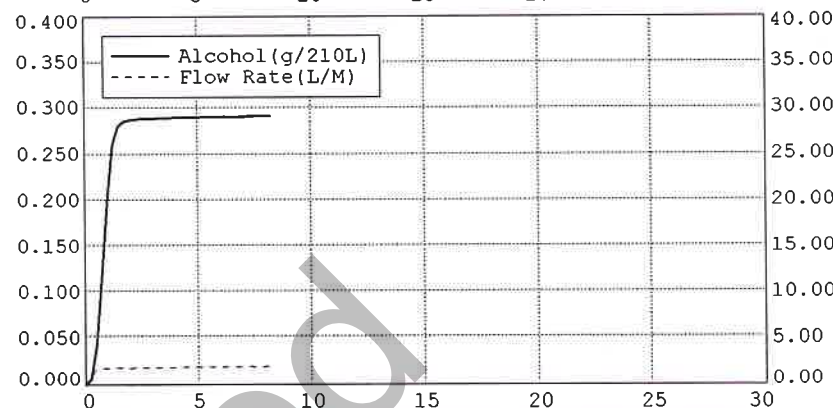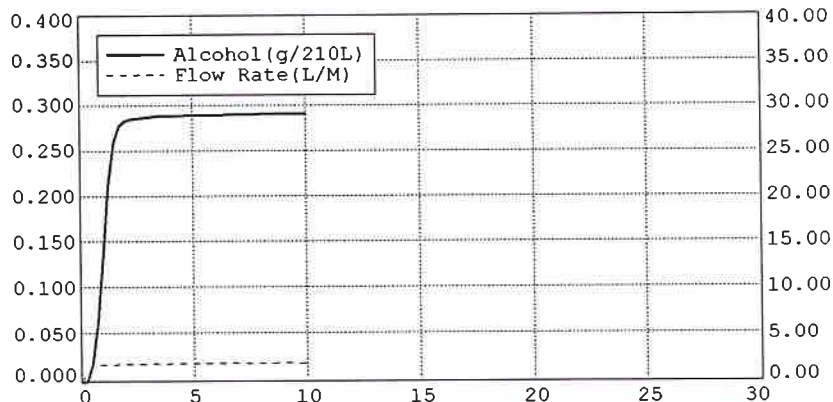

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100382

Date: 12/08/2025
Time: 13:52:14

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:54
BLANK TEST	0.000	13:54
INTERNAL STANDARD	VERIFIED	13:54
EXTERNAL STANDARD	0.079	13:54
BLANK TEST	0.000	13:55
SUBJECT SAMPLE	INCOMPLETE	13:57

CMS

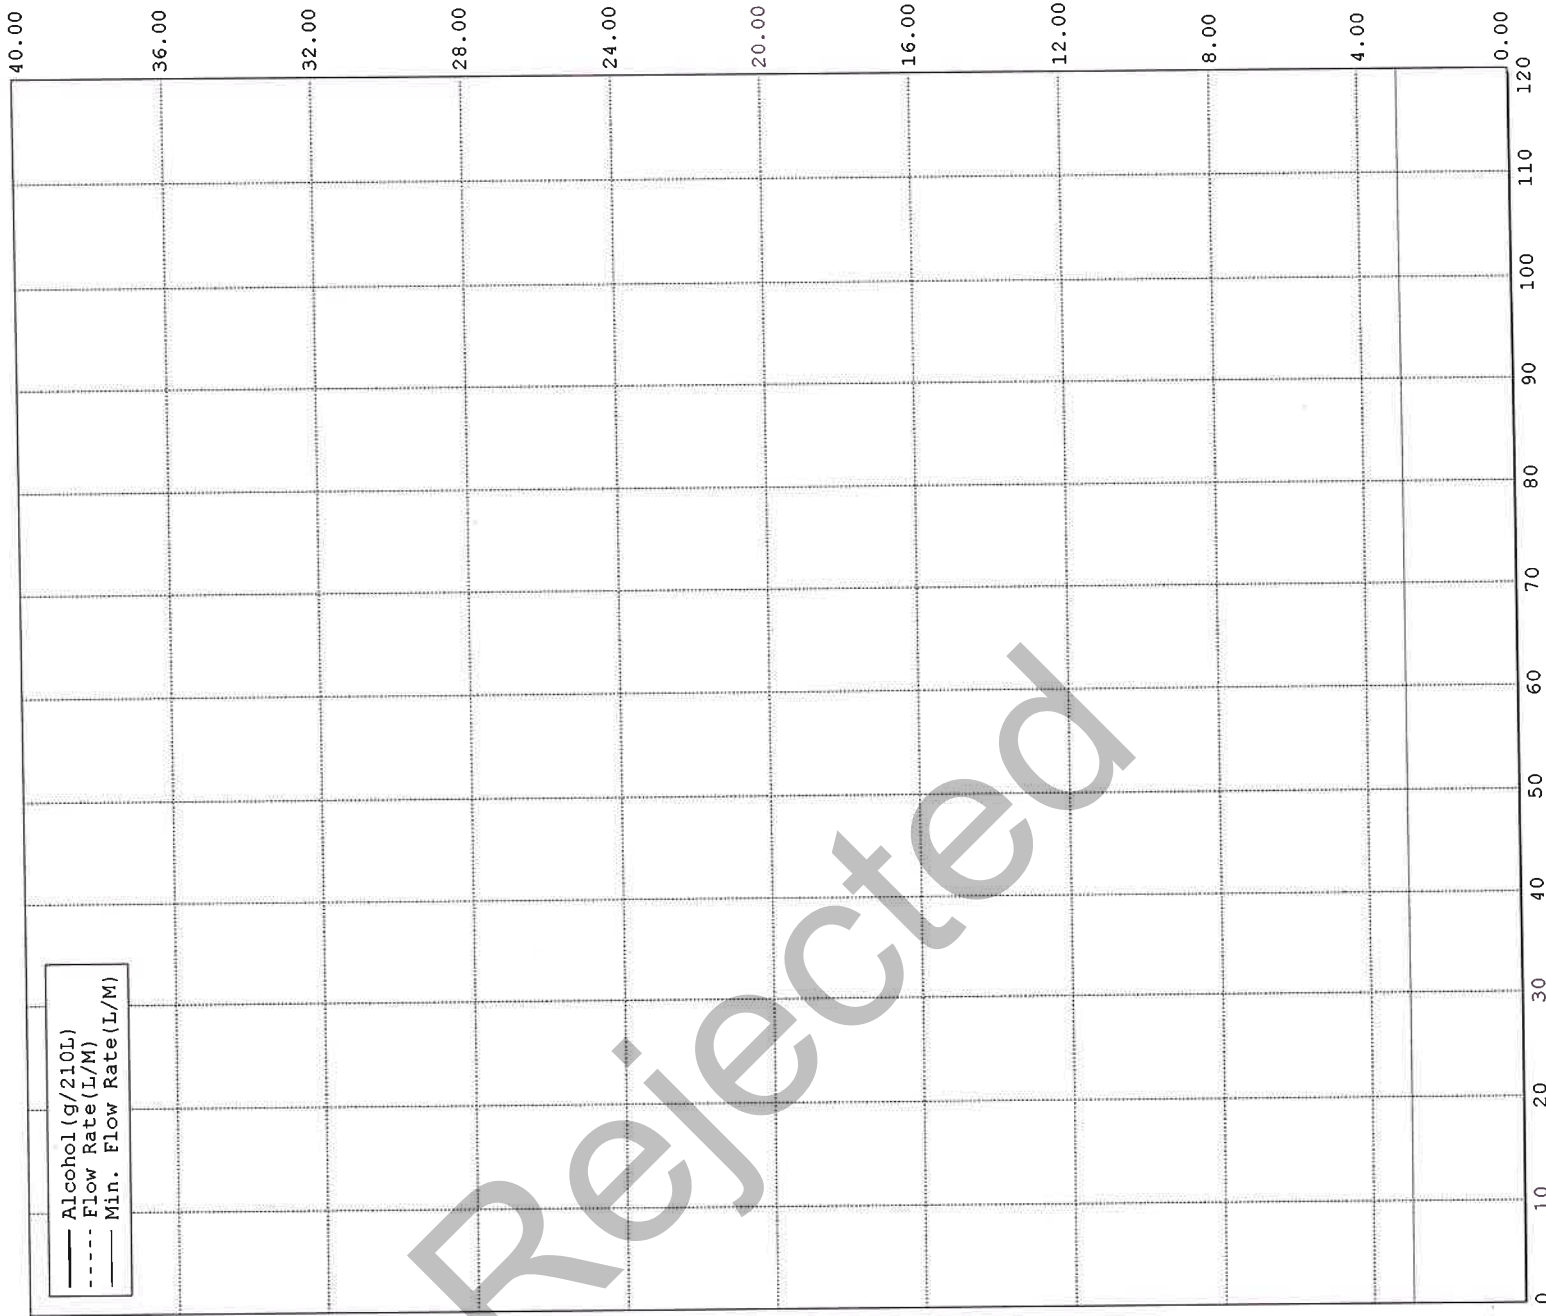

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100382

Date: 12/08/2025
Time: 13:59:09

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
MAX ATTEMPTS EXCEEDED
CASE/REPORT: XXXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:00
BLANK TEST	0.000	14:00
INTERNAL STANDARD	VERIFIED	14:00
EXTERNAL STANDARD	0.078	14:00
BLANK TEST	0.000	14:01
SUBJECT SAMPLE	XXX	14:02

Maximum Attempts Exceeded

OK

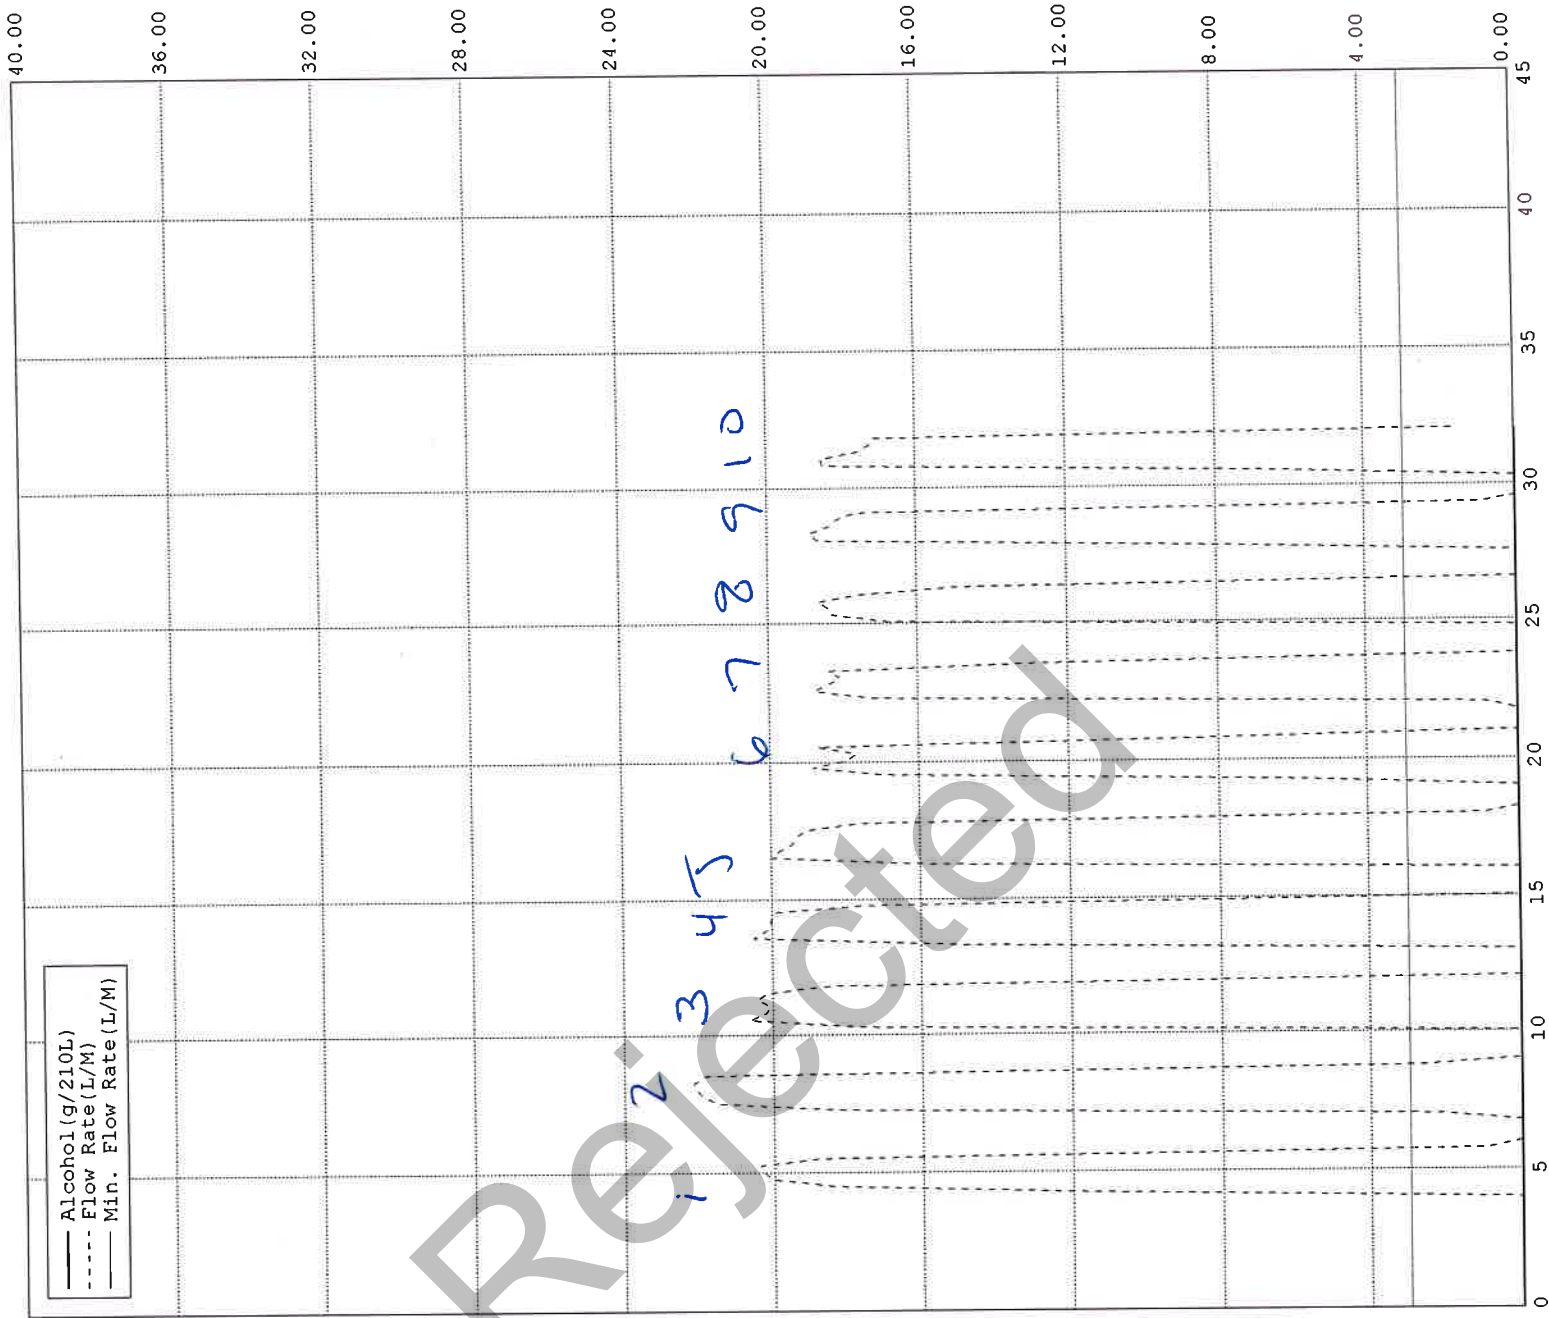

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100382

Date: 12/08/2025
Time: 14:04:14

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INVALID
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:05
BLANK TEST	0.000	14:05
INTERNAL STANDARD	VERIFIED	14:05
EXTERNAL STANDARD	0.079	14:05
BLANK TEST	0.000	14:06
SUBJECT SAMPLE	INVALID	14:07

[Handwritten signature]

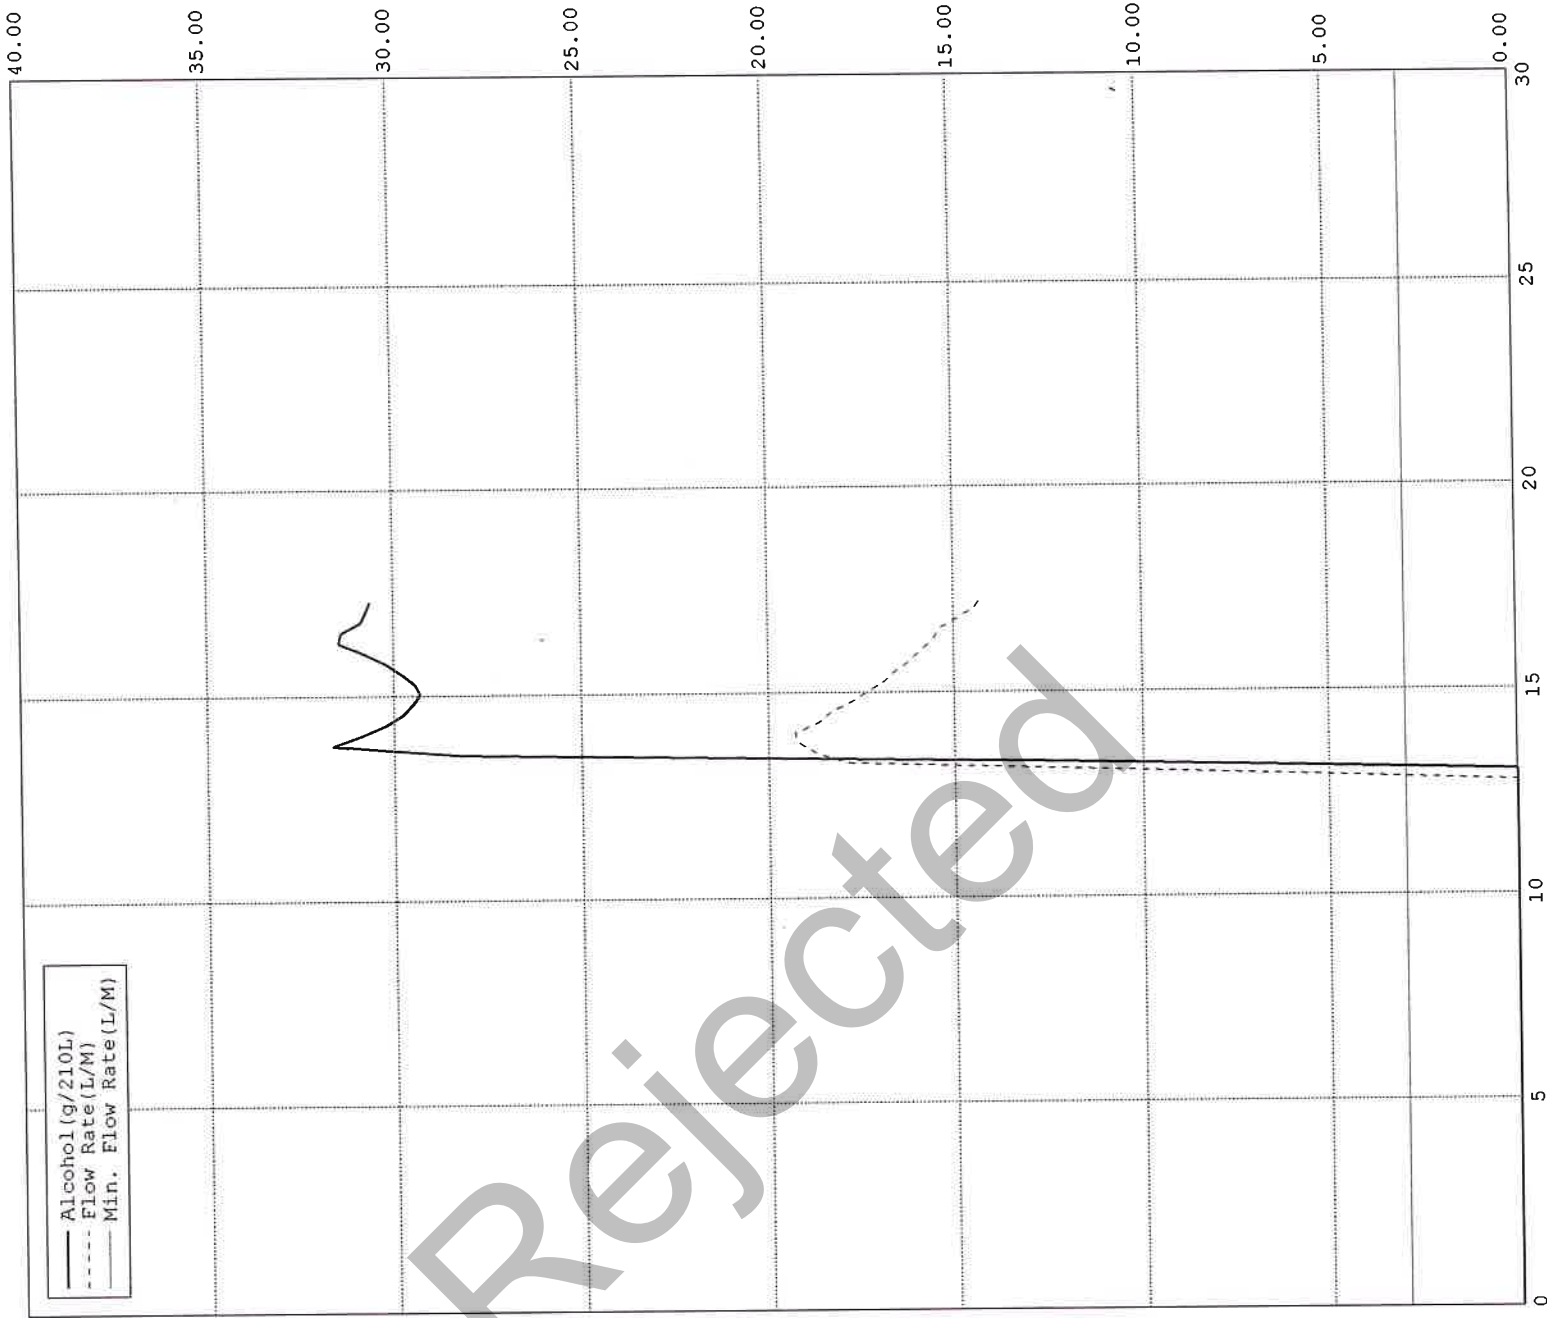

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100382

Date: 12/08/2025
Time: 14:09:34

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

RFI

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.27: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

PASSED 14:11

0.000 14:11


VERIFIED 14:11

0.077 14:12

0.000 14:13

RFI DETECTED

CMC

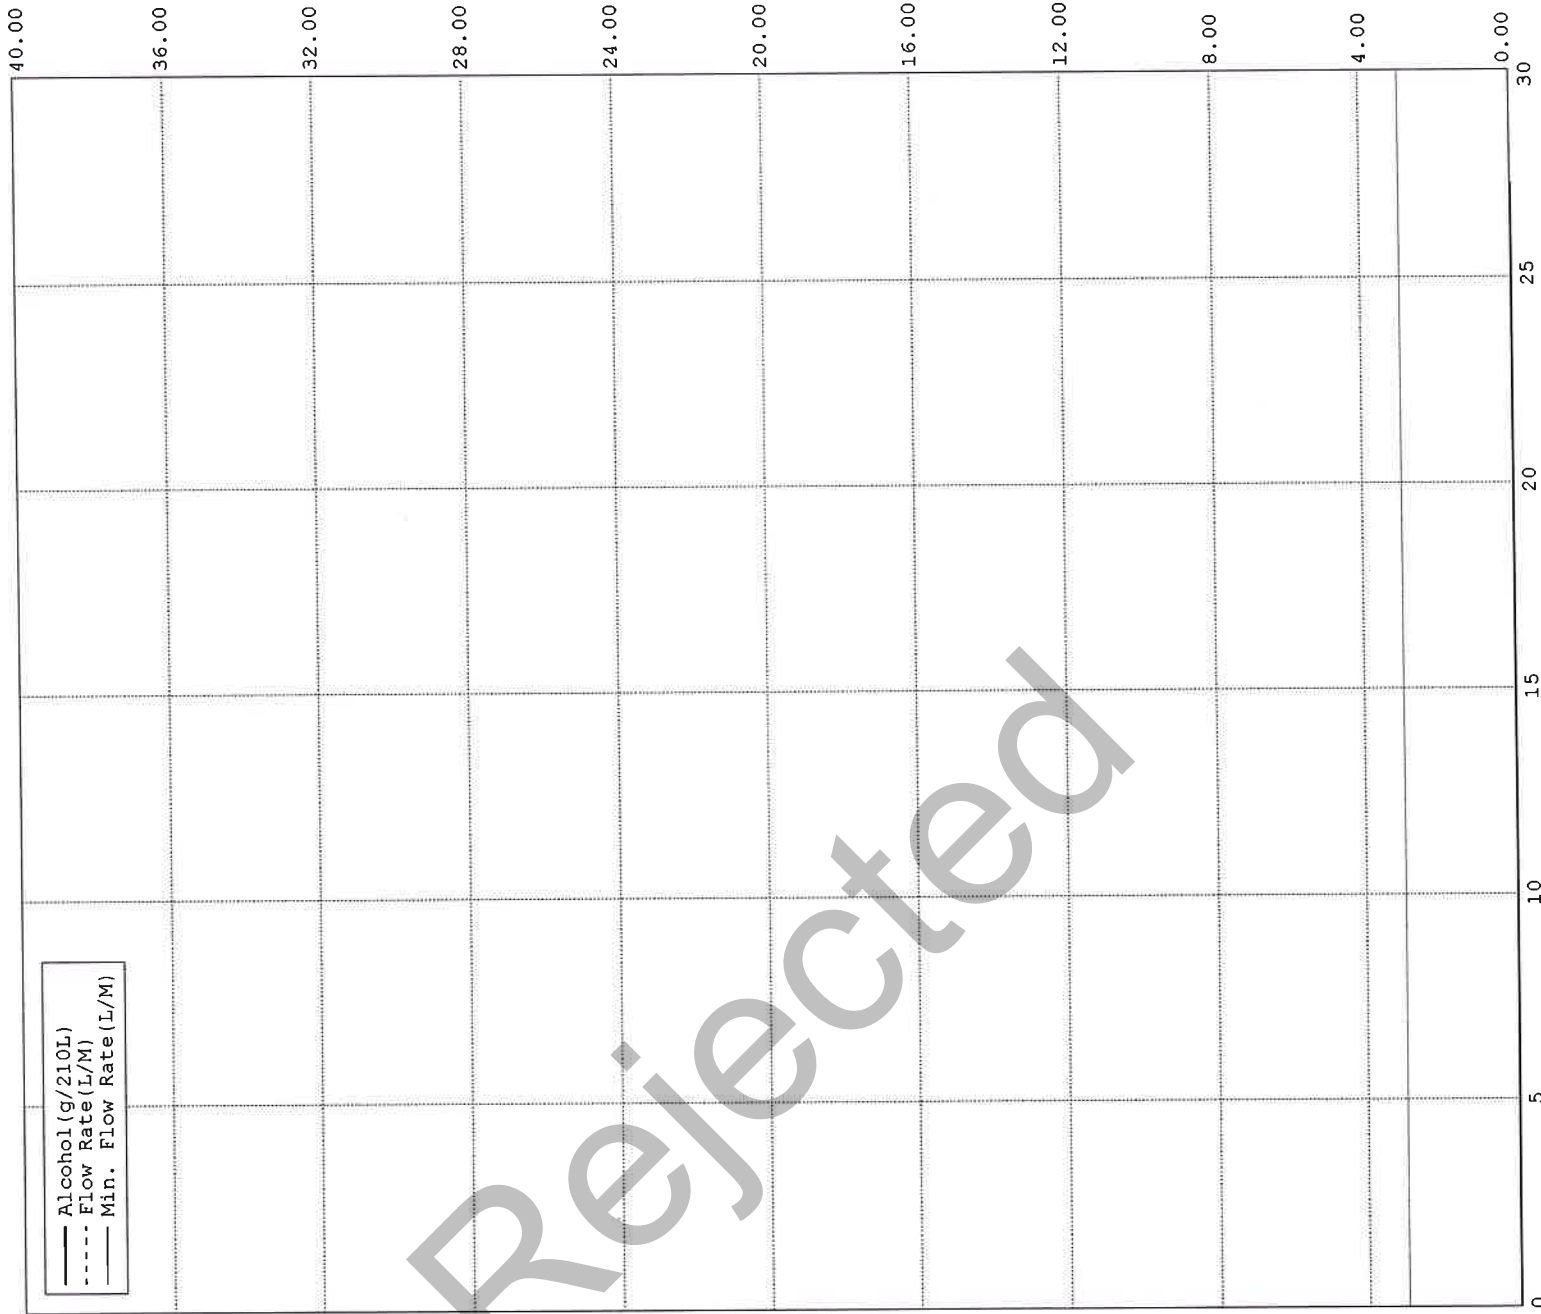

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100382

Date: 12/08/2025
Time: 14:17:22

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
INTERFERENCE - ACETONE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:18
BLANK TEST	0.000	14:18
INTERNAL STANDARD	VERIFIED	14:18
EXTERNAL STANDARD	0.078	14:18
BLANK TEST	0.000	14:19
SUBJECT SAMPLE	XXX	14:20

Interference Detected

QW

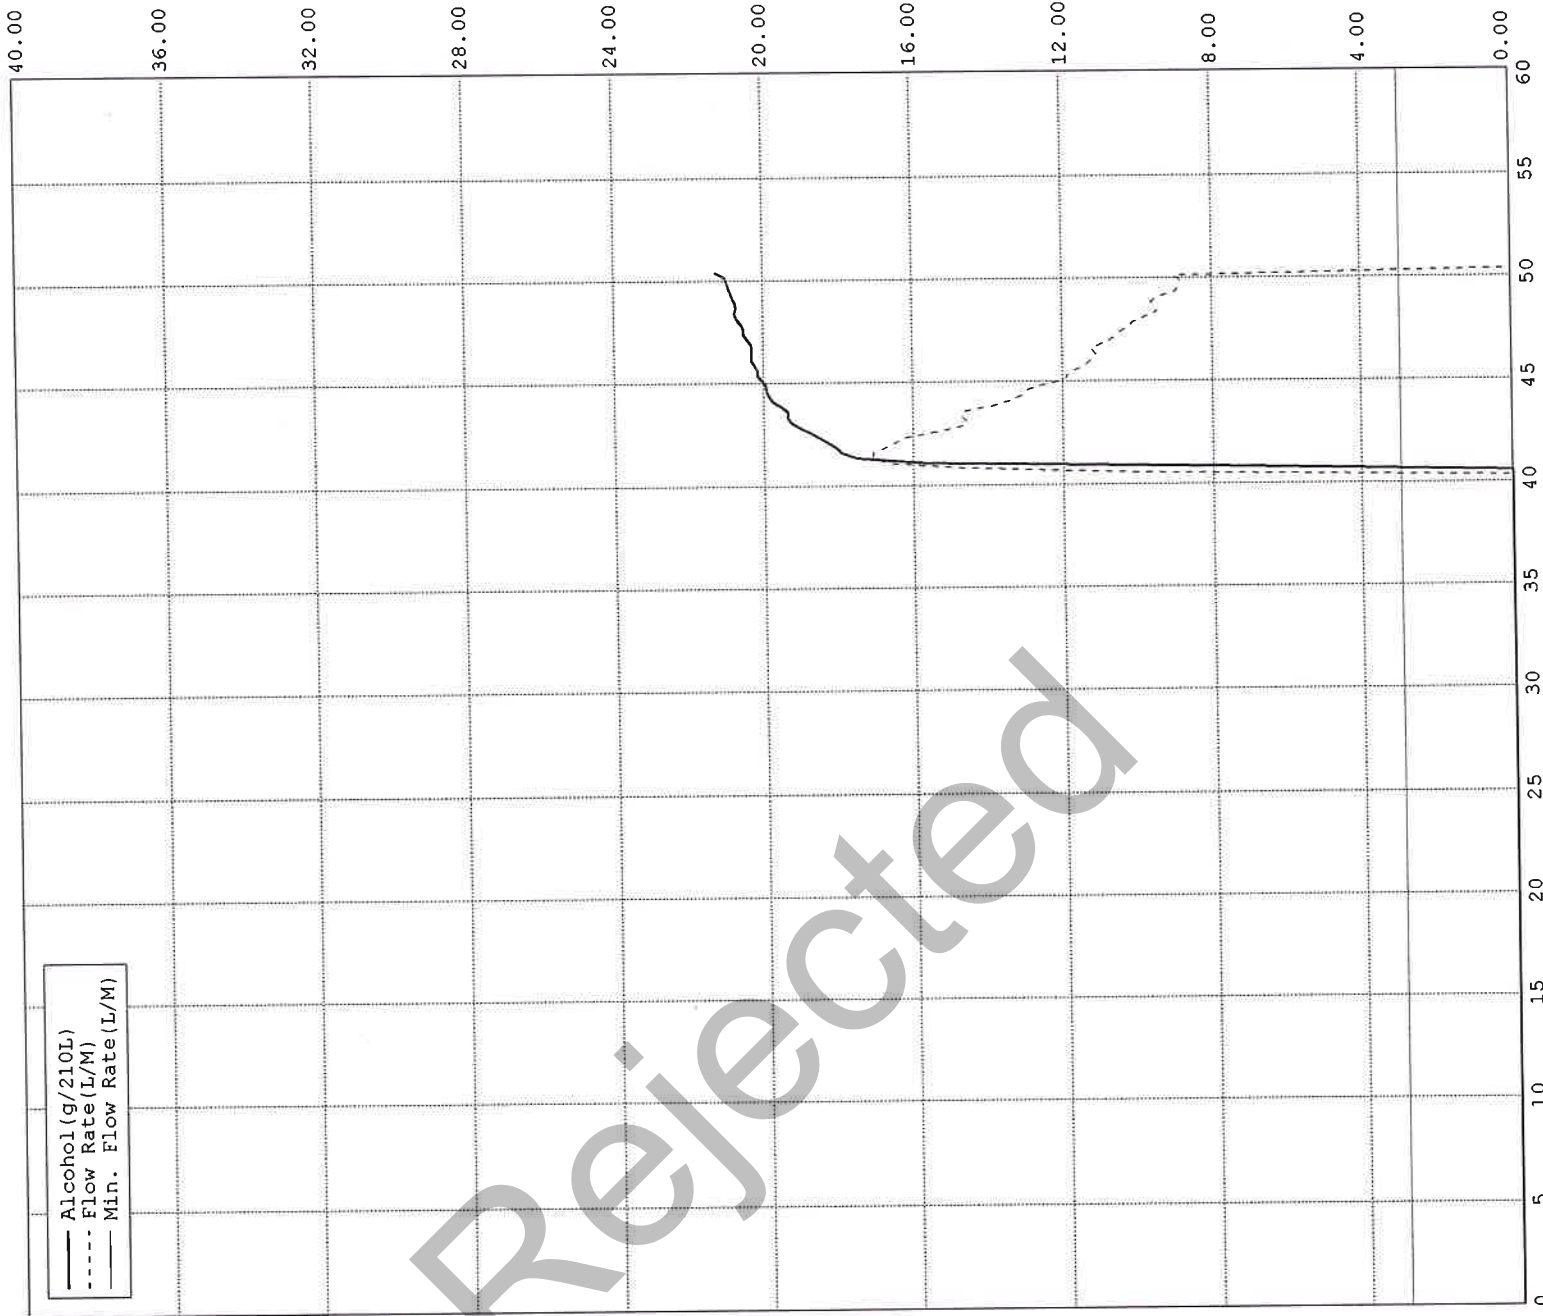

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100382

Date: 12/08/2025
Time: 14:23:19

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE - IPA
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:25
BLANK TEST	0.000	14:25
INTERNAL STANDARD	VERIFIED	14:25
EXTERNAL STANDARD	0.078	14:25
BLANK TEST	0.000	14:26

Static Analysis Error

Static analysis error
observed. Interference-
IPA test restarted
CWB- 12/18/25

CWB

2 sample attempts administered
using 2000 mL. 1st did not accept,
2nd did - then static analysis error.
CWB- 12/18/25

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100382

Date: 12/08/2025
Time: 14:29:41

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE - IPA
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:30
BLANK TEST	0.000	14:31
INTERNAL STANDARD	VERIFIED	14:31
EXTERNAL STANDARD	0.078	14:31
BLANK TEST	0.000	14:32

Static Analysis Error

4 sample attempts administered
using 2000 ml. First 3 did not accept,
4th did - then static analysis error.
DW-1218125.

CMS