




State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100695

Report Issue Date: 03/12/2026
Date Received: 2025-12-23
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.021	0.020	0.021	0.020	0.021	0.021
0.080	0.080	AG436502	0.080	0.081	0.080	0.080	0.081	0.080
0.300	0.301	AG427706	0.300	0.301	0.301	0.301	0.301	0.301

As Found - Evaluation Analyst: Carlie Glaister

As Found Conditions - Barometric Pressure (inHg): 30.00 Barometer Used: VWR S/N 240680771 Temperature (C): 21.7 Relative Humidity (%): 0

As-Found Lab Activity Date Range: 12/23/2025 - 12/23/2025

Tank interference detected on first VOC. 2nd VOC passed.

Barometer is not displaying humidity as this time, unable to record this condition. During linearity the humidity readout on the barometer changed to 0%, this value used.

Some recent tests from the field were reviewed. IS generally around 2.5% for completed tested and ~4-5% for failed tests due to IS error. IS observed to be equal to or less than 1% during eval. Adjustment is being recommended anyways due to recent status messages from the field.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.021	0.020	0.021	0.021	0.021	0.021	+/- 0.002
0.040	0.040	AG407908	0.040	0.039	0.040	0.040	0.039	0.040	+/- 0.003
0.080	0.079	AG436502	0.079	0.078	0.079	0.079	0.079	0.079	+/- 0.004
0.100	0.099	AG516101	0.098	0.098	0.098	0.098	0.098	0.098	+/- 0.004
0.150	0.149	AG515604	0.147	0.147	0.147	0.147	0.146	0.147	+/- 0.006
0.300	0.297	AG516110	0.292	0.292	0.293	0.293	0.293	0.293	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.64 Barometer Used: VWR S/N 240680771 Temperature (C): 22.0 Relative Humidity (%): 1

As-Left Lab Activity Date Range: 03/09/2026 - 03/09/2026

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.


The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.



State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Serial Number: 100695

Results authorized by Carlie Glaister on 03/09/2026

carlie.glaister@alaska.gov

Technically and administratively reviewed by Colleen O'Bryant on 03/12/2026

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100695 Analyst or Technician Name: Carlie Glauster

DataMaster DMT Calibration Start Date: 3/9/26

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 9/10/2026
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.64 Temperature(C) 22.0 Relative Humidity(%) 1
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

- Acetone Reagent Lot Number: 20260218008 Expiration Date: 5/18/26/3/19/27
Simulator S/N: SD1088 Thermometer Verification Performed?
- Isopropanol Reagent Lot Number: 20260218008 Expiration Date: 5/18/26/3/19/27
Simulator S/N: SD1199 Thermometer Verification Performed?
- Negative (Ethanol Only) Lot Number: 25CP41280 Expiration Date: 3/19/27 (5/18/26 prep)
Simulator S/N: SD1177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 250159297
Calibration Due Date: 5/14/27 06-3/9/26

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 3/9/26
Data Interpretation Date (Technician): 3/9/26 06-3/9/26 (if applicable)
Data Interpretation Date (Analyst): NA

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 03/09/2026
Time: 11:18:11

VERSIONS

DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 45.4°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.79 V PASSED
(1.07 V - 2.51 V)
Cooler Voltage = 1.85 V PASSED
(1.11 V - 2.59 V)
Bias Voltage = 78 V PASSED
(47 V - 109 V)
Chopper Freq = 548 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.6 in

PUMP INFO

Flow Rate = 4.272 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.003 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.115 1.29% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100695

Date: 03/09/2026
Time: 11:22 AM

Temperatures (°C)

Sample Cell: 48.7°C
Breath Tube: 46.0°C

Current Barometer 29.6 in
Volume (Ltr) 1.56

Settings

Lamp: 1.84 V
Bias: 78 V
Cooler: 1.85 V
Chopper: 547 Hz

Voltages (V)

Flow: 1.04 V
Detector: -0.097 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 01/08/2026
Time: 15:24:30

OPERATOR NAME:
DEREK WALTON
CERTIFICATE #: 9508

Ca = 0.1000
CAL = 0.980687 0.800 <= CAL < 1.200
b1 = 0.0005 0.0000 <= b1 < 0.0040
b2 = 0.0058 0.0010 <= b2 < 0.0100
b3 = 0.0003 0.0000 <= b3 < 0.0040
Xq = 0.1161 0.0500 <= Xq < 0.2000
a21 = 1.148788 1.050 <= a21 < 1.300
a31 = 0.535871 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 03/09/2026
Time: 11:25:26


SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.64: 0.079
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	11:27
BLANK TEST	0.000	11:28
INTERNAL STANDARD	VERIFIED	11:28
EXTERNAL STANDARD	0.079	11:28
BLANK TEST	0.000	11:29
SUBJECT SAMPLE (Vol=1.58L)	0.000	11:30
BLANK TEST	0.000	11:31
EXTERNAL STANDARD	0.079	11:31
BLANK TEST	0.000	11:32

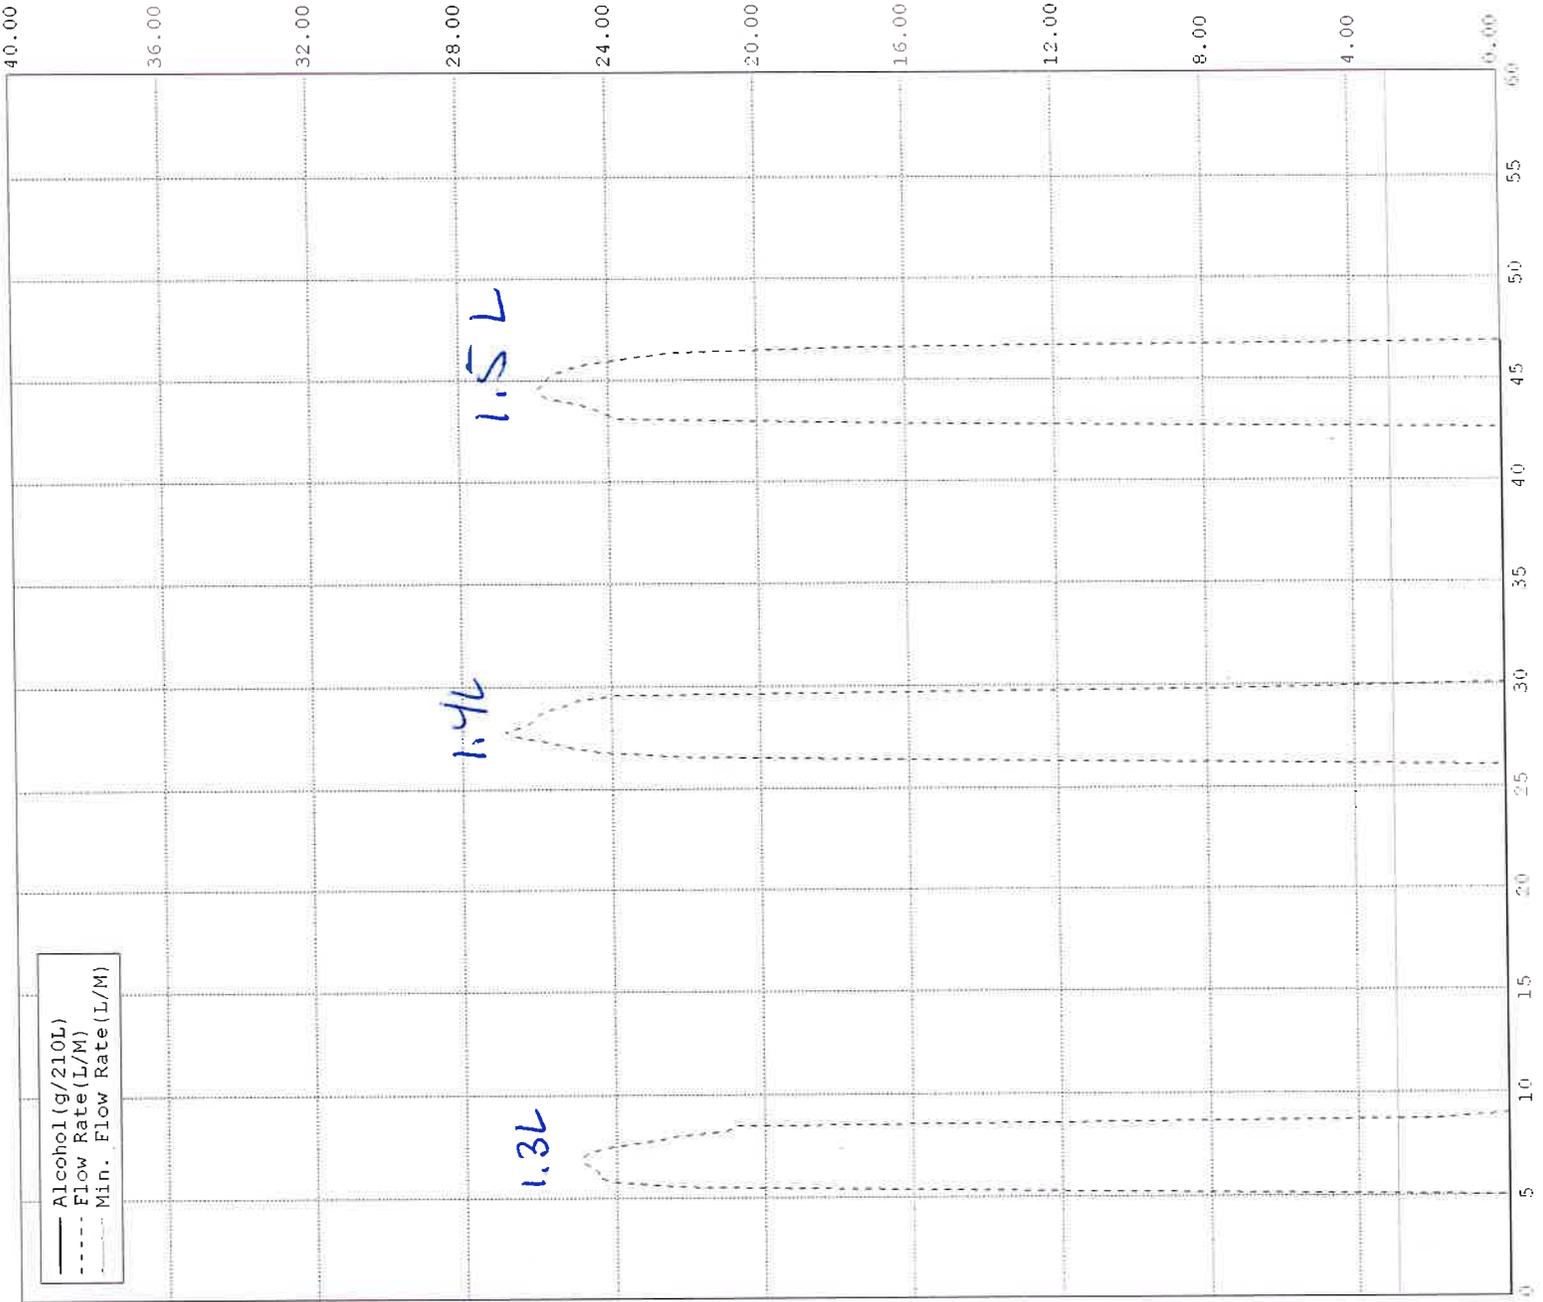

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100695

Date: 03/09/2026
 Time: 11:39:59

SUPERVISOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.020	0.0208	0.0004
0.040	0.0396	0.0005
0.079	0.0788	0.0004
0.099	0.0980	0.0000
0.149	0.1468	0.0004
0.297	0.2926	0.0005

SLOPE = 0.982055
 R² = 0.999986

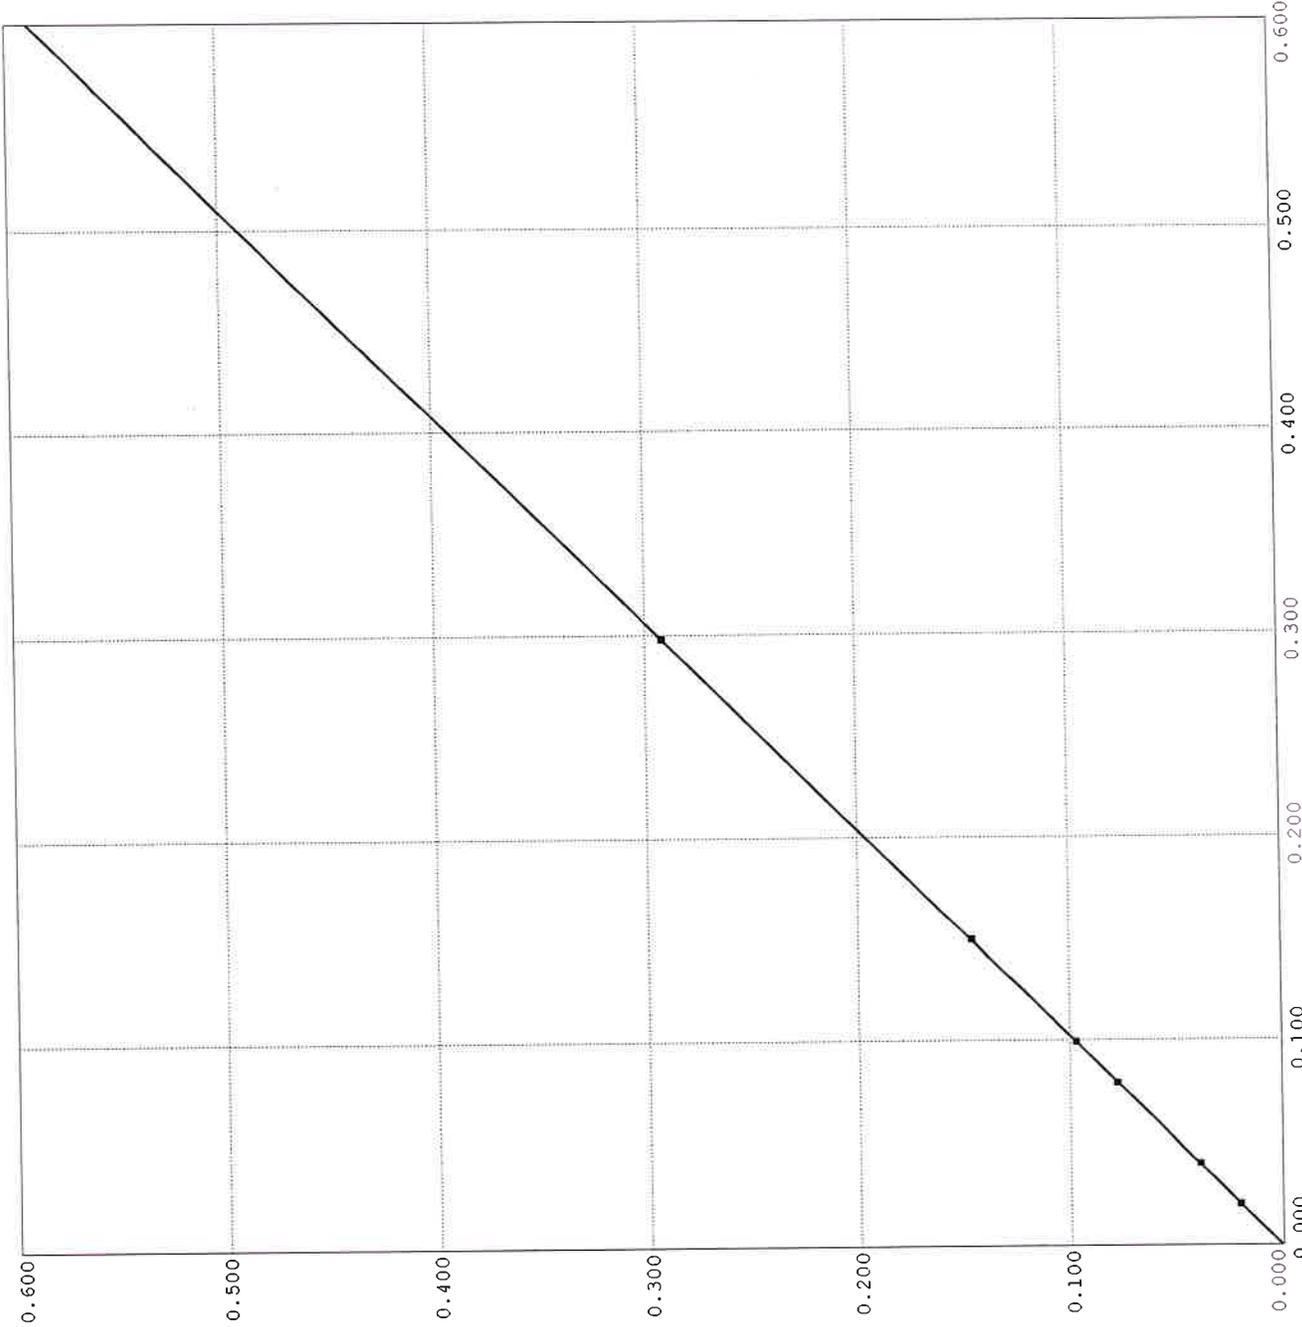

Handwritten signature

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100695






Date: 03/09/2026
Time: 11:40:01

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.64: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 554 psi

BLANK TEST	0.000	11:41
INTERNAL STANDARD	VERIFIED	11:41
EXTERNAL STANDARD	0.021	11:41
BLANK TEST	0.000	11:42
EXTERNAL STANDARD	0.020	11:42
BLANK TEST	0.000	11:43
EXTERNAL STANDARD	0.021	11:43
BLANK TEST	0.000	11:44
EXTERNAL STANDARD	0.021	11:44
BLANK TEST	0.000	11:45
EXTERNAL STANDARD	0.021	11:45
BLANK TEST	0.000	11:46

Average = 0.0208
Std Dev = 0.0004

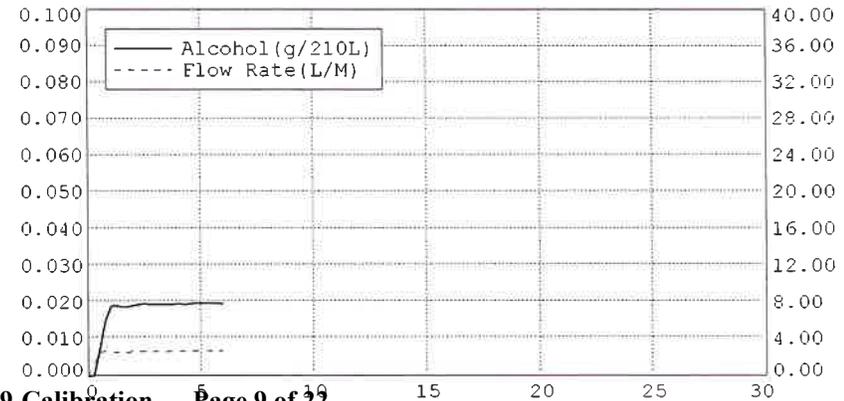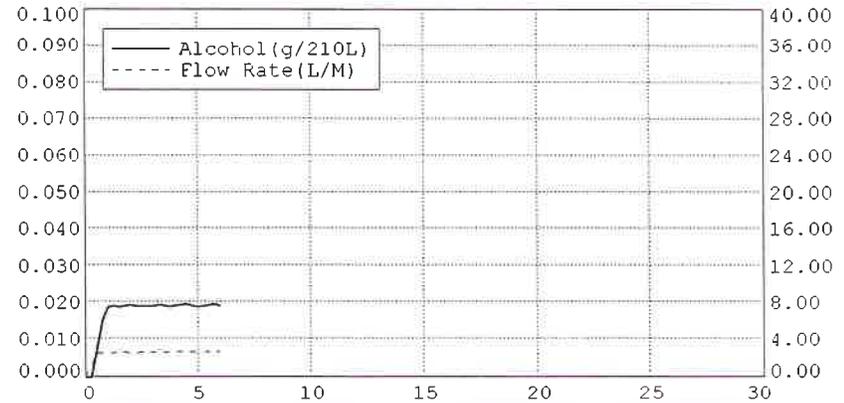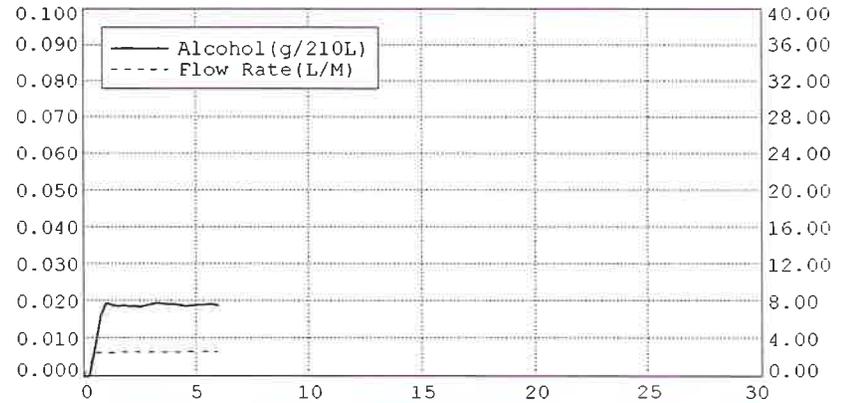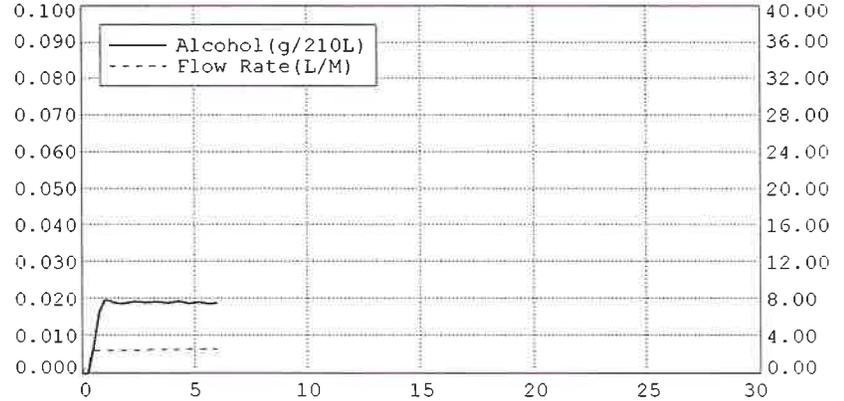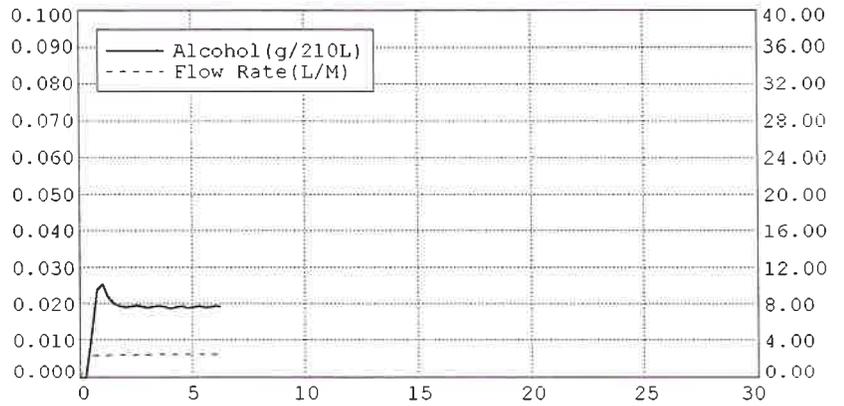

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100695






Date: 03/09/2026
 Time: 11:49:05

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 29.64: 0.040
 LOT #: AG407908
 EXPIRATION: 03/19/2026
 TANK PRESSURE: 996 psi

BLANK TEST	0.000	11:50
INTERNAL STANDARD	VERIFIED	11:50
EXTERNAL STANDARD	0.040	11:50
BLANK TEST	0.000	11:51
EXTERNAL STANDARD	0.039	11:51
BLANK TEST	0.000	11:52
EXTERNAL STANDARD	0.040	11:52
BLANK TEST	0.000	11:53
EXTERNAL STANDARD	0.040	11:53
BLANK TEST	0.000	11:54
EXTERNAL STANDARD	0.039	11:55
BLANK TEST	0.000	11:55

Average = 0.0396
 Std Dev = 0.0005

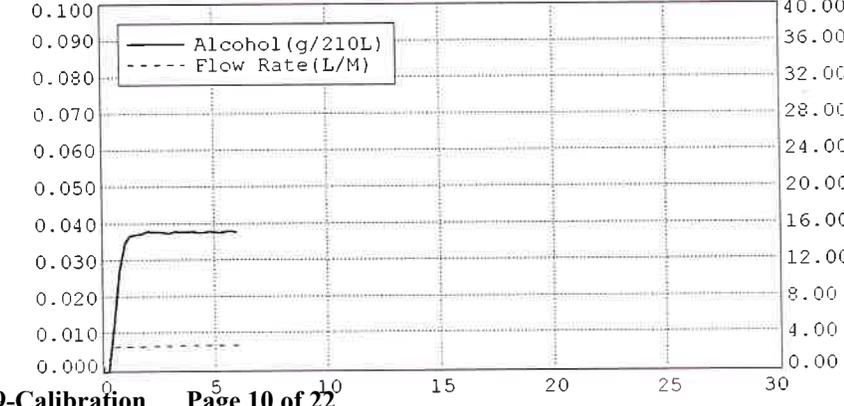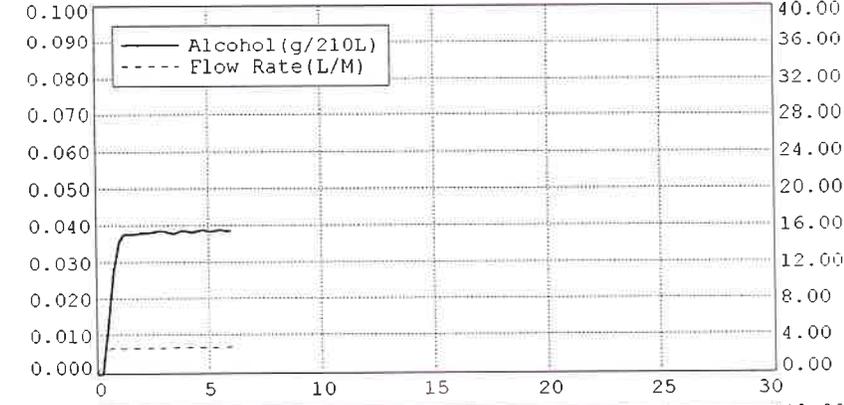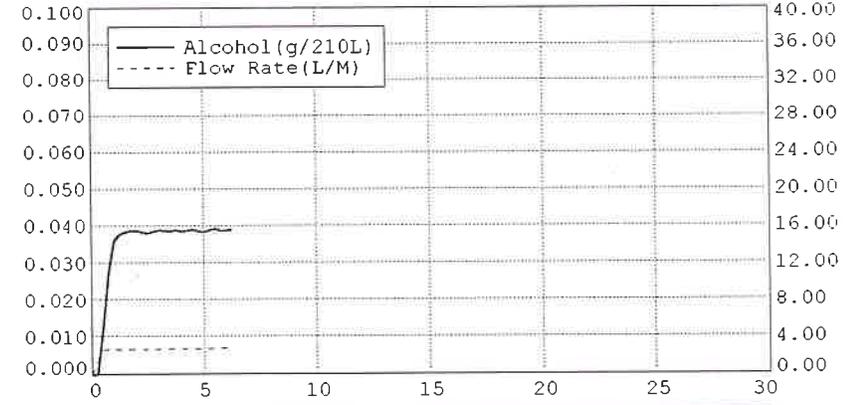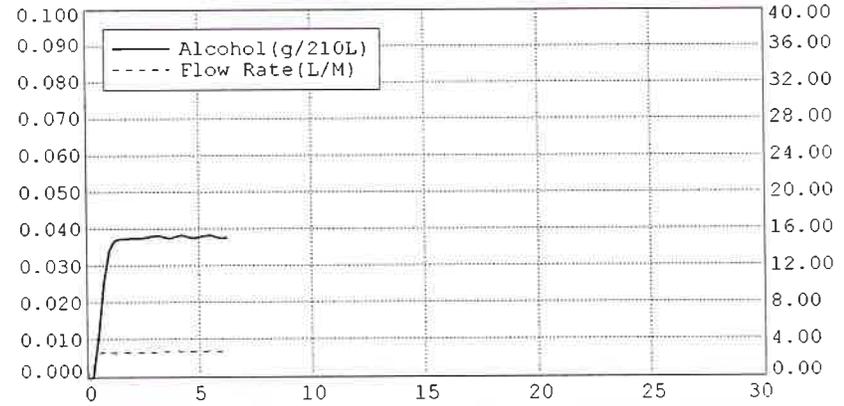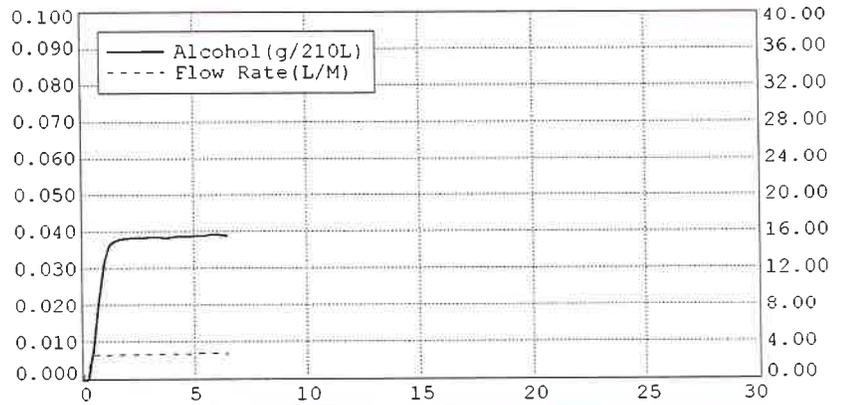

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100695






Date: 03/09/2026
 Time: 11:59:07

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.64: 0.079
 LOT #: AG436502
 EXPIRATION: 12/30/2026
 TANK PRESSURE: 813 psi

BLANK TEST	0.000	12:00
INTERNAL STANDARD	VERIFIED	12:00
EXTERNAL STANDARD	0.079	12:00
BLANK TEST	0.000	12:01
EXTERNAL STANDARD	0.078	12:01
BLANK TEST	0.000	12:02
EXTERNAL STANDARD	0.079	12:02
BLANK TEST	0.000	12:03
EXTERNAL STANDARD	0.079	12:04
BLANK TEST	0.000	12:04
EXTERNAL STANDARD	0.079	12:05
BLANK TEST	0.000	12:06

Average = 0.0788
 Std Dev = 0.0004

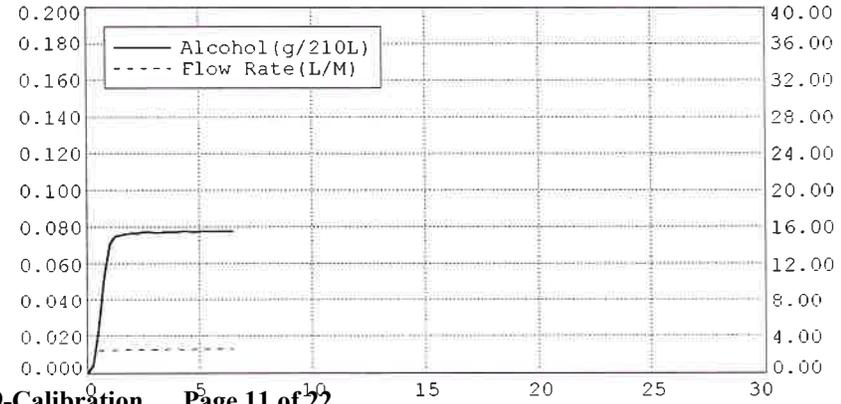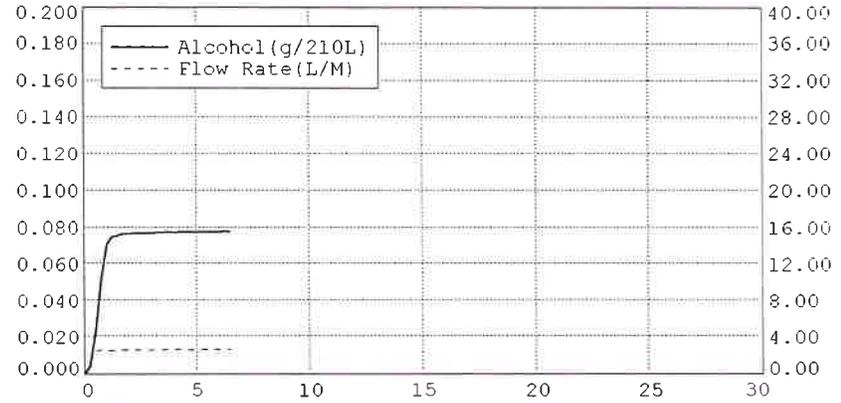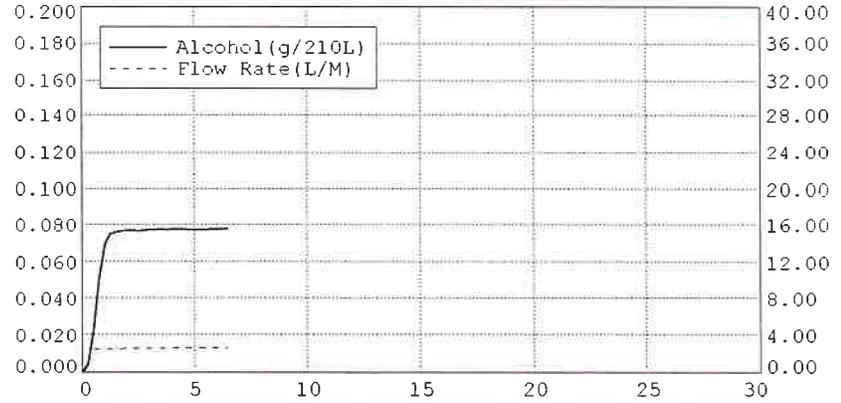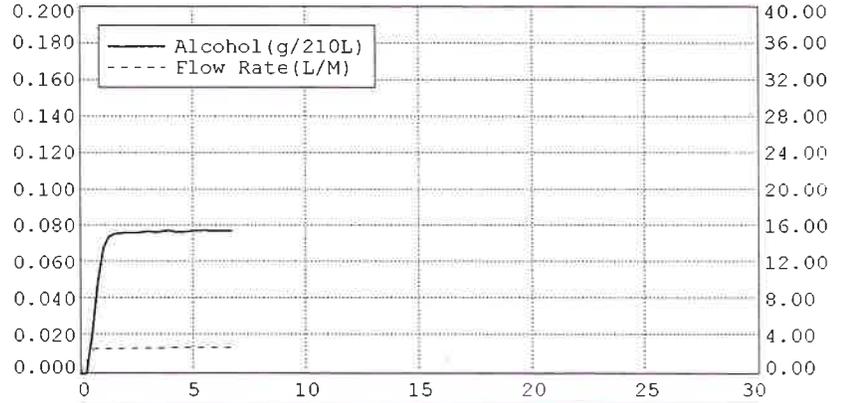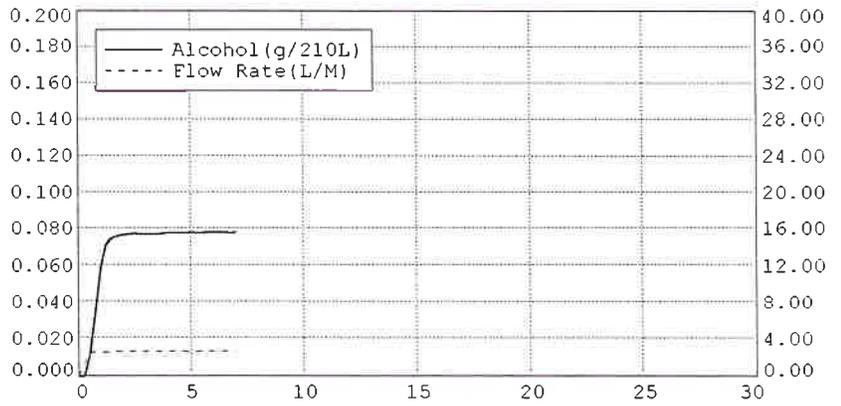

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100695






Date: 03/09/2026
 Time: 12:09:42

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.64: 0.099
 LOT #: AG516101
 EXPIRATION: 06/10/2027
 TANK PRESSURE: 931 psi

BLANK TEST	0.000	12:10
INTERNAL STANDARD	VERIFIED	12:10
EXTERNAL STANDARD	0.098	12:11
BLANK TEST	0.000	12:12
EXTERNAL STANDARD	0.098	12:12
BLANK TEST	0.000	12:13
EXTERNAL STANDARD	0.098	12:13
BLANK TEST	0.000	12:14
EXTERNAL STANDARD	0.098	12:14
BLANK TEST	0.000	12:15
EXTERNAL STANDARD	0.098	12:15
BLANK TEST	0.000	12:16

Average = 0.0980
 Std Dev = 0.0000

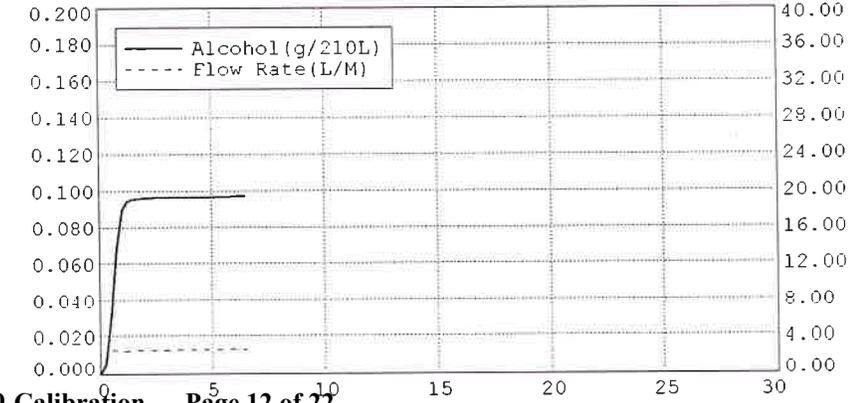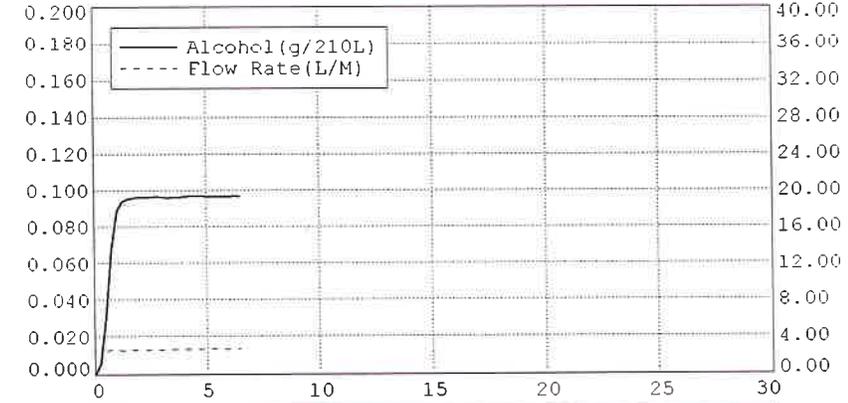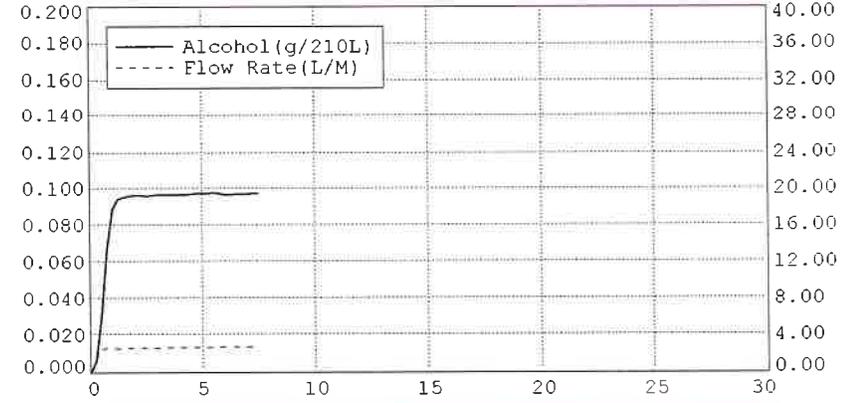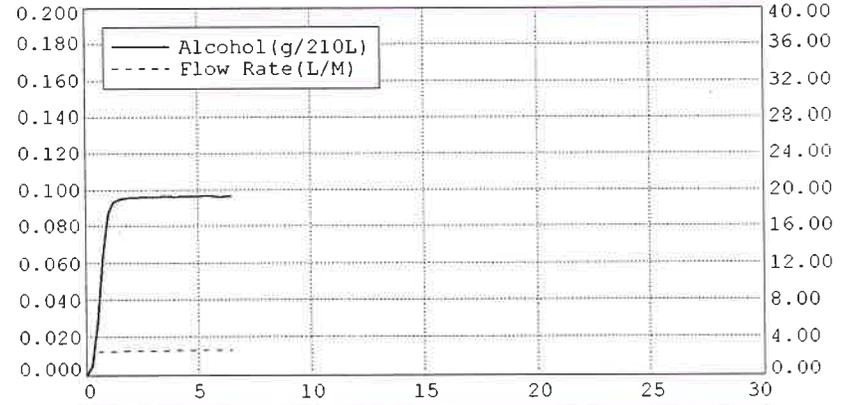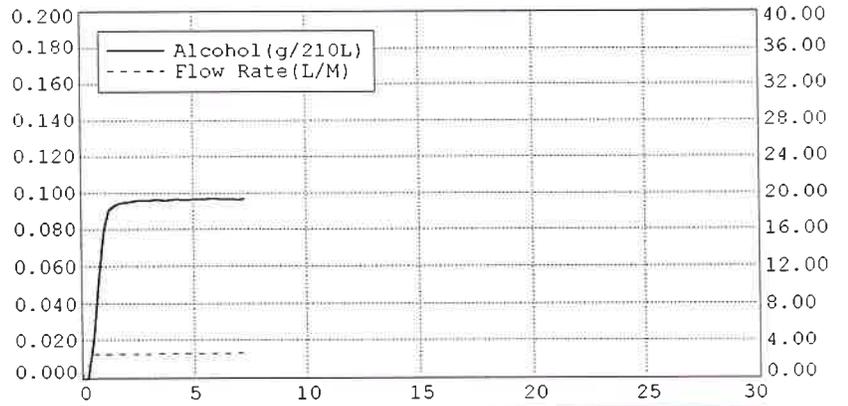

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100695






Date: 03/09/2026
 Time: 12:17:34

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 29.64: 0.149
 LOT #: AG515604
 EXPIRATION: 06/05/2027
 TANK PRESSURE: 663 psi

BLANK TEST	0.000	12:18
INTERNAL STANDARD	VERIFIED	12:18
EXTERNAL STANDARD	0.147	12:19
BLANK TEST	0.000	12:20
EXTERNAL STANDARD	0.147	12:20
BLANK TEST	0.000	12:21
EXTERNAL STANDARD	0.147	12:21
BLANK TEST	0.000	12:22
EXTERNAL STANDARD	0.147	12:22
BLANK TEST	0.000	12:23
EXTERNAL STANDARD	0.146	12:23
BLANK TEST	0.000	12:24

Average = 0.1468
 Std Dev = 0.0004

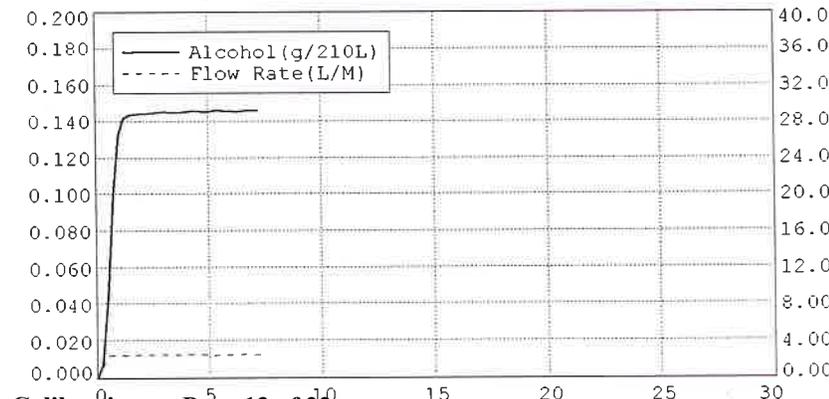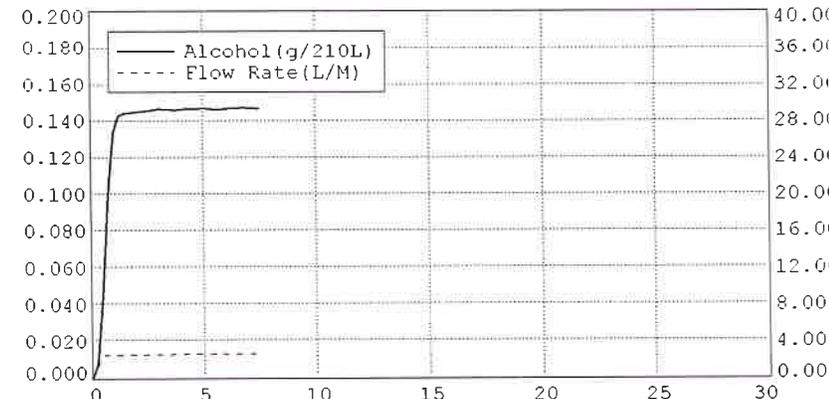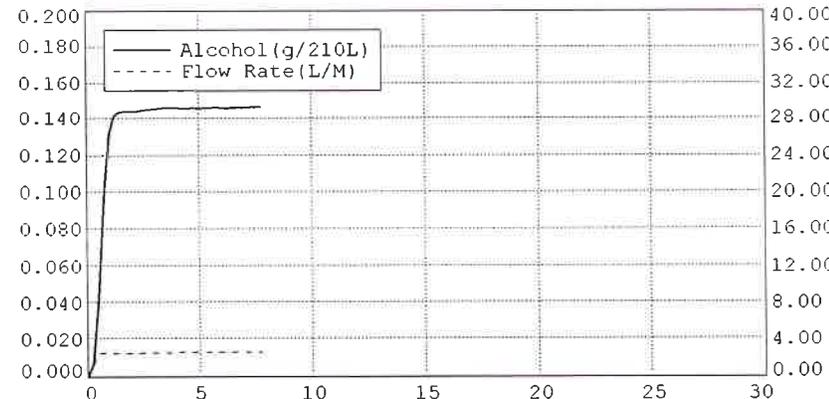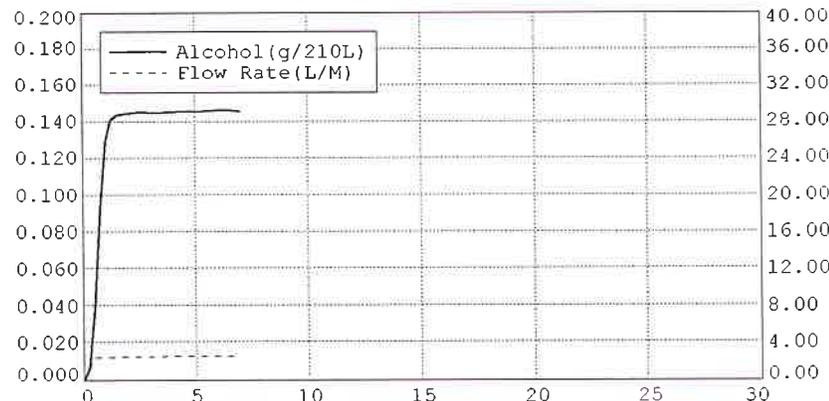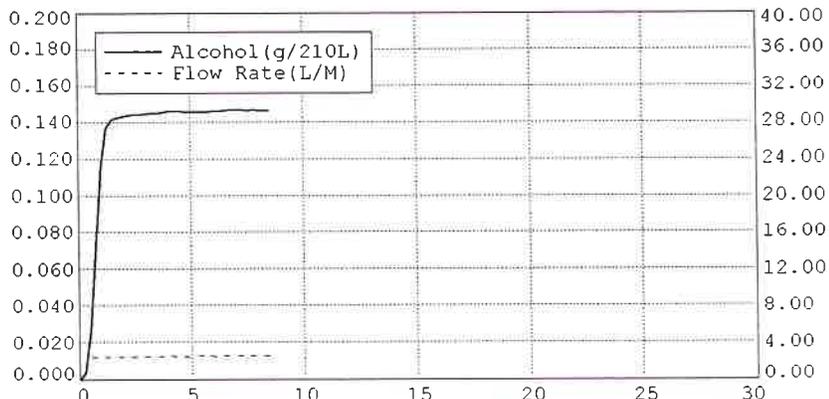

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100695






Date: 03/09/2026
Time: 12:28:43

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.64: 0.297
LOT #: AG516110
EXPIRATION: 06/10/2027
TANK PRESSURE: 327 psi

BLANK TEST	0.000	12:30
INTERNAL STANDARD	VERIFIED	12:30
EXTERNAL STANDARD	0.292	12:30
BLANK TEST	0.000	12:31
EXTERNAL STANDARD	0.292	12:31
BLANK TEST	0.000	12:32
EXTERNAL STANDARD	0.293	12:32
BLANK TEST	0.000	12:33
EXTERNAL STANDARD	0.293	12:33
BLANK TEST	0.000	12:34
EXTERNAL STANDARD	0.293	12:35
BLANK TEST	0.000	12:35

Average = 0.2926
Std Dev = 0.0005

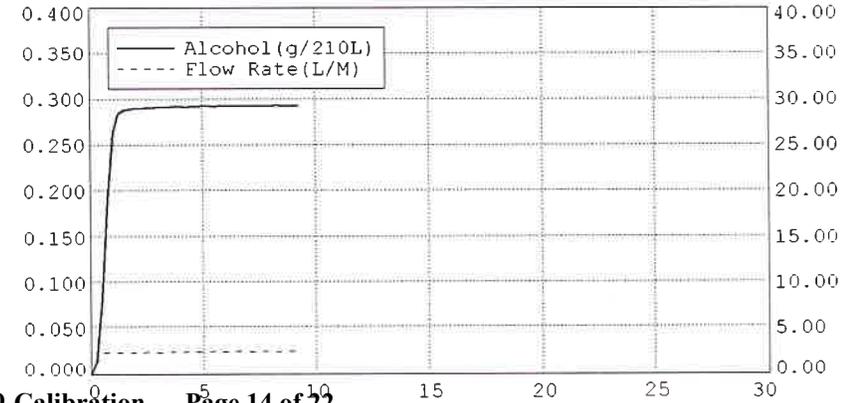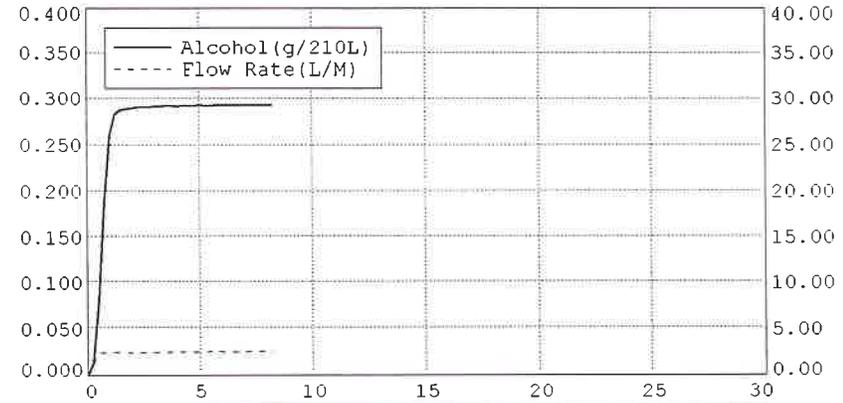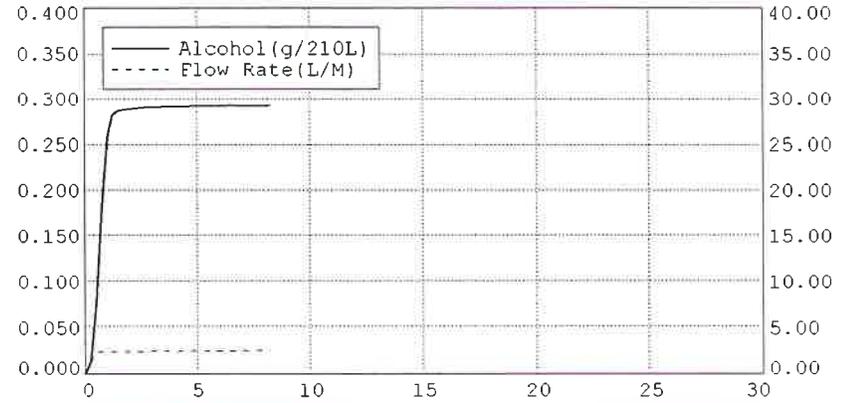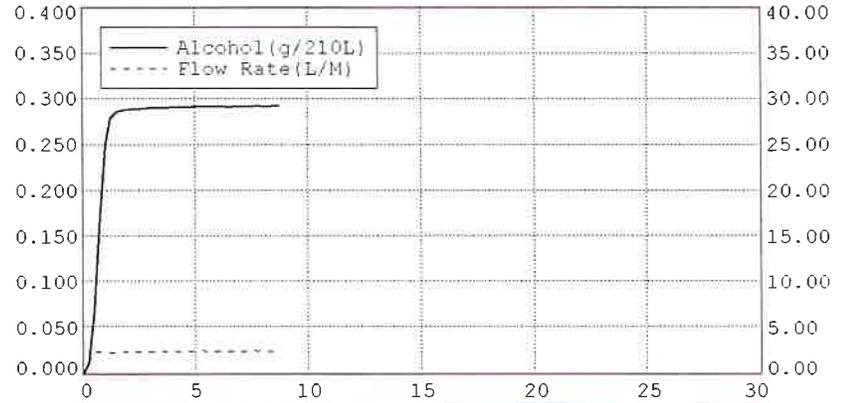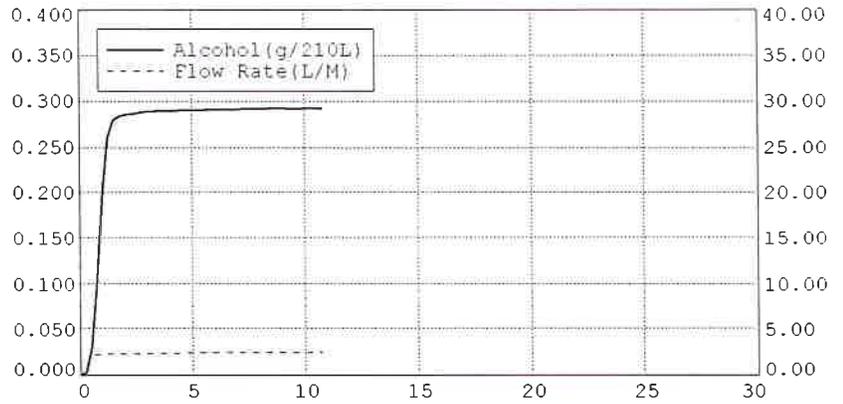

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 03/09/2026
Time: 12:39:55


SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.64: 0.079
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 12:41
BLANK TEST 0.000 12:41
INTERNAL STANDARD VERIFIED 12:41
EXTERNAL STANDARD 0.080 12:41
BLANK TEST 0.000 12:42
SUBJECT SAMPLE INCOMPLETE 12:44

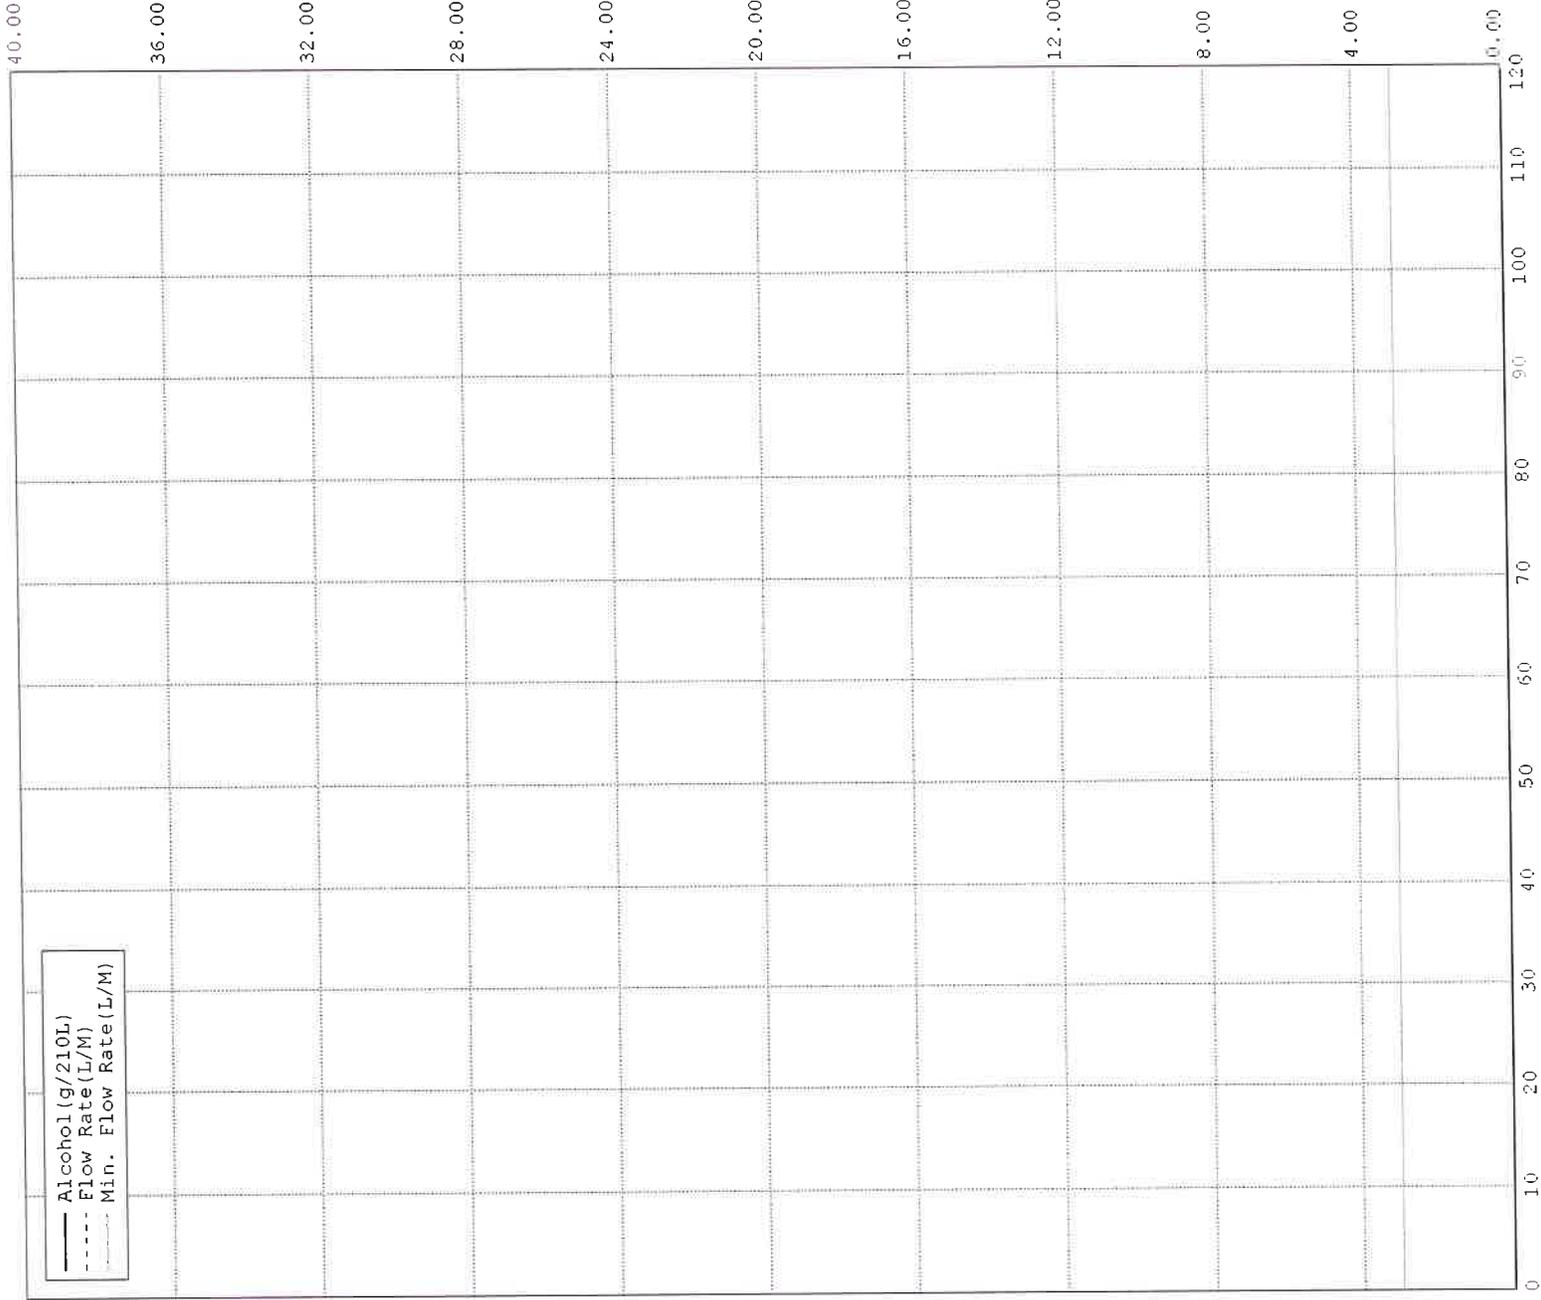

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 03/09/2026
Time: 12:47:26

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.63: 0.079
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 12:48
BLANK TEST 0.000 12:48
INTERNAL STANDARD VERIFIED 12:49
EXTERNAL STANDARD 0.080 12:49
BLANK TEST 0.000 12:50
SUBJECT SAMPLE XXX 12:50

Maximum Attempts Exceeded

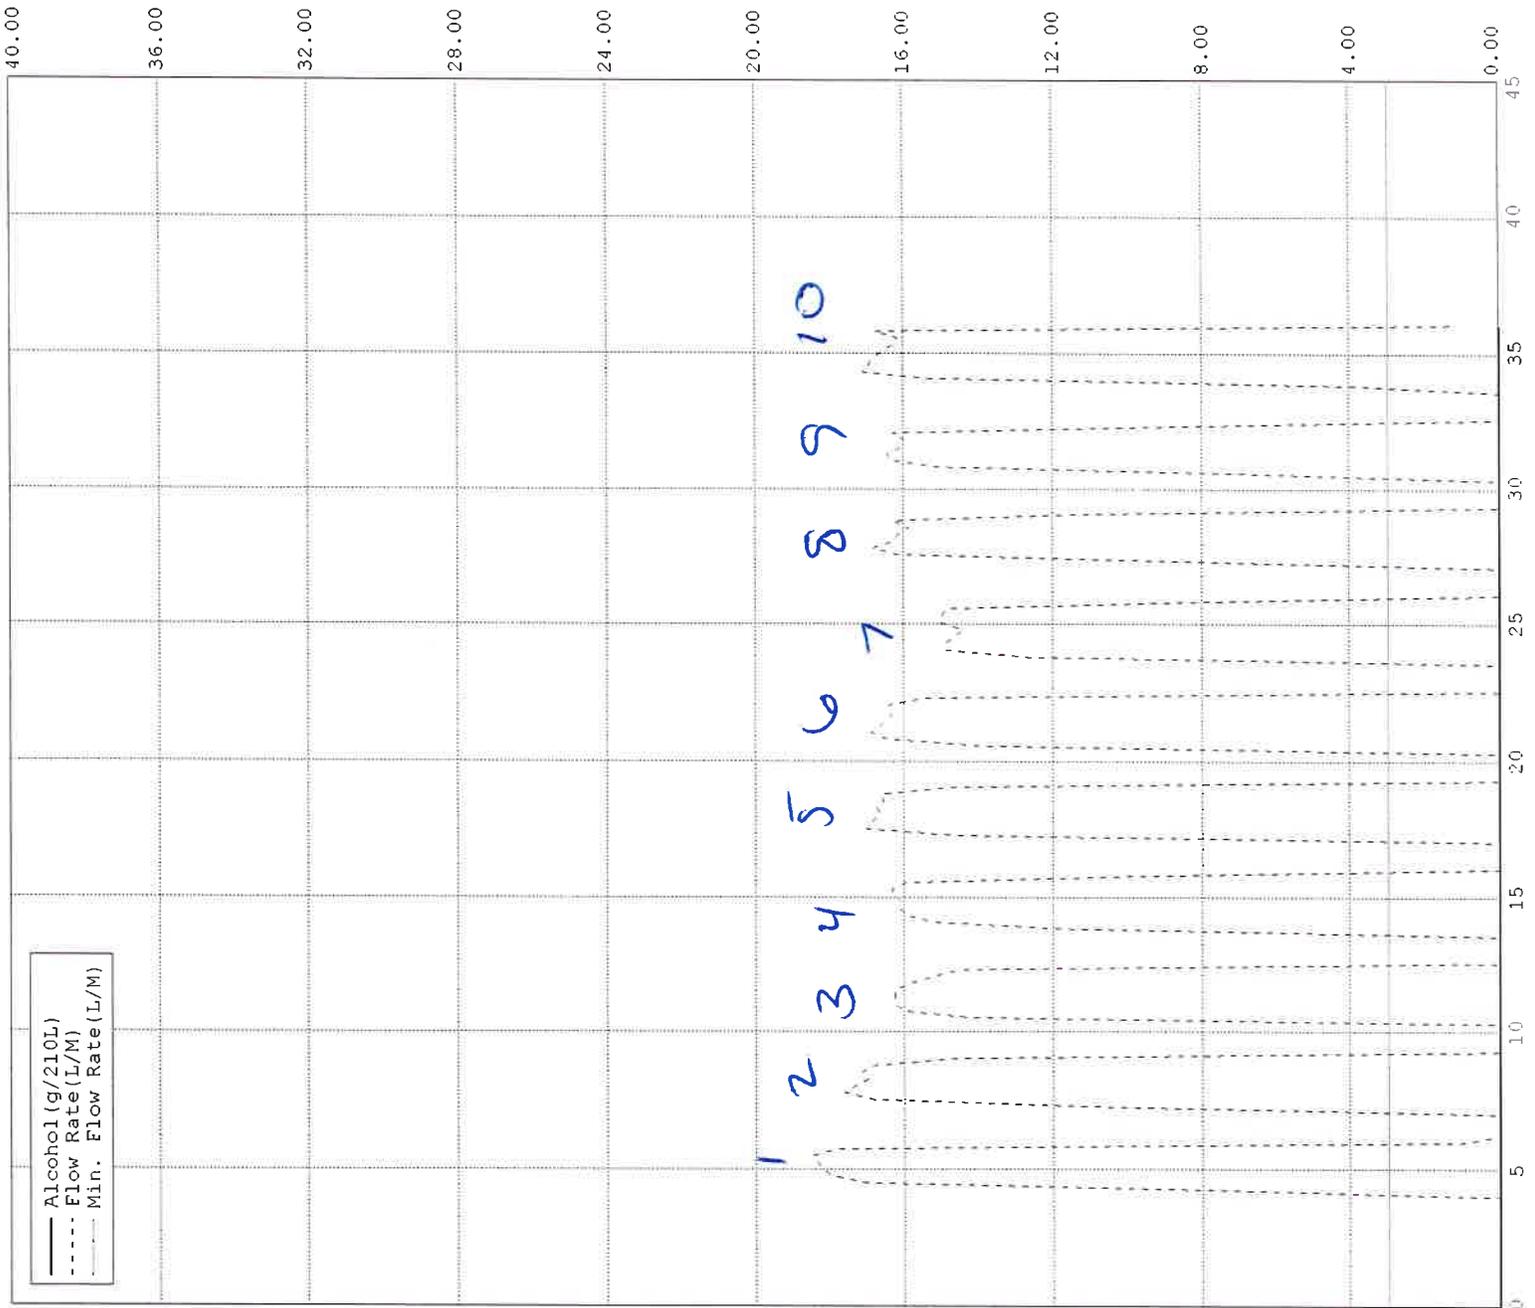

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 03/09/2026
Time: 12:52:57


SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INVALID
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.64: 0.079
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	12:54
BLANK TEST	0.000	12:54
INTERNAL STANDARD	VERIFIED	12:54
EXTERNAL STANDARD	0.080	12:54
BLANK TEST	0.000	12:55
SUBJECT SAMPLE	INVALID	12:56

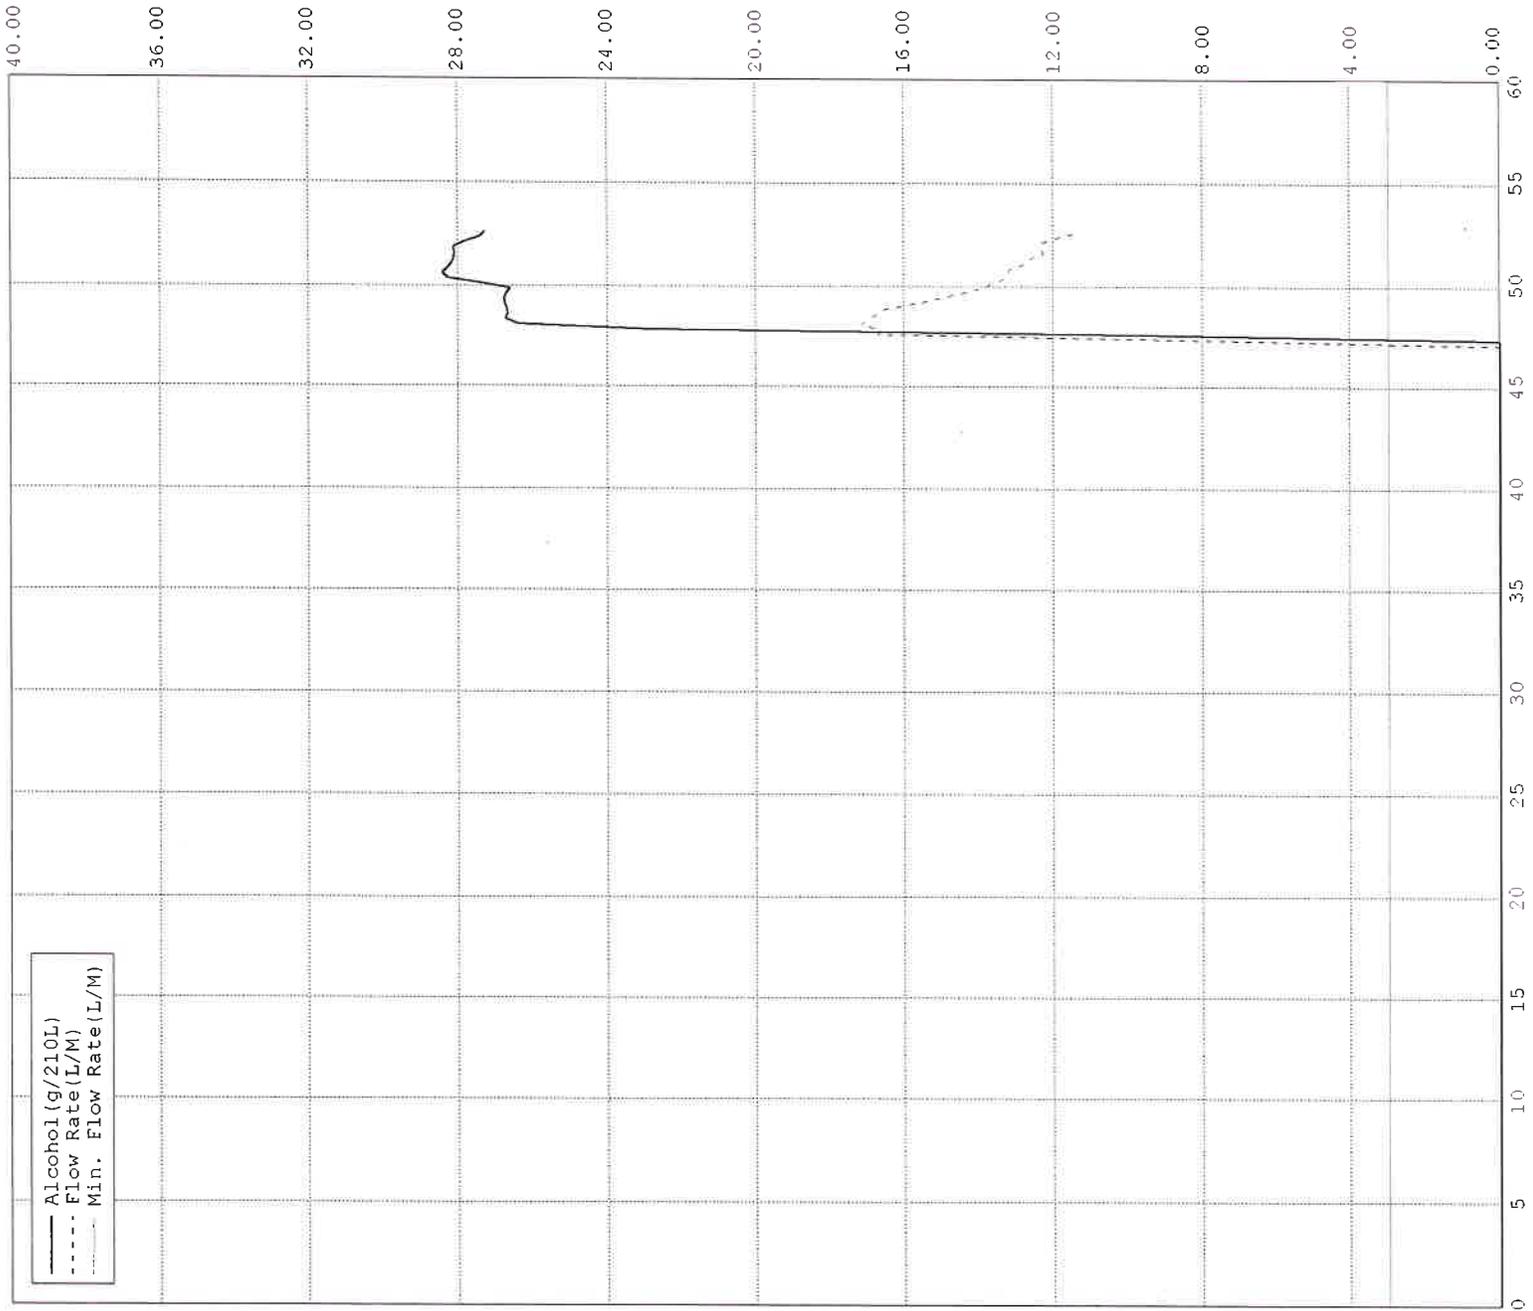

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 03/09/2026
Time: 13:03:41

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
RFI
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.63: 0.079
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK
BLANK TEST PASSED 13:04
INTERNAL STANDARD VERIFIED 13:04
EXTERNAL STANDARD 0.079 13:05
BLANK TEST 0.000 13:06

RFI DETECTED

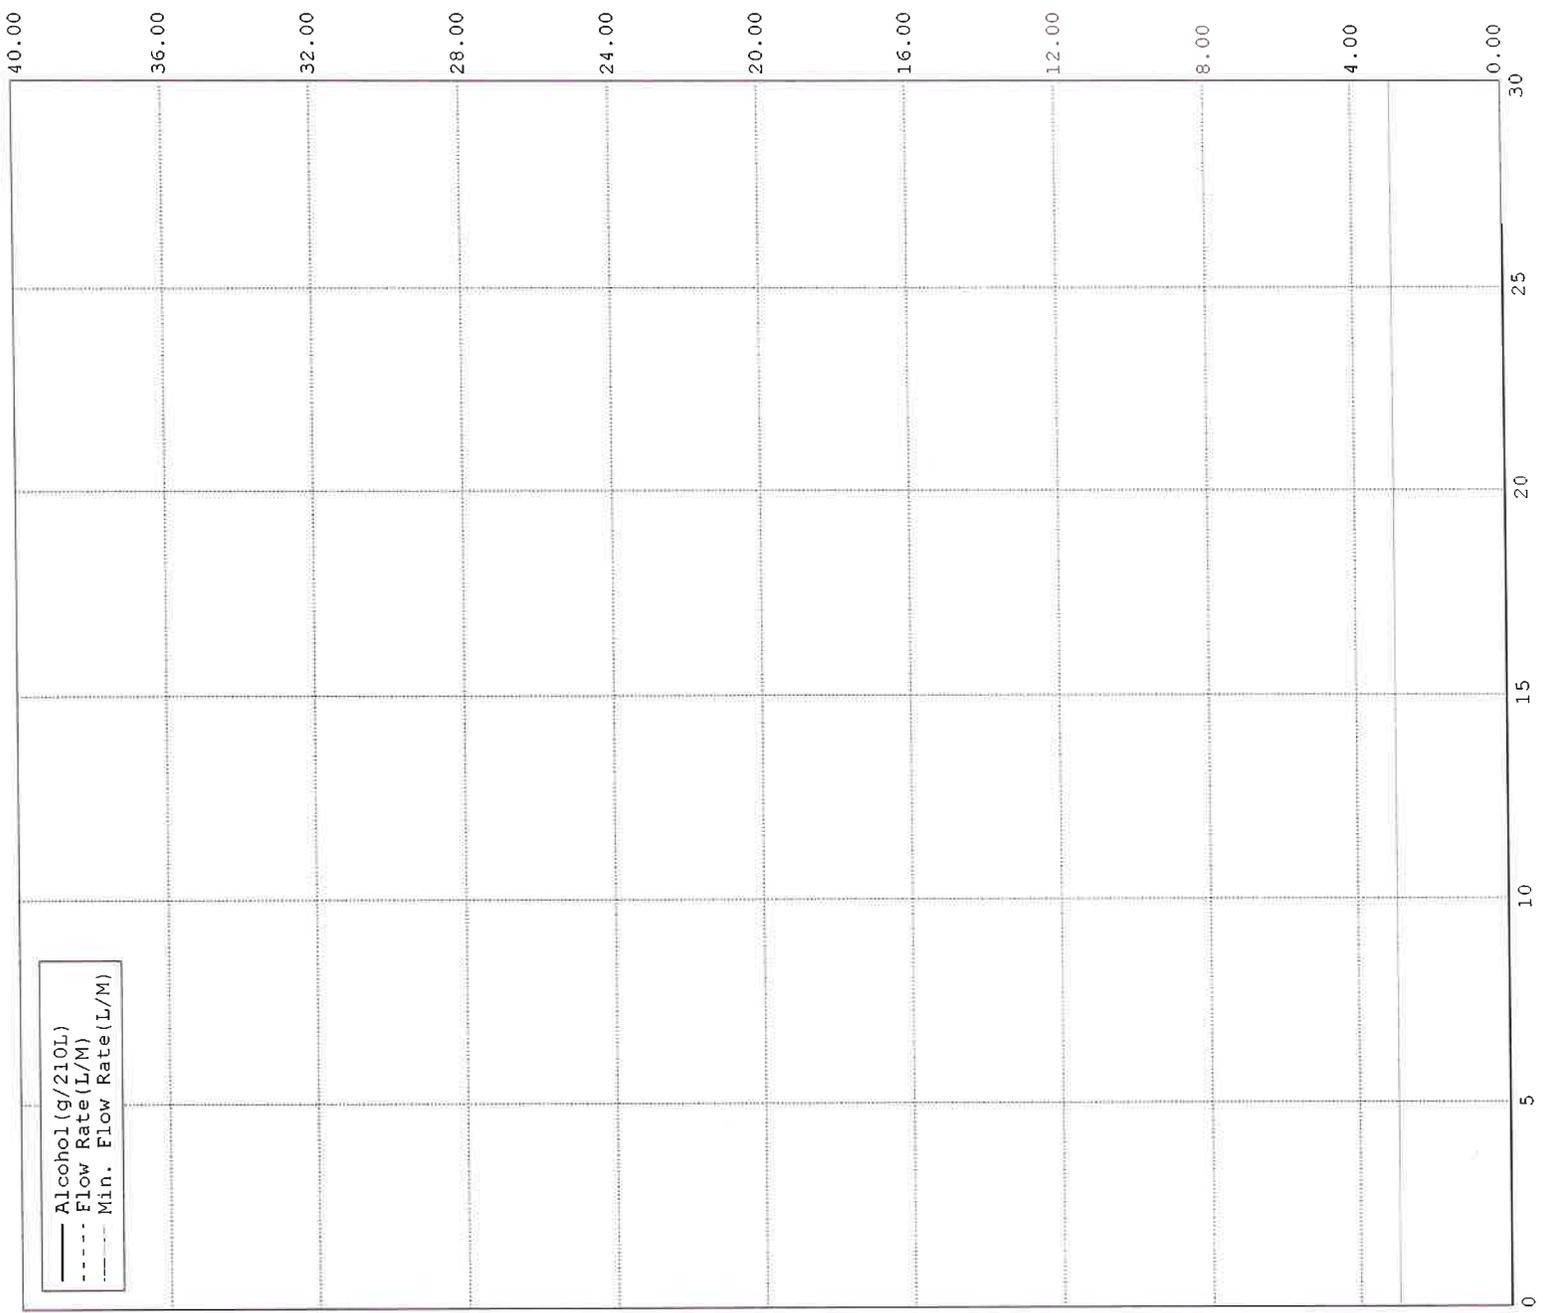

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 03/09/2026
Time: 13:38:35

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE - ACETONE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.63: 0.079
LOT #: AG436502
EXPIRATION: 12/30/2026


DIAGNOSTIC CHECK	PASSED	13:39
BLANK TEST	0.000	13:39
INTERNAL STANDARD	VERIFIED	13:39
Xg = 0.115 (1.07%)		
EXTERNAL STANDARD	0.079	13:40
X[1] = 0.0786 (-0.0015) (0.0039)		
BLANK TEST	0.000	13:41
SUBJECT SAMPLE	XXX	13:41
X[1] = 0.1062 (-0.0178) (0.0028)		

Interference Detected

Filter 2 Avg: -0.0012

Filter 3 Avg: 0.0036

UW 3/9/26

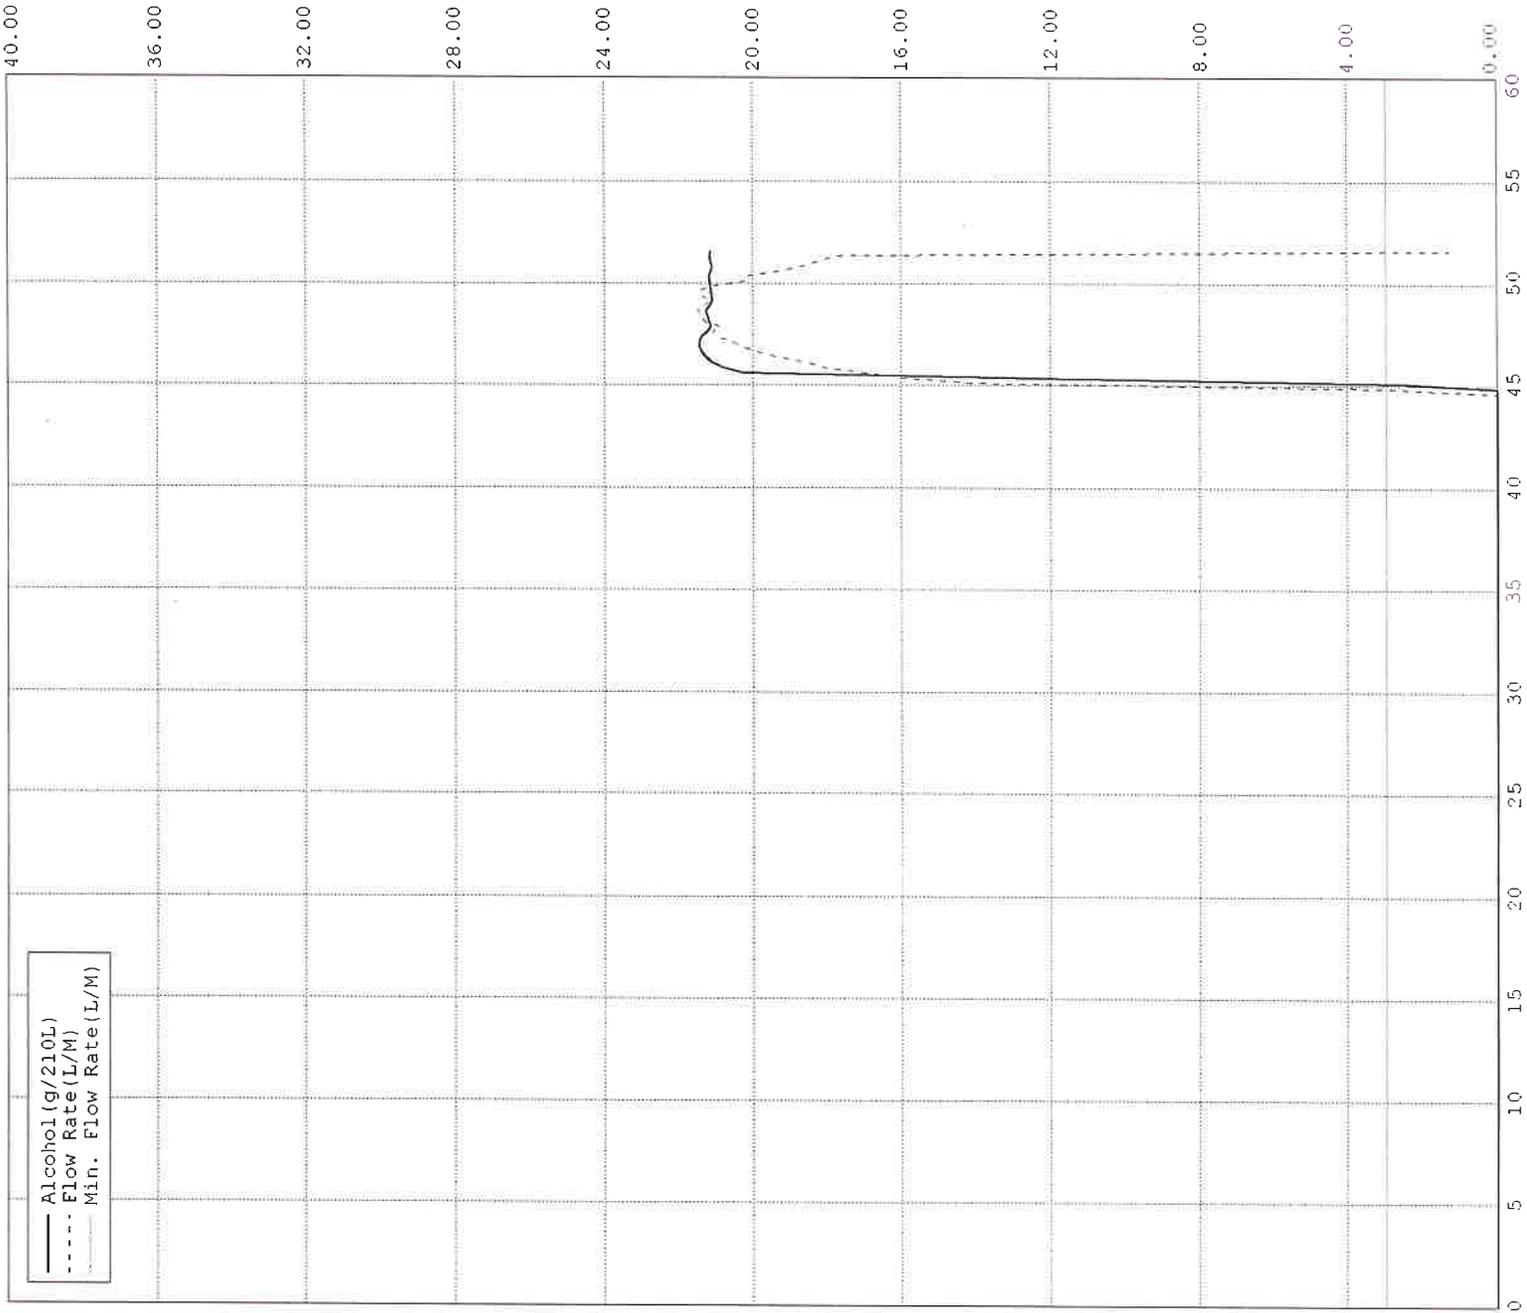

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 03/09/2026
Time: 13:46:16

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE - IPA
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.62: 0.079
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	13:47
BLANK TEST	0.000	13:47
INTERNAL STANDARD	VERIFIED	13:47
Xg = 0.115 (1.07%)		
EXTERNAL STANDARD	0.079	13:47
X[1] = 0.0791 (-0.0008) (0.0044)		
BLANK TEST	0.000	13:48
SUBJECT SAMPLE	XXX	13:49
X[1] = 0.1174 (-0.0199) (0.0028)		

Interference Detected

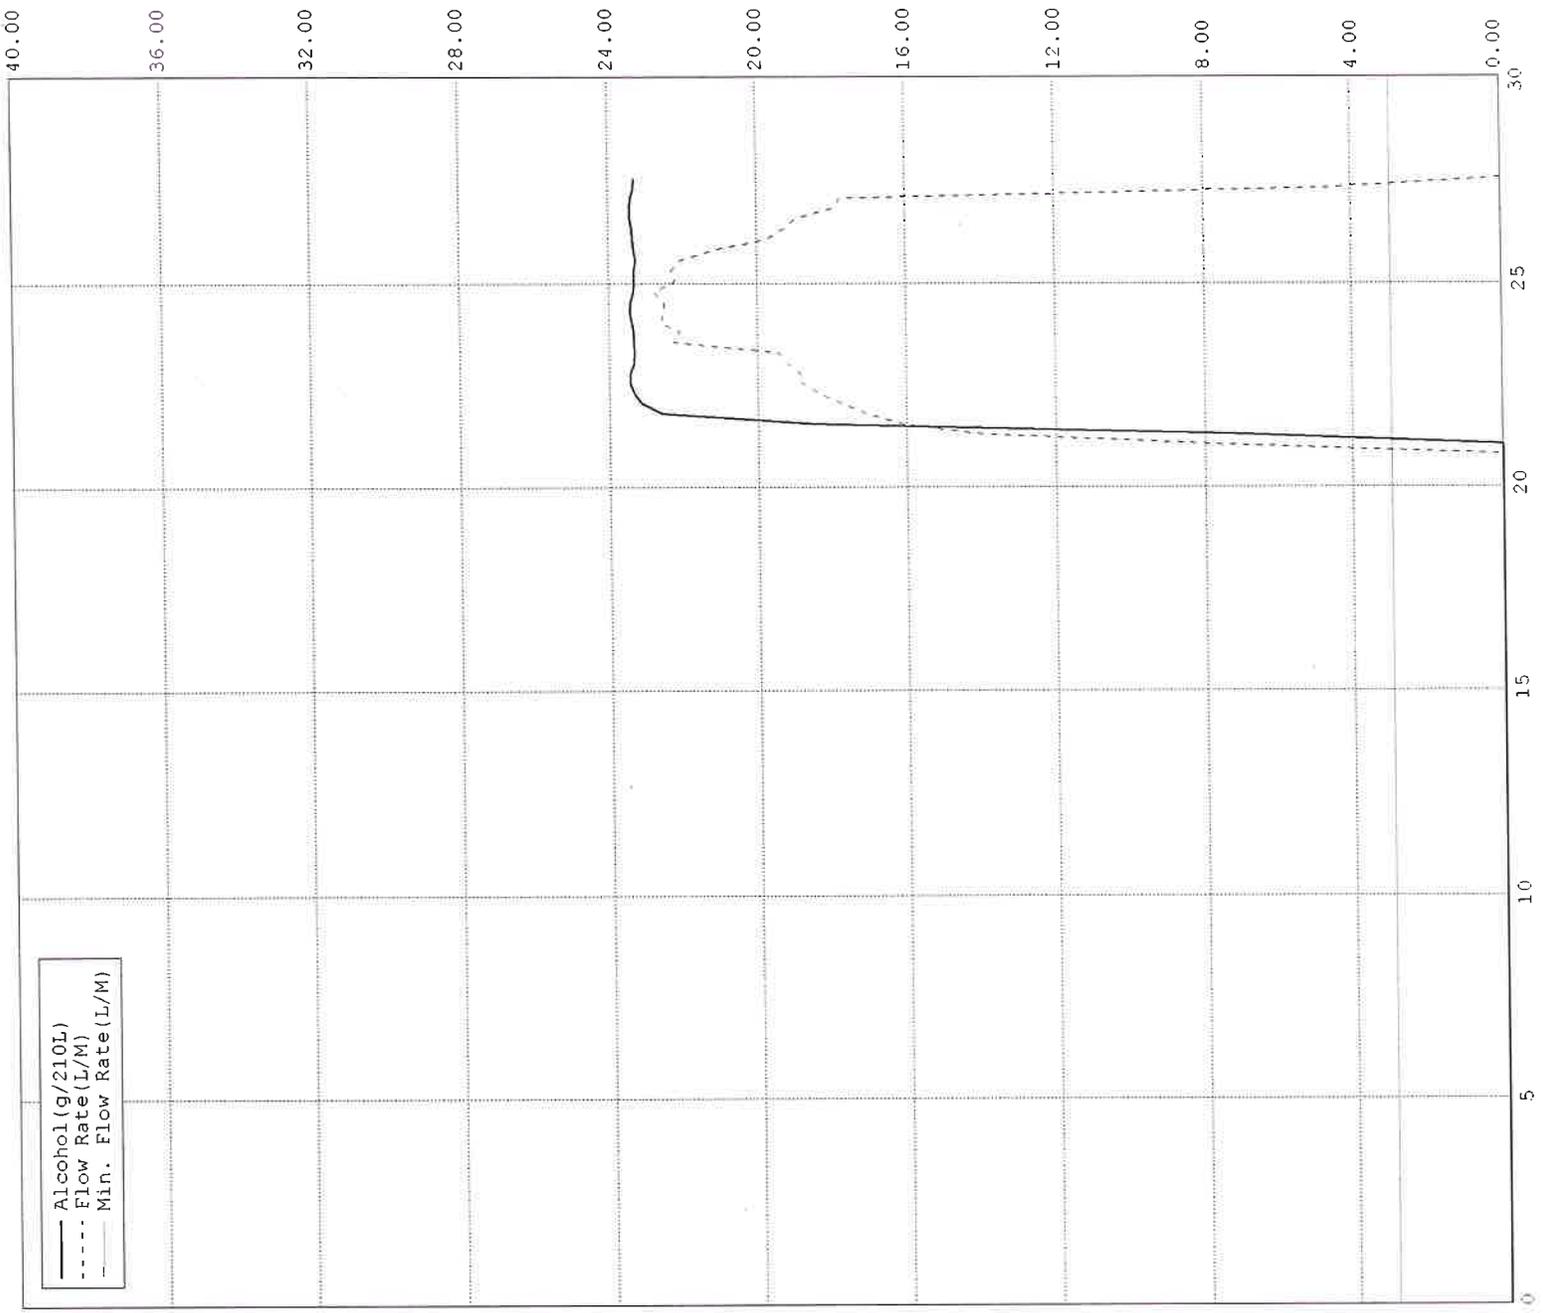

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 03/09/2026
Time: 13:28:14



SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE - NEGATIVE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.62: 0.079
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	13:29
BLANK TEST	0.000	13:29
INTERNAL STANDARD	VERIFIED	13:29
Xg = 0.114 (1.83%)		
EXTERNAL STANDARD	0.079	13:29
X[1] = 0.0786 (-0.0011)	(0.0034)	
BLANK TEST	0.000	13:30
SUBJECT SAMPLE (Vol=2.09L)	0.094	13:31
X[1] = 0.0944 (0.0008)	(0.0022)	
BLANK TEST	0.000	13:32
EXTERNAL STANDARD	0.079	13:32
X[1] = 0.0788 (-0.0013)	(0.0028)	
BLANK TEST	0.000	13:33

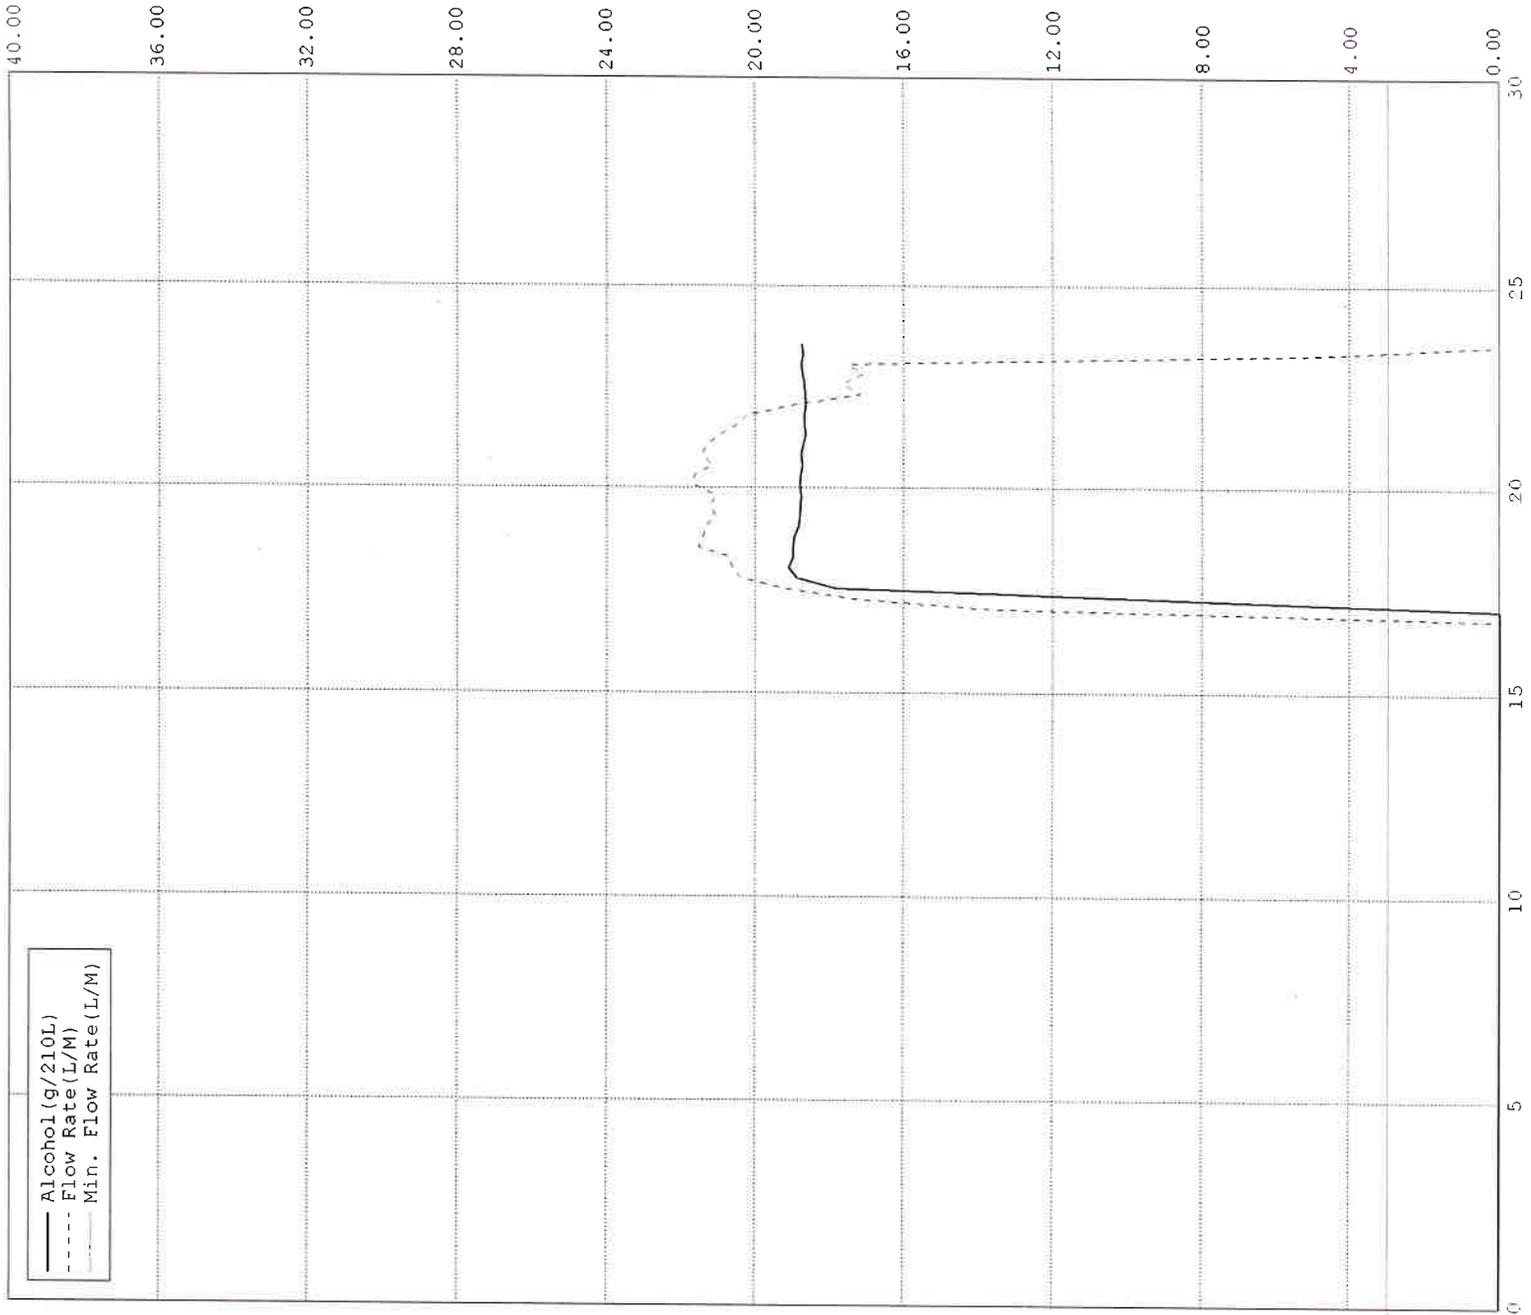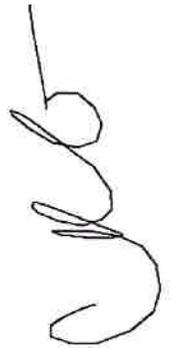

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 03/09/2026
Time: 15:31:02

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.60: 0.079
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	15:32
BLANK TEST	0.000	15:32
INTERNAL STANDARD	VERIFIED	15:32
EXTERNAL STANDARD	0.079	15:32
BLANK TEST	0.000	15:33
SUBJECT SAMPLE (Vol=2.25L)	0.000	15:33
BLANK TEST	0.000	15:34
EXTERNAL STANDARD	0.079	15:34
BLANK TEST	0.000	15:35

